

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061022\
 Data File : VN072773.D
 Acq On : 10 Jun 2022 18:36
 Operator : JC\MD
 Sample : N3293-14
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 40806

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060822W.M
 Title : SW846 8260

Signal : TIC: VN072773.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.234	32	42	51	rBV2	12271	32059	2.14%	0.436%
2	2.740	122	128	129	rBV3	8899	16466	1.10%	0.224%
3	4.587	430	442	452	rBV2	12359	39820	2.65%	0.542%
4	8.016	1015	1025	1031	rBV	242881	595029	39.66%	8.092%
5	8.086	1031	1037	1050	rVB2	250182	577131	38.47%	7.849%
6	8.433	1087	1096	1108	rBV	287675	649877	43.31%	8.838%
7	8.963	1177	1186	1201	rBV	386634	806558	53.76%	10.969%
8	10.327	1412	1418	1425	rBV3	8959	18834	1.26%	0.256%
9	10.439	1428	1437	1445	rVV	829751	1500353	100.00%	20.404%
10	10.498	1445	1447	1456	rVB2	15392	27574	1.84%	0.375%
11	11.139	1552	1556	1568	rVB3	16946	37491	2.50%	0.510%
12	11.745	1650	1659	1671	rBV	515311	924936	61.65%	12.579%
13	11.945	1687	1693	1700	rVB2	10718	21648	1.44%	0.294%
14	12.727	1819	1826	1836	rVB	592656	1013842	67.57%	13.788%
15	13.368	1929	1935	1941	rVB7	10215	22184	1.48%	0.302%
16	13.668	1978	1986	2001	rBV	444659	826519	55.09%	11.240%
17	14.621	2146	2148	2158	rVB7	9132	16639	1.11%	0.226%
18	15.504	2290	2298	2306	rBV2	36596	85028	5.67%	1.156%
19	16.192	2410	2415	2424	rVB5	9567	18469	1.23%	0.251%
20	16.615	2474	2487	2497	rBV3	47761	122668	8.18%	1.668%




Sum of corrected areas: 7353125

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061022\
Data File : VN072773.D
Acq On : 10 Jun 2022 18:36
Operator : JC\MD
Sample : N3293-14
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
40806

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

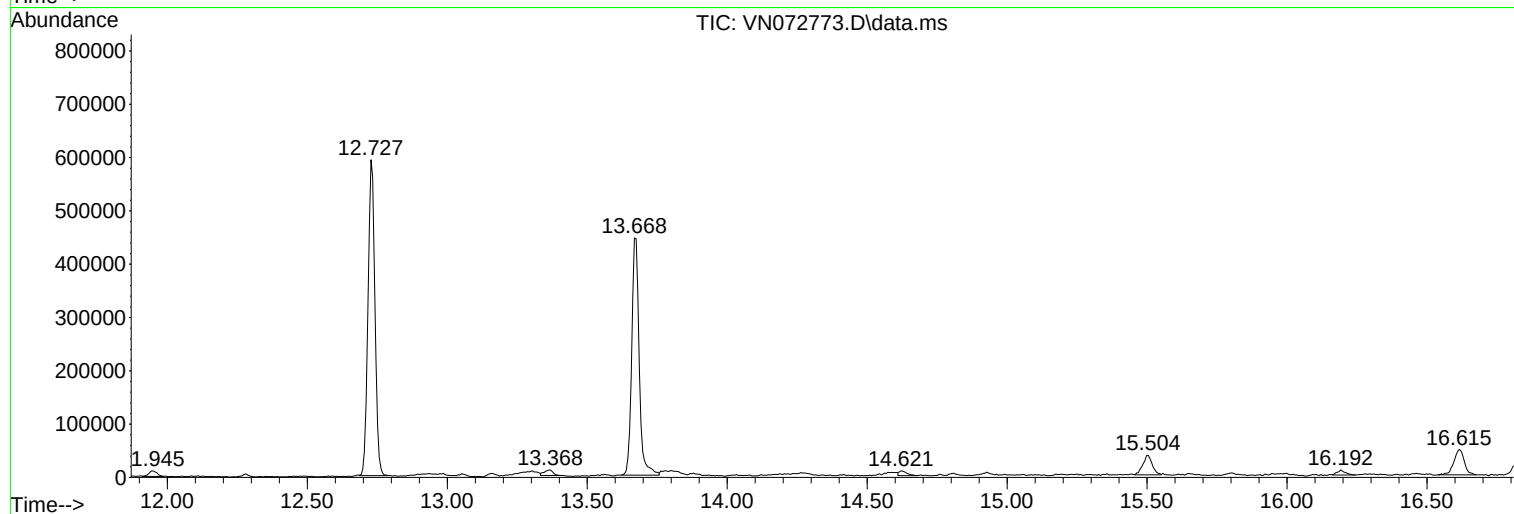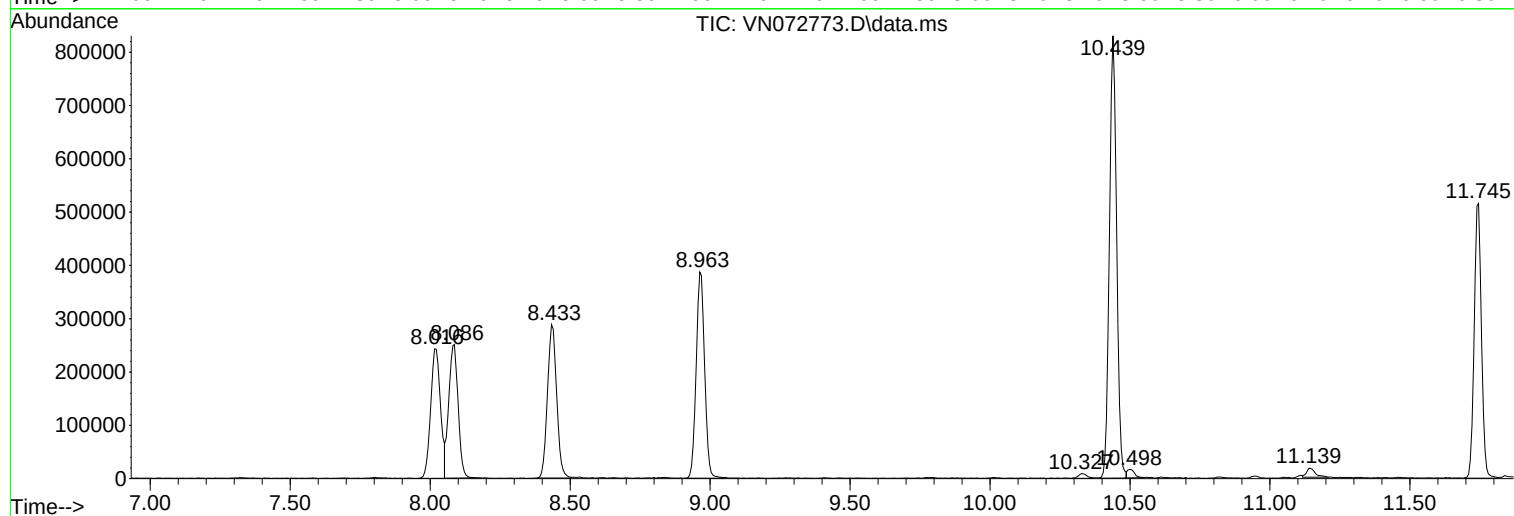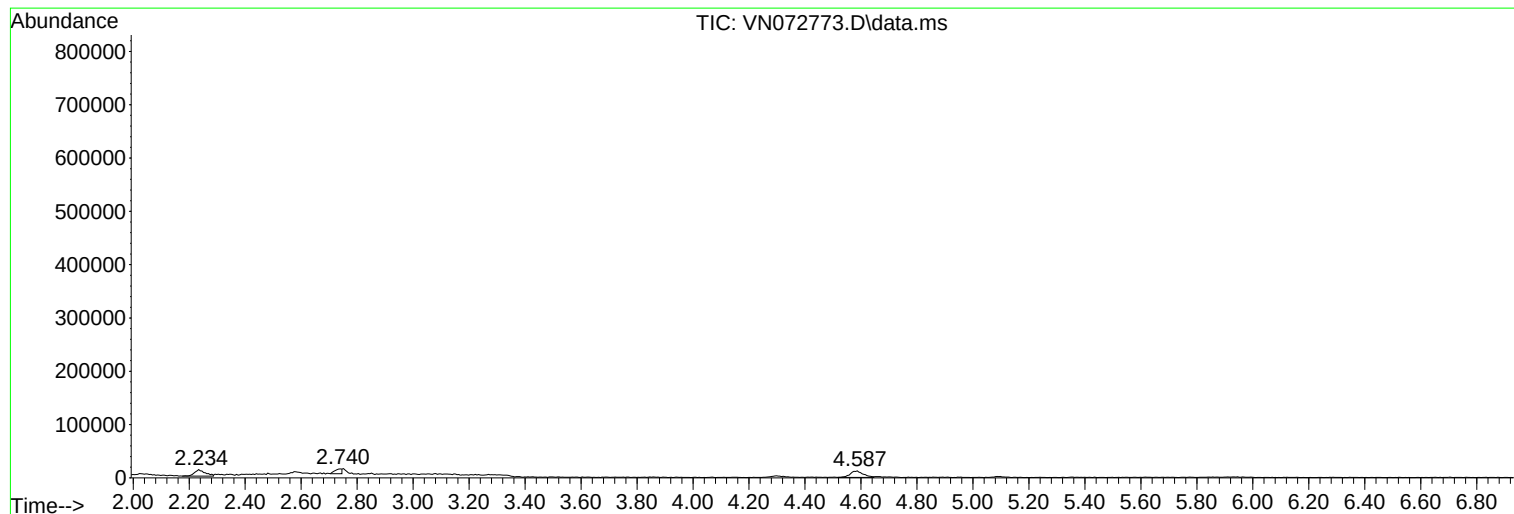

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061022\
Data File : VN072773.D
Acq On : 10 Jun 2022 18:36
Operator : JC\MD
Sample : N3293-14
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
40806










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Naphthalene, 1-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.615	7.42 ug/l	122668	1,4-Dichlorobenzene-d4	13.674

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Naphthalene, 1-methyl-	142	C11H10	000090-12-0	94
2			Naphthalene, 2-methyl-	142	C11H10	000091-57-6	94
3			Benzocycloheptatriene	142	C11H10	000264-09-5	90
4			1,4-Methanonaphthalene, 1,4-dihy...	142	C11H10	004453-90-1	87
5			3,4-Difluorobenzaldehyde	142	C7H4F2O	034036-07-2	64

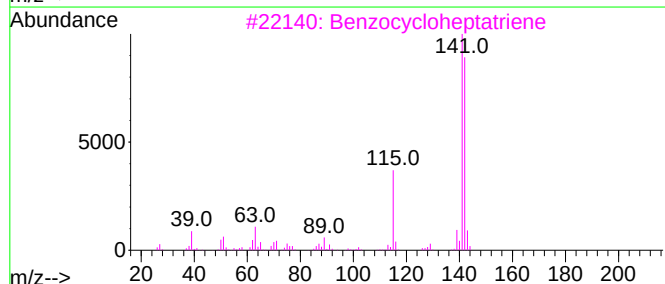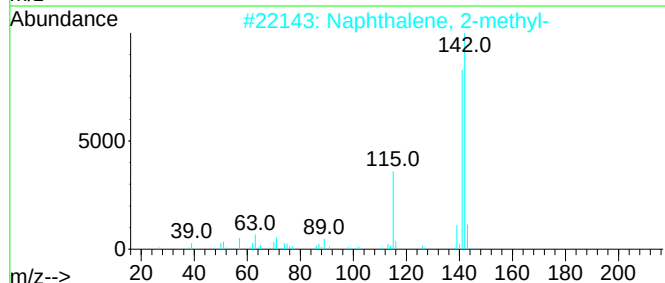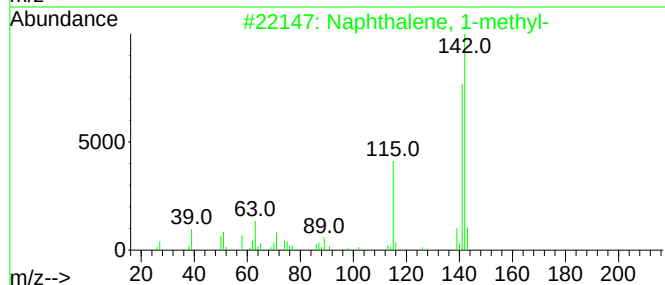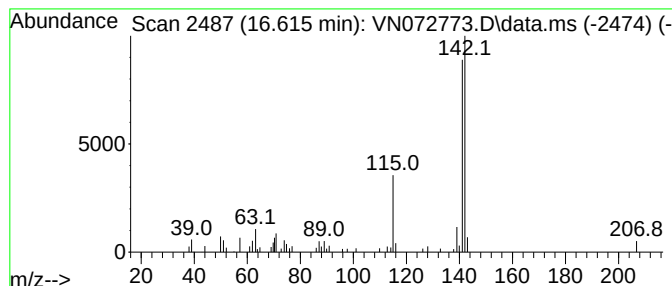

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061022\
Data File : VN072773.D
Acq On : 10 Jun 2022 18:36
Operator : JC\MD
Sample : N3293-14
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
40806

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Naphthalene, 1-...	16.615	7.4	ug/l	122668	4	13.674	826519	50.0