


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061022\
Data File : VN072756.D
Acq On : 10 Jun 2022 10:21
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060822W.M
Title : SW846 8260
Last Update : Thu Jun 09 05:17:31 2022

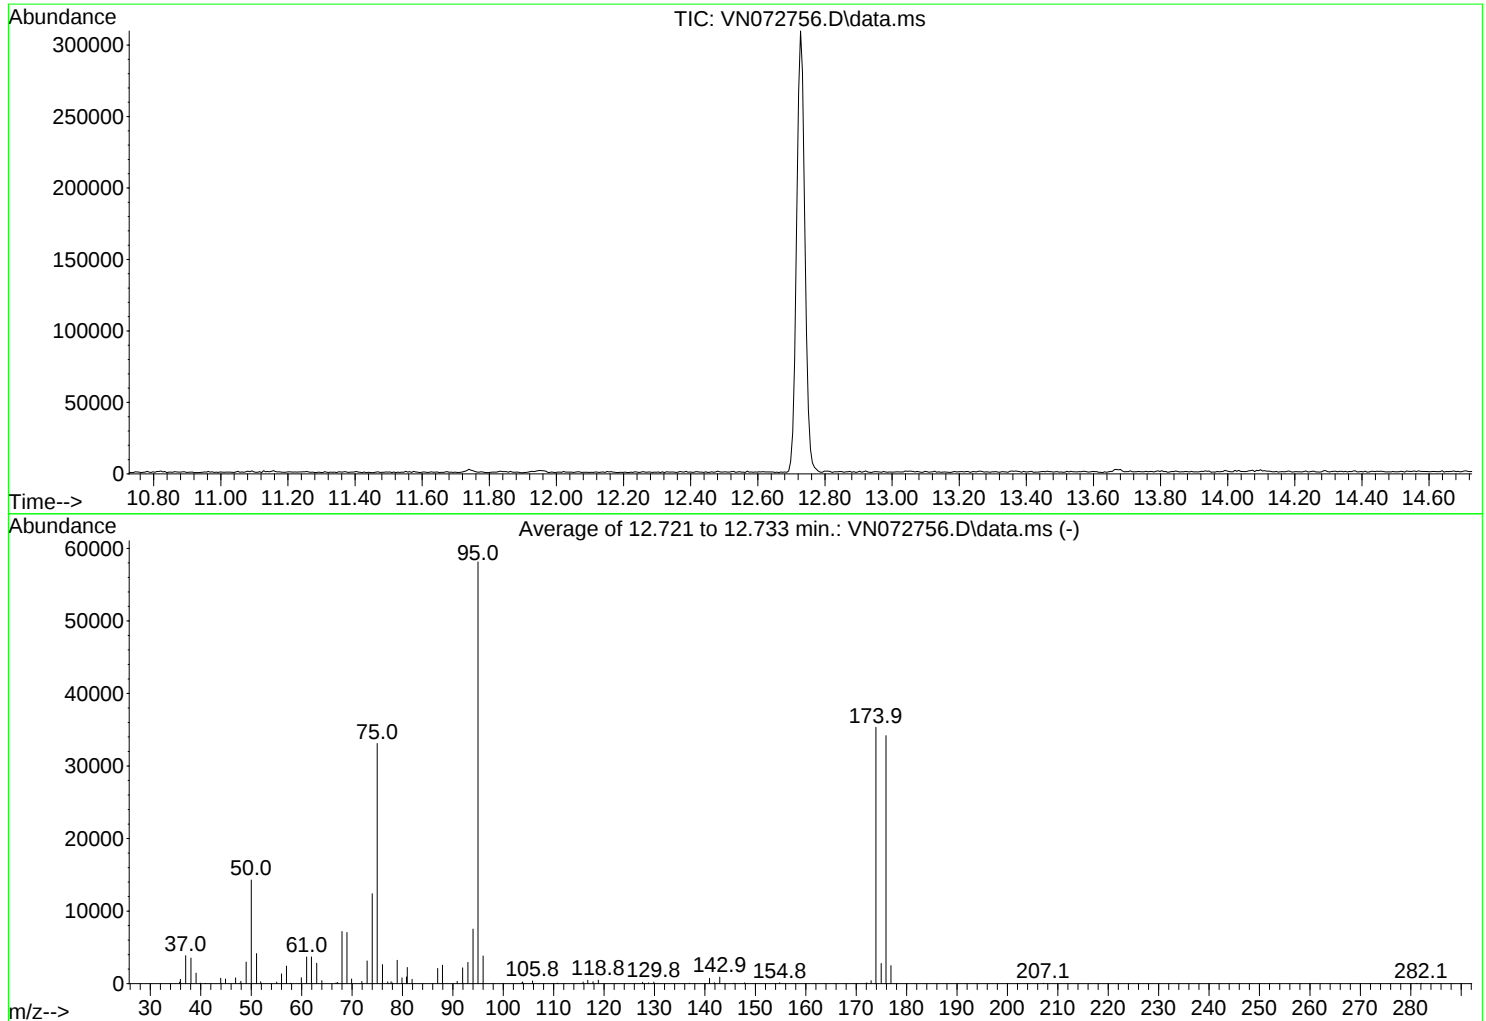

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1816

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.6	14301	PASS
75	95	30	60	57.0	33112	PASS
95	95	100	100	100.0	58141	PASS
96	95	5	9	6.6	3811	PASS
173	174	0.00	2	1.2	422	PASS
174	95	50	100	60.8	35328	PASS
175	174	5	9	7.9	2787	PASS
176	174	95	101	96.7	34179	PASS
177	176	5	9	7.3	2485	PASS