
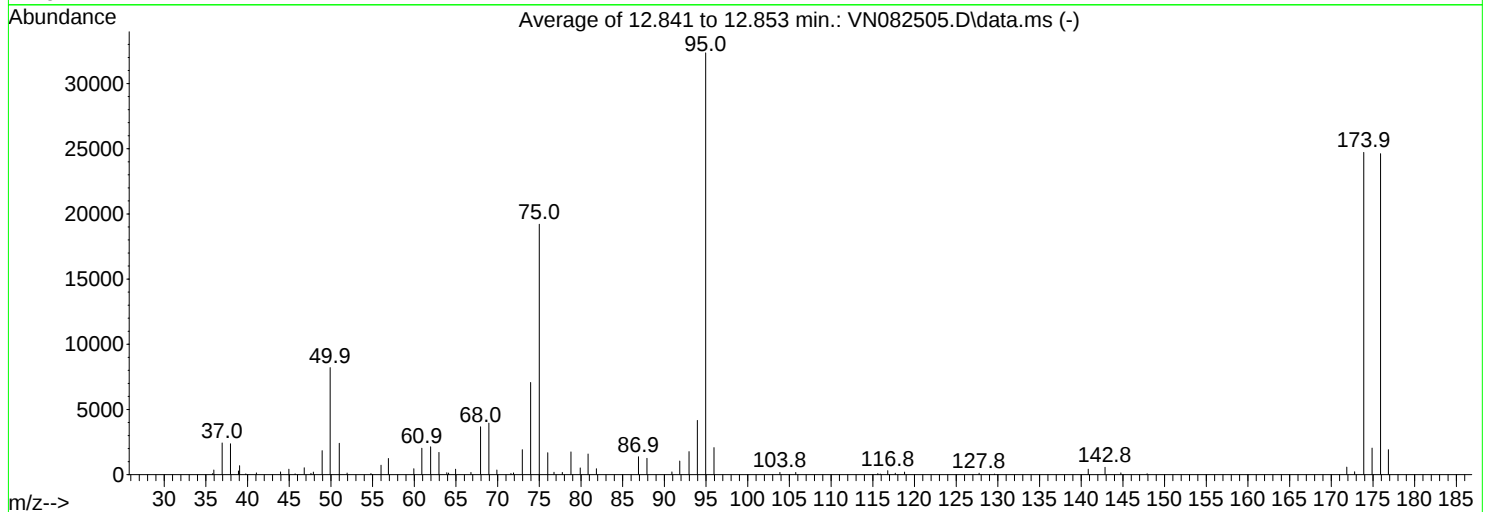


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061024\
Data File : VN082505.D
Acq On : 10 Jun 2024 09:55
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

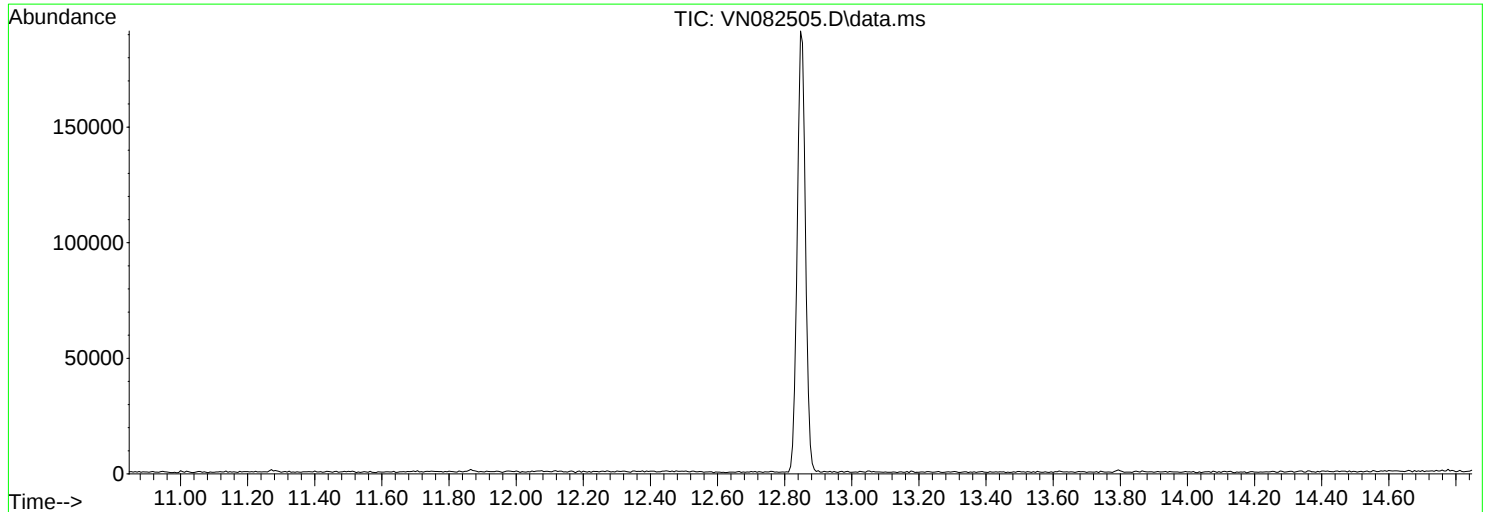

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	25.4	8216	PASS
75	95	30	60	59.4	19204	PASS
95	95	100	100	100.0	32357	PASS
96	95	5	9	6.4	2078	PASS
173	174	0.00	2	0.9	218	PASS
174	95	50	100	76.4	24725	PASS
175	174	5	9	8.3	2041	PASS
176	174	95	101	99.6	24624	PASS
177	176	5	9	7.8	1914	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	74	46.80	526	60.90	2026	71.90	130
35.95	361	47.60	97	61.95	2137	72.95	191
36.95	2428	47.90	203	62.95	1705	73.95	706
37.95	2368	48.95	1847	63.90	153	75.00	1920
38.90	288	49.90	8216	64.10	120	76.00	1688
39.05	693	51.00	2401	64.95	420	76.75	188
39.80	67	51.95	122	66.80	169	77.75	170
41.05	133	54.80	85	67.95	3670	78.80	1749
43.95	208	56.00	728	68.95	3955	79.90	518
44.95	418	56.90	1241	69.90	363	80.85	1583
45.70	63	59.95	453	71.60	84	81.85	454

Average of 12.841 to 12.853 min.: VN082505.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.90	1370	115.90	52	172.80	218		
87.90	1252	116.80	304	173.90	24725		
90.90	215	117.70	106	174.90	2041		
91.85	1038	118.80	193	175.90	24624		
92.95	1772	127.75	114	176.85	1914		
93.95	4160	129.60	55				
94.95	32357	140.85	420				
95.95	2078	142.85	571				
103.85	176	144.75	138				
105.75	174	147.90	70				
115.60	93	171.85	581				

Instrument :

MSVOA_N

ClientSampleId :

BFB