


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN061025\  
Data File : VN086912.D  
Acq On : 10 Jun 2025 08:39  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N060625W.M  
Title : SW846 8260  
Last Update : Sat Jun 07 02:12:50 2025

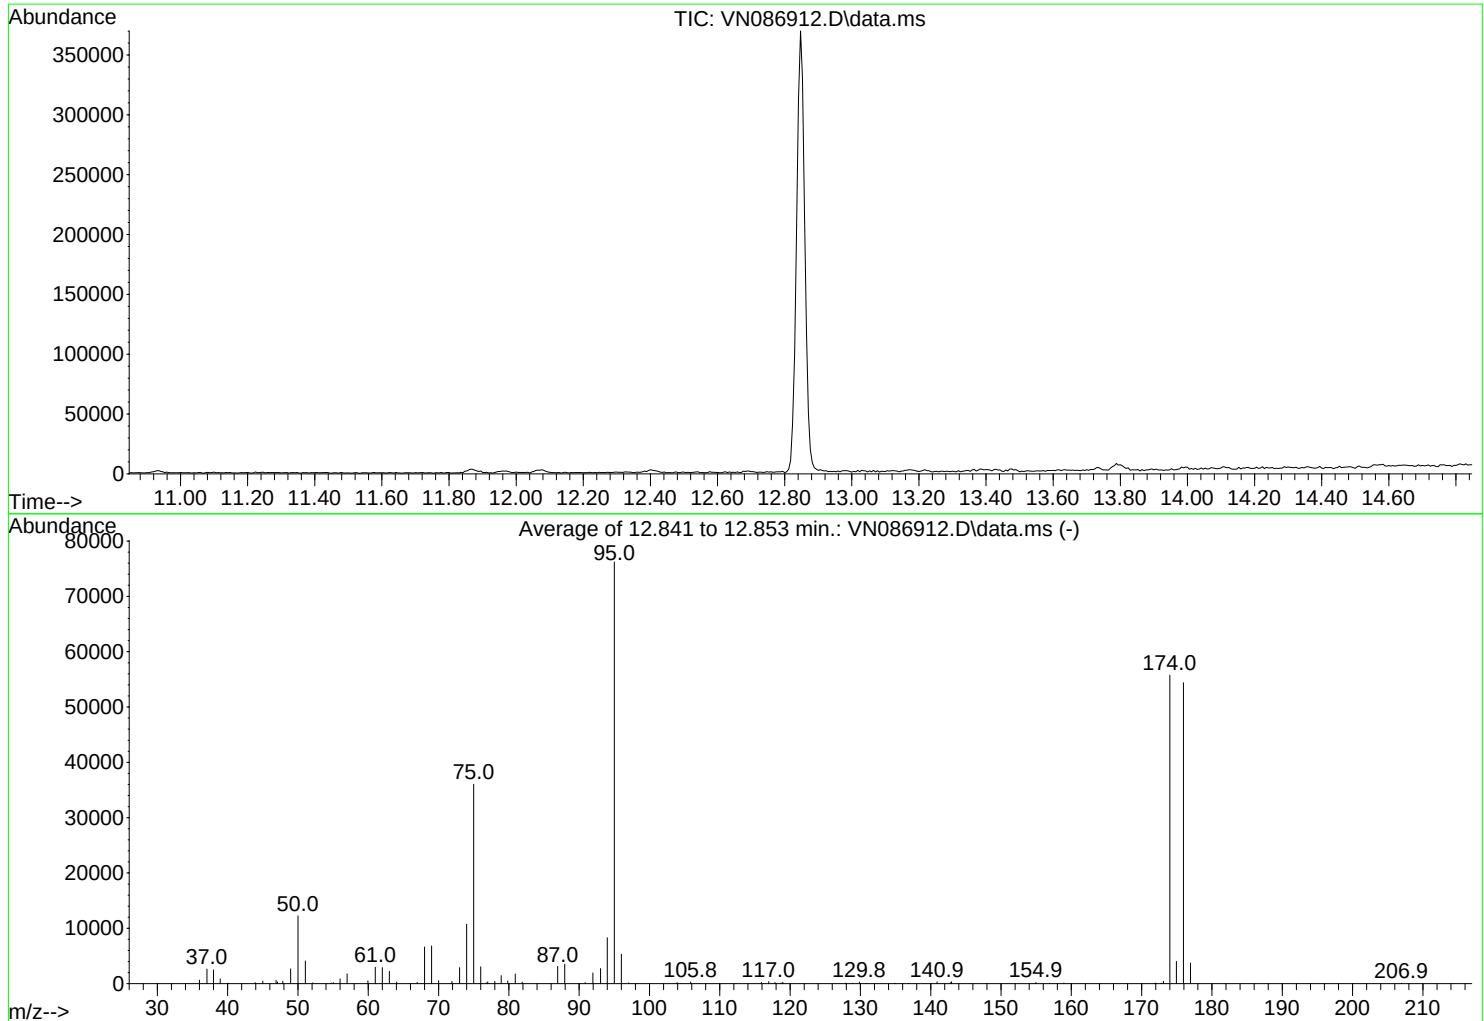

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 16.1         | 12262      | PASS                |
| 75             | 95              | 30              | 60              | 47.3         | 36032      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 76240      | PASS                |
| 96             | 95              | 5               | 9               | 7.0          | 5316       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.8          | 431        | PASS                |
| 174            | 95              | 50              | 100             | 73.1         | 55768      | PASS                |
| 175            | 174             | 5               | 9               | 7.2          | 4025       | PASS                |
| 176            | 174             | 95              | 101             | 97.5         | 54389      | PASS                |
| 177            | 176             | 5               | 9               | 6.9          | 3729       | PASS                |

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z   | abund. |
|-------|--------|-------|--------|-------|--------|-------|--------|
| 36.00 | 640    | 50.00 | 12262  | 64.05 | 291    | 77.00 | 311    |
| 37.05 | 2628   | 51.05 | 4110   | 66.95 | 223    | 78.00 | 411    |
| 38.00 | 2499   | 52.10 | 152    | 68.00 | 6638   | 78.90 | 145    |
| 38.95 | 876    | 54.80 | 105    | 69.00 | 6822   | 79.85 | 49     |
| 40.10 | 81     | 55.05 | 178    | 70.00 | 566    | 80.90 | 1738   |
| 43.90 | 205    | 56.00 | 882    | 71.90 | 407    | 81.90 | 283    |
| 45.00 | 472    | 57.00 | 1769   | 73.00 | 2882   | 86.95 | 3122   |
| 46.90 | 620    | 59.95 | 518    | 74.00 | 10736  | 87.95 | 3520   |
| 47.10 | 283    | 61.00 | 2993   | 75.00 | 36032  | 90.85 | 196    |
| 47.85 | 430    | 62.00 | 2881   | 76.00 | 3052   | 91.95 | 1931   |
| 48.95 | 2653   | 63.00 | 2217   | 76.80 | 133    | 93.05 | 2726   |

Average of 12.841 to 12.853 min.: VN086912.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z    | abund. | m/z    | abund. | m/z    | abund. |
|--------|--------|--------|--------|--------|--------|--------|--------|
| 94.00  | 8301   | 118.95 | 269    | 154.95 | 233    | 206.95 | 97     |
| 95.00  | 76240  | 127.95 | 108    | 156.90 | 55     |        |        |
| 96.00  | 5316   | 128.90 | 67     | 158.95 | 131    |        |        |
| 97.05  | 140    | 129.85 | 280    | 171.80 | 74     |        |        |
| 103.80 | 69     | 130.80 | 50     | 172.00 | 108    |        |        |
| 103.95 | 191    | 134.90 | 103    | 172.80 | 93     |        |        |
| 105.85 | 281    | 136.90 | 57     | 173.10 | 431    |        |        |
| 115.90 | 232    | 140.90 | 356    | 174.00 | 55768  |        |        |
| 116.95 | 376    | 142.80 | 178    | 174.95 | 4025   |        |        |
| 117.85 | 235    | 142.95 | 337    | 175.95 | 54389  |        |        |
| 118.70 | 117    | 147.90 | 67     | 176.95 | 3729   |        |        |

Instrument :

MSVOA\_N

ClientSampleId :

BFB