


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN061119\  
Data File : VN056208.D  
Acq On : 11 Jun 2019 8:46  
Operator : JC/SP  
Sample : BFB  
Misc : 5.00mL/MSVOA N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N060419W.M  
Title : SW846 8260  
Last Update : Tue Jun 04 11:02:09 2019

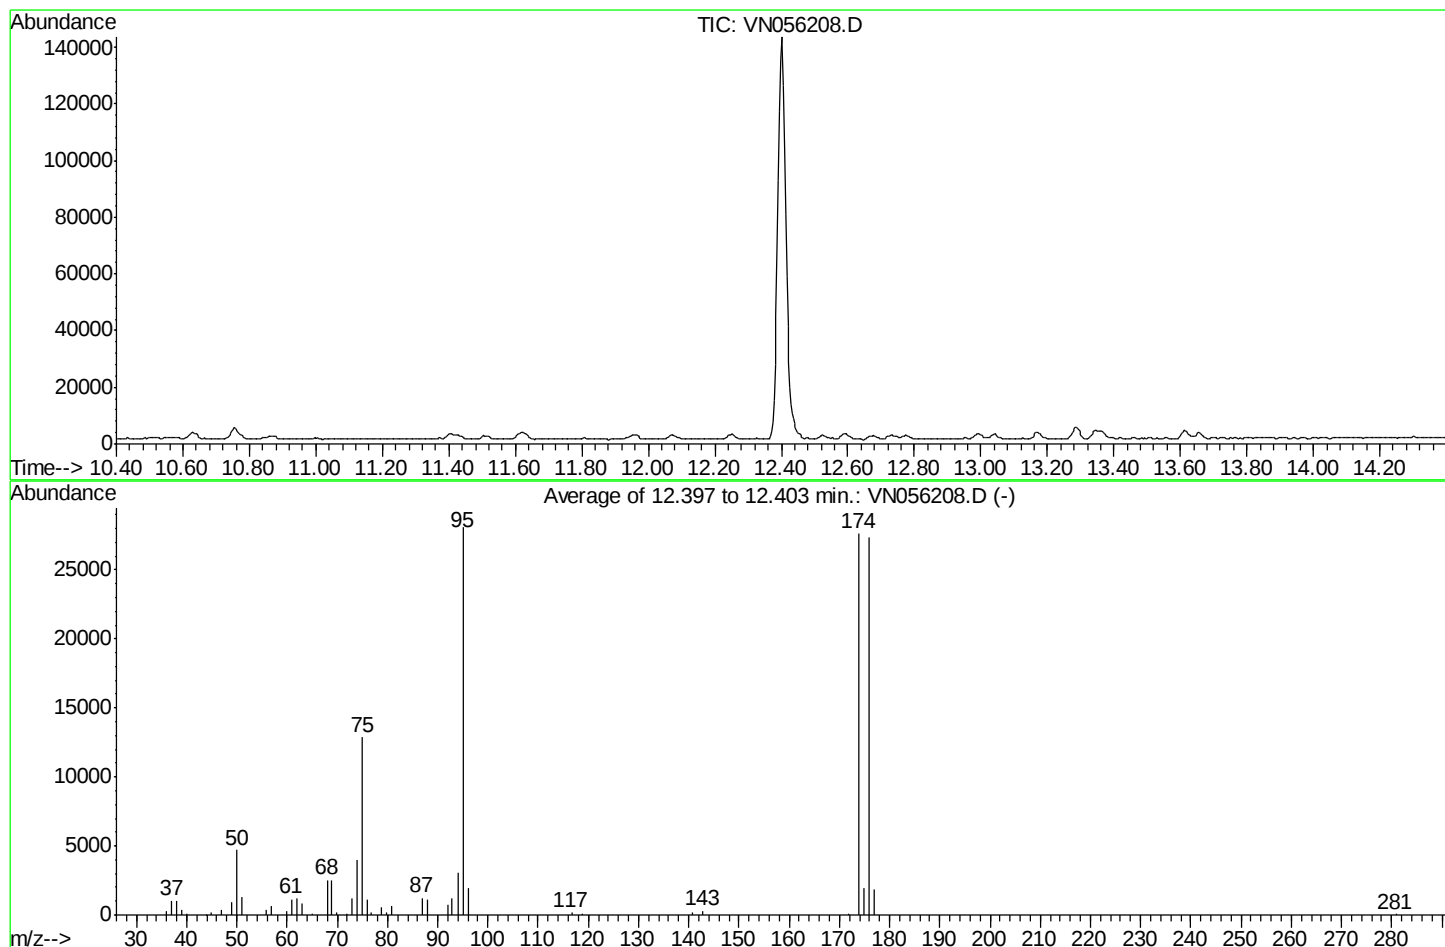

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 16.7      | 4687    | PASS             |
| 75          | 95           | 30           | 60           | 45.8      | 12849   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 28077   | PASS             |
| 96          | 95           | 5            | 9            | 6.8       | 1910    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 98.3      | 27608   | PASS             |
| 175         | 174          | 5            | 9            | 7.2       | 1988    | PASS             |
| 176         | 174          | 95           | 101          | 99.1      | 27370   | PASS             |
| 177         | 176          | 5            | 9            | 6.6       | 1817    | PASS             |