

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061121\
 Data File : VN067288.D
 Acq On : 11 Jun 2021 15:06
 Operator : JC/MD
 Sample : M2674-04 10X
 Misc : 5.27g/5mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TMR-DS-04-060921

Quant Time: Jun 12 04:26:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061021W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 11 05:27:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.086	168	403758	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.968	114	705677	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	669122	50.000	ug/l	# 0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	311089	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	346610	45.418	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	90.840%		
35) Dibromofluoromethane	8.021	113	224034	49.821	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	99.640%		
50) Toluene-d8	10.443	98	913302	51.681	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	103.360%		
62) 4-Bromofluorobenzene	12.733	95	395376	53.764	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	107.520%		
Target Compounds						
						Qvalue
13) Acrolein	4.041	56	564	1.082	ug/l #	17
16) Acetone	4.291	43	8722	2.830	ug/l #	86
18) Methyl Acetate	4.856	43	40046	4.669	ug/l #	69
20) Methylene Chloride	5.090	84	2929	0.530	ug/l #	90
25) 2-Butanone	7.356	43	6015	1.279	ug/l #	72
29) Tetrahydrofuran	7.694	42	613	0.231	ug/l #	59
31) Cyclohexane	8.086	56	11526	1.227	ug/l #	40
36) 1,1-Dichloropropene	8.083	75	40850	5.465	ug/l #	44
38) Carbon Tetrachloride	8.086	117	47551	6.101	ug/l #	15
40) Benzene	8.456	78	14164	0.663	ug/l	99
52) Toluene	10.507	92	142177	10.571	ug/l	98
58) 2-Chloroethyl Vinyl ether	10.038	63	264	28.184	ug/l #	45
59) 2-Hexanone	11.089	43	10595	1.589	ug/l	66
67) Ethyl Benzene	11.846	91	229331	8.218	ug/l	95
68) m/p-Xylenes	11.953	106	231534	23.048	ug/l	81
69) o-Xylene	12.283	106	124107	12.596	ug/l	82
70) Styrene	12.291	104	29143	1.767	ug/l #	16
73) Isopropylbenzene	12.581	105	28519	0.973	ug/l	94
76) 1,2,3-Trichloropropane	12.733	75	226645	27.425	ug/l #	100
78) n-propylbenzene	12.921	91	137024	4.006	ug/l	93
79) 2-Chlorotoluene	13.058	91	16596	0.790	ug/l #	39
80) 1,3,5-Trimethylbenzene	13.061	105	129332	5.167	ug/l	93
81) trans-1,4-Dichloro-2-b...	12.733	75	226645	70.156	ug/l #	16
82) 4-Chlorotoluene	12.983	91	34557	1.668	ug/l #	40
83) tert-Butylbenzene	13.562	119	29529	1.434	ug/l	75
84) 1,2,4-Trimethylbenzene	13.369	105	423800	17.286	ug/l	91
85) sec-Butylbenzene	13.503	105	12723	0.443	ug/l	90
86) p-Isopropyltoluene	13.613	119	61972	2.549	ug/l	89
89) n-Butylbenzene	13.943	91	91403	4.084	ug/l #	79
90) Hexachloroethane	14.214	117	15511	3.516	ug/l #	4
92) 1,2-Dibromo-3-Chloropr...	14.632	75	34527	16.413	ug/l #	1
95) Naphthalene	15.507	128	591816	36.183	ug/l	99
96) 1,2,3-Trichlorobenzene	15.697	180	1018	0.212	ug/l #	54

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

MSVOA_N


ClientSampleId :


TMR-DS-04-060921

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061121\
Data File : VN067288.D
Acq On : 11 Jun 2021 15:06
Operator : JC/MD
Sample : M2674-04 10X
Misc : 5.27g/5mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TMR-DS-04-060921


Quant Time: Jun 12 04:26:49 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061021W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 11 05:27:41 2021
Response via : Initial Calibration

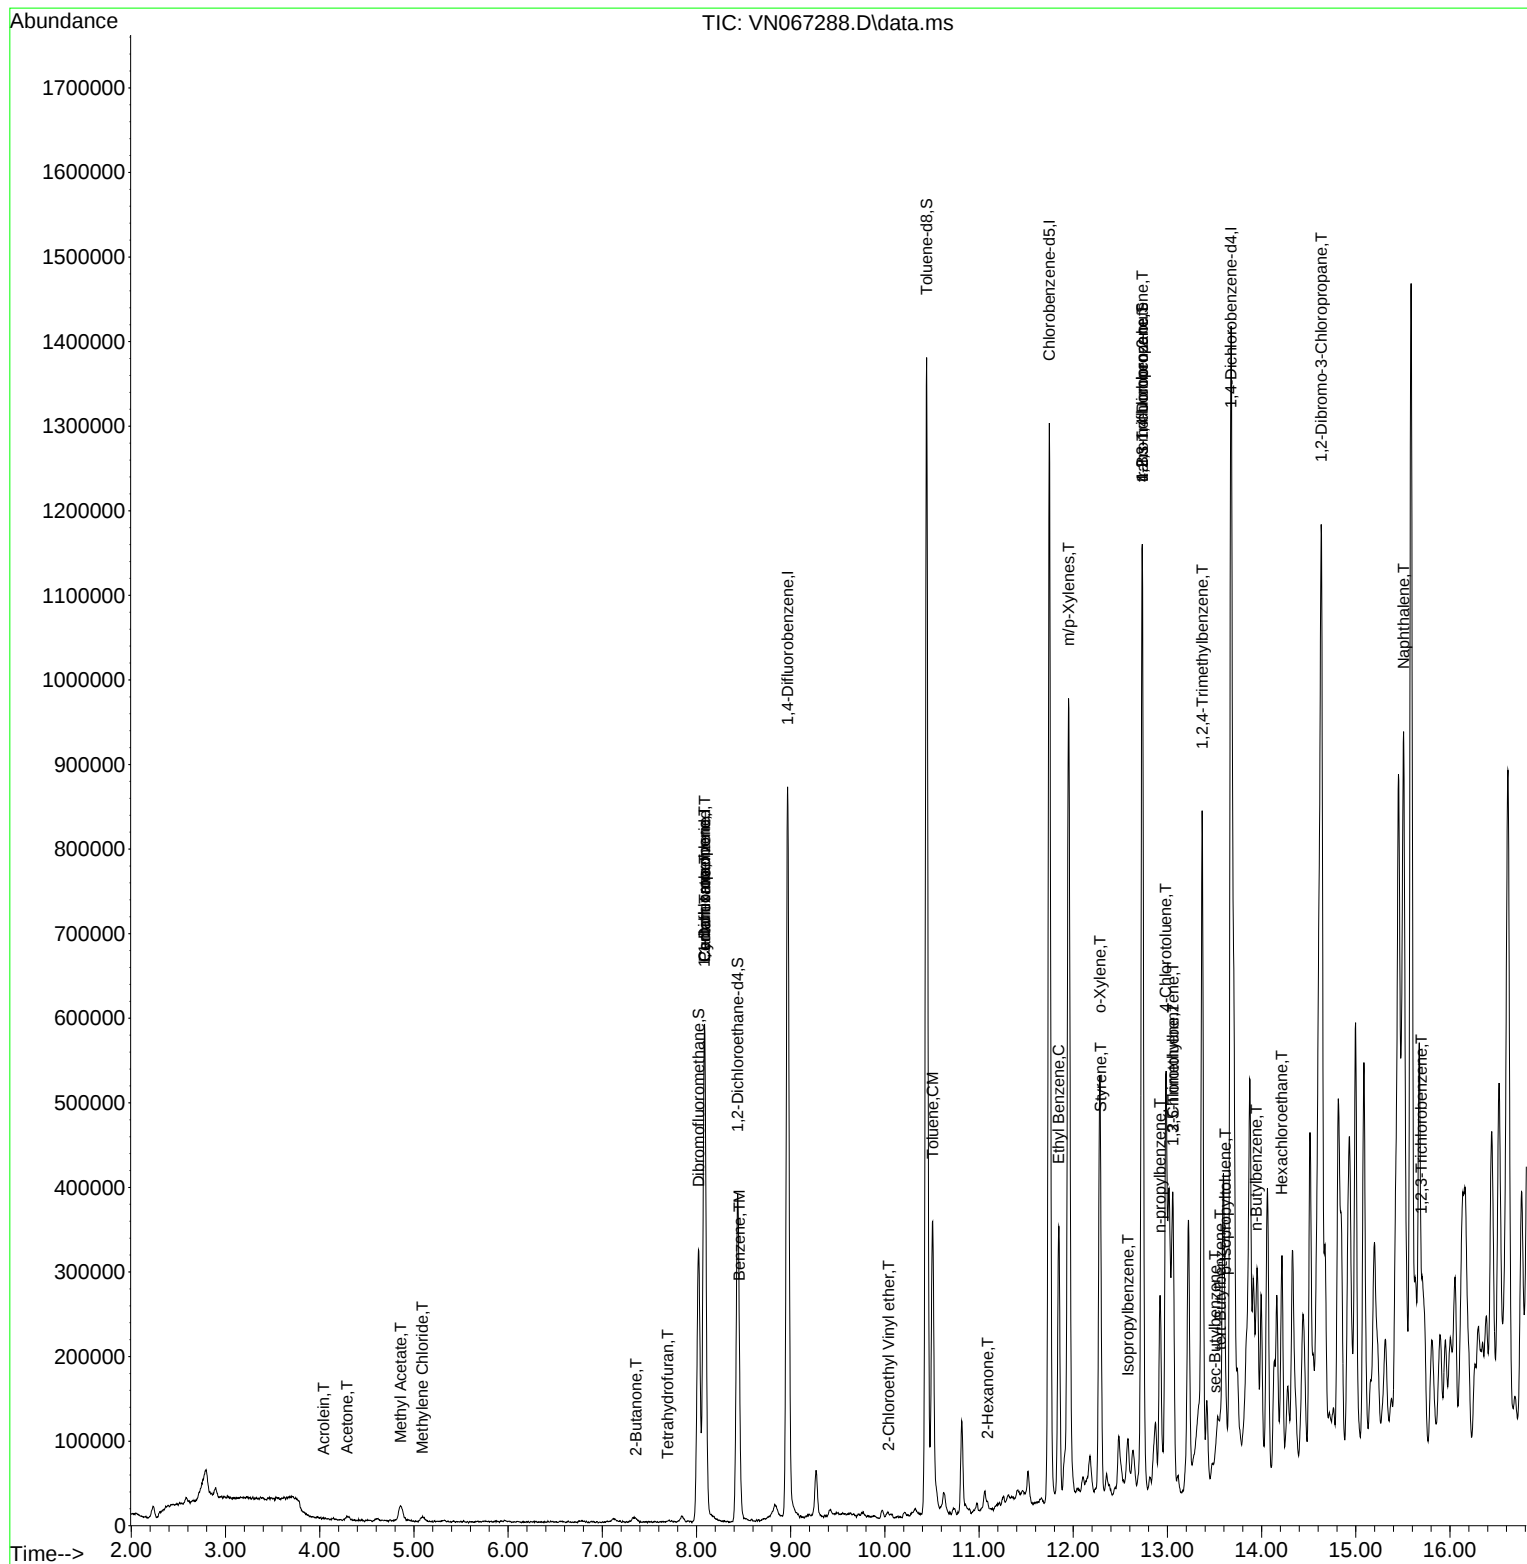






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.002 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06

Instrument :
MSVOA_N
ClientSampleId :
TMR-DS-04-060921







Tgt Ion:168 Resp: 403758
Ion Ratio Lower Upper
168 100
99 75.6 38.5 57.7#



#13
Acrolein
Concen: 1.082 ug/l
RT: 4.041 min Scan# 765
Delta R.T. 0.003 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06

Tgt Ion: 56 Resp: 564
Ion Ratio Lower Upper
56 100
55 133.5 53.8 80.6#


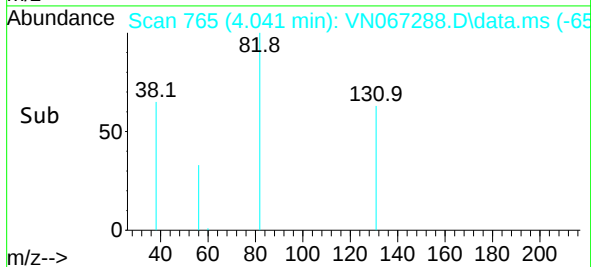

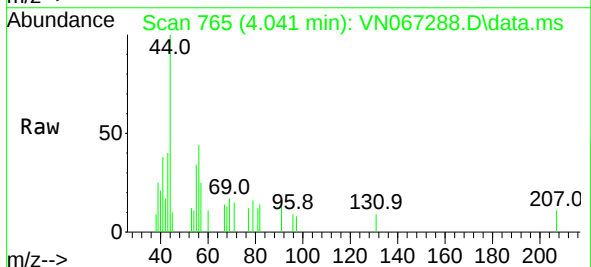




#16
Acetone
Concen: 2.830 ug/l
RT: 4.291 min Scan# 858
Delta R.T. -0.003 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampleId :
TMR-DS-04-060921


Tgt Ion: 43 Resp: 8722
Ion Ratio Lower Upper
43 100
58 26.1 27.2 40.8#



#18
Methyl Acetate
Concen: 4.669 ug/l
RT: 4.856 min Scan# 1069
Delta R.T. -0.003 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06

Tgt Ion: 43 Resp: 40046
Ion Ratio Lower Upper
43 100
74 10.6 21.4 32.2#









#20
Methylene Chloride
Concen: 0.530 ug/l
RT: 5.090 min Scan# 1156
Delta R.T. -0.008 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampleId :
TMR-DS-04-060921


Tgt Ion:	84	Resp:	2929
Ion	Ratio	Lower	Upper
84	100		
49	96.8	88.3	132.5
51	40.8	26.7	40.1#
86	60.2	51.1	76.7



#25
2-Butanone
Concen: 1.279 ug/l
RT: 7.356 min Scan# 2001
Delta R.T. 0.013 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06

Tgt Ion:	43	Resp:	6015
Ion	Ratio	Lower	Upper
43	100		
72	15.4	24.4	36.6#

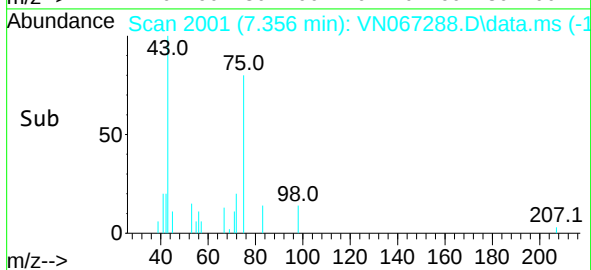



#29

Tetrahydrofuran

Concen: 0.231 ug/l

RT: 7.694 min Scan# 2127





Delta R.T. 0.003 min

Lab File: VN067288.D

Acq: 11 Jun 2021 15:06

Instrument :
MSVOA_N
ClientSampleId :
TMR-DS-04-060921

Tgt Ion:	42	Resp:	613
Ion	Ratio	Lower	Upper
42	100		
72	4.2	40.1	60.1#
71	37.8	37.9	56.9#

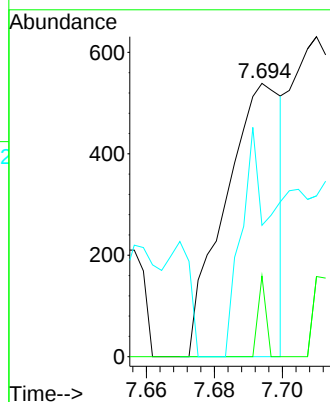

#31

Cyclohexane

Concen: 1.227 ug/l




RT: 8.086 min Scan# 2273


Delta R.T. -0.008 min

Lab File: VN067288.D

Acq: 11 Jun 2021 15:06

Tgt Ion:	56	Resp:	11526
Ion	Ratio	Lower	Upper
56	100		
69	158.0	28.0	42.0#
84	94.8	74.2	111.2

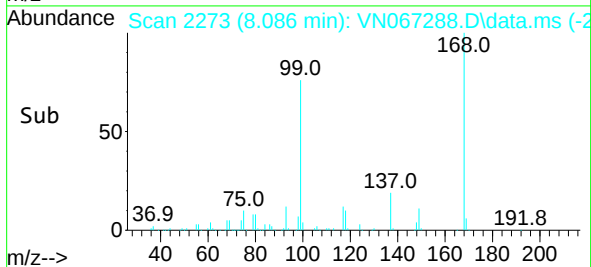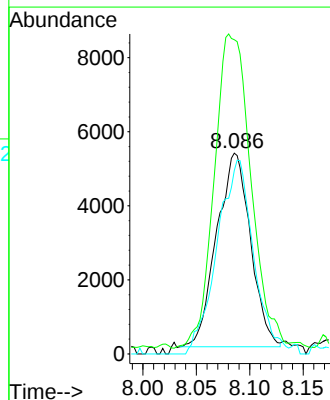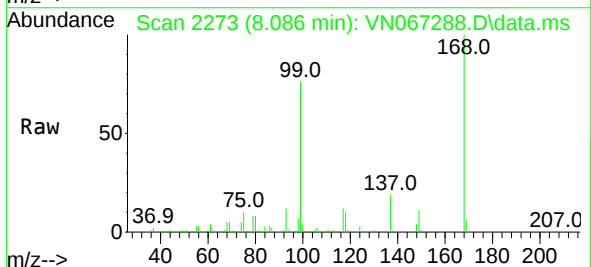







#33

1,2-Dichloroethane-d4
Concen: 45.418 ug/l
RT: 8.437 min Scan# 2404
Delta R.T. -0.000 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06

Instrument :
MSVOA_N
ClientSampleId :
TMR-DS-04-060921




Tgt Ion: 65 Resp: 346610
Ion Ratio Lower Upper
65 100
67 48.3 0.0 110.4




#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 2602
Delta R.T. -0.003 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06

Tgt Ion: 114 Resp: 705677
Ion Ratio Lower Upper
114 100
63 25.0 0.0 35.8
88 17.6 0.0 30.4


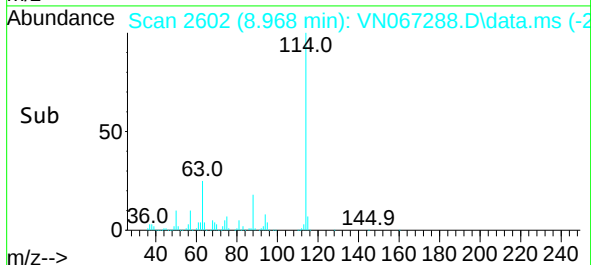

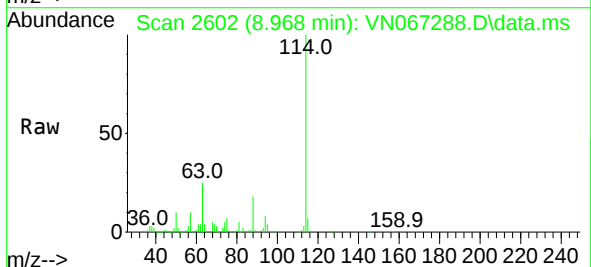




#35
Dibromofluoromethane
Concen: 49.821 ug/l
RT: 8.021 min Scan# 2249
Delta R.T. -0.003 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampleId :
TMR-DS-04-060921


Tgt Ion:113 Resp: 224034
Ion Ratio Lower Upper
113 100
111 106.6 82.6 124.0
192 17.2 18.2 27.4#

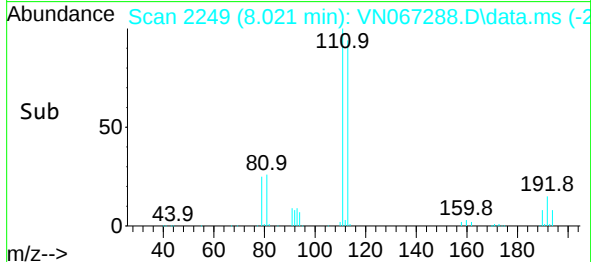

#36
1,1-Dichloropropene
Concen: 5.465 ug/l
RT: 8.083 min Scan# 2272
Delta R.T. -0.140 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06

Tgt Ion: 75 Resp: 40850
Ion Ratio Lower Upper
75 100
110 4.8 19.1 57.3#
77 0.0 24.8 37.2#

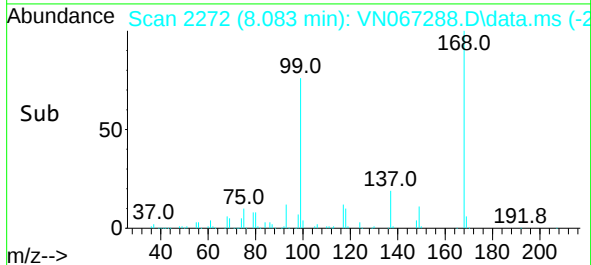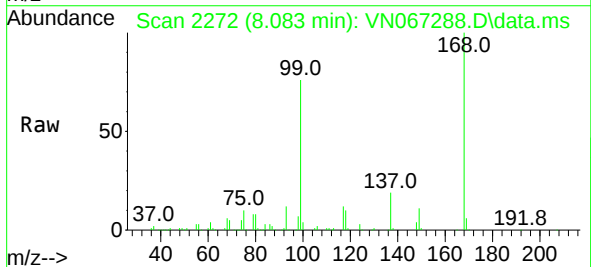



#38

Carbon Tetrachloride

Concen: 6.101 ug/l

RT: 8.086 min Scan# 2273

Delta R.T. -0.123 min

Lab File: VN067288.D


Acq: 11 Jun 2021 15:06

Instrument :




MSVOA_N

ClientSampleId :

TMR-DS-04-060921

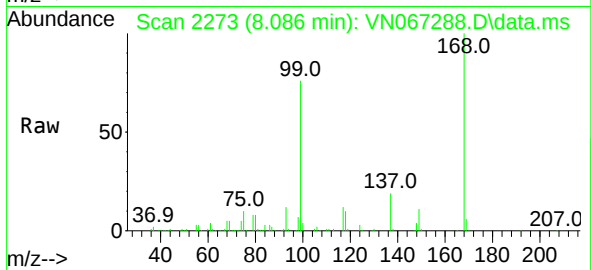

Tgt Ion:	117	Resp:	47551
Ion	Ratio	Lower	Upper
117	100		
119	4.7	78.2	117.2#
121	0.0	24.7	37.1#

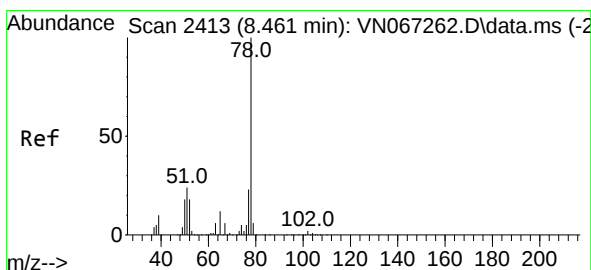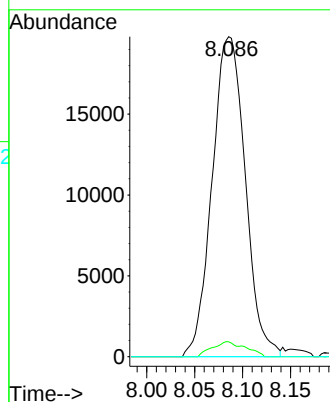

#40

Benzene

Concen: 0.663 ug/l




RT: 8.456 min Scan# 2411


Delta R.T. -0.005 min

Lab File: VN067288.D

Acq: 11 Jun 2021 15:06

Tgt Ion:	78	Resp:	14164
Ion	Ratio	Lower	Upper
78	100		
77	22.7	18.4	27.6



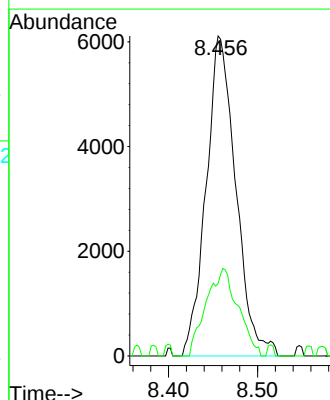
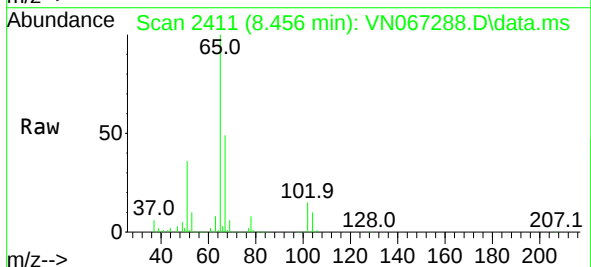


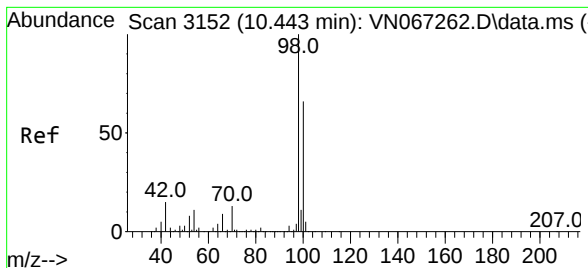

#50
Toluene-d8
Concen: 51.681 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. -0.000 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampleId :
TMR-DS-04-060921


Tgt Ion: 98 Resp: 913302
Ion Ratio Lower Upper
98 100
100 63.9 51.8 77.8

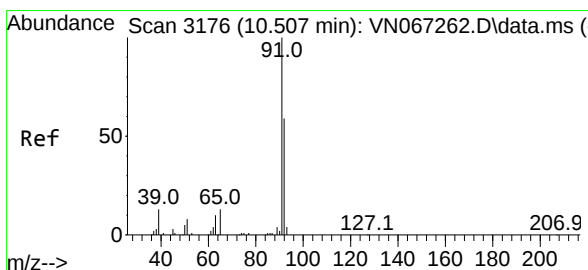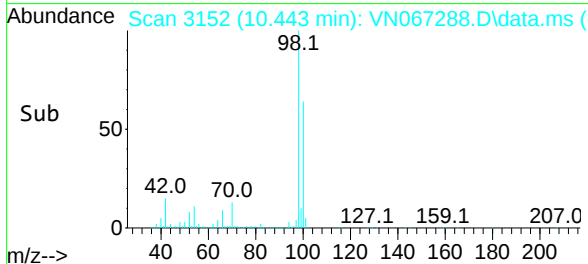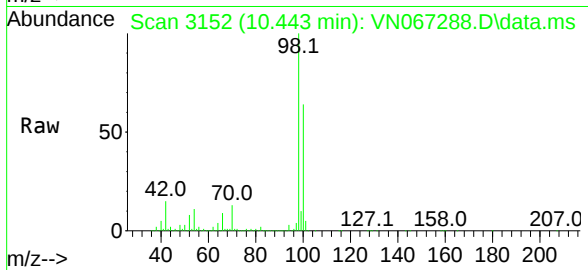

#52
Toluene
Concen: 10.571 ug/l
RT: 10.507 min Scan# 3176
Delta R.T. -0.000 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06

Tgt Ion: 92 Resp: 142177
Ion Ratio Lower Upper
92 100
91 176.7 138.7 208.1


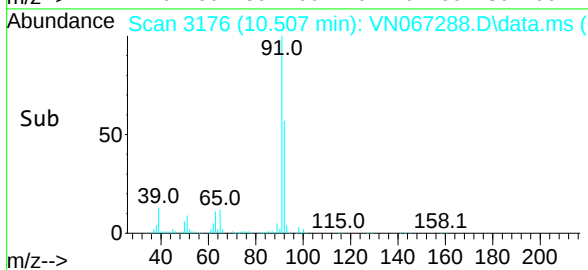

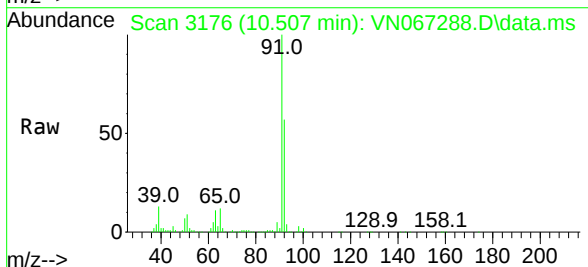




#58
2-Chloroethyl Vinyl ether
Concen: 28.184 ug/l
RT: 10.038 min Scan# 3001
Delta R.T. -0.005 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampleId :
TMR-DS-04-060921


Tgt Ion: 63 Resp: 264
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#

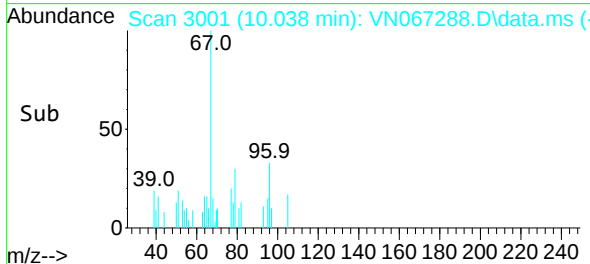

#59
2-Hexanone
Concen: 1.589 ug/l
RT: 11.089 min Scan# 3393
Delta R.T. -0.000 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06

Tgt Ion: 43 Resp: 10595
Ion Ratio Lower Upper
43 100
58 34.0 29.8 89.5


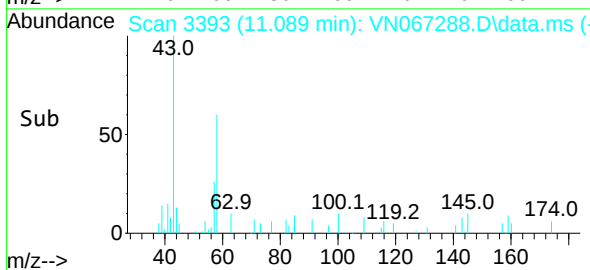

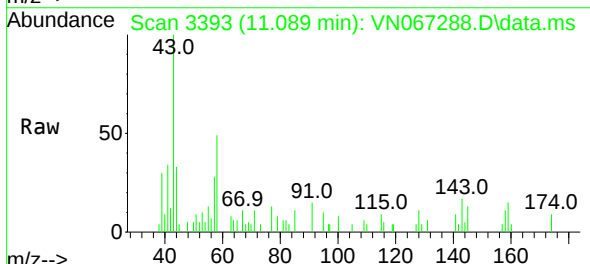




#62
4-Bromofluorobenzene
Concen: 53.764 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.000 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampleId :
TMR-DS-04-060921


Tgt Ion: 95 Resp: 395376
Ion Ratio Lower Upper
95 100
174 61.6 0.0 182.8
176 60.1 0.0 176.6

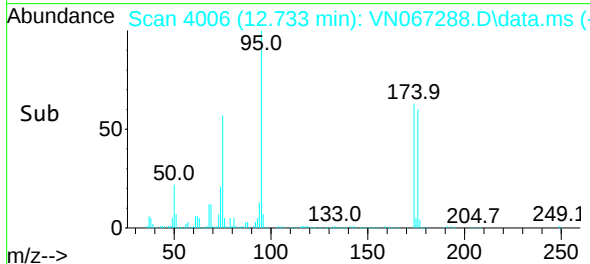

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. -0.000 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06

Tgt Ion: 117 Resp: 669122
Ion Ratio Lower Upper
117 100
82 64.2 42.2 63.2#
119 31.9 25.8 38.6


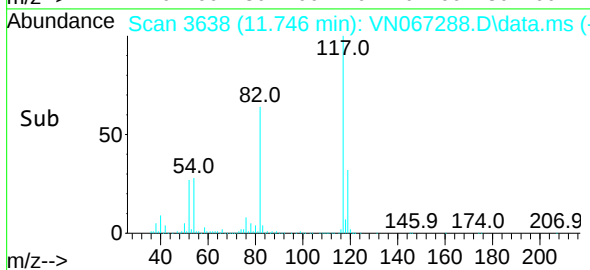

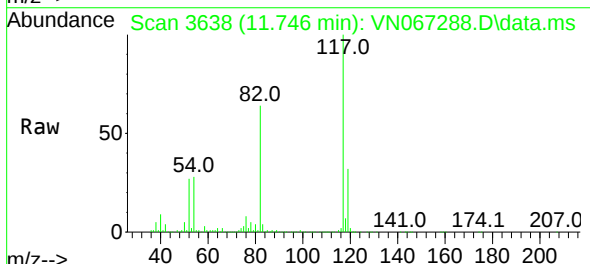


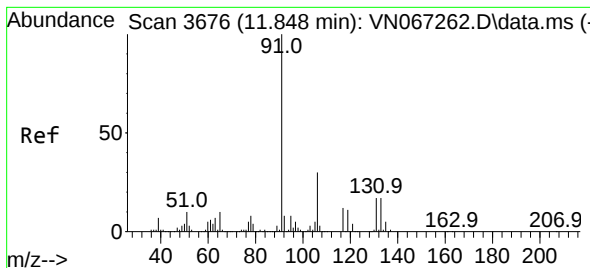

#67
Ethyl Benzene
Concen: 8.218 ug/l
RT: 11.846 min Scan# 3675
Delta R.T. -0.003 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampleId :
TMR-DS-04-060921


Tgt Ion: 91 Resp: 229331
Ion Ratio Lower Upper
91 100
106 30.0 26.2 39.2

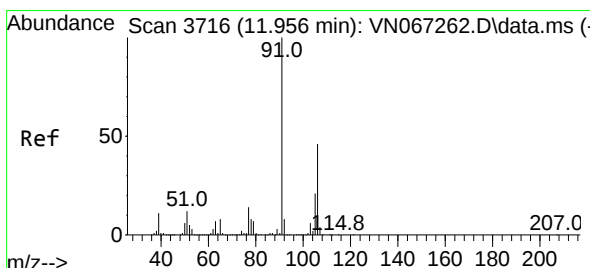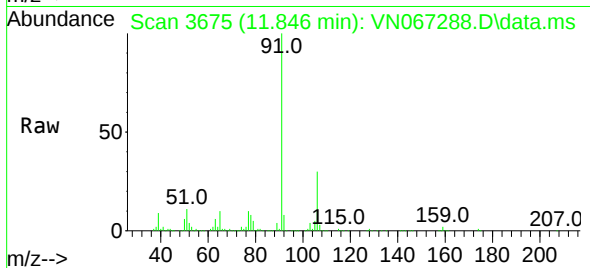

#68
m/p-Xylenes
Concen: 23.048 ug/l
RT: 11.953 min Scan# 3715
Delta R.T. -0.003 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06

Tgt Ion:106 Resp: 231534
Ion Ratio Lower Upper
106 100
91 222.0 155.2 232.8


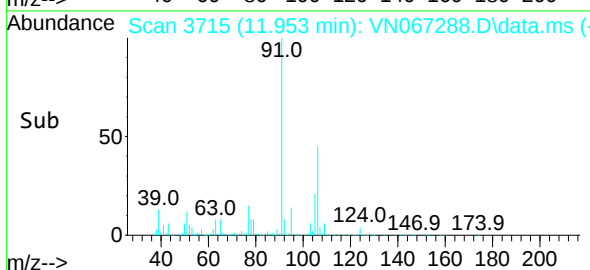




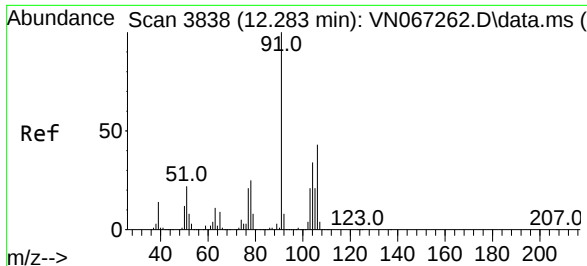

#69
o-Xylene
Concen: 12.596 ug/l
RT: 12.283 min Scan# 3838
Delta R.T. -0.000 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampleId :
TMR-DS-04-060921


Tgt Ion:106 Resp: 124107
Ion Ratio Lower Upper
106 100
91 231.9 102.3 306.8

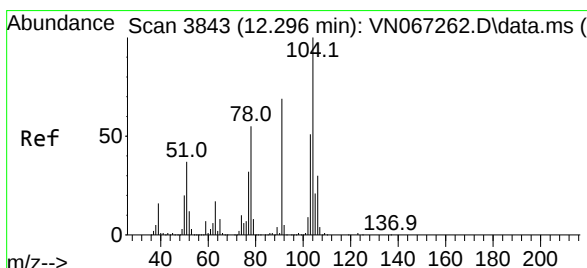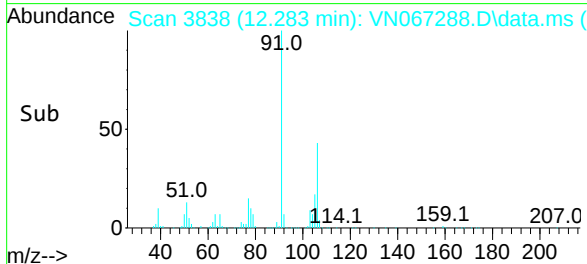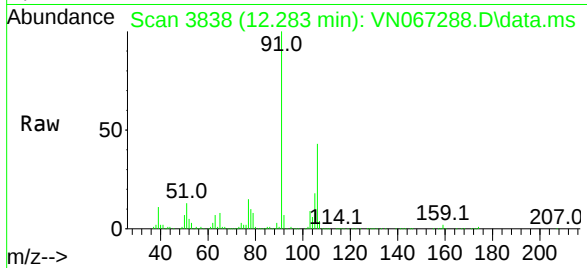

#70
Styrene
Concen: 1.767 ug/l
RT: 12.291 min Scan# 3841
Delta R.T. -0.005 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06

Tgt Ion:104 Resp: 29143
Ion Ratio Lower Upper
104 100
78 117.2 37.7 56.5#
103 103.9 44.2 66.4#


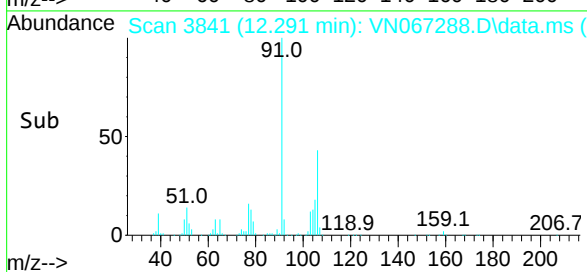

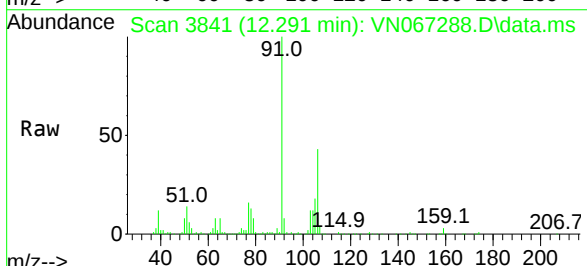




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. -0.003 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampleId :
TMR-DS-04-060921


Tgt Ion:152 Resp: 311089
Ion Ratio Lower Upper
152 100
115 74.9 27.0 80.8
150 154.3 0.0 350.2

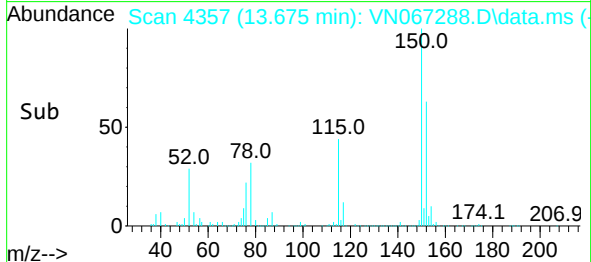

#73
Isopropylbenzene
Concen: 0.973 ug/l
RT: 12.581 min Scan# 3949
Delta R.T. -0.000 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06

Tgt Ion:105 Resp: 28519
Ion Ratio Lower Upper
105 100
120 24.2 13.7 41.0


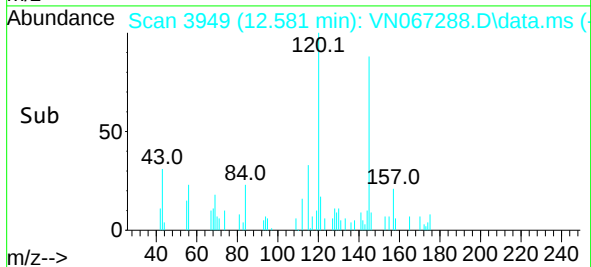

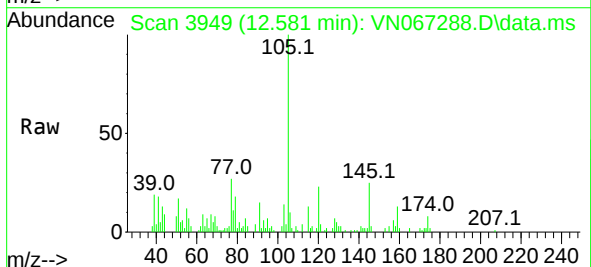




#76
1,2,3-Trichloropropane
Concen: 27.425 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.150 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampleId :
TMR-DS-04-060921


Tgt Ion: 75 Resp: 226645
Ion Ratio Lower Upper
75 100
77 1.6 0.0 0.0#

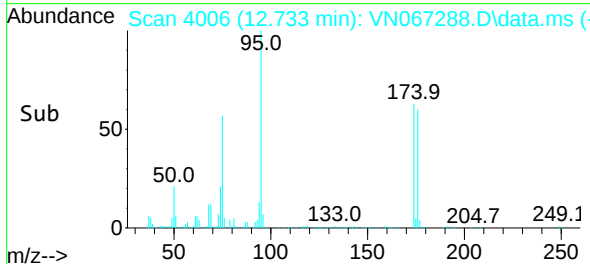

#78
n-propylbenzene
Concen: 4.006 ug/l
RT: 12.921 min Scan# 4076
Delta R.T. -0.000 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06

Tgt Ion: 91 Resp: 137024
Ion Ratio Lower Upper
91 100
120 22.0 12.7 38.0


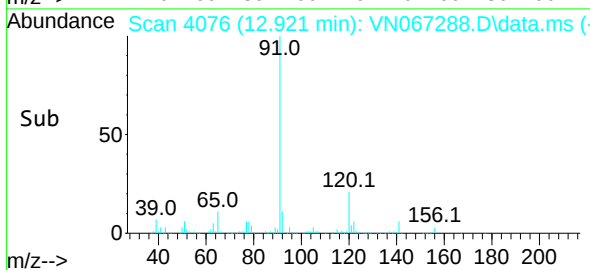

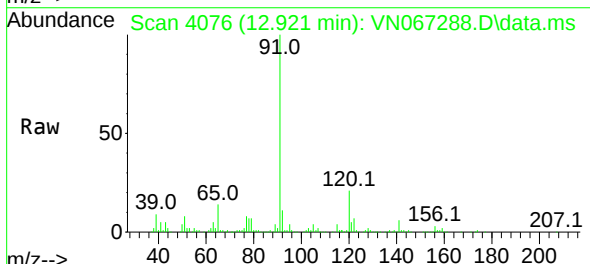




#79
2-Chlorotoluene
Concen: 0.790 ug/l
RT: 13.058 min Scan# 4127
Delta R.T. -0.048 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampleId :
TMR-DS-04-060921


Tgt Ion: 91 Resp: 16596
Ion Ratio Lower Upper
91 100
126 0.5 18.3 54.8#

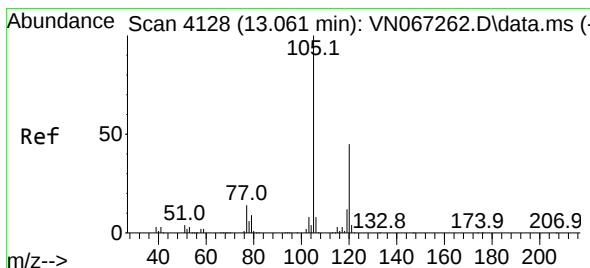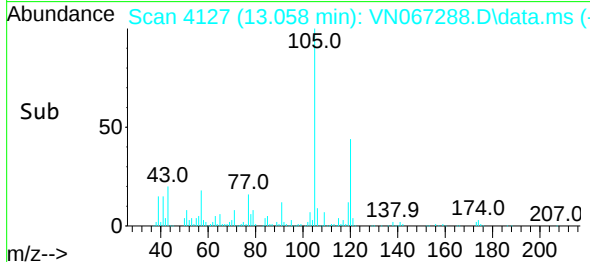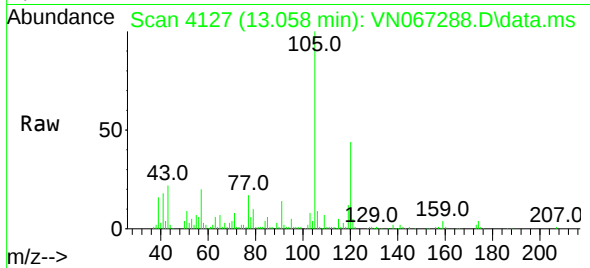

#80
1,3,5-Trimethylbenzene
Concen: 5.167 ug/l
RT: 13.061 min Scan# 4128
Delta R.T. -0.000 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06

Tgt Ion: 105 Resp: 129332
Ion Ratio Lower Upper
105 100
120 45.1 25.0 75.0


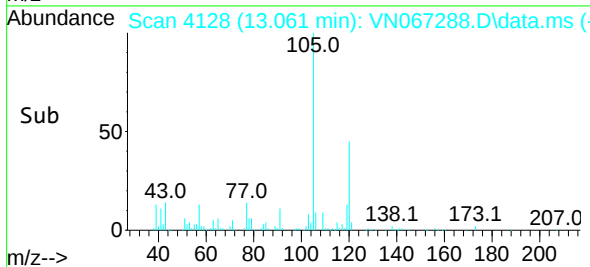

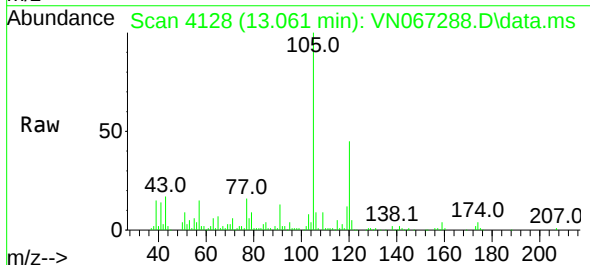




#81
trans-1,4-Dichloro-2-butene
Concen: 70.156 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.104 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampleId :
TMR-DS-04-060921


Tgt Ion: 75 Resp: 226645
Ion Ratio Lower Upper
75 100
53 0.2 66.3 99.5#
89 0.1 39.5 59.3#



#82
4-Chlorotoluene
Concen: 1.668 ug/l
RT: 12.983 min Scan# 4099
Delta R.T. -0.027 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06

Tgt Ion: 91 Resp: 34557
Ion Ratio Lower Upper
91 100
126 0.6 17.7 53.1#


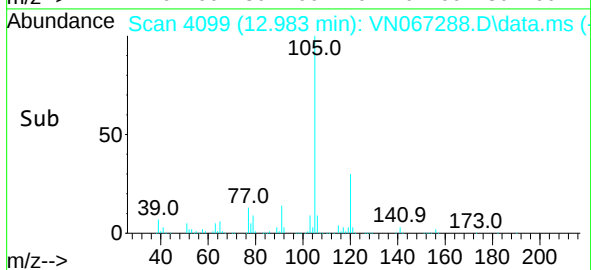

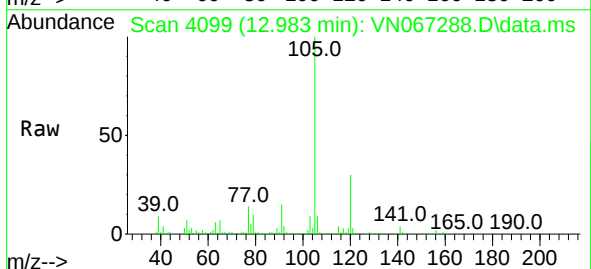




#83
tert-Butylbenzene
Concen: 1.434 ug/l
RT: 13.562 min Scan# 4315
Delta R.T. 0.236 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampleId :
TMR-DS-04-060921


Tgt Ion:119 Resp: 29529
Ion Ratio Lower Upper
119 100
91 34.3 30.2 90.6
134 23.8 13.0 39.0

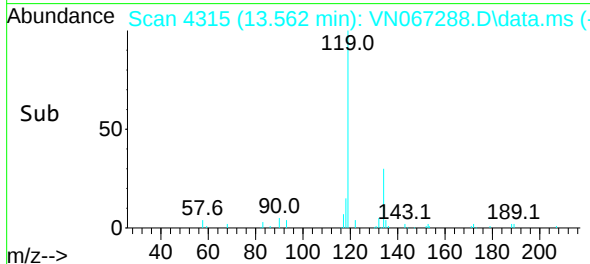

#84
1,2,4-Trimethylbenzene
Concen: 17.286 ug/l
RT: 13.369 min Scan# 4243
Delta R.T. -0.000 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06

Tgt Ion:105 Resp: 423800
Ion Ratio Lower Upper
105 100
120 41.2 23.8 71.2


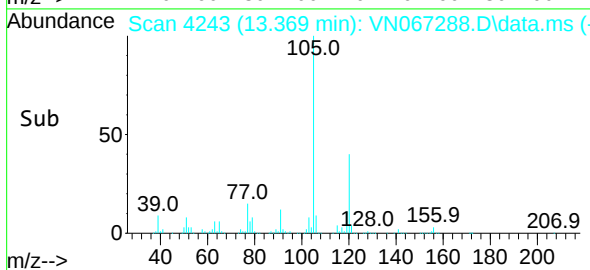

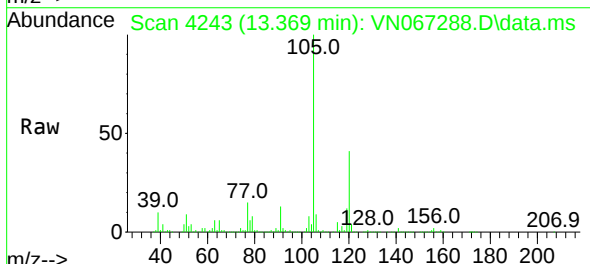




#85
 sec-Butylbenzene
 Concen: 0.443 ug/l
 RT: 13.503 min Scan# 4293
 Delta R.T. -0.000 min
 Lab File: VN067288.D
 Acq: 11 Jun 2021 15:06




Instrument :
 MSVOA_N
 ClientSampleId :
 TMR-DS-04-060921


Tgt Ion:105 Resp: 12723
 Ion Ratio Lower Upper
 105 100
 134 16.2 10.5 31.5



#86
 p-Isopropyltoluene
 Concen: 2.549 ug/l
 RT: 13.613 min Scan# 4334
 Delta R.T. -0.005 min
 Lab File: VN067288.D
 Acq: 11 Jun 2021 15:06

Tgt Ion:119 Resp: 61972
 Ion Ratio Lower Upper
 119 100
 134 18.9 13.3 39.9
 91 18.9 10.7 32.1


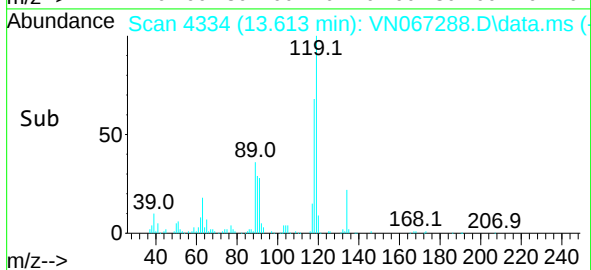






#89
n-Butylbenzene
Concen: 4.084 ug/l
RT: 13.943 min Scan# 4457
Delta R.T. -0.000 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06




Instrument :
MSVOA_N
ClientSampleId :
TMR-DS-04-060921


Tgt Ion:	91	Resp:	91403
Ion	Ratio	Lower	Upper
91	100		
92	50.6	26.5	79.5
134	0.0	14.3	42.9#

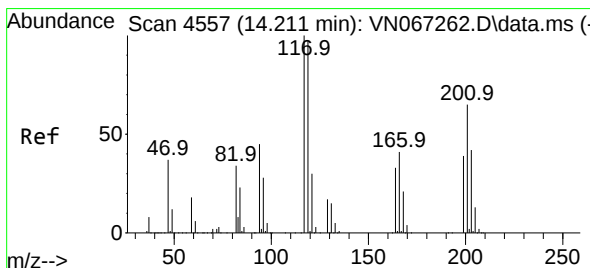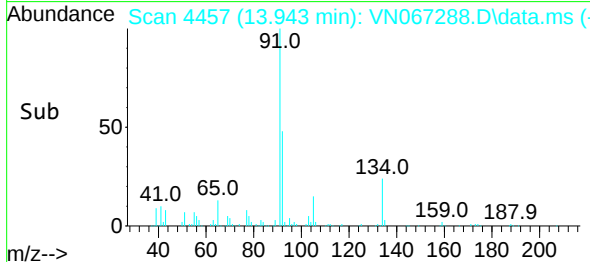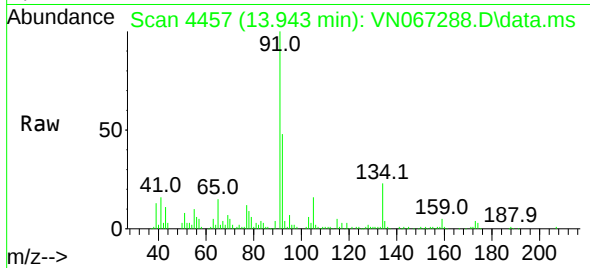

#90
Hexachloroethane
Concen: 3.516 ug/l
RT: 14.214 min Scan# 4558
Delta R.T. 0.003 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06


Tgt Ion:	117	Resp:	15511
Ion	Ratio	Lower	Upper
117	100		
201	0.0	45.5	136.5#

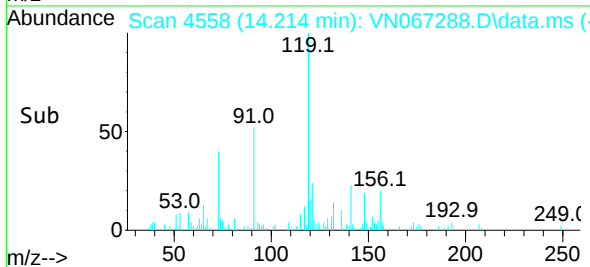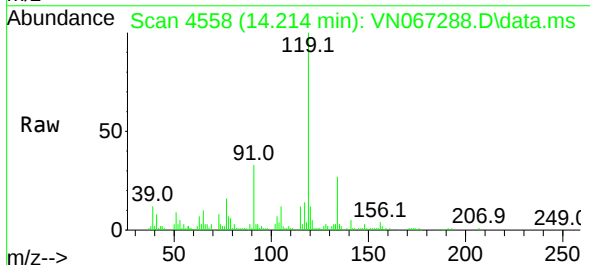



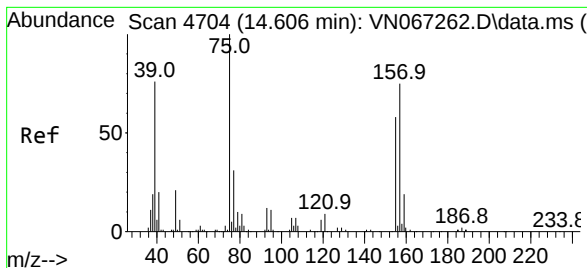


#92
1,2-Dibromo-3-Chloropropane
Concen: 16.413 ug/l
RT: 14.632 min Scan# 4714
Delta R.T. 0.027 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06

Instrument :
MSVOA_N
ClientSampleId :
TMR-DS-04-060921



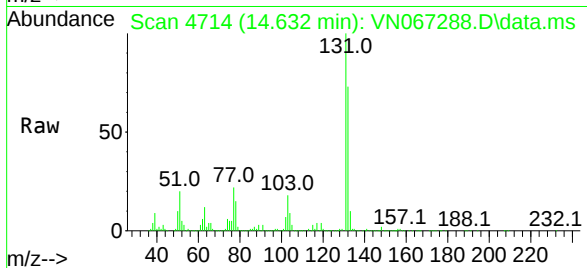



Tgt Ion: 75 Resp: 34527
Ion Ratio Lower Upper
75 100
155 1.3 49.9 149.7#
157 4.4 63.8 191.4#

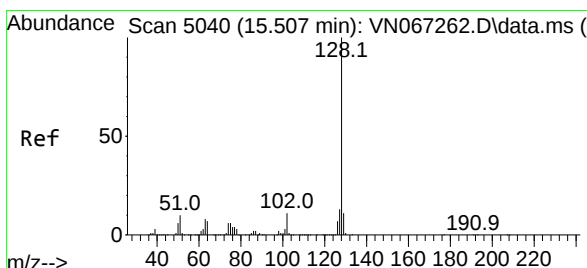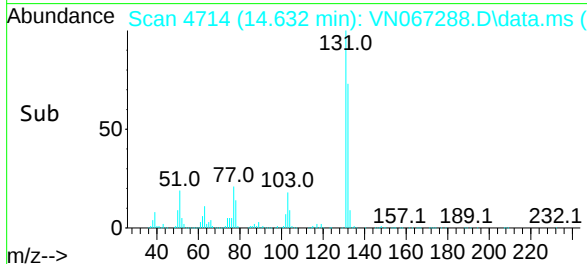

#95
Naphthalene
Concen: 36.183 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. -0.000 min
Lab File: VN067288.D
Acq: 11 Jun 2021 15:06


Tgt Ion: 128 Resp: 591816
Ion Ratio Lower Upper
128 100
127 13.4 10.2 15.2
129 11.2 8.6 13.0

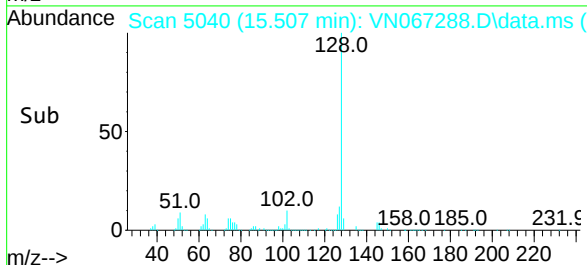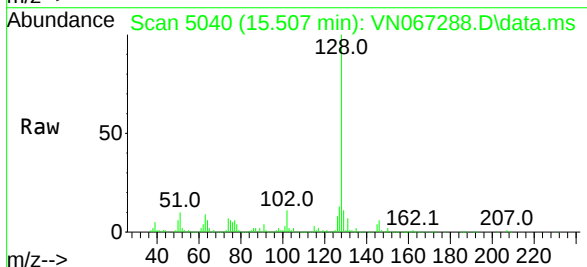

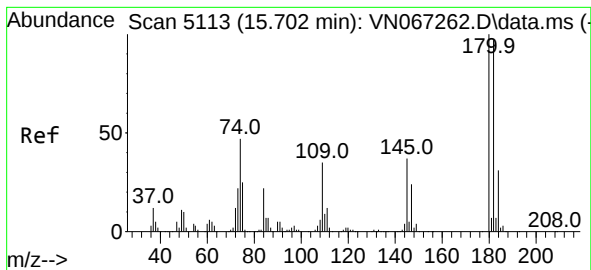

#96
 1,2,3-Trichlorobenzene
 Concen: 0.212 ug/l
 RT: 15.697 min Scan# 5111
 Delta R.T. -0.005 min
 Lab File: VN067288.D
 Acq: 11 Jun 2021 15:06

Instrument :
 MSVOA_N
 ClientSampleId :
 TMR-DS-04-060921

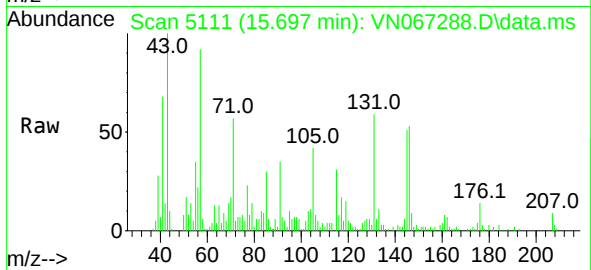

Tgt Ion:180 Resp: 1018
 Ion Ratio Lower Upper
 180 100
 182 55.2 48.5 145.6
 145 0.0 15.4 46.2#

