

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061121\
 Data File : VN067312.D
 Acq On : 12 Jun 2021 3:13
 Operator : JC/MD
 Sample : M2699-01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 001-WILLETS-PT-BLVD(JUNE)

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N061121W.M

Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VN067312.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.236	78	92	108	rBV3	15337	30353	2.08%	0.475%
2	7.662	2093	2115	2142	rBV2	207478	534412	36.68%	8.363%
3	8.440	2386	2405	2428	rBV	236347	542741	37.25%	8.493%
4	8.971	2585	2603	2626	rBV	490240	1023224	70.22%	16.012%
5	10.336	3098	3112	3128	rBV4	24304	48146	3.30%	0.753%
6	10.443	3133	3152	3173	rBV	773231	1457151	100.00%	22.803%
7	11.186	3419	3429	3441	rVB6	14316	25885	1.78%	0.405%
8	11.296	3461	3470	3477	rBV8	11207	18203	1.25%	0.285%
9	11.403	3495	3510	3511	rBV8	9528	16022	1.10%	0.251%
10	11.529	3541	3557	3566	rVB8	9518	20461	1.40%	0.320%
11	11.639	3581	3598	3610	rBV7	18239	34462	2.37%	0.539%
12	11.746	3622	3638	3658	rBV	677279	1239940	85.09%	19.404%
13	11.996	3721	3731	3747	rVB3	23360	43868	3.01%	0.686%
14	12.733	3990	4006	4028	rVB	515132	918053	63.00%	14.366%
15	13.270	4194	4206	4222	rVB2	47338	79903	5.48%	1.250%
16	13.342	4222	4233	4252	rVB3	24270	50296	3.45%	0.787%
17	13.468	4256	4280	4305	rVB5	64416	178047	12.22%	2.786%
18	13.616	4317	4335	4345	rBV2	41850	71307	4.89%	1.116%
19	13.675	4345	4357	4364	rBV5	32140	57811	3.97%	0.905%


Sum of corrected areas: 6390285

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061121\
Data File : VN067312.D
Acq On : 12 Jun 2021 3:13
Operator : JC/MD
Sample : M2699-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(JUNE)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N061121W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

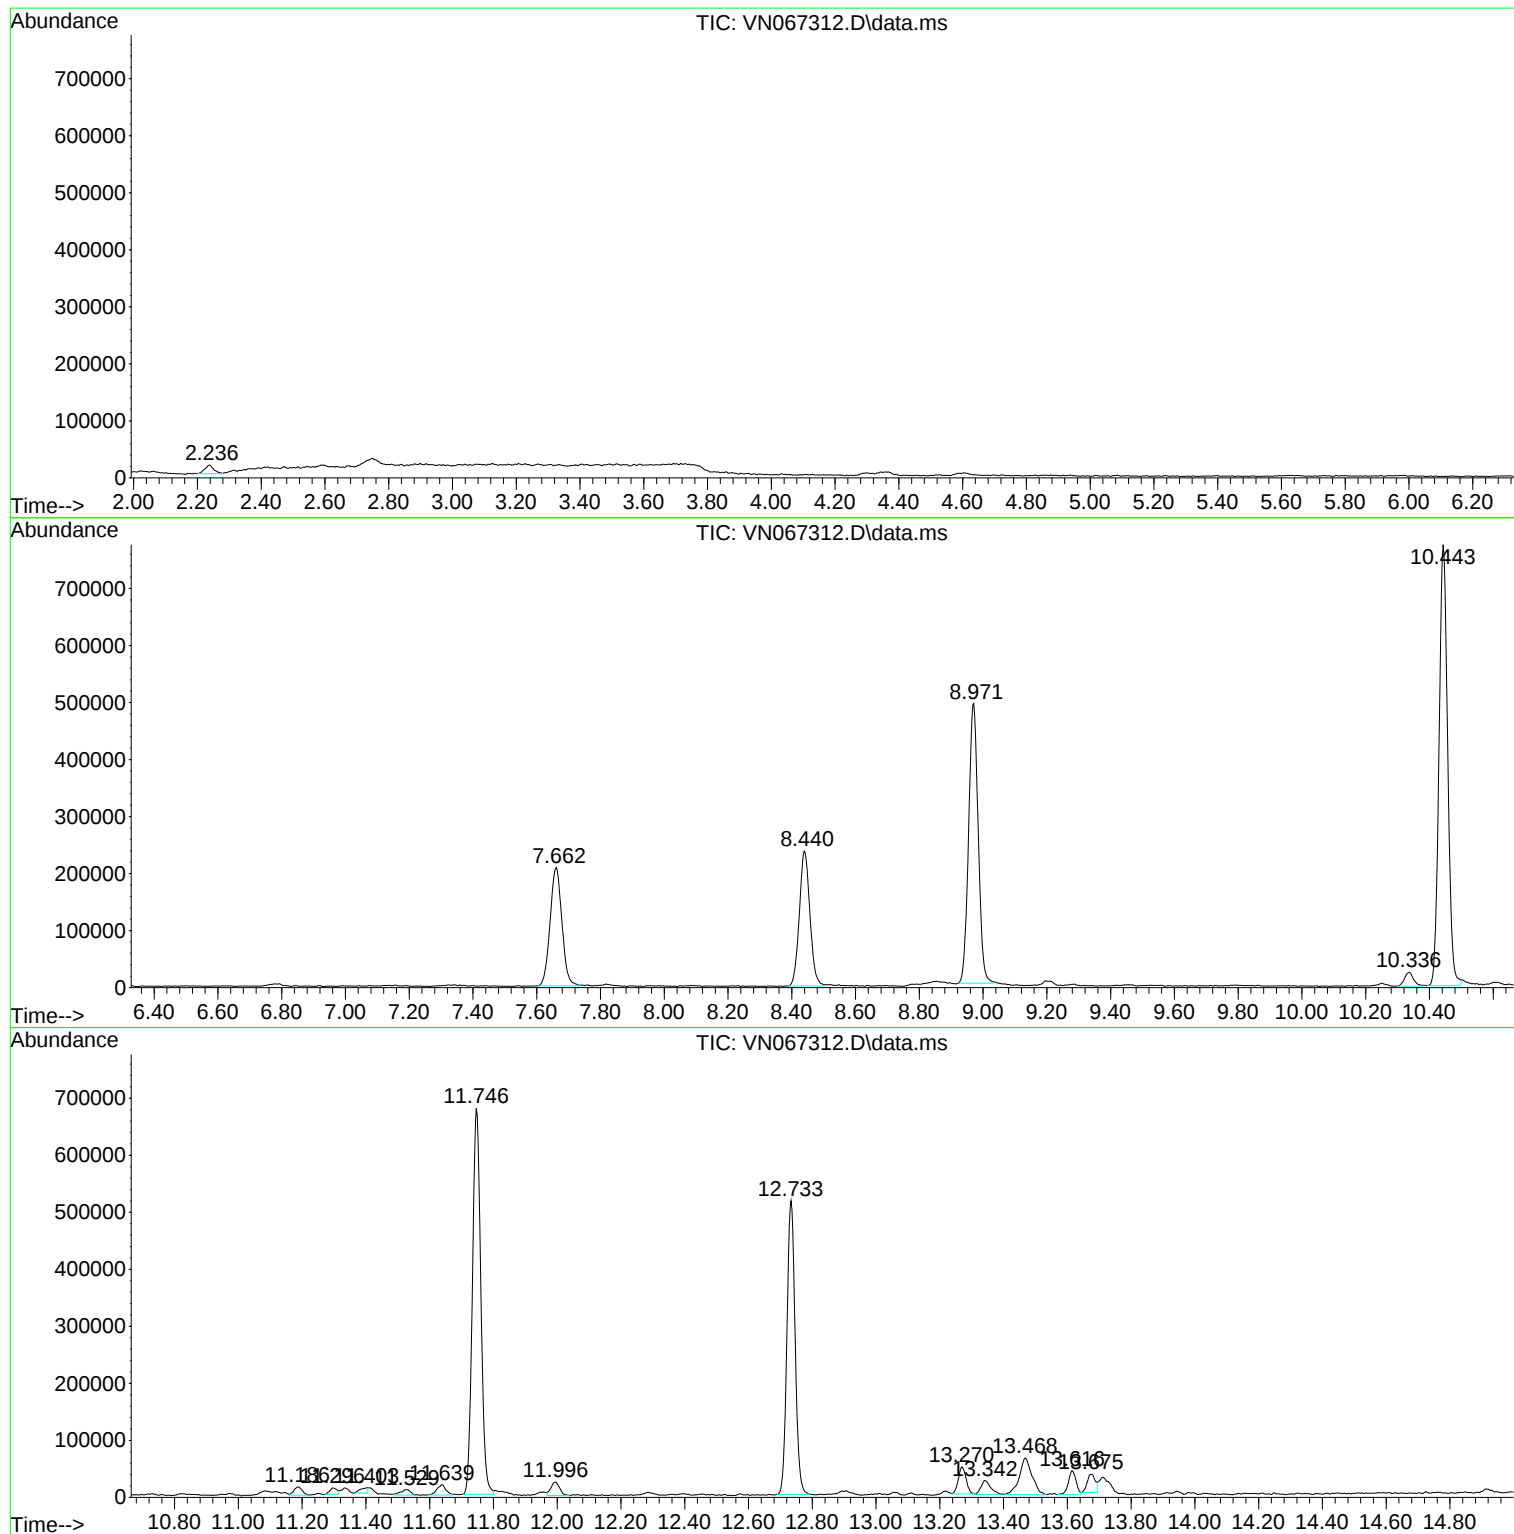

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061121\
Data File : VN067312.D
Acq On : 12 Jun 2021 3:13
Operator : JC/MD
Sample : M2699-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(JUNE)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N061121W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061121\
Data File : VN067312.D
Acq On : 12 Jun 2021 3:13
Operator : JC/MD
Sample : M2699-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(JUNE)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N061121W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
