

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061121\
 Data File : VN067315.D
 Acq On : 12 Jun 2021 4:25
 Operator : JC/MD
 Sample : M2703-01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 210609018-02-VOA

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N061121W.M

Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VN067315.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.738	268	279	292	rBV	198419	303090	2.56%	0.789%
2	3.706	632	640	671	rVB	88789	177100	1.50%	0.461%
3	4.291	836	858	880	rBV	424186	1241117	10.50%	3.233%
4	5.385	1237	1266	1321	rVB2	1959023	6940645	58.70%	18.079%
5	7.329	1963	1991	2056	rBV2	3984485	11823613	100.00%	30.798%
6	7.689	2095	2125	2158	rBV5	1084990	3373613	28.53%	8.787%
7	8.442	2383	2406	2423	rBV4	267459	737568	6.24%	1.921%
8	8.528	2424	2438	2462	rVB6	190246	539453	4.56%	1.405%
9	8.968	2584	2602	2633	rVB	496565	1045725	8.84%	2.724%
10	10.443	3136	3152	3166	rBV	790738	1492614	12.62%	3.888%
11	10.508	3167	3176	3183	rBV	92423	145630	1.23%	0.379%
12	11.060	3360	3382	3404	rVV	308233	587695	4.97%	1.531%
13	11.666	3593	3608	3620	rVV7	49553	149160	1.26%	0.389%
14	11.747	3621	3638	3659	rVV	710494	1423814	12.04%	3.709%
15	11.846	3660	3675	3694	rVV2	270608	575224	4.87%	1.498%
16	11.950	3694	3714	3742	rVB3	194767	477916	4.04%	1.245%
17	12.280	3824	3837	3851	rBV2	165145	296786	2.51%	0.773%
18	12.578	3935	3948	3962	rVB5	68308	129576	1.10%	0.338%
19	12.731	3993	4005	4026	rVB	577421	1029778	8.71%	2.682%
20	13.066	4118	4130	4148	rVB8	71318	184827	1.56%	0.481%
21	13.367	4218	4242	4260	rBV3	107459	253420	2.14%	0.660%
22	13.495	4273	4290	4304	rBV4	139956	271712	2.30%	0.708%
23	13.699	4355	4366	4374	rBV6	108861	206211	1.74%	0.537%
24	13.742	4374	4382	4383	rVV2	143284	160684	1.36%	0.419%
25	13.772	4385	4393	4411	rVB	461427	781998	6.61%	2.037%
26	13.879	4423	4433	4455	rVB	84808	162869	1.38%	0.424%
27	14.144	4519	4532	4542	rBV3	133812	252044	2.13%	0.657%
28	14.203	4545	4554	4566	rVB	195504	332467	2.81%	0.866%
29	14.560	4668	4687	4703	rBV	1557048	2750571	23.26%	7.165%
30	14.812	4760	4781	4805	rBV	70106	259443	2.19%	0.676%
31	14.911	4809	4818	4833	rVB4	63889	118248	1.00%	0.308%
32	14.984	4834	4845	4847	rBV2	140749	166843	1.41%	0.435%




Sum of corrected areas: 38391454

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061121\
Data File : VN067315.D
Acq On : 12 Jun 2021 4:25
Operator : JC/MD
Sample : M2703-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
210609018-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N061121W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

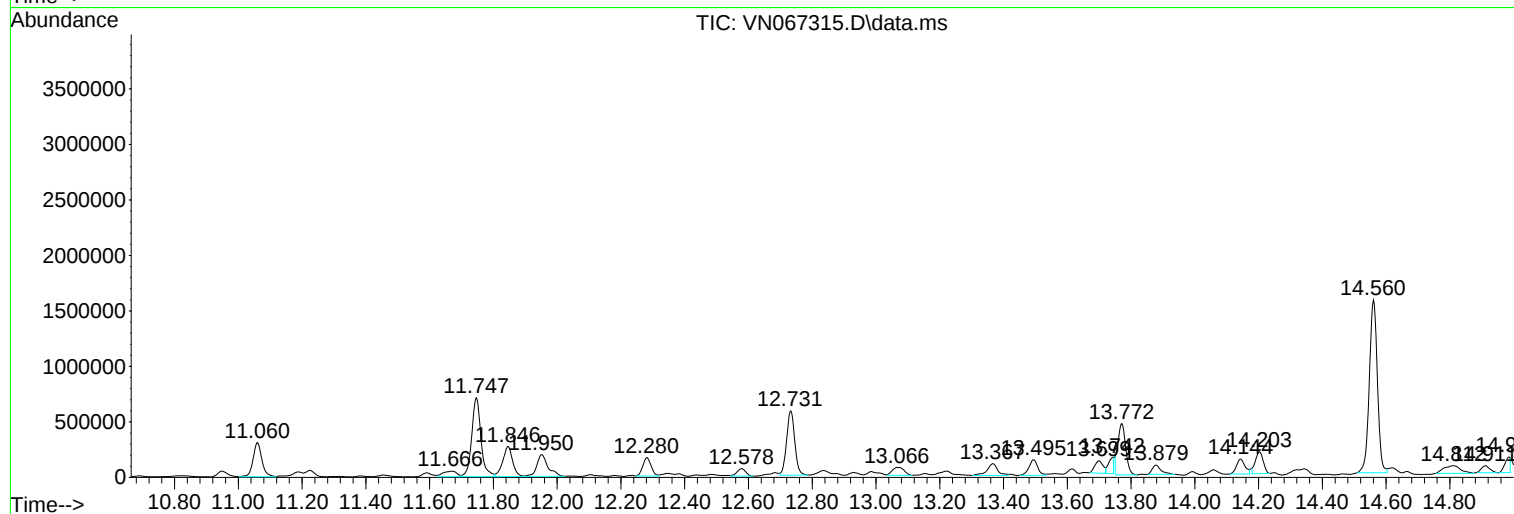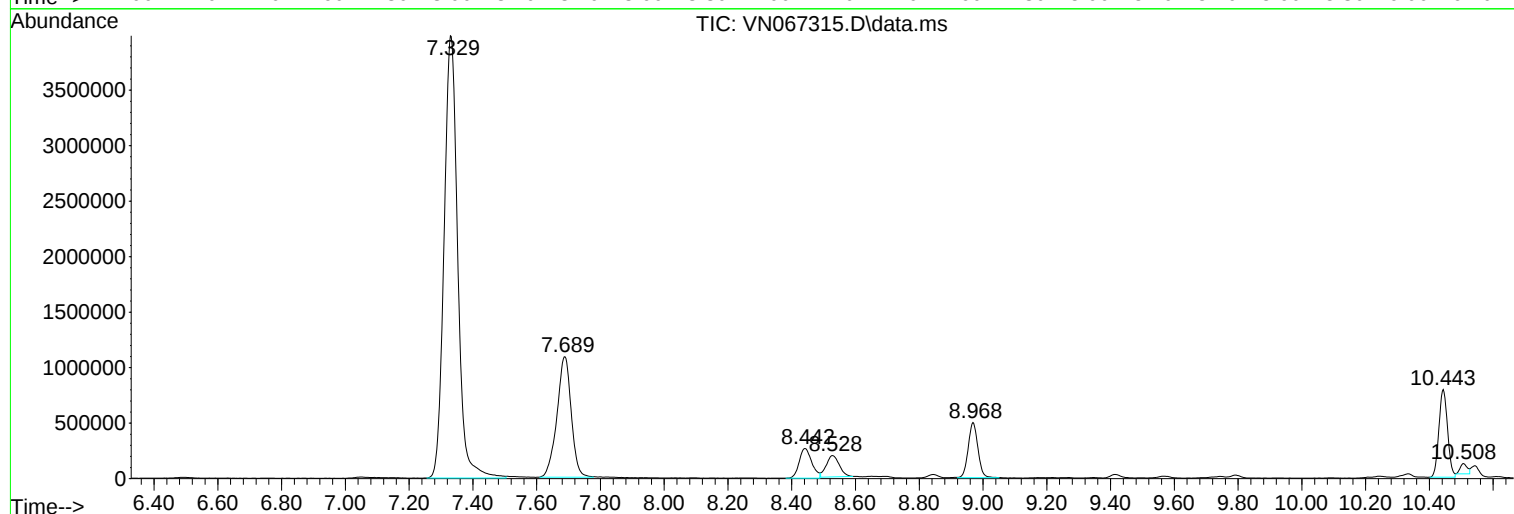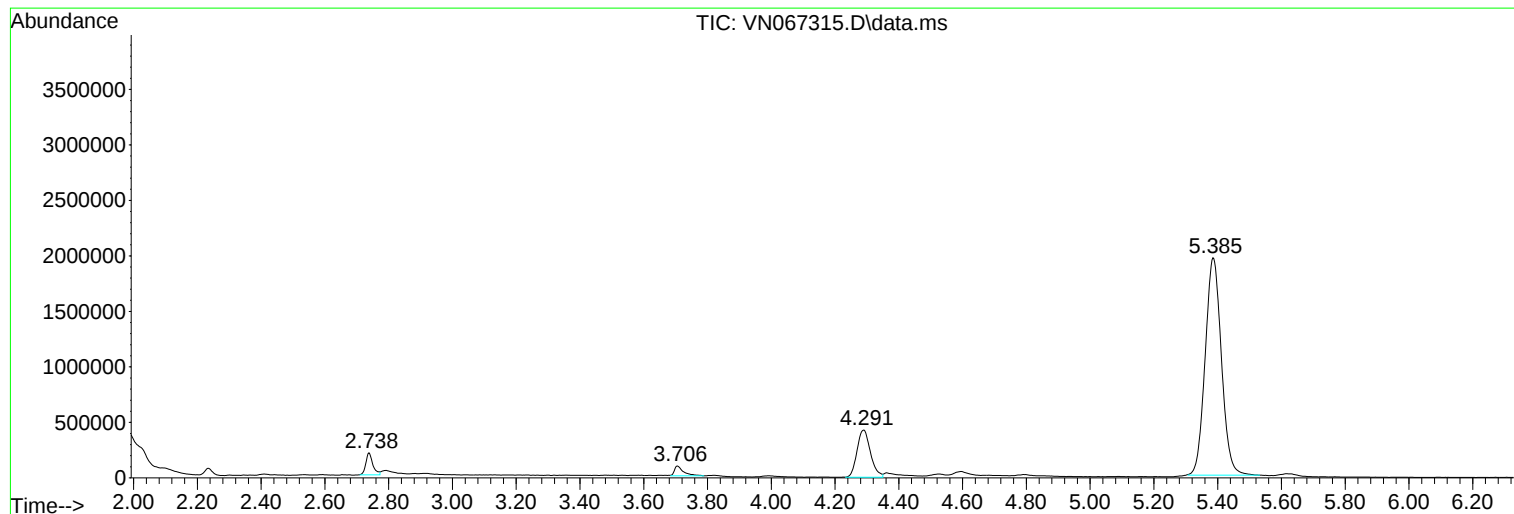

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061121\
Data File : VN067315.D
Acq On : 12 Jun 2021 4:25
Operator : JC/MD
Sample : M2703-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
210609018-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N061121W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061121\
Data File : VN067315.D
Acq On : 12 Jun 2021 4:25
Operator : JC/MD
Sample : M2703-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
210609018-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N061121W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
