
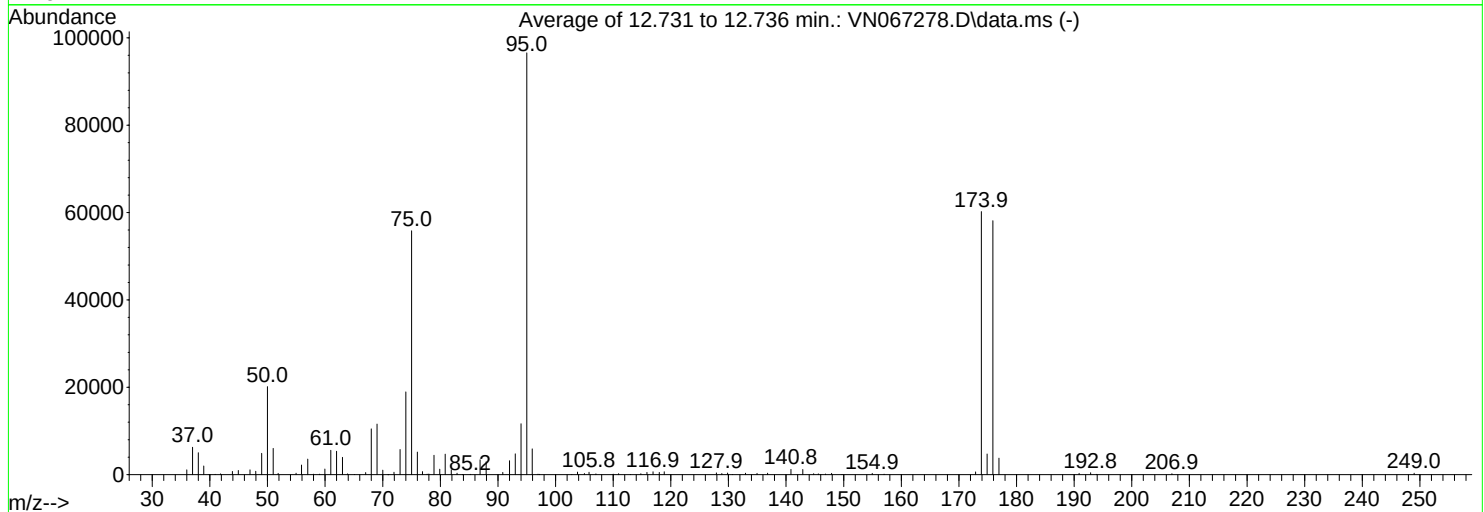


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061121\
Data File : VN067278.D
Acq On : 11 Jun 2021 9:35
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061021W.M
Title : SW846 8260
Last Update : Fri Jun 11 05:27:41 2021

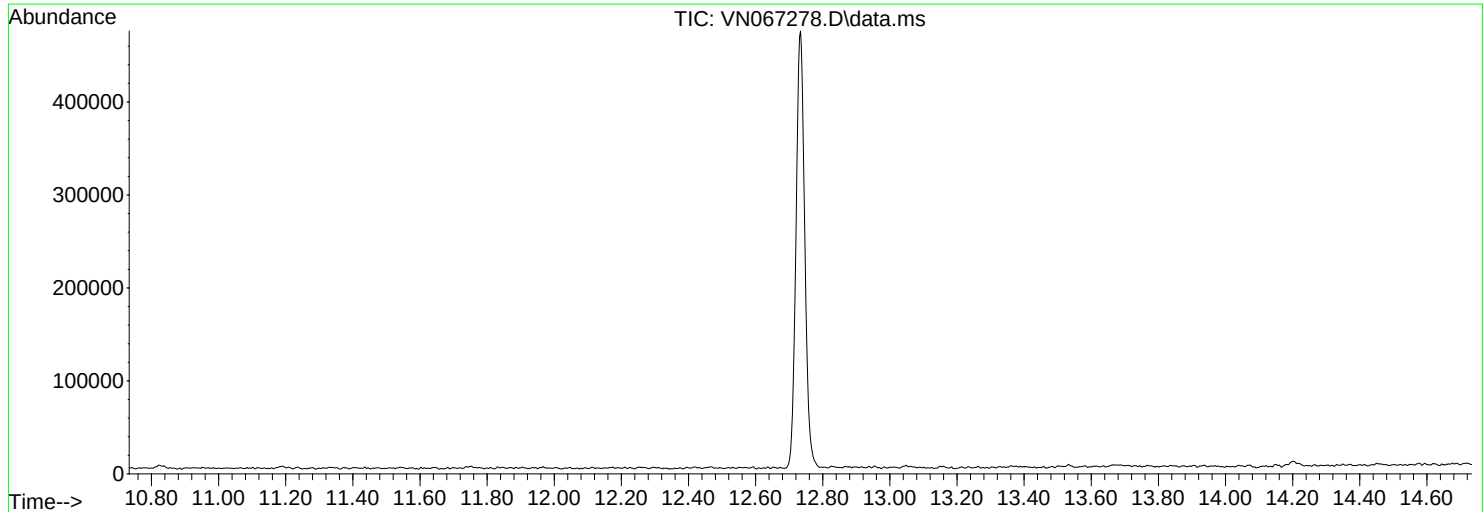

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3987

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	20141	PASS
75	95	30	60	57.8	55819	PASS
95	95	100	100	100.0	96568	PASS
96	95	5	9	6.1	5908	PASS
173	174	0.00	2	1.0	620	PASS
174	95	50	100	62.4	60213	PASS
175	174	5	9	7.8	4721	PASS
176	174	95	101	96.6	58139	PASS
177	176	5	9	6.5	3759	PASS