
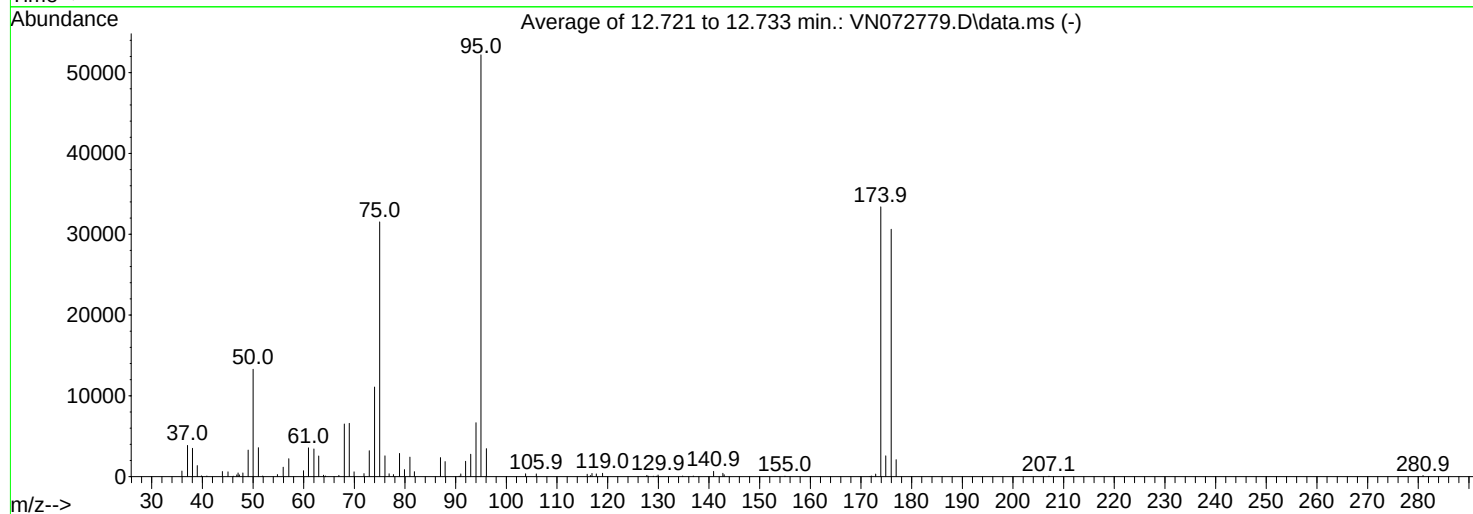


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061122\
 Data File : VN072779.D
 Acq On : 11 Jun 2022 10:10
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N060622W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Mon Jun 06 14:10:15 2022

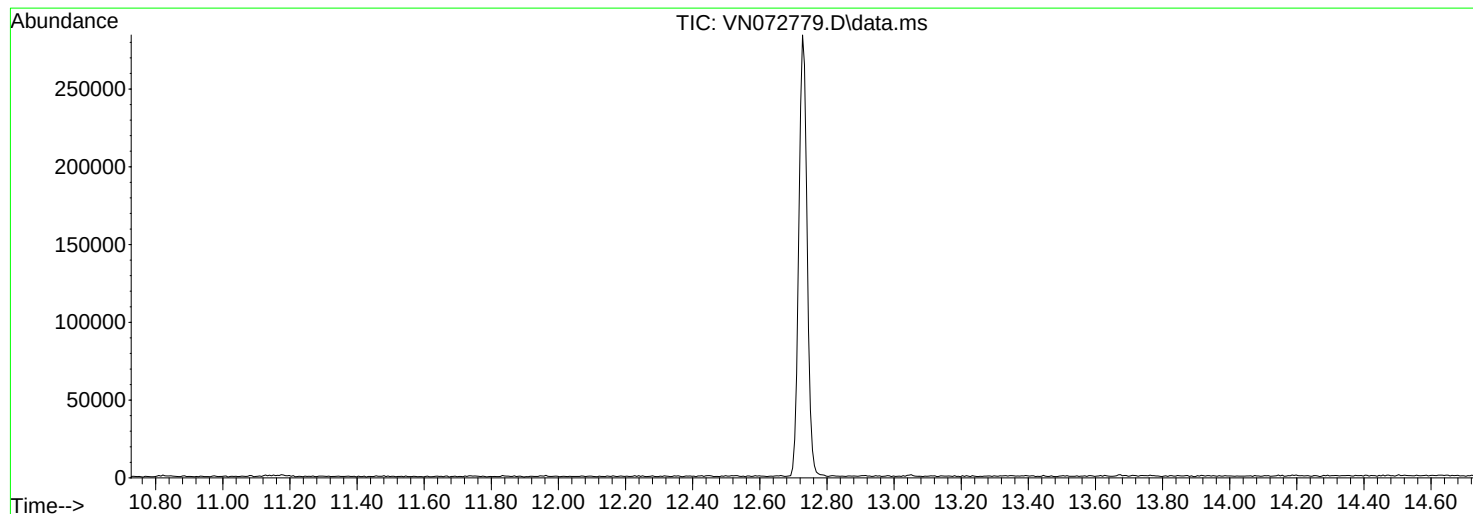

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1818

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.4	13280	PASS
75	95	30	60	60.4	31523	FAIL*
95	95	100	100	100.0	52203	PASS
96	95	5	9	6.6	3462	PASS
173	174	0.00	2	1.0	325	PASS
174	95	50	100	64.0	33387	PASS
175	174	5	9	7.7	2573	PASS
176	174	95	101	91.7	30619	FAIL*
177	176	5	9	6.9	2105	PASS