

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061125\
 Data File : VN086949.D
 Acq On : 11 Jun 2025 15:28
 Operator : JC\MD
 Sample : Q2202-06
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TB-20250603

Quant Time: Jun 12 01:34:20 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 07 02:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	324235	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	611383	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	538730	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	263158	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	212072	48.852	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	97.700%
35) Dibromofluoromethane	8.177	113	178799	49.348	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.700%
50) Toluene-d8	10.571	98	743447	51.832	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	103.660%
62) 4-Bromofluorobenzene	12.847	95	264799	49.691	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	99.380%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061125\
Data File : VN086949.D
Acq On : 11 Jun 2025 15:28
Operator : JC\MD
Sample : Q2202-06
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TB-20250603

Quant Time: Jun 12 01:34:20 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 07 02:12:50 2025
Response via : Initial Calibration




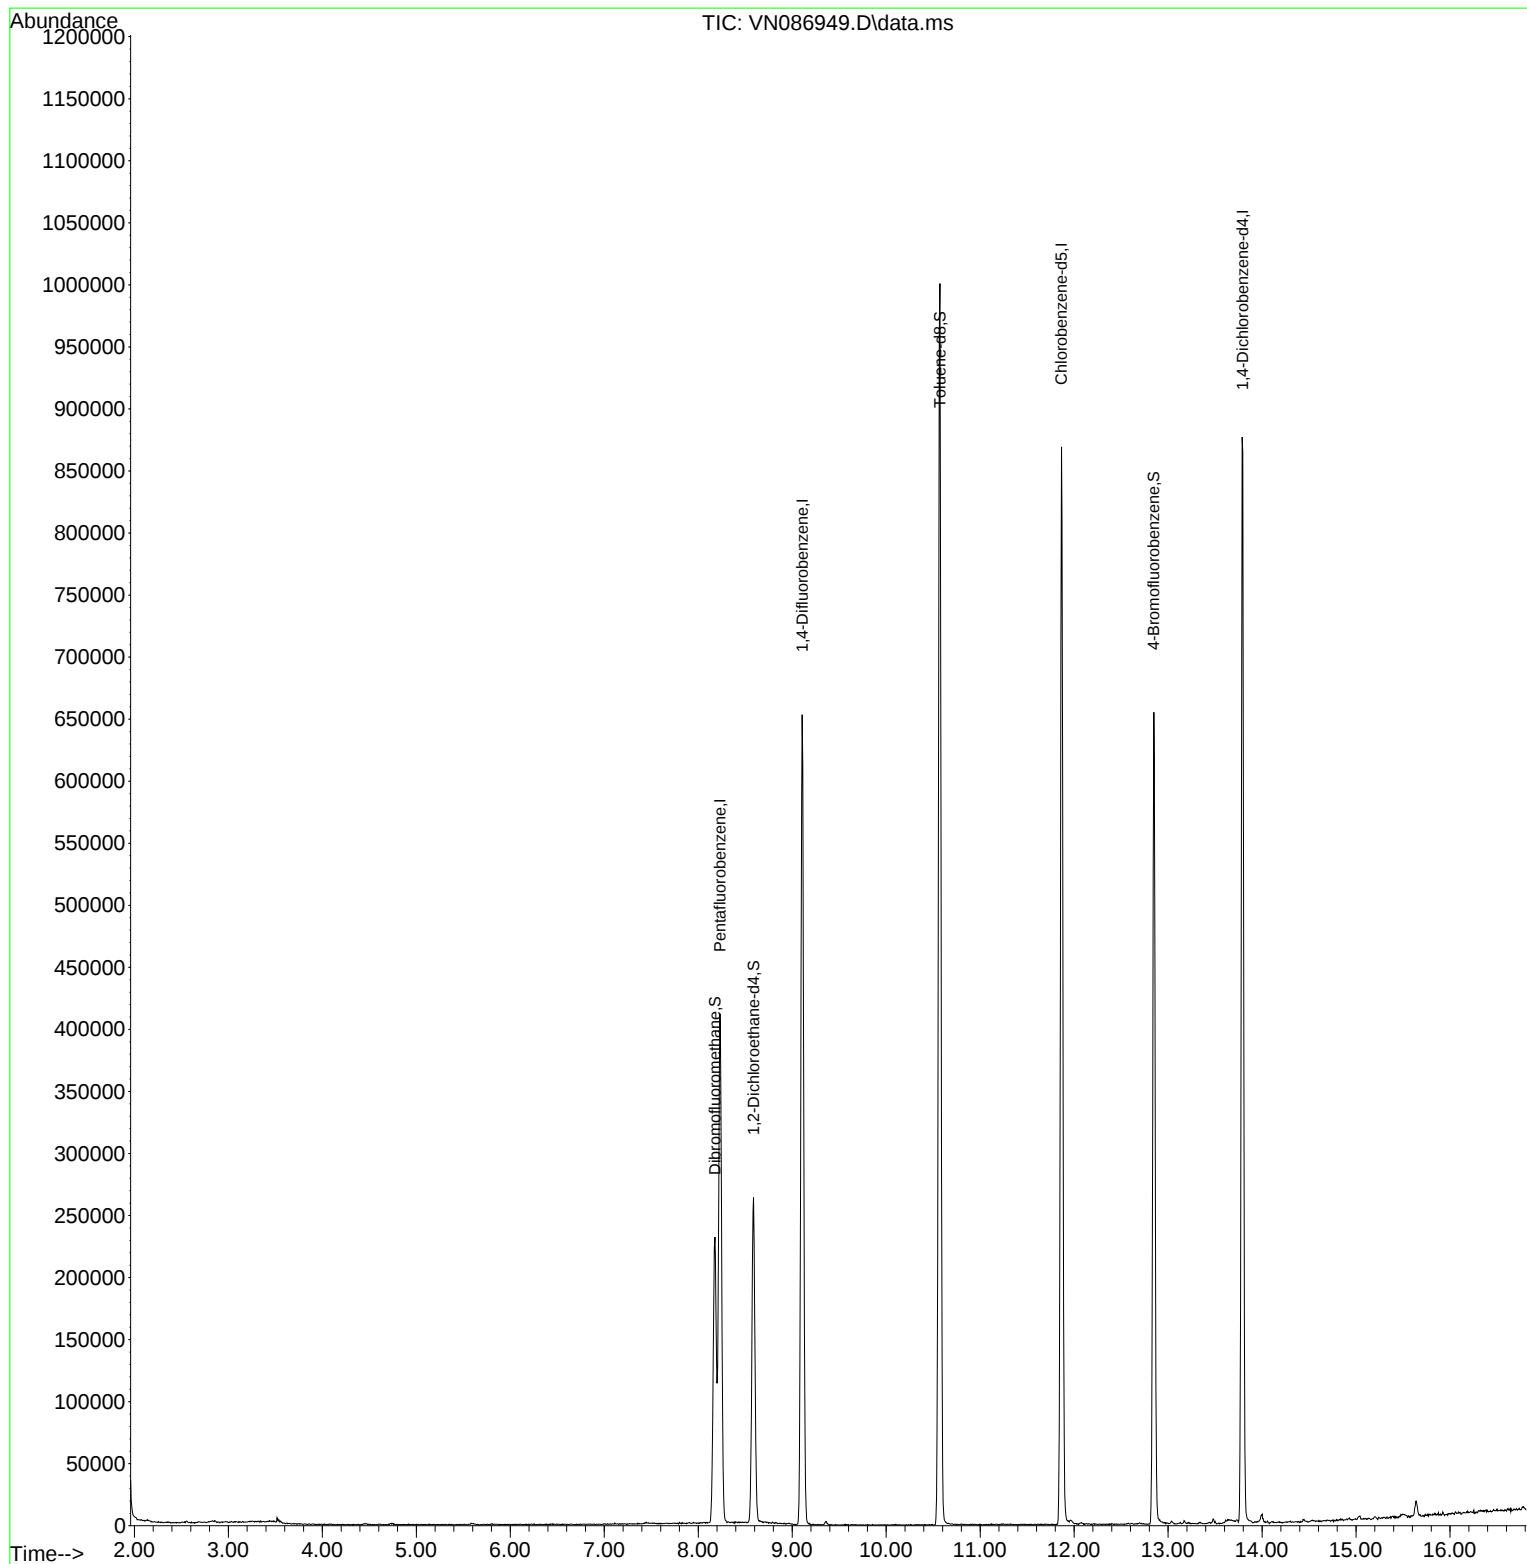


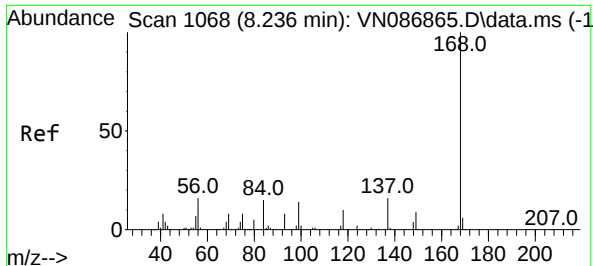

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1106
Delta R.T. -0.006 min
Lab File: VN086949.D
Acq: 11 Jun 2025 15:28




Instrument :
MSVOA_N
ClientSampleId :
TB-20250603


Tgt Ion:168 Resp: 324235
Ion Ratio Lower Upper
168 100
99 57.3 49.1 73.7

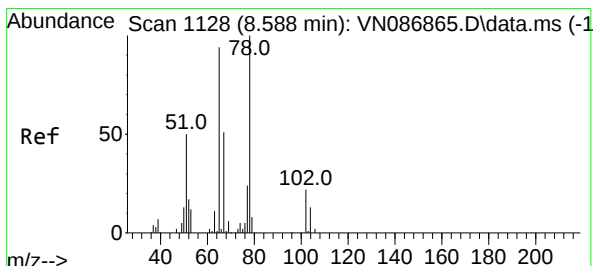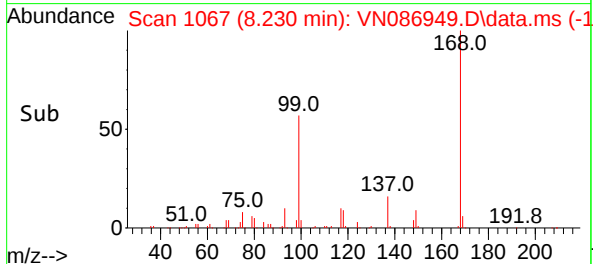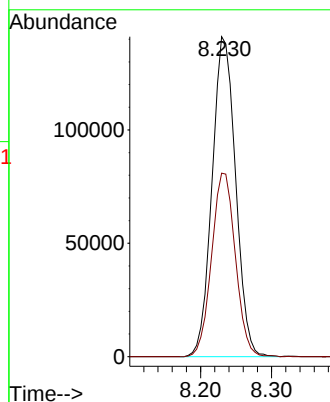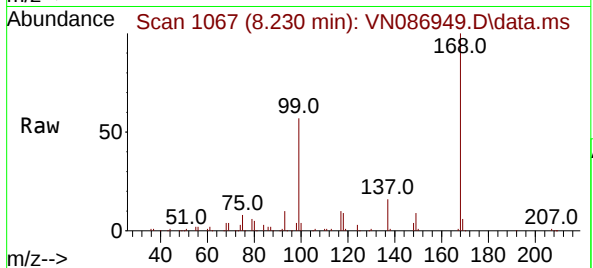

#33
1,2-Dichloroethane-d4
Concen: 48.852 ug/l
RT: 8.588 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VN086949.D
Acq: 11 Jun 2025 15:28

Tgt Ion: 65 Resp: 212072
Ion Ratio Lower Upper
65 100
67 54.7 0.0 105.6


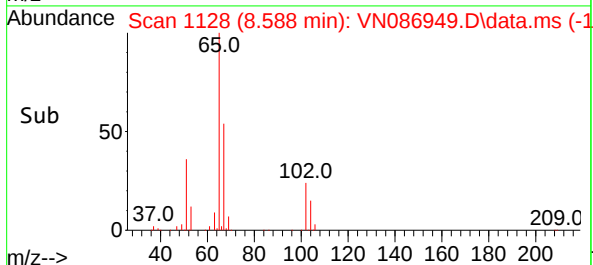
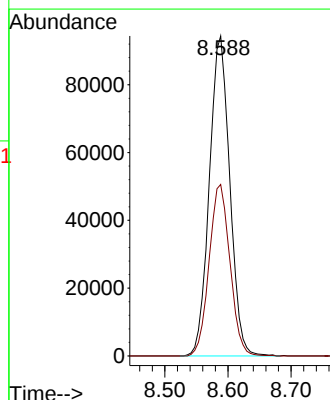
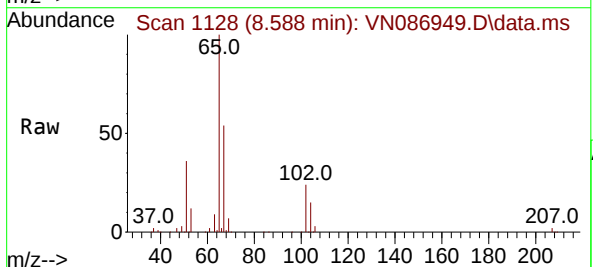


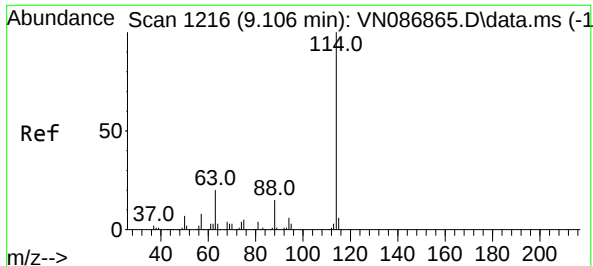

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN086949.D
Acq: 11 Jun 2025 15:28




Instrument :
MSVOA_N
ClientSampleId :
TB-20250603


Tgt Ion:114 Resp: 611383
Ion Ratio Lower Upper
114 100
63 19.9 0.0 39.6
88 16.0 0.0 30.2

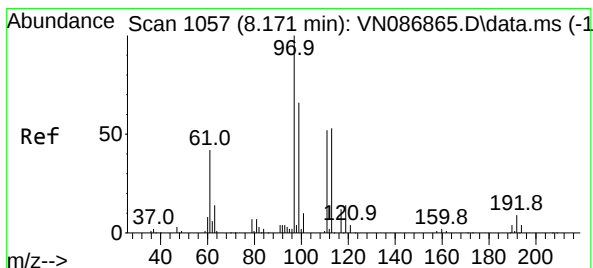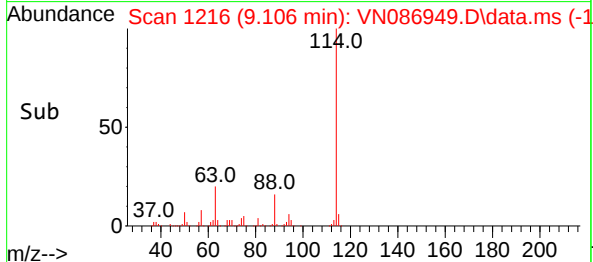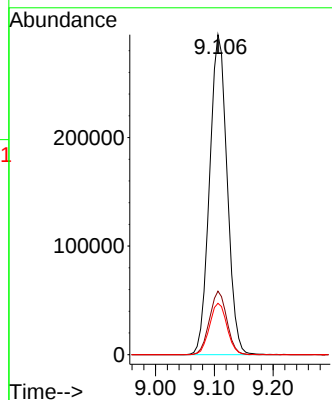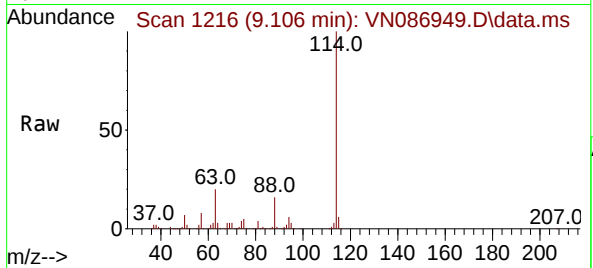

#35
Dibromofluoromethane
Concen: 49.348 ug/l
RT: 8.177 min Scan# 1058
Delta R.T. 0.006 min
Lab File: VN086949.D
Acq: 11 Jun 2025 15:28

Tgt Ion:113 Resp: 178799
Ion Ratio Lower Upper
113 100
111 102.6 84.2 126.2
192 17.7 14.2 21.4


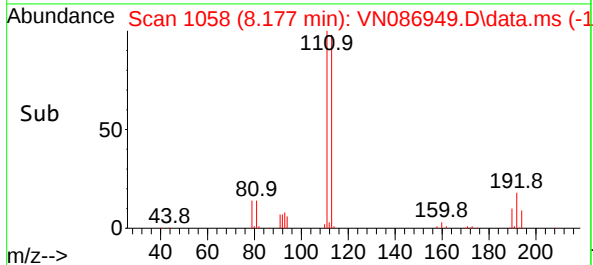
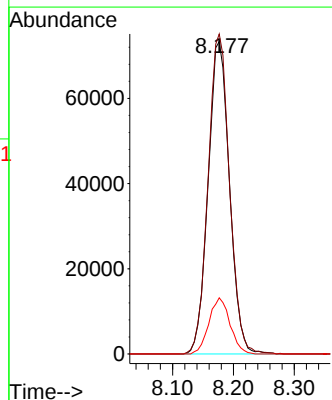
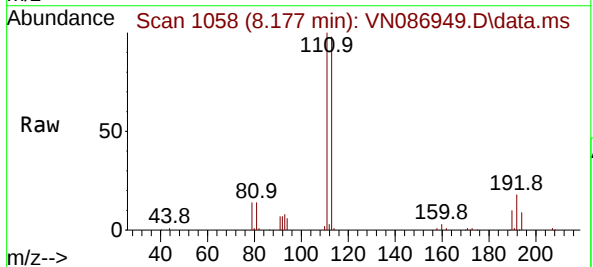


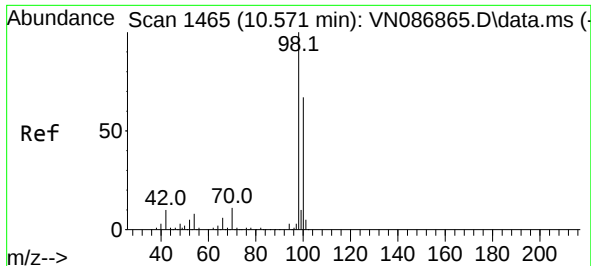

#50
Toluene-d8
Concen: 51.832 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN086949.D
Acq: 11 Jun 2025 15:28




Instrument :
MSVOA_N
ClientSampleId :
TB-20250603


Tgt Ion: 98 Resp: 743447
Ion Ratio Lower Upper
98 100
100 66.6 53.4 80.0

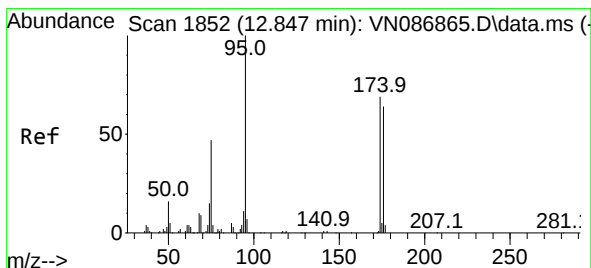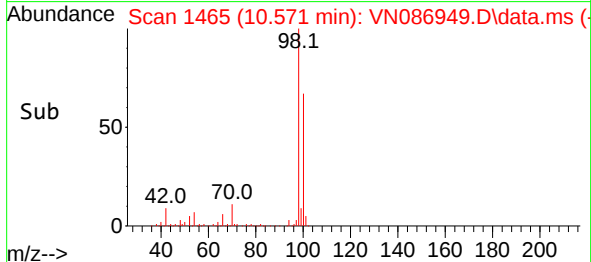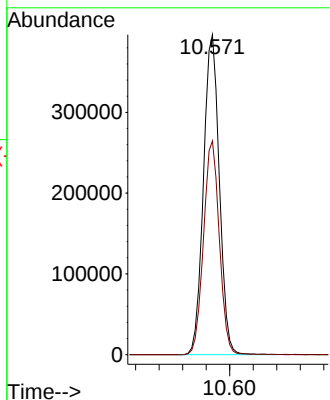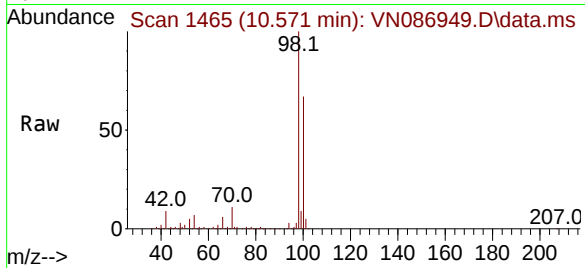

#62
4-Bromofluorobenzene
Concen: 49.691 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN086949.D
Acq: 11 Jun 2025 15:28

Tgt Ion: 95 Resp: 264799
Ion Ratio Lower Upper
95 100
174 71.5 0.0 141.8
176 68.6 0.0 132.6


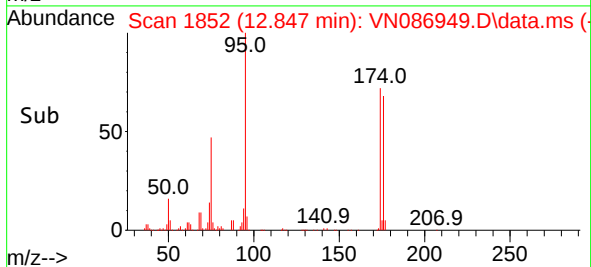
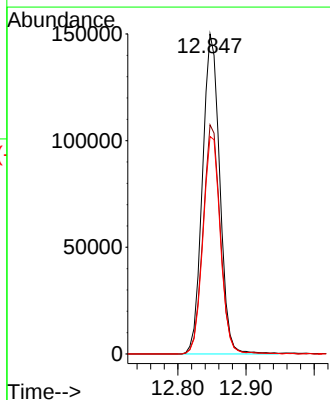
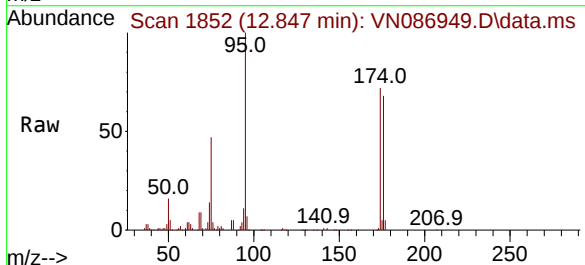


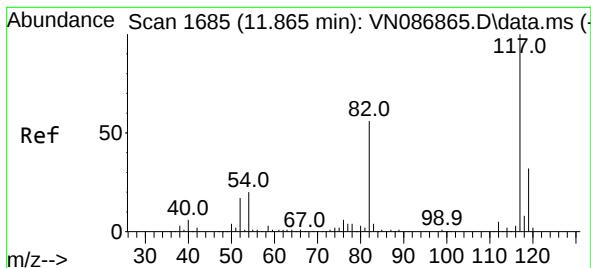

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN086949.D
Acq: 11 Jun 2025 15:28

Instrument :
MSVOA_N
ClientSampleId :
TB-20250603

Tgt Ion:117 Resp: 538730
Ion Ratio Lower Upper
117 100
82 55.3 44.6 67.0
119 32.6 25.5 38.3

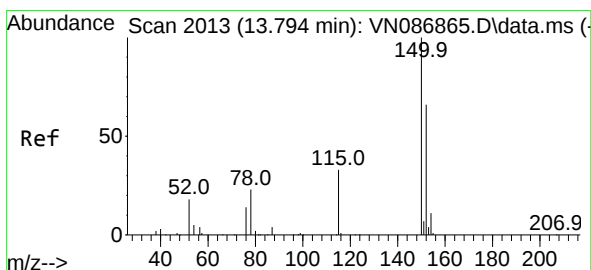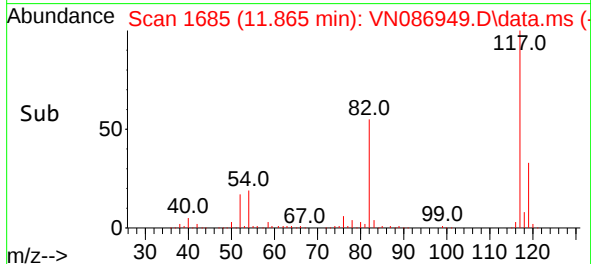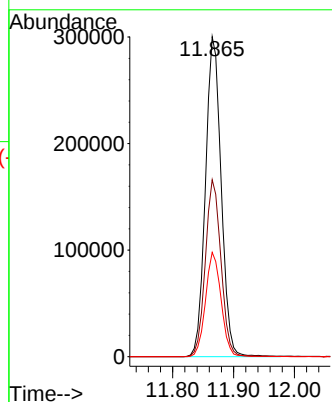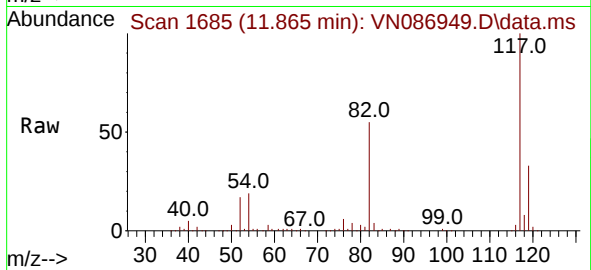

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN086949.D
Acq: 11 Jun 2025 15:28

Tgt Ion:152 Resp: 263158
Ion Ratio Lower Upper
152 100
115 59.8 30.1 90.5
150 155.6 0.0 345.0

