


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN061219\
Data File : VN056234.D
Acq On : 12 Jun 2019 8:27
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N060619W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Jun 06 04:02:53 2019

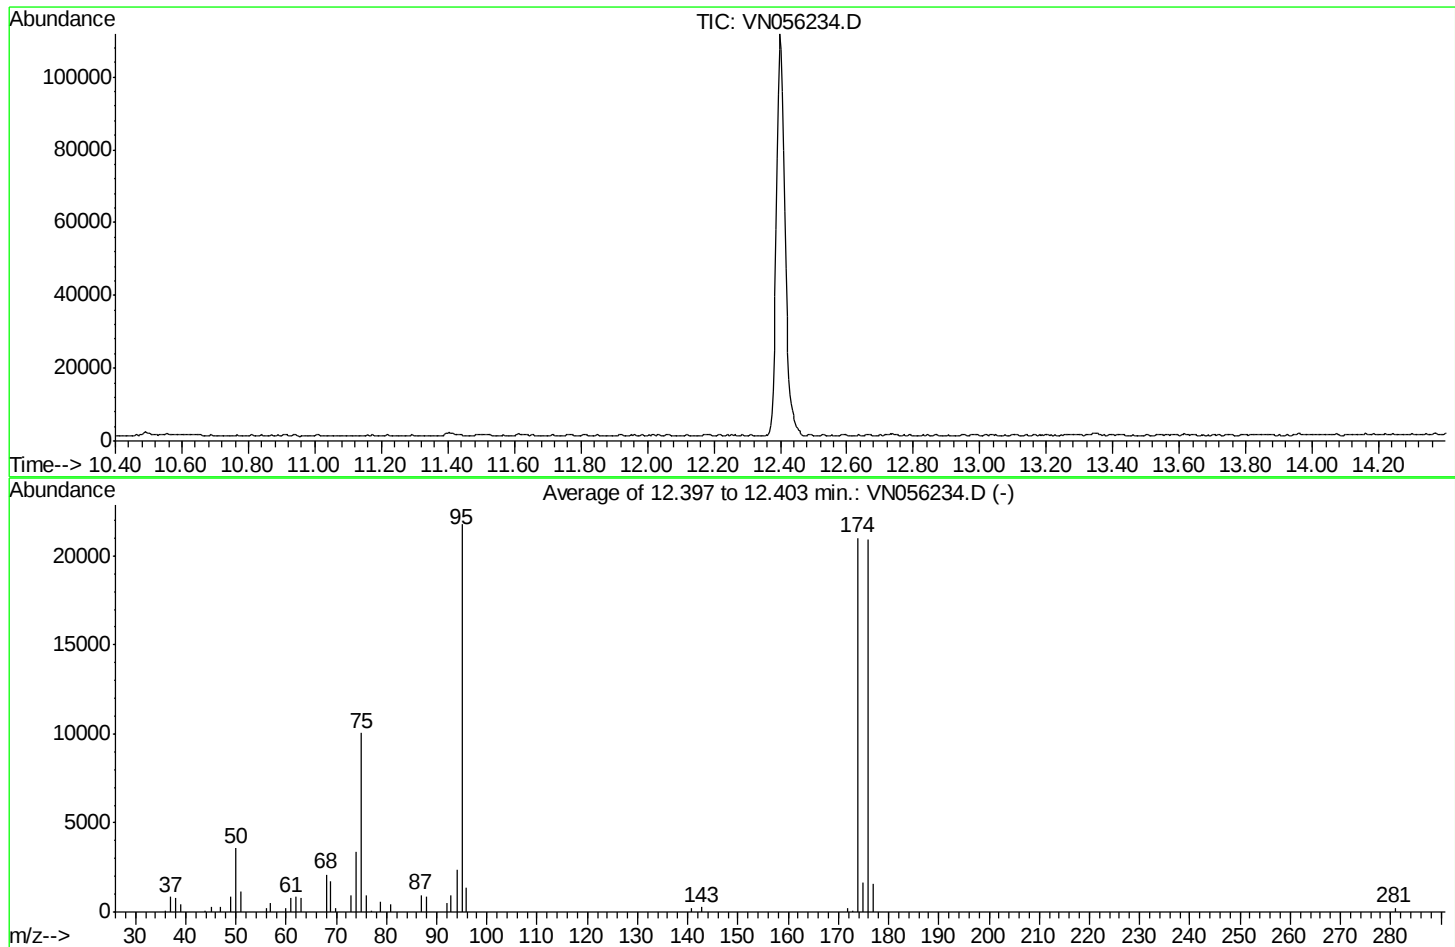

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	3582	PASS
75	95	30	60	46.2	10051	PASS
95	95	100	100	100.0	21770	PASS
96	95	5	9	6.2	1347	PASS
173	174	0.00	2	0.3	70	PASS
174	95	50	100	96.5	21010	PASS
175	174	5	9	7.9	1660	PASS
176	174	95	101	99.5	20909	PASS
177	176	5	9	7.6	1598	PASS