


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN061219\
Data File : VN056244.D
Acq On : 12 Jun 2019 12:59
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N060419W.M
Title : SW846 8260
Last Update : Tue Jun 04 11:02:09 2019

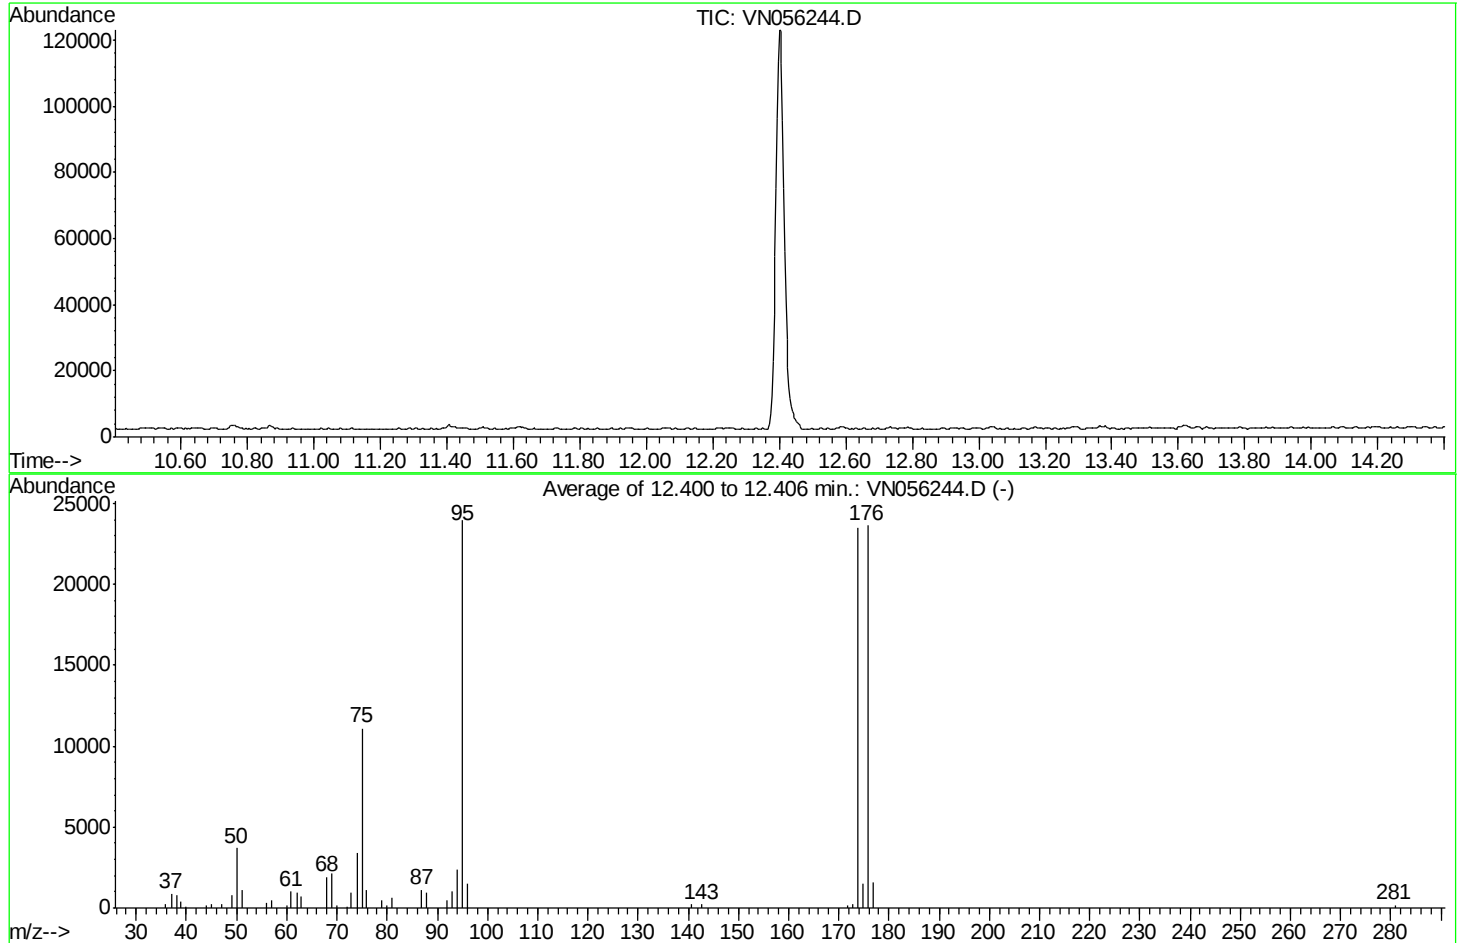

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	3690	PASS
75	95	30	60	46.3	11084	PASS
95	95	100	100	100.0	23957	PASS
96	95	5	9	6.3	1517	PASS
173	174	0.00	2	1.1	247	PASS
174	95	50	100	98.1	23493	PASS
175	174	5	9	6.4	1499	PASS
176	174	95	101	100.7	23658	PASS
177	176	5	9	6.6	1556	PASS