

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN061220\
 Data File : VN061801.D
 Acq On : 12 Jun 2020 19:07
 Operator : JC/MD
 Sample : L2989-03
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 RE125D1-20200609

Quant Time: Jun 13 05:14:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052820W.M
 Quant Title : SW846 8260
 QLast Update : Fri May 29 02:14:10 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	272825	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	463070	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	453615	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	199835	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.99	65	153134	47.11	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.22%	
35) Dibromofluoromethane	7.55	113	134399	57.21	ug/l	0.00
Spiked Amount 50.000			Recovery	=	114.42%	
50) Toluene-d8	10.06	98	554682	50.95	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.90%	
62) 4-Bromofluorobenzene	12.38	95	186495	46.96	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.92%	
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.83	85	772	1.388	ug/l	87
3) Chloromethane	2.03	50	3810	1.145	ug/l	93
5) Bromomethane	2.55	94	604	0.231	ug/l #	78
9) 1,1,2-Trichlorotrifluoroet	3.72	101	27287	10.457	ug/l	95
12) 1,1-Dichloroethene	3.70	96	5527	1.983	ug/l	96
14) Allyl chloride	4.02	41	2580	0.708	ug/l #	66
16) Acetone	3.79	43	2525	Below Cal	#	41
18) Methyl Acetate	4.02	43	4358	1.481	ug/l #	46
19) Methyl tert-butyl Ether	5.00	73	3539	0.372	ug/l #	56
24) 1,1-Dichloroethane	5.79	63	3218	0.632	ug/l #	91
27) cis-1,2-Dichloroethene	6.78	96	13257	3.724	ug/l	89
28) Bromochloromethane	7.33	49	99	Below Cal	#	3
30) Chloroform	7.33	83	4206	0.746	ug/l	98
31) Cyclohexane	7.62	56	4627	1.010	ug/l #	1
36) 1,1-Dichloropropene	7.63	75	17930	4.374	ug/l #	48
38) Carbon Tetrachloride	7.63	117	25863	6.541	ug/l #	17
39) Methylcyclohexane	8.80	83	9481	1.876	ug/l #	1
42) 1,2-Dichloroethane	8.09	62	929	0.219	ug/l #	72
44) Trichloroethene	8.80	130	848287	218.227	ug/l	96
49) 1,4-Dioxane	9.17	88	1038	25.070	ug/l #	89
55) 1,1,2-Trichloroethane	10.54	97	695	0.211	ug/l	97
60) Dibromochloromethane	10.60	129	24489	6.549	ug/l #	11
64) Tetrachloroethene	10.60	164	28096	6.580	ug/l	96
71) Bromoform	12.38	173	988	0.365	ug/l #	1
76) 1,2,3-Trichloropropane	12.38	75	90742	24.972	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.38	75	90742	63.860	ug/l #	15


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN061220\
Data File : VN061801.D
Acq On : 12 Jun 2020 19:07
Operator : JC/MD
Sample : L2989-03
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
RE125D1-20200609

Quant Time: Jun 13 05:14:43 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052820W.M
Quant Title : SW846 8260
QLast Update : Fri May 29 02:14:10 2020
Response via : Initial Calibration

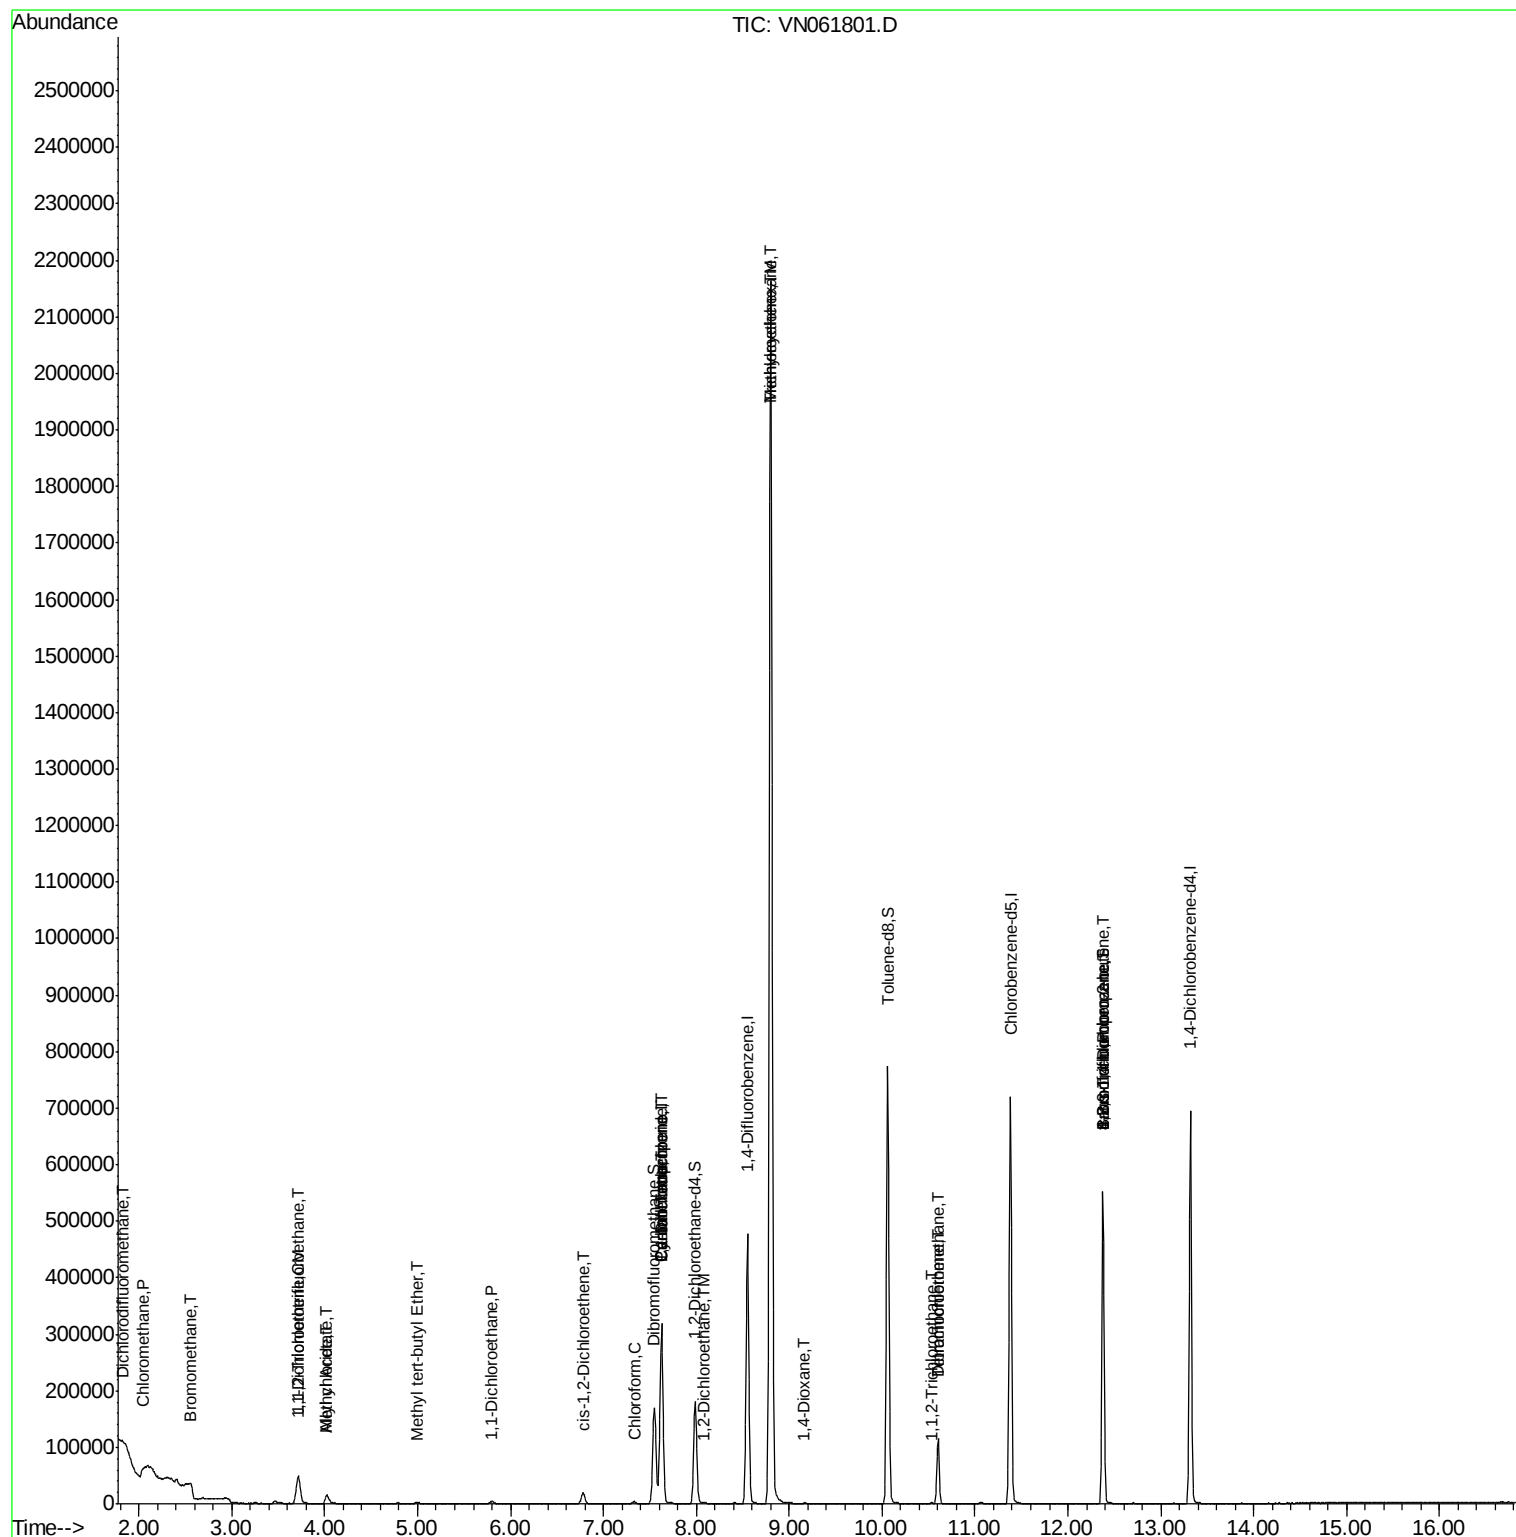

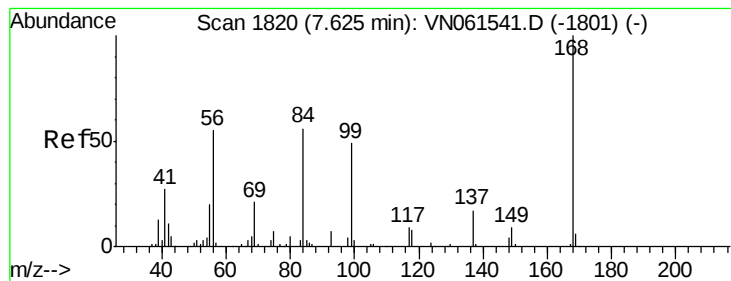

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. 0.00 min

Lab File: VN061801.D

Acq: 12 Jun 2020 19:07

Instrument :

MSVOA_N

ClientSampleId :


RE125D1-20200609

Tot Ion:168 Resp: 272825

Ion Ratio Lower Upper

168 100

99 51.5 45.0 67.4



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO



7.63

100000

50000

0

Time--> 7.50 7.60 7.70



#2

Dichlorodifluoromethane

Concen: 1.388 ug/l

RT: 1.83 min Scan# 18

Delta R.T. 0.00 min

Lab File: VN061801.D


Acq: 12 Jun 2020 19:07

Tgt Ion: 85 Resp: 772

Ion Ratio Lower Upper

85 100

87 38.2 15.6 46.8



Abundance Ion 84.90 (84.60 to 85.60): VNO

Ion 86.90 (86.60 to 87.60): VNO

1.83


600


400

200

0

Time--> 1.80 1.82 1.84 1.86



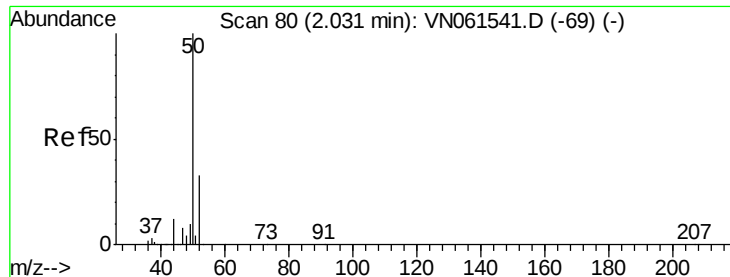

#3

Chloromethane

Concen: 1.145 ug/l

RT: 2.03 min Scan# 81

Delta R.T. 0.00 min

Lab File: VN061801.D

Acq: 12 Jun 2020 19:07

Instrument :

MSVOA_N

ClientSampleId :





RE125D1-20200609

Tot Ion: 50 Resp: 3810

Ion Ratio Lower Upper

50 100

52 37.5 26.7 40.1

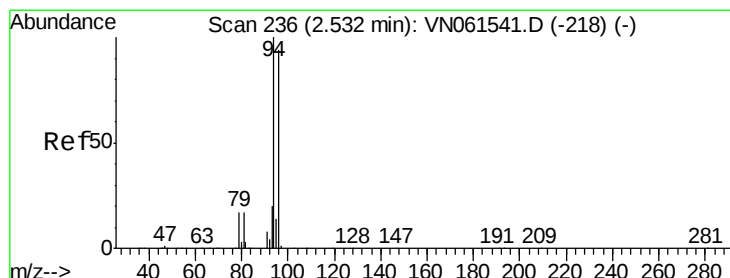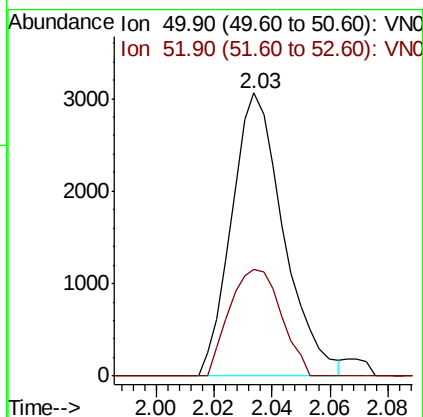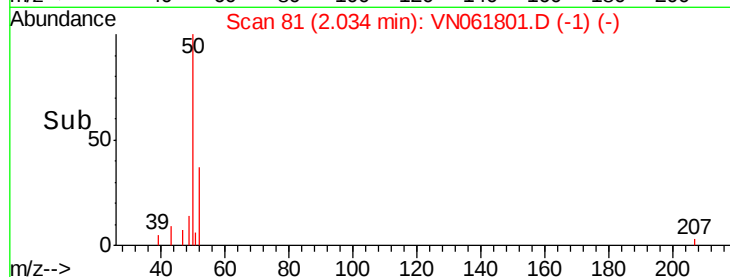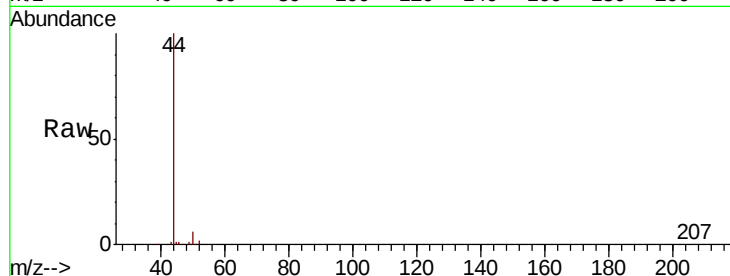

#5

Bromomethane

Concen: 0.231 ug/l

RT: 2.55 min Scan# 241

Delta R.T. 0.02 min

Lab File: VN061801.D




Acq: 12 Jun 2020 19:07


Tgt Ion: 94 Resp: 604

Ion Ratio Lower Upper

94 100

96 72.0 74.8 112.2#

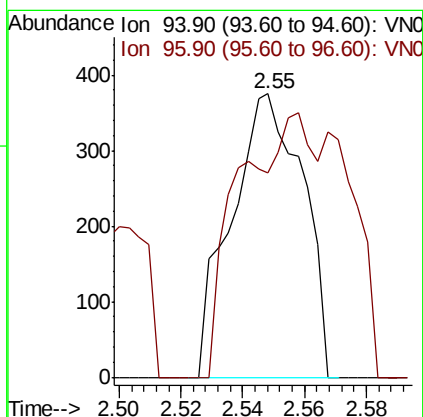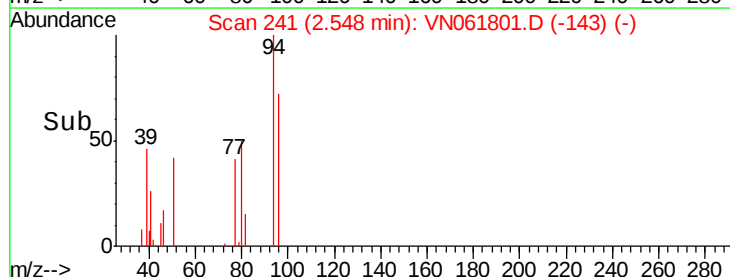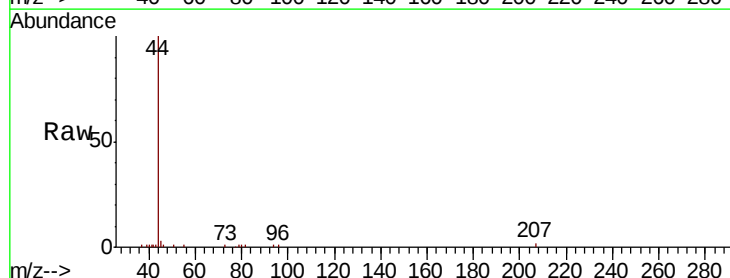

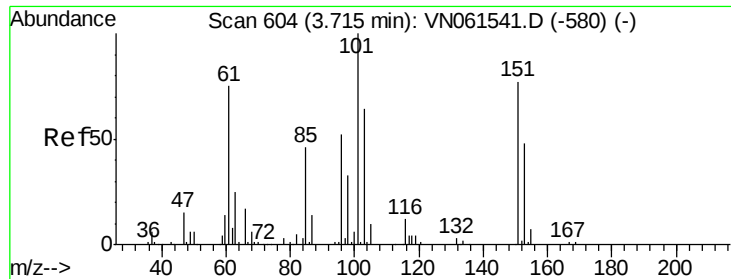

#9

1,1,2-Trichlorotrifluoroethane

Concen: 10.457 ug/l

RT: 3.72 min Scan# 605

Delta R.T. 0.00 min

Lab File: VN061801.D

Acq: 12 Jun 2020 19:07

Instrument :

MSVOA_N

ClientSampleId :

RE125D1-20200609


Tot Ion:101 Resp: 27287

Ion Ratio Lower Upper

101 100

85 43.0 35.2 52.8




151 81.7 61.0 91.6



Abundance Ion 100.90 (100.60 to 101.60): V

Ion 84.90 (84.60 to 85.60): VNO

Ion 150.80 (150.50 to 151.50): V

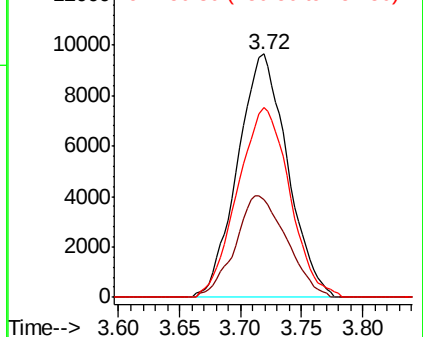

#12

1,1-Dichloroethene

Concen: 1.983 ug/l

RT: 3.70 min Scan# 598

Delta R.T. 0.00 min

Lab File: VN061801.D

Acq: 12 Jun 2020 19:07


Tgt Ion: 96 Resp: 5527

Ion Ratio Lower Upper

96 100

61 147.7 120.5 180.7



98 57.0 50.8 76.2




Abundance Ion 95.90 (95.60 to 96.60): VNO

Ion 60.90 (60.60 to 61.60): VNO

Ion 97.90 (97.60 to 98.60): VNO




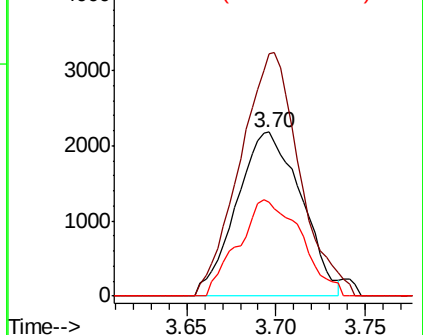




#14
Allvl chloride
Concen: 0.708 ug/l
RT: 4.02 min Scan# 700
Delta R.T. -0.25 min
Lab File: VN061801.D
Acq: 12 Jun 2020 19:07




Instrument :
MSVOA_N
ClientSampleId :
RE125D1-20200609


Tot Ion: 41 Resp: 2580
Ion Ratio Lower Upper
41 100
39 85.1 58.6 88.0
76 0.0 34.2 51.4#

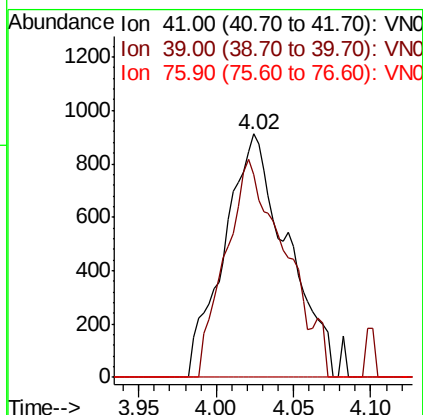

#16
Acetone
Concen: Below Cal
RT: 3.79 min Scan# 626
Delta R.T. 0.01 min
Lab File: VN061801.D
Acq: 12 Jun 2020 19:07

Tgt Ion: 43 Resp: 2525
Ion Ratio Lower Upper
43 100
58 0.0 27.2 40.8#

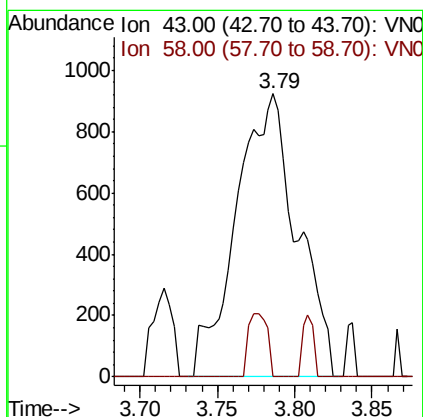

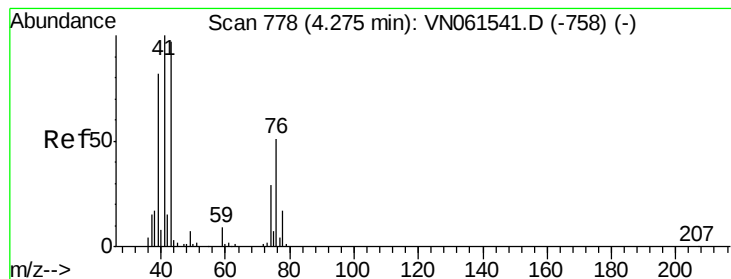

#18

Methyl Acetate

Concen: 1.481 ug/l

RT: 4.02 min Scan# 699

Delta R.T. -0.25 min

Lab File: VN061801.D

Acq: 12 Jun 2020 19:07

Instrument :

MSVOA_N

ClientSampleId :





RE125D1-20200609

Tot Ion: 43 Resp: 4358

Ion Ratio Lower Upper

43 100

74 0.0 23.2 34.8#

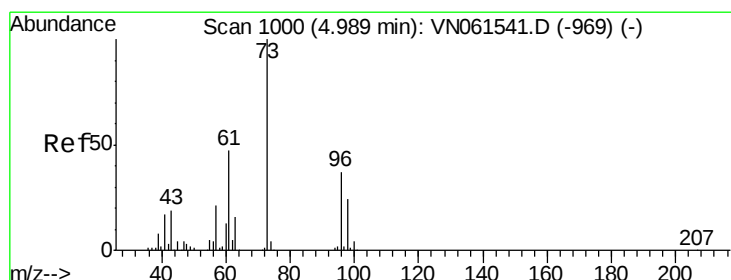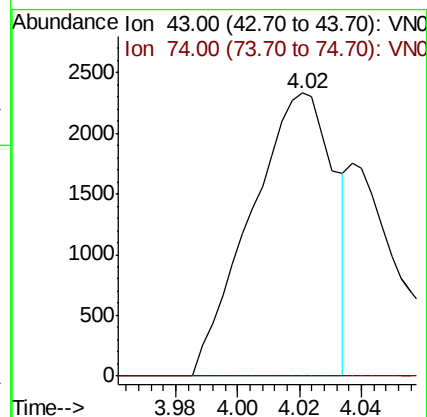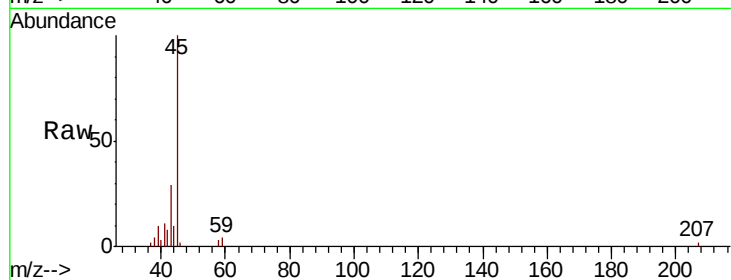

#19

Methyl tert-butyl Ether

Concen: 0.372 ug/l

RT: 5.00 min Scan# 1004

Delta R.T. 0.01 min

Lab File: VN061801.D




Acq: 12 Jun 2020 19:07


Tgt Ion: 73 Resp: 3539

Ion Ratio Lower Upper

73 100

57 0.0 16.4 24.6#

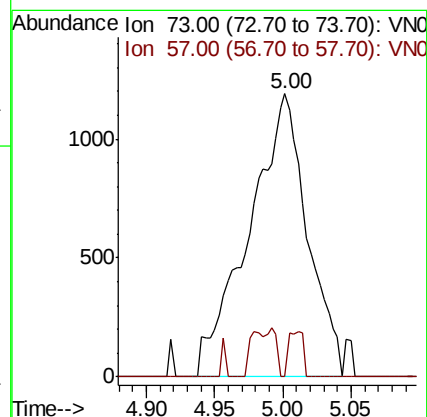



#24

1,1-Dichloroethane

Concen: 0.632 ug/l

RT: 5.79 min Scan# 1249

Delta R.T. -0.01 min

Lab File: VN061801.D

Acq: 12 Jun 2020 19:07

Instrument :

MSVOA_N

ClientSampleId :

RE125D1-20200609


Tot Ion: 63 Resp: 3218

Ion Ratio Lower Upper




63 100

98 9.3 3.8 11.4

100 0.0 2.5 7.6#



Abundance Ion 62.90 (62.60 to 63.60): VN0
Ion 97.90 (97.60 to 98.60): VN0
Ion 99.90 (99.60 to 100.60): VN0

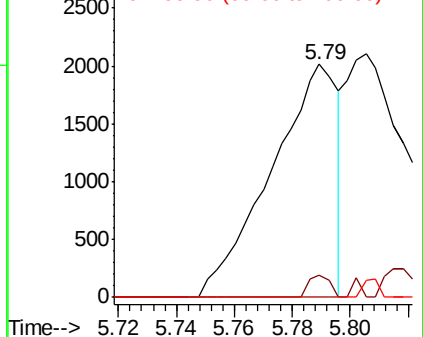

#27

cis-1,2-Dichloroethene

Concen: 3.724 ug/l

RT: 6.78 min Scan# 1558

Delta R.T. 0.00 min

Lab File: VN061801.D

Acq: 12 Jun 2020 19:07


Tgt Ion: 96 Resp: 13257

Ion Ratio Lower Upper



96 100


61 109.2 0.0 252.2

98 62.8 0.0 129.2



Abundance Ion 95.90 (95.60 to 96.60): VN0
Ion 60.90 (60.60 to 61.60): VN0
Ion 97.90 (97.60 to 98.60): VN0

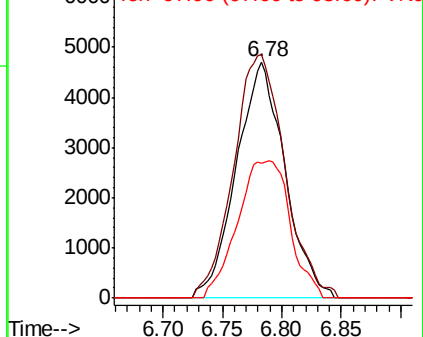



#28

Bromochloromethane

Concen: Below Cal

RT: 7.33 min Scan# 1729

Delta R.T. 0.18 min


Lab File: VN061801.D

Acq: 12 Jun 2020 19:07

Instrument :
MSVOA_N
ClientSampleId :
RE125D1-20200609

Tot Ion: 49 Resp: 99




Ion	Ratio	Lower	Upper
49	100		
129	0.0	0.0	4.8
130	0.0	78.8	118.2



Abundance Ion 48.90 (48.60 to 49.60): VN061801.D (-1579) (-)

Ion 128.80 (128.50 to 129.50): VN061801.D (-1579) (-)

Ion 129.80 (129.50 to 130.50): VN061801.D (-1579) (-)

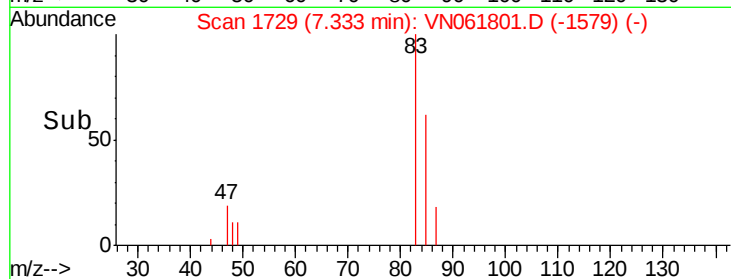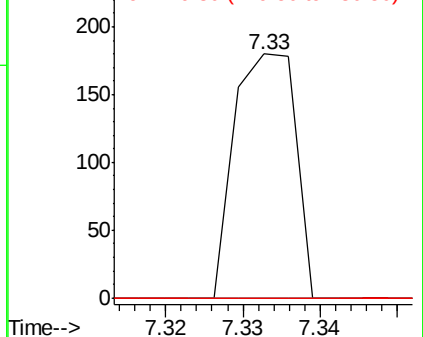

#30

Chloroform

Concen: 0.746 ug/l

RT: 7.33 min Scan# 1728


Delta R.T. 0.00 min

Lab File: VN061801.D

Acq: 12 Jun 2020 19:07



Tgt Ion: 83 Resp: 4206


Ion	Ratio	Lower	Upper
83	100		
85	66.4	51.7	77.5



Abundance Ion 82.90 (82.60 to 83.60): VN061801.D (-1634) (-)

Ion 84.90 (84.60 to 85.60): VN061801.D (-1634) (-)

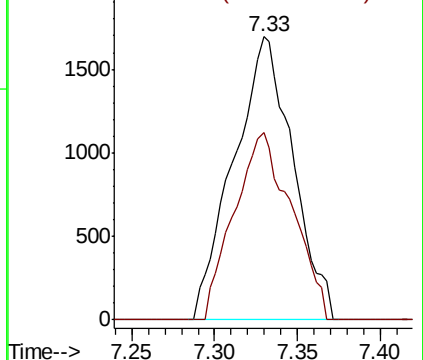

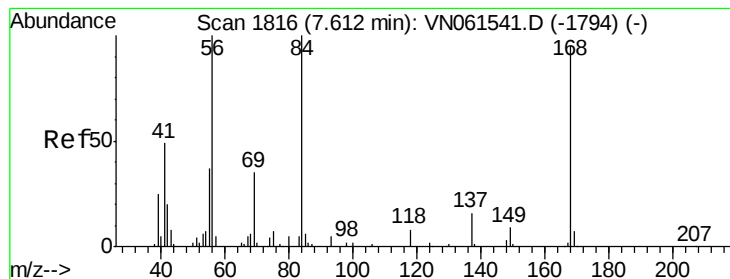

#31

Cyclohexane

Concen: 1.010 ug/l

RT: 7.62 min Scan# 1819

Delta R.T. 0.01 min

Lab File: VN061801.D

Acq: 12 Jun 2020 19:07

Instrument :

MSVOA_N

ClientSampleId :

RE125D1-20200609


Tot Ion: 56 Resp: 4627

Ion Ratio Lower Upper

56 100

69 182.3 27.8 41.8#




84 180.2 79.9 119.9#

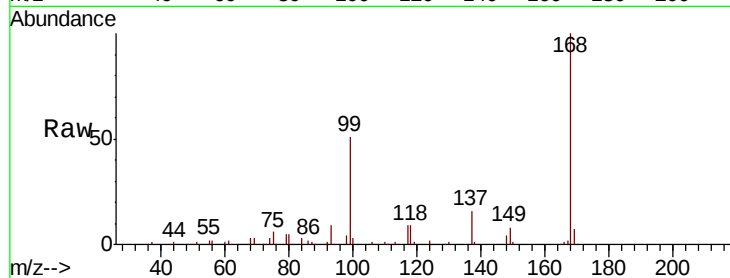

Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 84.00 (83.70 to 84.70): VN0

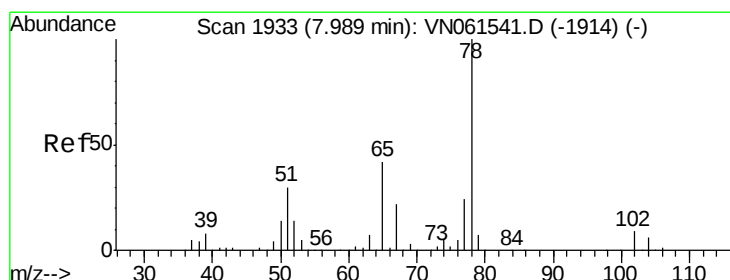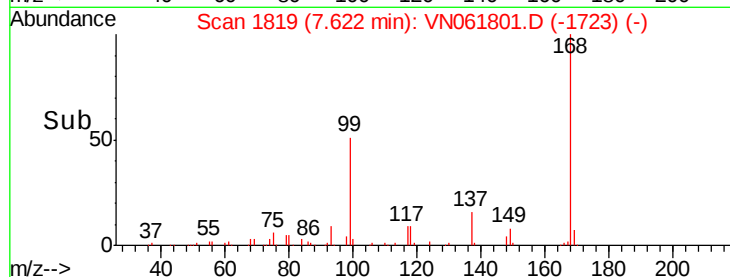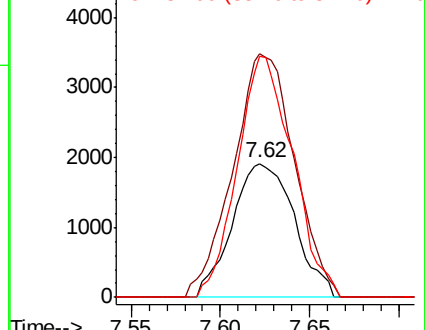

#33

1,2-Dichloroethane-d4

Concen: 47.110 ug/l

RT: 7.99 min Scan# 1933

Delta R.T. 0.00 min

Lab File: VN061801.D


Acq: 12 Jun 2020 19:07

Tgt Ion: 65 Resp: 153134

Ion Ratio Lower Upper



65 100


67 52.5 0.0 104.8

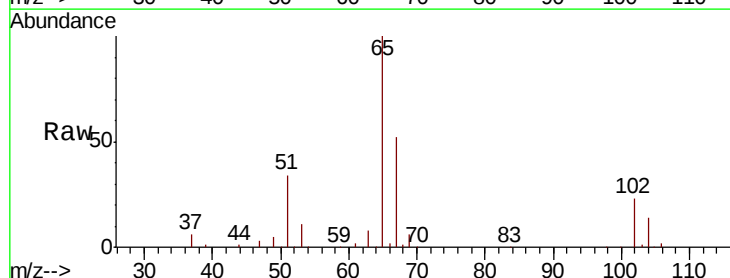

Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

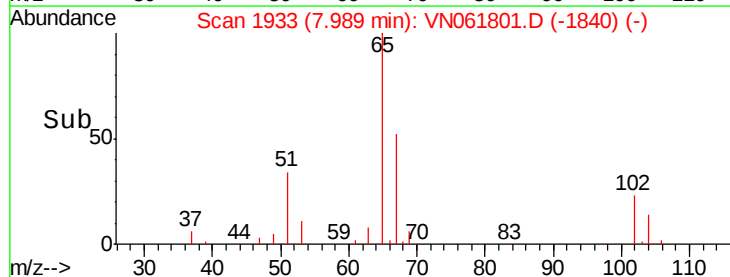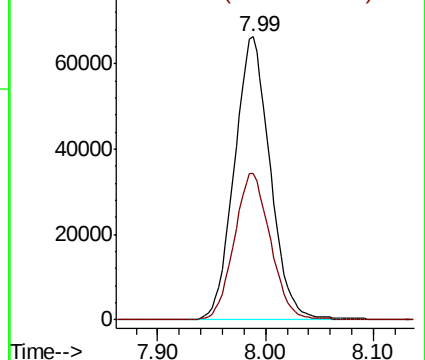







#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2108
 Delta R.T. 0.00 min
 Lab File: VN061801.D
 Acq: 12 Jun 2020 19:07

Instrument :
 MSVOA_N
 ClientSampleId :
 RE125D1-20200609

Tot Ion	Ratio	Lower	Upper
114	100		
63	17.0	0.0	35.8
88	14.1	0.0	31.0

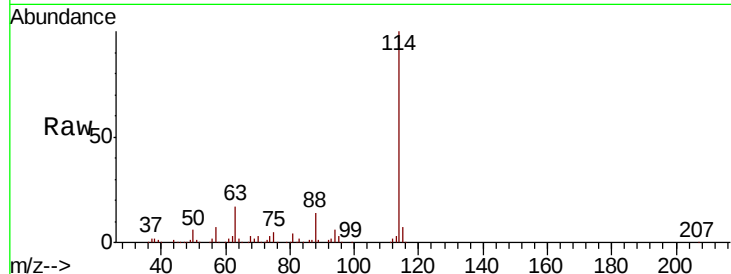


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

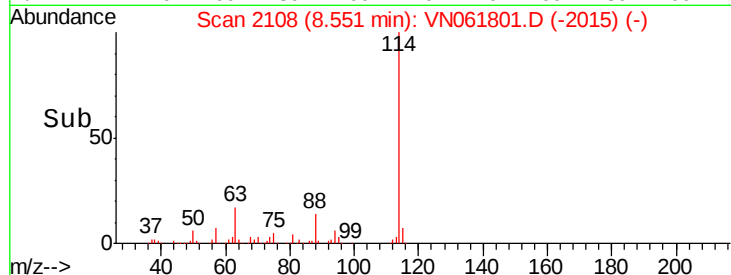
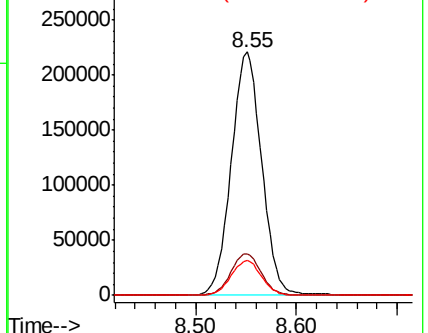



#35
 Dibromofluoromethane
 Concen: 57.214 ug/l
 RT: 7.55 min Scan# 1797
 Delta R.T. 0.00 min
 Lab File: VN061801.D
 Acq: 12 Jun 2020 19:07

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.2	83.4	125.0
192	19.6	15.4	23.2



Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V




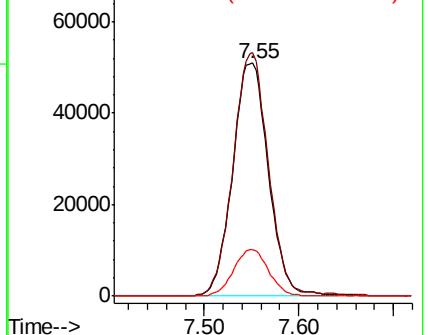


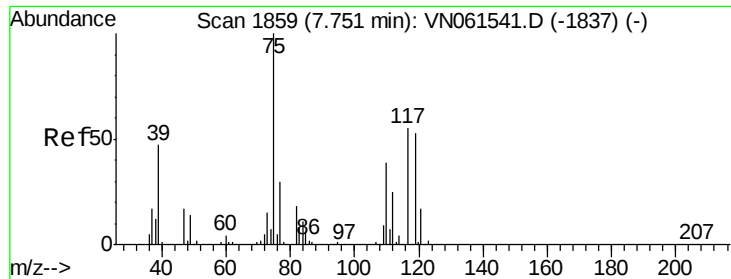

#36
 1,1-Dichloropropene
 Concen: 4.374 ug/l
 RT: 7.63 min Scan# 1820
 Delta R.T. -0.13 min
 Lab File: VN061801.D
 Acq: 12 Jun 2020 19:07




Instrument :
 MSVOA_N
 ClientSampleId :
 RE125D1-20200609


Tot Ion	Ratio	Lower	Upper
75	100		
110	9.8	19.5	58.5#
77	0.0	24.7	37.1#

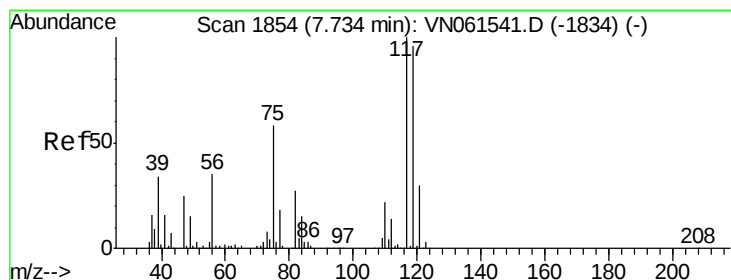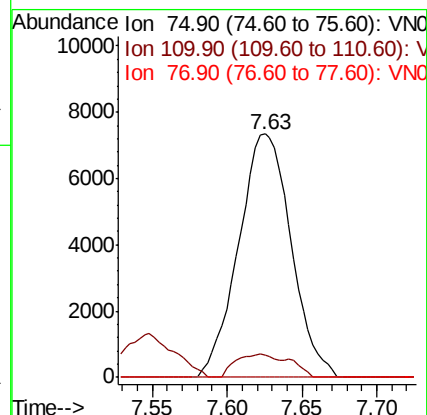

#38
 Carbon Tetrachloride
 Concen: 6.541 ug/l
 RT: 7.63 min Scan# 1820
 Delta R.T. -0.11 min
 Lab File: VN061801.D
 Acq: 12 Jun 2020 19:07

Tgt Ion	Ratio	Lower	Upper
117	100		
119	5.6	76.5	114.7#
121	0.0	24.1	36.1#



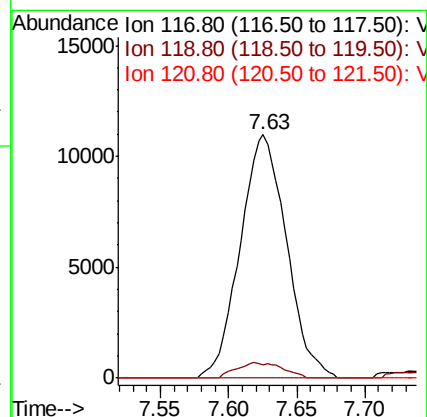





#39
Methylcyclohexane
Concen: 1.876 ug/l
RT: 8.80 min Scan# 2185
Delta R.T. -0.25 min
Lab File: VN061801.D
Acq: 12 Jun 2020 19:07




Instrument :
MSVOA_N
ClientSampleId :
RE125D1-20200609


Tot Ion: 83 Resp: 9481
Ion Ratio Lower Upper
83 100
55 0.0 54.9 82.3#
98 190.5 41.0 61.4#

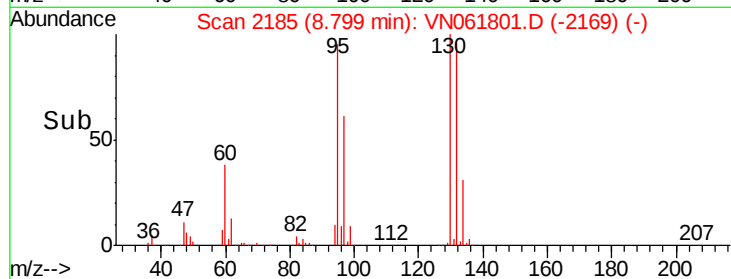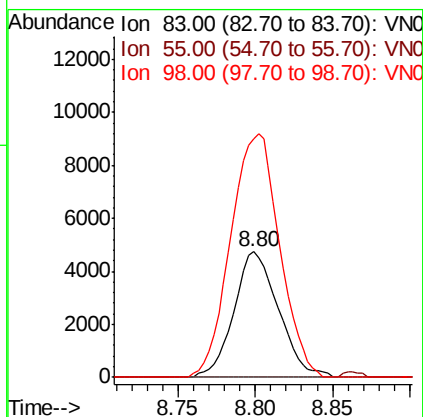

#42
1,2-Dichloroethane
Concen: 0.219 ug/l
RT: 8.09 min Scan# 1964
Delta R.T. 0.00 min
Lab File: VN061801.D
Acq: 12 Jun 2020 19:07

Tgt Ion: 62 Resp: 929
Ion Ratio Lower Upper
62 100
98 0.0 0.0 21.4


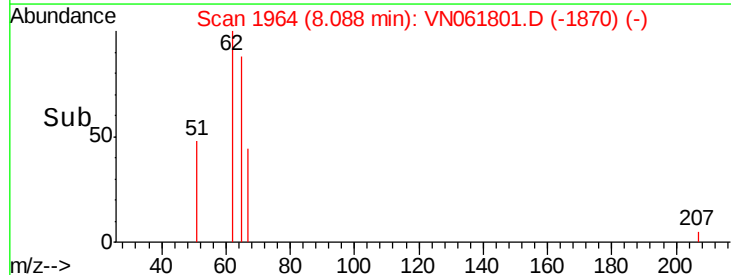
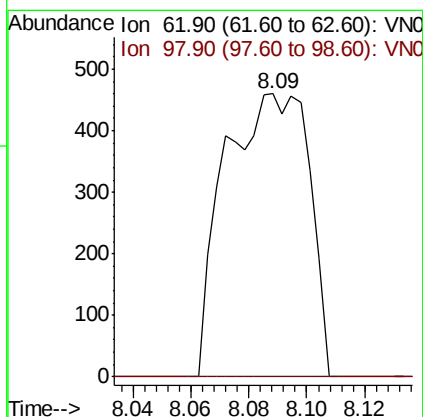





#44
 Trichloroethene
 Concen: 218.227 ug/l
 RT: 8.80 min Scan# 2186
 Delta R.T. 0.00 min
 Lab File: VN061801.D
 Acq: 12 Jun 2020 19:07




Instrument :
 MSVOA_N
 ClientSampleId :
 RE125D1-20200609


Tot Ion:130 Resp: 848287
 Ion Ratio Lower Upper
 130 100
 95 94.5 0.0 196.6

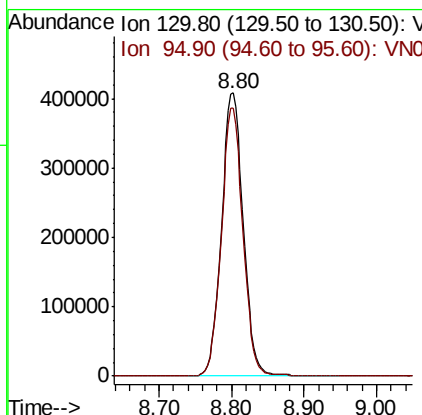

#49
 1,4-Dioxane
 Concen: 25.070 ug/l
 RT: 9.17 min Scan# 2299
 Delta R.T. 0.00 min
 Lab File: VN061801.D
 Acq: 12 Jun 2020 19:07

Tgt Ion: 88 Resp: 1038
 Ion Ratio Lower Upper
 88 100
 43 16.2 23.1 34.7#
 58 57.0 48.3 72.5

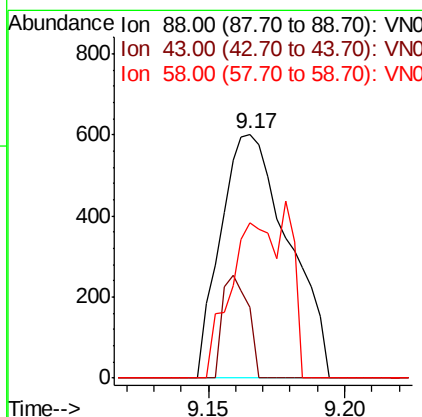

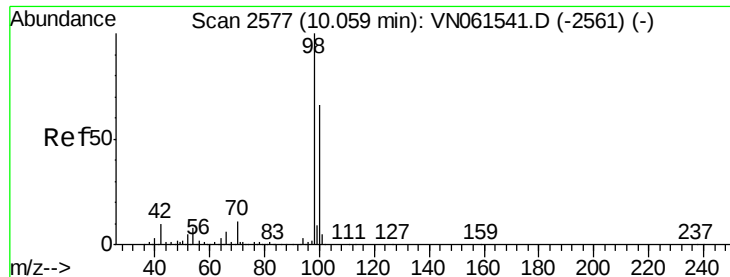

#50

Toluene-d8

Concen: 50.954 ug/l

RT: 10.06 min Scan# 2577

Delta R.T. 0.00 min

Lab File: VN061801.D

Acq: 12 Jun 2020 19:07

Instrument :

MSVOA_N

ClientSampleId :


RE125D1-20200609

Tot Ion: 98 Resp: 554682




Ion Ratio Lower Upper

98 100

100 66.4 52.8 79.2

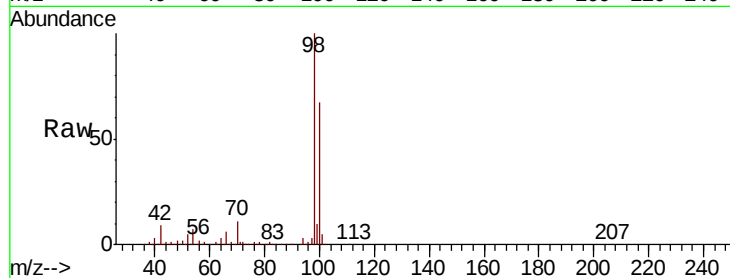

Abundance Ion 98.00 (97.70 to 98.70): VN061801.D (-2484) (-)

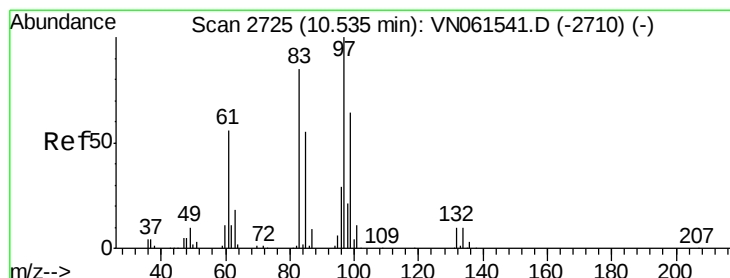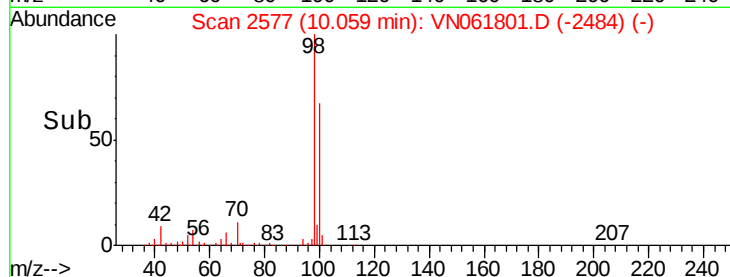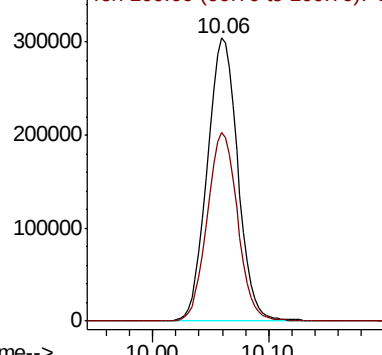

#55

1,1,2-Trichloroethane

Concen: 0.211 ug/l

RT: 10.54 min Scan# 2725

Delta R.T. 0.00 min

Lab File: VN061801.D

Acq: 12 Jun 2020 19:07

Tgt Ion: 97 Resp: 695


Ion Ratio Lower Upper

97 100



83 85.2 68.1 102.1


85 60.5 44.1 66.1

99 61.0 51.1 76.7

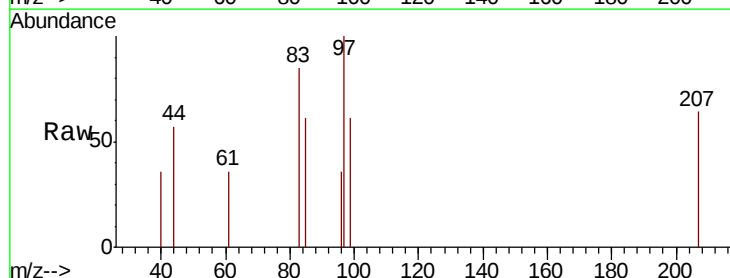

Abundance Ion 96.90 (96.60 to 97.60): VN061801.D (-2632) (-)



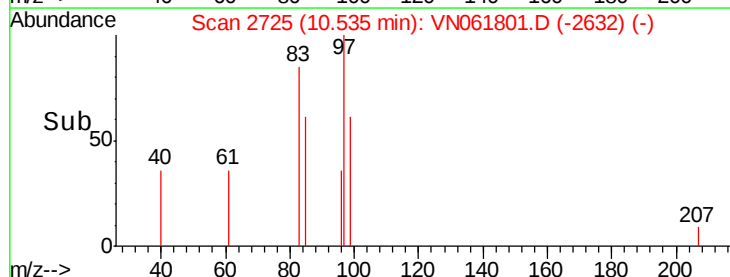
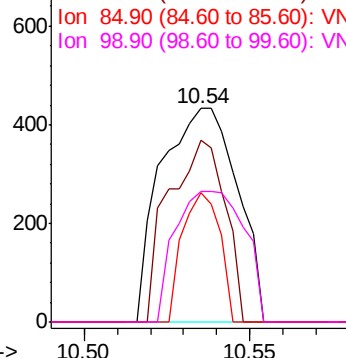




#60
 Dibromochloromethane
 Concen: 6.549 ug/l
 RT: 10.60 min Scan# 2746
 Delta R.T. -0.27 min
 Lab File: VN061801.D
 Acq: 12 Jun 2020 19:07




Instrument :
 MSVOA_N
 ClientSampleId :
 RE125D1-20200609


Tot Ion:129 Resp: 24489
 Ion Ratio Lower Upper
 129 100
 127 0.0 38.8 116.3#

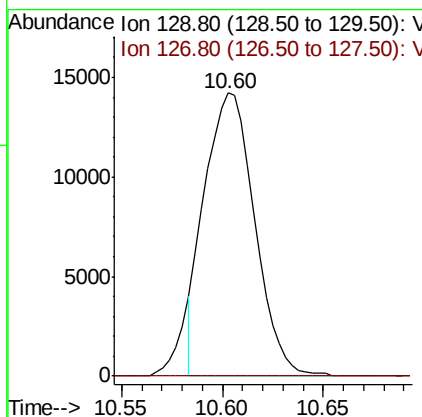

#62
 4-Bromofluorobenzene
 Concen: 46.958 ug/l
 RT: 12.38 min Scan# 3298
 Delta R.T. 0.00 min
 Lab File: VN061801.D
 Acq: 12 Jun 2020 19:07

Tgt Ion: 95 Resp: 186495
 Ion Ratio Lower Upper
 95 100
 174 89.7 0.0 172.8
 176 85.6 0.0 164.8



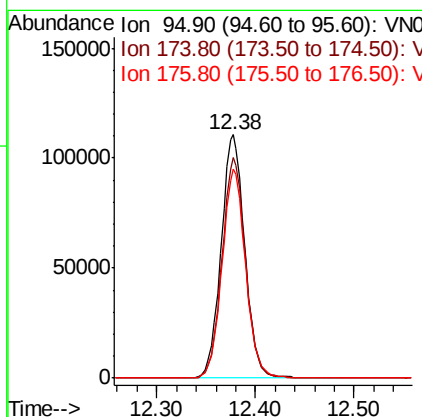





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2988
Delta R.T. 0.00 min
Lab File: VN061801.D
Acq: 12 Jun 2020 19:07




Instrument :
MSVOA_N
ClientSampleId :
RE125D1-20200609


Tot Ion	Ratio	Lower	Upper
117	100		
82	50.8	41.5	62.3
119	31.7	25.6	38.4

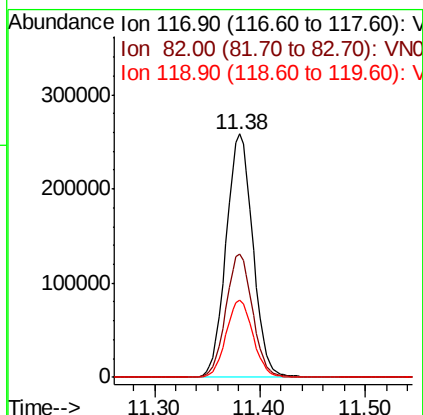

#64
Tetrachloroethene
Concen: 6.580 ug/l
RT: 10.60 min Scan# 2746
Delta R.T. 0.00 min
Lab File: VN061801.D
Acq: 12 Jun 2020 19:07

Tgt Ion	Ratio	Lower	Upper
164	100		
166	131.7	101.5	152.3
129	91.6	74.9	112.3
131	96.9	72.2	108.2

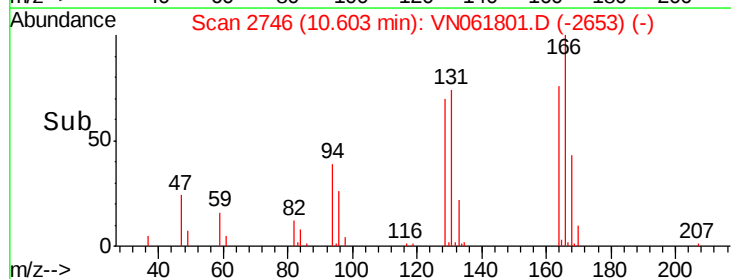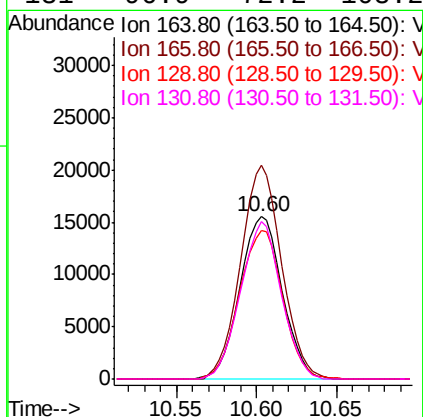



#71

Bromoform

Concen: 0.365 ug/l

RT: 12.38 min Scan# 3299

Delta R.T. 0.28 min

Lab File: VN061801.D

Acq: 12 Jun 2020 19:07

Instrument :

MSVOA_N

ClientSampleId :

RE125D1-20200609


Tot Ion:173 Resp: 988

Ion Ratio Lower Upper

173 100

175 1053.9 24.4 73.2#




254 0.0 0.0 0.0



Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

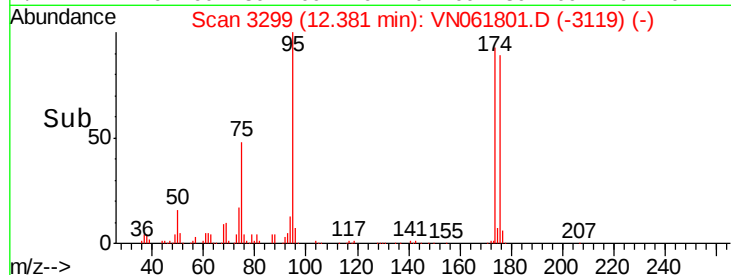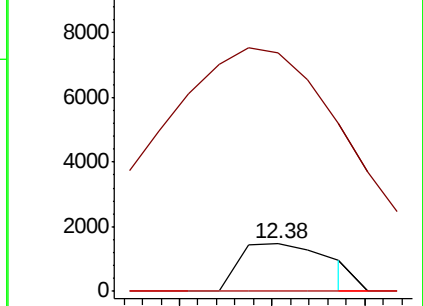

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3591

Delta R.T. 0.00 min

Lab File: VN061801.D

Acq: 12 Jun 2020 19:07


Tgt Ion:152 Resp: 199835

Ion Ratio Lower Upper

152 100

115 54.9 28.0 84.0



150 158.3 0.0 344.0




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

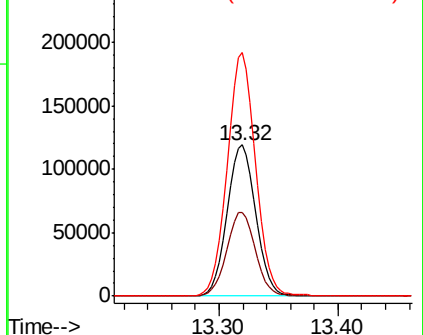

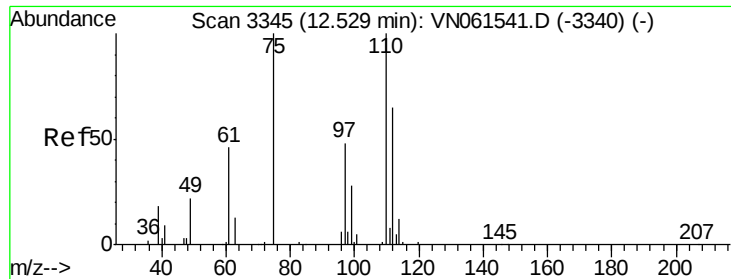

#76

1,2,3-Trichloropropane

Concen: 24.972 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. -0.15 min

Lab File: VN061801.D

Acq: 12 Jun 2020 19:07

Instrument :

MSVOA_N

ClientSampleId :





RE125D1-20200609

Tot Ion: 75 Resp: 90742

Ion Ratio Lower Upper

75 100

77 1.3 0.0 0.0#

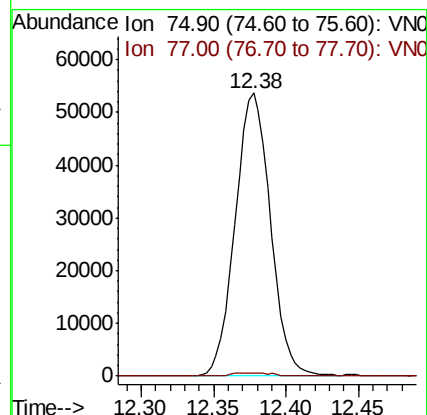

#81

trans-1,4-Dichloro-2-butene

Concen: 63.860 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. 0.10 min

Lab File: VN061801.D

Acq: 12 Jun 2020 19:07

Tgt Ion: 75 Resp: 90742

Ion Ratio Lower Upper

75 100

53 0.0 67.8 101.8#

89 0.0 37.1 55.7#

