
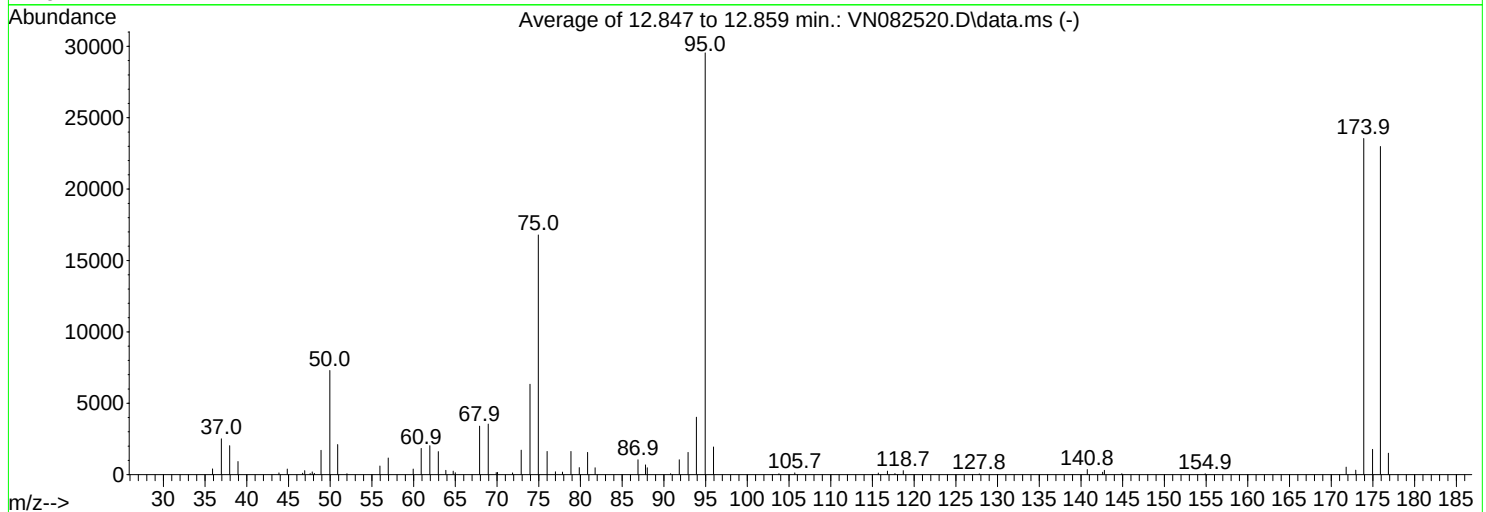


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061224\
Data File : VN082520.D
Acq On : 12 Jun 2024 10:38
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

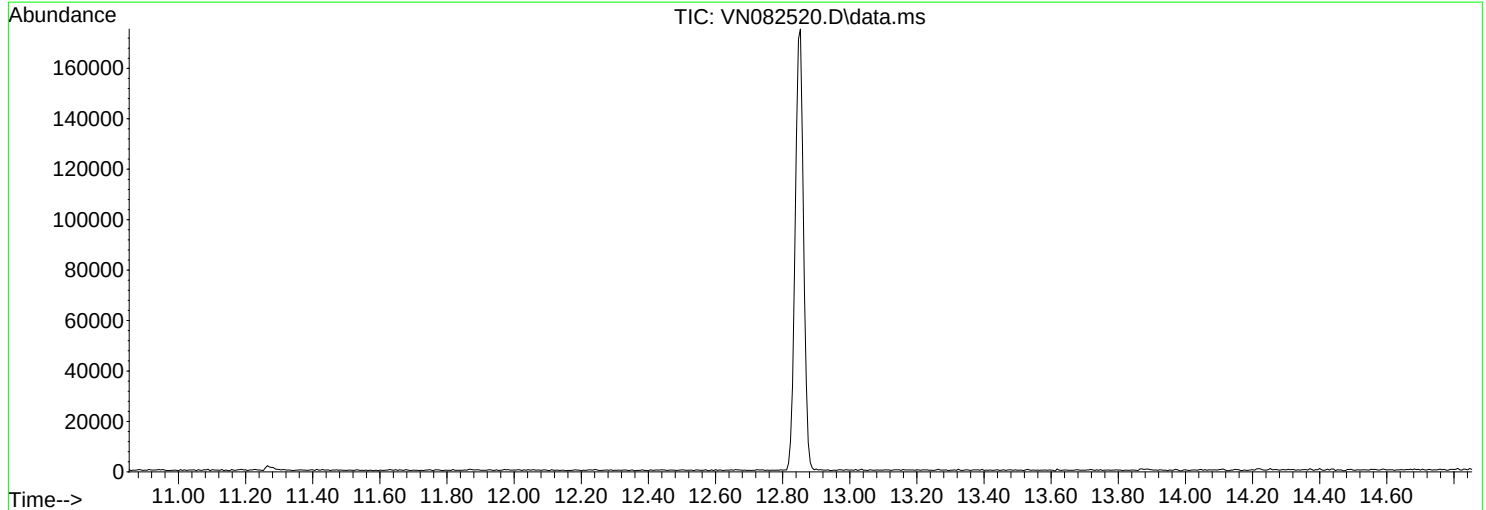

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.7	7301	PASS
75	95	30	60	56.8	16791	PASS
95	95	100	100	100.0	29544	PASS
96	95	5	9	6.6	1938	PASS
173	174	0.00	2	1.3	310	PASS
174	95	50	100	79.7	23547	PASS
175	174	5	9	7.5	1774	PASS
176	174	95	101	97.6	22981	PASS
177	176	5	9	6.5	1500	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	401	48.90	1709	64.75	246	77.00	20
36.95	2515	49.95	7301	65.00	130	77.85	18
37.95	2024	50.90	2103	67.90	3394	78.85	162
38.95	915	52.00	69	68.95	3544	79.85	49
43.85	128	55.95	600	69.90	143	80.85	1558
44.85	395	56.95	1171	70.05	153	81.75	479
46.70	97	59.95	397	71.85	126	86.90	1045
46.95	279	60.90	1833	72.90	1713	87.80	679
47.60	84	61.95	2028	73.95	6334	88.00	478
47.85	186	62.95	1616	74.95	16791	90.80	73
48.10	91	63.85	303	76.00	1626	91.85	1037

Average of 12.847 to 12.859 min.: VN082520.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.90	1558	140.75	362				
93.90	4022	142.60	165				
94.95	29544	142.80	298				
95.95	1938	144.90	63				
103.80	71	154.90	68				
105.70	124	171.80	531				
115.70	116	172.95	310				
116.80	242	173.90	23547				
117.70	77	174.95	1774				
118.70	277	175.90	22981				
127.80	54	176.85	1500				

Instrument :

MSVOA_N

ClientSampleId :

BFB