
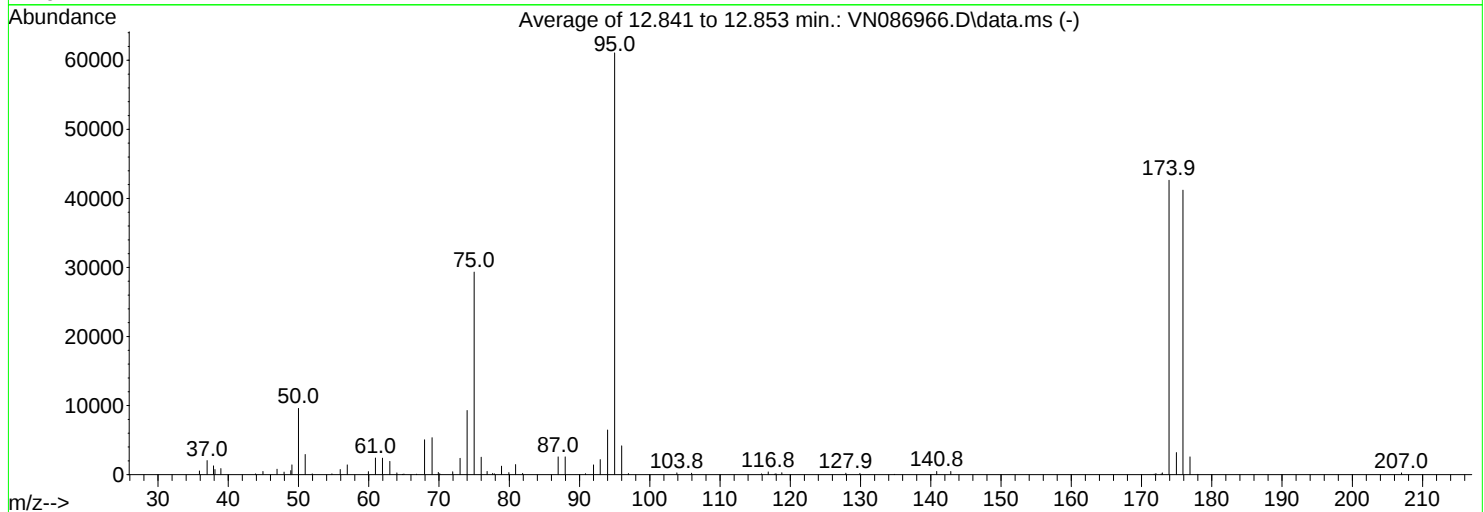


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061225\
Data File : VN086966.D
Acq On : 12 Jun 2025 10:25
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
Title : SW846 8260
Last Update : Sat Jun 07 02:12:50 2025

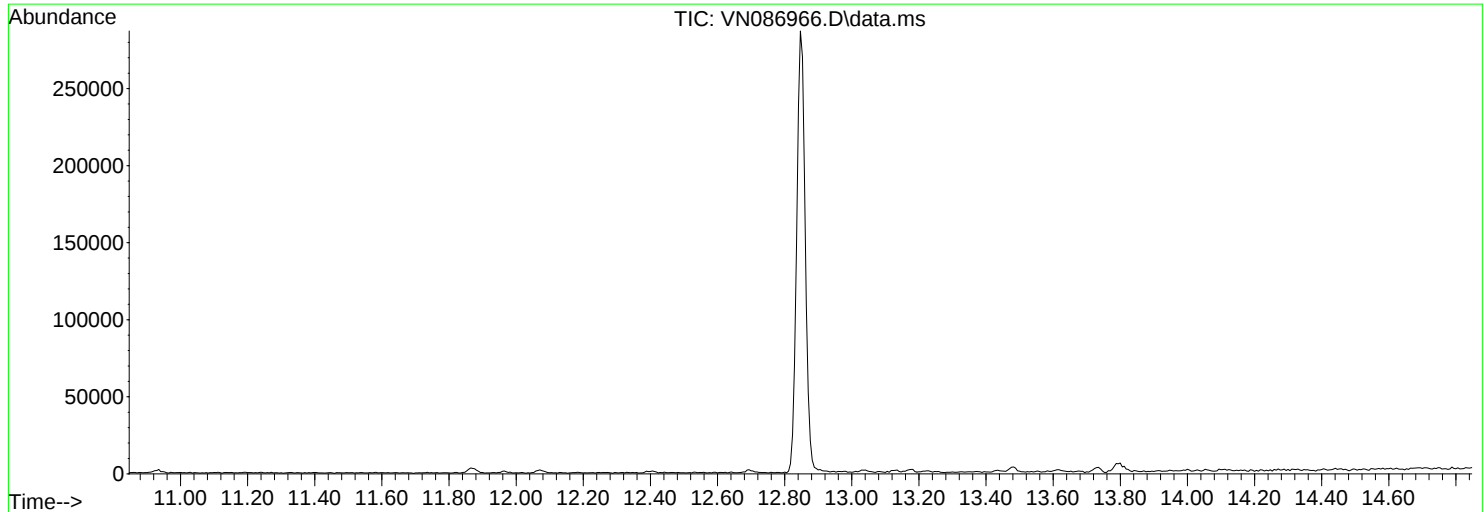

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.7	9593	PASS
75	95	30	60	48.0	29333	PASS
95	95	100	100	100.0	61077	PASS
96	95	5	9	6.8	4173	PASS
173	174	0.00	2	0.6	261	PASS
174	95	50	100	69.8	42635	PASS
175	174	5	9	7.5	3192	PASS
176	174	95	101	96.6	41189	PASS
177	176	5	9	6.2	2568	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	524	50.00	9593	64.80	52	76.00	252
37.00	2036	50.95	2916	65.00	82	76.85	46
37.90	1270	51.95	114	66.80	72	77.65	19
38.10	748	54.75	125	67.95	5061	77.90	12
38.95	873	55.95	733	69.00	5363	78.90	1239
43.90	127	56.95	1405	69.90	331	79.95	312
44.95	472	59.95	453	70.10	138	80.90	1450
46.95	797	60.95	2414	71.95	420	81.90	197
47.95	360	61.95	2399	73.00	2369	86.95	2566
48.90	571	63.00	1927	74.00	9297	87.95	2571
49.05	1425	64.00	259	75.00	29333	90.85	132

Average of 12.841 to 12.853 min.: VN086966.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.00	1404	117.95	135	173.90	42635		
92.95	2173	118.80	291	174.95	3192		
94.00	6466	127.90	200	175.90	41189		
95.00	61077	129.90	179	176.90	2568		
96.00	4173	134.80	53	178.00	56		
96.95	155	140.85	472	207.00	257		
103.85	255	142.85	455				
105.95	221	171.80	64				
115.90	128	172.05	159				
116.85	389	172.80	93				
117.80	63	172.95	261				

Instrument :

MSVOA_N

ClientSampleId :

BFB