


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN061318\
Data File : VN049210.D
Acq On : 13 Jun 2018 19:44
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061318W.M
Title : SW846 8260
Last Update : Thu Jun 14 05:15:23 2018

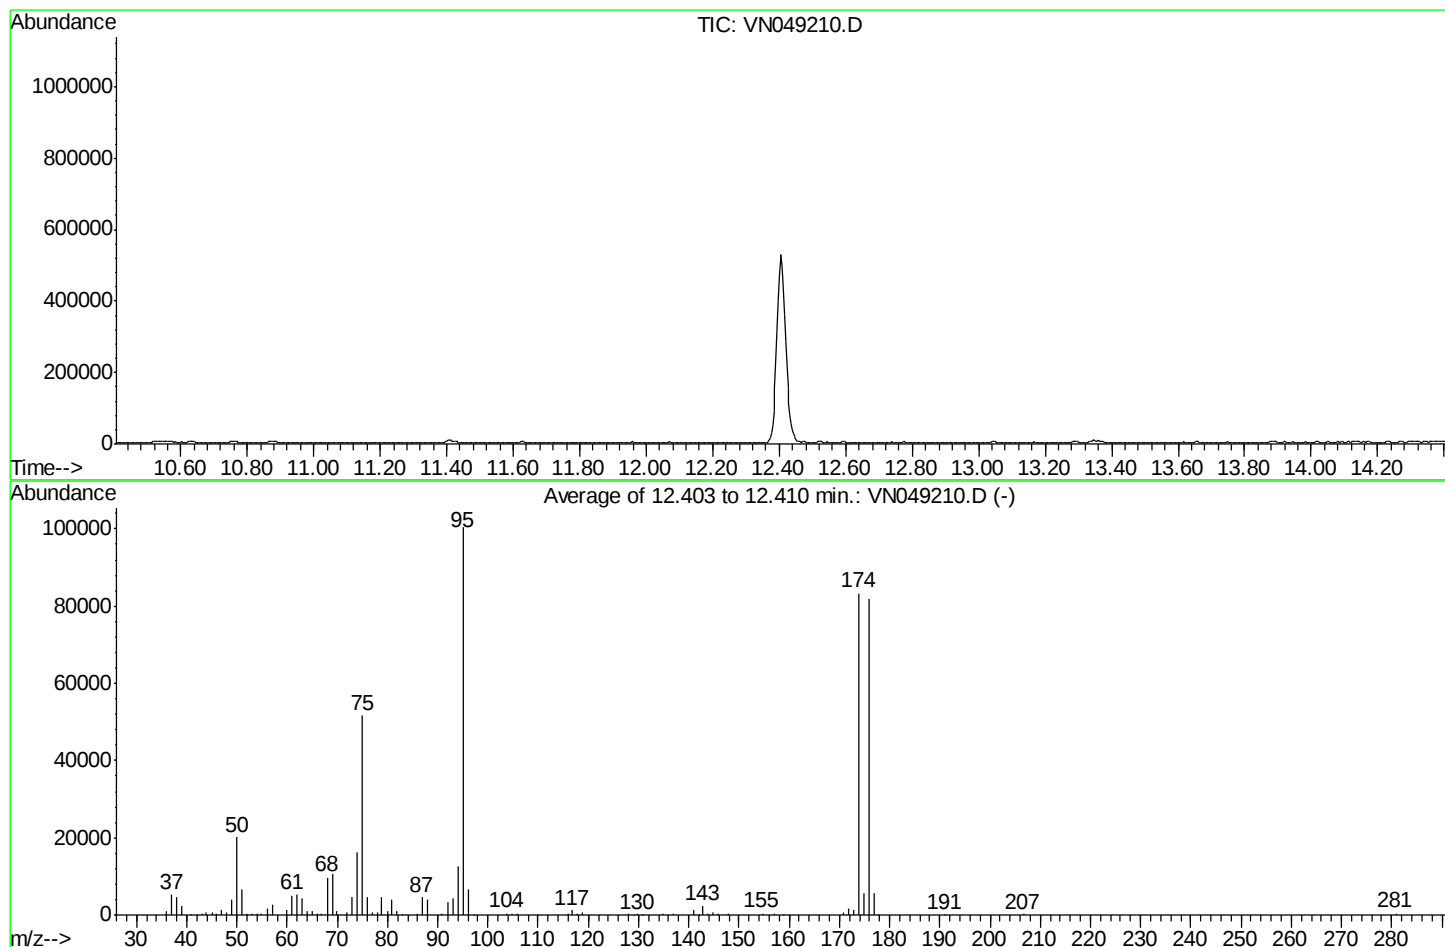

AutoFind: Scans 3363, 3364, 3365; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	20149	PASS
75	95	30	60	51.4	51640	PASS
95	95	100	100	100.0	100402	PASS
96	95	5	9	6.6	6610	PASS
173	174	0.00	2	1.5	1243	PASS
174	95	50	100	82.9	83218	PASS
175	174	5	9	6.6	5493	PASS
176	174	95	101	98.5	81936	PASS
177	176	5	9	6.9	5614	PASS