

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061322\
 Data File : VN072824.D
 Acq On : 14 Jun 2022 03:25
 Operator : JC\MD
 Sample : N3304-12
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 WC-14A-1A-6-G

Quant Time: Jun 14 05:25:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061322W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 13 17:28:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.081	168	143626	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.963	114	299651	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.745	117	271680	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.668	152	96980	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	230084	57.216	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 114.440%			
35) Dibromofluoromethane	8.016	113	156308	52.376	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 104.760%			
50) Toluene-d8	10.439	98	517411	43.171	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 86.340%			
62) 4-Bromofluorobenzene	12.727	95	186650	44.070	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 88.140%			
Target Compounds						
					Qvalue	
3) Chloromethane	2.293	50	77	Below Cal	#	43
6) Chloroethane	2.999	64	313	Below Cal	#	42
11) Tert butyl alcohol	5.304	59	1126	0.285	ug/l #	72
16) Acetone	4.281	43	69529	38.074	ug/l	92
17) Carbon Disulfide	4.510	76	1145	Below Cal	#	75
18) Methyl Acetate	4.857	43	11197	2.333	ug/l	91
20) Methylene Chloride	5.087	84	29015	10.613	ug/l #	82
25) 2-Butanone	7.334	43	10423	3.639	ug/l #	69
29) Tetrahydrofuran	7.698	42	880	0.496	ug/l #	53
31) Cyclohexane	8.086	56	5237	Below Cal	#	42
36) 1,1-Dichloropropene	8.081	75	15939	3.833	ug/l #	49
38) Carbon Tetrachloride	8.086	117	18443	4.231	ug/l #	15
39) Methylcyclohexane	9.457	83	1484	0.315	ug/l #	79
43) Isopropyl Acetate	8.563	43	50426	5.127	ug/l #	76
45) 1,2-Dichloropropane	9.616	63	1923	0.555	ug/l #	44
48) Methyl methacrylate	9.539	41	11148	2.443	ug/l #	10
49) 1,4-Dioxane	9.628	88	139	1.783	ug/l #	1
51) 4-Methyl-2-Pentanone	10.328	43	9251	1.418	ug/l #	85
54) cis-1,3-Dichloropropene	10.239	75	46914	8.621	ug/l #	75
55) 1,1,2-Trichloroethane	10.875	97	845	0.255	ug/l #	16
57) 1,3-Dichloropropane	11.086	76	23431	3.938	ug/l #	42
59) 2-Hexanone	11.086	43	391035	80.918	ug/l #	44
74) N-amyl acetate	12.363	43	3013	0.636	ug/l #	41
76) 1,2,3-Trichloropropane	12.727	75	110906	33.320	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.727	75	110906	101.556	ug/l #	10
87) 1,3-Dichlorobenzene	13.692	146	2677	0.787	ug/l #	42
88) 1,4-Dichlorobenzene	13.692	146	2677	0.798	ug/l #	40
90) Hexachloroethane	14.315	117	516	0.325	ug/l #	9
95) Naphthalene	15.504	128	3374	0.560	ug/l #	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061322\
Data File : VN072824.D
Acq On : 14 Jun 2022 03:25
Operator : JC\MD
Sample : N3304-12
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-6-G

Quant Time: Jun 14 05:25:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061322W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 13 17:28:28 2022
Response via : Initial Calibration




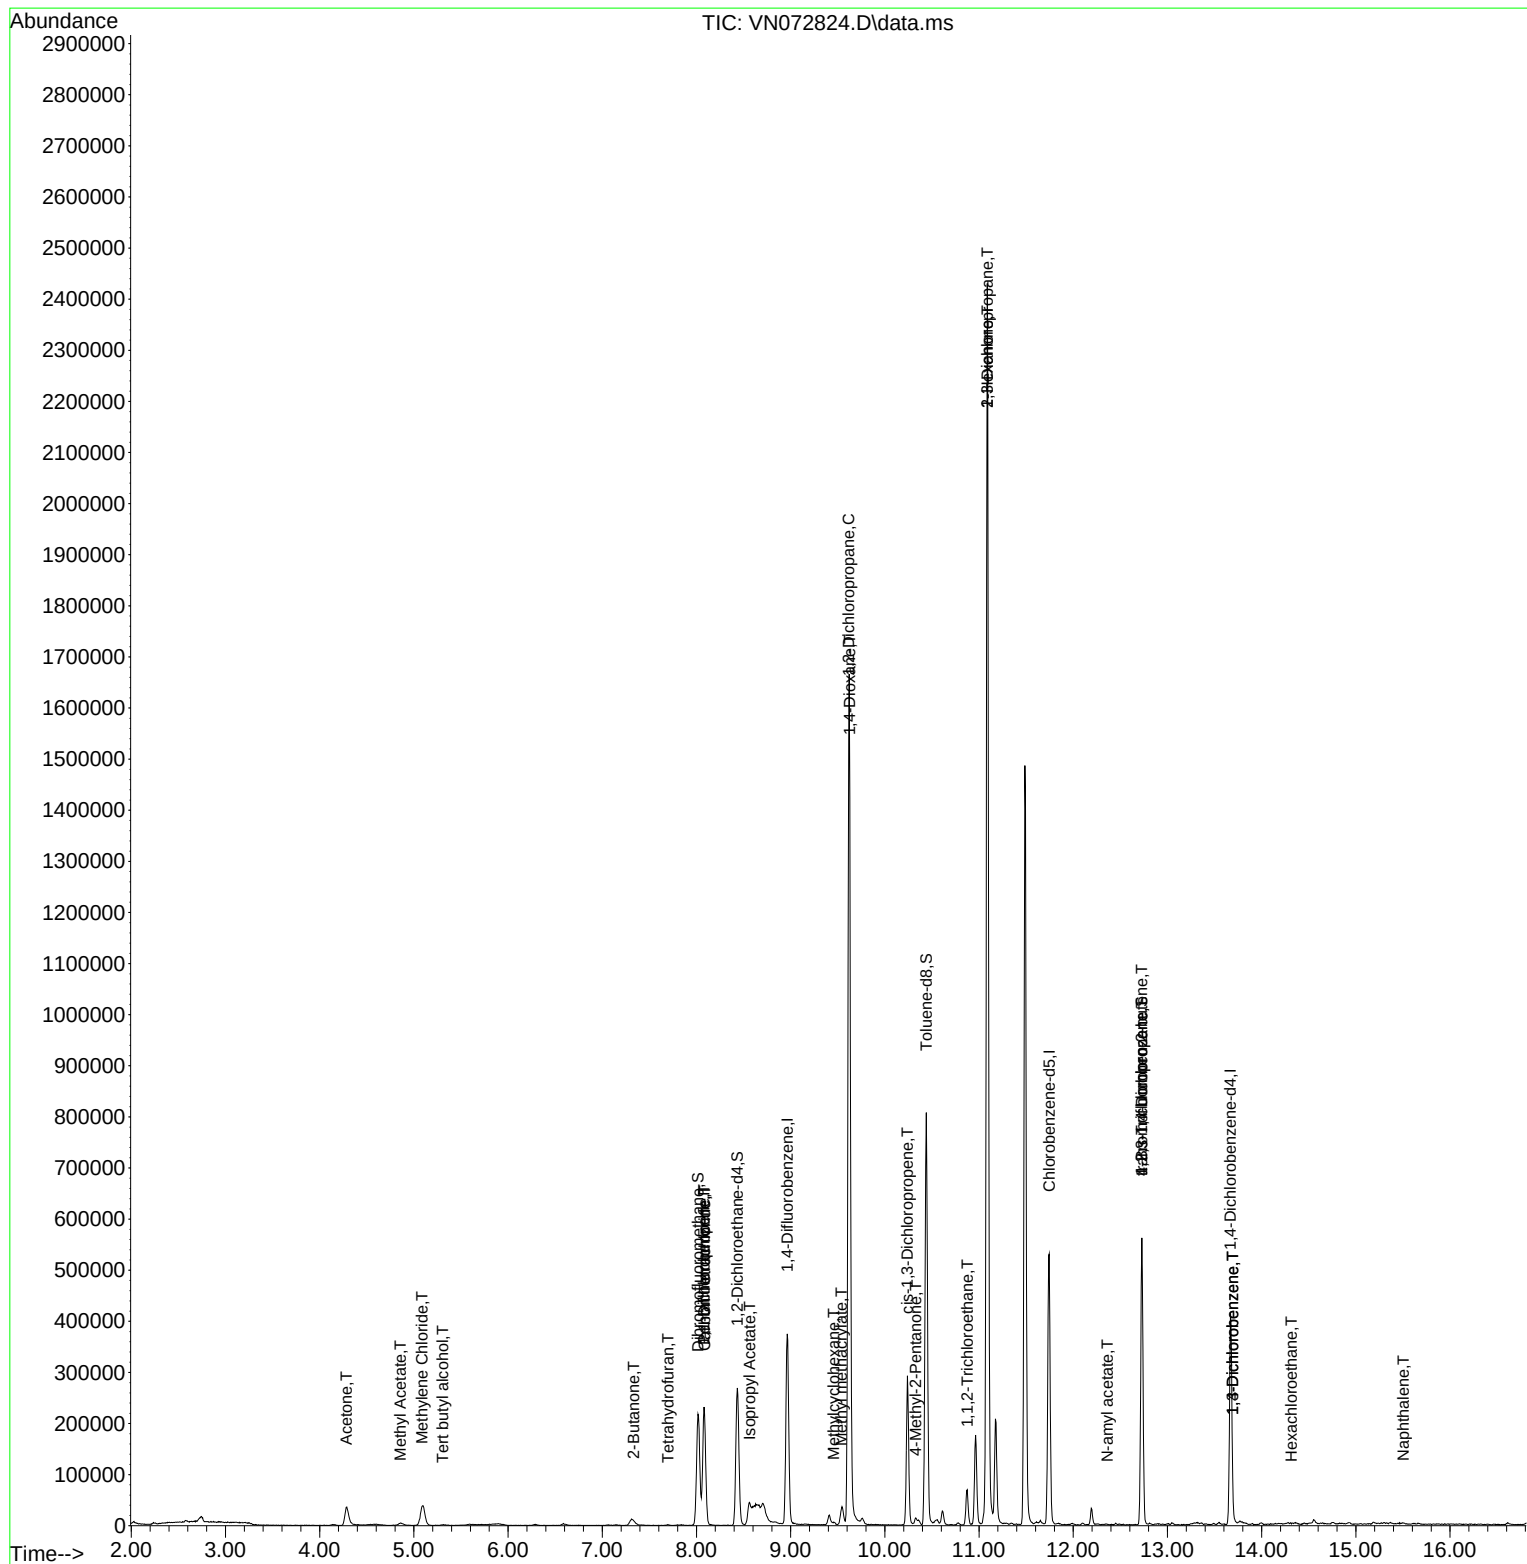




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. 0.001 min
Lab File: VN072824.D
Acq: 14 Jun 2022 03:25




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-6-G


Tgt Ion:168 Resp: 143626
Ion Ratio Lower Upper
168 100
99 82.1 42.3 63.5#

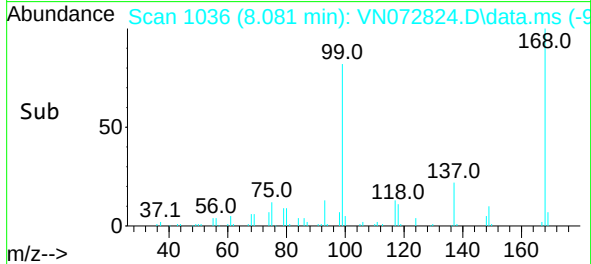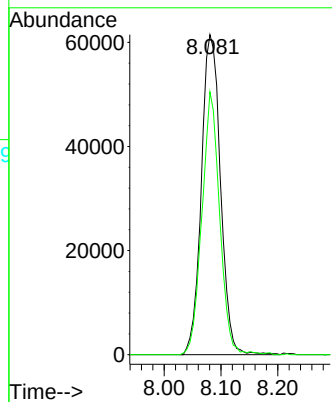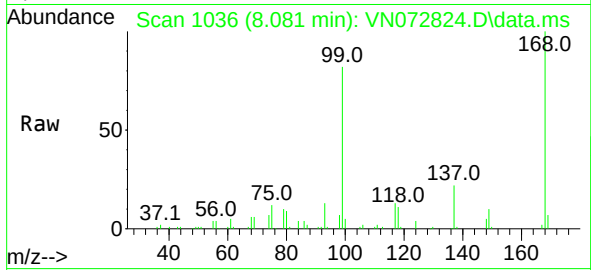

#3
Chloromethane
Concen: Below Cal
RT: 2.293 min Scan# 52
Delta R.T. -0.000 min
Lab File: VN072824.D
Acq: 14 Jun 2022 03:25

Tgt Ion: 50 Resp: 77
Ion Ratio Lower Upper
50 100
52 0.0 25.7 38.5#


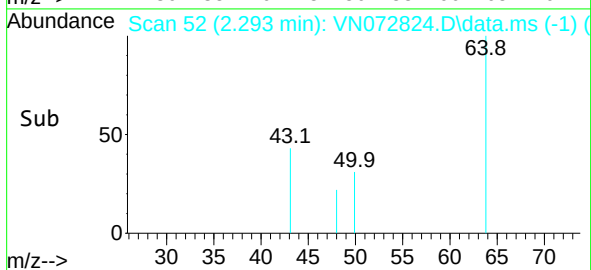

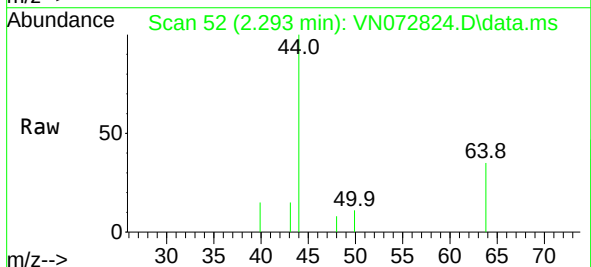




#6
Chloroethane
Concen: Below Cal
RT: 2.999 min Scan# 11
Delta R.T. 0.001 min
Lab File: VN072824.D
Acq: 14 Jun 2022 03:25




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-6-G


Tgt Ion: 64 Resp: 313
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#

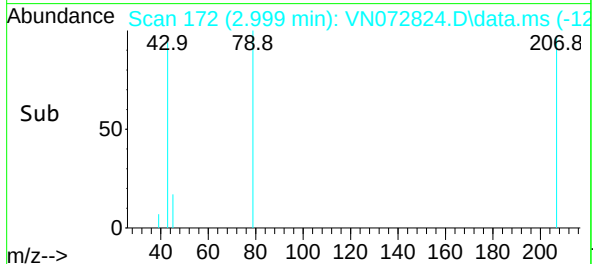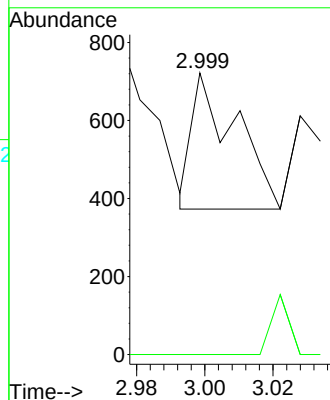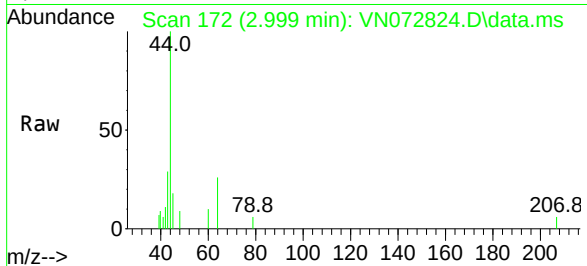

#11
Tert butyl alcohol
Concen: 0.285 ug/l
RT: 5.304 min Scan# 564
Delta R.T. -0.059 min
Lab File: VN072824.D
Acq: 14 Jun 2022 03:25

Tgt Ion: 59 Resp: 1126
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

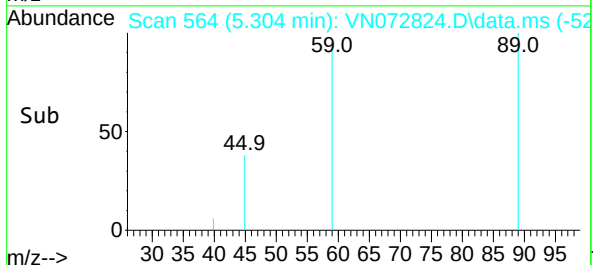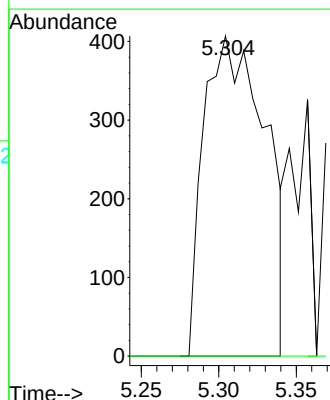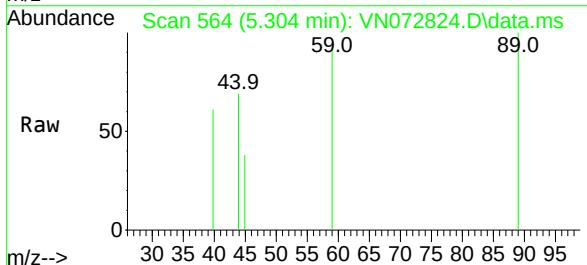



#16

Acetone

Concen: 38.074 ug/l

RT: 4.281 min Scan# 390

Delta R.T. -0.000 min

Lab File: VN072824.D

Acq: 14 Jun 2022 03:25

Instrument :

MSVOA_N

ClientSampleId :





WC-14A-1A-6-G

Tgt Ion: 43 Resp: 69529

Ion Ratio Lower Upper

43 100

58 28.1 26.0 39.0

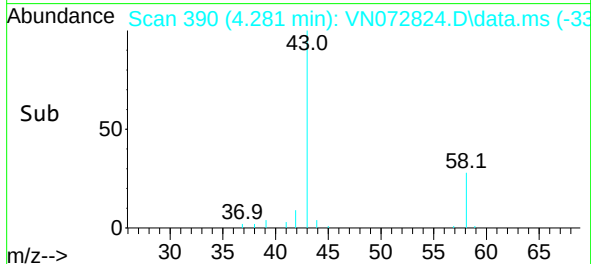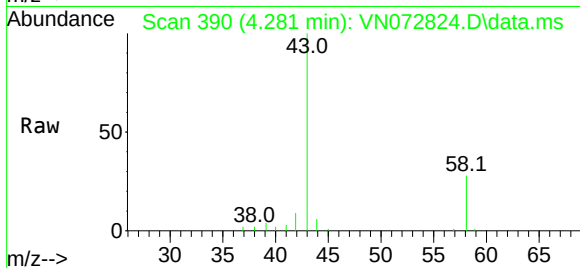

#17

Carbon Disulfide

Concen: Below Cal

RT: 4.510 min Scan# 429

Delta R.T. -0.012 min

Lab File: VN072824.D




Acq: 14 Jun 2022 03:25


Tgt Ion: 76 Resp: 1145

Ion Ratio Lower Upper

76 100

78 0.0 7.2 10.8#


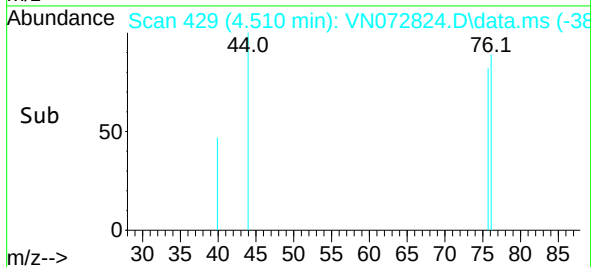

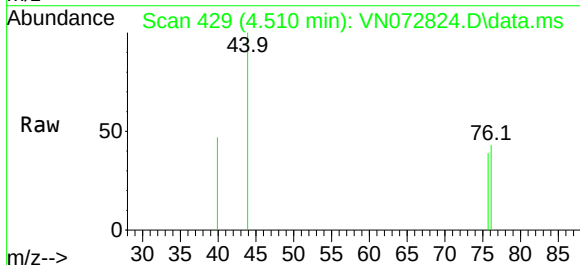


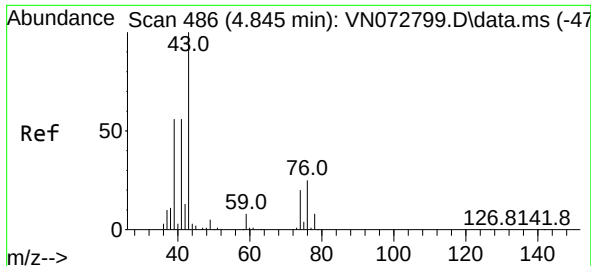

#18
Methyl Acetate
Concen: 2.333 ug/l
RT: 4.857 min Scan# 486
Delta R.T. 0.012 min
Lab File: VN072824.D
Acq: 14 Jun 2022 03:25




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-6-G


Tgt Ion: 43 Resp: 11197
Ion Ratio Lower Upper
43 100
74 22.1 21.6 32.4

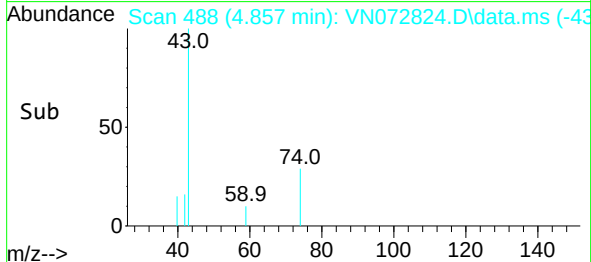

#20
Methylene Chloride
Concen: 10.613 ug/l
RT: 5.087 min Scan# 527
Delta R.T. -0.000 min
Lab File: VN072824.D
Acq: 14 Jun 2022 03:25

Tgt Ion: 84 Resp: 29015
Ion Ratio Lower Upper
84 100
49 135.0 88.3 132.5#
51 48.8 28.2 42.2#
86 59.7 50.6 76.0

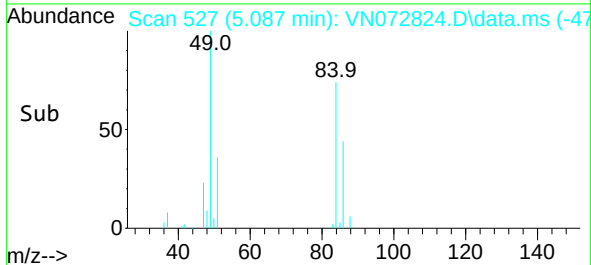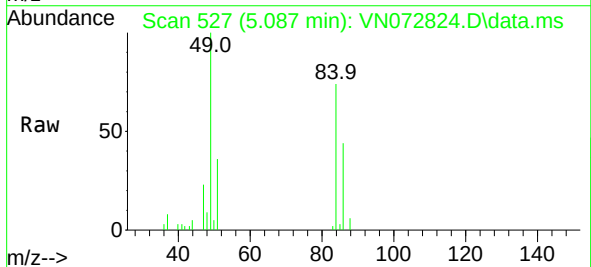



#25

2-Butanone

Concen: 3.639 ug/l

RT: 7.334 min Scan# 908

Delta R.T. 0.006 min

Lab File: VN072824.D

Acq: 14 Jun 2022 03:25

Instrument :

MSVOA_N

ClientSampleId :





WC-14A-1A-6-G

Tgt Ion: 43 Resp: 10423

Ion Ratio Lower Upper

43 100

72 13.0 23.7 35.5#

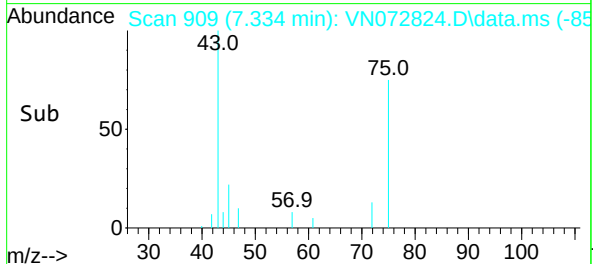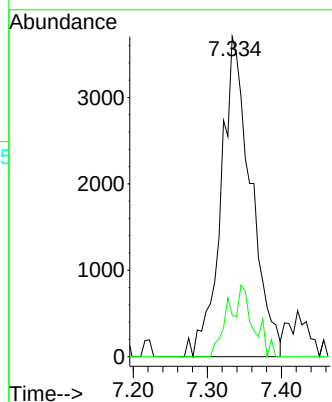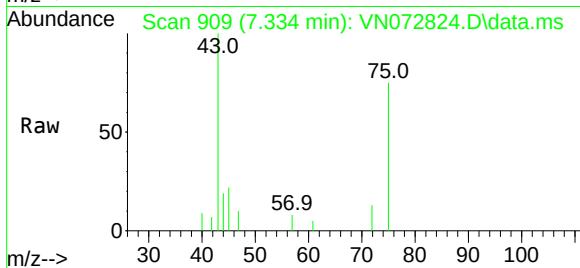

#29

Tetrahydrofuran

Concen: 0.496 ug/l

RT: 7.698 min Scan# 971

Delta R.T. 0.017 min

Lab File: VN072824.D

Acq: 14 Jun 2022 03:25




Tgt Ion: 42 Resp: 880


Ion Ratio Lower Upper

42 100

72 22.8 39.7 59.5#

71 8.4 36.6 55.0#




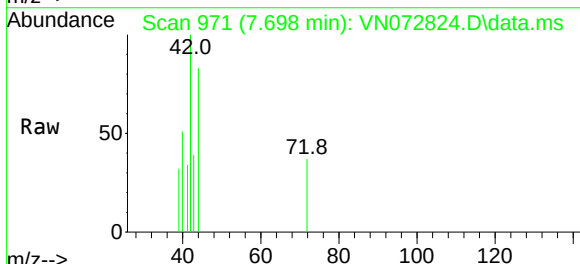




#31
Cyclohexane
Concen: Below Cal
RT: 8.086 min Scan# 1037
Delta R.T. -0.006 min
Lab File: VN072824.D
Acq: 14 Jun 2022 03:25




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-6-G


Tgt Ion: 56 Resp: 5237
Ion Ratio Lower Upper
56 100
69 139.0 27.8 41.8#
84 82.9 76.9 115.3

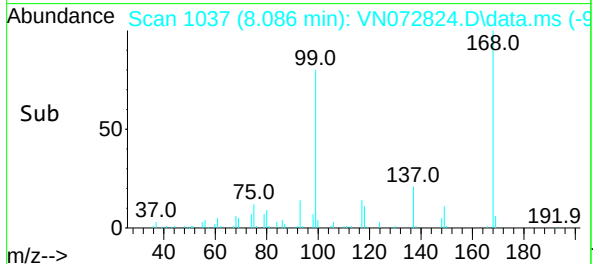

#33
1,2-Dichloroethane-d4
Concen: 57.216 ug/l
RT: 8.434 min Scan# 1096
Delta R.T. 0.001 min
Lab File: VN072824.D
Acq: 14 Jun 2022 03:25

Tgt Ion: 65 Resp: 230084
Ion Ratio Lower Upper
65 100
67 50.1 0.0 104.8

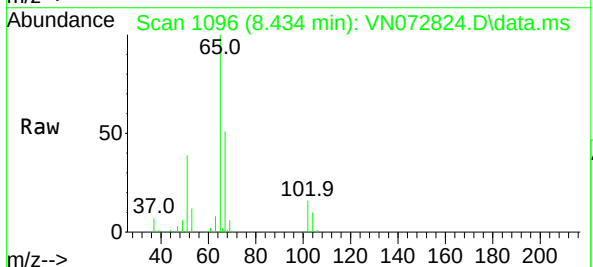



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. -0.000 min

Lab File: VN072824.D

Acq: 14 Jun 2022 03:25

Instrument :

MSVOA_N

ClientSampleId :

WC-14A-1A-6-G





Tgt Ion:114 Resp: 299651

Ion Ratio Lower Upper

114 100

63 25.9 0.0 40.0

88 18.1 0.0 32.6

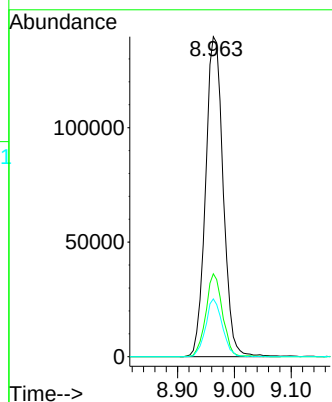

#35

Dibromofluoromethane

Concen: 52.376 ug/l

RT: 8.016 min Scan# 1025

Delta R.T. -0.000 min

Lab File: VN072824.D

Acq: 14 Jun 2022 03:25




Tgt Ion:113 Resp: 156308


Ion Ratio Lower Upper

113 100

111 104.5 81.4 122.0

192 14.6 17.0 25.6#

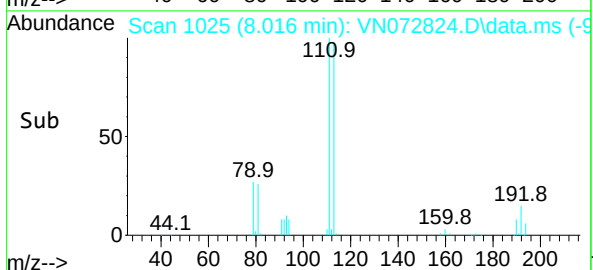



#36

1,1-Dichloropropene

Concen: 3.833 ug/l

RT: 8.081 min Scan# 1036

Delta R.T. -0.135 min

Lab File: VN072824.D

Acq: 14 Jun 2022 03:25

Instrument :

MSVOA_N

ClientSampleId :

WC-14A-1A-6-G





Tgt Ion: 75 Resp: 15939

Ion Ratio Lower Upper

75 100

110 8.8 18.3 54.8#

77 0.0 25.1 37.7#

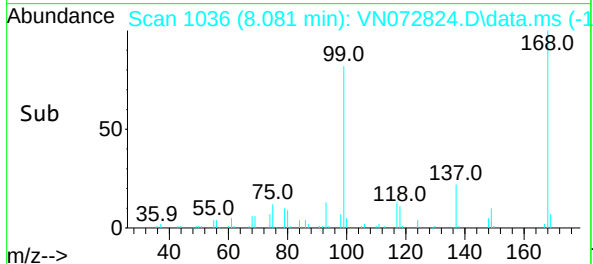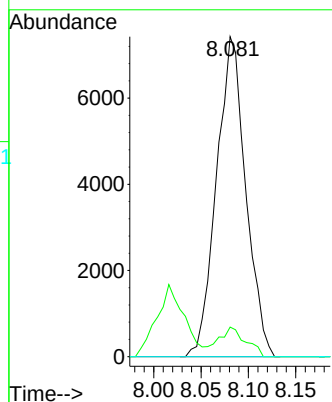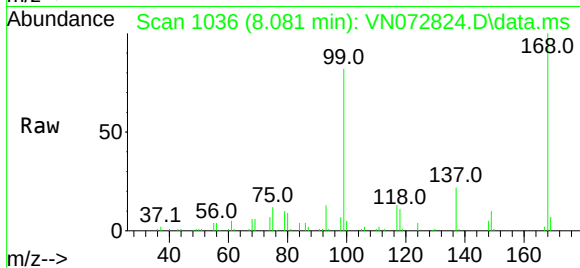

#38

Carbon Tetrachloride

Concen: 4.231 ug/l

RT: 8.086 min Scan# 1037

Delta R.T. -0.118 min

Lab File: VN072824.D

Acq: 14 Jun 2022 03:25




Tgt Ion: 117 Resp: 18443


Ion Ratio Lower Upper

117 100

119 3.7 75.8 113.8#

121 0.0 24.6 37.0#

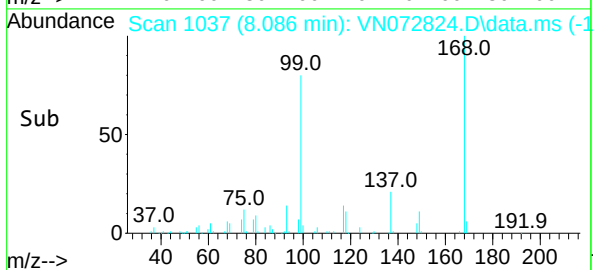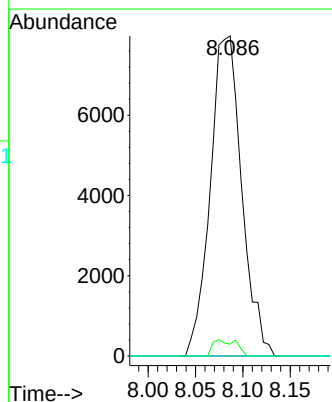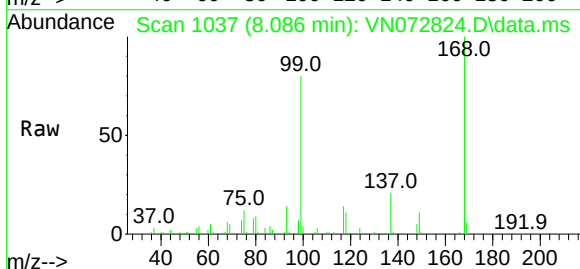



#39

Methylcyclohexane

Concen: 0.315 ug/l

RT: 9.457 min Scan# 1117

Delta R.T. -0.000 min

Lab File: VN072824.D

Acq: 14 Jun 2022 03:25





Instrument :

MSVOA_N

ClientSampleId :

WC-14A-1A-6-G

Tgt Ion: 83	Resp: 1484
Ion Ratio	Lower Upper
83	100
55	53.0 57.8 86.8#
98	37.8 39.4 59.2#

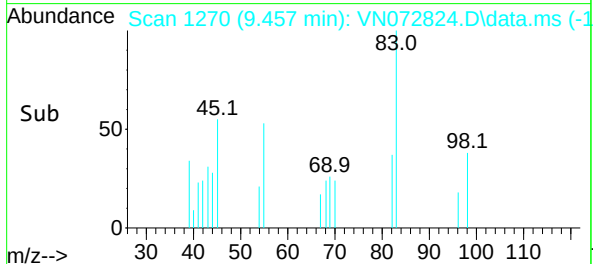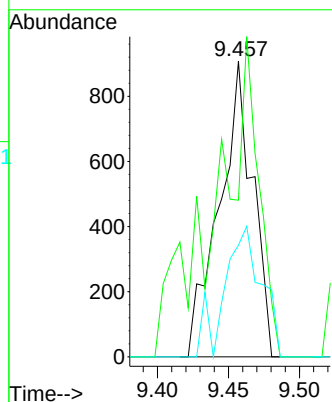

#43

Isopropyl Acetate

Concen: 5.127 ug/l




RT: 8.563 min Scan# 1118


Delta R.T. 0.006 min

Lab File: VN072824.D

Acq: 14 Jun 2022 03:25

Tgt Ion: 43	Resp: 50426
Ion Ratio	Lower Upper
43	100
61	13.4 21.9 32.9#
87	7.7 12.0 18.0#

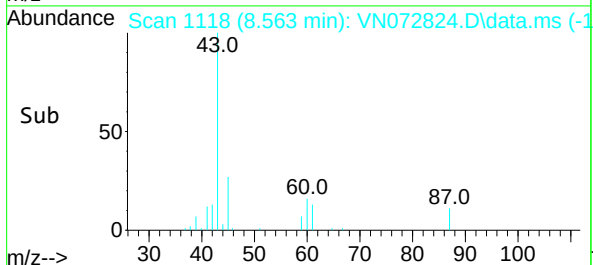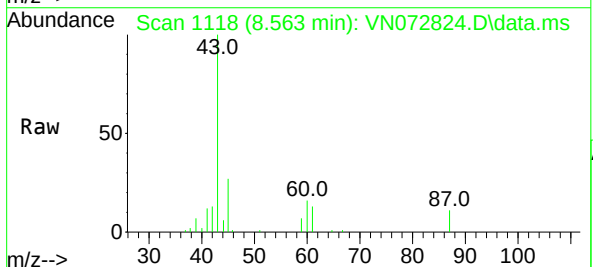



#45

1,2-Dichloropropane

Concen: 0.555 ug/l

RT: 9.616 min Scan# 1297

Delta R.T. 0.130 min

Lab File: VN072824.D

Acq: 14 Jun 2022 03:25

Instrument :

MSVOA_N

ClientSampleId :





WC-14A-1A-6-G

Tgt Ion: 63 Resp: 1923

Ion Ratio Lower Upper

63 100

65 0.0 24.9 37.3#

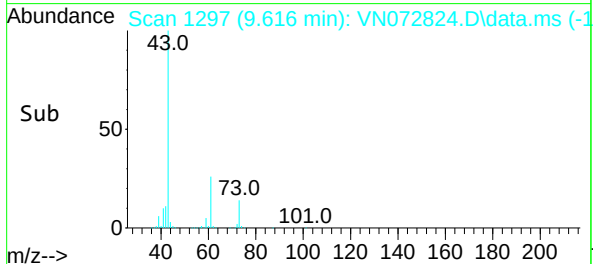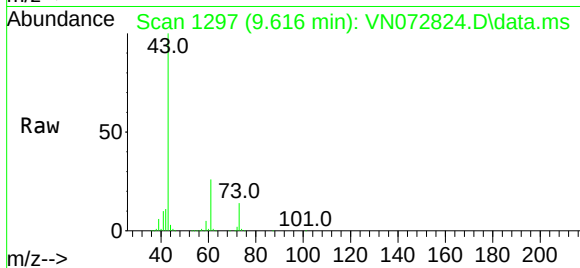

#48

Methyl methacrylate

Concen: 2.443 ug/l

RT: 9.539 min Scan# 1284

Delta R.T. -0.018 min

Lab File: VN072824.D

Acq: 14 Jun 2022 03:25




Tgt Ion: 41 Resp: 11148


Ion Ratio Lower Upper

41 100

69 0.0 74.7 112.1#

39 0.0 45.6 68.4#

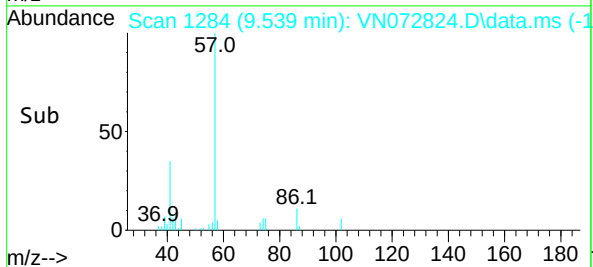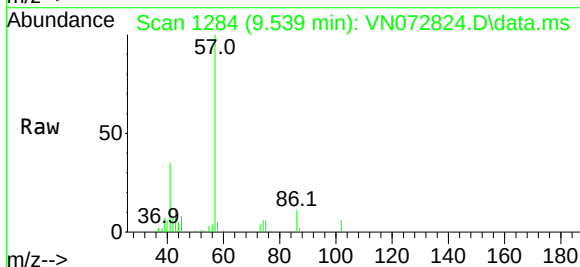



#49

1,4-Dioxane

Concen: 1.783 ug/l

RT: 9.628 min Scan# 1288

Delta R.T. 0.065 min

Lab File: VN072824.D

Acq: 14 Jun 2022 03:25

Instrument :

MSVOA_N

ClientSampleId :

WC-14A-1A-6-G





Tgt Ion: 88 Resp: 139

Ion Ratio Lower Upper

88 100

43 1196819.4 20.2 30.4#

58 5223.0 54.2 81.4#

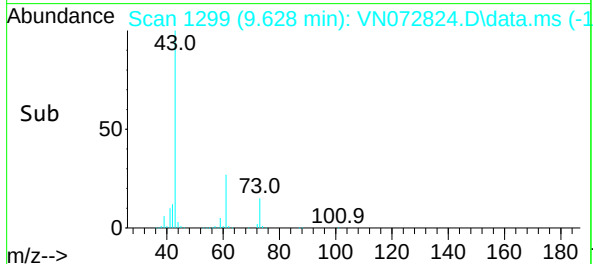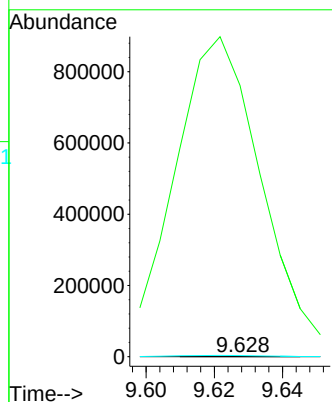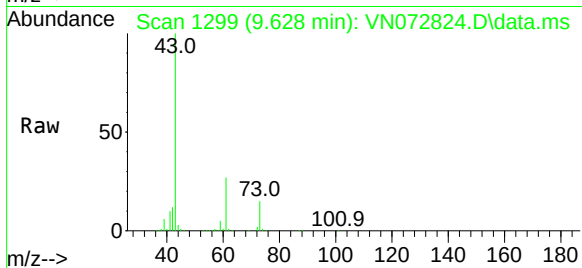

#50

Toluene-d8

Concen: 43.171 ug/l

RT: 10.439 min Scan# 1437

Delta R.T. 0.000 min

Lab File: VN072824.D




Acq: 14 Jun 2022 03:25


Tgt Ion: 98 Resp: 517411

Ion Ratio Lower Upper

98 100

100 64.5 52.6 78.8


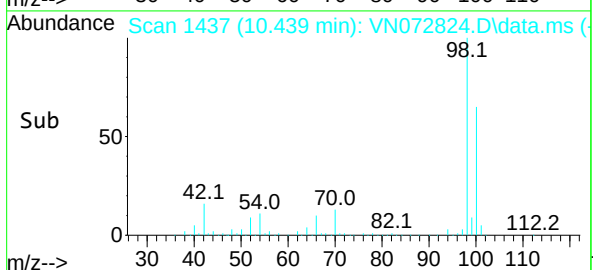

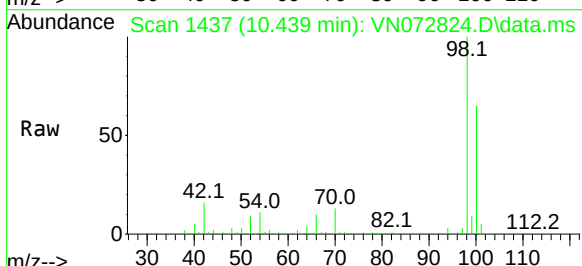




#51
4-Methyl-2-Pentanone
Concen: 1.418 ug/l
RT: 10.328 min Scan# 1418
Delta R.T. 0.001 min
Lab File: VN072824.D
Acq: 14 Jun 2022 03:25




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-6-G


Tgt Ion: 43 Resp: 9251
Ion Ratio Lower Upper
43 100
58 32.9 34.1 51.1#

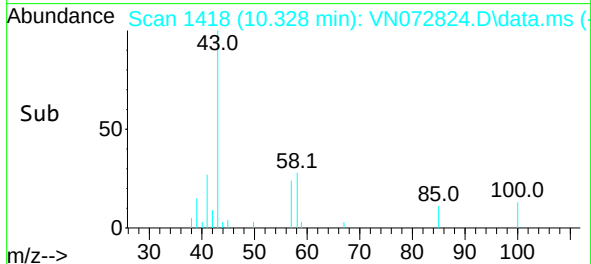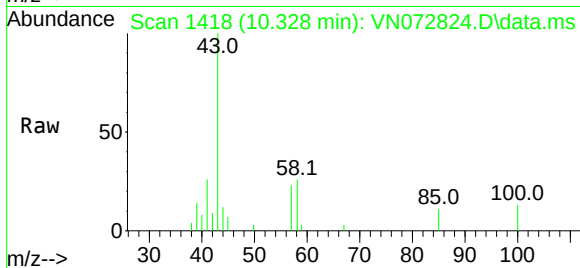

#54
cis-1,3-Dichloropropene
Concen: 8.621 ug/l
RT: 10.239 min Scan# 1403
Delta R.T. 0.053 min
Lab File: VN072824.D
Acq: 14 Jun 2022 03:25

Tgt Ion: 75 Resp: 46914
Ion Ratio Lower Upper
75 100
77 0.7 25.2 37.8#
39 42.2 35.7 53.5


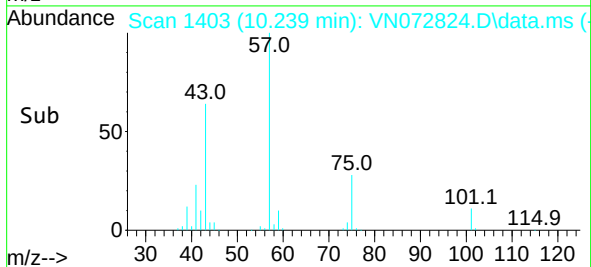

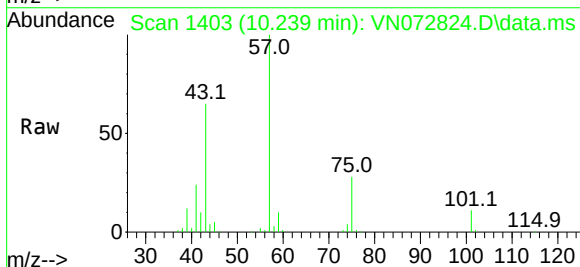


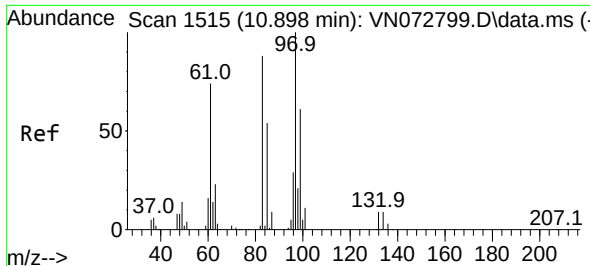

#55
 1,1,2-Trichloroethane
 Concen: 0.255 ug/l
 RT: 10.875 min Scan# 11
 Delta R.T. -0.023 min
 Lab File: VN072824.D
 Acq: 14 Jun 2022 03:25




Instrument :
 MSVOA_N
 ClientSampleId :
 WC-14A-1A-6-G


Tgt Ion: 97	Resp:	845
Ion	Ratio	Lower Upper
97	100	
83	0.0	66.2 99.4#
85	0.0	43.9 65.9#
99	0.0	50.6 76.0#

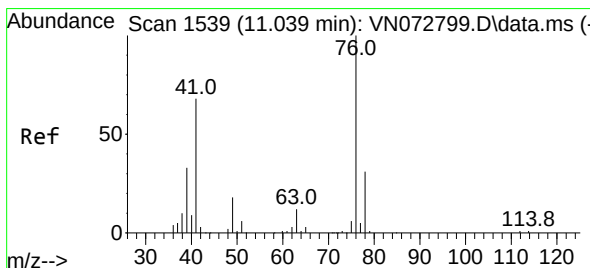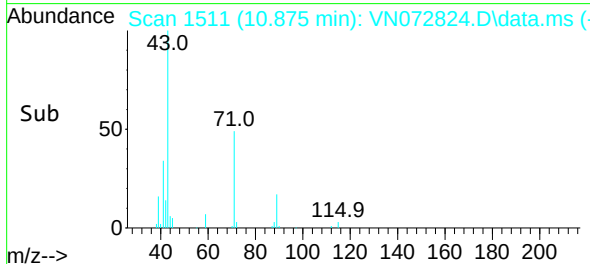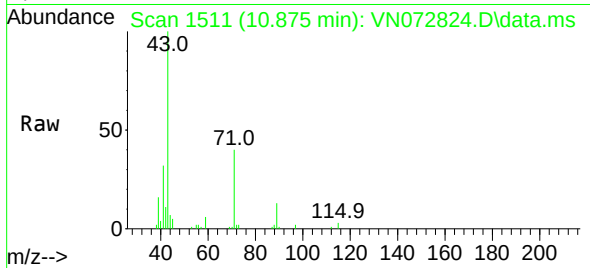

#57
 1,3-Dichloropropane
 Concen: 3.938 ug/l
 RT: 11.086 min Scan# 1547
 Delta R.T. 0.047 min
 Lab File: VN072824.D
 Acq: 14 Jun 2022 03:25

Tgt Ion: 76	Resp:	23431
Ion	Ratio	Lower Upper
76	100	
78	0.0	26.2 39.2#


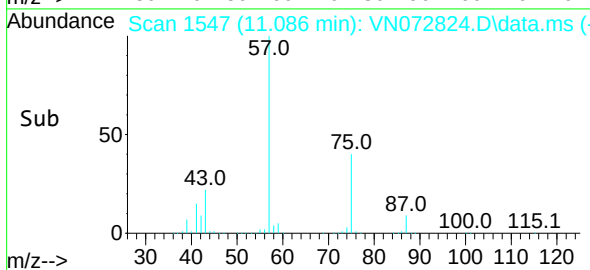

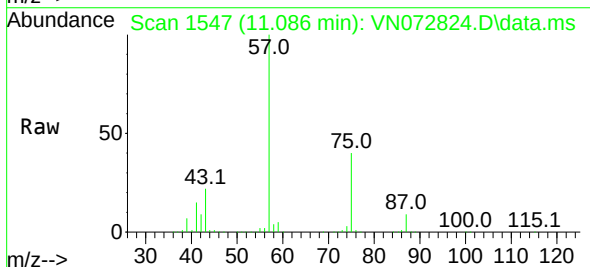


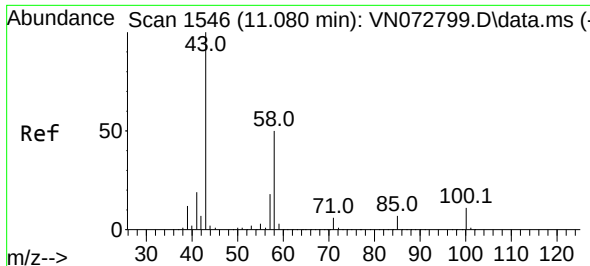

#59
2-Hexanone
Concen: 80.918 ug/l
RT: 11.086 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN072824.D
Acq: 14 Jun 2022 03:25




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-6-G


Tgt Ion: 43 Resp: 391035
Ion Ratio Lower Upper
43 100
58 17.2 29.7 89.1#

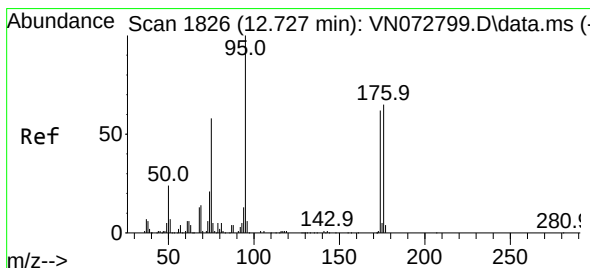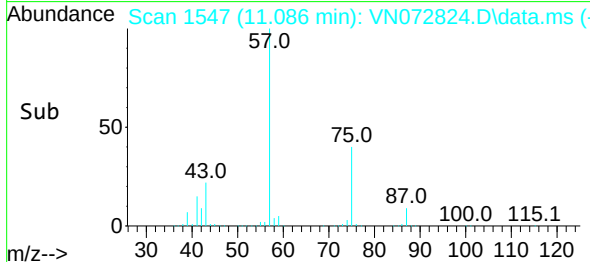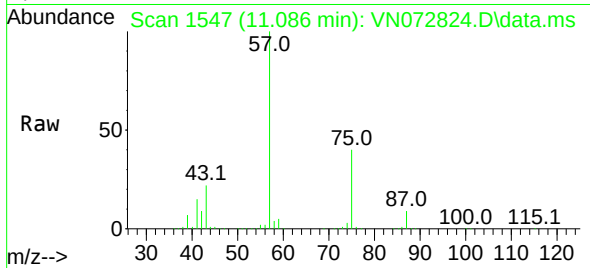

#62
4-Bromofluorobenzene
Concen: 44.070 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN072824.D
Acq: 14 Jun 2022 03:25

Tgt Ion: 95 Resp: 186650
Ion Ratio Lower Upper
95 100
174 61.4 0.0 167.6
176 57.6 0.0 163.4


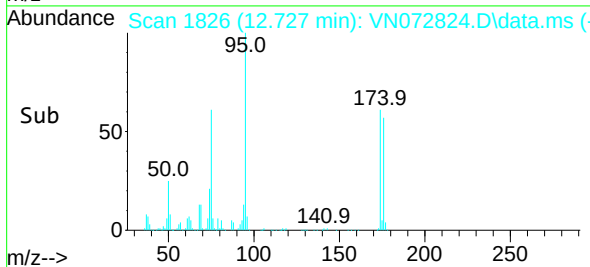

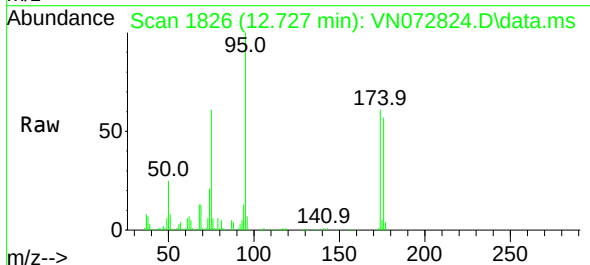


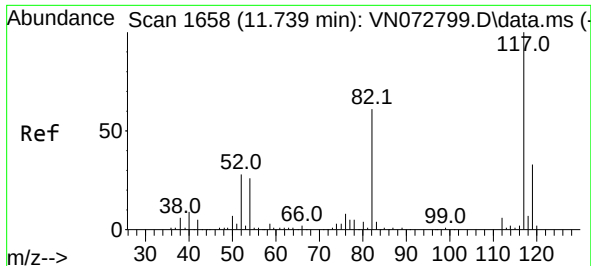

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.745 min Scan# 117
Delta R.T. 0.006 min
Lab File: VN072824.D
Acq: 14 Jun 2022 03:25




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-6-G


Tgt Ion:117 Resp: 271680
Ion Ratio Lower Upper
117 100
82 63.2 44.2 66.2
119 32.8 25.4 38.0

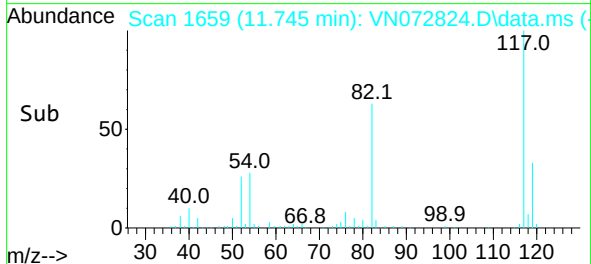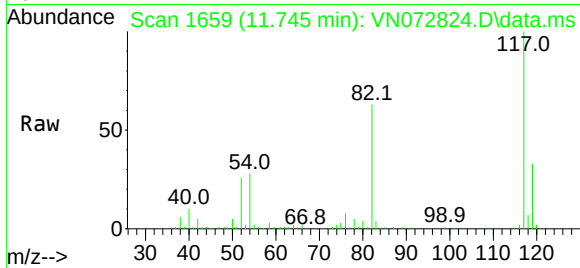

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.668 min Scan# 1986
Delta R.T. 0.000 min
Lab File: VN072824.D
Acq: 14 Jun 2022 03:25

Tgt Ion:152 Resp: 96980
Ion Ratio Lower Upper
152 100
115 67.7 28.9 86.7
150 156.7 0.0 356.2

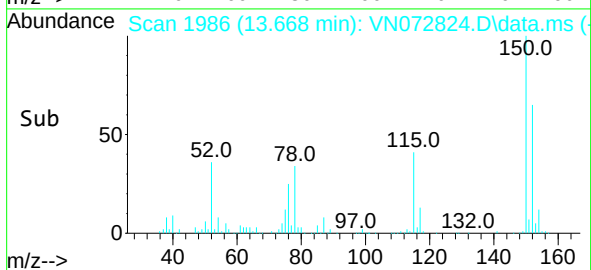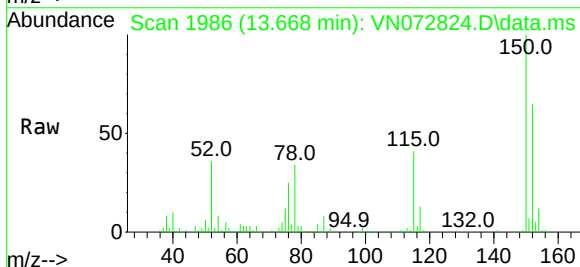

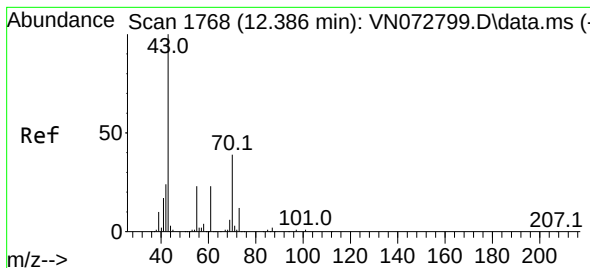

#74

N-amy1 acetate

Concen: 0.636 ug/l

RT: 12.363 min Scan# 1

Delta R.T. -0.023 min

Lab File: VN072824.D


Acq: 14 Jun 2022 03:25

Instrument :

MSVOA_N

ClientSampleId :

WC-14A-1A-6-G

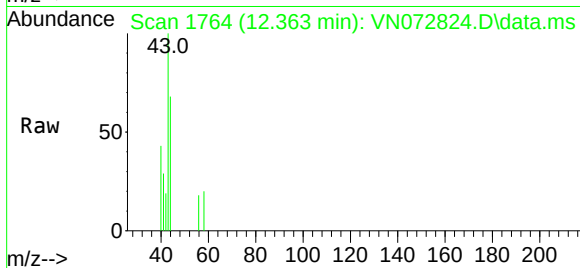

Tgt Ion: 43 Resp: 3013




Ion Ratio Lower Upper

43 100

70 2.1 39.0 58.4#

55 2.0 21.1 31.7#

61 0.0 21.1 31.7#

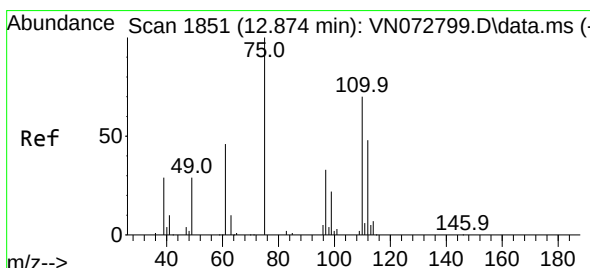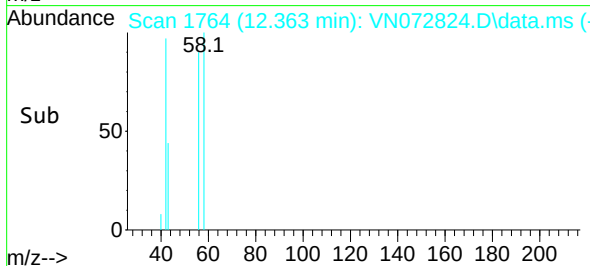

#76

1,2,3-Trichloropropane

Concen: 33.320 ug/l

RT: 12.727 min Scan# 1826

Delta R.T. -0.147 min

Lab File: VN072824.D




Acq: 14 Jun 2022 03:25


Tgt Ion: 75 Resp: 110906

Ion Ratio Lower Upper

75 100

77 1.4 98.5 295.5#


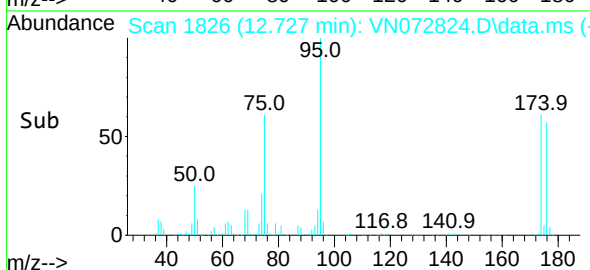

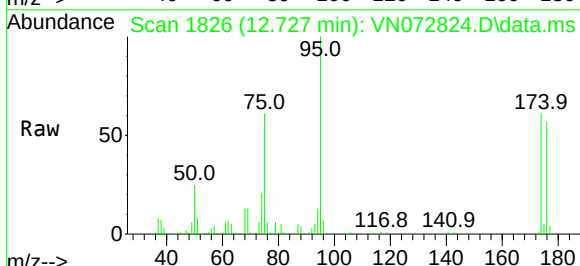




#81
trans-1,4-Dichloro-2-butene
Concen: 101.556 ug/l
RT: 12.727 min Scan# 11
Delta R.T. 0.106 min
Lab File: VN072824.D
Acq: 14 Jun 2022 03:25




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-6-G


Tgt Ion: 75 Resp: 110906
Ion Ratio Lower Upper
75 100
53 0.1 78.0 117.0#
89 0.0 37.2 55.8#

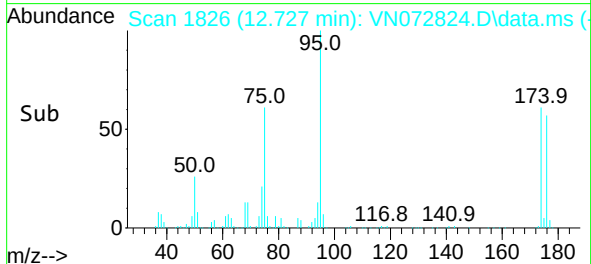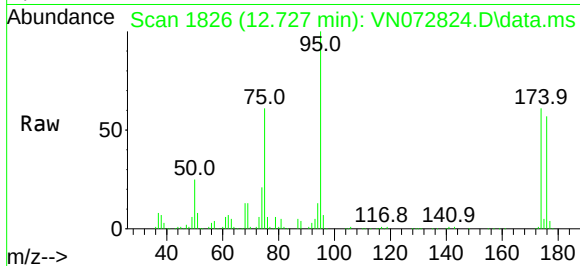

#87
1,3-Dichlorobenzene
Concen: 0.787 ug/l
RT: 13.692 min Scan# 1990
Delta R.T. 0.082 min
Lab File: VN072824.D
Acq: 14 Jun 2022 03:25

Tgt Ion:146 Resp: 2677
Ion Ratio Lower Upper
146 100
111 107.1 20.0 60.0#
148 84.5 32.0 96.0


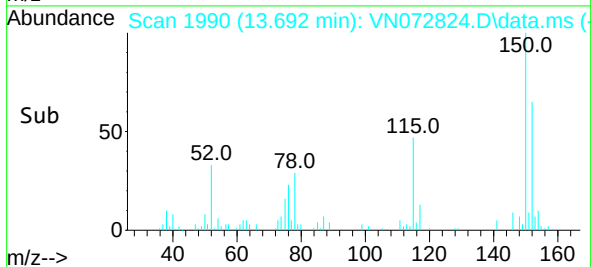

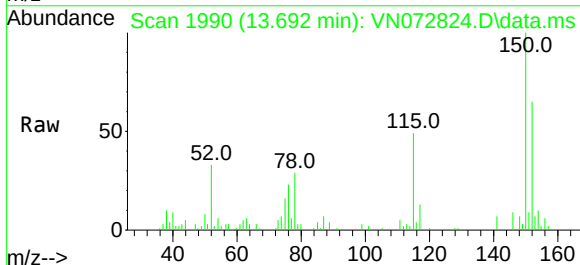




#88
1,4-Dichlorobenzene
Concen: 0.798 ug/l
RT: 13.692 min Scan# 1990
Delta R.T. -0.000 min
Lab File: VN072824.D
Acq: 14 Jun 2022 03:25




Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-6-G


Tgt Ion:146 Resp: 2677
Ion Ratio Lower Upper
146 100
111 107.1 19.1 57.1#
148 84.5 31.4 94.3

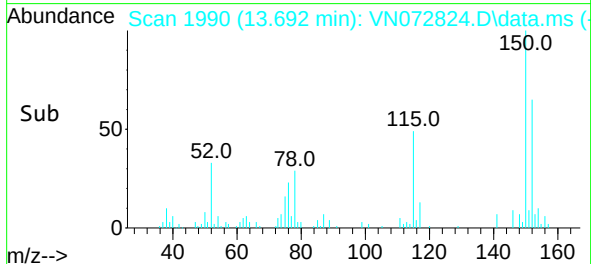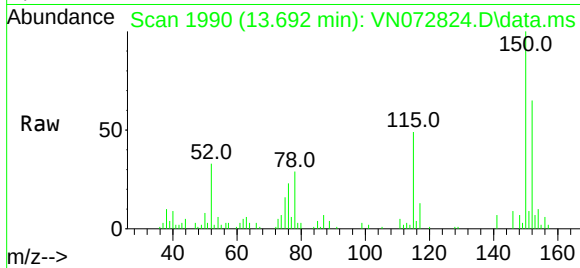

#90
Hexachloroethane
Concen: 0.325 ug/l
RT: 14.315 min Scan# 2096
Delta R.T. 0.106 min
Lab File: VN072824.D
Acq: 14 Jun 2022 03:25


Tgt Ion:117 Resp: 516
Ion Ratio Lower Upper
117 100
201 0.0 40.6 122.0#

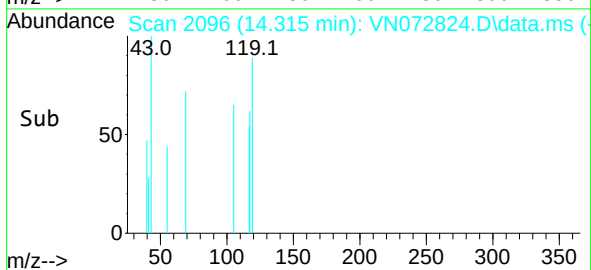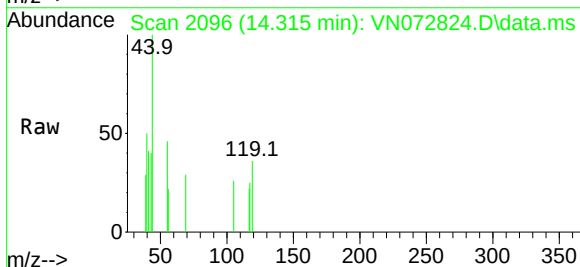

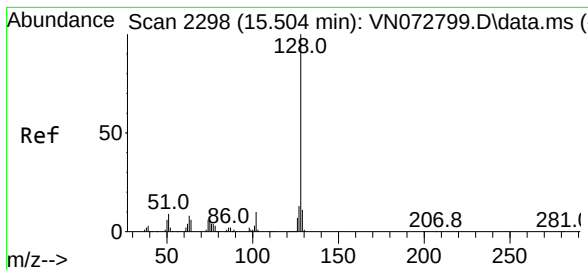

#95
Naphthalene
Concen: 0.560 ug/l
RT: 15.504 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN072824.D
Acq: 14 Jun 2022 03:25

Instrument :
MSVOA_N
ClientSampleId :
WC-14A-1A-6-G

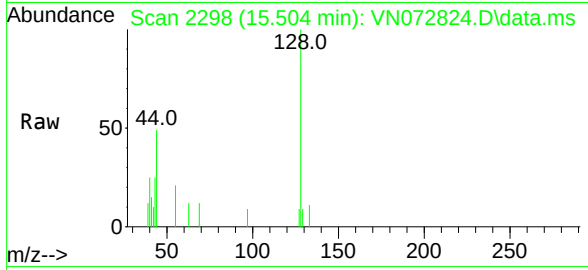

Tgt Ion:	128	Resp:	3374
Ion	Ratio	Lower	Upper
128	100		
127	5.5	10.3	15.5#
129	6.9	8.6	13.0#

