

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061323\
 Data File : VN078185.D
 Acq On : 13 Jun 2023 14:48
 Operator : JC\MD
 Sample : 03172-01 20X
 Misc : 5.04g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BUR-1578DL

Quant Time: Jun 14 02:19:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 07 05:05:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.236	168	379548	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	695262	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	618345	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	195339	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	256789	50.743	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 101.480%			
35) Dibromofluoromethane	8.177	113	228485	51.975	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 103.960%			
50) Toluene-d8	10.571	98	856941	50.565	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 101.140%			
62) 4-Bromofluorobenzene	12.853	95	250820	47.608	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 95.220%			
Target Compounds						
					Qvalue	
3) Chloromethane	2.371	50	1475	Below Cal	#	82
5) Bromomethane	2.948	94	1052	0.248	ug/l #	20
11) Tert butyl alcohol	5.512	59	4583	6.559	ug/l #	72
16) Acetone	4.436	43	675523	463.764	ug/l	97
20) Methylene Chloride	5.277	84	1689	0.351	ug/l	89
25) 2-Butanone	7.524	43	602	0.269	ug/l #	37
31) Cyclohexane	8.224	56	11228	1.730	ug/l #	42
36) 1,1-Dichloropropene	8.224	75	32754	5.194	ug/l #	49
38) Carbon Tetrachloride	8.230	117	41977	6.305	ug/l #	16
39) Methylcyclohexane	9.600	83	2853	0.437	ug/l #	81
43) Isopropyl Acetate	8.718	43	2879	0.306	ug/l #	49
48) Methyl methacrylate	9.688	41	4110	1.040	ug/l #	78
51) 4-Methyl-2-Pentanone	10.453	43	12498	2.519	ug/l	93
52) Toluene	10.635	92	350878	29.521	ug/l	97
67) Ethyl Benzene	11.965	91	7520	0.329	ug/l #	86
68) m/p-Xylenes	12.071	106	9106	1.046	ug/l	92
69) o-Xylene	12.406	106	5327	0.623	ug/l	81
74) N-amyl acetate	12.488	43	2045	0.336	ug/l #	47
75) 1,1,2,2-Tetrachloroethane	12.947	83	282	Below Cal	#	26
76) 1,2,3-Trichloropropane	12.853	75	134709	29.171	ug/l #	1
78) n-propylbenzene	13.035	91	10873	0.542	ug/l	99
80) 1,3,5-Trimethylbenzene	13.182	105	15883	1.062	ug/l	94
81) trans-1,4-Dichloro-2-b...	12.853	75	134709	89.623	ug/l #	15
83) tert-Butylbenzene	13.482	119	9318	0.717	ug/l #	71
84) 1,2,4-Trimethylbenzene	13.488	105	63478	4.378	ug/l	100
85) sec-Butylbenzene	13.618	105	7078	0.416	ug/l	99
86) p-Isopropyltoluene	13.735	119	12540	0.908	ug/l	94
89) n-Butylbenzene	14.059	91	10865	0.998	ug/l #	80
90) Hexachloroethane	14.329	117	4050	1.653	ug/l #	21
95) Naphthalene	15.647	128	13040	1.535	ug/l #	95
96) 1,2,3-Trichlorobenzene	15.847	180	688	0.244	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061323\
Data File : VN078185.D
Acq On : 13 Jun 2023 14:48
Operator : JC\MD
Sample : 03172-01 20X
Misc : 5.04g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BUR-1578DL

Quant Time: Jun 14 02:19:49 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 07 05:05:00 2023
Response via : Initial Calibration




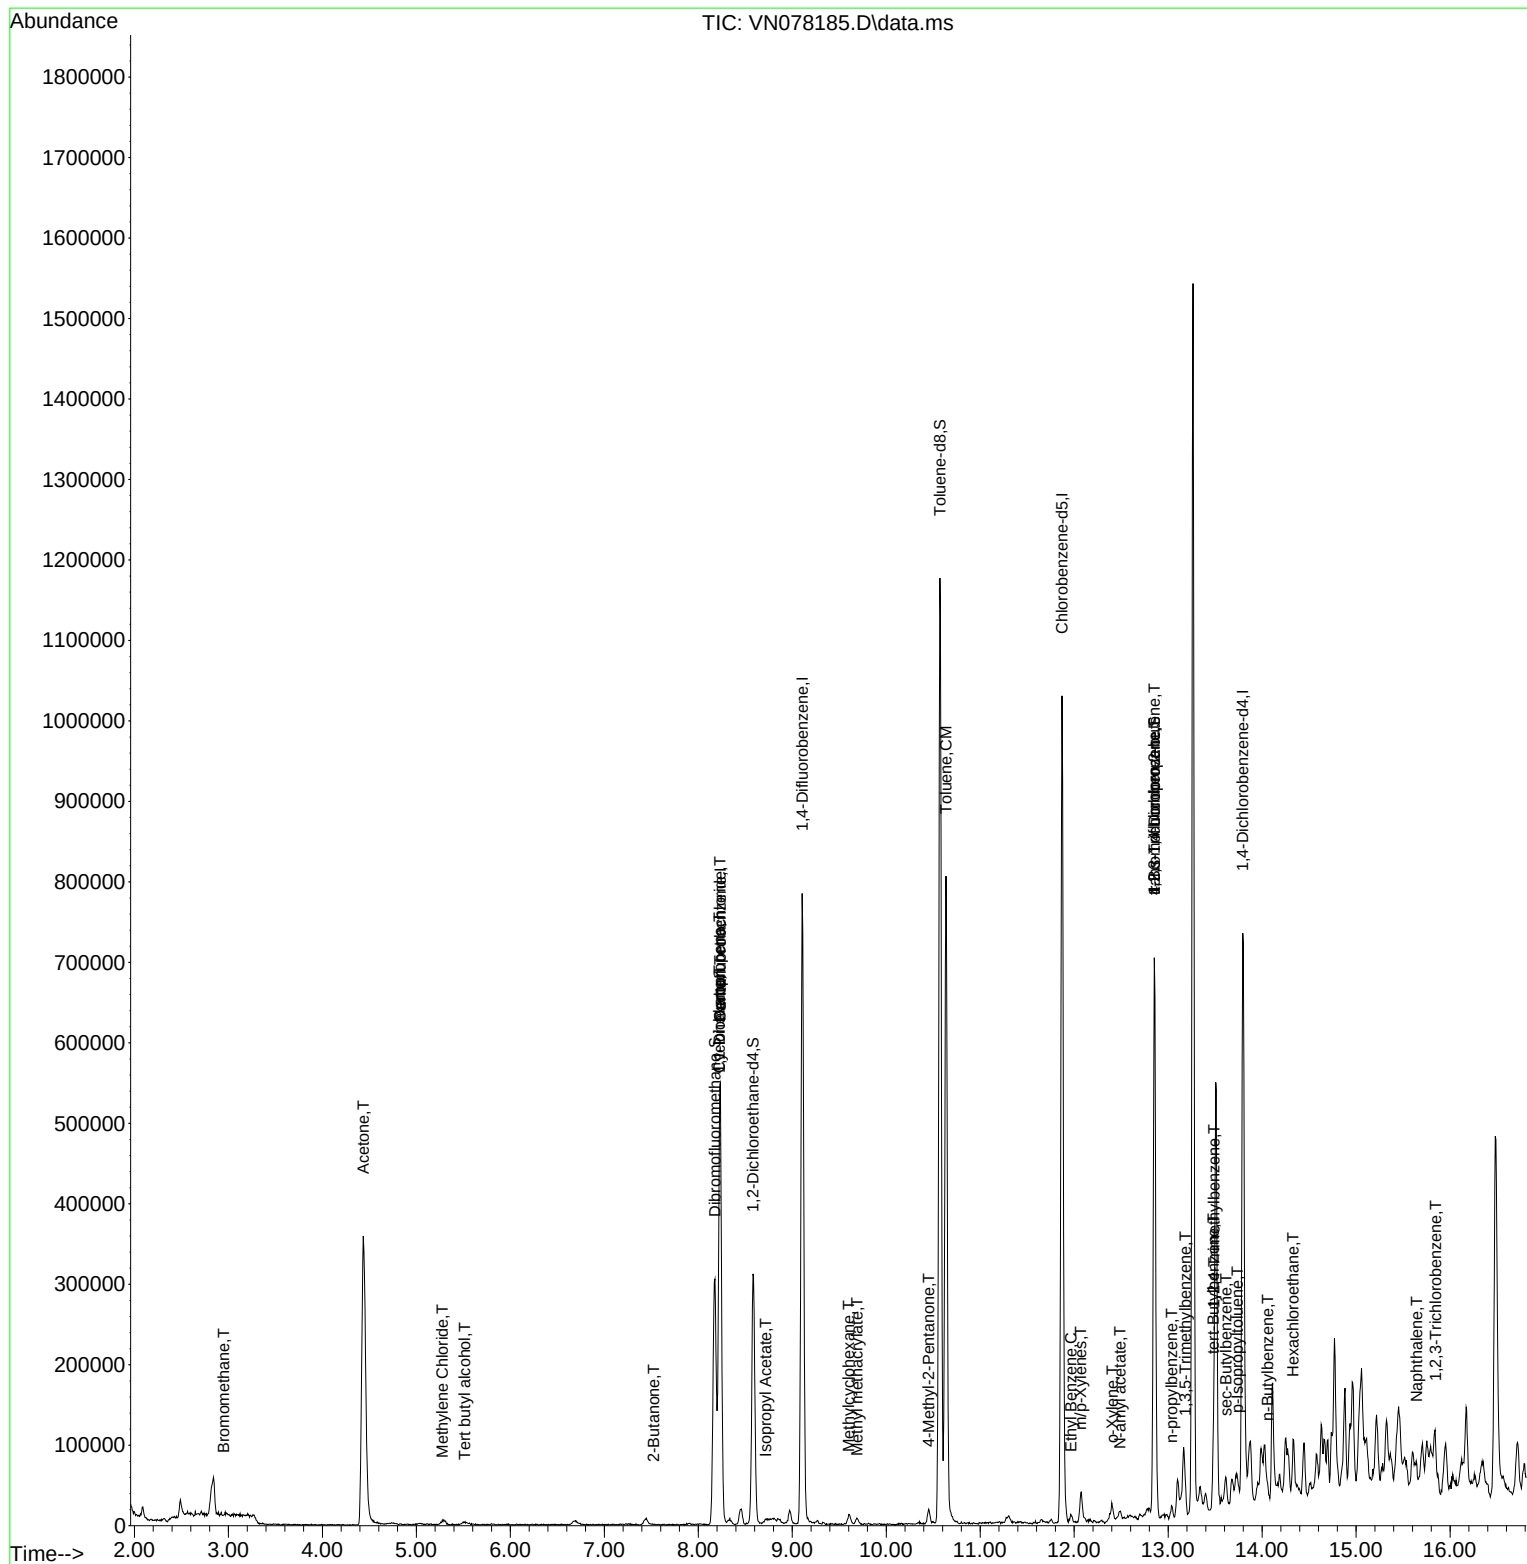




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.236 min Scan# 1068
Delta R.T. 0.001 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48




Instrument :
MSVOA_N
ClientSampleId :
BUR-1578DL


Tgt Ion:168 Resp: 379548
Ion Ratio Lower Upper
168 100
99 62.4 53.0 79.6

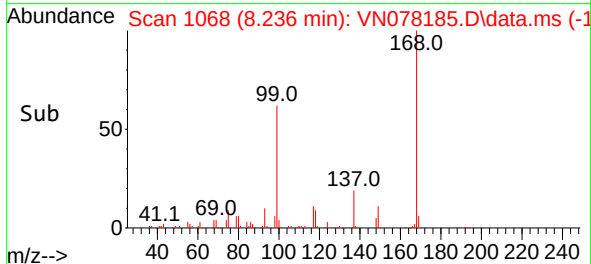

#3
Chloromethane
Concen: Below Cal
RT: 2.371 min Scan# 71
Delta R.T. 0.000 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48

Tgt Ion: 50 Resp: 1475
Ion Ratio Lower Upper
50 100
52 23.1 26.5 39.7#


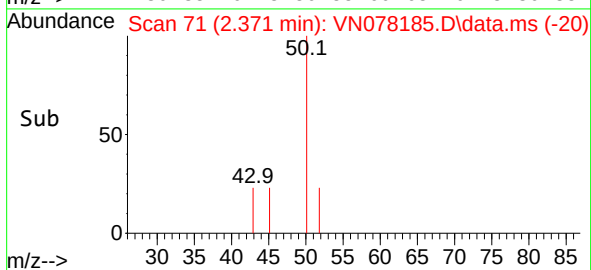

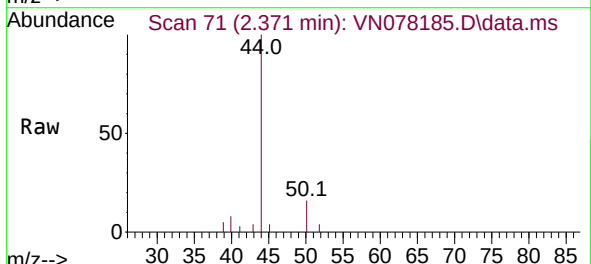




#5
Bromomethane
Concen: 0.248 ug/l
RT: 2.948 min Scan# 1
Delta R.T. -0.006 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48




Instrument :
MSVOA_N
ClientSampleId :
BUR-1578DL


Tgt Ion: 94 Resp: 1052
Ion Ratio Lower Upper
94 100
96 15.8 73.1 109.7#

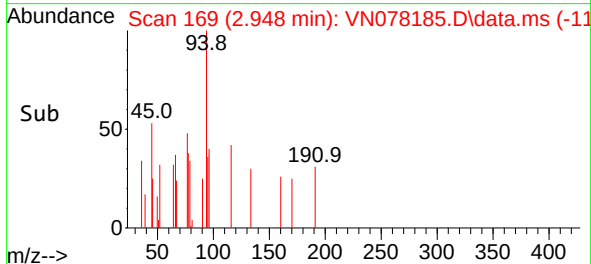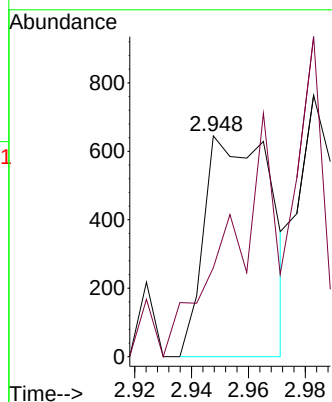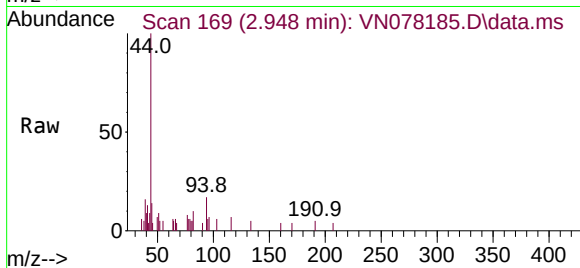

#11
Tert butyl alcohol
Concen: 6.559 ug/l
RT: 5.512 min Scan# 605
Delta R.T. -0.023 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48

Tgt Ion: 59 Resp: 4583
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#


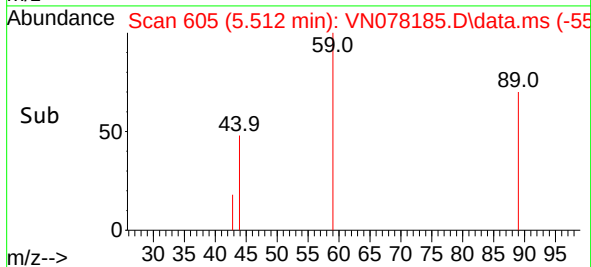
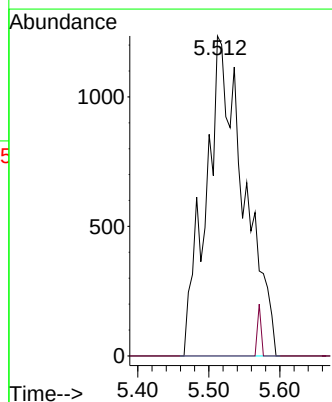
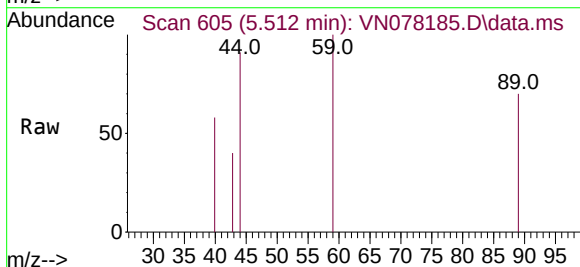




#16
Acetone
Concen: 463.764 ug/l
RT: 4.436 min Scan# 41
Delta R.T. 0.000 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48




Instrument :
MSVOA_N
ClientSampleId :
BUR-1578DL


Tgt Ion: 43 Resp: 675523
Ion Ratio Lower Upper
43 100
58 33.4 28.0 42.0

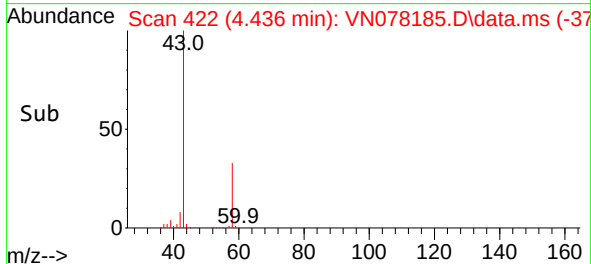

#20
Methylene Chloride
Concen: 0.351 ug/l
RT: 5.277 min Scan# 565
Delta R.T. -0.006 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48

Tgt Ion: 84 Resp: 1689
Ion Ratio Lower Upper
84 100
49 83.4 79.7 119.5
51 27.0 25.2 37.8
86 70.1 53.3 79.9


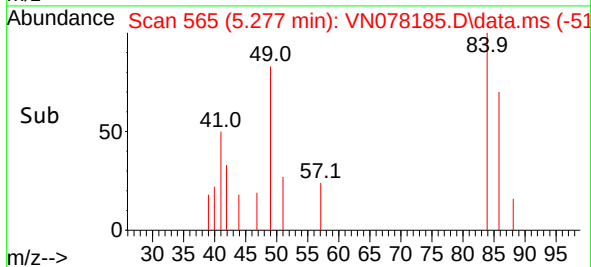

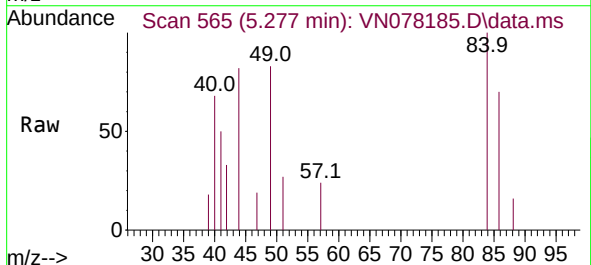




#25
2-Butanone
Concen: 0.269 ug/l
RT: 7.524 min Scan# 94
Delta R.T. 0.030 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48




Instrument :
MSVOA_N
ClientSampleId :
BUR-1578DL


Tgt Ion: 43 Resp: 602
Ion Ratio Lower Upper
43 100
72 0.0 30.2 45.2#

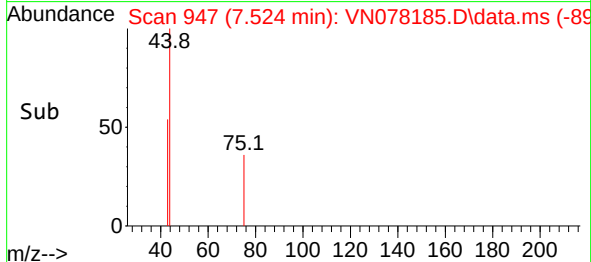

#31
Cyclohexane
Concen: 1.730 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.041 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48

Tgt Ion: 56 Resp: 11228
Ion Ratio Lower Upper
56 100
69 100.6 26.8 40.2#
84 141.5 81.8 122.6#

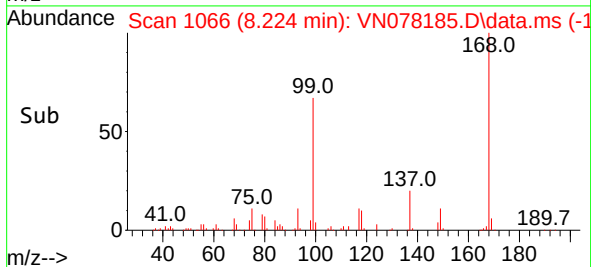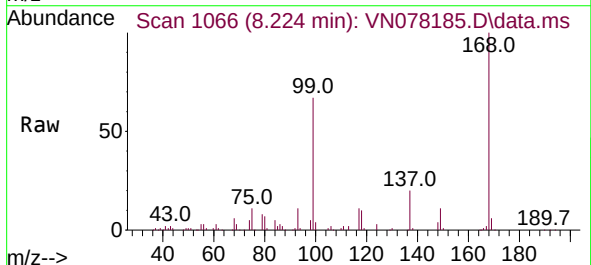

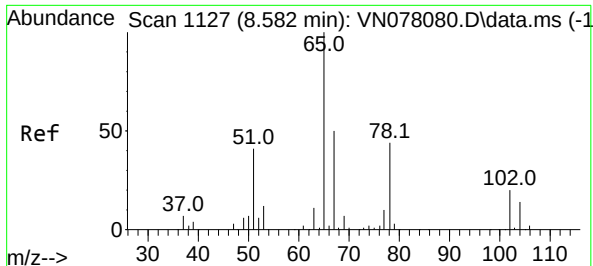

#33

1,2-Dichloroethane-d4

Concen: 50.743 ug/l

RT: 8.583 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VN078185.D

Acq: 13 Jun 2023 14:48

Instrument :

MSVOA_N

ClientSampleId :





BUR-1578DL

Tgt Ion: 65 Resp: 256789

Ion Ratio Lower Upper

65 100

67 52.3 0.0 106.6

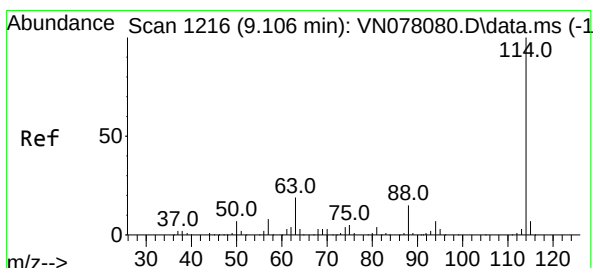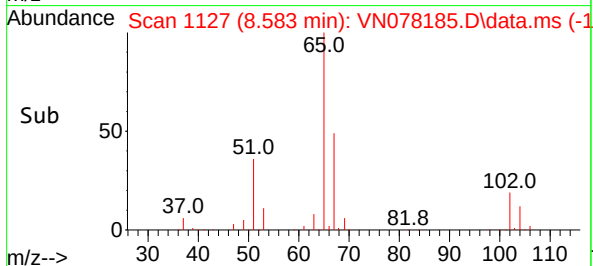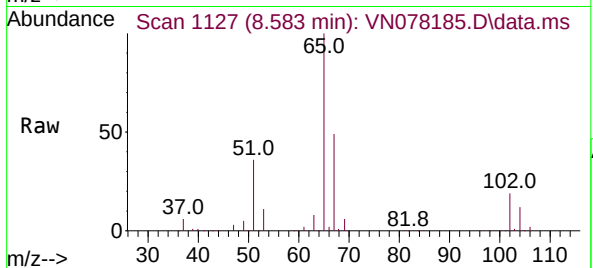

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. 0.000 min

Lab File: VN078185.D

Acq: 13 Jun 2023 14:48




Tgt Ion: 114 Resp: 695262


Ion Ratio Lower Upper

114 100

63 19.3 0.0 36.4

88 15.4 0.0 30.6

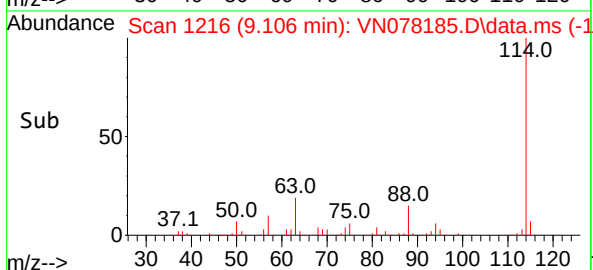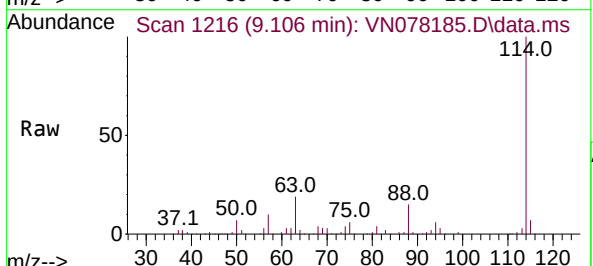

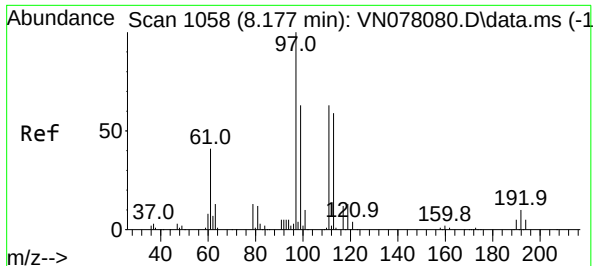

#35

Dibromofluoromethane

Concen: 51.975 ug/l

RT: 8.177 min Scan# 1058

Delta R.T. 0.000 min

Lab File: VN078185.D

Acq: 13 Jun 2023 14:48

Instrument :

MSVOA_N

ClientSampleId :

BUR-1578DL





Tgt Ion:113 Resp: 228485

Ion Ratio Lower Upper

113 100

111 103.3 82.6 123.8

192 16.2 12.7 19.1

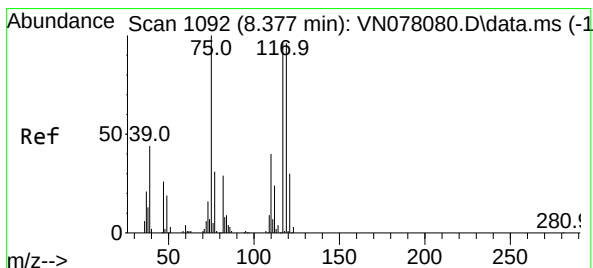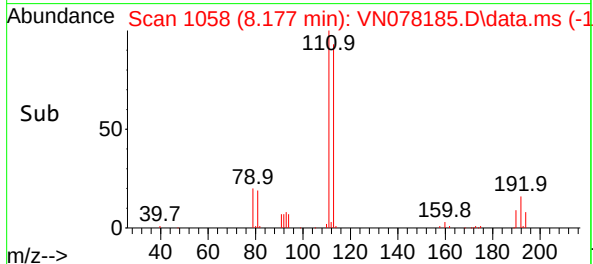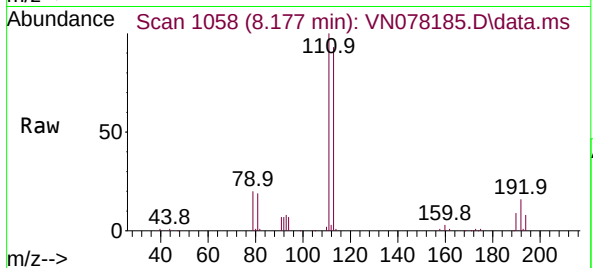

#36

1,1-Dichloropropene

Concen: 5.194 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.153 min

Lab File: VN078185.D

Acq: 13 Jun 2023 14:48




Tgt Ion: 75 Resp: 32754


Ion Ratio Lower Upper

75 100

110 10.5 19.1 57.3#

77 0.0 25.0 37.4#


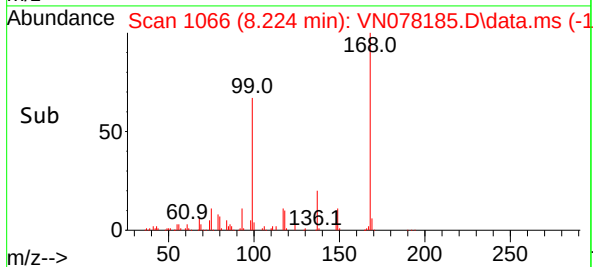

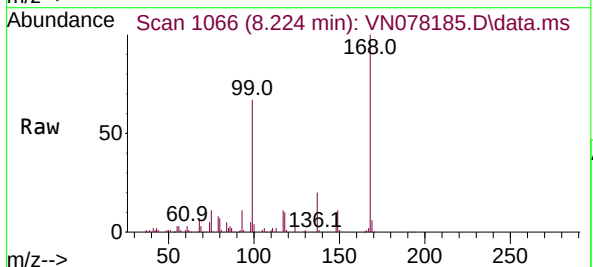


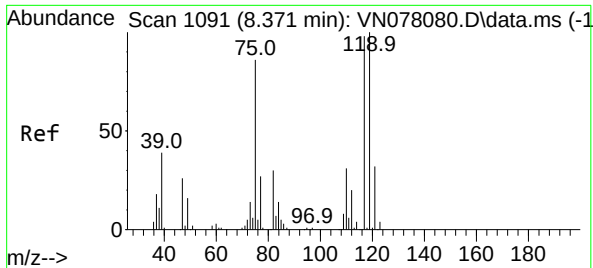

#38
Carbon Tetrachloride
Concen: 6.305 ug/l
RT: 8.230 min Scan# 1091
Delta R.T. -0.141 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48




Instrument :
MSVOA_N
ClientSampleId :
BUR-1578DL


Tgt Ion:117 Resp: 41977
Ion Ratio Lower Upper
117 100
119 5.7 77.3 115.9#
121 0.0 23.3 34.9#

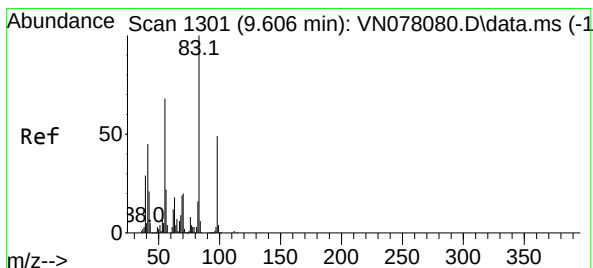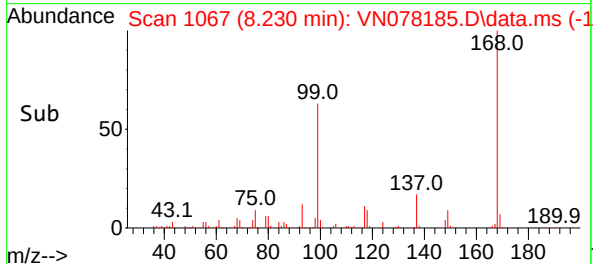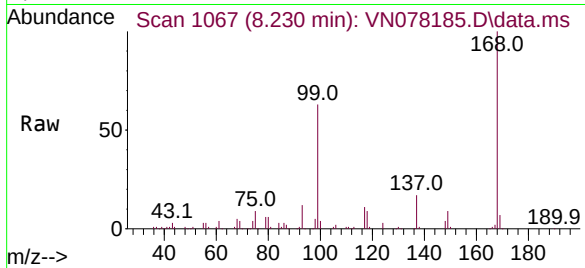

#39
Methylcyclohexane
Concen: 0.437 ug/l
RT: 9.600 min Scan# 1300
Delta R.T. -0.006 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48

Tgt Ion: 83 Resp: 2853
Ion Ratio Lower Upper
83 100
55 69.7 49.1 73.7
98 30.2 40.6 61.0#

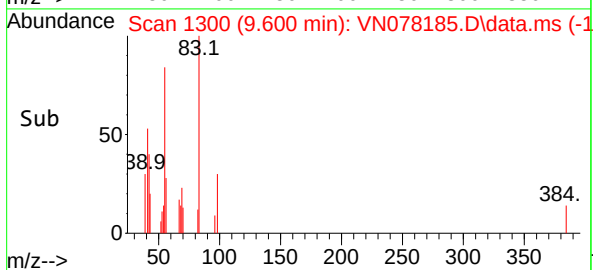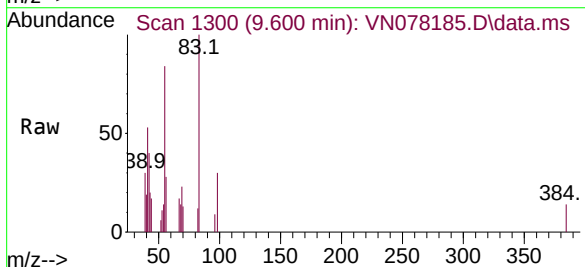

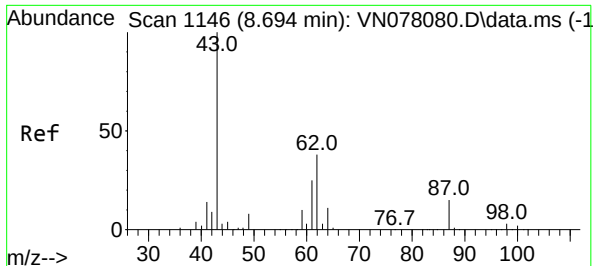

#43

Isopropyl Acetate

Concen: 0.306 ug/l

RT: 8.718 min Scan# 1150

Delta R.T. 0.024 min

Lab File: VN078185.D

Acq: 13 Jun 2023 14:48

Instrument :

MSVOA_N

ClientSampleId :

BUR-1578DL





Tgt Ion: 43 Resp: 2879

Ion Ratio Lower Upper

43 100

61 0.0 24.7 37.1#

87 0.0 14.6 21.8#

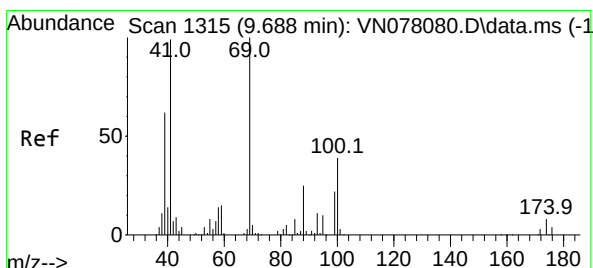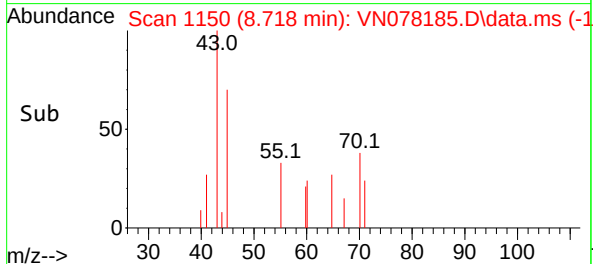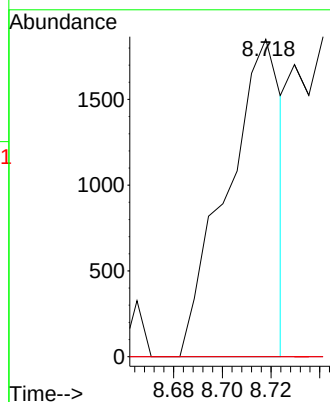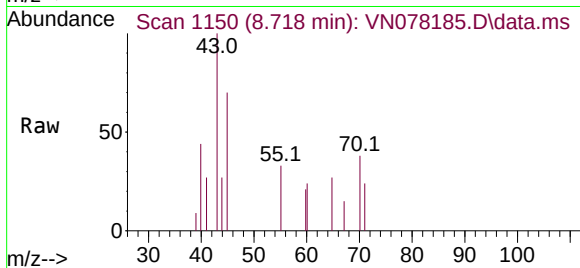

#48

Methyl methacrylate

Concen: 1.040 ug/l

RT: 9.688 min Scan# 1315

Delta R.T. 0.000 min

Lab File: VN078185.D

Acq: 13 Jun 2023 14:48




Tgt Ion: 41 Resp: 4110


Ion Ratio Lower Upper

41 100

69 80.4 90.4 135.6#

39 74.7 54.6 81.8


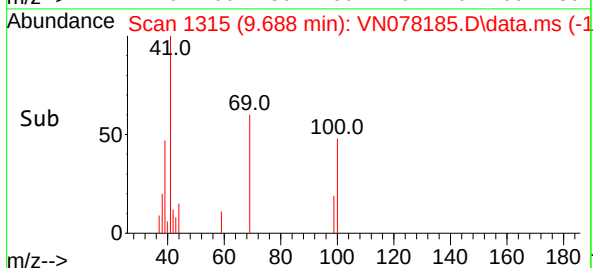

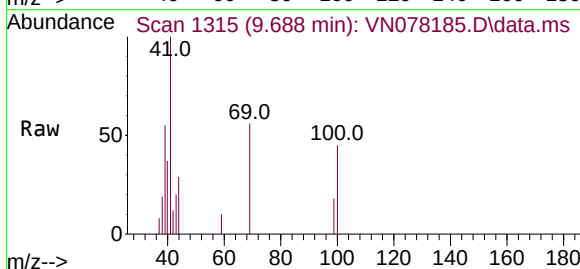




#50
Toluene-d8
Concen: 50.565 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48




Instrument :
MSVOA_N
ClientSampleId :
BUR-1578DL


Tgt Ion: 98 Resp: 856941
Ion Ratio Lower Upper
98 100
100 62.7 52.0 78.0

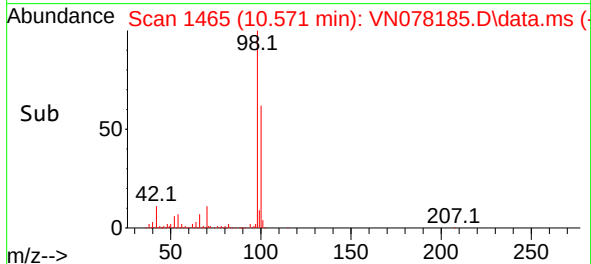

#51
4-Methyl-2-Pentanone
Concen: 2.519 ug/l
RT: 10.453 min Scan# 1445
Delta R.T. 0.000 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48

Tgt Ion: 43 Resp: 12498
Ion Ratio Lower Upper
43 100
58 41.2 36.6 54.8


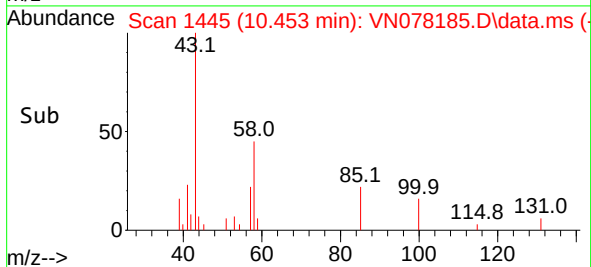

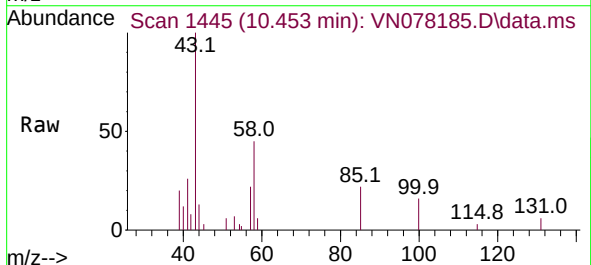


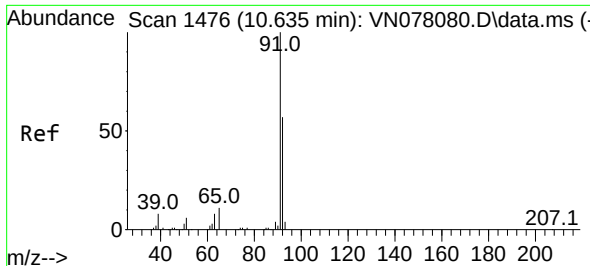

#52
Toluene
Concen: 29.521 ug/l
RT: 10.635 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48




Instrument :
MSVOA_N
ClientSampleId :
BUR-1578DL


Tgt Ion: 92 Resp: 350878
Ion Ratio Lower Upper
92 100
91 176.3 137.4 206.0

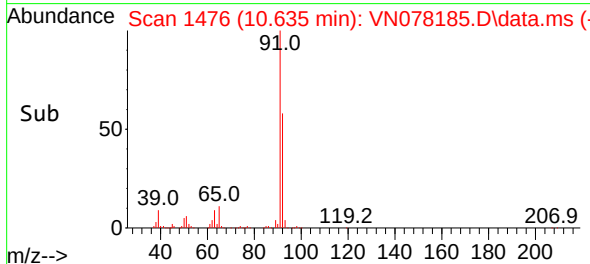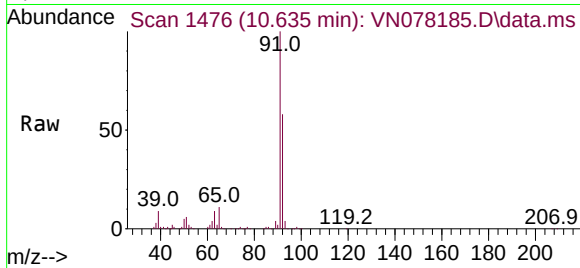

#62
4-Bromofluorobenzene
Concen: 47.608 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48

Tgt Ion: 95 Resp: 250820
Ion Ratio Lower Upper
95 100
174 73.9 0.0 143.8
176 69.9 0.0 135.8



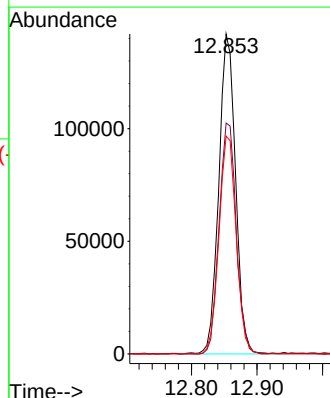
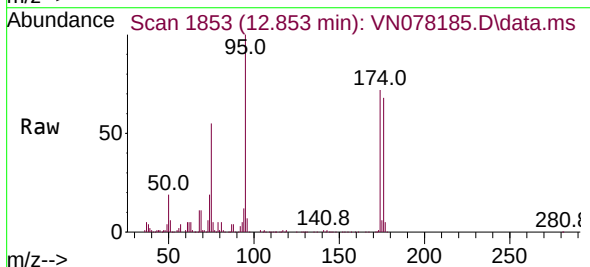


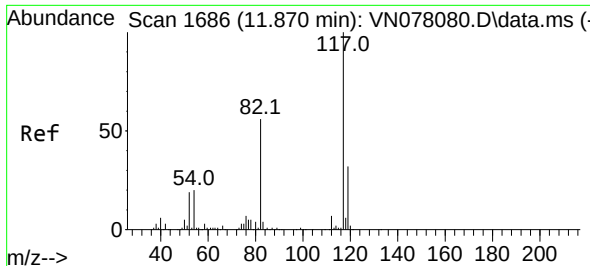

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1170
Delta R.T. 0.000 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48




Instrument :
MSVOA_N
ClientSampleId :
BUR-1578DL


Tgt Ion:117 Resp: 618345
Ion Ratio Lower Upper
117 100
82 53.2 44.0 66.0
119 31.0 25.6 38.4

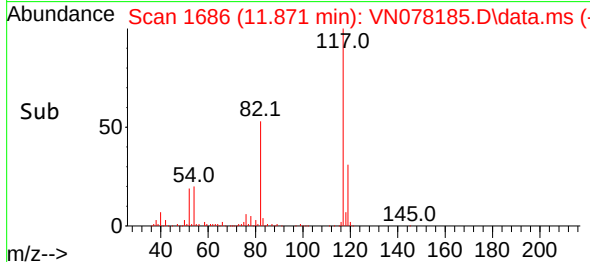

#67
Ethyl Benzene
Concen: 0.329 ug/l
RT: 11.965 min Scan# 1702
Delta R.T. -0.006 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48

Tgt Ion: 91 Resp: 7520
Ion Ratio Lower Upper
91 100
106 24.1 25.6 38.4#


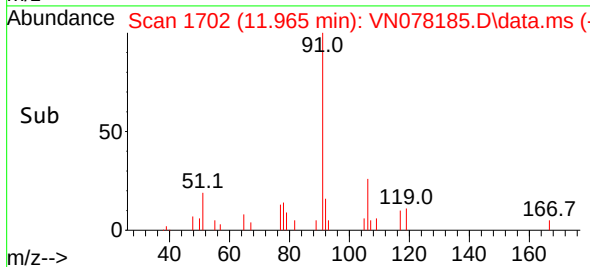

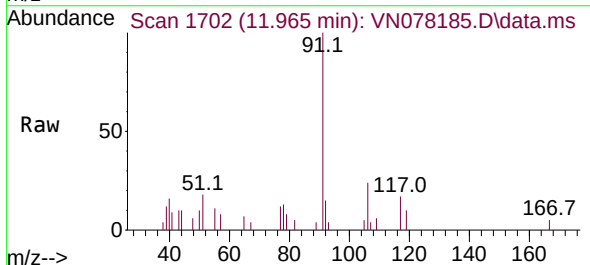




#68
m/p-Xylenes
Concen: 1.046 ug/l
RT: 12.071 min Scan# 1721
Delta R.T. -0.006 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48




Instrument :
MSVOA_N
ClientSampleId :
BUR-1578DL


Tgt Ion:106 Resp: 9106
Ion Ratio Lower Upper
106 100
91 211.5 159.6 239.4

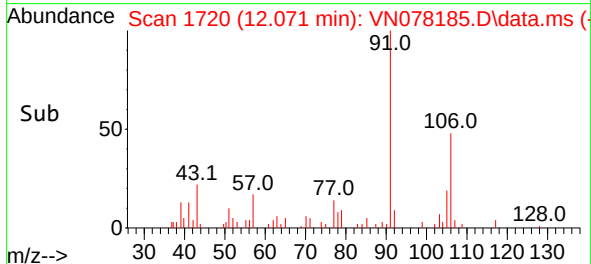

#69
o-Xylene
Concen: 0.623 ug/l
RT: 12.406 min Scan# 1777
Delta R.T. 0.000 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48

Tgt Ion:106 Resp: 5327
Ion Ratio Lower Upper
106 100
91 239.5 105.2 315.5


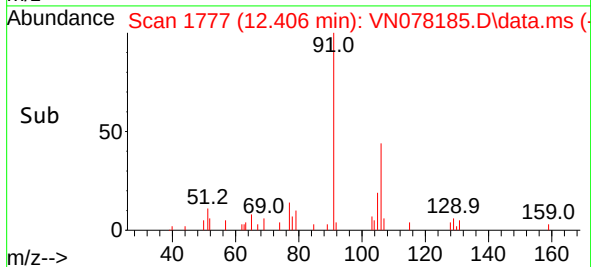

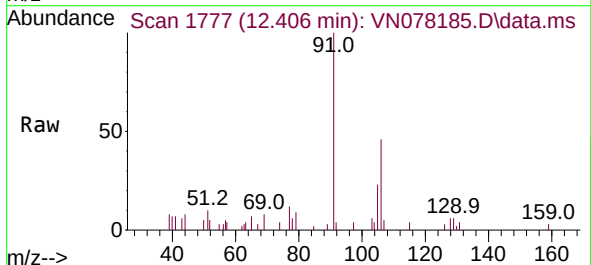


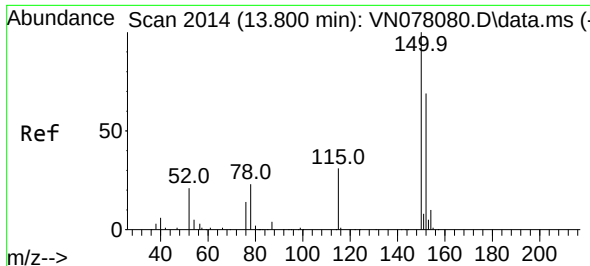

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2014
Delta R.T. -0.006 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48




Instrument :
MSVOA_N
ClientSampleId :
BUR-1578DL


Tgt Ion:152 Resp: 195339
Ion Ratio Lower Upper
152 100
115 60.8 32.3 96.8
150 154.4 0.0 355.8

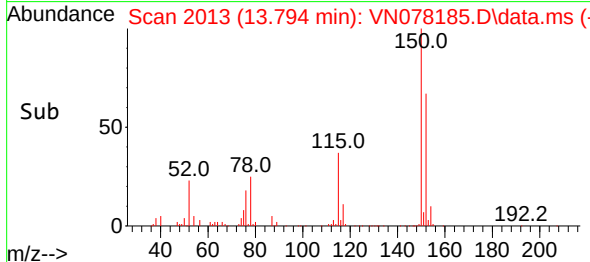

#74
N-ethyl acetate
Concen: 0.336 ug/l
RT: 12.488 min Scan# 1791
Delta R.T. -0.012 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48

Tgt Ion: 43 Resp: 2045
Ion Ratio Lower Upper
43 100
70 18.8 43.4 65.2#
55 58.1 21.4 32.0#
61 0.0 22.8 34.2#


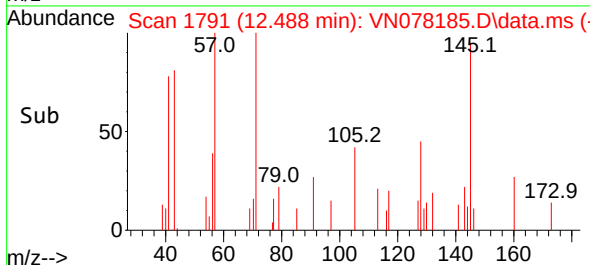
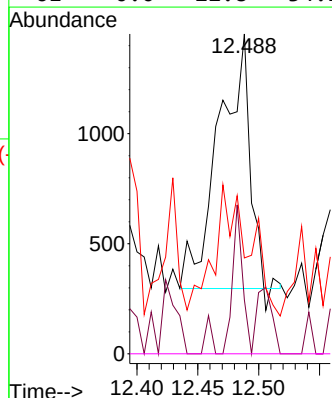
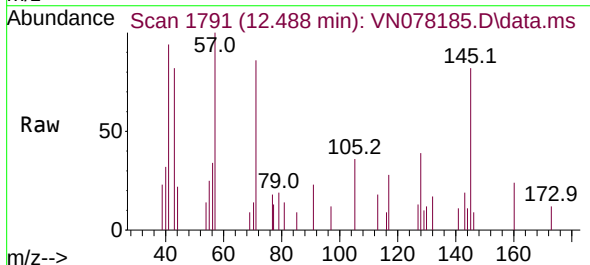




#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.947 min Scan# 1869
Delta R.T. 0.006 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48




Instrument :
MSVOA_N
ClientSampleId :
BUR-1578DL


Tgt Ion: 83 Resp: 282
Ion Ratio Lower Upper
83 100
131 0.0 5.0 15.0#
85 0.0 31.9 95.7#

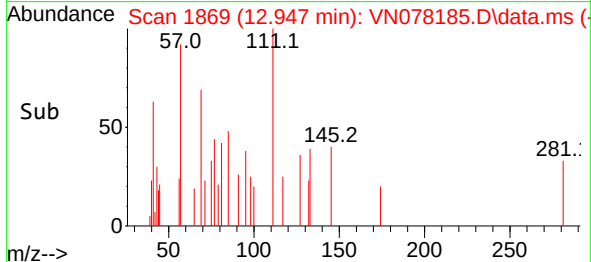

#76
1,2,3-Trichloropropane
Concen: 29.171 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.147 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48

Tgt Ion: 75 Resp: 134709
Ion Ratio Lower Upper
75 100
77 1.7 84.5 253.5#


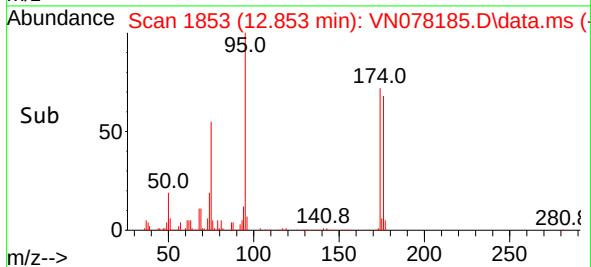

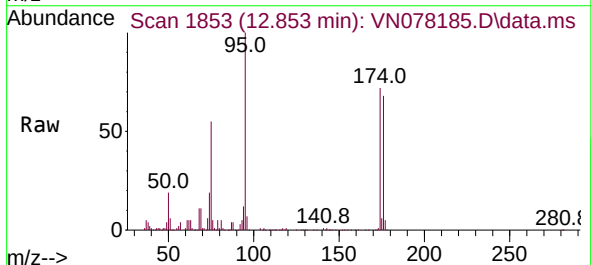


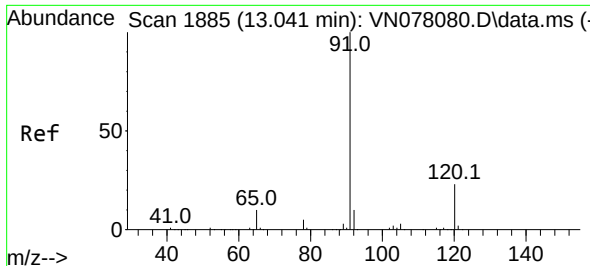

#78
n-propylbenzene
Concen: 0.542 ug/l
RT: 13.035 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48




Instrument :
MSVOA_N
ClientSampleId :
BUR-1578DL


Tgt Ion: 91 Resp: 10873
Ion Ratio Lower Upper
91 100
120 23.4 11.5 34.4

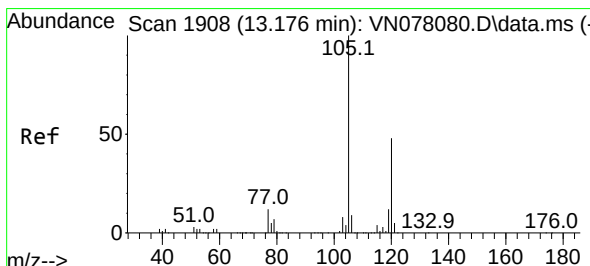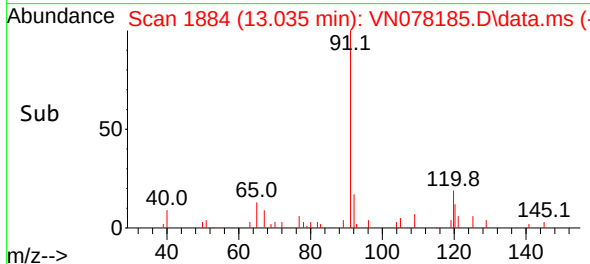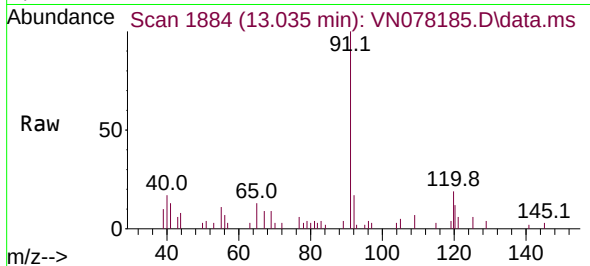

#80
1,3,5-Trimethylbenzene
Concen: 1.062 ug/l
RT: 13.182 min Scan# 1909
Delta R.T. 0.006 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48

Tgt Ion: 105 Resp: 15883
Ion Ratio Lower Upper
105 100
120 51.9 24.1 72.3


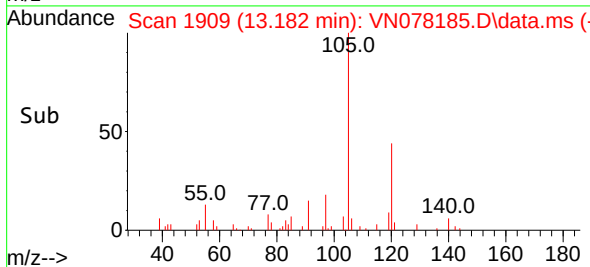

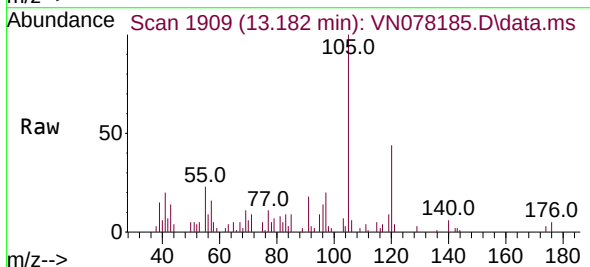


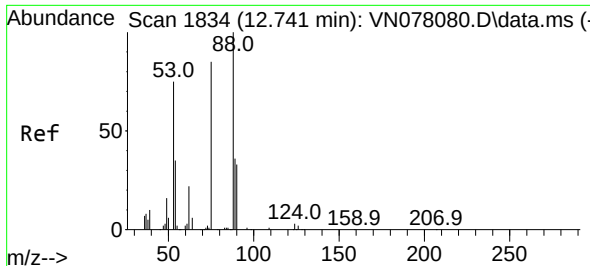

#81
 trans-1,4-Dichloro-2-butene
 Concen: 89.623 ug/l
 RT: 12.853 min Scan# 11
 Delta R.T. 0.112 min
 Lab File: VN078185.D
 Acq: 13 Jun 2023 14:48




Instrument :
 MSVOA_N
 ClientSampleId :
 BUR-1578DL


Tgt Ion: 75 Resp: 134709
 Ion Ratio Lower Upper
 75 100
 53 0.3 67.4 101.2#
 89 0.0 38.8 58.2#

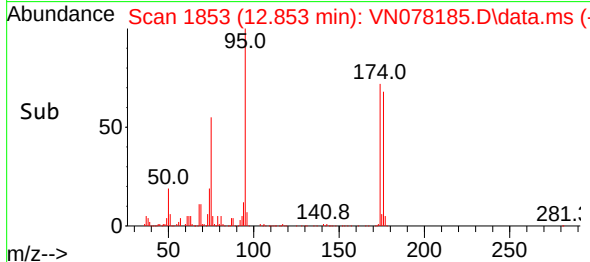

#83
 tert-Butylbenzene
 Concen: 0.717 ug/l
 RT: 13.482 min Scan# 1960
 Delta R.T. 0.041 min
 Lab File: VN078185.D
 Acq: 13 Jun 2023 14:48

Tgt Ion: 119 Resp: 9318
 Ion Ratio Lower Upper
 119 100
 91 83.8 33.9 101.7
 134 0.0 13.2 39.6#

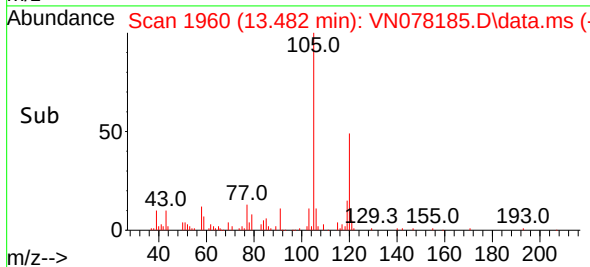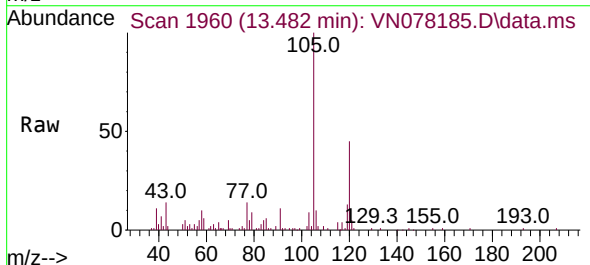



#84

1,2,4-Trimethylbenzene

Concen: 4.378 ug/l

RT: 13.488 min Scan# 1961

Delta R.T. 0.000 min

Lab File: VN078185.D

Acq: 13 Jun 2023 14:48

Instrument :

MSVOA_N

ClientSampleId :





BUR-1578DL

Tgt Ion:105 Resp: 63478

Ion Ratio Lower Upper

105 100

120 43.9 22.0 66.0

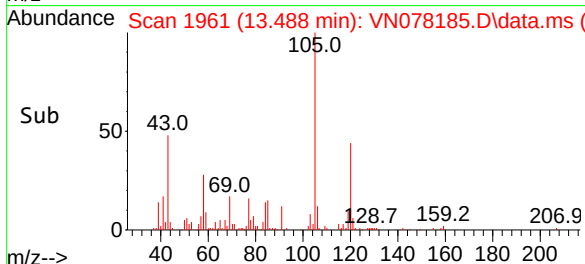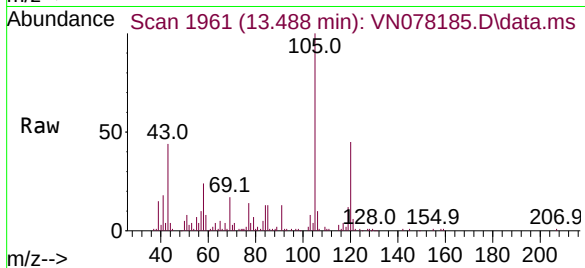

#85

sec-Butylbenzene

Concen: 0.416 ug/l

RT: 13.618 min Scan# 1983

Delta R.T. -0.006 min

Lab File: VN078185.D




Acq: 13 Jun 2023 14:48


Tgt Ion:105 Resp: 7078

Ion Ratio Lower Upper

105 100

134 20.0 9.8 29.3


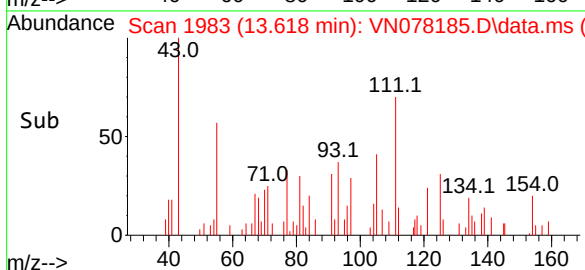

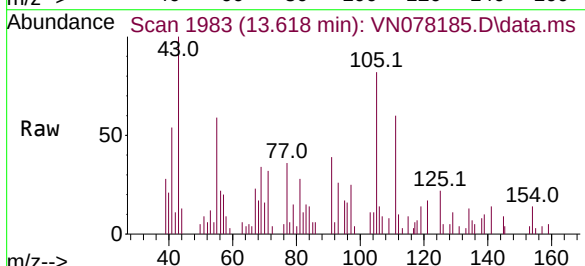


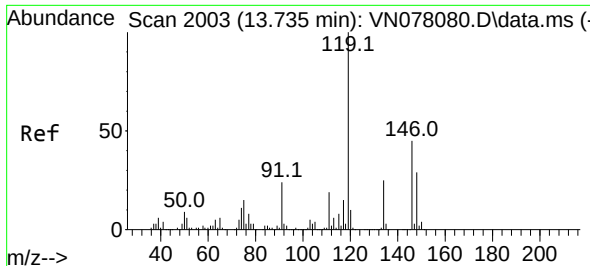

#86
p-Isopropyltoluene
Concen: 0.908 ug/l
RT: 13.735 min Scan# 2003
Delta R.T. 0.000 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48




Instrument :
MSVOA_N
ClientSampleId :
BUR-1578DL


Tgt Ion:	119	Resp:	12540
Ion	Ratio	Lower	Upper
119	100		
134	26.2	12.6	37.8
91	29.9	12.4	37.2

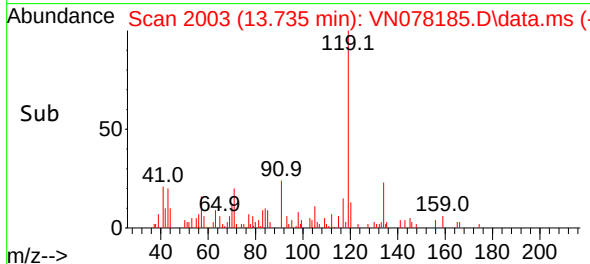

#89
n-Butylbenzene
Concen: 0.998 ug/l
RT: 14.059 min Scan# 2058
Delta R.T. -0.006 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48

Tgt Ion:	91	Resp:	10865
Ion	Ratio	Lower	Upper
91	100		
92	56.5	26.4	79.0
134	0.0	12.6	37.6#


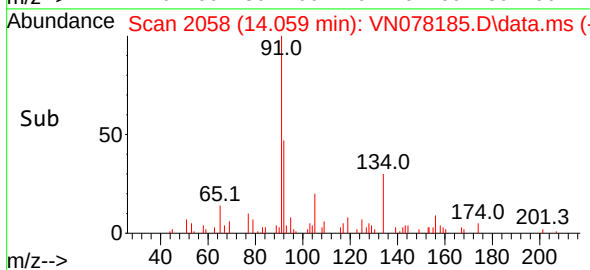

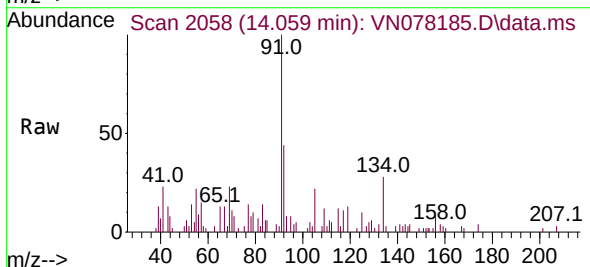


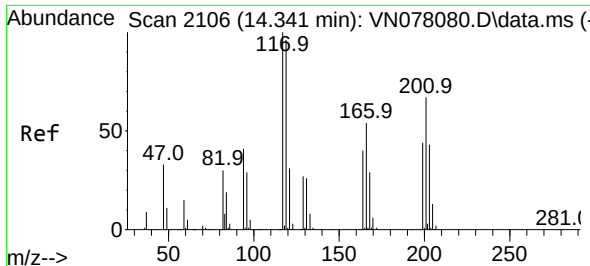

#90
Hexachloroethane
Concen: 1.653 ug/l
RT: 14.329 min Scan# 2104
Delta R.T. -0.012 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48




Instrument :
MSVOA_N
ClientSampleId :
BUR-1578DL


Tgt Ion:117 Resp: 4050
Ion Ratio Lower Upper
117 100
201 0.0 29.3 88.0#

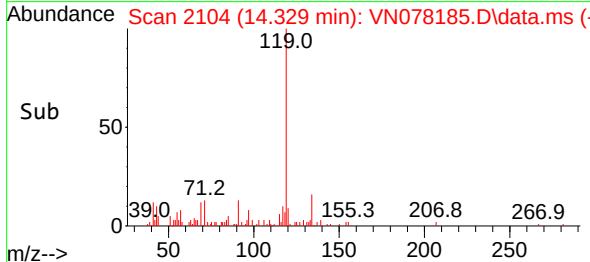

#95
Naphthalene
Concen: 1.535 ug/l
RT: 15.647 min Scan# 2328
Delta R.T. 0.000 min
Lab File: VN078185.D
Acq: 13 Jun 2023 14:48

Tgt Ion:128 Resp: 13040
Ion Ratio Lower Upper
128 100
127 13.8 10.0 15.0
129 13.7 8.7 13.1#

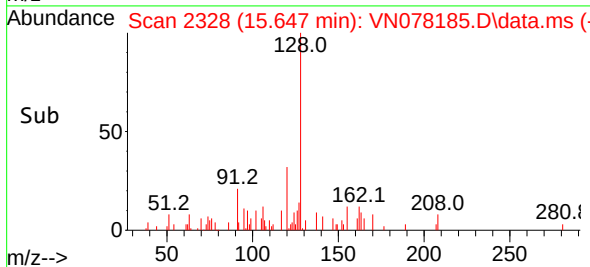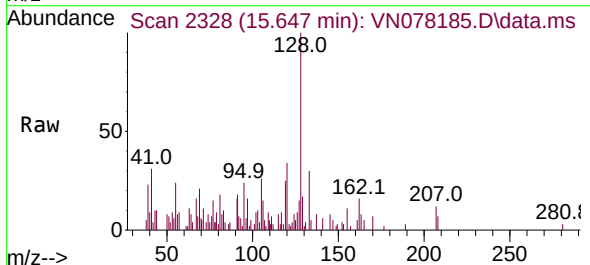

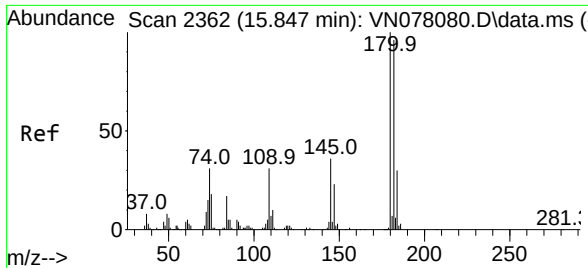

#96
 1,2,3-Trichlorobenzene
 Concen: 0.244 ug/l
 RT: 15.847 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VN078185.D
 Acq: 13 Jun 2023 14:48

Instrument :
 MSVOA_N
 ClientSampleId :
 BUR-1578DL

Tgt Ion:	180	Resp:	688
Ion	Ratio	Lower	Upper
180	100		
182	32.3	46.2	138.6#
145	827.5	17.5	52.6#

