
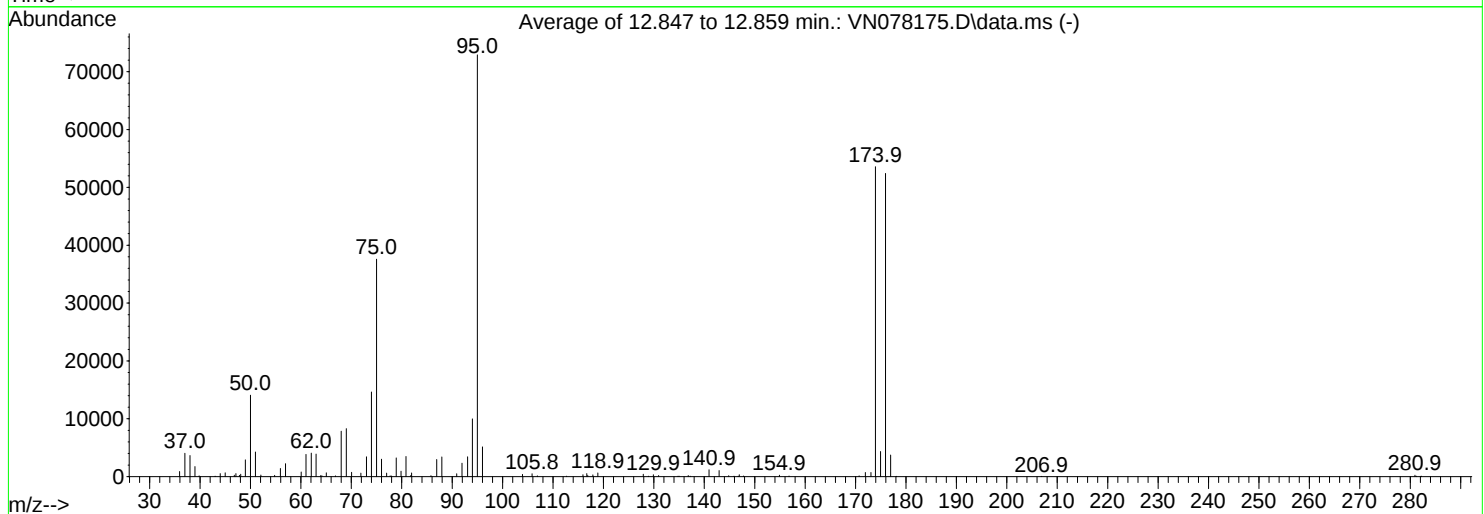


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN061323\  
Data File : VN078175.D  
Acq On : 13 Jun 2023 09:17  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N060623W.M  
Title : SW846 8260  
Last Update : Wed Jun 07 05:05:00 2023

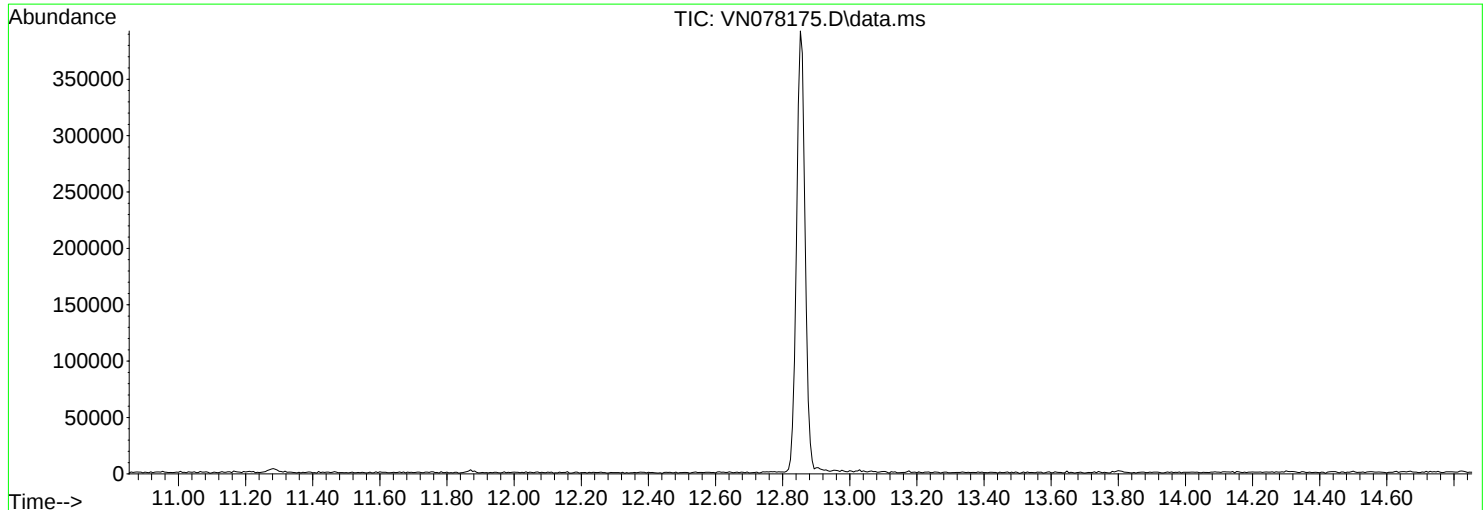

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 19.3  | 14095 | PASS      |
| 75     | 95      | 30     | 60     | 51.6  | 37592 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 72912 | PASS      |
| 96     | 95      | 5      | 9      | 7.1   | 5159  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.4   | 735   | PASS      |
| 174    | 95      | 50     | 100    | 73.5  | 53573 | PASS      |
| 175    | 174     | 5      | 9      | 8.1   | 4357  | PASS      |
| 176    | 174     | 95     | 101    | 97.8  | 52403 | PASS      |
| 177    | 176     | 5      | 9      | 7.1   | 3732  | PASS      |

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z   | abund. |
|-------|--------|-------|--------|-------|--------|-------|--------|
| 35.95 | 896    | 48.05 | 404    | 63.00 | 3909   | 75.00 | 3759   |
| 37.00 | 4036   | 49.00 | 2914   | 63.90 | 167    | 76.00 | 302    |
| 38.00 | 3662   | 50.00 | 14095  | 64.15 | 165    | 77.00 | 59     |
| 39.00 | 1738   | 51.00 | 4248   | 65.05 | 665    | 77.70 | 14     |
| 39.80 | 131    | 52.05 | 265    | 66.85 | 142    | 78.00 | 125    |
| 43.00 | 93     | 54.80 | 225    | 68.00 | 7860   | 78.90 | 3242   |
| 44.00 | 538    | 55.95 | 1416   | 69.00 | 8295   | 79.85 | 928    |
| 45.00 | 657    | 56.95 | 2229   | 70.05 | 752    | 80.85 | 3491   |
| 46.80 | 260    | 60.05 | 807    | 71.90 | 602    | 81.80 | 188    |
| 47.10 | 531    | 61.00 | 3857   | 73.00 | 3444   | 81.95 | 629    |
| 47.80 | 229    | 62.05 | 4060   | 74.00 | 14645  | 85.80 | 166    |

Average of 12.847 to 12.859 min.: VN078175.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z    | abund. | m/z    | abund. | m/z    | abund. |
|--------|--------|--------|--------|--------|--------|--------|--------|
| 86.95  | 2969   | 112.70 | 85     | 135.00 | 97     | 156.80 | 119    |
| 87.95  | 3405   | 115.95 | 321    | 136.80 | 188    | 170.70 | 144    |
| 90.90  | 488    | 116.70 | 532    | 137.20 | 89     | 171.95 | 708    |
| 91.95  | 2331   | 116.90 | 209    | 140.95 | 1202   | 173.05 | 735    |
| 93.05  | 3442   | 117.90 | 309    | 142.95 | 1057   | 173.95 | 53573  |
| 94.00  | 9973   | 118.90 | 629    | 144.85 | 170    | 174.95 | 4357   |
| 95.00  | 72912  | 127.90 | 413    | 145.90 | 72     | 175.95 | 52403  |
| 96.00  | 5159   | 128.90 | 84     | 146.70 | 95     | 176.95 | 3732   |
| 103.95 | 400    | 129.90 | 339    | 146.95 | 324    | 178.10 | 58     |
| 105.85 | 497    | 130.95 | 191    | 147.80 | 114    | 206.90 | 53     |
| 106.90 | 128    | 134.80 | 74     | 154.90 | 249    | 280.95 | 240    |

Average of 12.847 to 12.859 min.: VN078175.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z | abund. | m/z | abund. | m/z | abund. |
|--------|--------|-----|--------|-----|--------|-----|--------|
| 281.20 | 74     |     |        |     |        |     |        |
| 282.00 | 50     |     |        |     |        |     |        |
| 282.20 | 83     |     |        |     |        |     |        |

Instrument :

MSVOA\_N

ClientSampleId :

BFB