
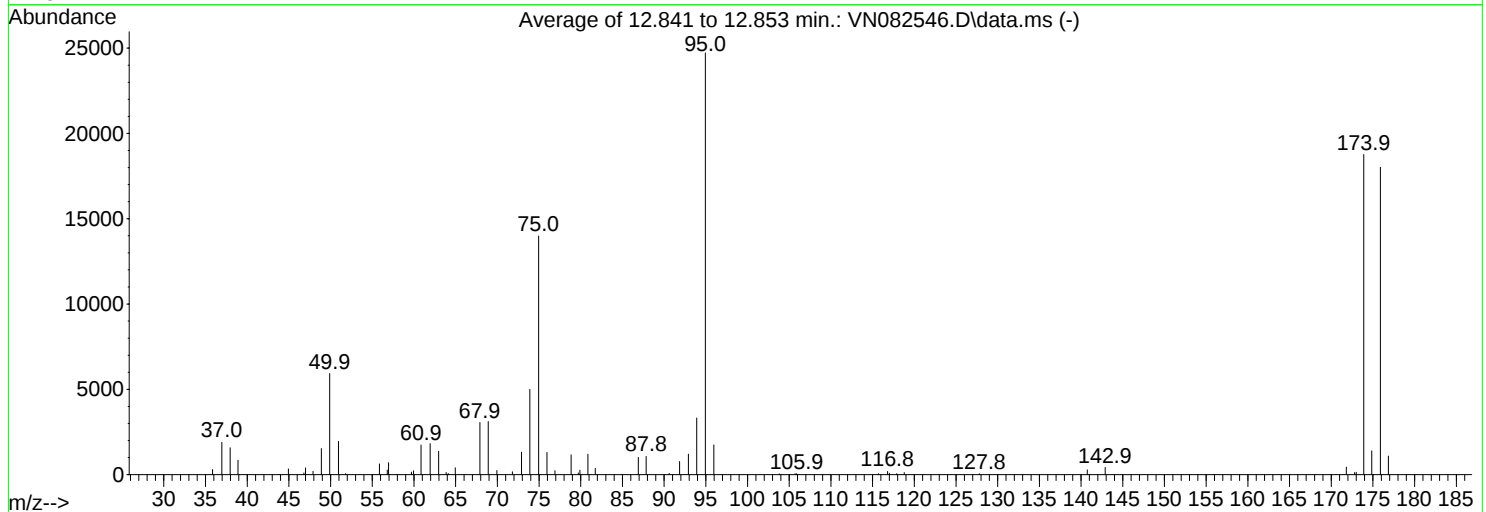


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061324\
Data File : VN082546.D
Acq On : 13 Jun 2024 08:34
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

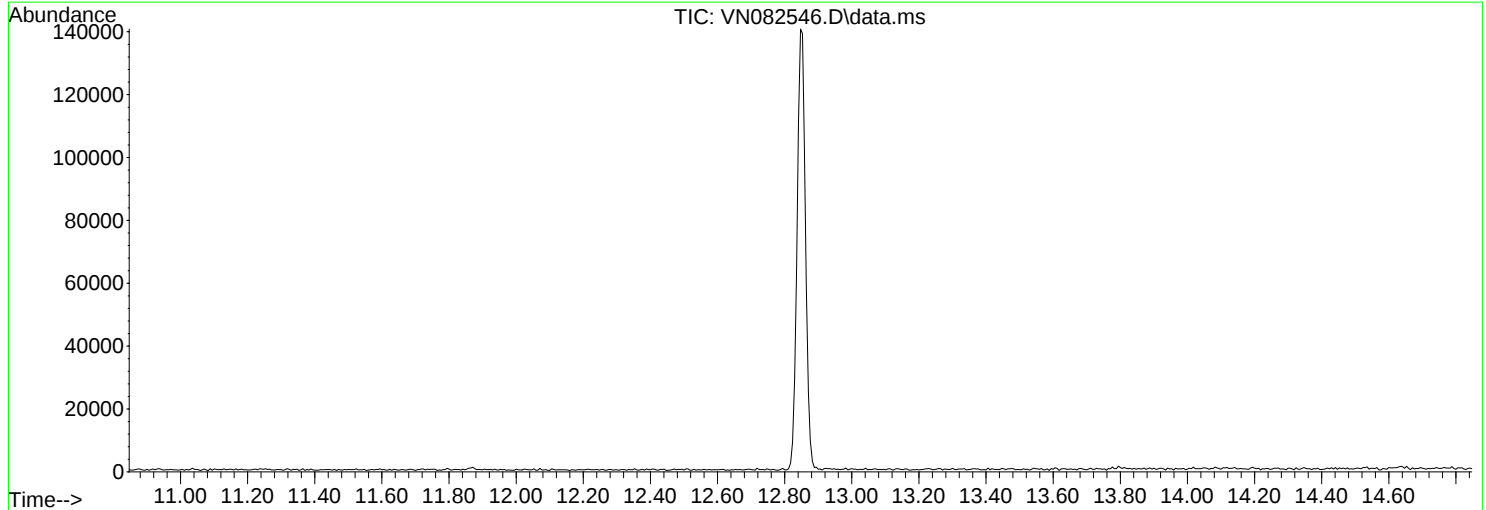

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.0	5930	PASS
75	95	30	60	56.6	13985	PASS
95	95	100	100	100.0	24723	PASS
96	95	5	9	7.1	1748	PASS
173	174	0.00	2	0.7	137	PASS
174	95	50	100	75.9	18762	PASS
175	174	5	9	7.5	1402	PASS
176	174	95	101	96.0	18013	PASS
177	176	5	9	6.0	1085	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	304	50.95	1947	64.10	67	78.85	116
36.95	1898	51.80	53	64.95	401	79.70	10
37.95	1580	55.85	624	67.90	3060	79.90	26
38.90	840	56.80	270	68.90	3112	80.85	120
43.80	11	56.95	702	69.95	242	81.75	368
44.95	340	59.70	153	71.80	167	86.90	1016
46.80	99	59.95	227	72.90	1325	87.85	1071
47.00	390	60.85	1733	73.90	5003	90.60	73
47.90	197	61.95	1823	74.95	13985	91.85	766
48.90	1530	62.95	1371	75.95	1307	92.90	1198
49.90	5930	63.85	136	76.90	233	93.90	3324

Average of 12.841 to 12.853 min.: VN082546.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.95	24723	140.75	277				
95.95	1748	142.90	419				
103.80	51	171.80	441				
105.70	59	172.80	123				
105.90	61	173.00	137				
115.70	54	173.90	18762				
116.80	190	174.85	1402				
117.00	81	175.90	18013				
117.90	54	176.85	1085				
118.80	122						
127.80	52						

Instrument :

MSVOA_N

ClientSampleId :

BFB