

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061325\
 Data File : VN086997.D
 Acq On : 13 Jun 2025 13:26
 Operator : JC\MD
 Sample : VN0613MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0613MBL01

Quant Time: Jun 14 00:26:56 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 07 02:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	200312	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	386949	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	337516	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	163660	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	131365	48.981	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	97.960%
35) Dibromofluoromethane	8.177	113	115591	50.407	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	100.820%
50) Toluene-d8	10.571	98	464342	51.150	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	102.300%
62) 4-Bromofluorobenzene	12.847	95	163773	48.558	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	97.120%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061325\
Data File : VN086997.D
Acq On : 13 Jun 2025 13:26
Operator : JC\MD
Sample : VN0613MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0613MBL01

Quant Time: Jun 14 00:26:56 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 07 02:12:50 2025
Response via : Initial Calibration




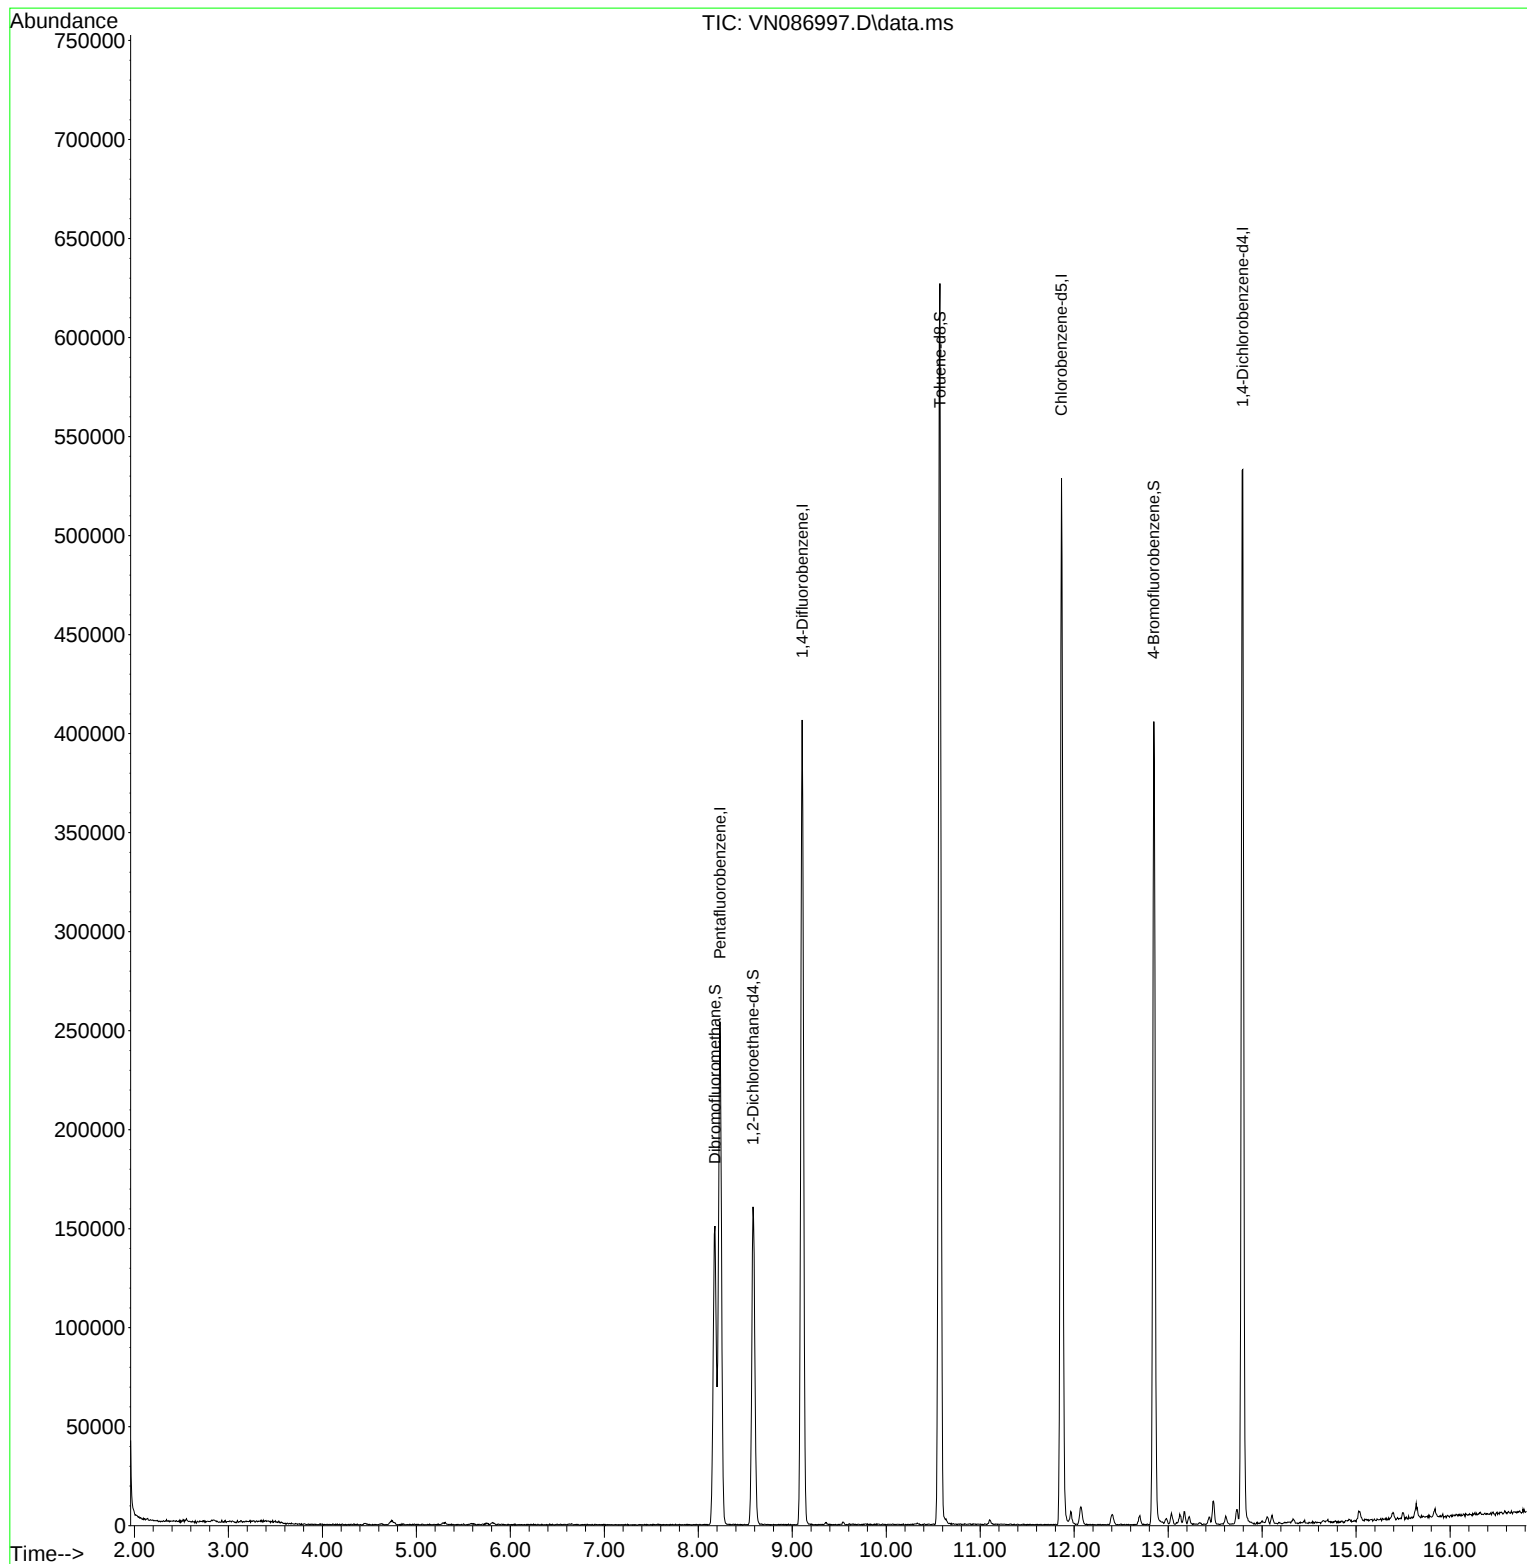


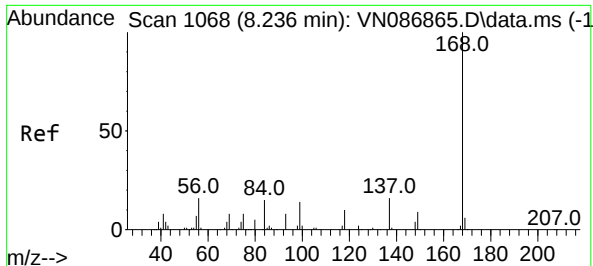

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 110
Delta R.T. -0.006 min
Lab File: VN086997.D
Acq: 13 Jun 2025 13:26




Instrument :
MSVOA_N
ClientSampleId :
VN0613MBL01


Tgt Ion:168 Resp: 200312
Ion Ratio Lower Upper
168 100
99 59.7 49.1 73.7

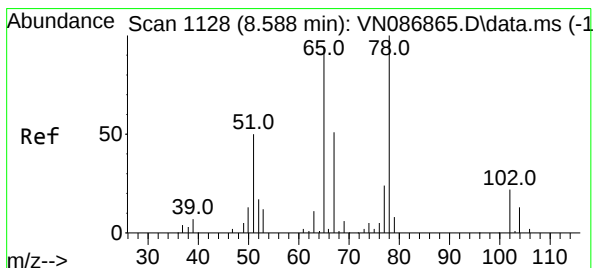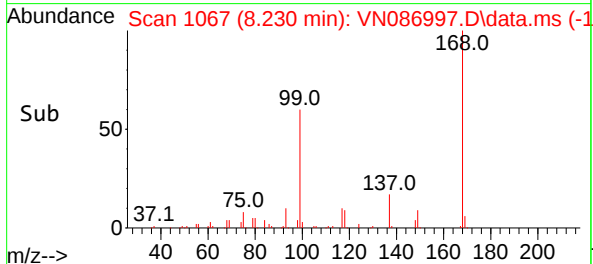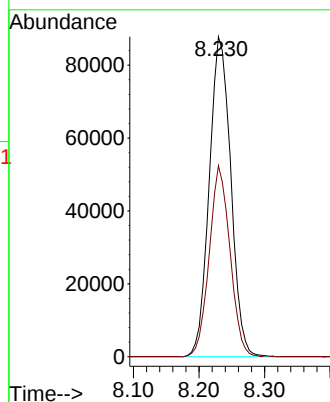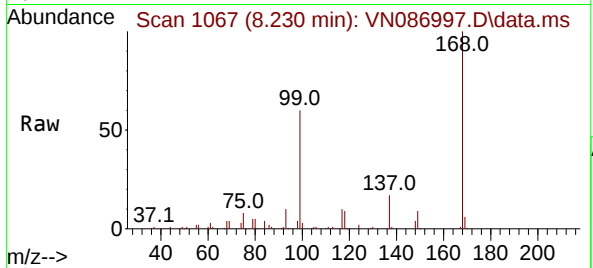

#33
1,2-Dichloroethane-d4
Concen: 48.981 ug/l
RT: 8.583 min Scan# 1127
Delta R.T. -0.006 min
Lab File: VN086997.D
Acq: 13 Jun 2025 13:26

Tgt Ion: 65 Resp: 131365
Ion Ratio Lower Upper
65 100
67 54.9 0.0 105.6

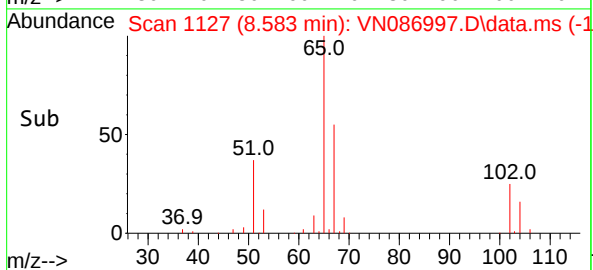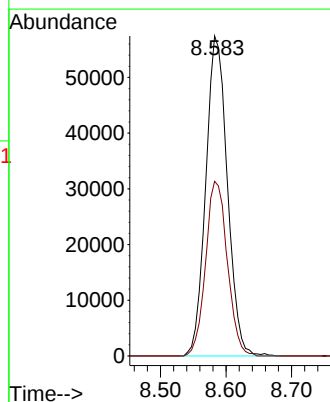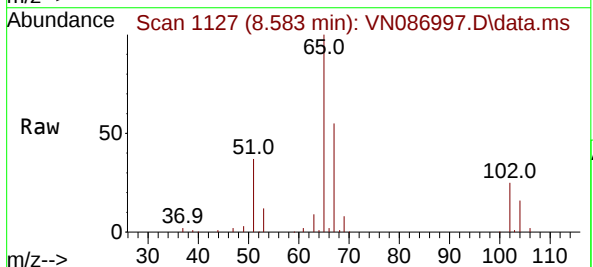

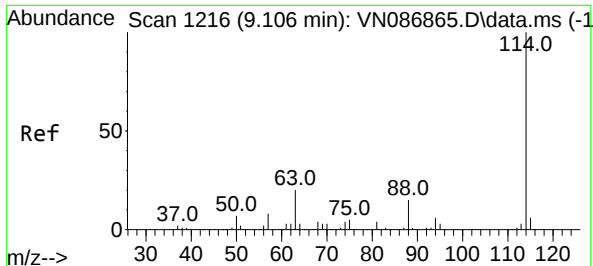

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 11

Delta R.T. -0.000 min

Lab File: VN086997.D

Acq: 13 Jun 2025 13:26

Instrument :

MSVOA_N

ClientSampleId :

VN0613MBL01





Tgt Ion:114 Resp: 386949

Ion Ratio Lower Upper

114 100

63 19.0 0.0 39.6

88 15.6 0.0 30.2

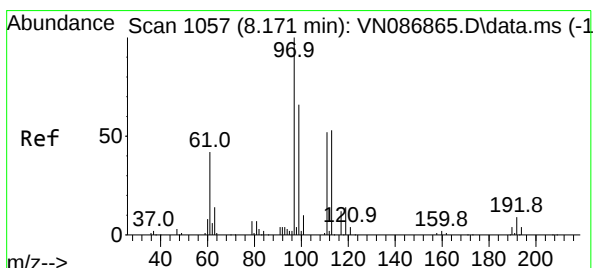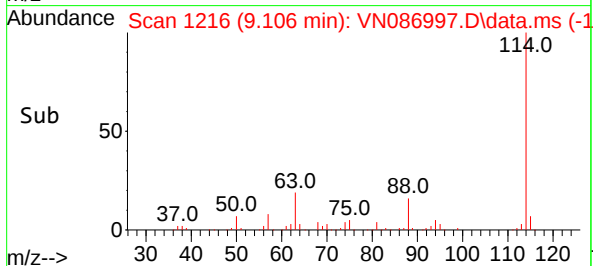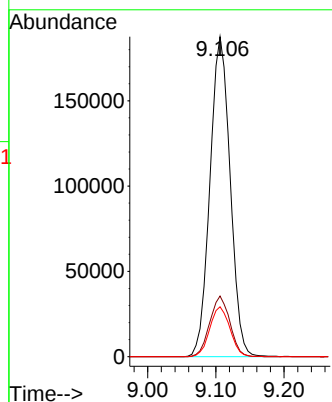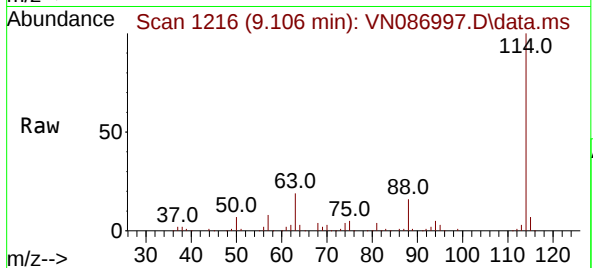

#35

Dibromofluoromethane

Concen: 50.407 ug/l

RT: 8.177 min Scan# 1058

Delta R.T. 0.006 min

Lab File: VN086997.D

Acq: 13 Jun 2025 13:26




Tgt Ion:113 Resp: 115591


Ion Ratio Lower Upper

113 100

111 102.7 84.2 126.2

192 18.4 14.2 21.4


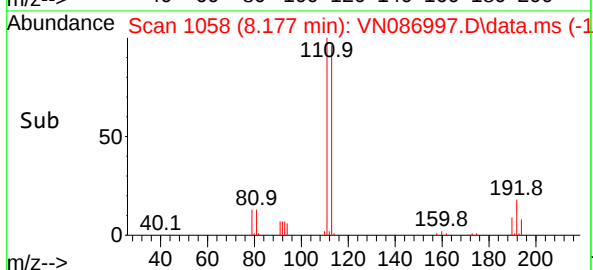
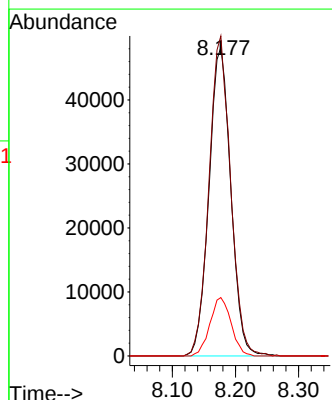
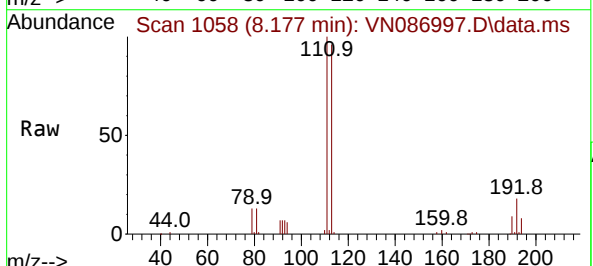


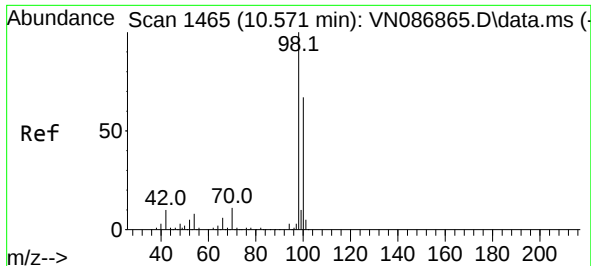

#50
Toluene-d8
Concen: 51.150 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN086997.D
Acq: 13 Jun 2025 13:26




Instrument :
MSVOA_N
ClientSampleId :
VN0613MBL01


Tgt Ion: 98 Resp: 464342
Ion Ratio Lower Upper
98 100
100 66.6 53.4 80.0

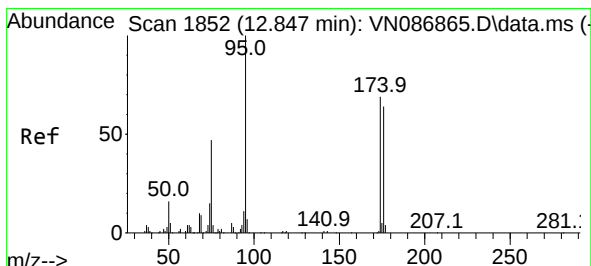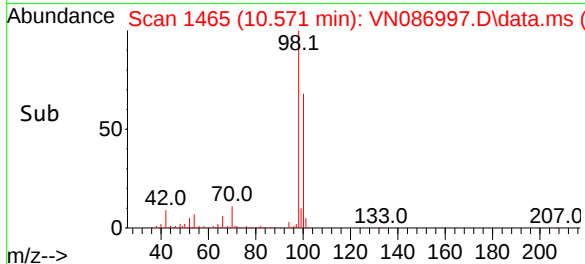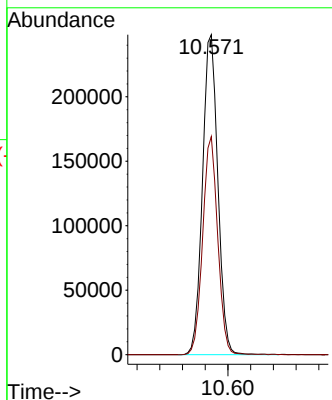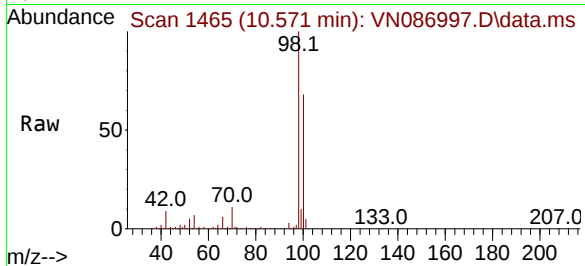

#62
4-Bromofluorobenzene
Concen: 48.558 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN086997.D
Acq: 13 Jun 2025 13:26

Tgt Ion: 95 Resp: 163773
Ion Ratio Lower Upper
95 100
174 72.5 0.0 141.8
176 69.3 0.0 132.6


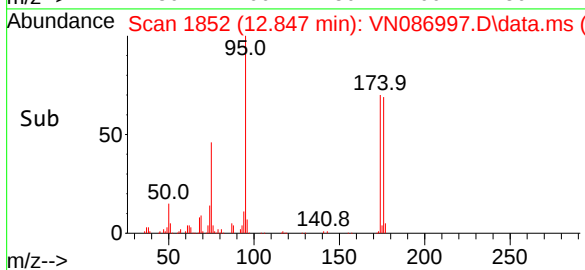
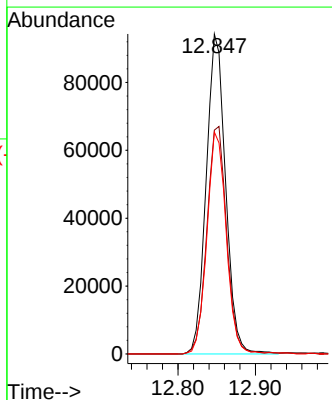
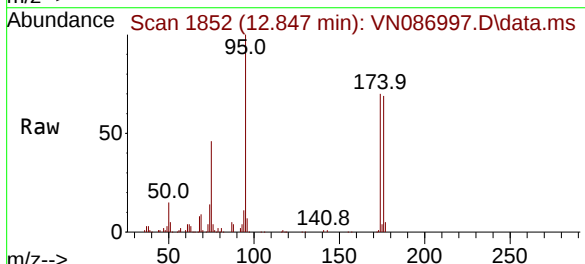


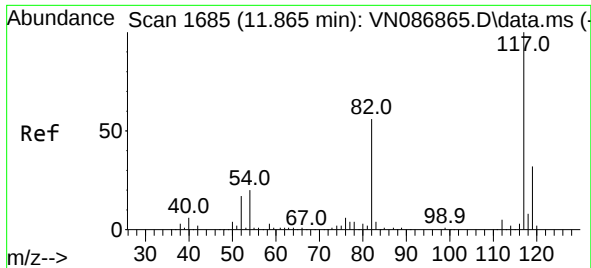

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN086997.D
Acq: 13 Jun 2025 13:26

Instrument :
MSVOA_N
ClientSampleId :
VN0613MBL01

Tgt Ion:117 Resp: 337516
Ion Ratio Lower Upper
117 100
82 53.5 44.6 67.0
119 32.2 25.5 38.3

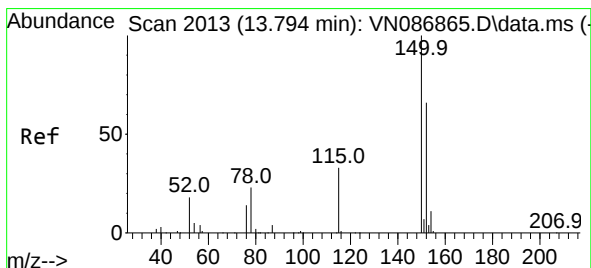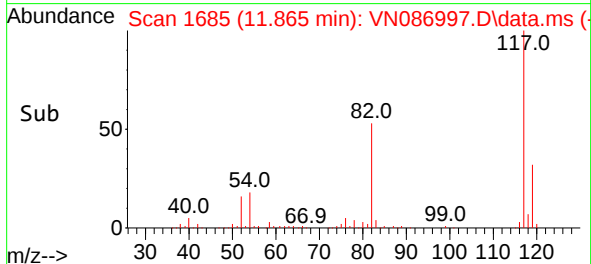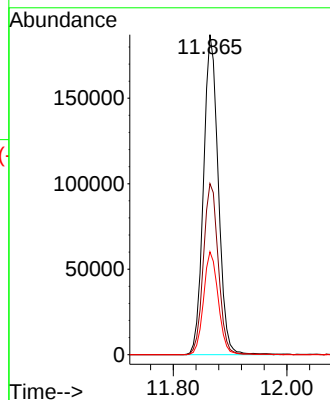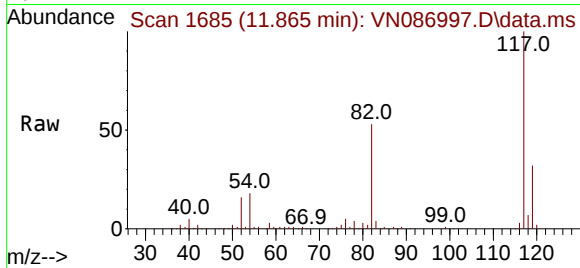

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN086997.D
Acq: 13 Jun 2025 13:26

Tgt Ion:152 Resp: 163660
Ion Ratio Lower Upper
152 100
115 60.1 30.1 90.5
150 158.9 0.0 345.0

