
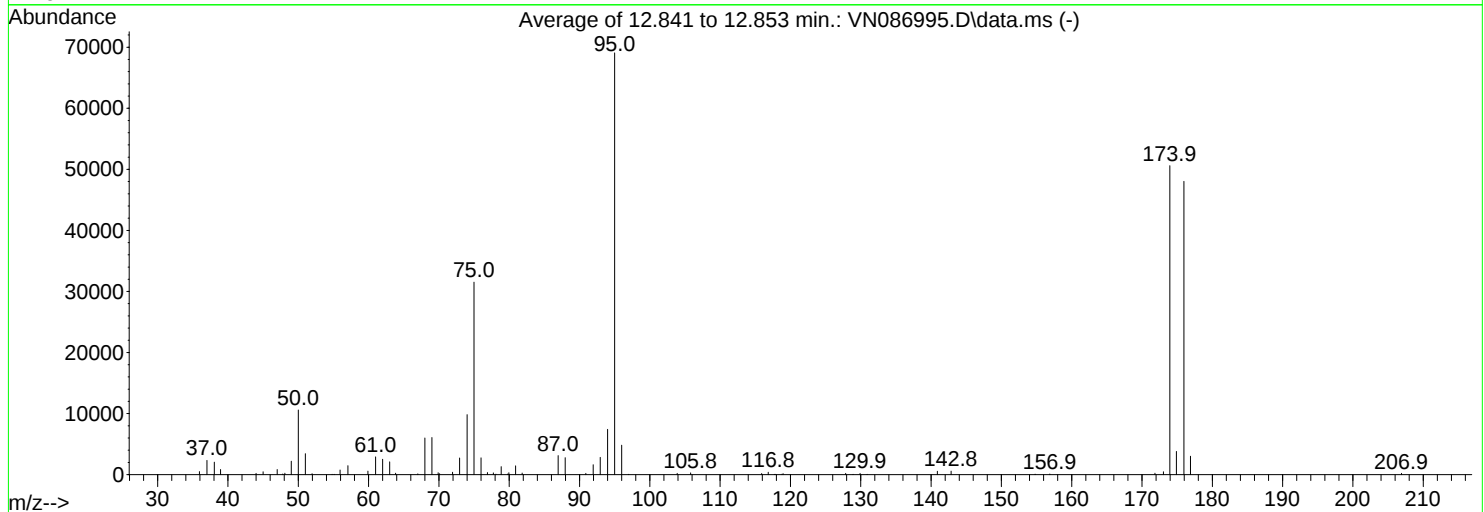


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061325\
Data File : VN086995.D
Acq On : 13 Jun 2025 10:26
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
Title : SW846 8260
Last Update : Sat Jun 07 02:12:50 2025

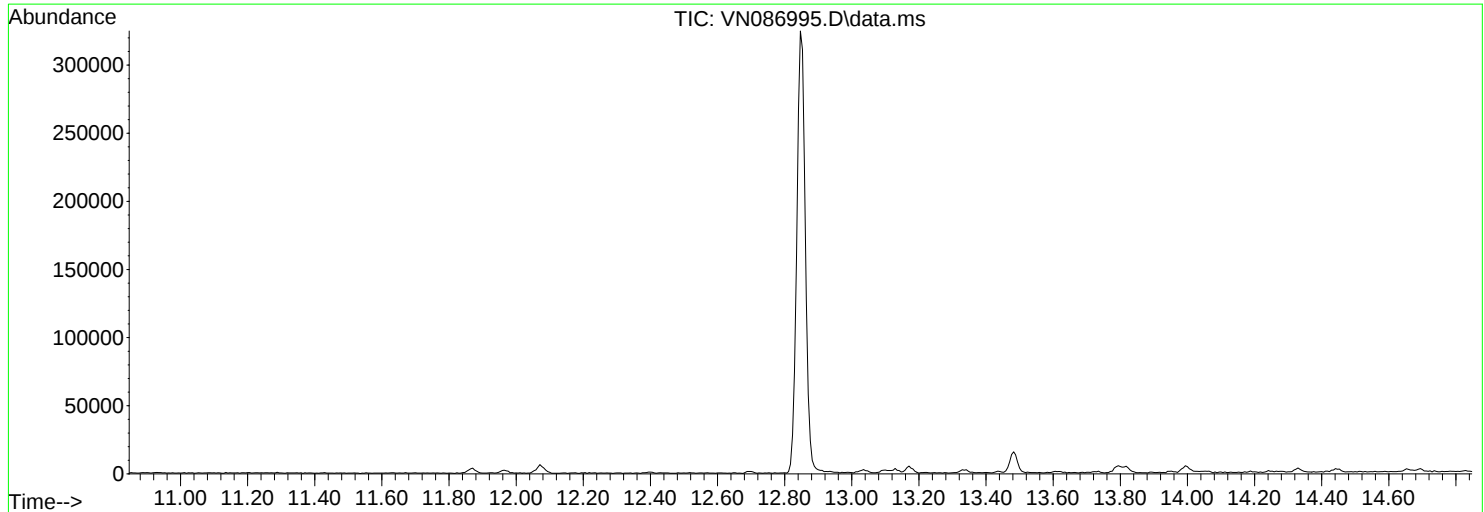

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	10594	PASS
75	95	30	60	45.6	31528	PASS
95	95	100	100	100.0	69080	PASS
96	95	5	9	7.0	4824	PASS
173	174	0.00	2	0.9	467	PASS
174	95	50	100	73.2	50592	PASS
175	174	5	9	7.5	3797	PASS
176	174	95	101	94.9	48037	PASS
177	176	5	9	6.3	3018	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	502	51.00	3443	67.00	147	77.75	279
37.00	2347	51.95	163	68.00	5999	78.10	8
38.05	2058	54.80	50	69.00	6072	78.85	130
38.95	843	55.10	54	69.90	305	79.80	11
44.00	215	55.95	750	70.10	171	79.95	318
45.00	483	57.05	1476	71.95	403	80.90	1433
47.00	846	59.90	569	72.95	2733	81.85	252
47.80	104	61.00	2919	74.00	9842	86.95	3110
48.10	225	62.00	2530	75.00	31528	87.95	2782
49.00	2194	63.00	2107	76.00	2749	90.90	210
50.00	10594	63.85	232	76.90	348	91.95	1631

Average of 12.841 to 12.853 min.: VN086995.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.95	2835	118.80	70	173.05	467		
94.00	7405	118.95	170	173.95	50592		
95.00	69080	127.85	212	174.90	3797		
96.00	4824	128.90	62	175.95	48037		
97.00	51	129.90	216	176.90	3018		
103.90	222	130.90	53	206.90	203		
105.80	301	140.90	561				
115.90	197	142.85	568				
116.85	390	154.80	70				
117.70	57	156.90	104				
117.90	67	171.85	231				

Instrument :

MSVOA_N

ClientSampleId :

BFB