


Methyl Iodide

Response Ratio

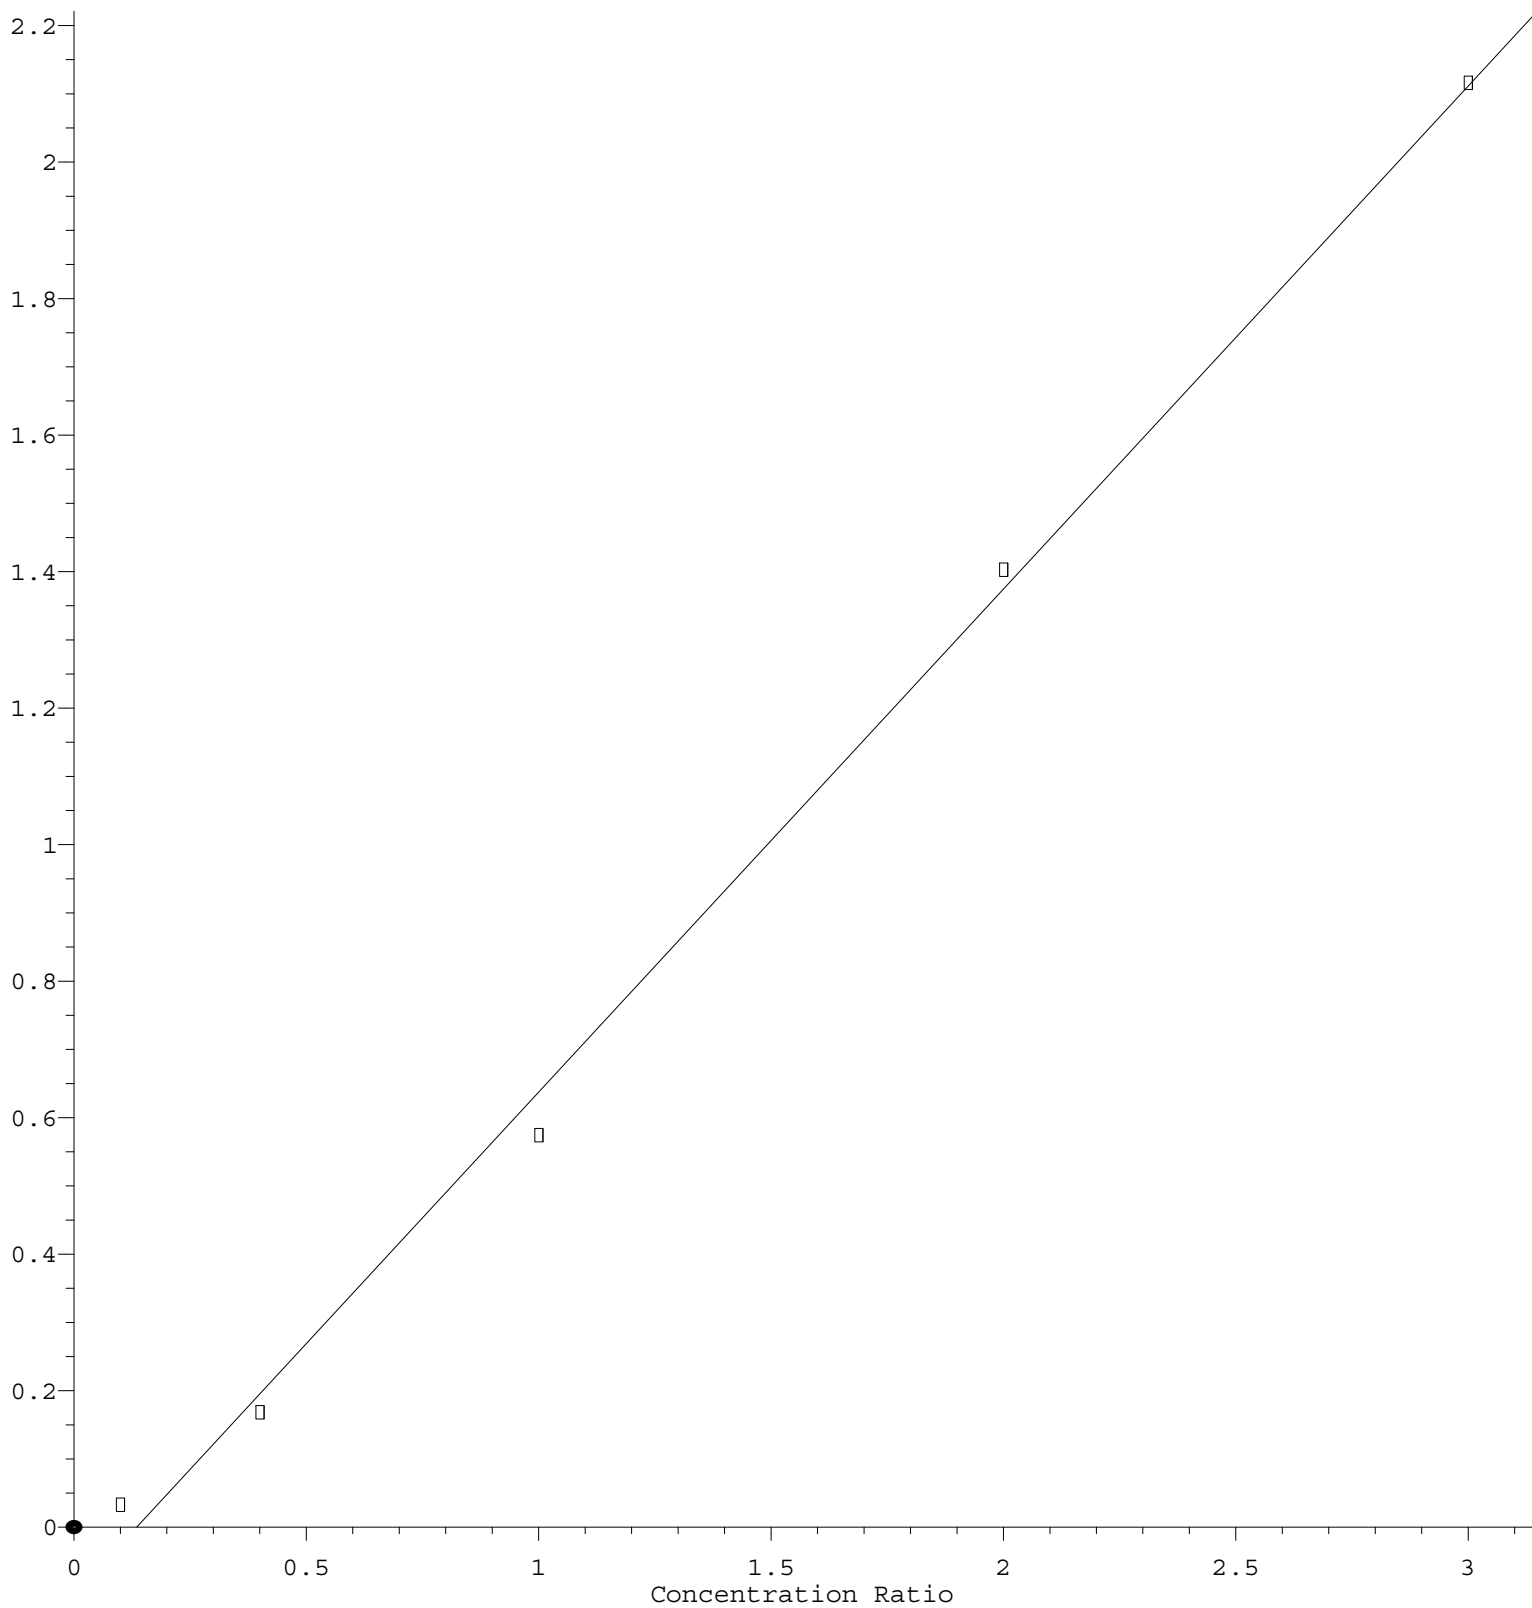

$$\text{Response} = 7.371\text{e-}001 * \text{Amt} - 9.941\text{e-}002$$


Coef of Det (r^2) = 0.997115 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N061421W.M

Calibration Table Last Updated: Tue Jun 15 05:19:42 2021

Dichlorodifluoromethane

Response Ratio

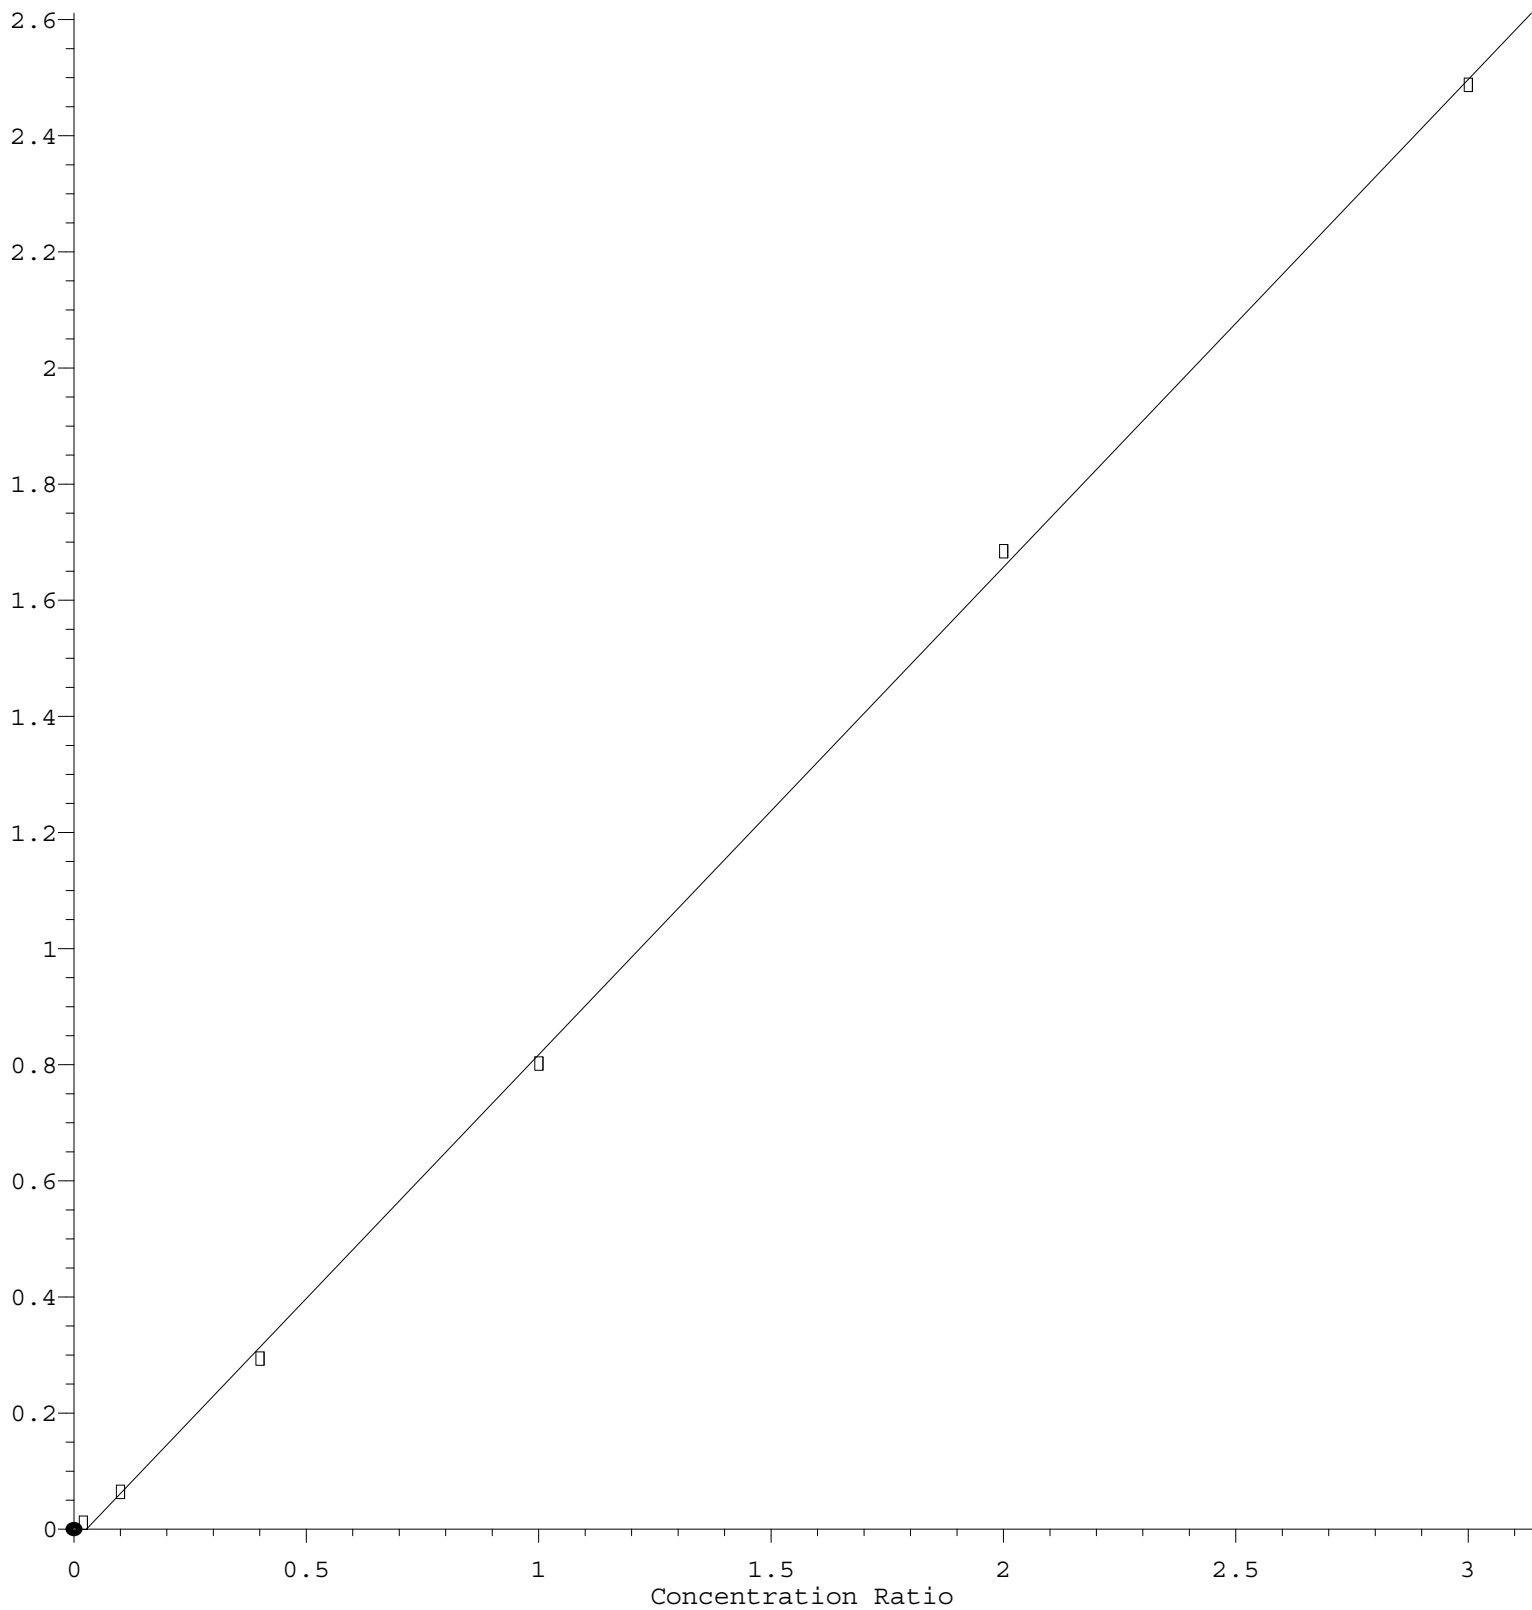

$$\text{Response} = 8.400\text{e-}001 * \text{Amt} - 2.228\text{e-}002$$


Coef of Det (r^2) = 0.999652 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N061421W.M

Calibration Table Last Updated: Tue Jun 15 05:19:42 2021

Naphthalene

Response Ratio

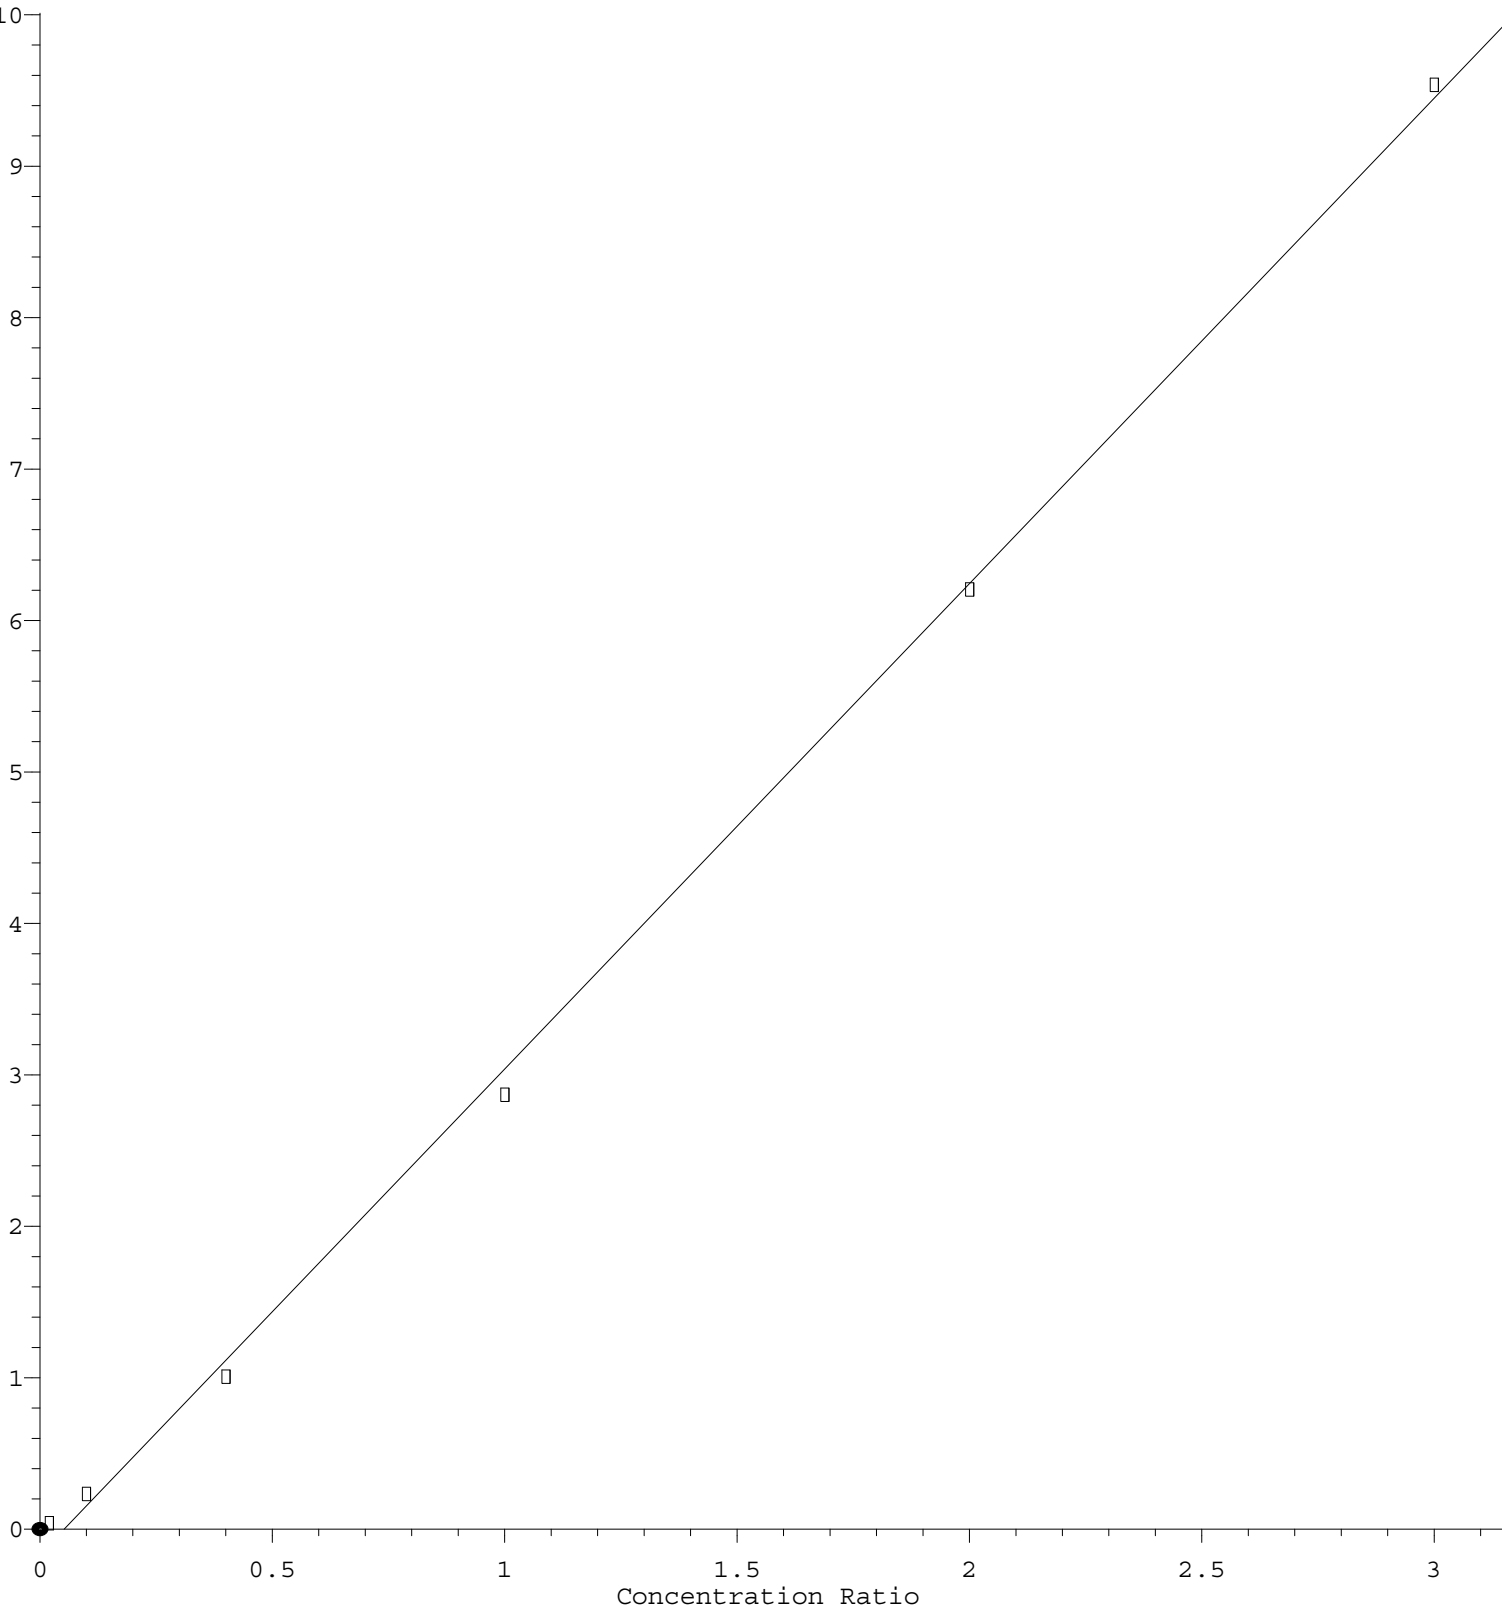

$$\text{Response} = 3.204\text{e}+000 * \text{Amt} - 1.671\text{e}-001$$

Coef of Det (r^2) = 0.998952 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N061421W.M

Calibration Table Last Updated: Tue Jun 15 05:19:42 2021