

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061423\
 Data File : VN078198.D
 Acq On : 14 Jun 2023 12:08
 Operator : JC\MD
 Sample : 03225-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 GWOW-BR-05-75-87-061323

Quant Time: Jun 15 02:41:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 07 05:05:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.229	168	479844	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	879500	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	778052	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	250250	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	333732	52.164	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 104.320%	
35) Dibromofluoromethane	8.177	113	306176	55.058	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 110.120%	
50) Toluene-d8	10.570	98	1045417	48.764	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 97.520%	
62) 4-Bromofluorobenzene	12.853	95	328635	49.311	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 98.620%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.377	50	1273	Below Cal	#	75
4) Vinyl Chloride	2.524	62	5266	0.741	ug/l #	87
5) Bromomethane	2.971	94	1441	0.268	ug/l #	46
9) 1,1,2-Trichlorotrifluo...	4.359	101	1255	0.247	ug/l #	32
12) 1,1-Dichloroethene	4.353	96	493238	94.131	ug/l	90
16) Acetone	4.447	43	5623	3.053	ug/l	90
20) Methylene Chloride	5.283	84	1816	0.298	ug/l #	45
21) trans-1,2-Dichloroethene	5.794	96	34248	6.060	ug/l	85
24) 1,1-Dichloroethane	6.577	63	63202	6.368	ug/l	98
25) 2-Butanone	7.500	43	1153	0.407	ug/l #	24
27) cis-1,2-Dichloroethene	7.494	96	307905	45.675	ug/l	97
31) Cyclohexane	8.229	56	12120	1.477	ug/l #	13
36) 1,1-Dichloropropene	8.235	75	42487	5.327	ug/l #	47
38) Carbon Tetrachloride	8.224	117	52689	6.256	ug/l #	17
40) Benzene	8.606	78	5810	0.244	ug/l	93
42) 1,2-Dichloroethane	8.682	62	34719	4.252	ug/l	100
44) Trichloroethene	9.359	130	360697	57.355	ug/l	100
49) 1,4-Dioxane	9.700	88	7975	75.872	ug/l #	92
52) Toluene	10.635	92	236316	15.718	ug/l	94
59) 2-Hexanone	11.206	43	1082	0.248	ug/l	90
60) Dibromochloromethane	11.106	129	2110	0.339	ug/l #	11
64) Tetrachloroethene	11.100	164	2485	0.479	ug/l #	60
68) m/p-Xylenes	12.076	106	3826	0.349	ug/l	97
71) Bromoform	12.853	173	3237	0.818	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	12.935	83	114	Below Cal	#	26
76) 1,2,3-Trichloropropane	12.853	75	180590	30.526	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	180590	93.785	ug/l #	15
93) 1,2,4-Trichlorobenzene	15.394	180	687	0.212	ug/l #	50
94) Hexachlorobutadiene	15.511	225	603	Below Cal	#	66

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_N
ClientSampleId :
GWOW-BR-05-75-87-061323

Instrument :
MSVOA_N
ClientSampleId :
GWOW-BR-05-75-87-061323









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.229 min Scan# 1068
Delta R.T. -0.006 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08




Instrument :
MSVOA_N
ClientSampleId :
GWOW-BR-05-75-87-061323


Tgt Ion:168 Resp: 479844
Ion Ratio Lower Upper
168 100
99 64.7 53.0 79.6

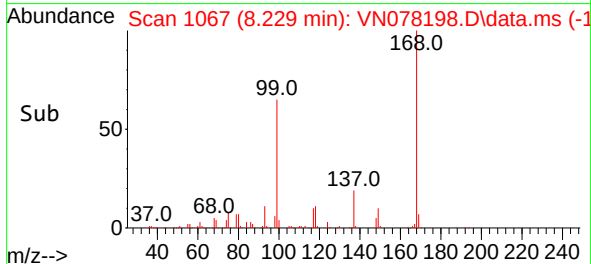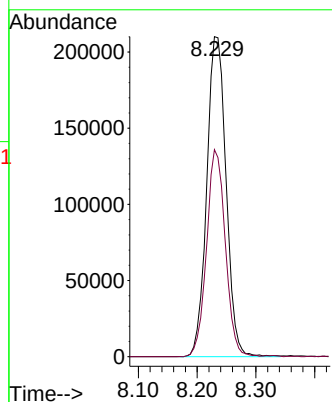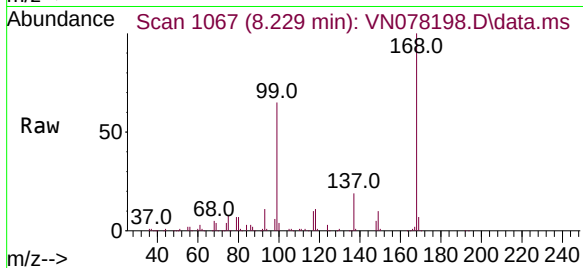

#3
Chloromethane
Concen: Below Cal
RT: 2.377 min Scan# 72
Delta R.T. 0.006 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08

Tgt Ion: 50 Resp: 1273
Ion Ratio Lower Upper
50 100
52 18.7 26.5 39.7#


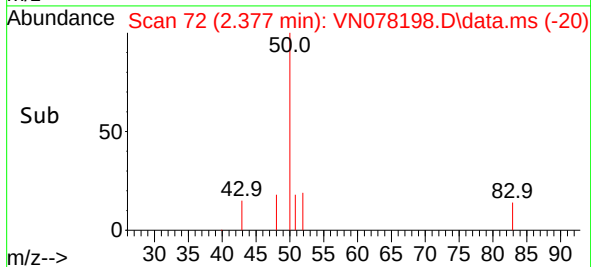
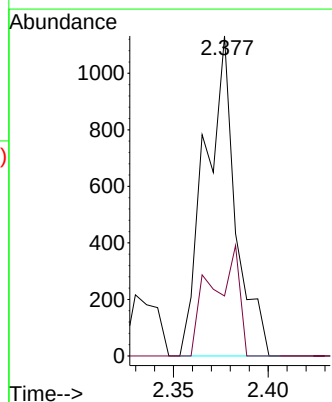
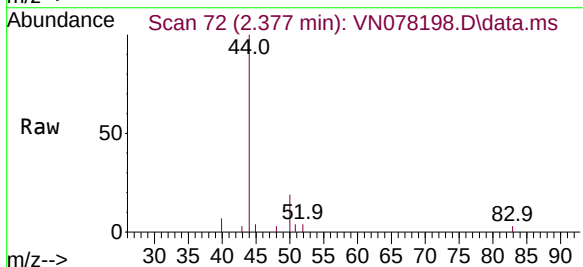


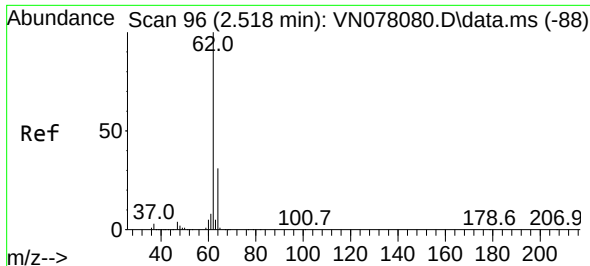

#4
 Vinyl Chloride
 Concen: 0.741 ug/l
 RT: 2.524 min Scan# 91
 Delta R.T. 0.006 min
 Lab File: VN078198.D
 Acq: 14 Jun 2023 12:08




Instrument :
 MSVOA_N
 ClientSampleId :
 GWOW-BR-05-75-87-061323


Tgt Ion: 62 Resp: 5266
 Ion Ratio Lower Upper
 62 100
 64 39.9 26.2 39.2#

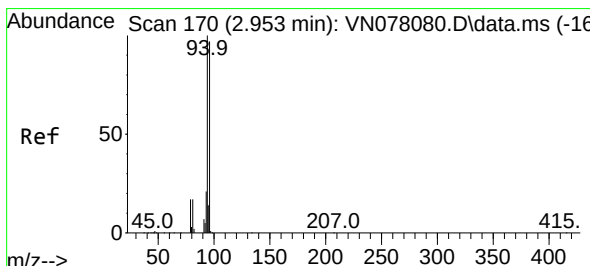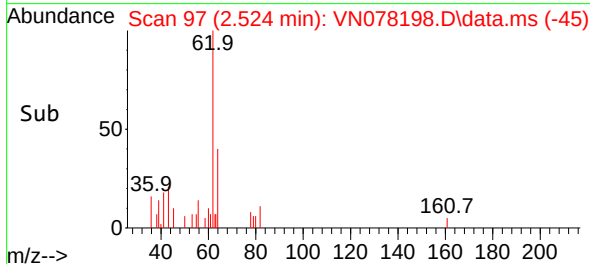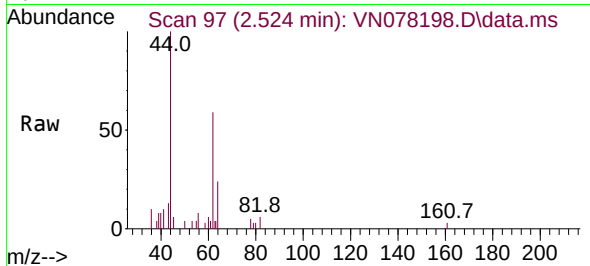

#5
 Bromomethane
 Concen: 0.268 ug/l
 RT: 2.971 min Scan# 173
 Delta R.T. 0.018 min
 Lab File: VN078198.D
 Acq: 14 Jun 2023 12:08

Tgt Ion: 94 Resp: 1441
 Ion Ratio Lower Upper
 94 100
 96 40.5 73.1 109.7#


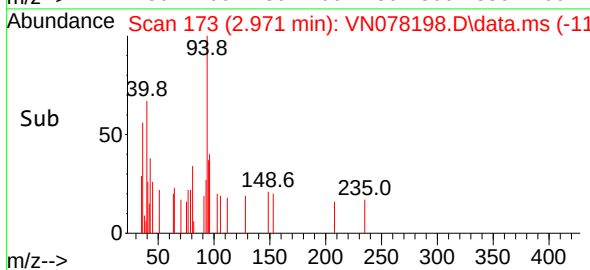

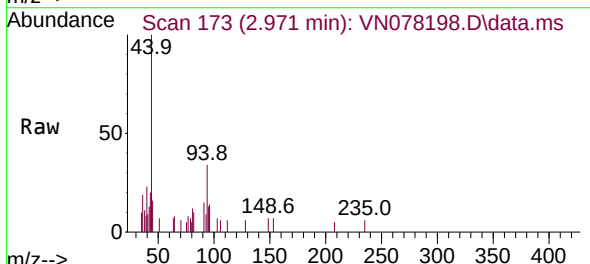




#9
 1,1,2-Trichlorotrifluoroethane
 Concen: 0.247 ug/l
 RT: 4.359 min Scan# 409
 Delta R.T. -0.018 min
 Lab File: VN078198.D
 Acq: 14 Jun 2023 12:08




Instrument :
 MSVOA_N
 ClientSampleId :
 GWOW-BR-05-75-87-061323


Tgt Ion:101 Resp: 1255
 Ion Ratio Lower Upper
 101 100
 85 19.7 36.6 55.0#
 151 0.0 57.6 86.4#

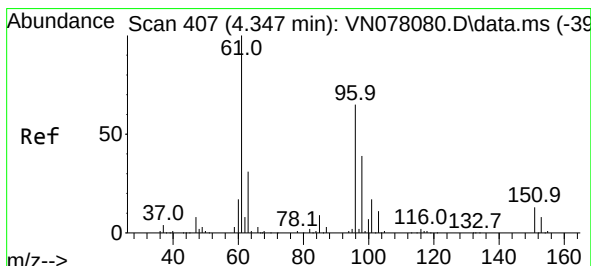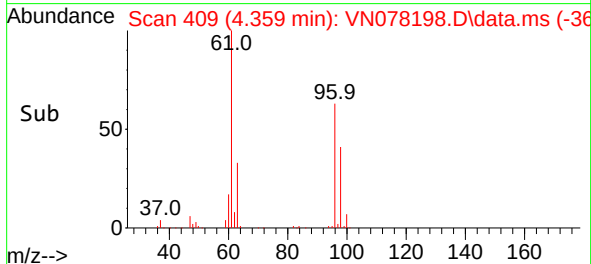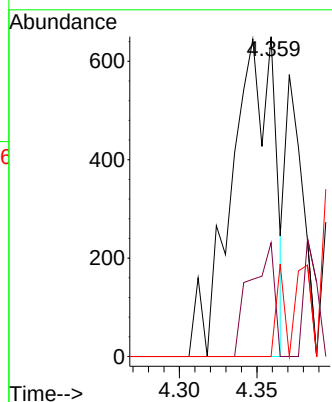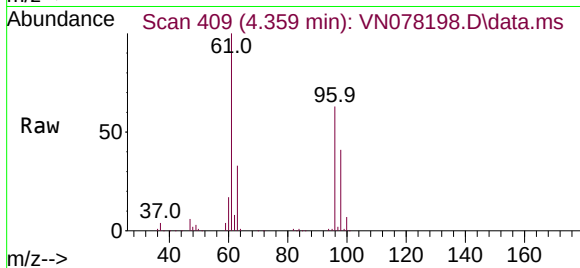

#12
 1,1-Dichloroethene
 Concen: 94.131 ug/l
 RT: 4.353 min Scan# 408
 Delta R.T. 0.006 min
 Lab File: VN078198.D
 Acq: 14 Jun 2023 12:08

Tgt Ion: 96 Resp: 493238
 Ion Ratio Lower Upper
 96 100
 61 158.4 112.7 169.1
 98 64.6 51.2 76.8

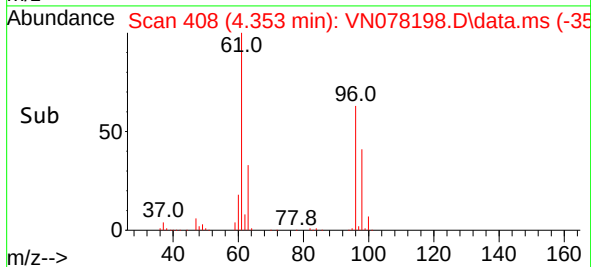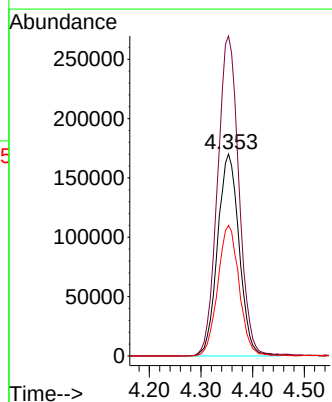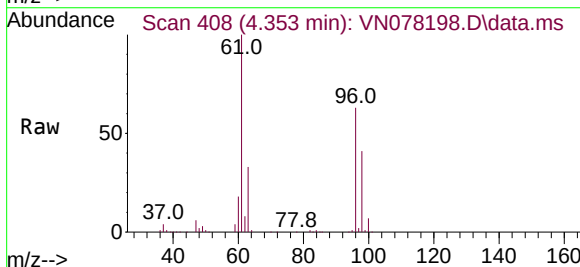

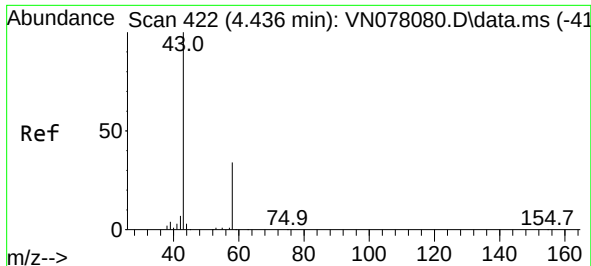

#16

Acetone

Concen: 3.053 ug/l

RT: 4.447 min Scan# 41

Delta R.T. 0.012 min

Lab File: VN078198.D

Acq: 14 Jun 2023 12:08

Instrument :

MSVOA_N

ClientSampleId :





GWOW-BR-05-75-87-061323

Tgt Ion: 43 Resp: 5623

Ion Ratio Lower Upper

43 100

58 29.2 28.0 42.0

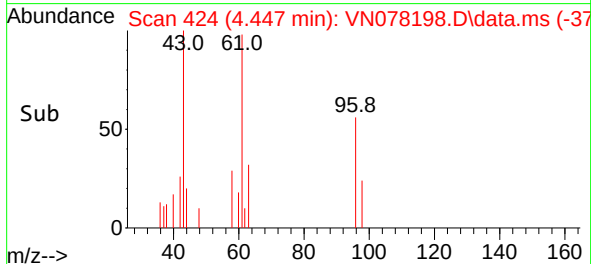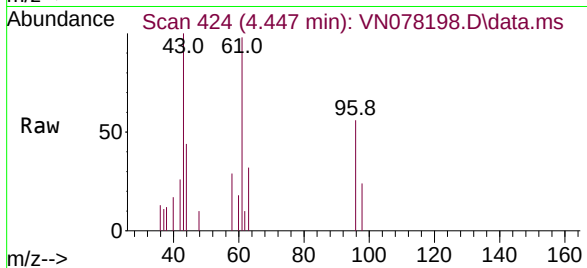

#20

Methylene Chloride

Concen: 0.298 ug/l

RT: 5.283 min Scan# 566

Delta R.T. -0.000 min

Lab File: VN078198.D

Acq: 14 Jun 2023 12:08

Tgt Ion: 84 Resp: 1816




Ion Ratio Lower Upper


84 100

49 30.4 79.7 119.5#

51 0.0 25.2 37.8#

86 39.6 53.3 79.9#


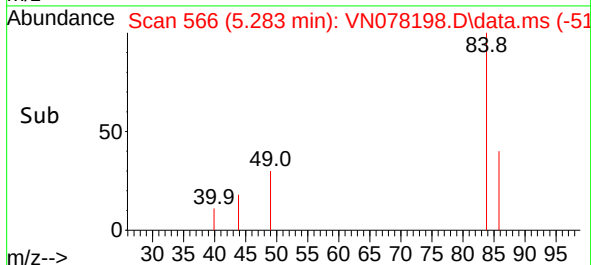

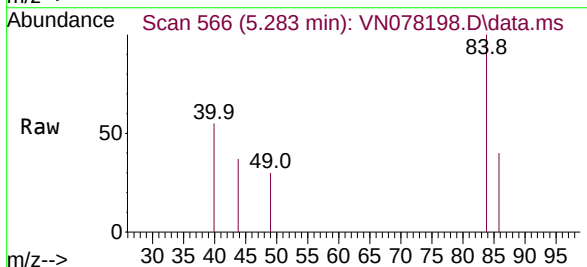


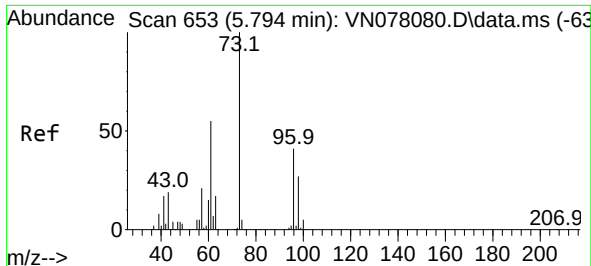

#21
trans-1,2-Dichloroethene
Concen: 6.060 ug/l
RT: 5.794 min Scan# 611
Delta R.T. -0.000 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08




Instrument :
MSVOA_N
ClientSampleId :
GWOW-BR-05-75-87-061323


Tgt Ion: 96 Resp: 34248
Ion Ratio Lower Upper
96 100
61 132.5 90.1 135.1
98 52.5 46.4 69.6

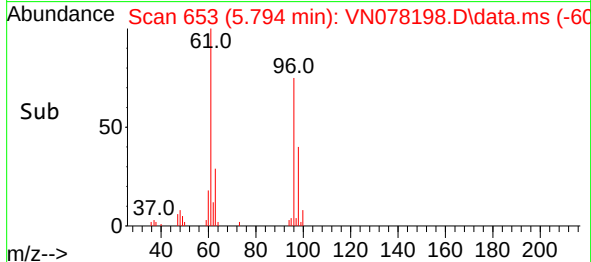

#24
1,1-Dichloroethane
Concen: 6.368 ug/l
RT: 6.577 min Scan# 786
Delta R.T. -0.000 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08

Tgt Ion: 63 Resp: 63202
Ion Ratio Lower Upper
63 100
98 7.1 3.9 11.7
100 4.6 2.5 7.4


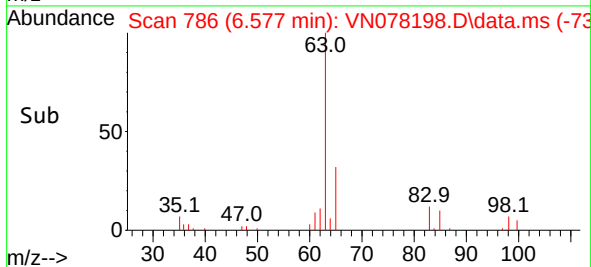

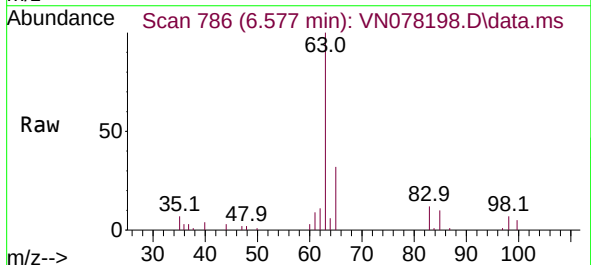


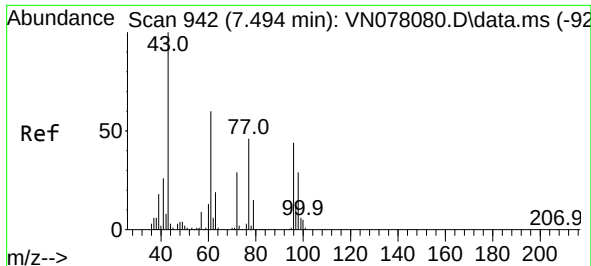

#25
2-Butanone
Concen: 0.407 ug/l
RT: 7.500 min Scan# 943
Delta R.T. 0.006 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08




Instrument :
MSVOA_N
ClientSampleId :
GWOW-BR-05-75-87-061323


Tgt Ion: 43 Resp: 1153
Ion Ratio Lower Upper
43 100
72 83.5 30.2 45.2#

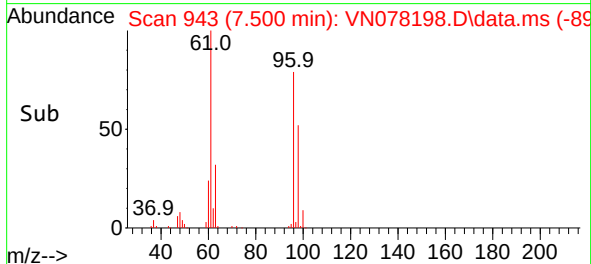

#27
cis-1,2-Dichloroethene
Concen: 45.675 ug/l
RT: 7.494 min Scan# 942
Delta R.T. -0.000 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08

Tgt Ion: 96 Resp: 307905
Ion Ratio Lower Upper
96 100
61 122.5 0.0 255.2
98 64.9 0.0 128.8


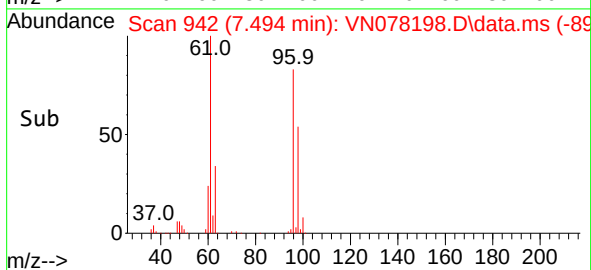

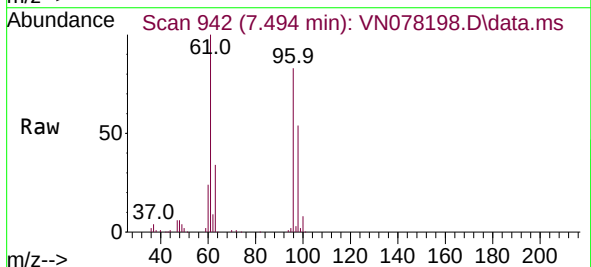


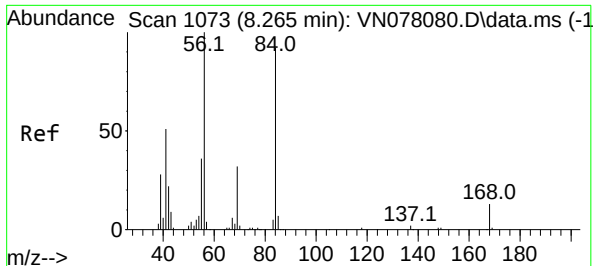

#31
Cyclohexane
Concen: 1.477 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.035 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08




Instrument :
MSVOA_N
ClientSampleId :
GWOW-BR-05-75-87-061323


Tgt Ion: 56 Resp: 12120
Ion Ratio Lower Upper
56 100
69 170.2 26.8 40.2#
84 138.9 81.8 122.6#

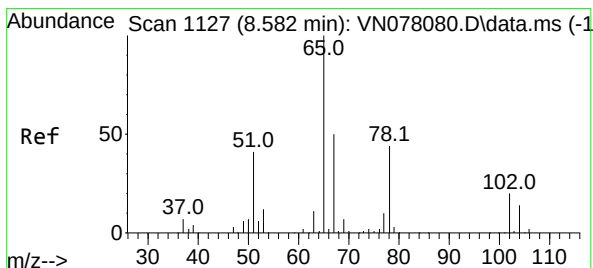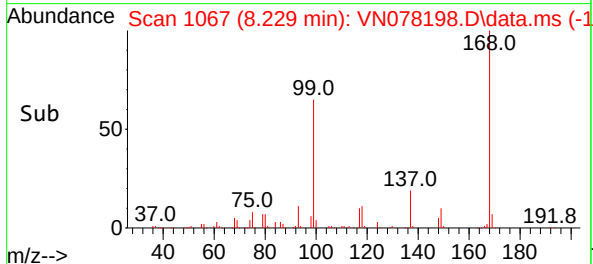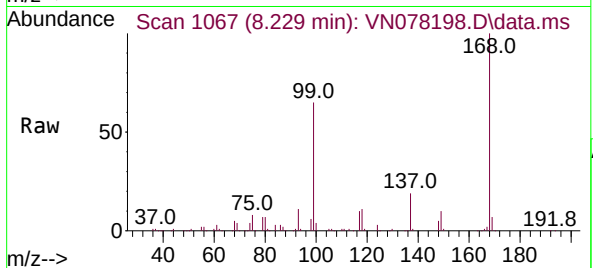

#33
1,2-Dichloroethane-d4
Concen: 52.164 ug/l
RT: 8.588 min Scan# 1128
Delta R.T. 0.006 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08

Tgt Ion: 65 Resp: 333732
Ion Ratio Lower Upper
65 100
67 51.8 0.0 106.6


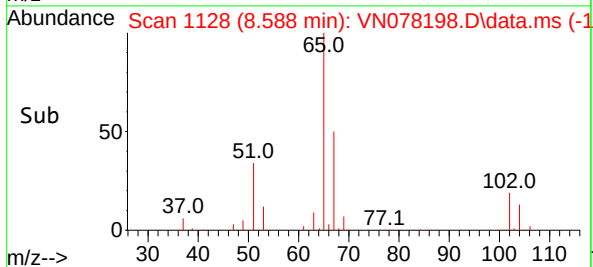

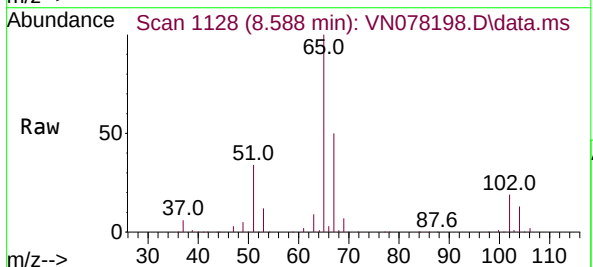


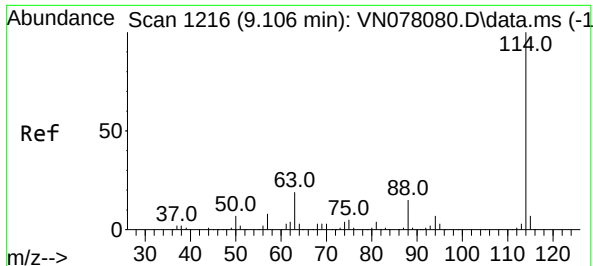

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08




Instrument :
MSVOA_N
ClientSampleId :
GWOW-BR-05-75-87-061323


Tgt Ion:114 Resp: 879500
Ion Ratio Lower Upper
114 100
63 19.7 0.0 36.4
88 15.8 0.0 30.6

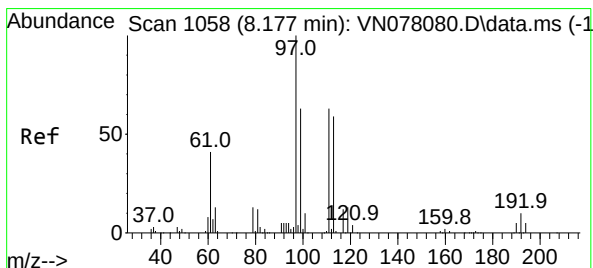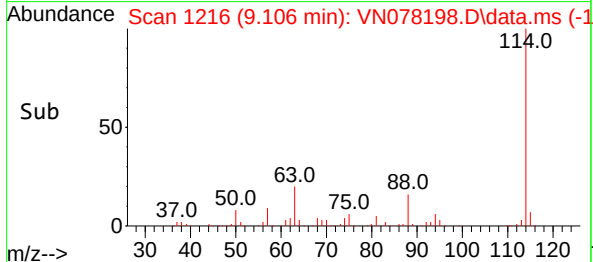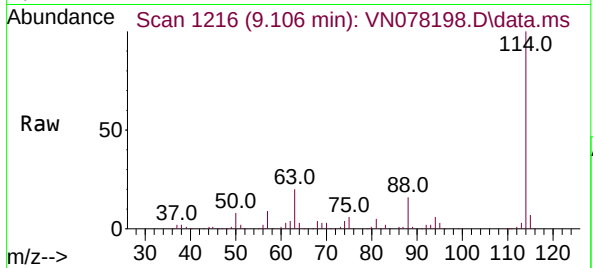

#35
Dibromofluoromethane
Concen: 55.058 ug/l
RT: 8.177 min Scan# 1058
Delta R.T. -0.000 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08

Tgt Ion:113 Resp: 306176
Ion Ratio Lower Upper
113 100
111 101.5 82.6 123.8
192 16.3 12.7 19.1

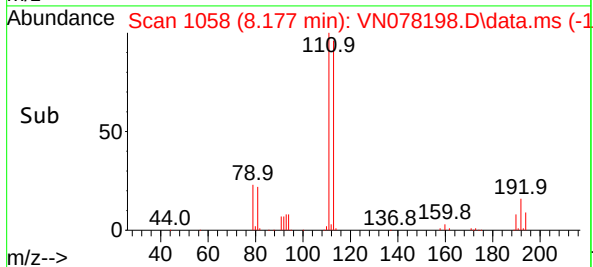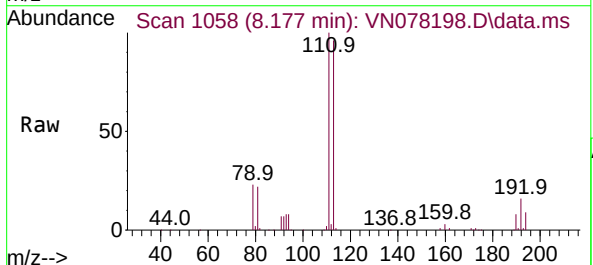

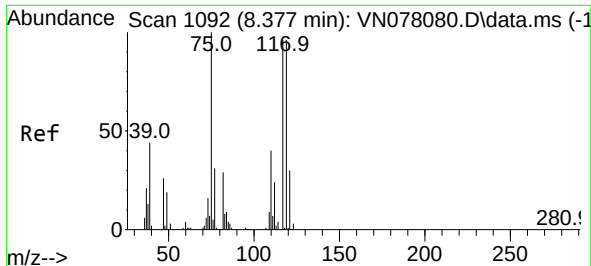

#36

1,1-Dichloropropene

Concen: 5.327 ug/l

RT: 8.235 min Scan# 1068

Delta R.T. -0.141 min

Lab File: VN078198.D

Acq: 14 Jun 2023 12:08

Instrument :

MSVOA_N

ClientSampleId :

GWOW-BR-05-75-87-061323





Tgt Ion: 75 Resp: 42487

Ion Ratio Lower Upper

75 100

110 7.9 19.1 57.3#

77 0.0 25.0 37.4#

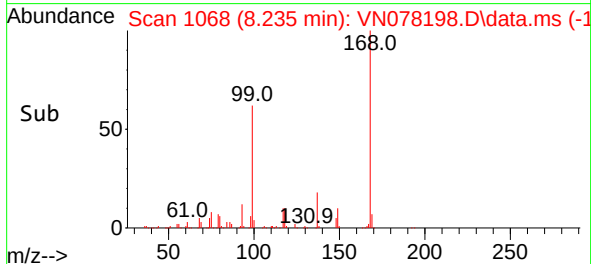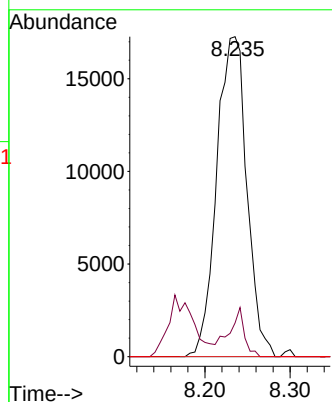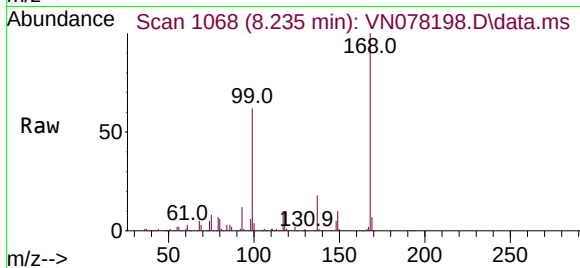

#38

Carbon Tetrachloride

Concen: 6.256 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.147 min

Lab File: VN078198.D

Acq: 14 Jun 2023 12:08




Tgt Ion: 117 Resp: 52689


Ion Ratio Lower Upper

117 100

119 7.2 77.3 115.9#

121 0.0 23.3 34.9#

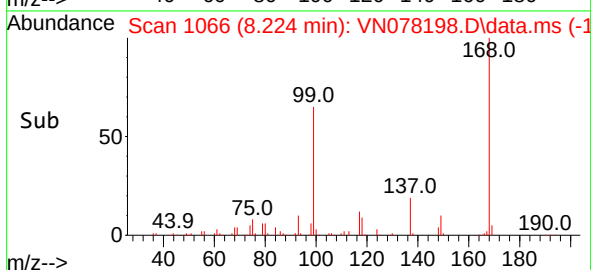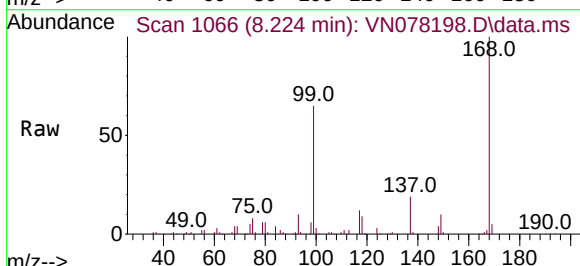

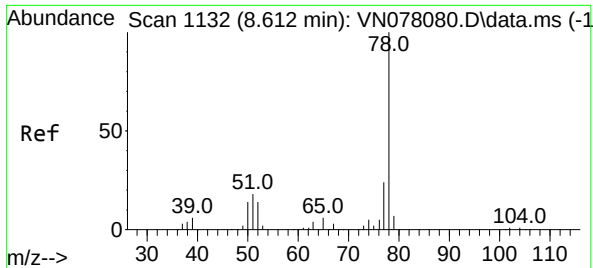

#40

Benzene

Concen: 0.244 ug/l

RT: 8.606 min Scan# 1131

Delta R.T. -0.006 min

Lab File: VN078198.D

Acq: 14 Jun 2023 12:08

Instrument :

MSVOA_N

ClientSampleId :





GWOW-BR-05-75-87-061323

Tgt Ion: 78 Resp: 5810

Ion Ratio Lower Upper

78 100

77 20.4 19.0 28.6

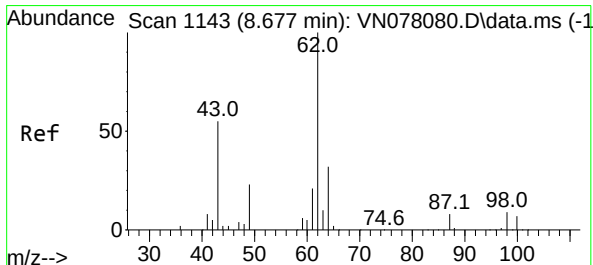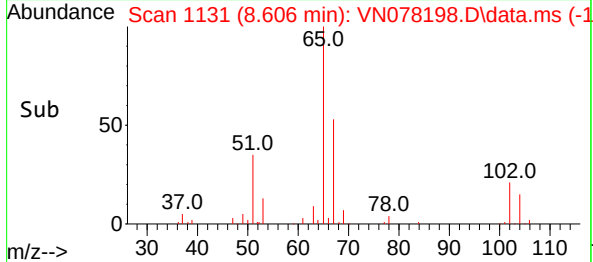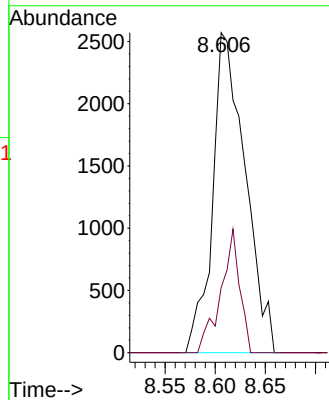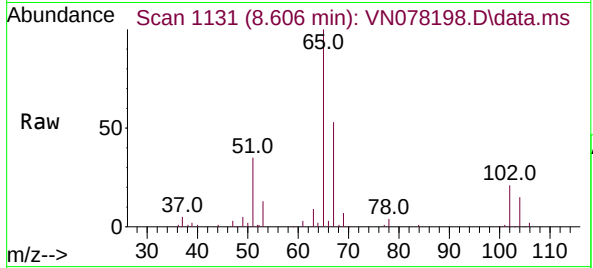

#42

1,2-Dichloroethane

Concen: 4.252 ug/l

RT: 8.682 min Scan# 1144

Delta R.T. 0.006 min

Lab File: VN078198.D




Acq: 14 Jun 2023 12:08


Tgt Ion: 62 Resp: 34719

Ion Ratio Lower Upper

62 100

98 9.9 0.0 19.8


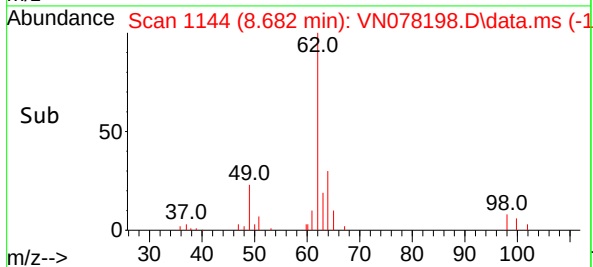
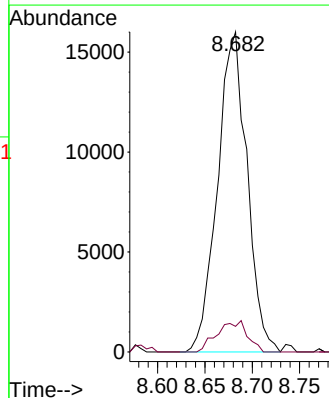
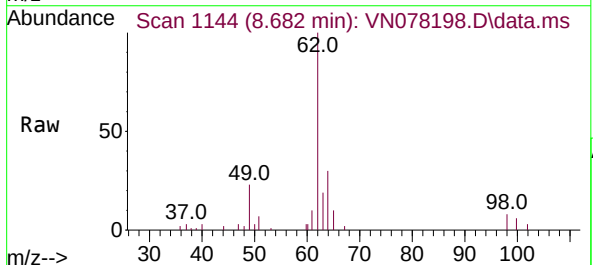


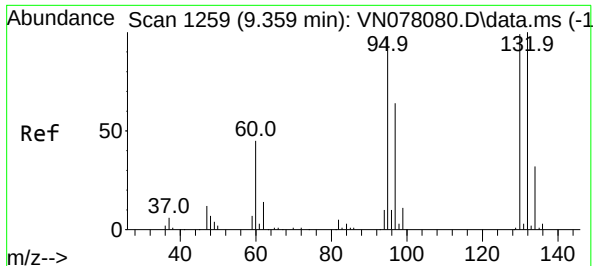

#44
Trichloroethene
Concen: 57.355 ug/l
RT: 9.359 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08




Instrument :
MSVOA_N
ClientSampleId :
GWOW-BR-05-75-87-061323


Tgt Ion:130 Resp: 360697
Ion Ratio Lower Upper
130 100
95 102.8 0.0 204.6

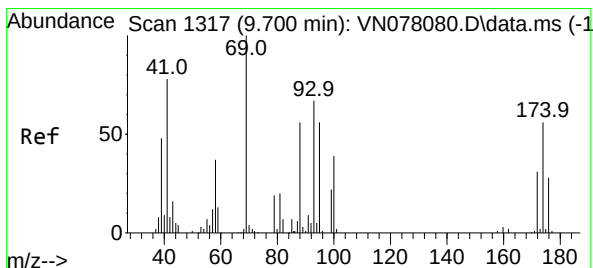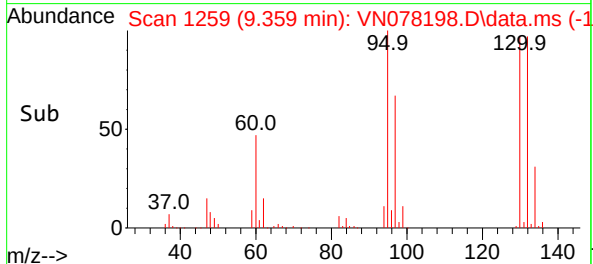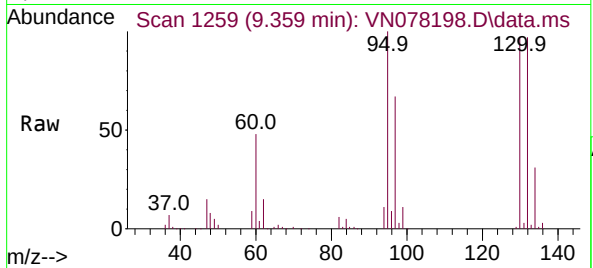

#49
1,4-Dioxane
Concen: 75.872 ug/l
RT: 9.700 min Scan# 1317
Delta R.T. -0.000 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08

Tgt Ion: 88 Resp: 7975
Ion Ratio Lower Upper
88 100
43 28.1 17.0 25.6#
58 62.7 47.0 70.4


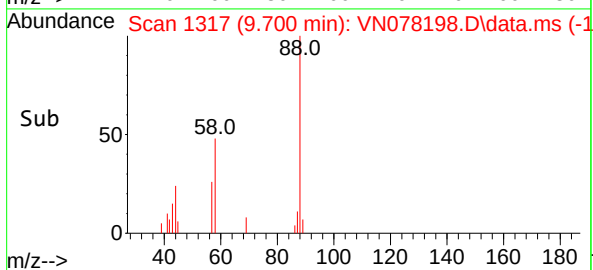

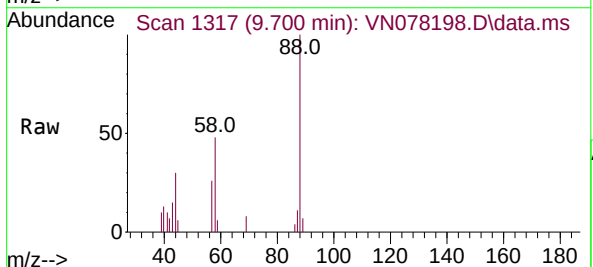




#50
Toluene-d8
Concen: 48.764 ug/l
RT: 10.570 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08




Instrument :
MSVOA_N
ClientSampleId :
GWOW-BR-05-75-87-061323


Tgt Ion: 98 Resp: 1045417
Ion Ratio Lower Upper
98 100
100 63.2 52.0 78.0

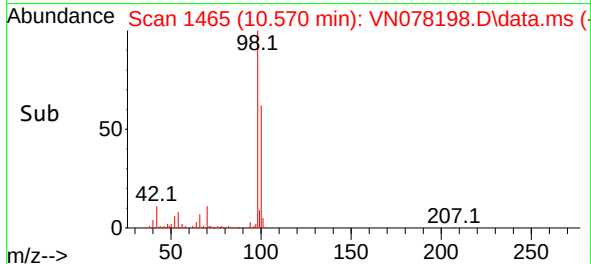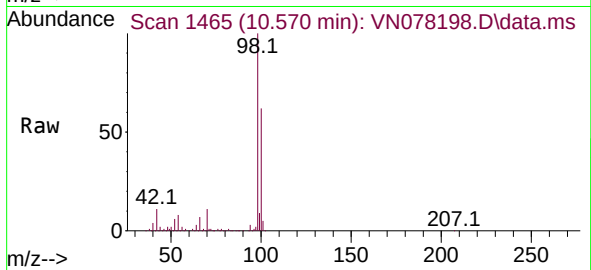

#52
Toluene
Concen: 15.718 ug/l
RT: 10.635 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08

Tgt Ion: 92 Resp: 236316
Ion Ratio Lower Upper
92 100
91 179.3 137.4 206.0


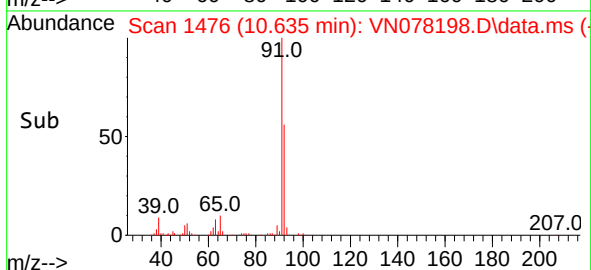

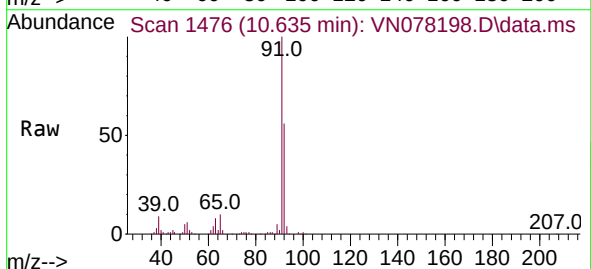


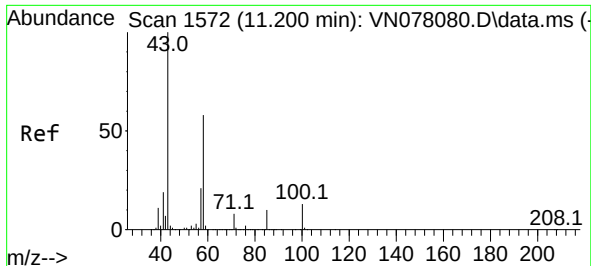

#59
2-Hexanone
Concen: 0.248 ug/l
RT: 11.206 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08




Instrument :
MSVOA_N
ClientSampleId :
GWOW-BR-05-75-87-061323


Tgt Ion: 43 Resp: 1082
Ion Ratio Lower Upper
43 100
58 55.8 31.7 95.1

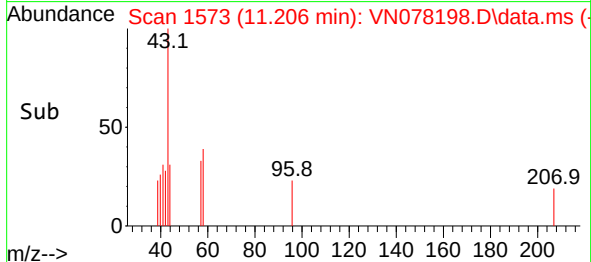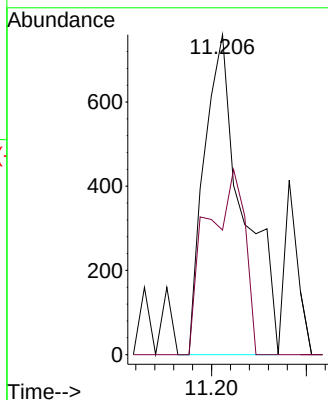

#60
Dibromochloromethane
Concen: 0.339 ug/l
RT: 11.106 min Scan# 1556
Delta R.T. -0.259 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08

Tgt Ion: 129 Resp: 2110
Ion Ratio Lower Upper
129 100
127 0.0 38.6 116.0#


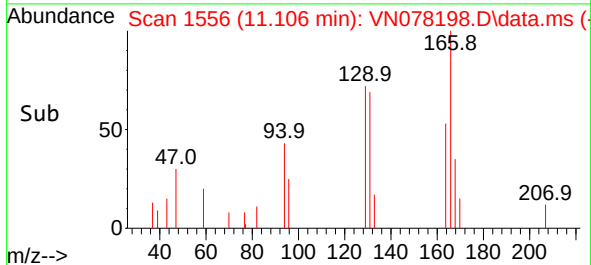
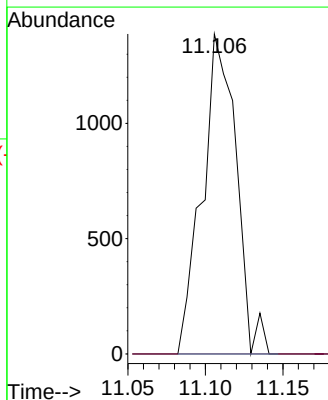
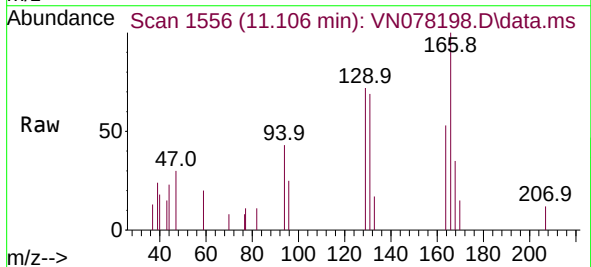


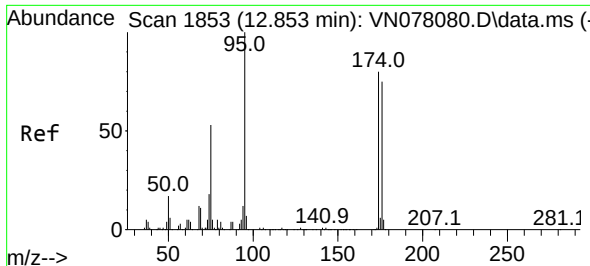

#62
4-Bromofluorobenzene
Concen: 49.311 ug/l
RT: 12.853 min Scan# 1185
Delta R.T. -0.000 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08




Instrument :
MSVOA_N
ClientSampleId :
GWOW-BR-05-75-87-061323


Tgt Ion:	95	Resp:	328635
Ion	Ratio	Lower	Upper
95	100		
174	74.2	0.0	143.8
176	70.4	0.0	135.8

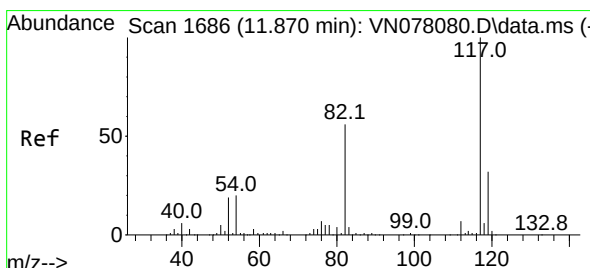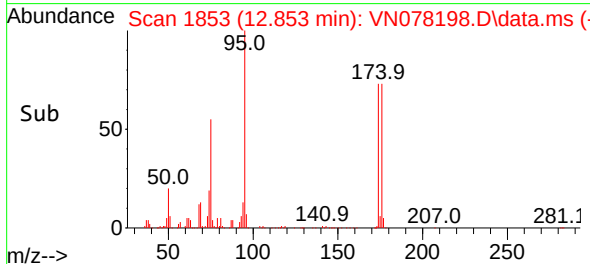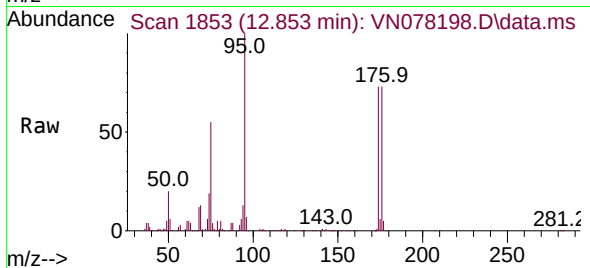

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1686
Delta R.T. -0.000 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08


Tgt Ion:	117	Resp:	778052
Ion	Ratio	Lower	Upper
117	100		
82	54.0	44.0	66.0
119	31.8	25.6	38.4

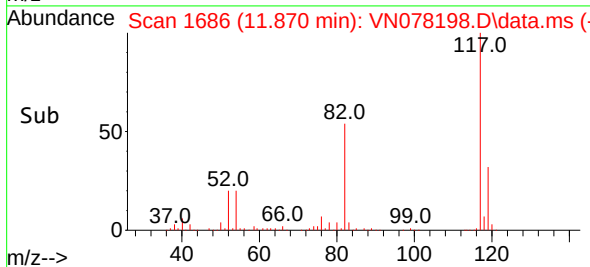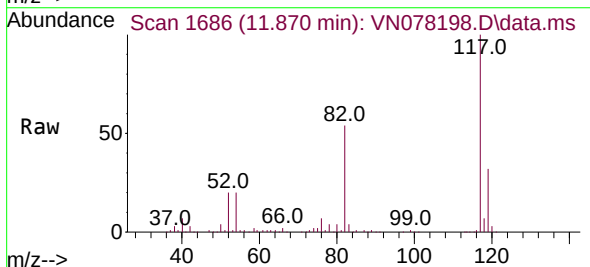



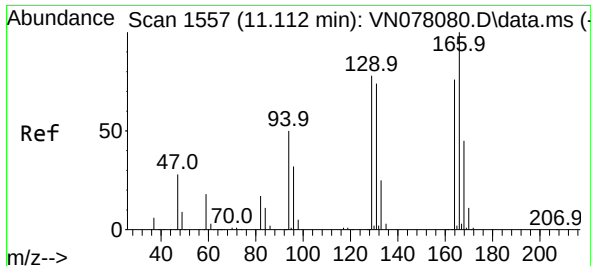


#64
Tetrachloroethene
Concen: 0.479 ug/l
RT: 11.100 min Scan# 11
Delta R.T. -0.012 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08

Instrument :
MSVOA_N
ClientSampleId :
GWOW-BR-05-75-87-061323







Tgt Ion:164 Resp: 2485
Ion Ratio Lower Upper
164 100
166 95.5 101.4 152.0#
129 44.3 82.4 123.6#
131 60.3 78.2 117.4#

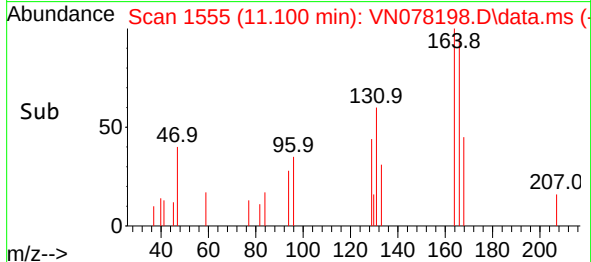

#68
m/p-Xylenes
Concen: 0.349 ug/l
RT: 12.076 min Scan# 1721
Delta R.T. -0.000 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08

Tgt Ion:106 Resp: 3826
Ion Ratio Lower Upper
106 100
91 203.4 159.6 239.4


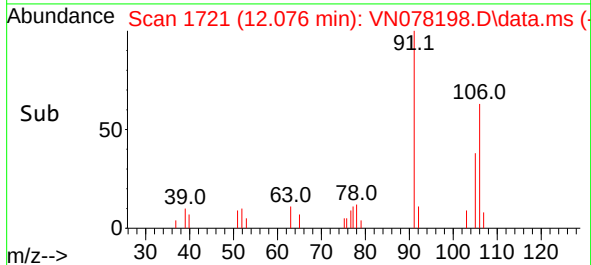
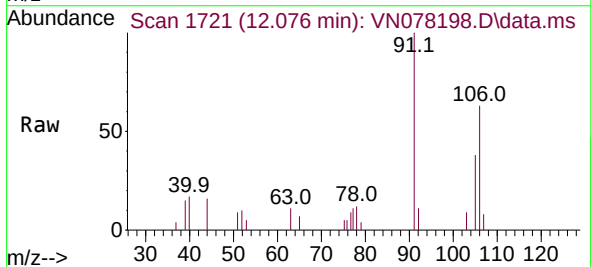



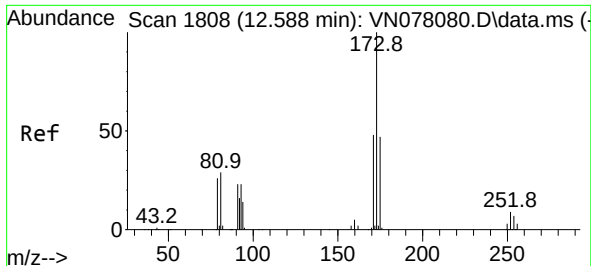

#71
Bromoform
Concen: 0.818 ug/l
RT: 12.853 min Scan# 1808
Delta R.T. 0.265 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08




Instrument :
MSVOA_N
ClientSampleId :
GWOW-BR-05-75-87-061323


Tgt Ion:173 Resp: 3237
Ion Ratio Lower Upper
173 100
175 471.9 24.3 73.0#
254 0.0 0.0 0.0

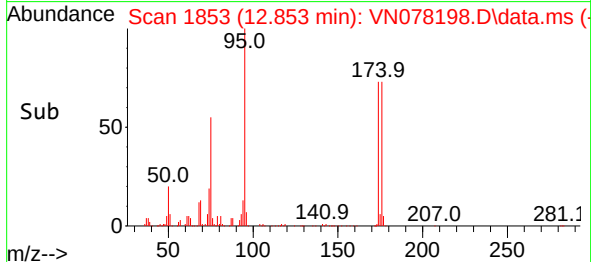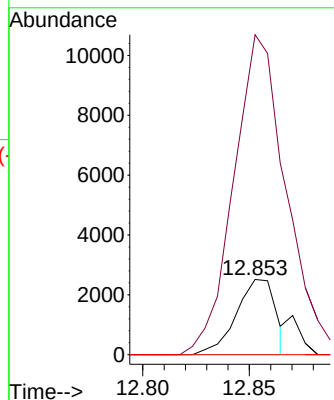

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.800 min Scan# 2014
Delta R.T. -0.000 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08

Tgt Ion:152 Resp: 250250
Ion Ratio Lower Upper
152 100
115 61.3 32.3 96.8
150 154.1 0.0 355.8


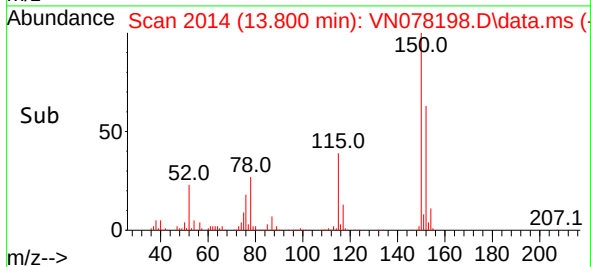
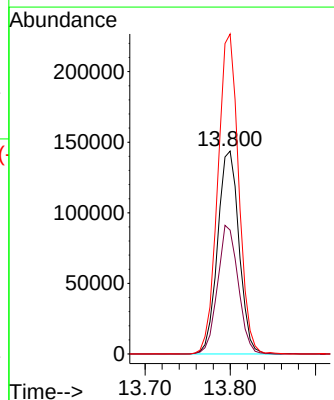
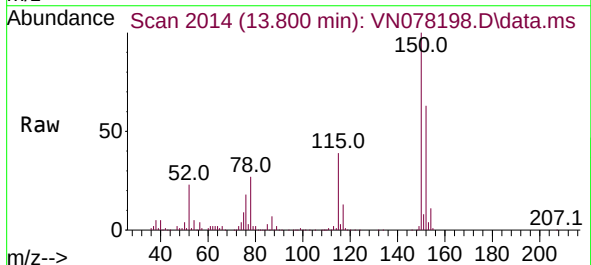


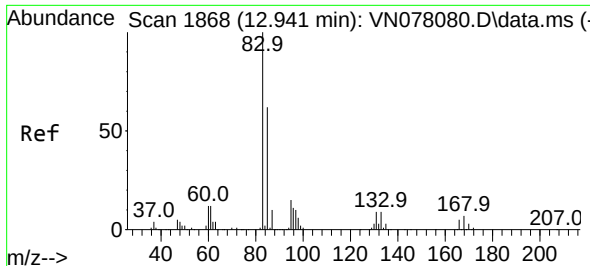

#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.935 min Scan# 1867
Delta R.T. -0.006 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08




Instrument : MSVOA_N
ClientSampleId : GWOW-BR-05-75-87-061323


Tgt Ion: 83 Resp: 114
Ion Ratio Lower Upper
83 100
131 0.0 5.0 15.0#
85 0.0 31.9 95.7#

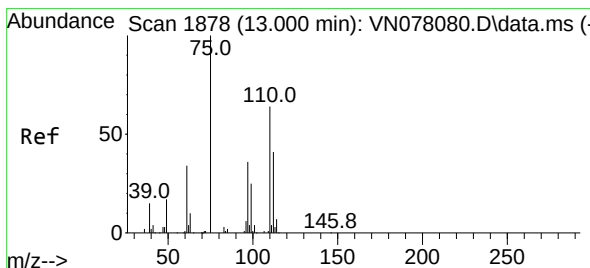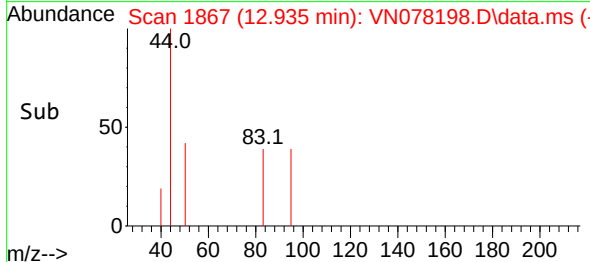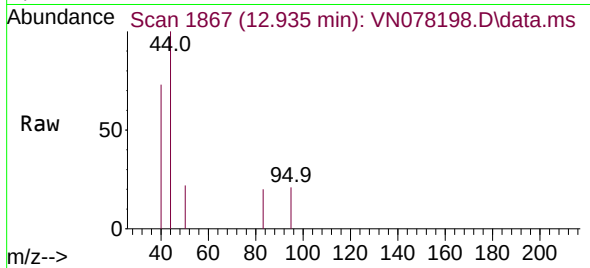

#76
1,2,3-Trichloropropane
Concen: 30.526 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.147 min
Lab File: VN078198.D
Acq: 14 Jun 2023 12:08

Tgt Ion: 75 Resp: 180590
Ion Ratio Lower Upper
75 100
77 1.4 84.5 253.5#


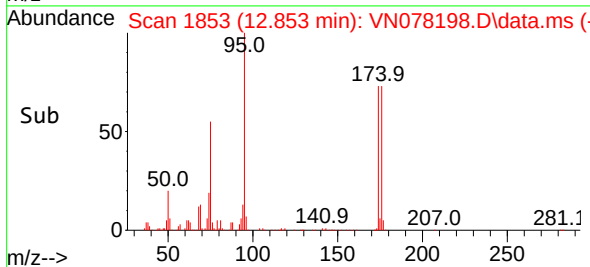

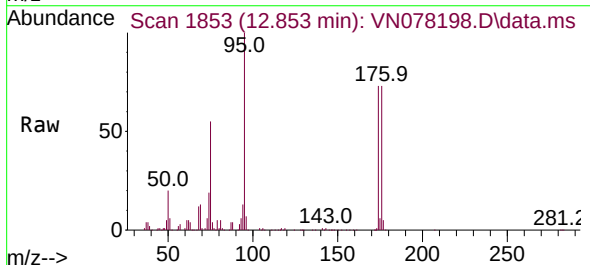


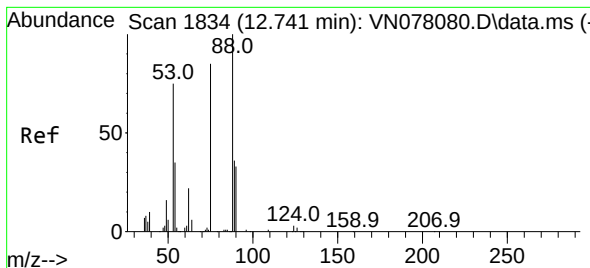

#81
 trans-1,4-Dichloro-2-butene
 Concen: 93.785 ug/l
 RT: 12.853 min Scan# 1853
 Delta R.T. 0.112 min
 Lab File: VN078198.D
 Acq: 14 Jun 2023 12:08




Instrument :
 MSVOA_N
 ClientSampleId :
 GWOW-BR-05-75-87-061323


Tgt Ion: 75 Resp: 180590
 Ion Ratio Lower Upper
 75 100
 53 0.0 67.4 101.2#
 89 0.0 38.8 58.2#

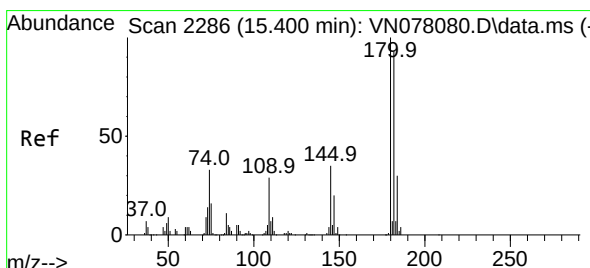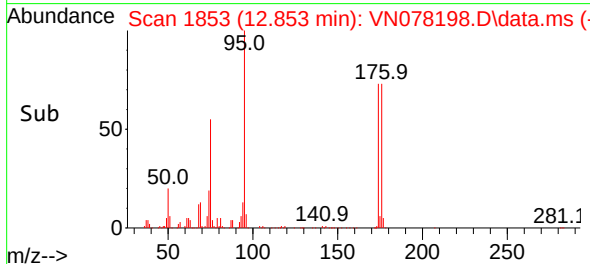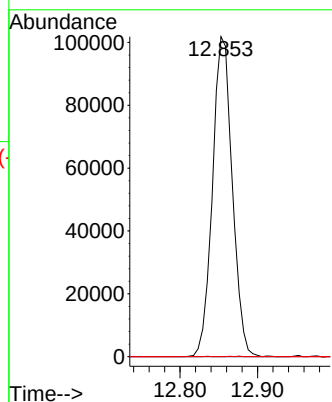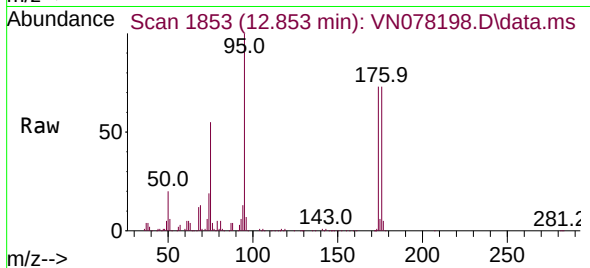

#93
 1,2,4-Trichlorobenzene
 Concen: 0.212 ug/l
 RT: 15.394 min Scan# 2285
 Delta R.T. -0.006 min
 Lab File: VN078198.D
 Acq: 14 Jun 2023 12:08

Tgt Ion:180 Resp: 687
 Ion Ratio Lower Upper
 180 100
 182 37.0 46.1 138.2#
 145 16.3 16.6 49.8#

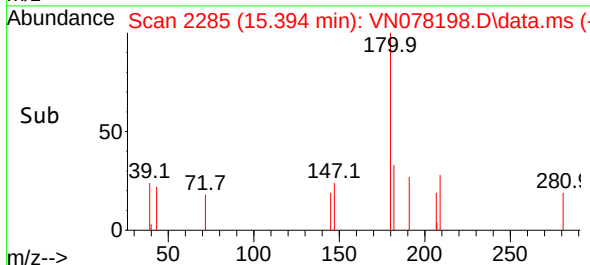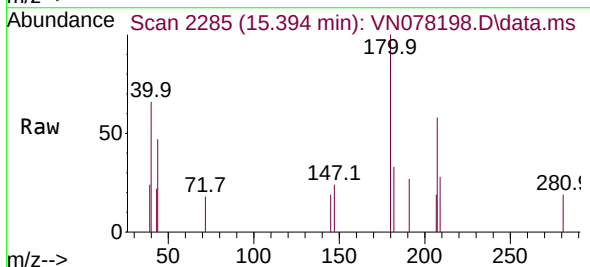

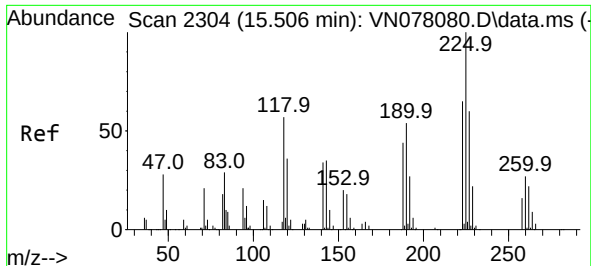

#94

Hexachlorobutadiene

Concen: Below Cal

RT: 15.511 min Scan# 21

Delta R.T. 0.005 min

Lab File: VN078198.D


Acq: 14 Jun 2023 12:08

Instrument :

MSVOA_N

ClientSampleId :

GWOW-BR-05-75-87-061323

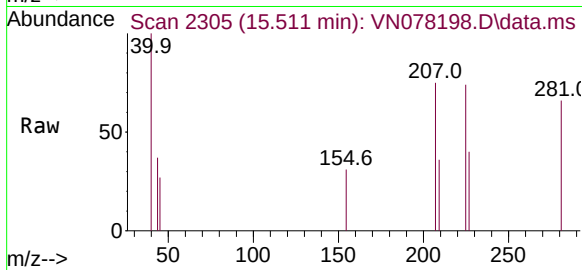

Tgt Ion:225 Resp: 603

Ion Ratio Lower Upper

225 100

223 13.8 31.3 93.8#

227 59.2 31.9 95.9

