

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061423\
 Data File : VN078217.D
 Acq On : 14 Jun 2023 19:45
 Operator : JC\MD
 Sample : 03231-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 FSND-MW-EVAL-1D-06132023

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
 Title : SW846 8260

Signal : TIC: VN078217.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.089	18	23	34	rVB2	115157	171379	2.00%	0.795%
2	2.489	84	91	97	rBV	52078	96033	1.12%	0.445%
3	8.177	1047	1058	1062	rBV	391173	919348	10.73%	4.263%
4	8.229	1062	1067	1082	rVB	609494	1397318	16.30%	6.480%
5	8.588	1117	1128	1139	rBV	389164	874557	10.20%	4.056%
6	9.106	1206	1216	1228	rBV	922438	1918464	22.38%	8.896%
7	9.359	1250	1259	1278	rBV	4226659	8572002	100.00%	39.751%
8	10.571	1457	1465	1478	rBV	1326589	2514028	29.33%	11.658%
9	11.870	1677	1686	1702	rBV	1237744	2204494	25.72%	10.223%
10	12.853	1846	1853	1864	rBV	845224	1473929	17.19%	6.835%
11	13.800	2006	2014	2024	rBV	800717	1422706	16.60%	6.598%




Sum of corrected areas: 21564258

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061423\
Data File : VN078217.D
Acq On : 14 Jun 2023 19:45
Operator : JC\MD
Sample : 03231-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FSND-MW-EVAL-1D-06132023

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

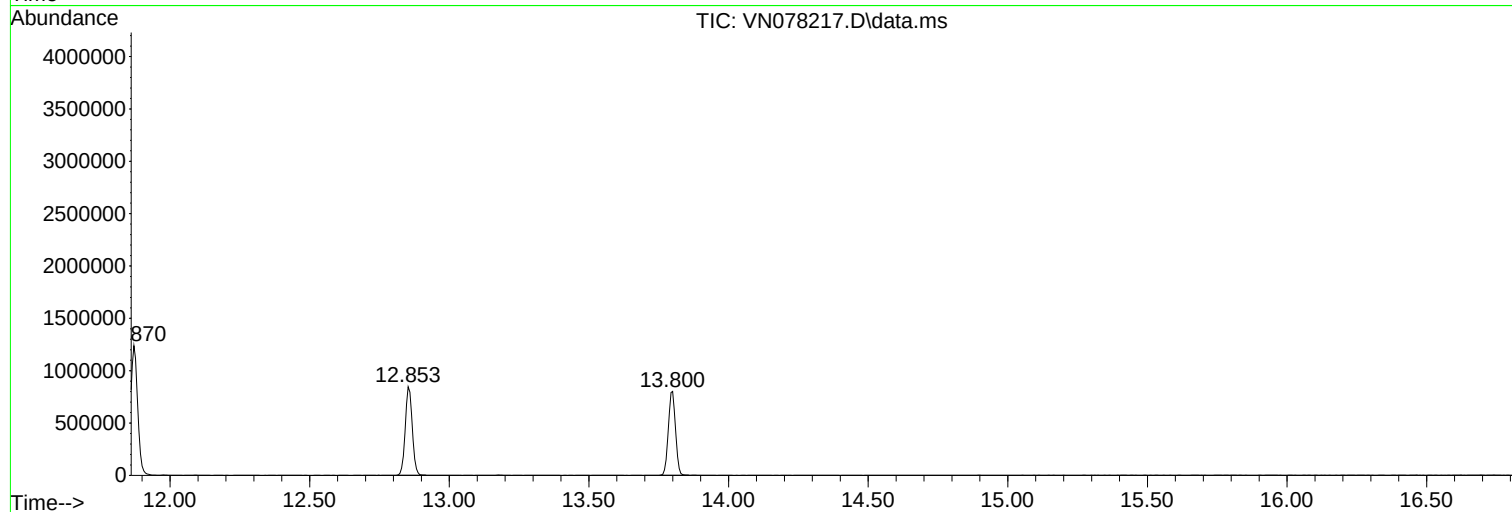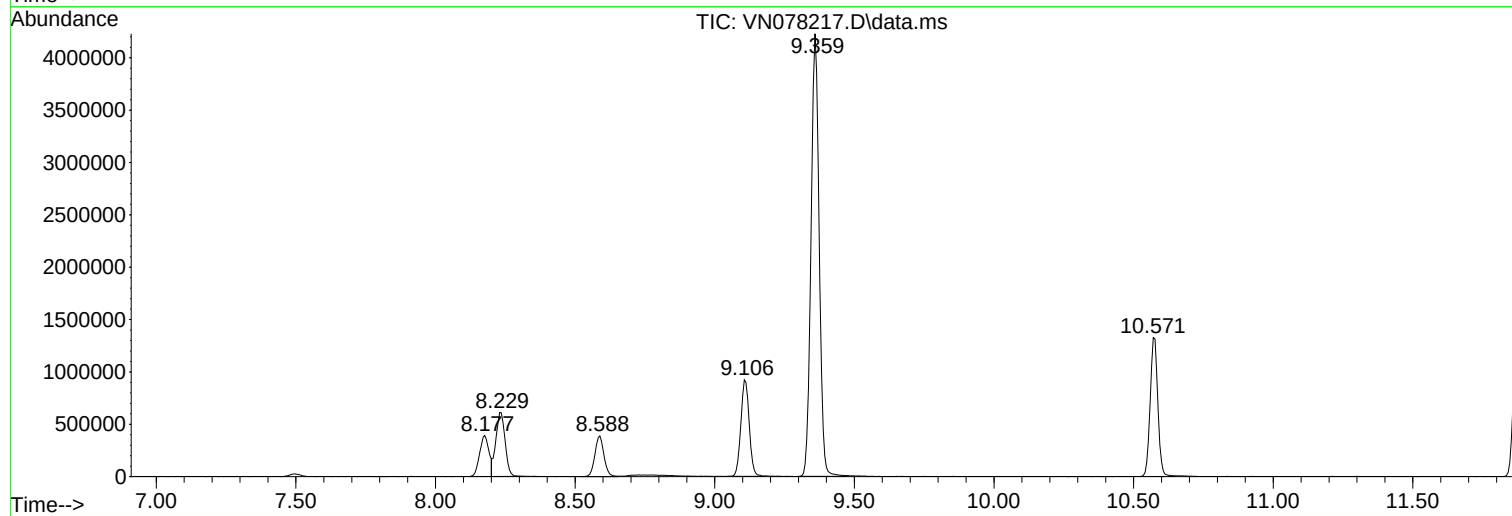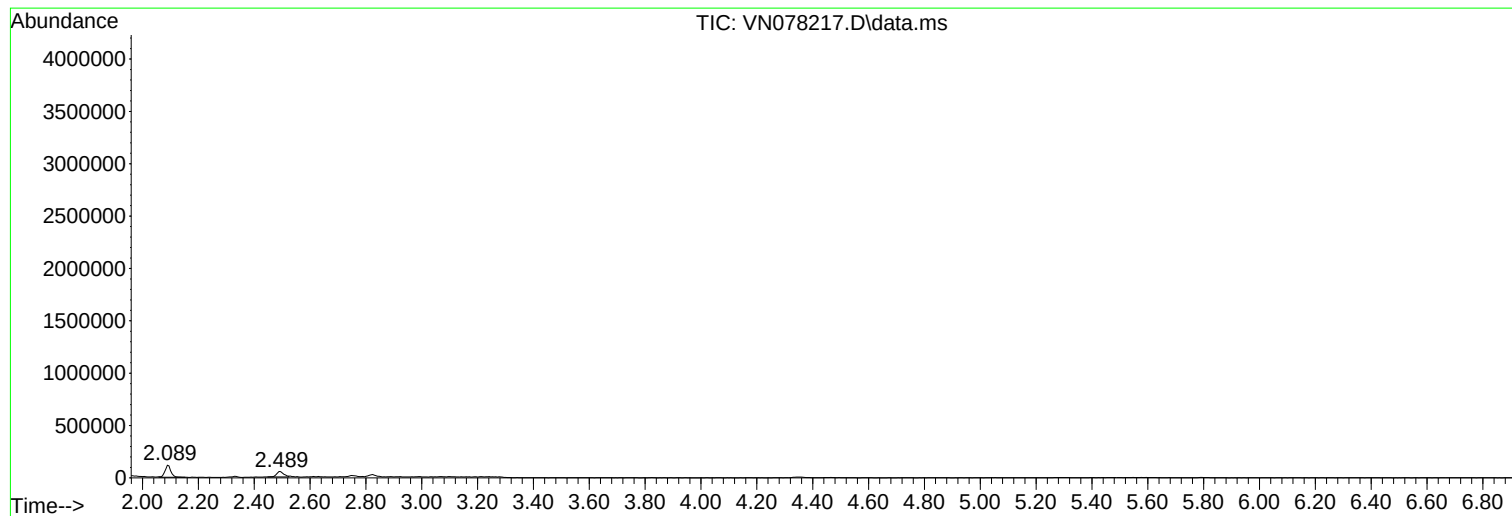

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061423\
Data File : VN078217.D
Acq On : 14 Jun 2023 19:45
Operator : JC\MD
Sample : 03231-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FSND-MW-EVAL-1D-06132023










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.089	6.13 ug/l	171379	Pentafluorobenzene	8.235

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propene	42	C3H6	000115-07-1	74
2			Cyclopropane	42	C3H6	000075-19-4	40
3			2-Oxetanone, 4-methyl-	86	C4H6O2	003068-88-0	4
4			Cyclopropene	40	C3H4	002781-85-3	2
5			1-Hexanamine	101	C6H15N	000111-26-2	2

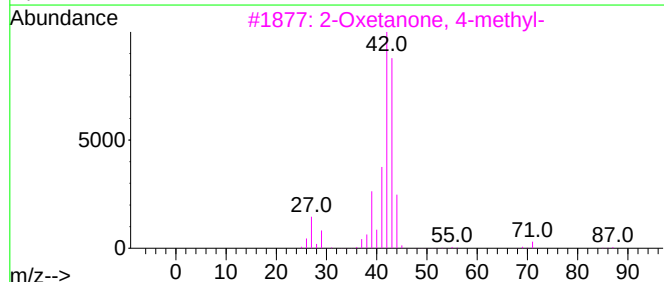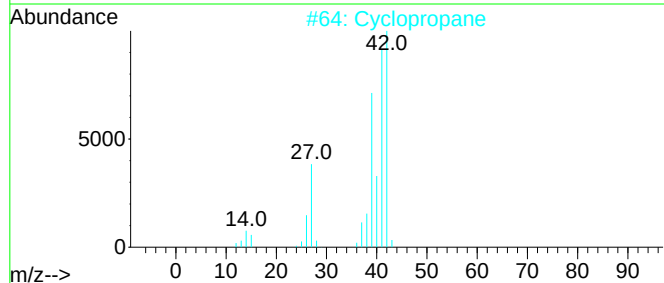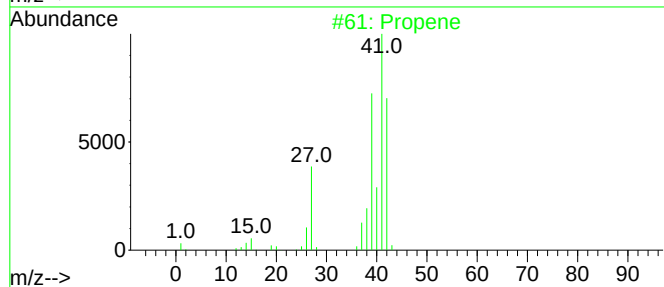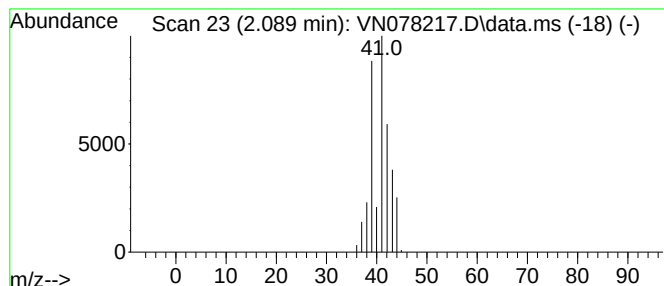

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061423\
Data File : VN078217.D
Acq On : 14 Jun 2023 19:45
Operator : JC\MD
Sample : 03231-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FSND-MW-EVAL-1D-06132023

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propene	2.089	6.1	ug/l	171379	1	8.235	1397320	50.0