
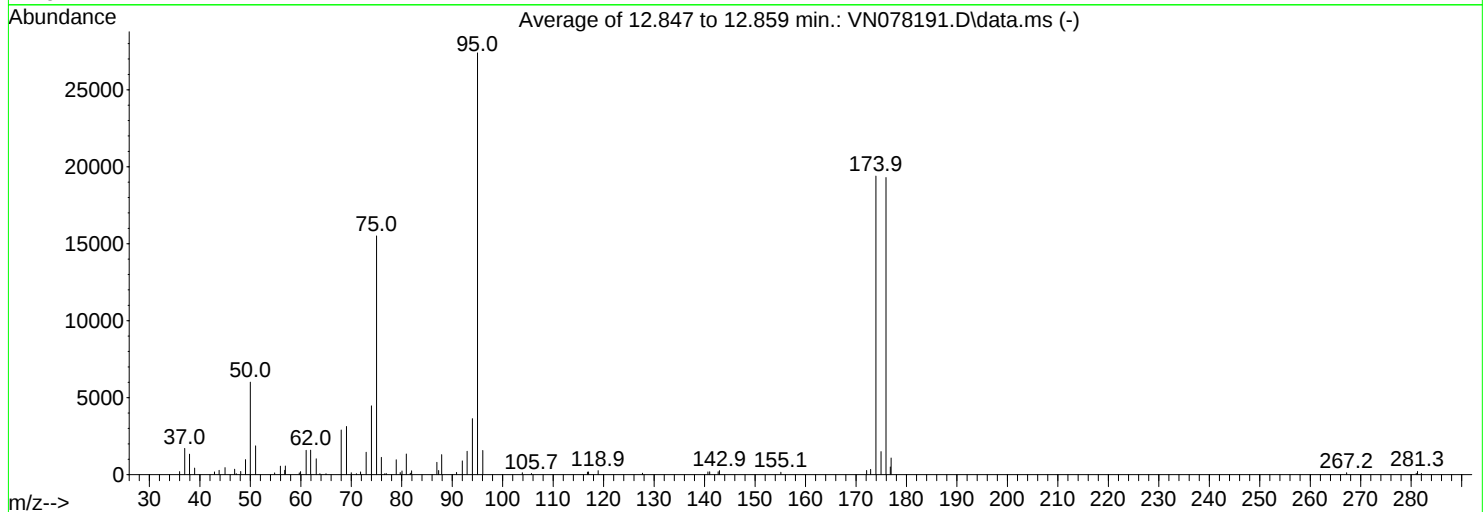


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061423\
Data File : VN078191.D
Acq On : 14 Jun 2023 08:44
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
Title : SW846 8260
Last Update : Wed Jun 07 05:05:00 2023

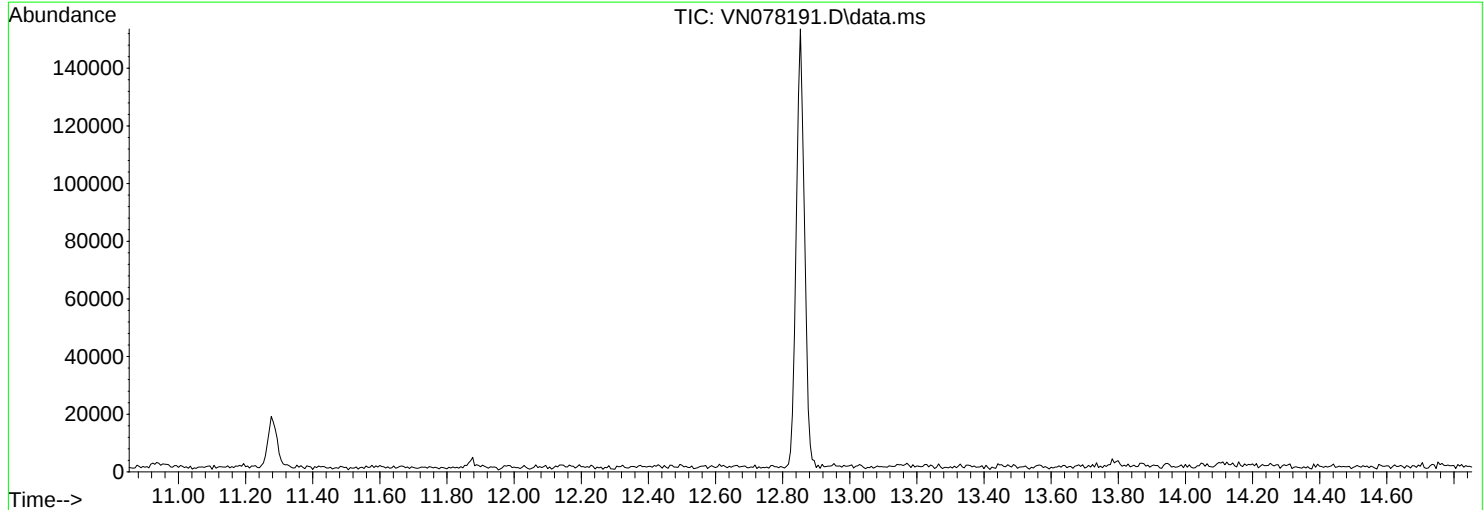

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.9	6009	PASS
75	95	30	60	56.6	15511	PASS
95	95	100	100	100.0	27400	PASS
96	95	5	9	5.7	1565	PASS
173	174	0.00	2	1.8	348	PASS
174	95	50	100	70.8	19400	PASS
175	174	5	9	7.7	1495	PASS
176	174	95	101	99.5	19301	PASS
177	176	5	9	5.6	1085	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	195	50.00	6009	63.80	65	76.60	51
37.00	1702	51.05	1867	65.00	60	76.90	79
37.95	1331	54.80	118	68.00	2896	78.90	96
38.95	424	55.95	547	69.05	3129	79.70	13
42.90	174	56.80	280	70.00	129	80.05	237
43.80	281	56.95	561	71.00	58	80.90	1346
45.00	460	59.70	110	71.85	173	81.70	94
46.90	354	59.95	195	72.95	1460	81.95	248
47.20	60	61.05	1582	74.00	4470	86.95	804
48.10	204	61.95	1590	75.00	15511	87.30	272
49.05	973	63.05	1033	75.95	1124	87.90	1296

Average of 12.847 to 12.859 min.: VN078191.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.85	150	127.70	94	176.80	504		
92.00	889	140.65	177	176.95	1085		
92.95	1523	141.00	190	267.20	120		
94.00	3640	142.70	184	281.00	79		
95.00	27400	142.95	260	281.25	211		
96.05	1565	155.10	154	282.00	77		
103.90	124	172.10	267				
105.70	71	172.90	348				
116.80	165	173.95	19400				
117.00	172	174.95	1495				
118.90	258	175.95	19301				

Instrument :
MSVOA_N
ClientSampleId :
BFB