

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061424\
 Data File : VN082579.D
 Acq On : 14 Jun 2024 13:37
 Operator : JC\MD
 Sample : P2891-05
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BP-VPB-196-EB-20240610

Quant Time: Jun 14 23:45:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 16 05:21:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	158056	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	294464	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	282992	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	119140	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	132784	53.204	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	106.400%
35) Dibromofluoromethane	8.171	113	95656	52.808	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	105.620%
50) Toluene-d8	10.571	98	349762	50.363	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	100.720%
62) 4-Bromofluorobenzene	12.853	95	115228	46.486	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	=	92.980%
Target Compounds						Qvalue
16) Acetone	4.436	43	7971	7.786	ug/l #	87
25) 2-Butanone	7.494	43	7705	4.964	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061424\
Data File : VN082579.D
Acq On : 14 Jun 2024 13:37
Operator : JC\MD
Sample : P2891-05
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-196-EB-20240610

Quant Time: Jun 14 23:45:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Quant Title : SW846 8260
QLast Update : Thu May 16 05:21:06 2024
Response via : Initial Calibration




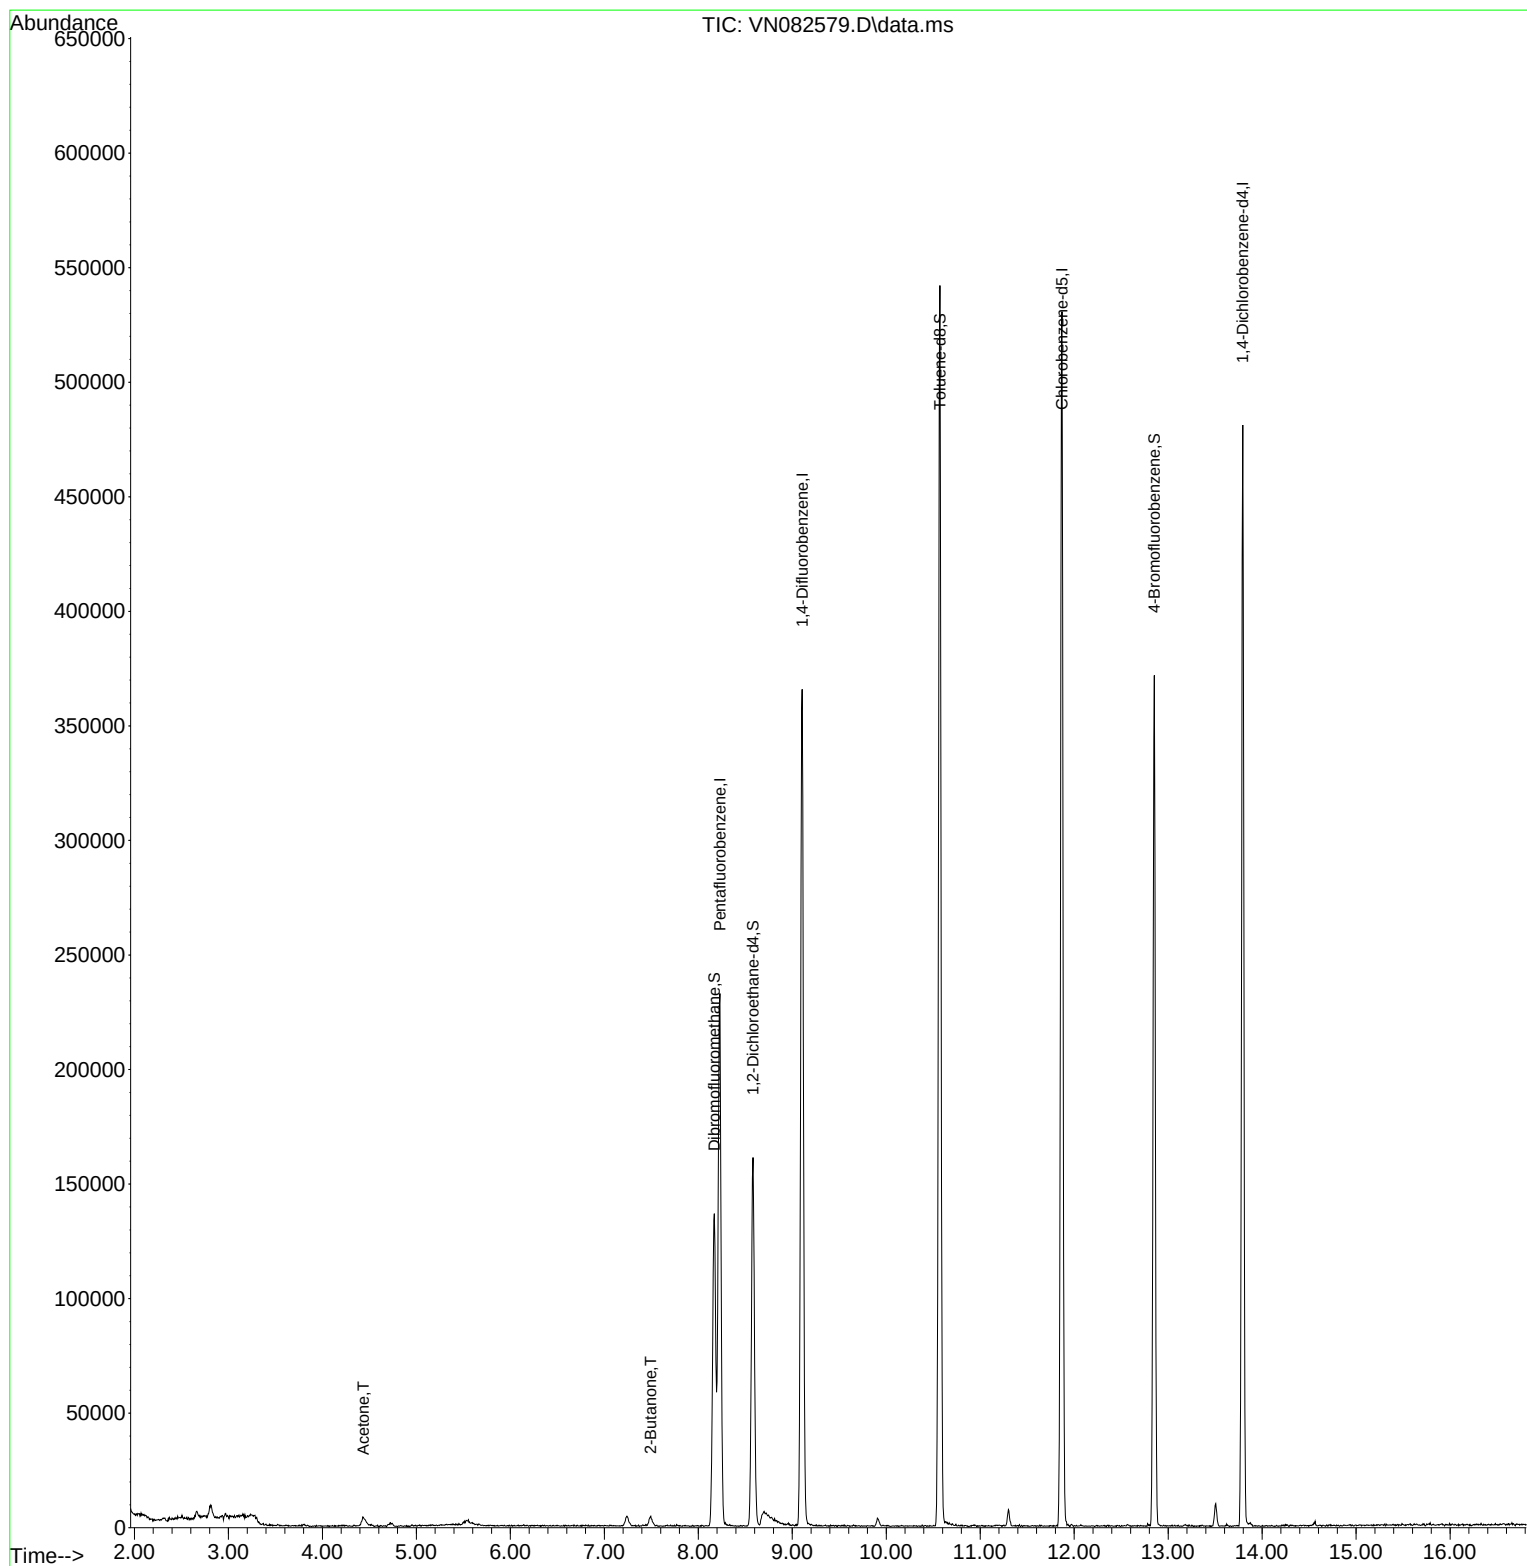


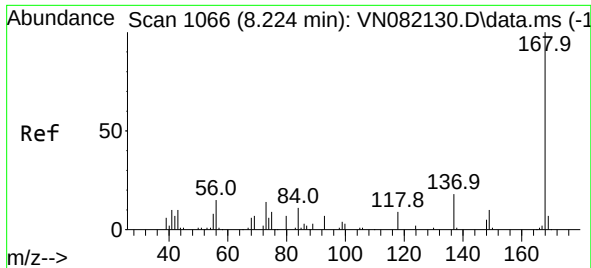

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VN082579.D
Acq: 14 Jun 2024 13:37




Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-196-EB-20240610


Tgt Ion:168 Resp: 158056
Ion Ratio Lower Upper
168 100
99 60.0 48.2 72.4

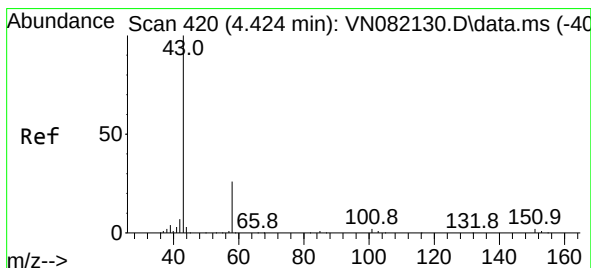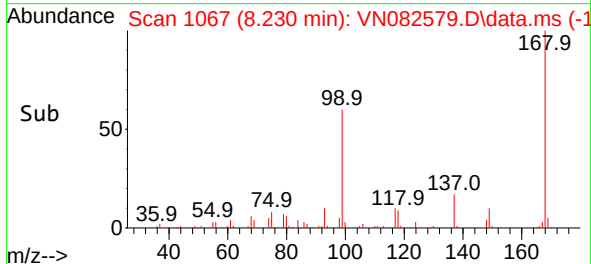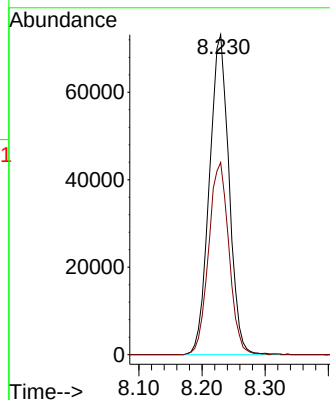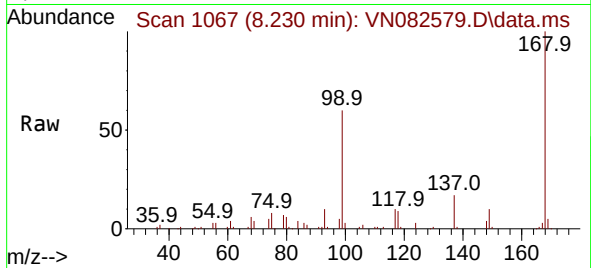

#16
Acetone
Concen: 7.786 ug/l
RT: 4.436 min Scan# 422
Delta R.T. 0.012 min
Lab File: VN082579.D
Acq: 14 Jun 2024 13:37

Tgt Ion: 43 Resp: 7971
Ion Ratio Lower Upper
43 100
58 24.1 25.2 37.8#


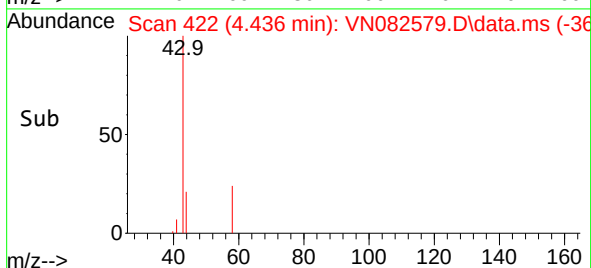
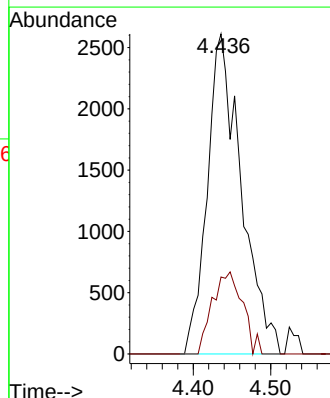
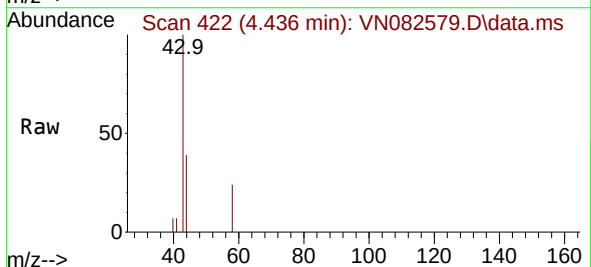


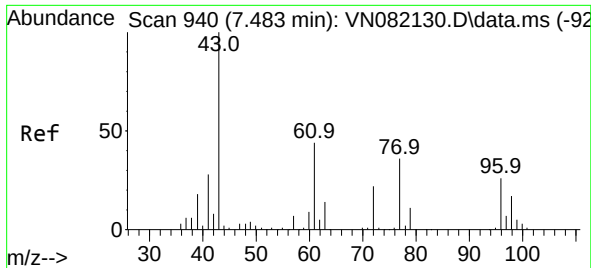

#25
2-Butanone
Concen: 4.964 ug/l
RT: 7.494 min Scan# 940
Delta R.T. 0.012 min
Lab File: VN082579.D
Acq: 14 Jun 2024 13:37




Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-196-EB-20240610


Tgt Ion: 43 Resp: 7705
Ion Ratio Lower Upper
43 100
72 14.6 25.3 37.9#

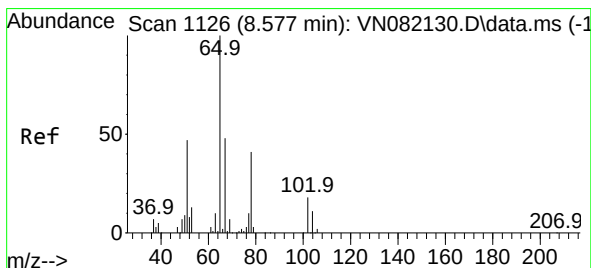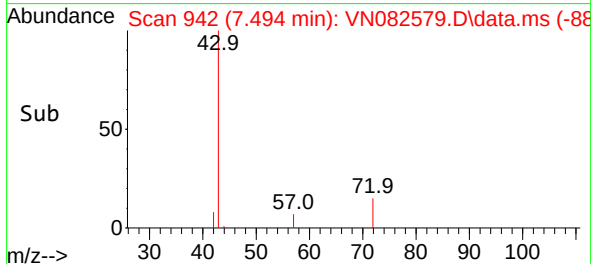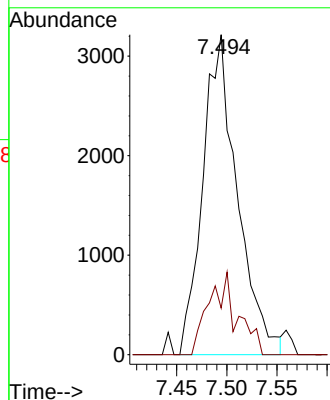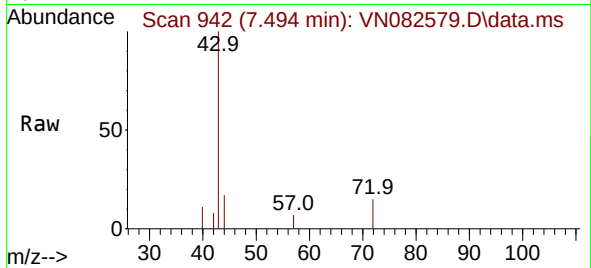

#33
1,2-Dichloroethane-d4
Concen: 53.204 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. 0.006 min
Lab File: VN082579.D
Acq: 14 Jun 2024 13:37

Tgt Ion: 65 Resp: 132784
Ion Ratio Lower Upper
65 100
67 50.1 0.0 103.0

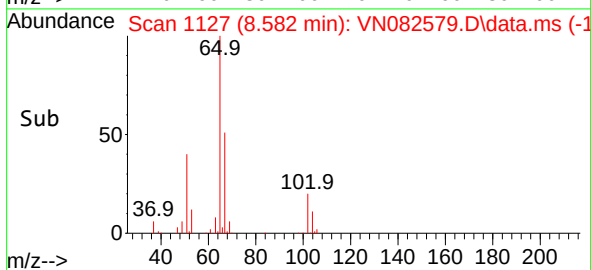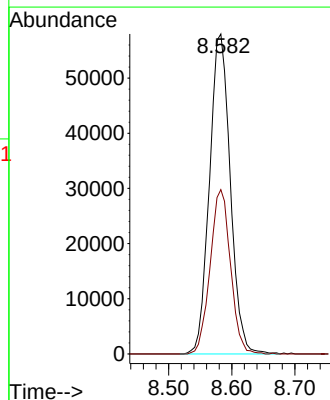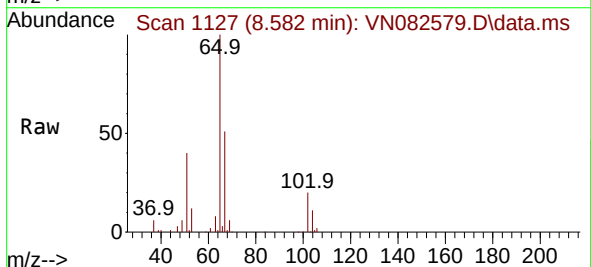

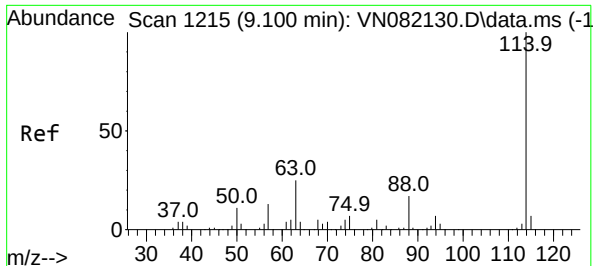

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 11

Delta R.T. 0.006 min

Lab File: VN082579.D

Acq: 14 Jun 2024 13:37

Instrument :

MSVOA_N

ClientSampleId :

BP-VPB-196-EB-20240610





Tgt Ion:114 Resp: 294464

Ion Ratio Lower Upper

114 100

63 23.8 0.0 41.0

88 15.8 0.0 31.4

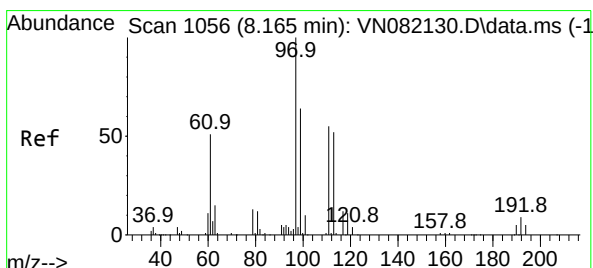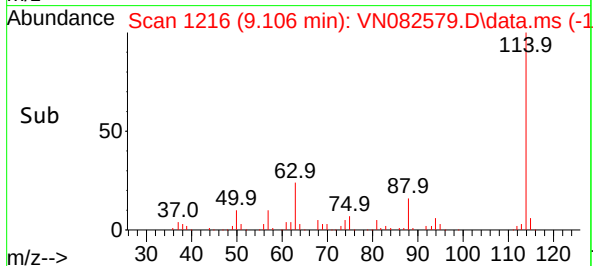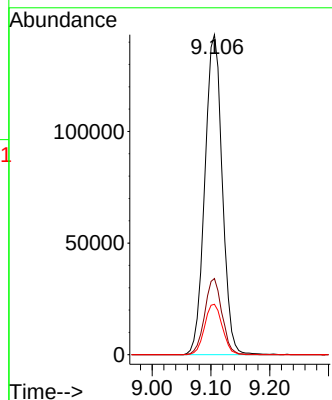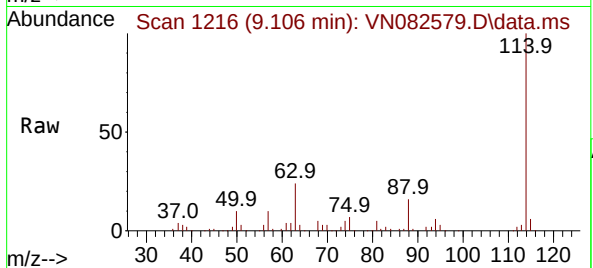

#35

Dibromofluoromethane

Concen: 52.808 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. 0.006 min

Lab File: VN082579.D

Acq: 14 Jun 2024 13:37




Tgt Ion:113 Resp: 95656


Ion Ratio Lower Upper

113 100

111 103.7 83.4 125.2

192 19.1 14.0 21.0


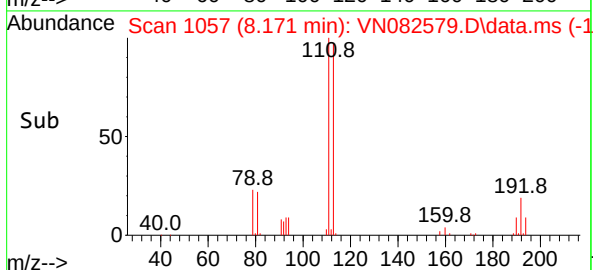
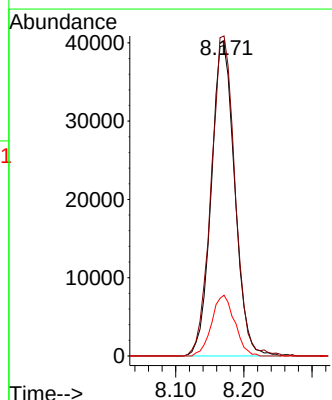
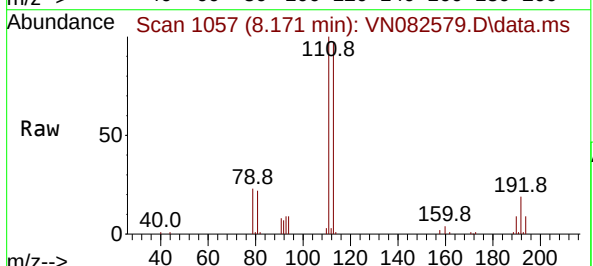


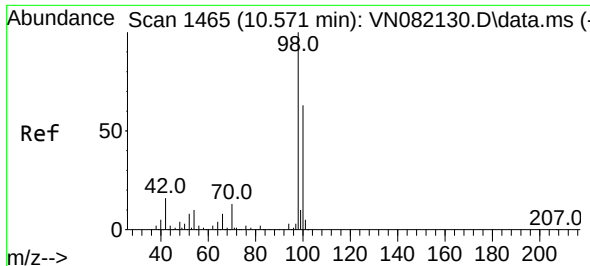

#50
Toluene-d8
Concen: 50.363 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN082579.D
Acq: 14 Jun 2024 13:37




Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-196-EB-20240610


Tgt Ion: 98 Resp: 349762
Ion Ratio Lower Upper
98 100
100 63.8 51.8 77.6

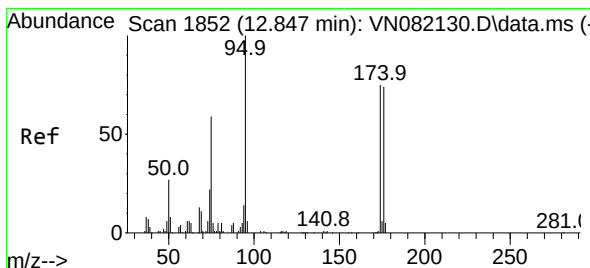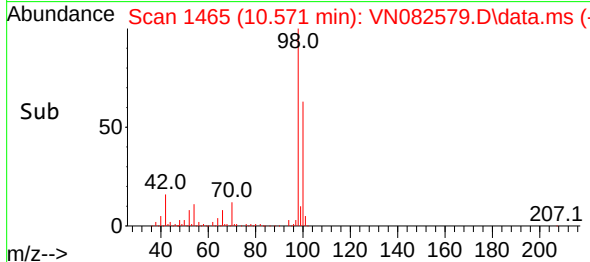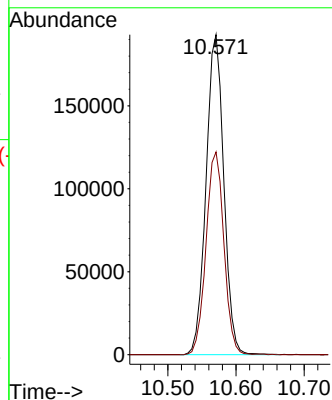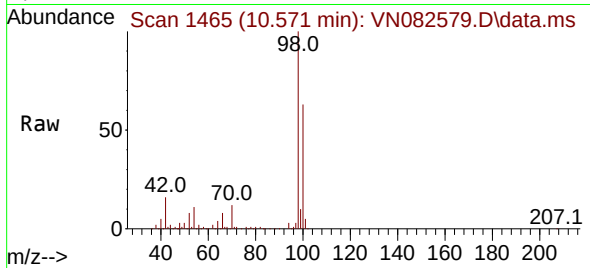

#62
4-Bromofluorobenzene
Concen: 46.486 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN082579.D
Acq: 14 Jun 2024 13:37

Tgt Ion: 95 Resp: 115228
Ion Ratio Lower Upper
95 100
174 77.7 0.0 160.6
176 75.7 0.0 152.8


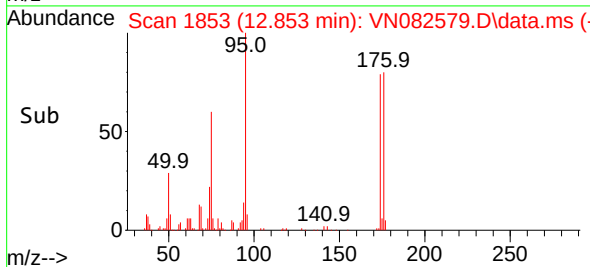
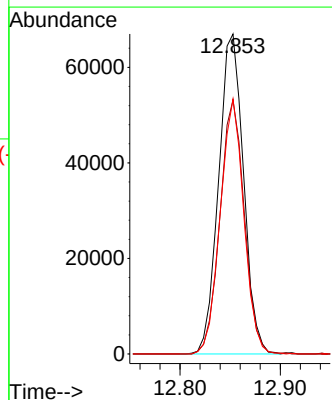
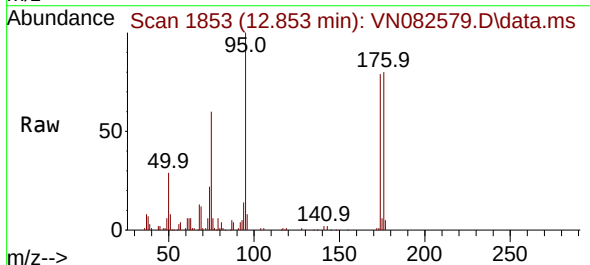


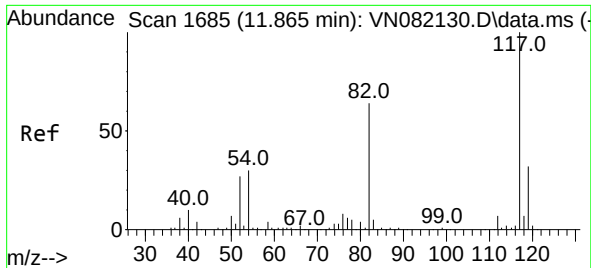

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN082579.D
Acq: 14 Jun 2024 13:37

Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-196-EB-20240610

Tgt Ion:117 Resp: 282992
Ion Ratio Lower Upper
117 100
82 61.3 44.6 66.8
119 32.6 25.9 38.9

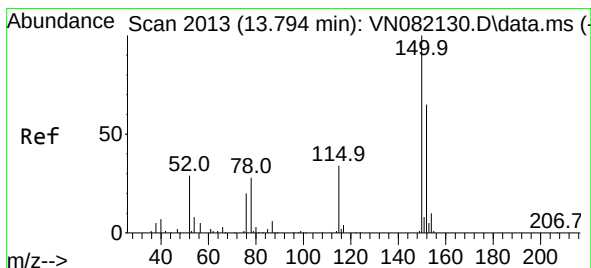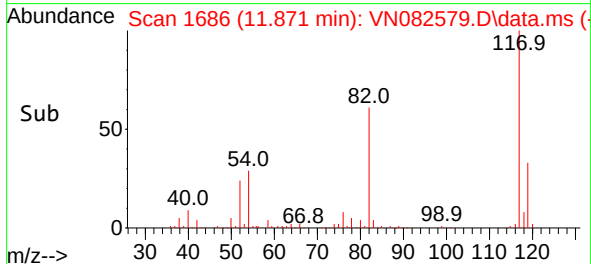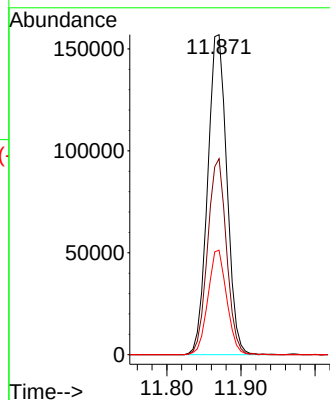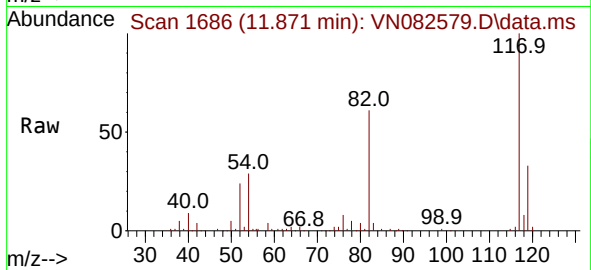

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN082579.D
Acq: 14 Jun 2024 13:37

Tgt Ion:152 Resp: 119140
Ion Ratio Lower Upper
152 100
115 60.2 30.4 91.3
150 160.0 0.0 353.2

