
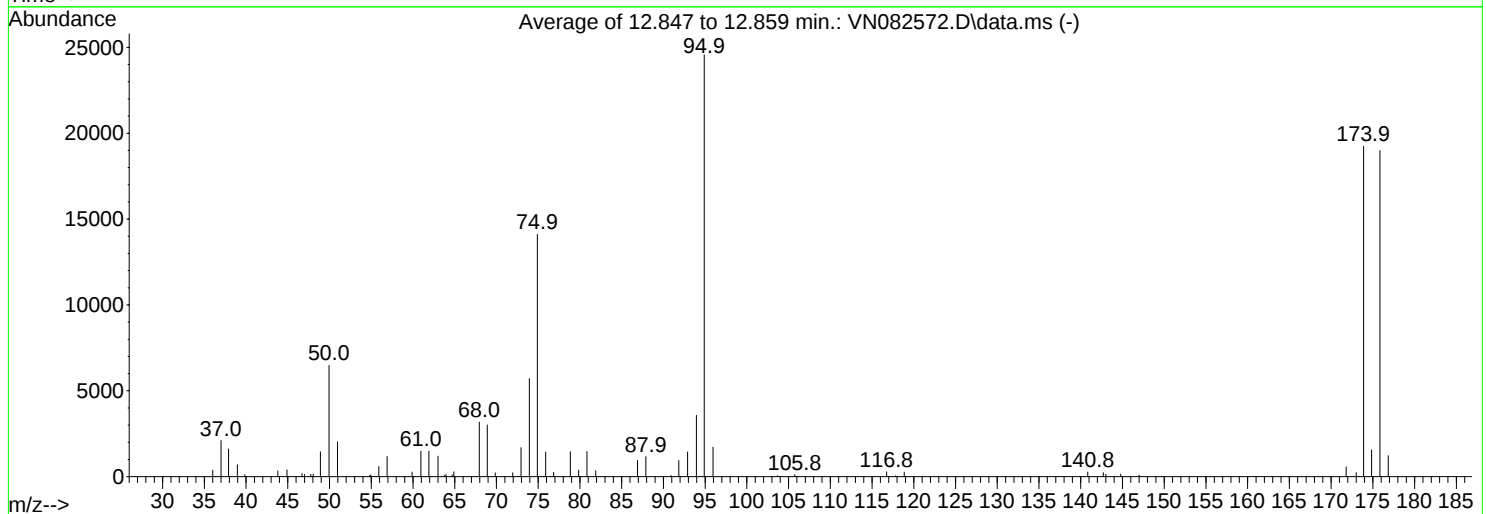


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061424\
Data File : VN082572.D
Acq On : 14 Jun 2024 08:37
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

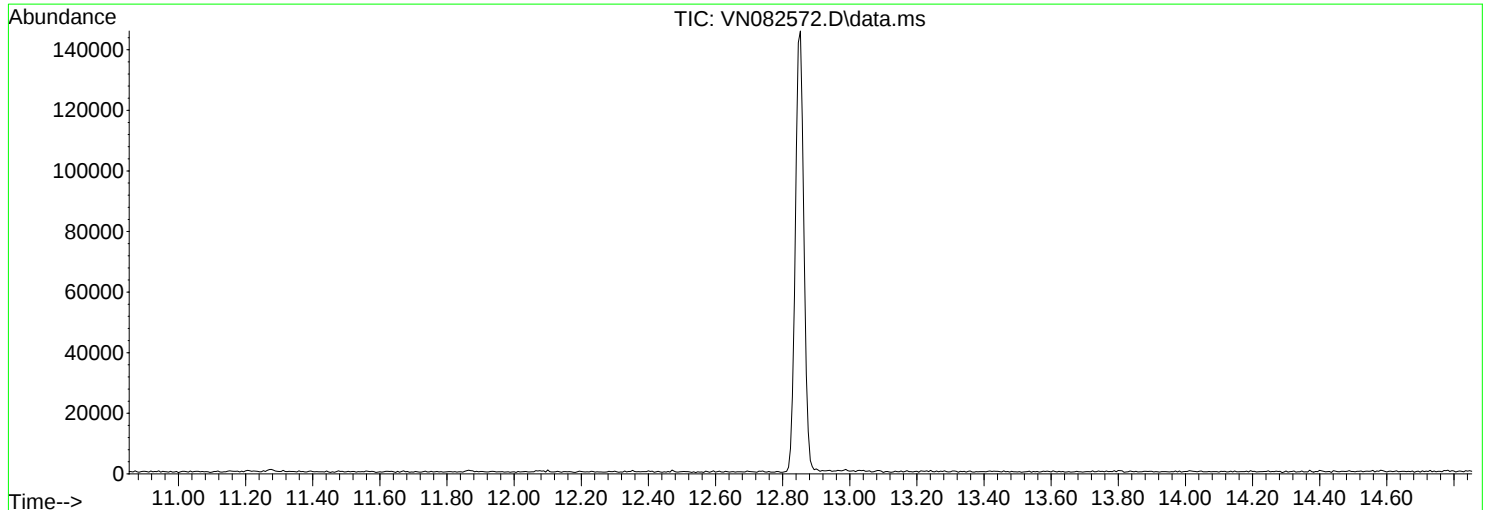

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.4	6481	PASS
75	95	30	60	57.4	14111	PASS
95	95	100	100	100.0	24565	PASS
96	95	5	9	7.0	1719	PASS
173	174	0.00	2	1.2	232	PASS
174	95	50	100	78.3	19237	PASS
175	174	5	9	8.1	1552	PASS
176	174	95	101	98.7	18989	PASS
177	176	5	9	6.4	1221	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	371	48.90	1449	63.80	86	75.90	1431
37.00	2107	49.95	6481	63.95	123	76.85	251
37.90	1609	50.95	2036	64.70	103	78.85	145
38.95	688	54.80	52	64.90	283	79.85	37
39.85	109	54.95	106	67.95	3177	80.85	1462
43.80	335	55.90	583	68.90	3014	81.90	347
44.90	393	56.90	1172	69.85	221	86.90	940
46.70	189	59.90	274	71.95	223	87.90	1161
47.00	131	60.95	1481	72.95	1684	90.90	65
47.75	143	61.90	1483	73.95	5709	91.85	937
48.05	149	63.00	1190	74.90	14111	92.90	1432

Average of 12.847 to 12.859 min.: VN082572.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.95	3566	144.80	152				
94.90	24565	147.00	93				
95.95	1719	171.80	573				
103.70	52	173.00	232				
105.75	121	173.90	19237				
116.75	278	174.85	1552				
117.80	50	175.85	18989				
118.85	260	176.85	1221				
140.85	269						
142.70	237						
143.00	130						

Instrument :

MSVOA_N

ClientSampleId :

BFB