

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061521\
 Data File : VN067340.D
 Acq On : 15 Jun 2021 12:34
 Operator : JC/MD
 Sample : M2262-09 .2PPB MDL
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MDL-WATER-03-QT2-2021DL

Manual Integrations
 APPROVED

MMDadoda
 6/16/2021 5:03:03 PM

Quant Time: Jun 16 04:30:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061421W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 16 04:29:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	452524	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	856441	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	773297	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	300421	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	444616	49.805	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	99.620%		
35) Dibromofluoromethane	8.024	113	284054	49.869	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	99.740%		
50) Toluene-d8	10.443	98	1084585	49.679	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	99.360%		
62) 4-Bromofluorobenzene	12.733	95	420583	46.681	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	93.360%		
Target Compounds						Qvalue
3) Chloromethane	2.301	50	1500	0.218	ug/l	98
5) Bromomethane	2.842	94	1153	0.404	ug/l #	24
6) Chloroethane	3.011	64	906m	0.219	ug/l	
11) Tert butyl alcohol	5.388	59	1006m	0.685	ug/l	
13) Acrolein	4.041	56	1727	1.883	ug/l #	54
14) Allyl chloride	4.827	41	3816m	0.317	ug/l	
15) Acrylonitrile	5.575	53	2231m	0.692	ug/l	
16) Acetone	4.291	43	5850	1.708	ug/l	97
18) Methyl Acetate	4.859	43	3848m	0.463	ug/l	
20) Methylene Chloride	5.095	84	3778m	0.530	ug/l	
23) Vinyl Acetate	6.447	43	13819m	0.678	ug/l	
25) 2-Butanone	7.348	43	5284m	1.079	ug/l	
29) Tetrahydrofuran	7.710	42	2258	0.732	ug/l #	78
31) Cyclohexane	8.083	56	16745	1.380	ug/l #	23
36) 1,1-Dichloropropene	8.225	75	2024	0.211	ug/l #	63
37) Ethyl Acetate	7.429	43	3068m	0.302	ug/l	
41) Methacrylonitrile	7.640	41	1604m	0.303	ug/l	
42) 1,2-Dichloroethane	8.536	62	2666	0.235	ug/l #	79
48) Methyl methacrylate	9.569	41	2283m	0.274	ug/l	
49) 1,4-Dioxane	9.579	88	307	2.694	ug/l #	49
51) 4-Methyl-2-Pentanone	10.333	43	7048	0.670	ug/l	96
58) 2-Chloroethyl Vinyl ether	10.043	63	2231	0.654	ug/l #	67
59) 2-Hexanone	11.092	43	6242	0.811	ug/l	95
68) m/p-Xylenes	11.950	106	3242	0.274	ug/l	98
88) 1,4-Dichlorobenzene	13.702	146	2470m	0.232	ug/l	
92) 1,2-Dibromo-3-Chloropr...	14.603	75	470	0.219	ug/l #	27
93) 1,2,4-Trichlorobenzene	15.268	180	1380	0.263	ug/l	96
95) Naphthalene	15.507	128	6249	0.391	ug/l #	87
96) 1,2,3-Trichlorobenzene	15.702	180	1582m	0.314	ug/l	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061521\
Data File : VN067340.D
Acq On : 15 Jun 2021 12:34
Operator : JC/MD
Sample : M2262-09 .2PPB MDL
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1


Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT2-2021DL

Manual Integrations
APPROVED


MMDadoda
6/16/2021 5:03:03 PM

Quant Time: Jun 16 04:30:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061421W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 16 04:29:50 2021
Response via : Initial Calibration


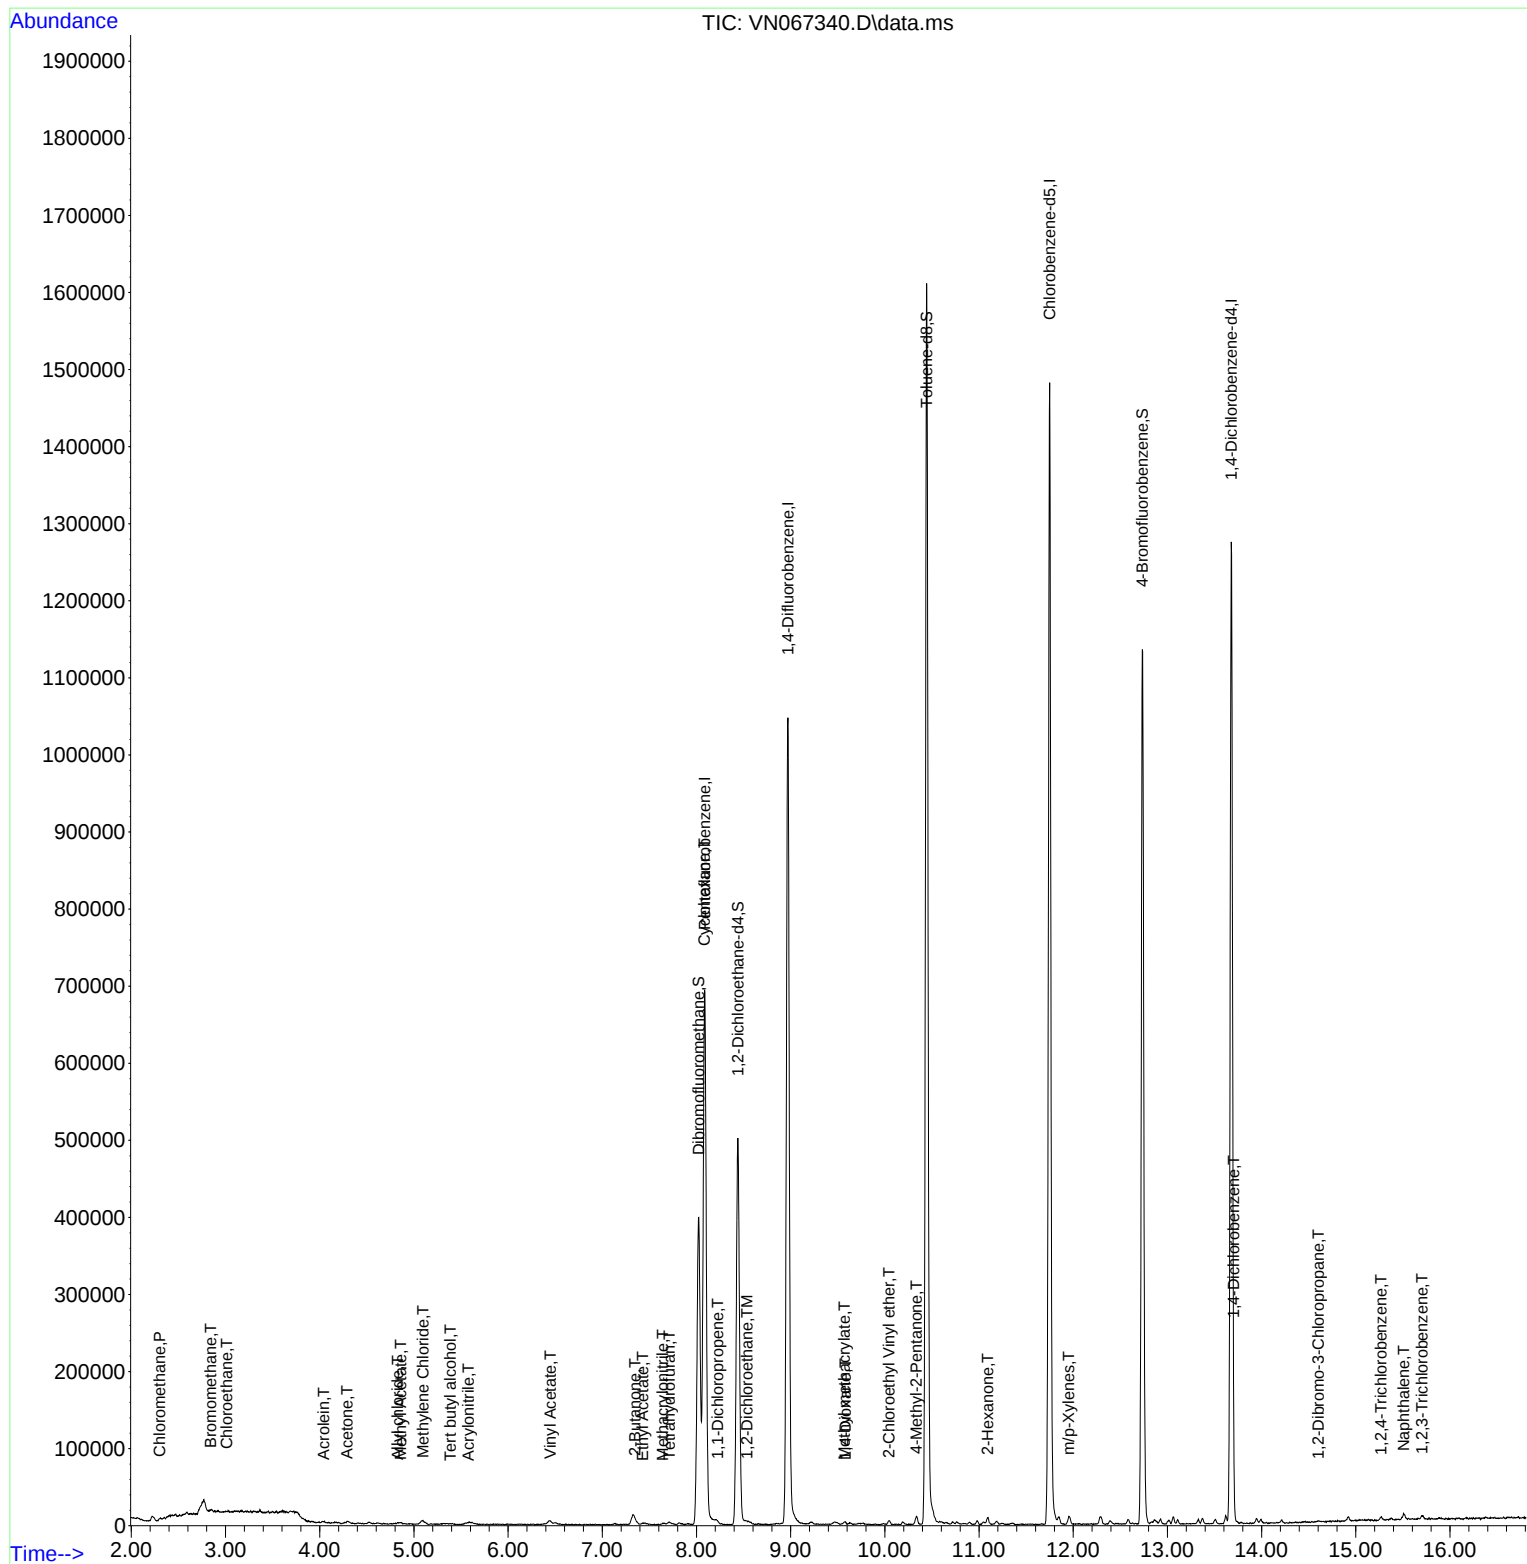




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.000 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34




Tgt Ion: 168 Resp: 452524
Ion Ratio Lower Upper
168 100
99 77.2 62.9 94.3

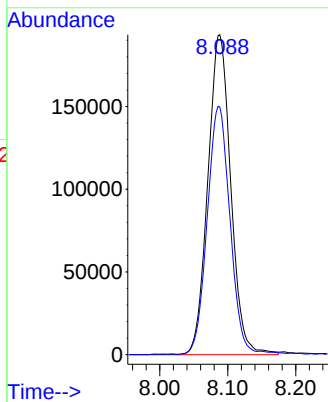


Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT2-2021DL

Manual Integrations
APPROVED



MMDadoda
6/16/2021 5:03:03 PM




#3
Chloromethane
Concen: 0.218 ug/l
RT: 2.301 min Scan# 116
Delta R.T. -0.000 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

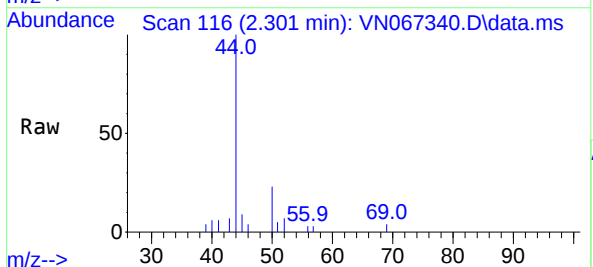

Tgt Ion: 50 Resp: 1500
Ion Ratio Lower Upper
50 100
52 30.9 25.6 38.4

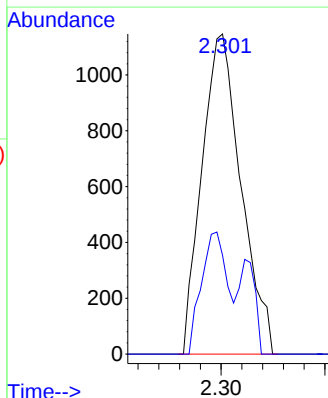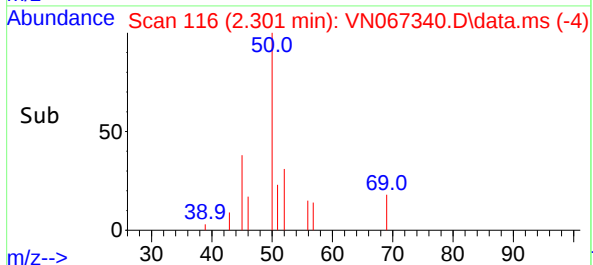







#5
Bromomethane
Concen: 0.404 ug/l
RT: 2.842 min Scan# 318
Delta R.T. 0.000 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

Tgt Ion: 94 Resp: 1153
Ion Ratio Lower Upper
94 100
96 19.3 73.7 110.5#

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT2-2021DL




Manual Integrations
APPROVED


MMDadoda
6/16/2021 5:03:03 PM

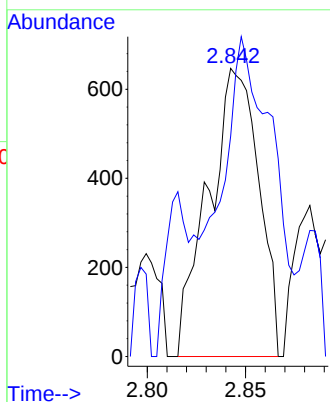

#6
Chloroethane
Concen: 0.219 ug/l m
RT: 3.011 min Scan# 381
Delta R.T. 0.000 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

Tgt Ion: 64 Resp: 906
Ion Ratio Lower Upper
64 100
66 63.9 24.7 37.1#

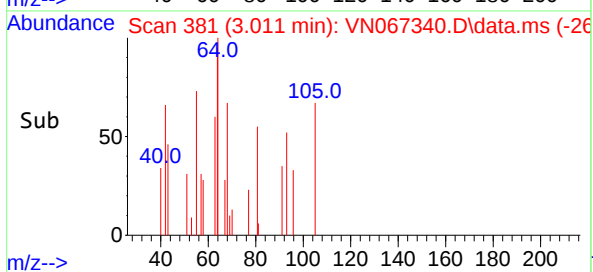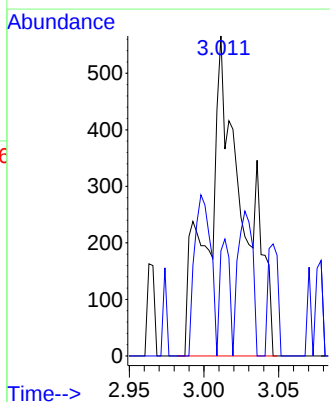



#11





Tert butyl alcohol
Concen: 0.685 ug/l m
RT: 5.388 min Scan# 1267
Delta R.T. -0.002 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

Tgt Ion: 59 Resp: 1006
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT2-2021DL

Manual Integrations
APPROVED




MMDadoda
6/16/2021 5:03:03 PM

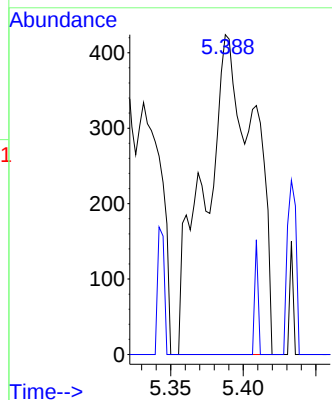


#13

Acrolein
Concen: 1.883 ug/l
RT: 4.041 min Scan# 765
Delta R.T. 0.003 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

Tgt Ion: 56 Resp: 1727
Ion Ratio Lower Upper
56 100
55 33.5 57.4 86.0#

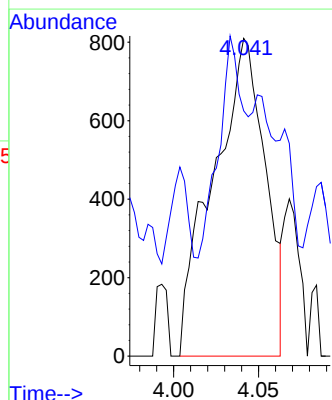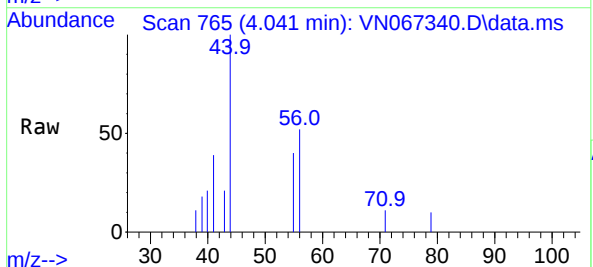



#14





Allyl chloride
Concen: 0.317 ug/l m
RT: 4.827 min Scan# 1058
Delta R.T. -0.008 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

Tgt Ion:	41	Resp:	3816
Ion	Ratio	Lower	Upper
41	100		
39	6.3	60.9	91.3#
76	2.6	24.3	36.5#

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT2-2021DL

Manual Integrations
APPROVED




MMDadoda
6/16/2021 5:03:03 PM

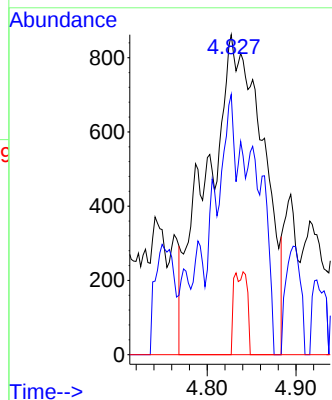


#15

Acrylonitrile
Concen: 0.692 ug/l m
RT: 5.575 min Scan# 1337
Delta R.T. 0.016 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34


Tgt Ion:	53	Resp:	2231
Ion	Ratio	Lower	Upper
53	100		
52	16.4	66.2	99.2#
51	7.9	30.2	45.4#

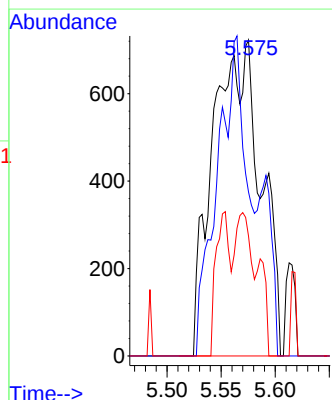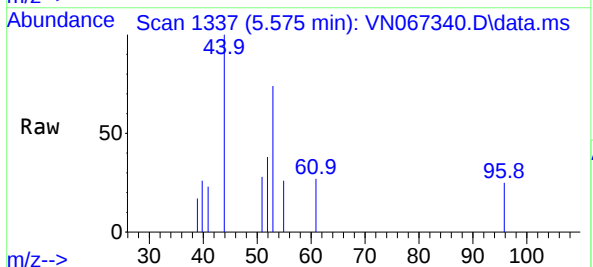

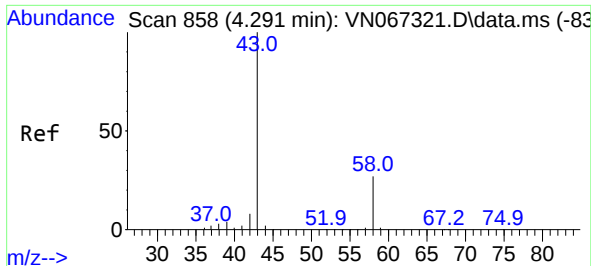

#16
Acetone
Concen: 1.708 ug/l
RT: 4.291 min Scan# 858
Delta R.T. -0.000 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34




Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT2-2021DL




Tgt Ion: 43 Resp: 5850
Ion Ratio Lower Upper
43 100
58 28.0 21.2 31.8

Manual Integrations
APPROVED



MMDadoda
6/16/2021 5:03:03 PM

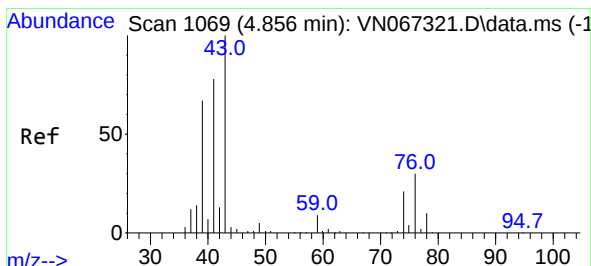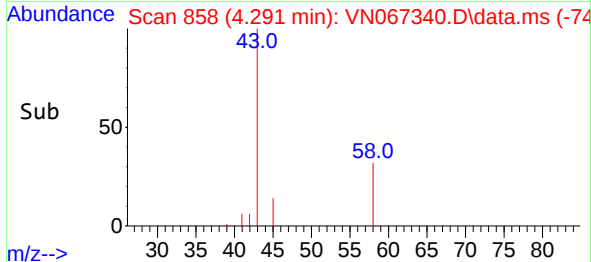


#18
Methyl Acetate
Concen: 0.463 ug/l m
RT: 4.859 min Scan# 1070
Delta R.T. 0.003 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

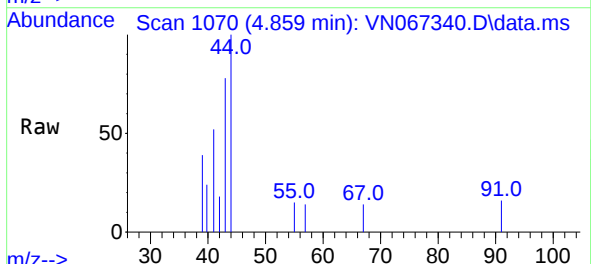


Tgt Ion: 43 Resp: 3848
Ion Ratio Lower Upper
43 100
74 4.7 17.4 26.0#

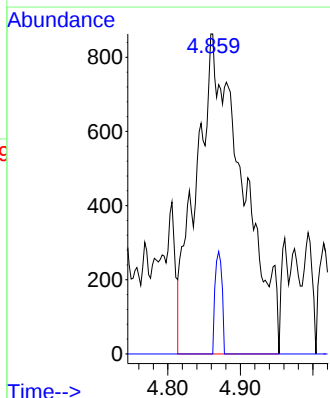



#20
Methylene Chloride
Concen: 0.530 ug/l m
RT: 5.095 min Scan# 1158
Delta R.T. 0.000 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT2-2021DL






Tgt Ion: 84 Resp: 3778


Ion	Ratio	Lower	Upper
84	100		
49	116.1	110.9	166.3
51	33.9	32.6	49.0
86	47.3	51.6	77.4#

Manual Integrations
APPROVED

MMDadoda
6/16/2021 5:03:03 PM

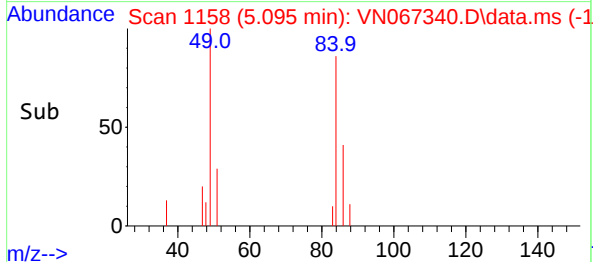
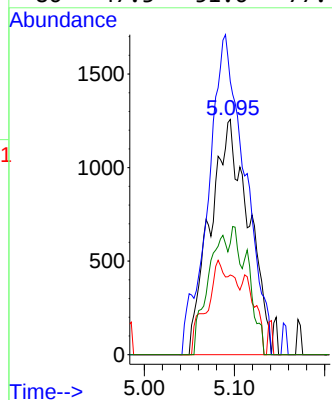



#23
Vinyl Acetate
Concen: 0.678 ug/l m
RT: 6.447 min Scan# 1662
Delta R.T. 0.011 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34



Tgt Ion: 43 Resp: 13819


Ion	Ratio	Lower	Upper
43	100		
86	8.1	7.3	10.9

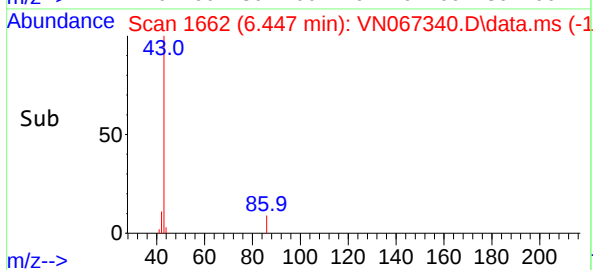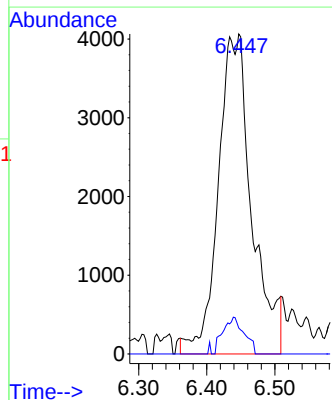



#25
2-Butanone
Concen: 1.079 ug/l m
RT: 7.348 min Scan# 1998
Delta R.T. 0.005 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34




Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT2-2021DL




Tgt Ion: 43 Resp: 5284
Ion Ratio Lower Upper
43 100
72 15.3 19.7 29.5#

Manual Integrations
APPROVED



MMDadoda
6/16/2021 5:03:03 PM

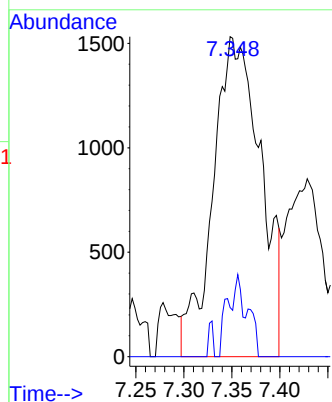


#29
Tetrahydrofuran
Concen: 0.732 ug/l
RT: 7.710 min Scan# 2133
Delta R.T. 0.021 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34




Tgt Ion: 42 Resp: 2258
Ion Ratio Lower Upper
42 100
72 17.4 32.8 49.2#
71 42.8 31.2 46.8

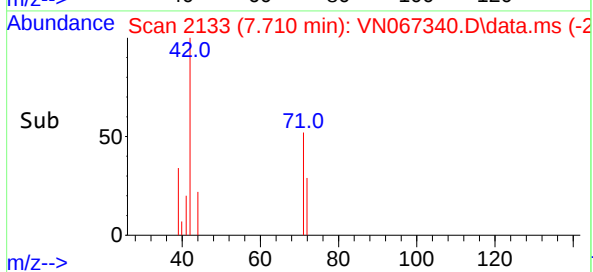
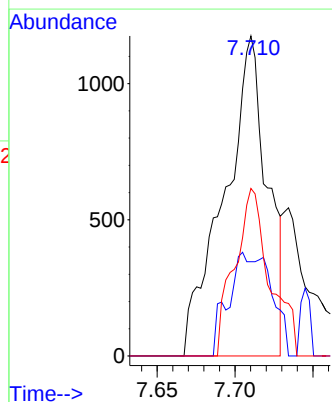




#31
Cyclohexane
Concen: 1.380 ug/l
RT: 8.083 min Scan# 2272
Delta R.T. -0.011 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34




Tgt Ion: 56 Resp: 16745
Ion Ratio Lower Upper
56 100
69 143.7 27.3 40.9#
84 106.3 64.9 97.3#

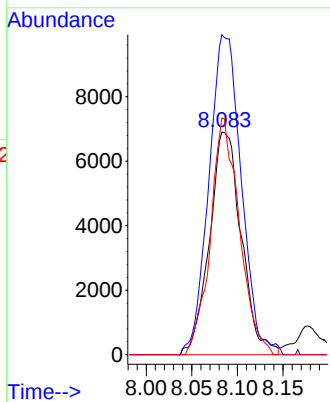


Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT2-2021DL

Manual Integrations
APPROVED



MMDadoda
6/16/2021 5:03:03 PM




#33
1,2-Dichloroethane-d4
Concen: 49.805 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

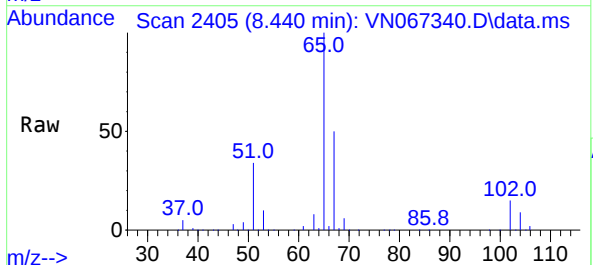

Tgt Ion: 65 Resp: 444616
Ion Ratio Lower Upper
65 100
67 49.8 0.0 98.6

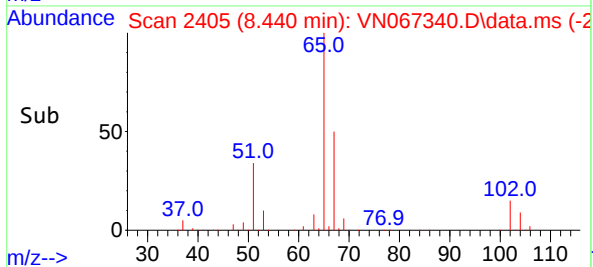

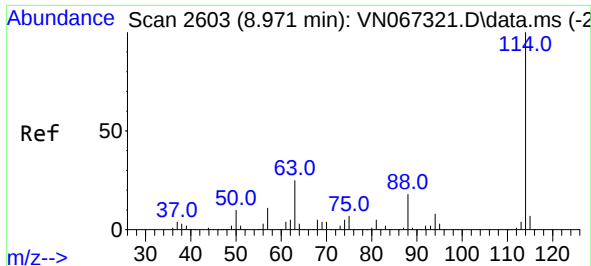





#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.000 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

Tgt Ion:	114	Resp:	856441
Ion Ratio	Lower	Upper	
114	100		
63	25.8	0.0	49.0
88	18.7	0.0	36.6

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT2-2021DL




Manual Integrations
APPROVED


MMDadoda
6/16/2021 5:03:03 PM

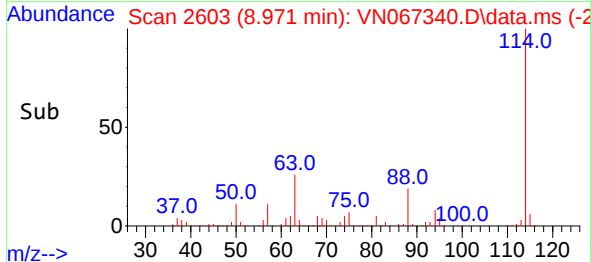


#35
Dibromofluoromethane
Concen: 49.869 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. -0.000 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

Tgt Ion:	113	Resp:	284054
Ion Ratio	Lower	Upper	
113	100		
111	101.8	83.8	125.8
192	16.2	13.4	20.0

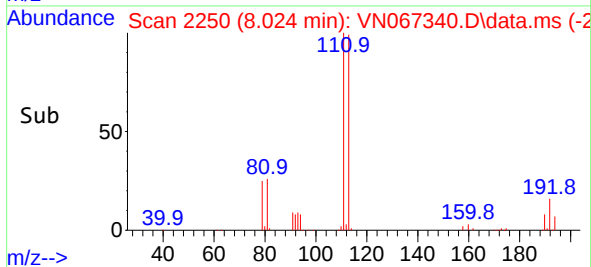

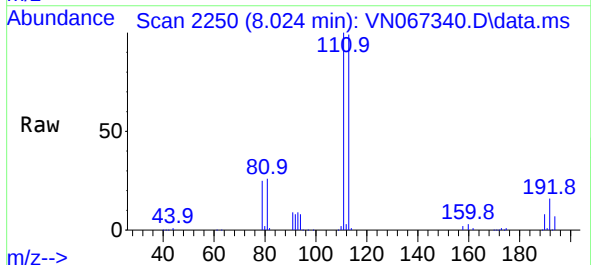





#36
1,1-Dichloropropene
Concen: 0.211 ug/l
RT: 8.225 min Scan# 2325
Delta R.T. 0.003 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34





Tgt Ion: 75 Resp: 2024
Ion Ratio Lower Upper
75 100
110 11.9 15.7 47.0#
77 9.3 24.6 37.0#



#37
Ethyl Acetate
Concen: 0.302 ug/l m
RT: 7.429 min Scan# 2028
Delta R.T. 0.011 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34




Tgt Ion: 43 Resp: 3068
Ion Ratio Lower Upper
43 100
61 0.0 10.6 16.0#
70 0.0 8.1 12.1#

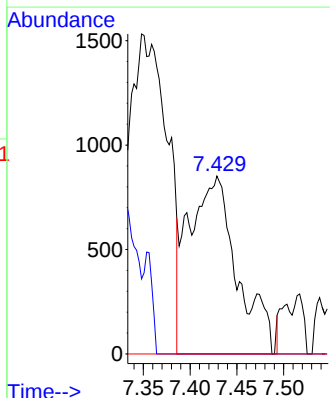


Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT2-2021DL

Manual Integrations
APPROVED

MMDadoda
6/16/2021 5:03:03 PM






#41
Methacrylonitrile
Concen: 0.303 ug/l m
RT: 7.640 min Scan# 2107
Delta R.T. 0.002 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34




Tgt Ion: 41 Resp: 1604

Ion	Ratio	Lower	Upper
41	100		
39	14.1	47.6	71.4#
67	0.0	57.7	86.5#
52	7.4	26.2	39.4#





#42
1,2-Dichloroethane
Concen: 0.235 ug/l
RT: 8.536 min Scan# 2441
Delta R.T. 0.005 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34



Tgt Ion: 62 Resp: 2666


Ion	Ratio	Lower	Upper
62	100		
98	0.0	0.0	14.2



Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT2-2021DL

Manual Integrations
APPROVED

MMDadoda
6/16/2021 5:03:03 PM







#48
Methyl methacrylate
Concen: 0.274 ug/l m
RT: 9.569 min Scan# 2826
Delta R.T. 0.008 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

Tgt Ion: 41 Resp: 2283
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 7.0 53.3 79.9#

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT2-2021DL




Manual Integrations
APPROVED


MMDadoda
6/16/2021 5:03:03 PM

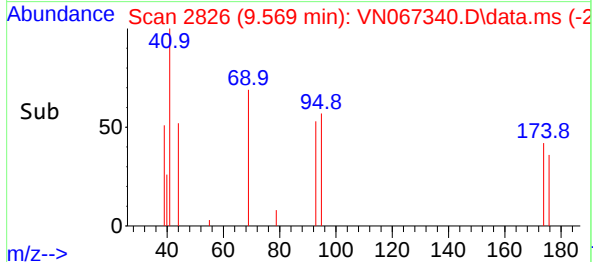

#49
1,4-Dioxane
Concen: 2.694 ug/l
RT: 9.579 min Scan# 2830
Delta R.T. 0.005 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34


Tgt Ion: 88 Resp: 307
Ion Ratio Lower Upper
88 100
43 77.9 28.8 43.2#
58 40.1 60.4 90.6#

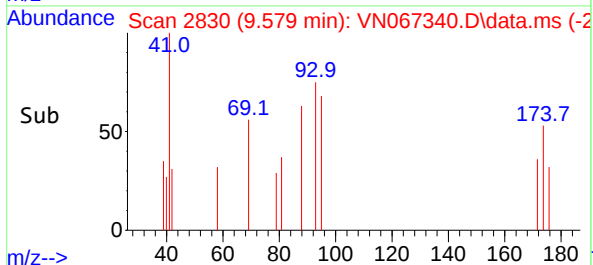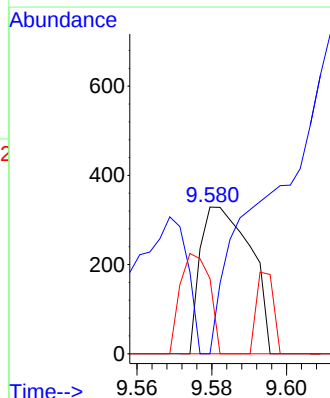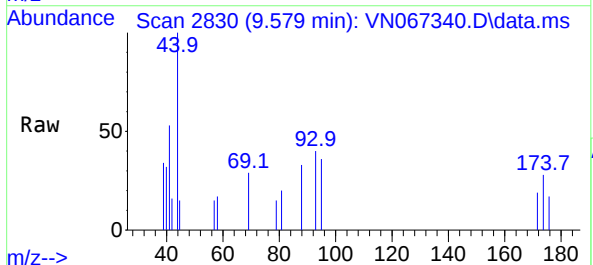

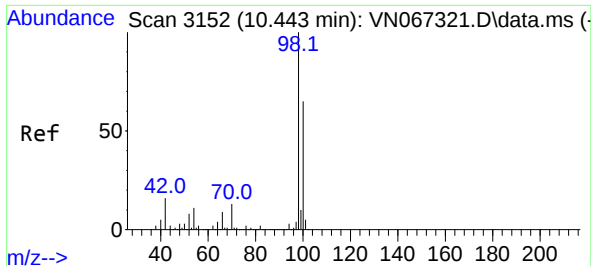

#50
Toluene-d8
Concen: 49.679 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34




Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT2-2021DL




Tgt Ion: 98 Resp: 1084585
Ion Ratio Lower Upper
98 100
100 63.8 51.7 77.5

Manual Integrations
APPROVED



MMDadoda
6/16/2021 5:03:03 PM

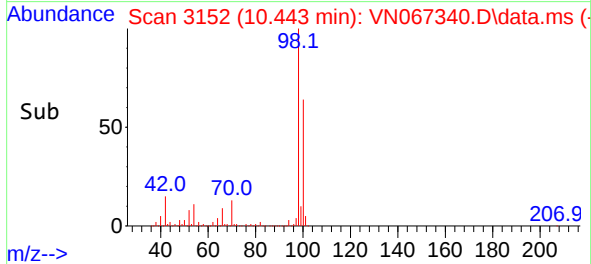


#51
4-Methyl-2-Pentanone
Concen: 0.670 ug/l
RT: 10.333 min Scan# 3111
Delta R.T. 0.000 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

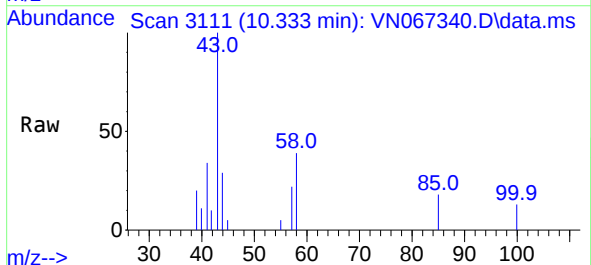

Tgt Ion: 43 Resp: 7048
Ion Ratio Lower Upper
43 100
58 37.9 28.6 43.0

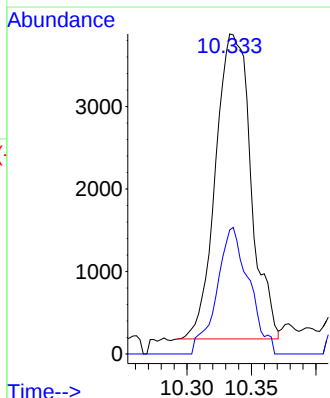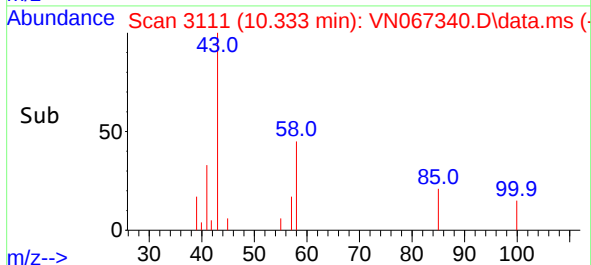

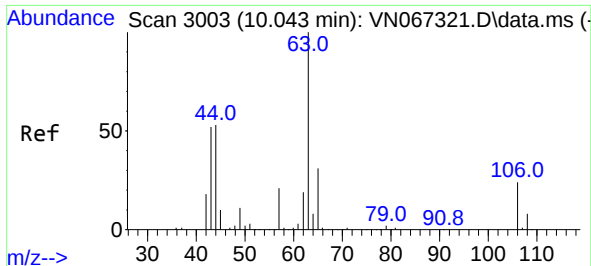





#58
2-Chloroethyl Vinyl ether
Concen: 0.654 ug/l
RT: 10.043 min Scan# 3003
Delta R.T. 0.000 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

Tgt Ion: 63 Resp: 2231
Ion Ratio Lower Upper
63 100
106 8.5 19.8 29.8#

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT2-2021DL




Manual Integrations
APPROVED


MMDadoda
6/16/2021 5:03:03 PM

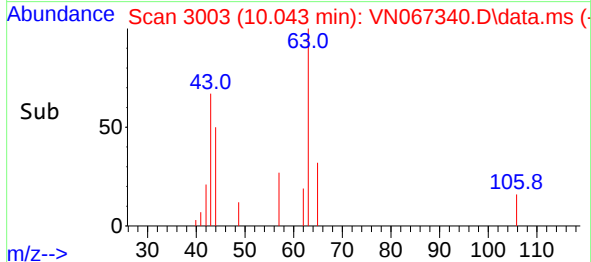

#59
2-Hexanone
Concen: 0.811 ug/l
RT: 11.092 min Scan# 3394
Delta R.T. 0.003 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

Tgt Ion: 43 Resp: 6242
Ion Ratio Lower Upper
43 100
58 53.1 24.7 74.1

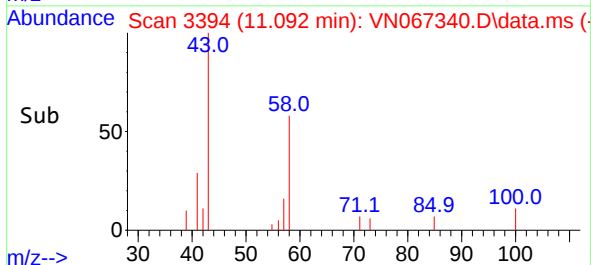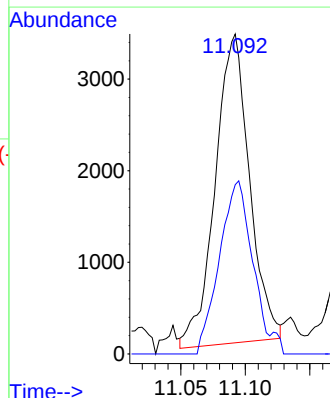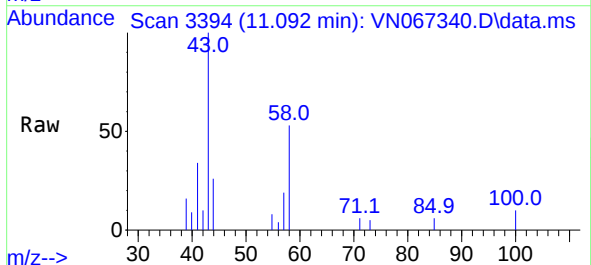

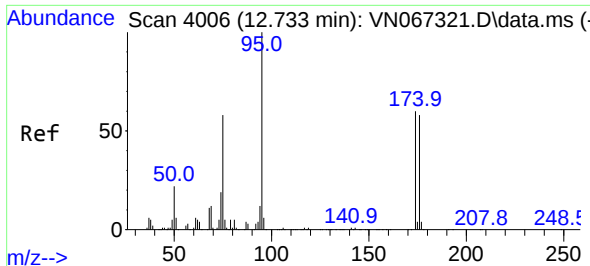





#62
4-Bromofluorobenzene
Concen: 46.681 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

Tgt Ion: 95 Resp: 420583
Ion Ratio Lower Upper
95 100
174 59.8 0.0 122.0
176 58.5 0.0 117.6

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT2-2021DL




Manual Integrations
APPROVED


MMDadoda
6/16/2021 5:03:03 PM

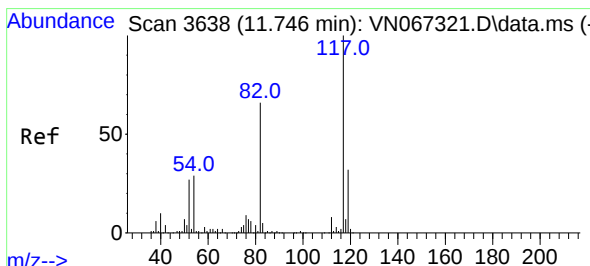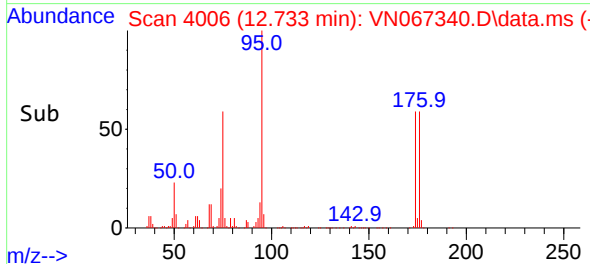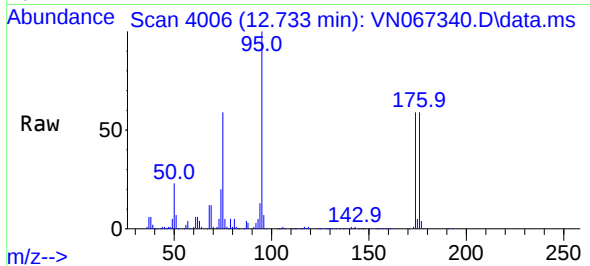

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.003 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34


Tgt Ion: 117 Resp: 773297
Ion Ratio Lower Upper
117 100
82 64.9 53.1 79.7
119 31.0 25.5 38.3

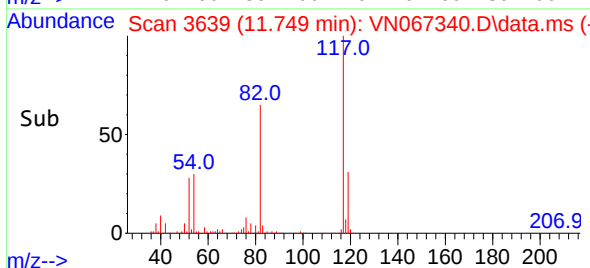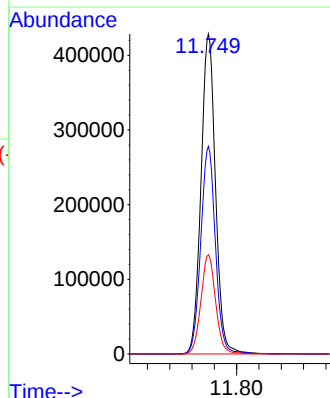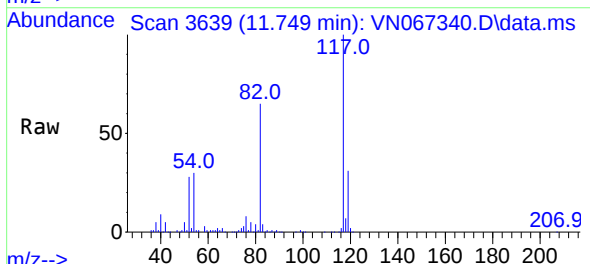

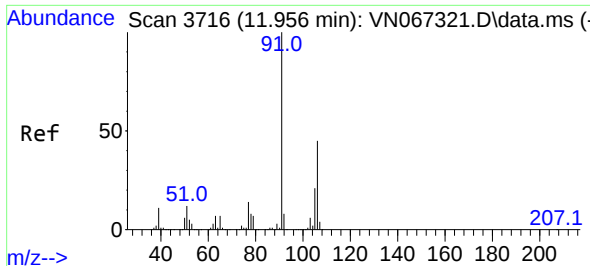

#68
m/p-Xylenes
Concen: 0.274 ug/l
RT: 11.950 min Scan# 3714
Delta R.T. -0.006 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34




Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT2-2021DL

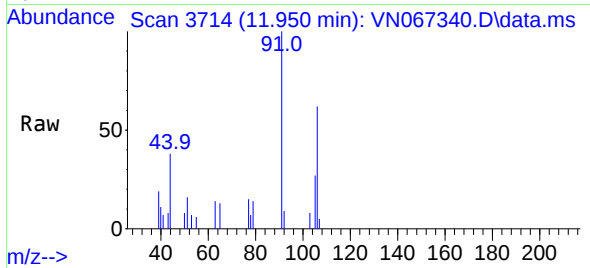


Tgt Ion:106 Resp: 3242
Ion Ratio Lower Upper
106 100
91 222.2 180.6 270.8

Manual Integrations
APPROVED



MMDadoda
6/16/2021 5:03:03 PM

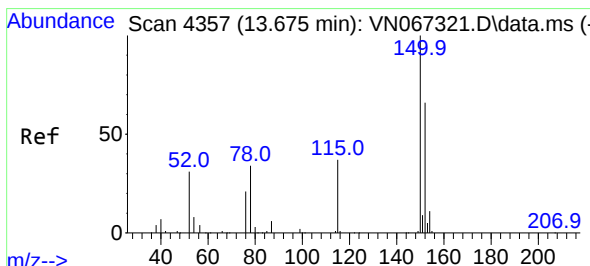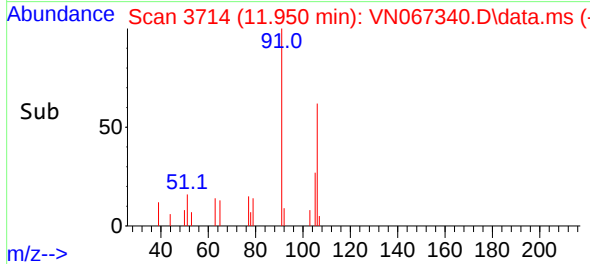


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.003 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

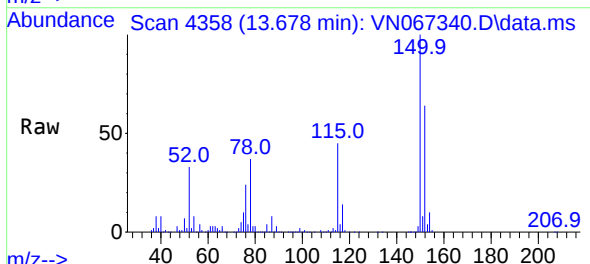


Tgt Ion:152 Resp: 300421
Ion Ratio Lower Upper
152 100
115 70.8 36.1 108.5
150 157.5 0.0 351.8


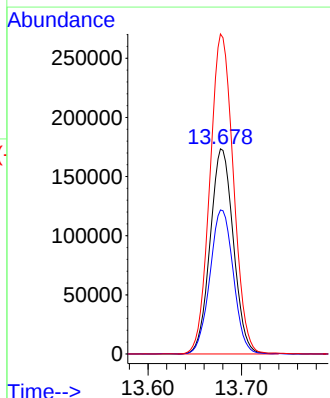
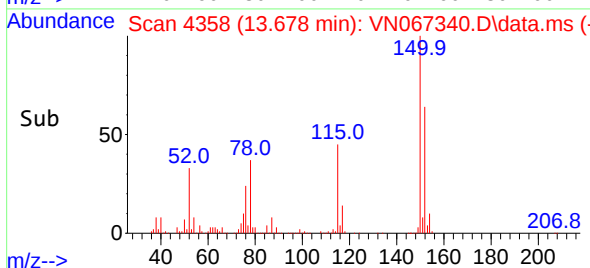


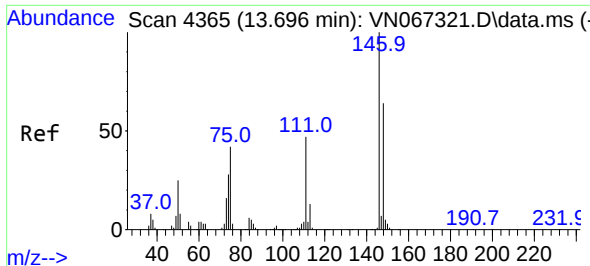


#88
1,4-Dichlorobenzene
Concen: 0.232 ug/l m
RT: 13.702 min Scan# 4367
Delta R.T. 0.006 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

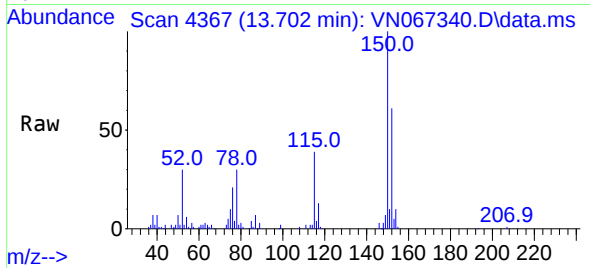



Tgt Ion:146 Resp: 2470
Ion Ratio Lower Upper
146 100
111 34.8 23.4 70.2
148 52.3 31.8 95.3

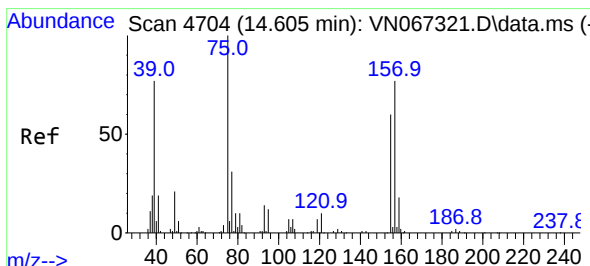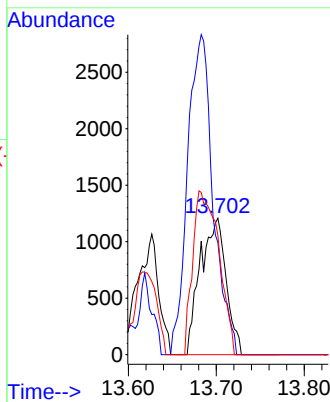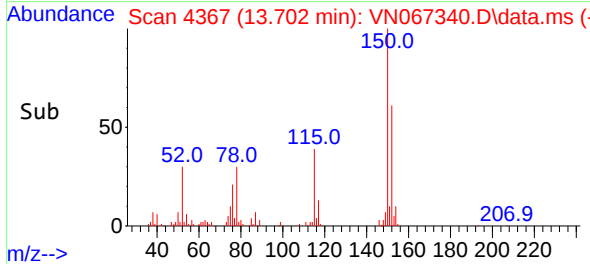

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.219 ug/l
RT: 14.603 min Scan# 4703
Delta R.T. -0.002 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

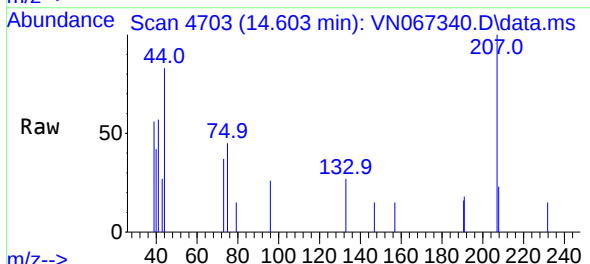


Tgt Ion: 75 Resp: 470
Ion Ratio Lower Upper
75 100
155 0.0 29.8 89.5#
157 16.6 37.6 112.8#

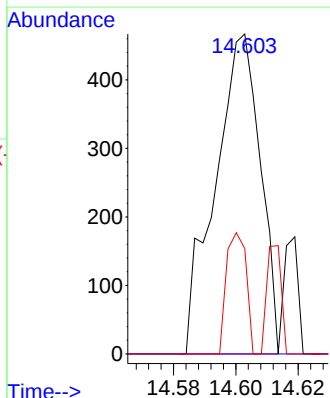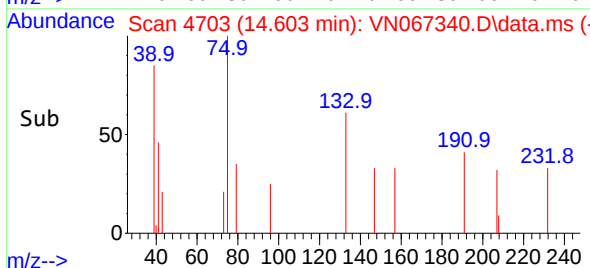


Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT2-2021DL

Manual Integrations
APPROVED




MMDadoda
6/16/2021 5:03:03 PM

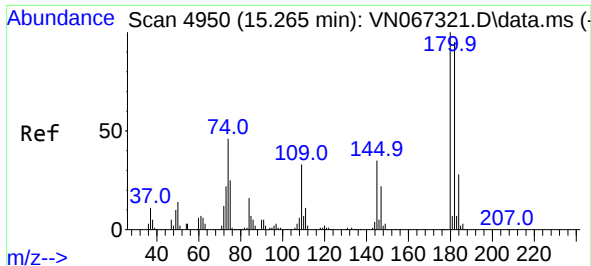


#93
1,2,4-Trichlorobenzene
Concen: 0.263 ug/l
RT: 15.268 min Scan# 4951
Delta R.T. 0.003 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34





Tgt Ion:180 Resp: 1380
Ion Ratio Lower Upper
180 100
182 94.9 47.5 142.5
145 25.9 17.2 51.6

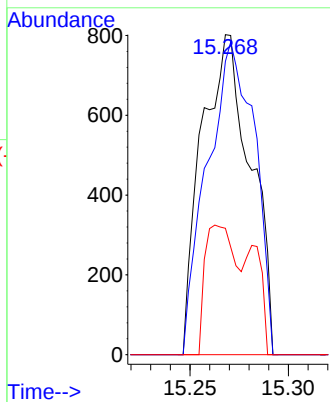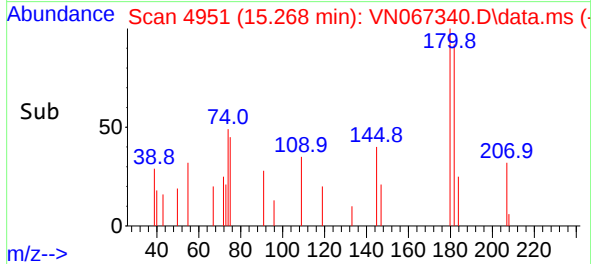

#95
Naphthalene
Concen: 0.391 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. -0.000 min
Lab File: VN067340.D
Acq: 15 Jun 2021 12:34

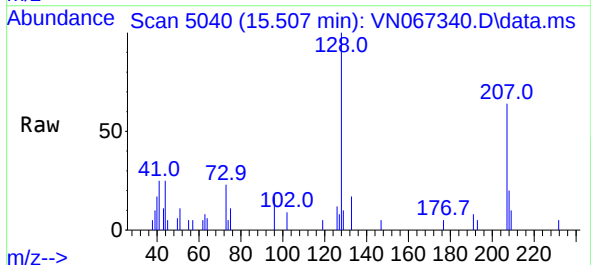


Tgt Ion:128 Resp: 6249
Ion Ratio Lower Upper
128 100
127 8.7 10.6 15.8#
129 5.0 8.6 12.8#

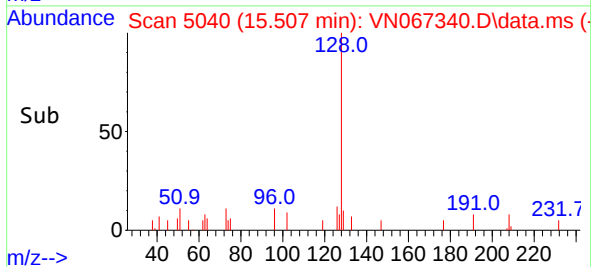

Instrument :
MSVOA_N
ClientSampleId :
MDL-WATER-03-QT2-2021DL


Manual Integrations
APPROVED

MMDadoda
6/16/2021 5:03:03 PM

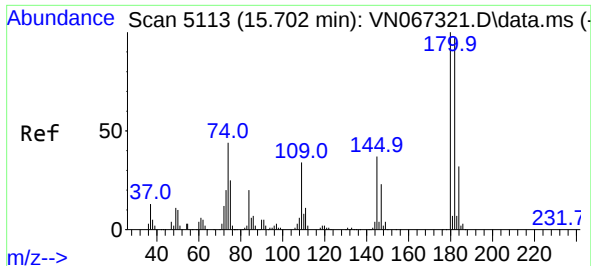

#96
 1,2,3-Trichlorobenzene
 Concen: 0.314 ug/l m
 RT: 15.702 min Scan# 5113
 Delta R.T. 0.000 min
 Lab File: VN067340.D
 Acq: 15 Jun 2021 12:34

Instrument :
 MSVOA_N
 ClientSampleId :
 MDL-WATER-03-QT2-2021DL

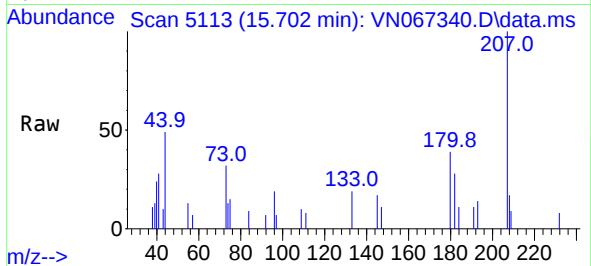

Tgt Ion:180 Resp: 1582
 Ion Ratio Lower Upper
 180 100
 182 45.1 47.8 143.3#
 145 27.0 18.2 54.6

Manual Integrations
 APPROVED

MMDadoda
 6/16/2021 5:03:03 PM

