
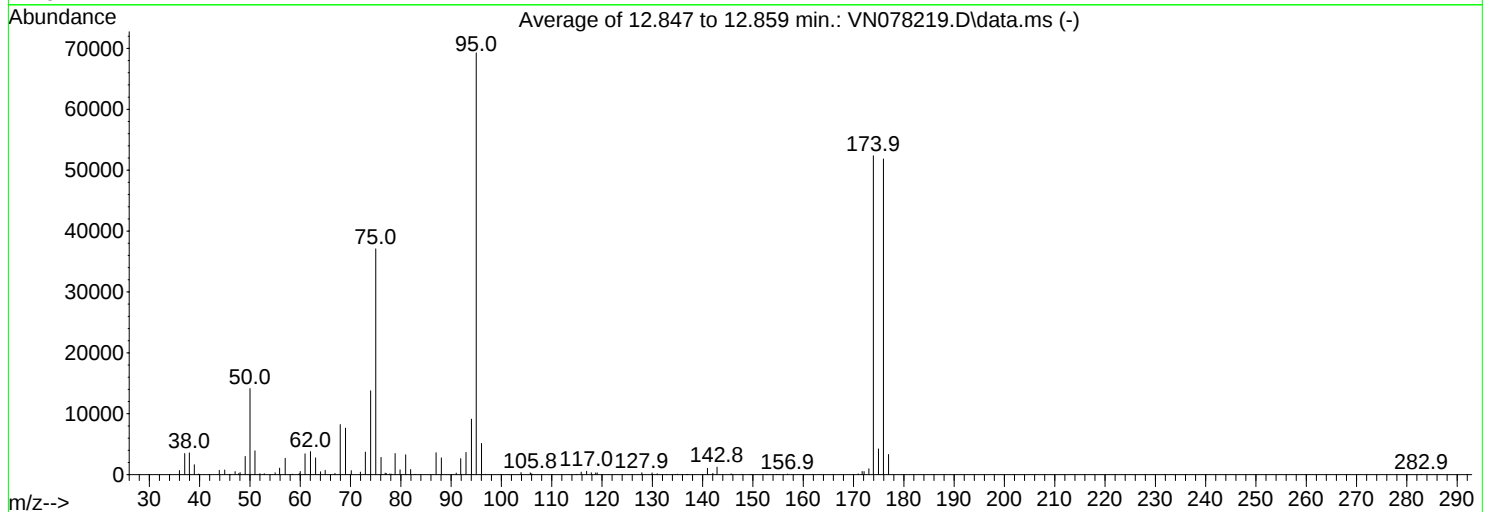


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061523\
Data File : VN078219.D
Acq On : 15 Jun 2023 10:59
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
Title : SW846 8260
Last Update : Wed Jun 07 05:05:00 2023

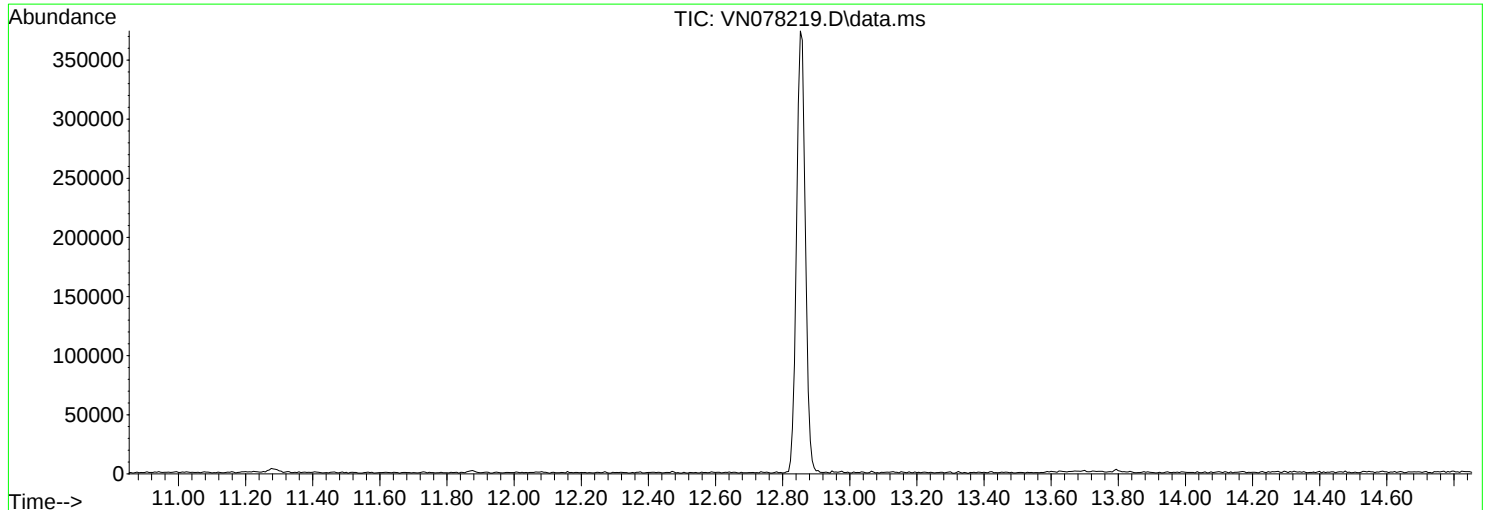

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	14145	PASS
75	95	30	60	53.5	37075	PASS
95	95	100	100	100.0	69272	PASS
96	95	5	9	7.4	5135	PASS
173	174	0.00	2	1.8	969	PASS
174	95	50	100	75.6	52381	PASS
175	174	5	9	8.1	4220	PASS
176	174	95	101	99.0	51848	PASS
177	176	5	9	6.4	3327	PASS

Average of 12.847 to 12.859 min.: VN078219.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	696	47.80	176	59.80	197	71.95	411
37.05	3462	48.05	334	60.00	530	72.95	369
37.95	3565	49.05	3005	60.95	3413	74.00	1377
38.95	1634	50.00	14145	62.05	3787	75.00	3707
39.85	103	51.00	3931	63.05	2759	76.05	2838
41.90	52	52.00	156	64.05	480	76.90	278
43.90	707	52.85	163	64.95	705	77.10	176
45.00	779	55.00	305	66.90	205	77.80	141
45.90	59	55.90	1085	67.95	8218	78.10	74
46.20	53	57.00	2668	69.00	7645	78.85	3467
47.05	491	58.40	81	70.15	661	79.85	788

Average of 12.847 to 12.859 min.: VN078219.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.95	3251	96.90	53	127.90	321	145.60	69
81.95	833	103.90	353	129.95	296	145.80	117
82.80	50	105.75	291	130.95	158	147.80	50
87.00	3602	105.90	159	132.80	55	149.60	54
88.05	2770	106.10	80	134.70	59	152.80	57
91.00	253	115.00	58	135.00	80	154.70	54
91.90	2625	115.85	427	136.80	51	155.20	66
92.95	3655	116.95	560	137.00	60	156.90	115
94.05	9129	117.85	317	140.95	1040	170.90	129
95.00	69272	118.75	300	142.05	203	171.70	535
96.05	5135	119.05	297	142.85	1228	172.10	511

Average of 12.847 to 12.859 min.: VN078219.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
173.05	969						
173.95	52381						
174.95	4220						
175.95	51848						
176.95	3327						
282.90	64						