



2-Hexanone

Response Ratio

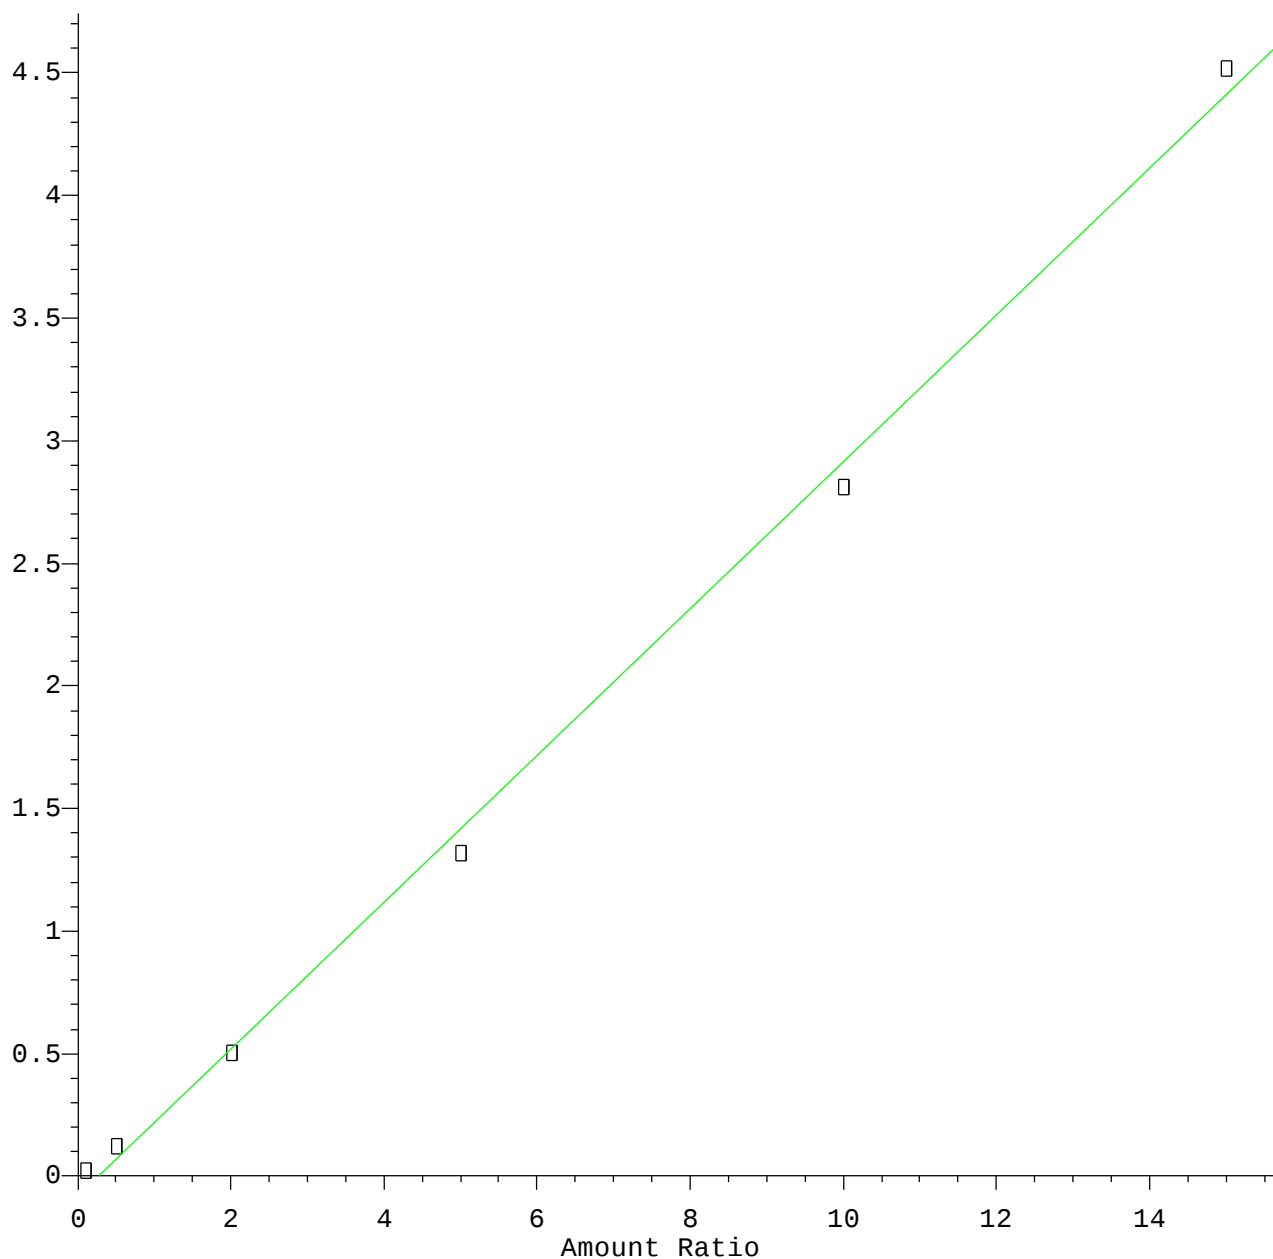


Resp Ratio = 2.99e-001 * Amt - 8.03e-002
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061620W.M
Calibration Table Last Updated: Wed Jun 17 01:19:44 2020

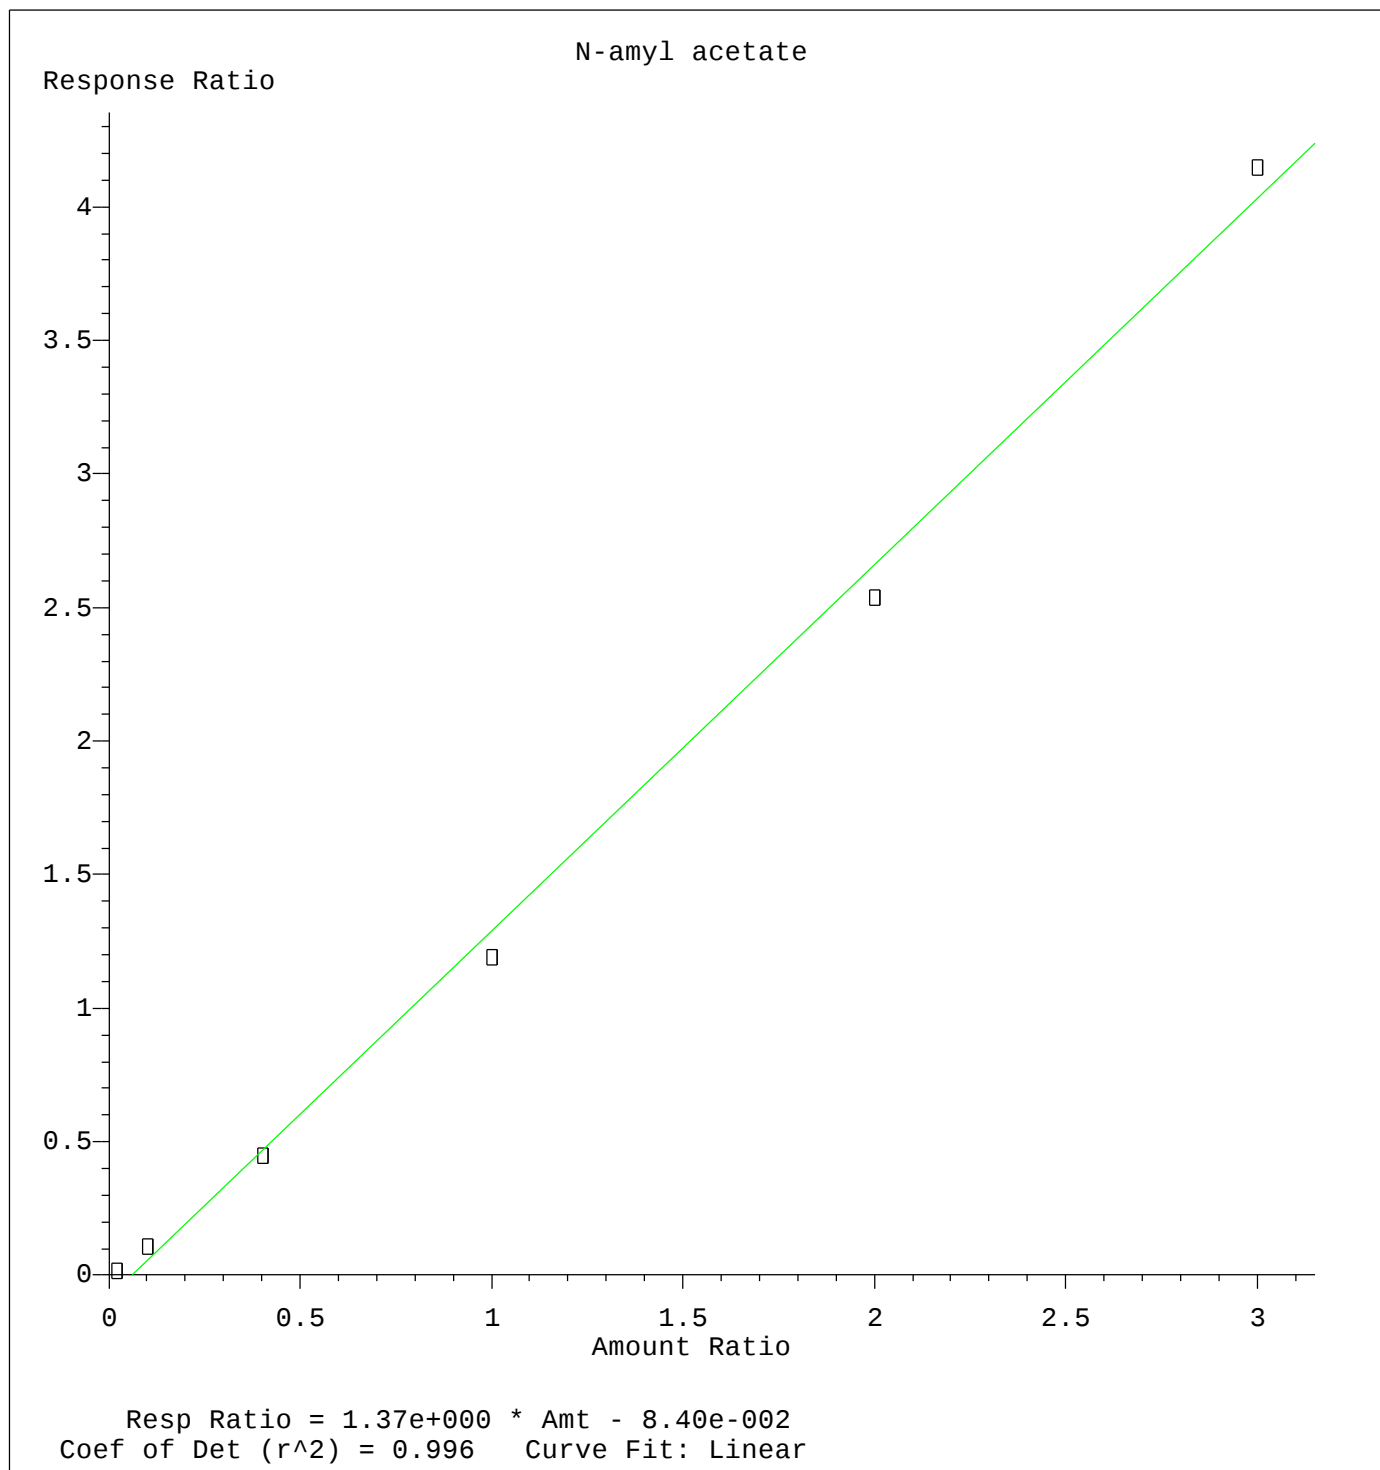


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061620W.M
Calibration Table Last Updated: Wed Jun 17 01:19:44 2020

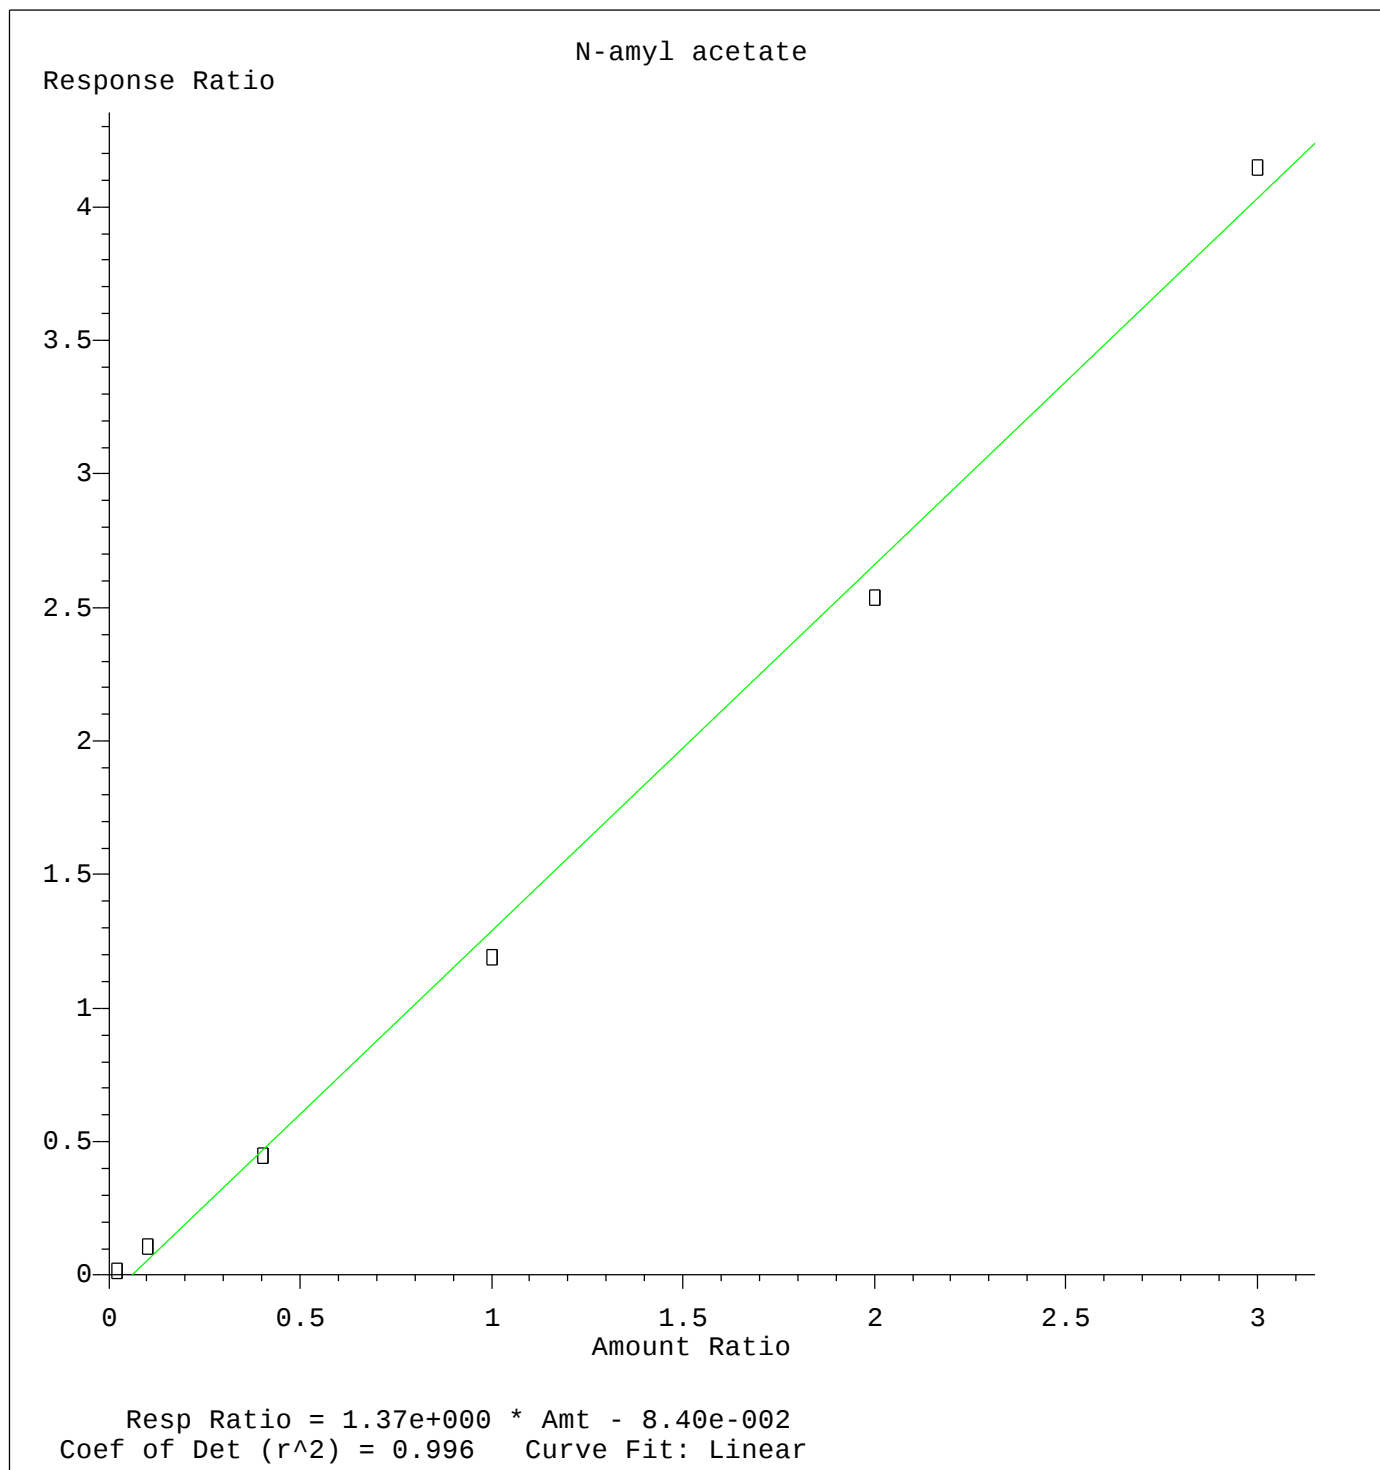

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061620W.M
Calibration Table Last Updated: Wed Jun 17 01:19:44 2020

Naphthalene

Response Ratio

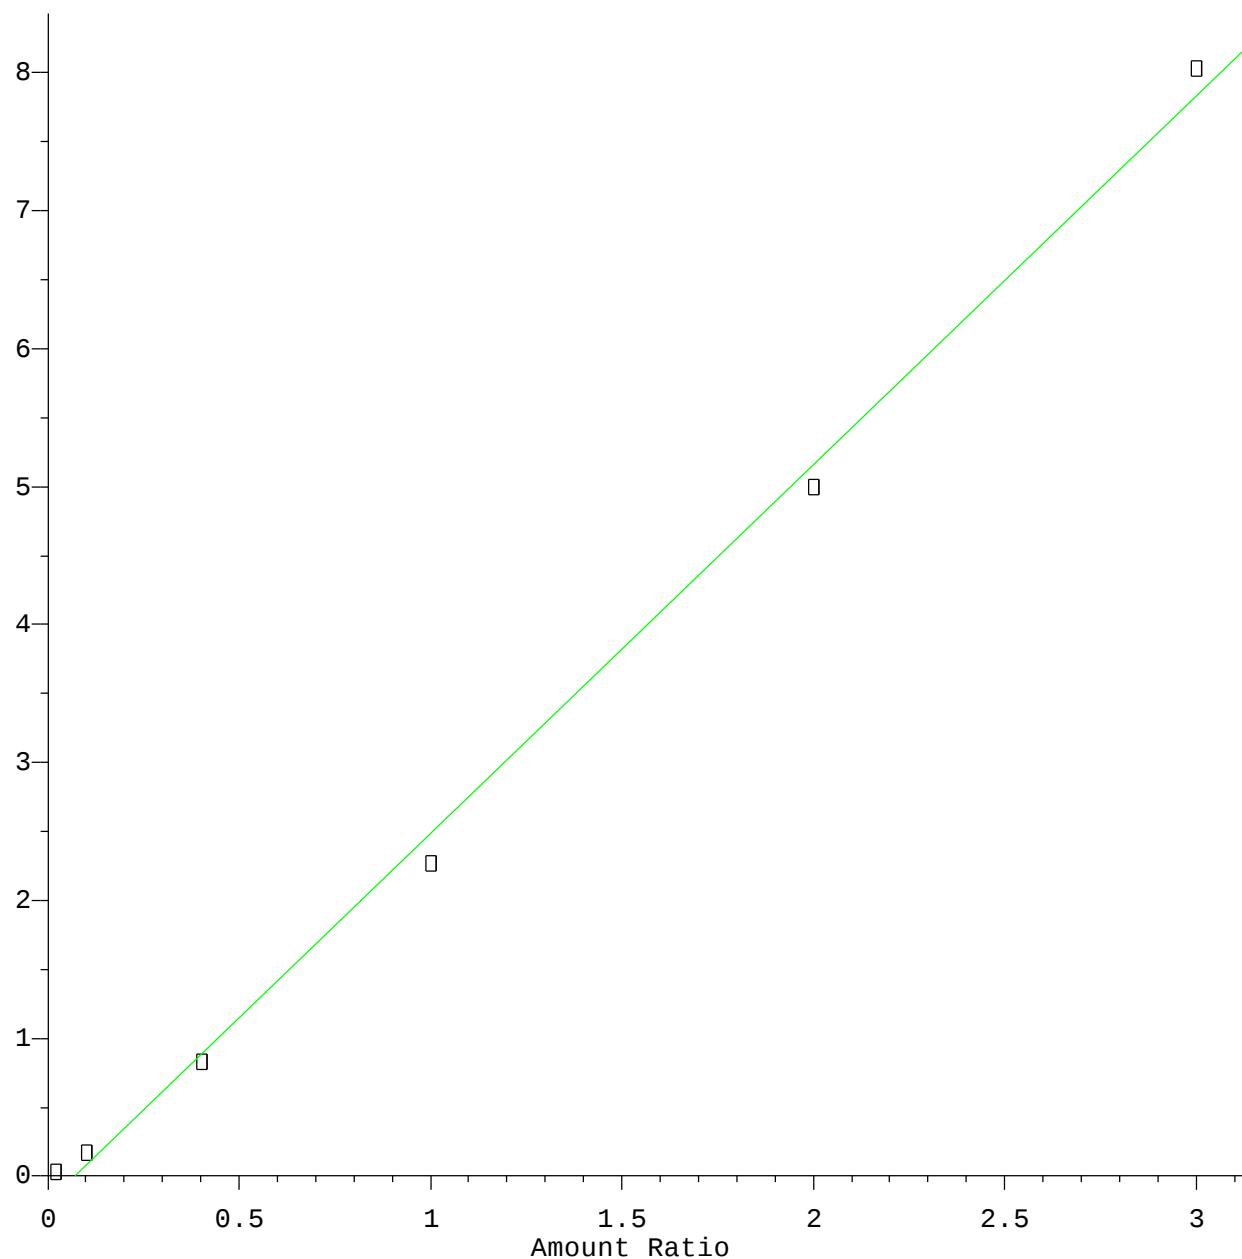


Resp Ratio = $2.67 \times 10^0 \times \text{Amt} - 1.86 \times 10^{-1}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061620W.M
Calibration Table Last Updated: Wed Jun 17 01:19:44 2020


Dichlorodifluoromethane

Response Ratio

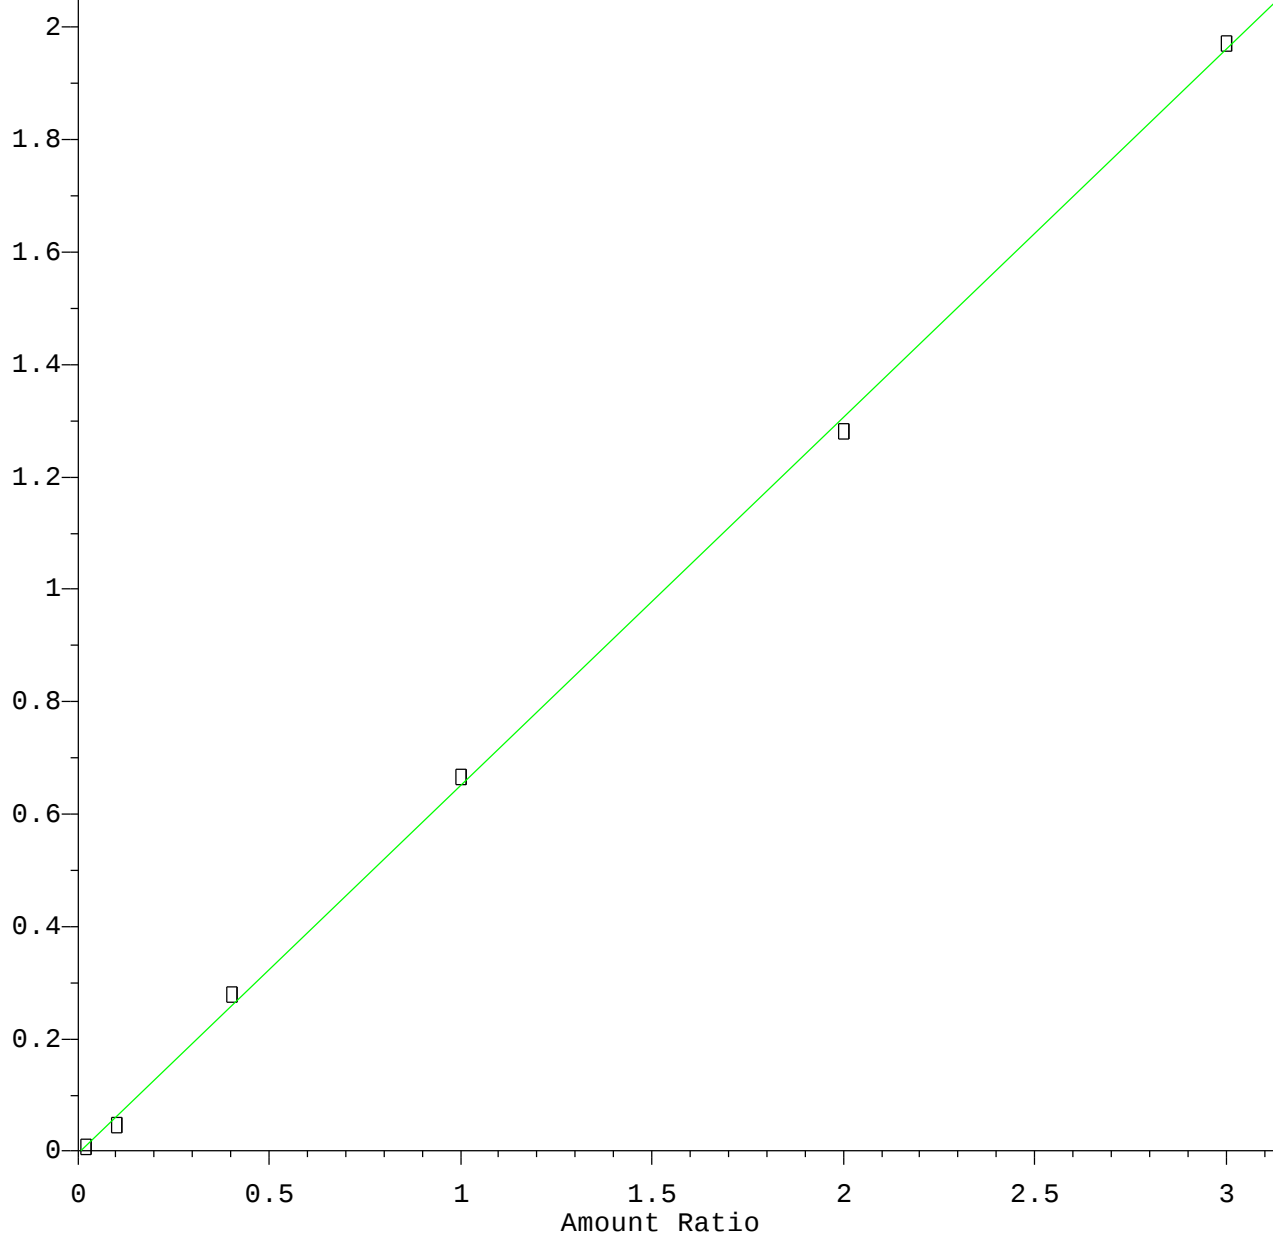

Resp Ratio = $6.54 \times 10^{-1} \times \text{Amt} - 3.82 \times 10^{-3}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061620W.M
Calibration Table Last Updated: Wed Jun 17 01:19:44 2020

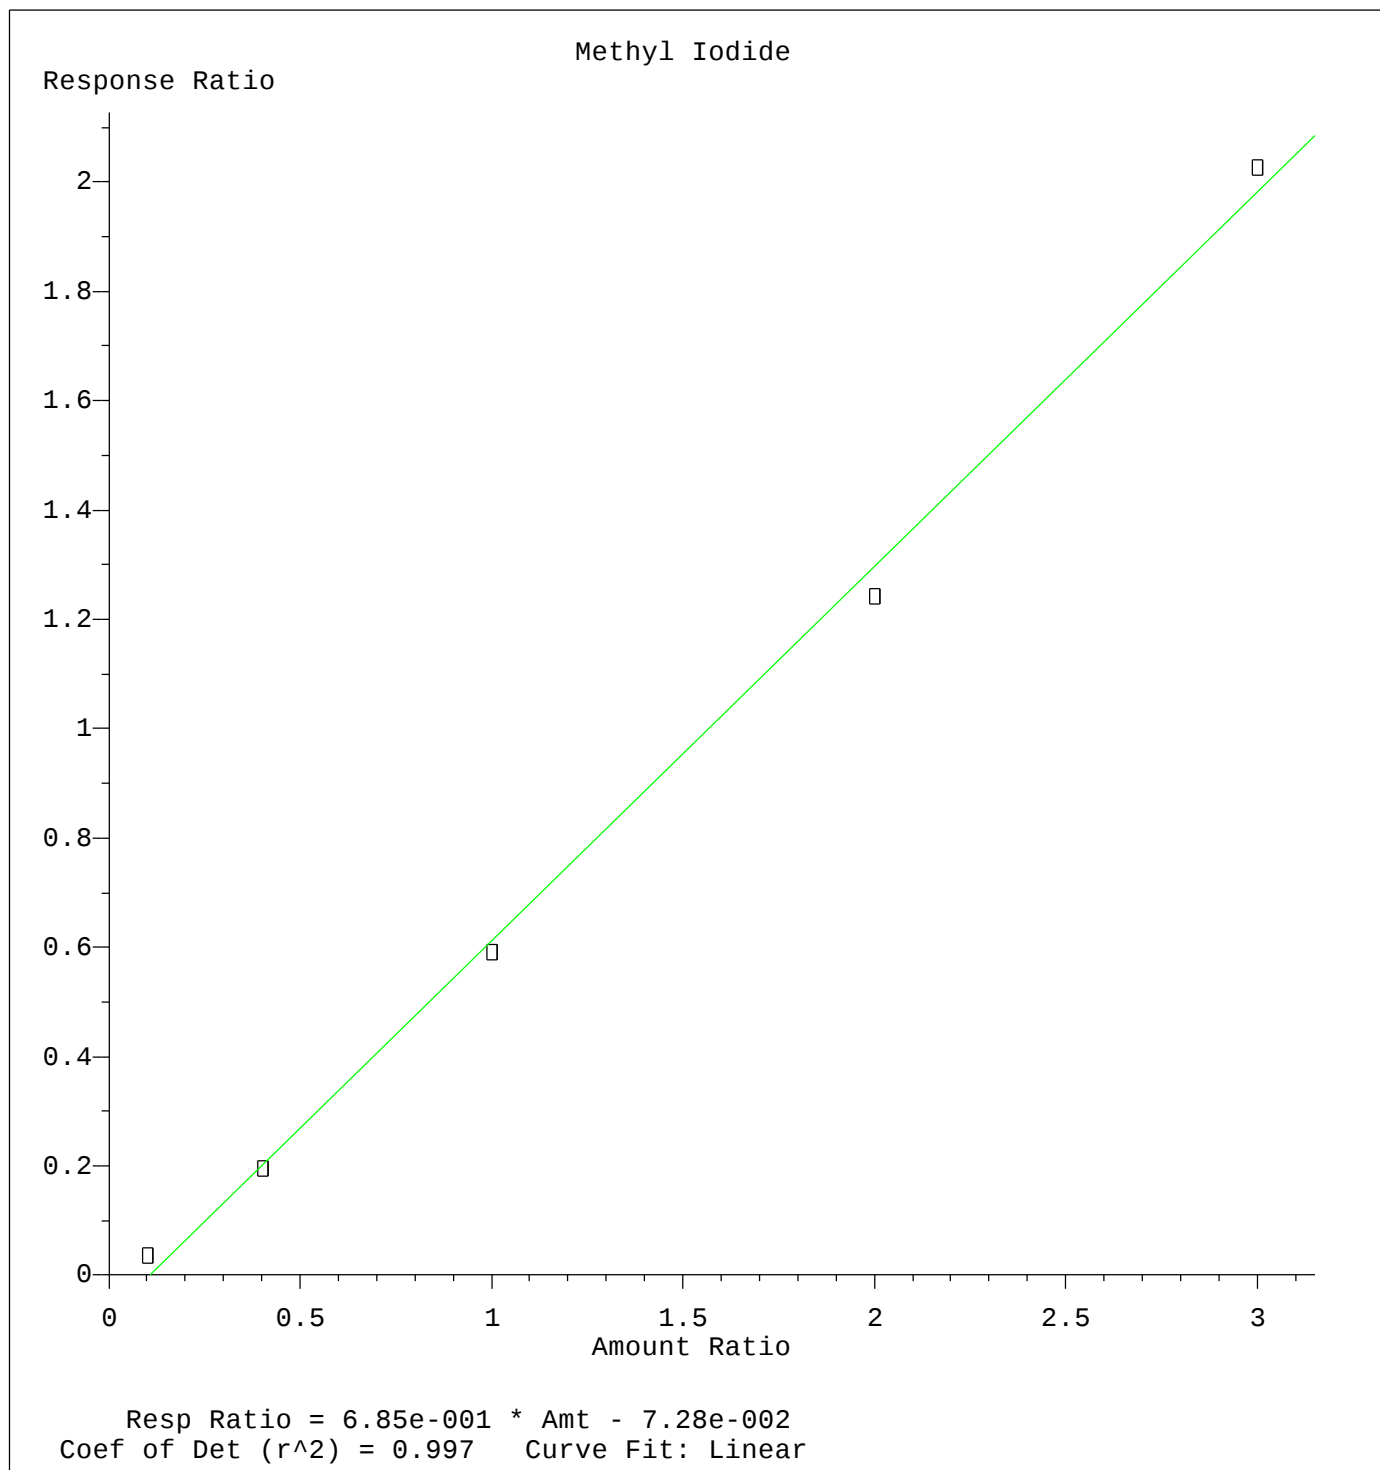

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061620W.M
Calibration Table Last Updated: Wed Jun 17 01:19:44 2020

Ethyl methacrylate

Response Ratio

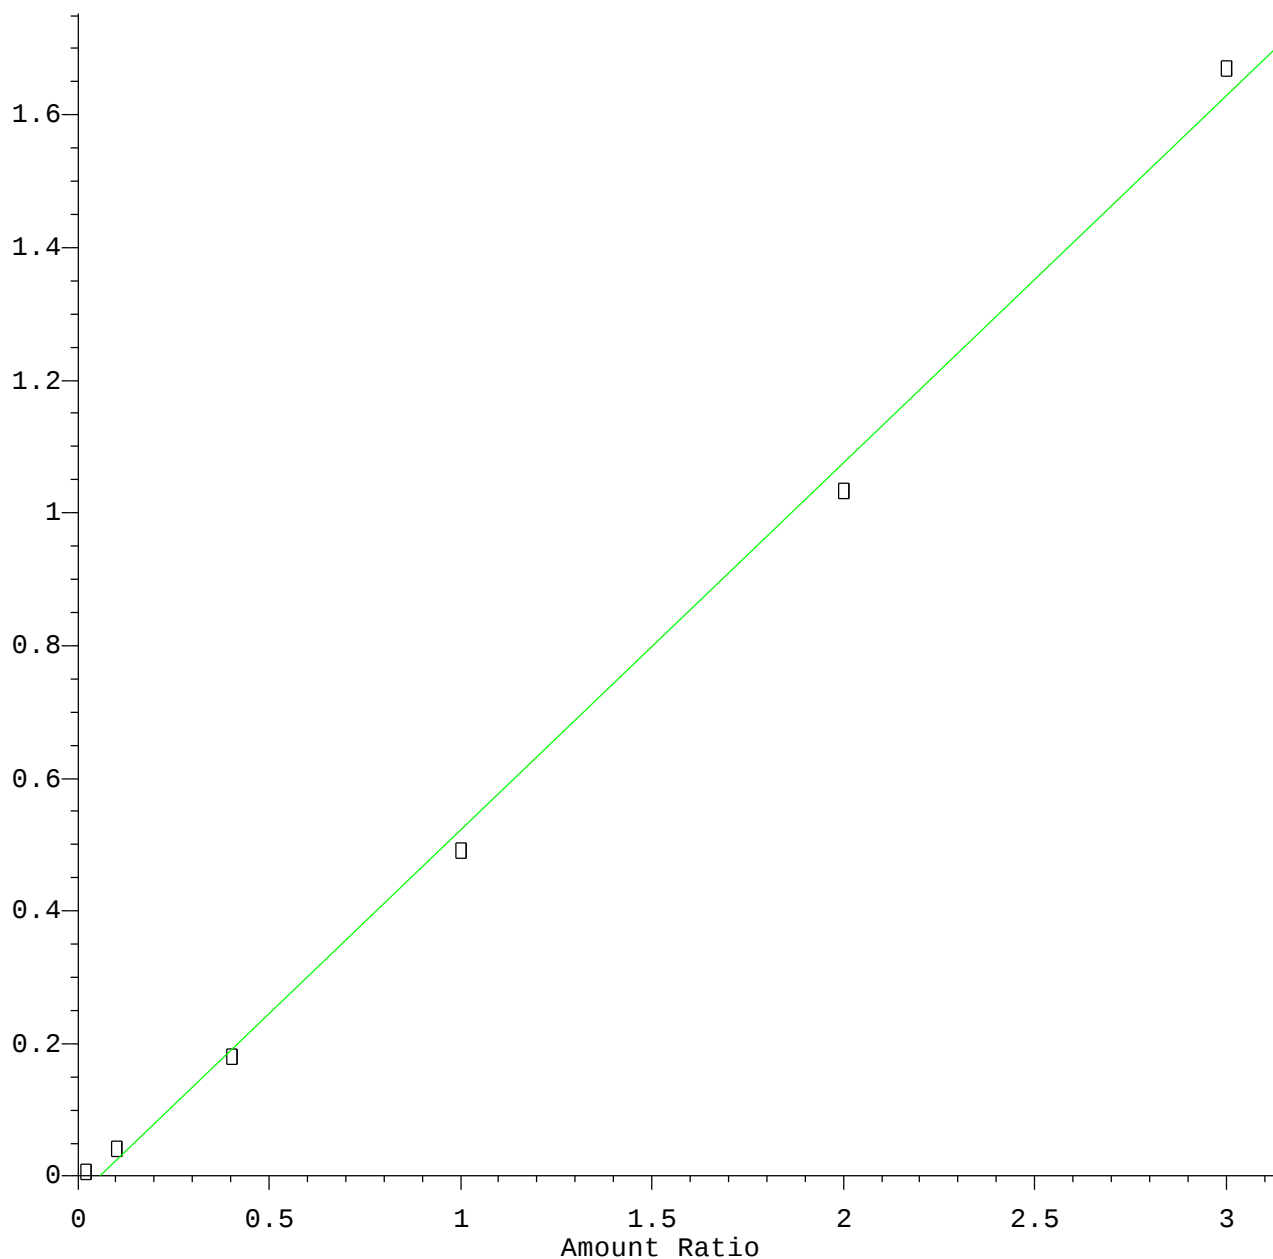

Resp Ratio = $5.54 \times 10^{-1} \times \text{Amt} - 3.21 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061620W.M
Calibration Table Last Updated: Wed Jun 17 01:19:44 2020