
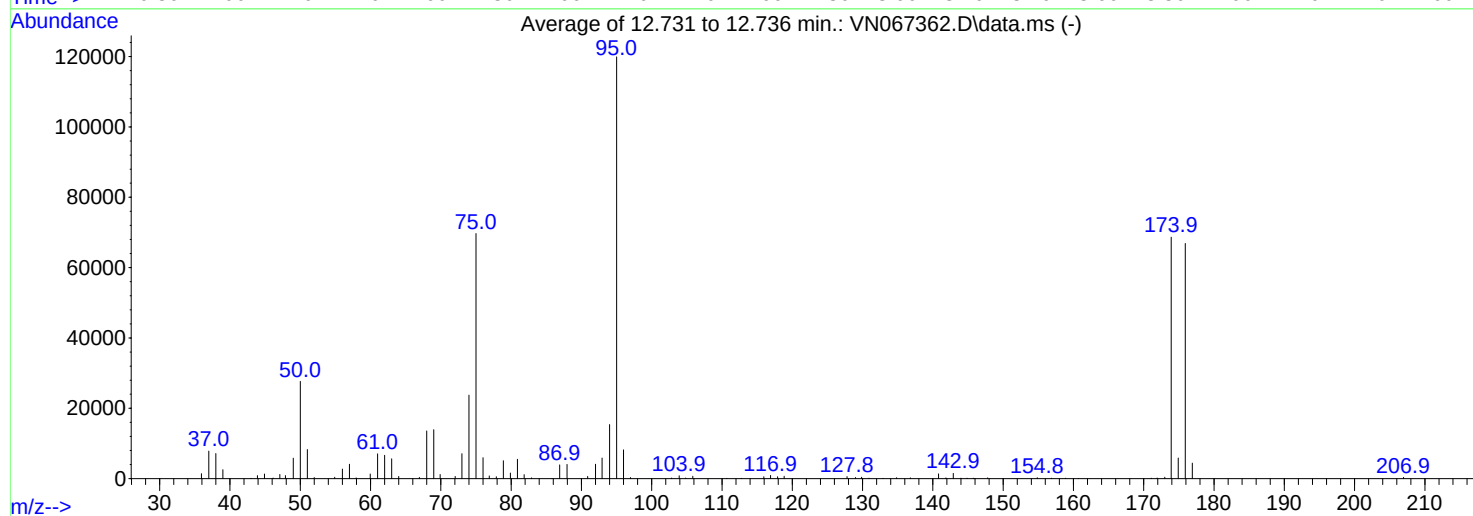


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061621\
 Data File : VN067362.D
 Acq On : 16 Jun 2021 12:05
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N061121W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Sat Jun 12 09:13:15 2021

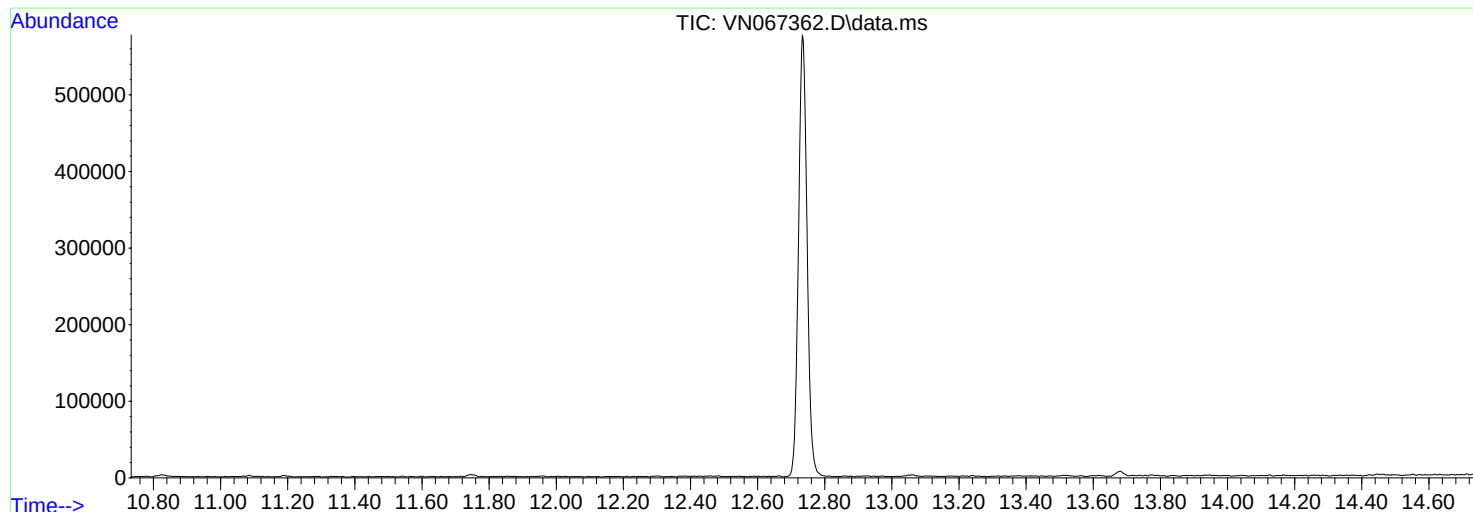

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3989

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	27656	PASS
75	95	30	60	58.1	69707	PASS
95	95	100	100	100.0	119920	PASS
96	95	5	9	6.8	8189	PASS
173	174	0.00	2	0.6	435	PASS
174	95	50	100	57.2	68635	PASS
175	174	5	9	8.5	5866	PASS
176	174	95	101	97.4	66867	PASS
177	176	5	9	6.6	4437	PASS