
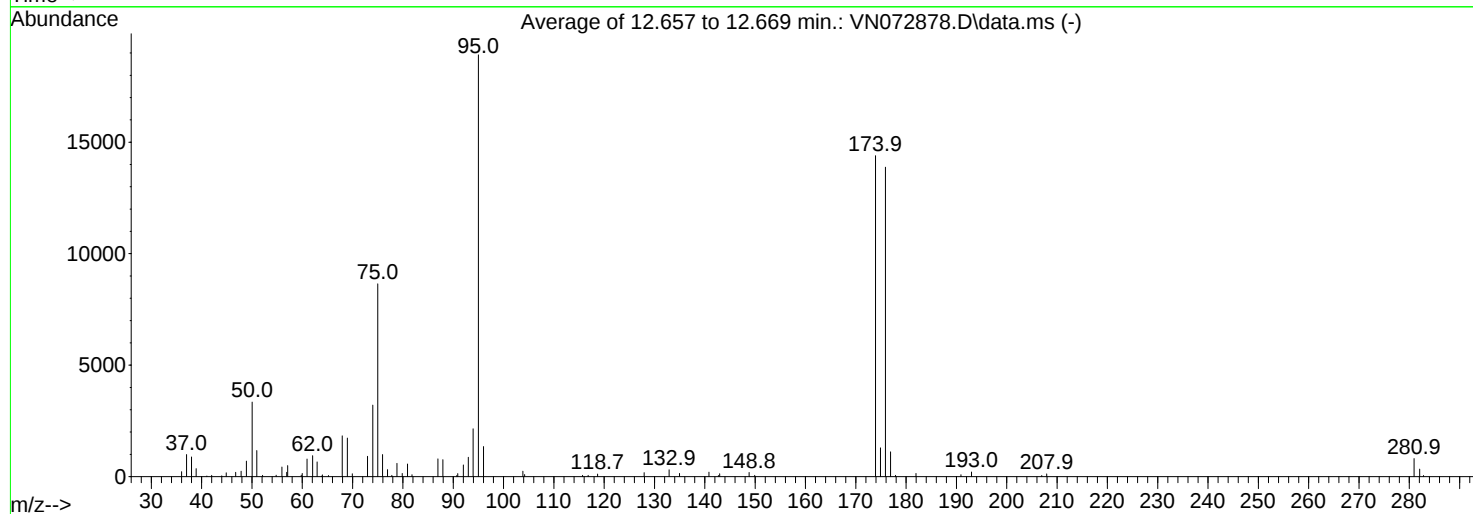


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061622\
Data File : VN072878.D
Acq On : 16 Jun 2022 09:34
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061622W.M
Title : SW846 8260
Last Update : Fri Jun 17 06:04:26 2022

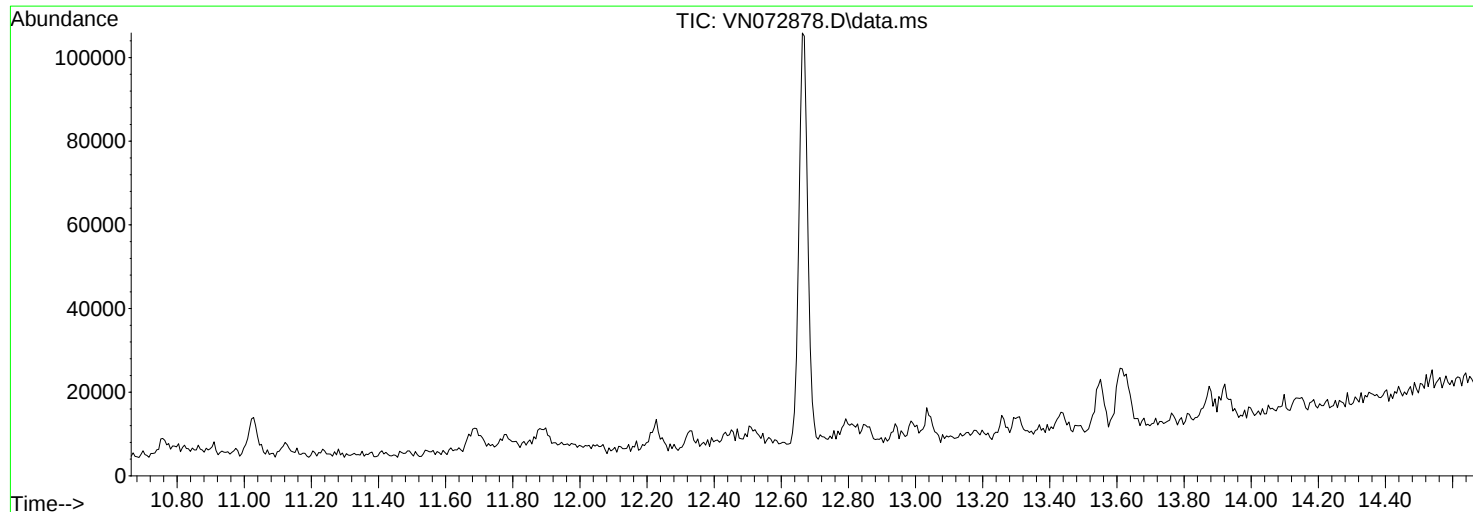

AutoFind: Scans 1814, 1815, 1816; Background Corrected with Scan 1807

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	3346	PASS
75	95	30	60	45.7	8645	PASS
95	95	100	100	100.0	18917	PASS
96	95	5	9	7.1	1352	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	76.1	14396	PASS
175	174	5	9	9.0	1292	PASS
176	174	95	101	96.4	13878	PASS
177	176	5	9	8.0	1115	PASS