

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061623\
 Data File : VN078253.D
 Acq On : 16 Jun 2023 12:26
 Operator : JC\MD
 Sample : 03299-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jun 17 02:21:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 07 05:05:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.235	168	456383	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	821582	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	737249	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	219545	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	320266	52.632	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 105.260%	
35) Dibromofluoromethane	8.171	113	287021	55.252	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 110.500%	
50) Toluene-d8	10.571	98	971870	48.530	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 97.060%	
62) 4-Bromofluorobenzene	12.853	95	300431	48.257	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 96.520%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.377	50	3528	Below Cal	#	76
5) Bromomethane	2.977	94	1959	0.384	ug/l #	63
11) Tert butyl alcohol	5.530	59	1058	1.259	ug/l #	72
13) Acrolein	4.206	56	526	0.568	ug/l #	36
15) Acrylonitrile	5.736	53	558	0.258	ug/l #	80
16) Acetone	4.471	43	2739	1.564	ug/l #	80
17) Carbon Disulfide	4.718	76	3057	0.238	ug/l #	75
20) Methylene Chloride	5.289	84	1884	0.326	ug/l #	88
25) 2-Butanone	7.512	43	1224	0.454	ug/l #	37
29) Tetrahydrofuran	7.865	42	424	0.235	ug/l #	20
31) Cyclohexane	8.235	56	11409	1.462	ug/l #	26
36) 1,1-Dichloropropene	8.230	75	40824	5.479	ug/l #	48
38) Carbon Tetrachloride	8.235	117	49933	6.346	ug/l #	16
47) Bromodichloromethane	9.894	83	6402	0.845	ug/l	99
59) 2-Hexanone	11.200	43	1945	0.477	ug/l	90
60) Dibromochloromethane	11.365	129	62756	10.794	ug/l	98
71) Bromoform	12.582	173	48831	13.030	ug/l #	94
74) N-amyl acetate	12.500	43	1416	0.207	ug/l #	64
75) 1,1,2,2-Tetrachloroethane	12.947	83	495	Below Cal	#	74
76) 1,2,3-Trichloropropane	12.853	75	161204	31.060	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	161204	95.425	ug/l #	15
82) 4-Chlorotoluene	13.229	91	2832	0.208	ug/l	92
87) 1,3-Dichlorobenzene	13.747	146	2294	0.281	ug/l	97
88) 1,4-Dichlorobenzene	13.747	146	2294	0.292	ug/l	99
89) n-Butylbenzene	14.059	91	3983	0.325	ug/l	96
91) 1,2-Dichlorobenzene	14.112	146	2209	0.277	ug/l	83
92) 1,2-Dibromo-3-Chloropr...	14.735	75	495	0.481	ug/l #	22
93) 1,2,4-Trichlorobenzene	15.400	180	1805	0.636	ug/l	85
94) Hexachlorobutadiene	15.506	225	1555	Below Cal		92
95) Naphthalene	15.647	128	6963	0.729	ug/l #	97
96) 1,2,3-Trichlorobenzene	15.853	180	2022	0.637	ug/l #	58

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061623\
Data File : VN078253.D
Acq On : 16 Jun 2023 12:26
Operator : JC\MD
Sample : 03299-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jun 17 02:21:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 07 05:05:00 2023
Response via : Initial Calibration

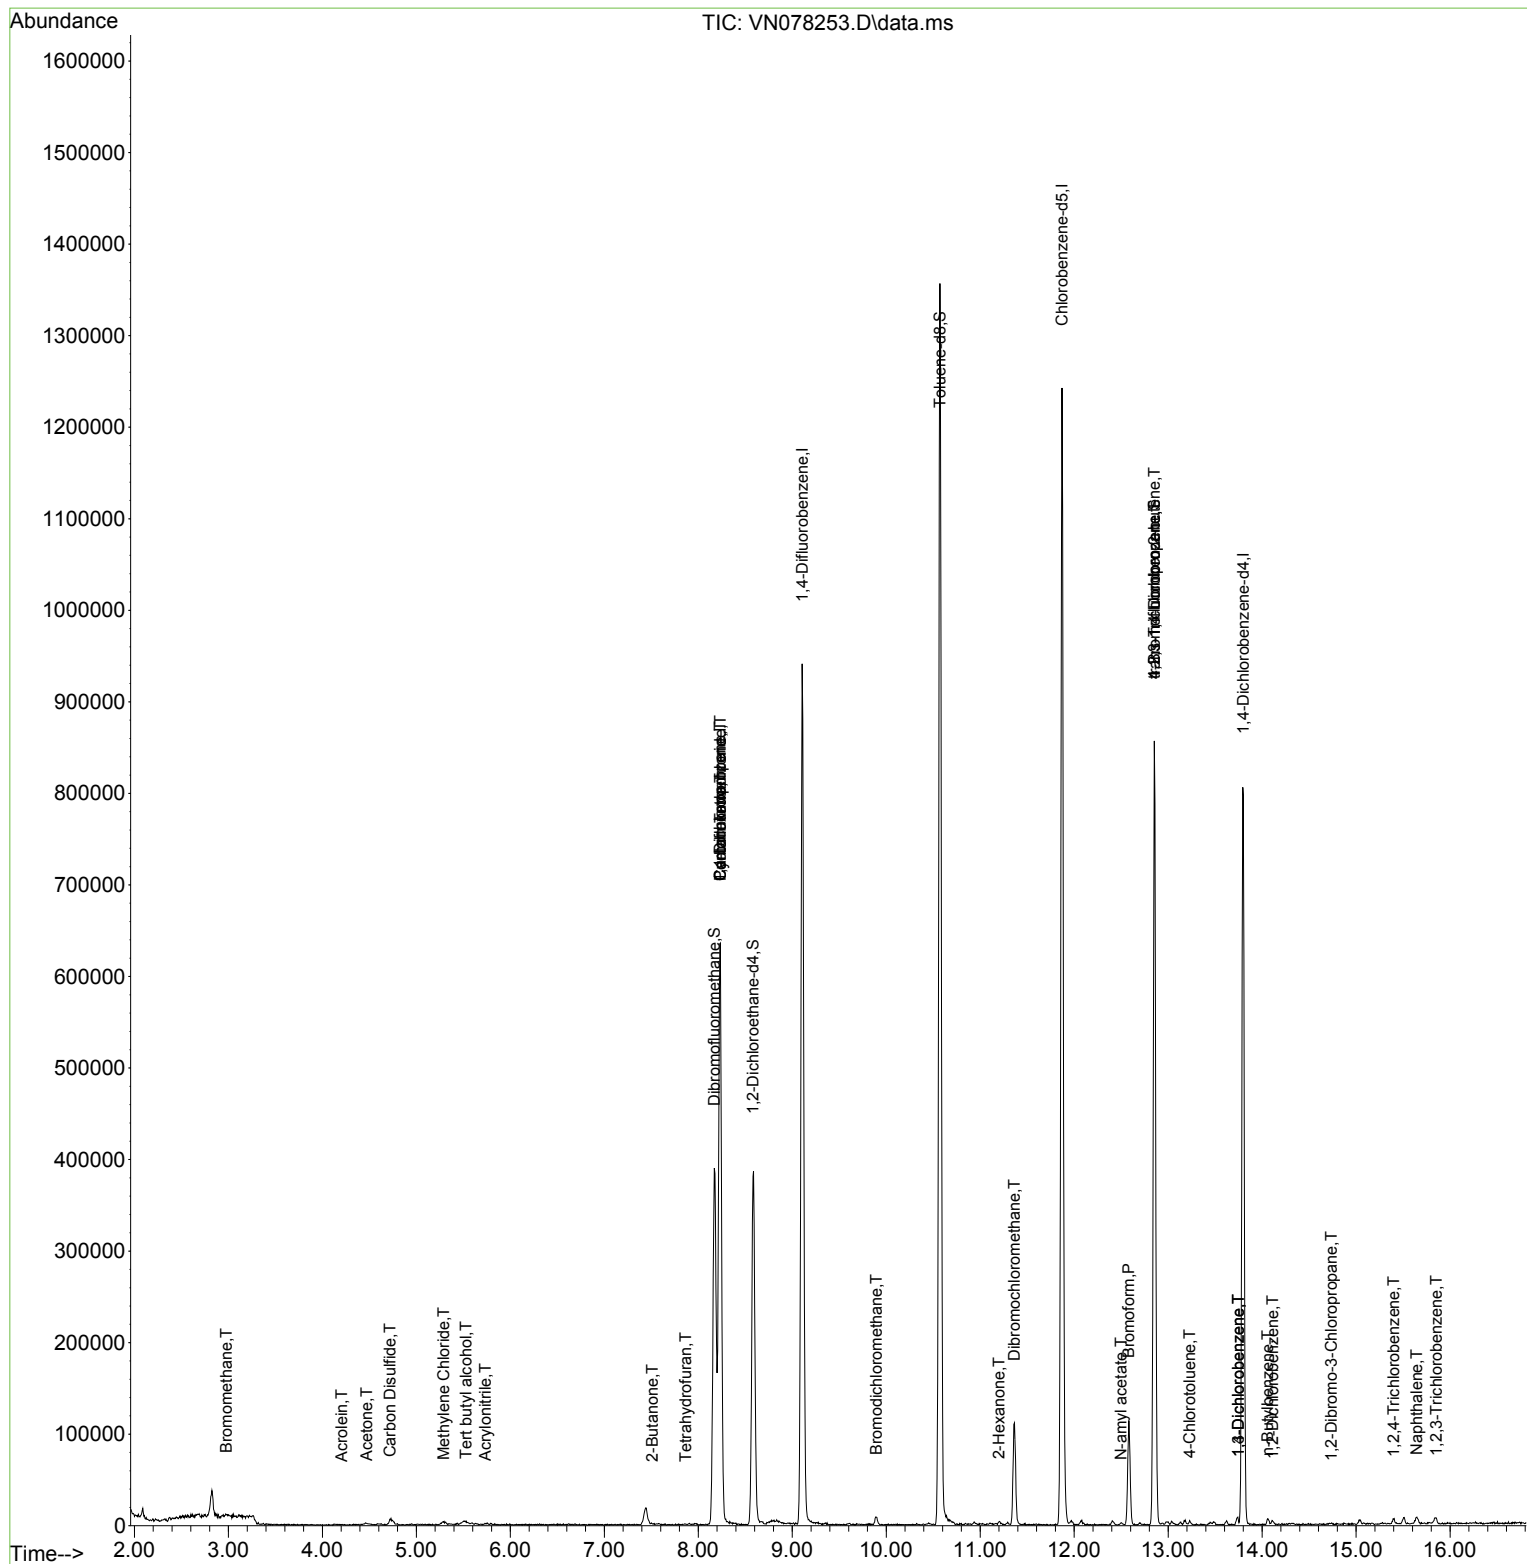



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.235 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN078253.D

Acq: 16 Jun 2023 12:26

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:168 Resp: 456383

Ion Ratio Lower Upper

168 100

99 61.3 53.0 79.6



#3

Chloromethane

Concen: Below Cal

RT: 2.377 min Scan# 72

Delta R.T. 0.006 min

Lab File: VN078253.D




Acq: 16 Jun 2023 12:26


Tgt Ion: 50 Resp: 3528

Ion Ratio Lower Upper

50 100

52 46.6 26.5 39.7#


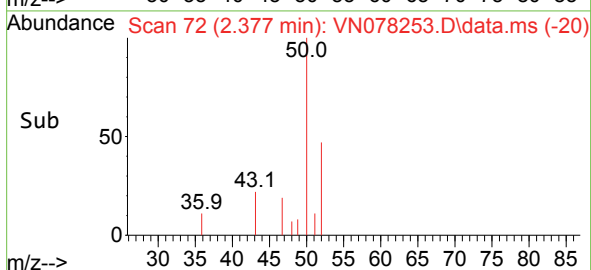






#5
Bromomethane
Concen: 0.384 ug/l
RT: 2.977 min Scan# 11
Delta R.T. 0.024 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 94 Resp: 1959
Ion Ratio Lower Upper
94 100
96 126.5 73.1 109.7#

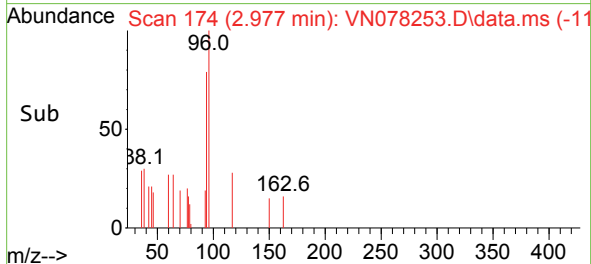

#11
Tert butyl alcohol
Concen: 1.259 ug/l
RT: 5.530 min Scan# 608
Delta R.T. -0.006 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26

Tgt Ion: 59 Resp: 1058
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#





#13

Acrolein

Concen: 0.568 ug/l

RT: 4.206 min Scan# 383

Delta R.T. 0.018 min


Lab File: VN078253.D

Acq: 16 Jun 2023 12:26

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion: 56 Resp: 526

Ion Ratio Lower Upper

56 100

55 16.7 54.5 81.7#



#15

Acrylonitrile

Concen: 0.258 ug/l

RT: 5.736 min Scan# 643

Delta R.T. 0.006 min

Lab File: VN078253.D

Acq: 16 Jun 2023 12:26




Tgt Ion: 53 Resp: 558


Ion Ratio Lower Upper

53 100

52 106.5 65.3 97.9#

51 38.0 28.9 43.3


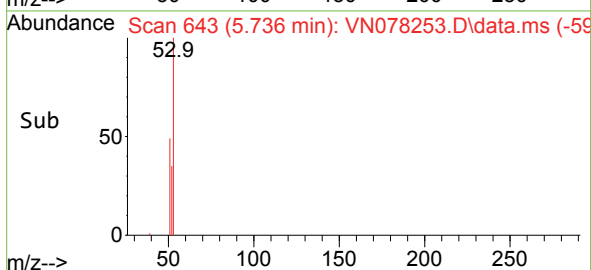






#16
Acetone
Concen: 1.564 ug/l
RT: 4.471 min Scan# 41
Delta R.T. 0.035 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 2739
Ion Ratio Lower Upper
43 100
58 23.1 28.0 42.0#

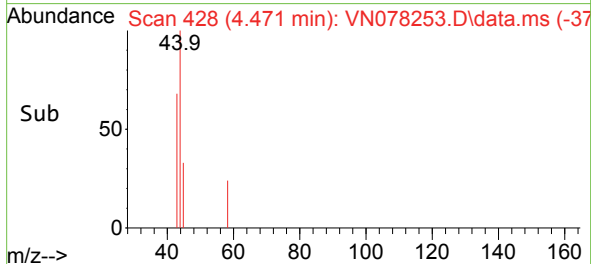

#17
Carbon Disulfide
Concen: 0.238 ug/l
RT: 4.718 min Scan# 470
Delta R.T. 0.000 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26


Tgt Ion: 76 Resp: 3057
Ion Ratio Lower Upper
76 100
78 0.0 7.4 11.0#

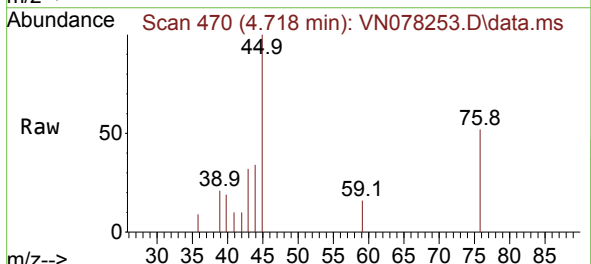






#20
Methylene Chloride
Concen: 0.326 ug/l
RT: 5.289 min Scan# 51
Delta R.T. 0.006 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 84 Resp: 1884
Ion Ratio Lower Upper
84 100
49 105.6 79.7 119.5
51 0.0 25.2 37.8#
86 65.7 53.3 79.9



#25
2-Butanone
Concen: 0.454 ug/l
RT: 7.512 min Scan# 945
Delta R.T. 0.018 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26

Tgt Ion: 43 Resp: 1224
Ion Ratio Lower Upper
43 100
72 0.0 30.2 45.2#



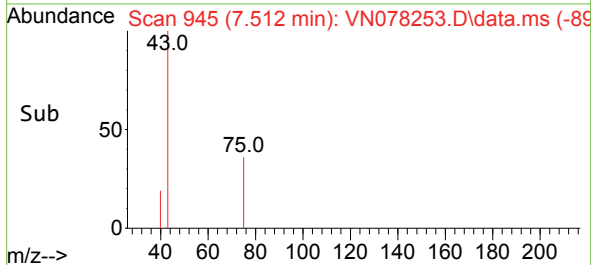





#29
Tetrahydrofuran
Concen: 0.235 ug/l
RT: 7.865 min Scan# 1005
Delta R.T. 0.018 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 42 Resp: 424
Ion Ratio Lower Upper
42 100
72 0.0 49.8 74.6#
71 0.0 47.4 71.2#

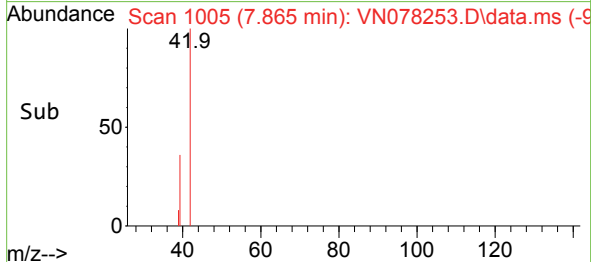

#31
Cyclohexane
Concen: 1.462 ug/l
RT: 8.235 min Scan# 1068
Delta R.T. -0.029 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26

Tgt Ion: 56 Resp: 11409
Ion Ratio Lower Upper
56 100
69 125.5 26.8 40.2#
84 148.3 81.8 122.6#

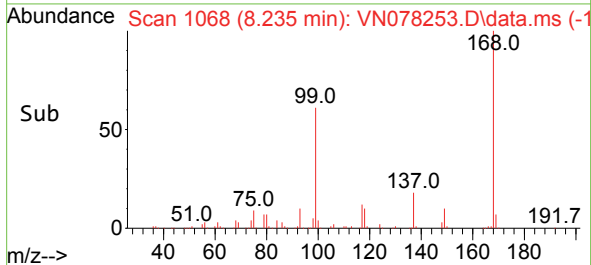



#33

1,2-Dichloroethane-d4

Concen: 52.632 ug/l

RT: 8.583 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VN078253.D

Acq: 16 Jun 2023 12:26

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 320266

Ion Ratio Lower Upper

65 100

67 53.4 0.0 106.6

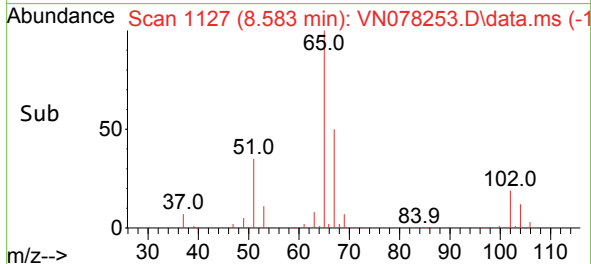

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. 0.000 min

Lab File: VN078253.D

Acq: 16 Jun 2023 12:26




Tgt Ion: 114 Resp: 821582


Ion Ratio Lower Upper

114 100

63 20.6 0.0 36.4

88 14.7 0.0 30.6









#35
Dibromofluoromethane
Concen: 55.252 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. -0.006 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:113 Resp: 287021
Ion Ratio Lower Upper
113 100
111 102.2 82.6 123.8
192 16.9 12.7 19.1

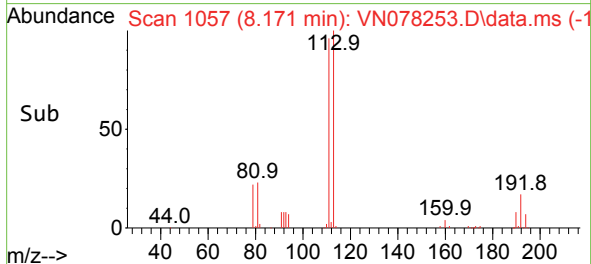

#36
1,1-Dichloropropene
Concen: 5.479 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.147 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26

Tgt Ion: 75 Resp: 40824
Ion Ratio Lower Upper
75 100
110 9.5 19.1 57.3#
77 0.0 25.0 37.4#

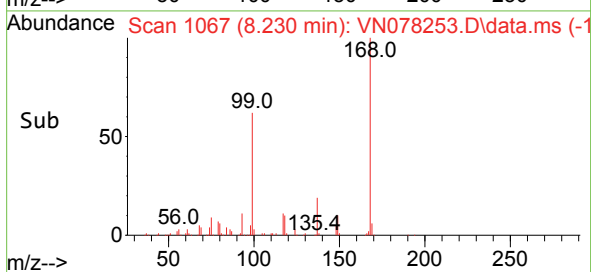

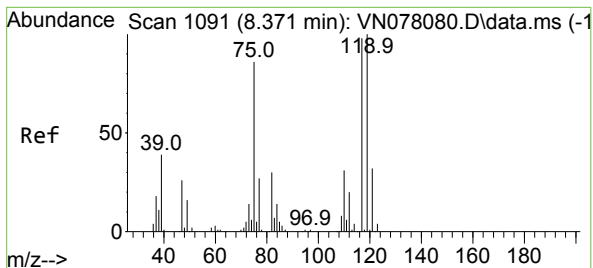

#38

Carbon Tetrachloride

Concen: 6.346 ug/l

RT: 8.235 min Scan# 1068

Delta R.T. -0.135 min


Lab File: VN078253.D

Acq: 16 Jun 2023 12:26

Instrument :

MSVOA_N

ClientSampleId :

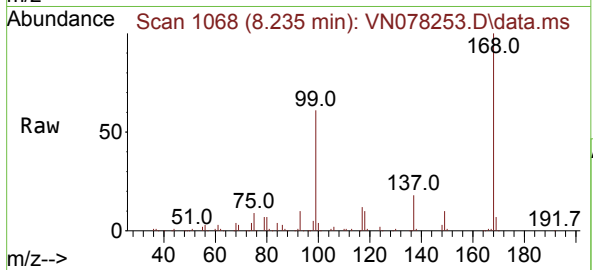




Tgt Ion:117 Resp: 49933

Ion Ratio Lower Upper

117 100

119 5.2 77.3 115.9#

121 0.0 23.3 34.9#

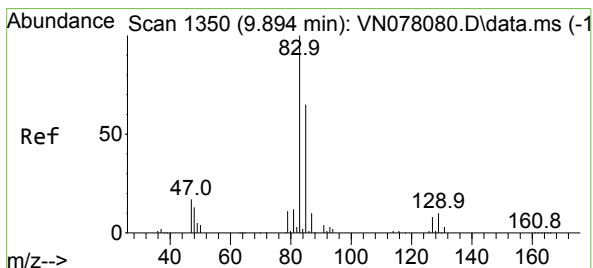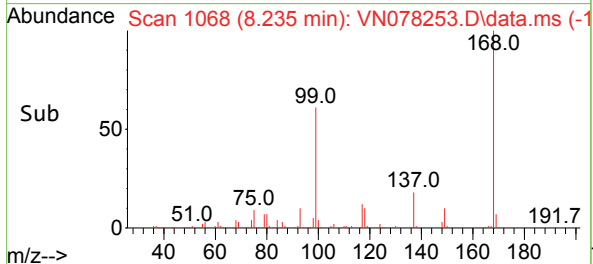

#47

Bromodichloromethane

Concen: 0.845 ug/l

RT: 9.894 min Scan# 1350

Delta R.T. 0.000 min

Lab File: VN078253.D

Acq: 16 Jun 2023 12:26




Tgt Ion: 83 Resp: 6402


Ion Ratio Lower Upper

83 100

85 62.5 49.6 74.4

127 10.0 7.0 10.6


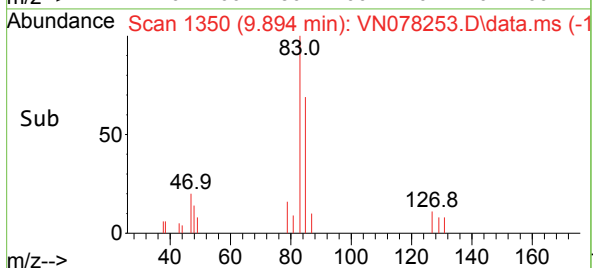
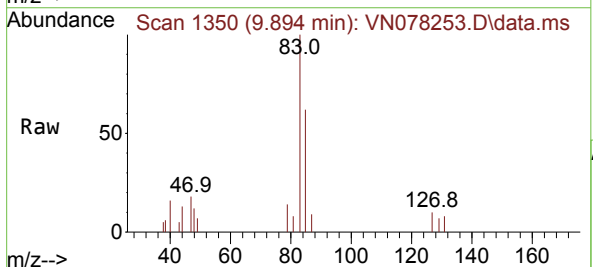





#50
Toluene-d8
Concen: 48.530 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 971870
Ion Ratio Lower Upper
98 100
100 63.4 52.0 78.0

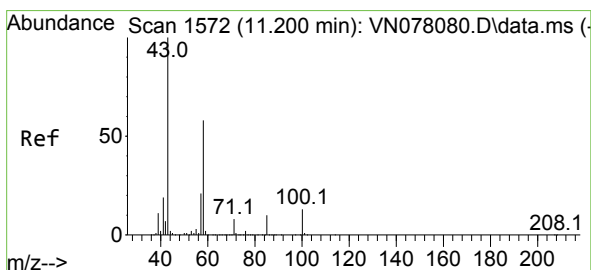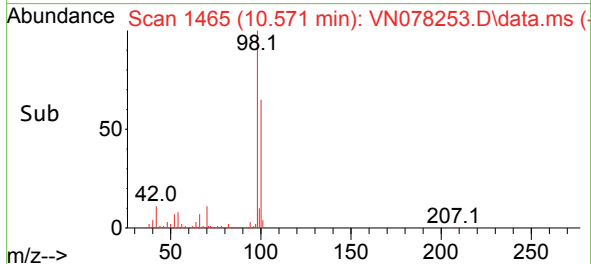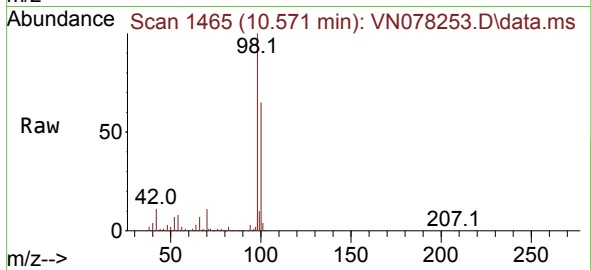

#59
2-Hexanone
Concen: 0.477 ug/l
RT: 11.200 min Scan# 1572
Delta R.T. 0.000 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26

Tgt Ion: 43 Resp: 1945
Ion Ratio Lower Upper
43 100
58 55.8 31.7 95.1





#60

Dibromochloromethane

Concen: 10.794 ug/l

RT: 11.365 min Scan# 1600

Delta R.T. 0.000 min

Lab File: VN078253.D

Acq: 16 Jun 2023 12:26

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:129 Resp: 62756

Ion Ratio Lower Upper

129 100

127 75.7 38.6 116.0

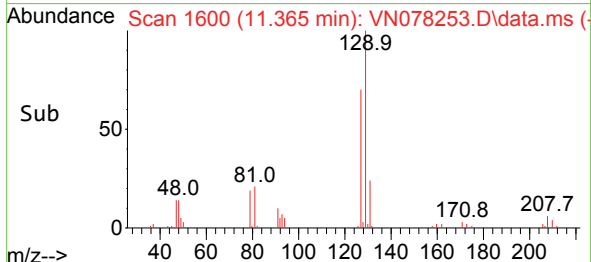

#62

4-Bromofluorobenzene

Concen: 48.257 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. 0.000 min

Lab File: VN078253.D

Acq: 16 Jun 2023 12:26




Tgt Ion: 95 Resp: 300431


Ion Ratio Lower Upper

95 100

174 74.5 0.0 143.8

176 72.4 0.0 135.8

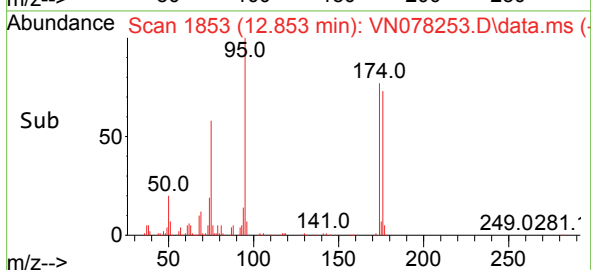



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.871 min Scan# 1

Delta R.T. 0.000 min


Lab File: VN078253.D

Acq: 16 Jun 2023 12:26

Instrument :

MSVOA_N

ClientSampleId :

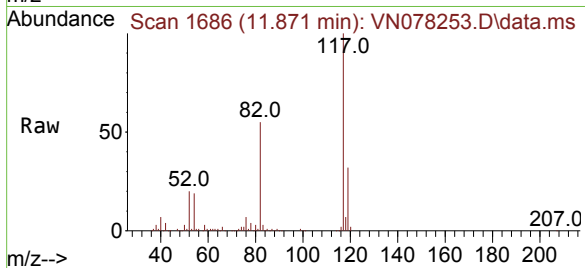




Tgt Ion:117 Resp: 737249

Ion Ratio Lower Upper

117 100

82 55.4 44.0 66.0

119 31.8 25.6 38.4



#71

Bromoform

Concen: 13.030 ug/l

RT: 12.582 min Scan# 1807

Delta R.T. -0.006 min

Lab File: VN078253.D

Acq: 16 Jun 2023 12:26




Tgt Ion:173 Resp: 48831


Ion Ratio Lower Upper

173 100

175 53.1 24.3 73.0


254 0.0 0.0 0.0

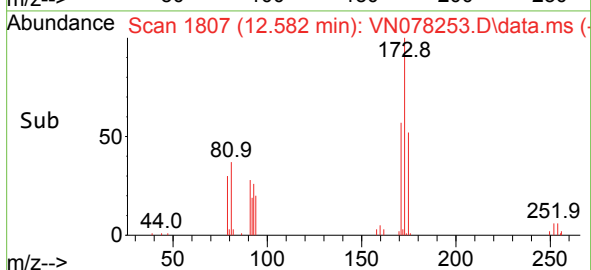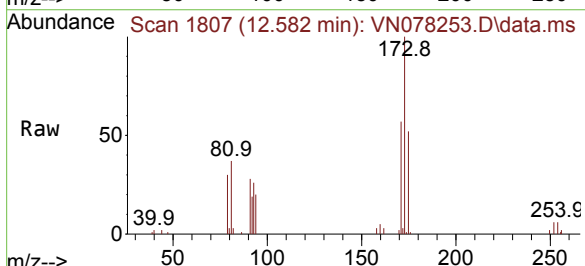



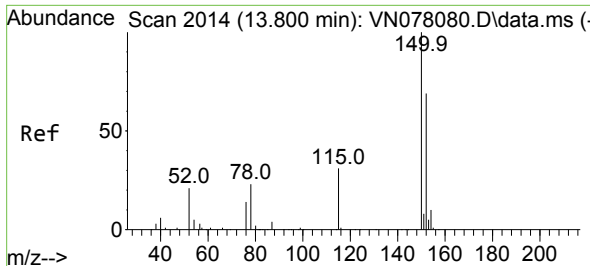


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.800 min Scan# 2014
Delta R.T. 0.000 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26


Instrument :
MSVOA_N
ClientSampleId :

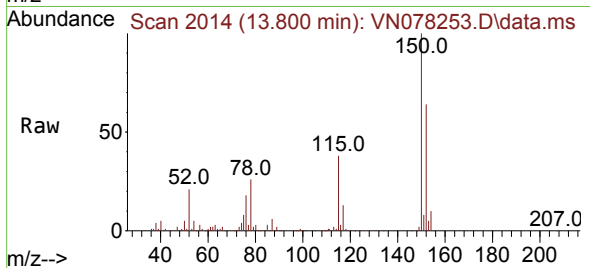



Tgt Ion:152 Resp: 219545
Ion Ratio Lower Upper
152 100
115 61.8 32.3 96.8
150 162.2 0.0 355.8

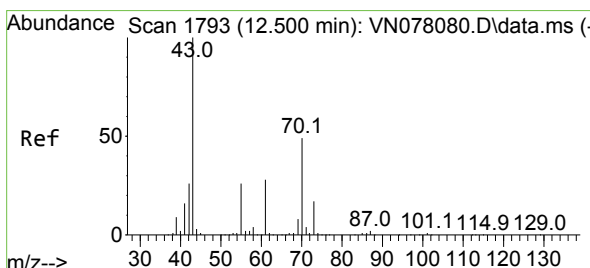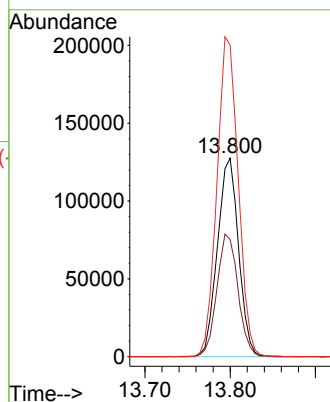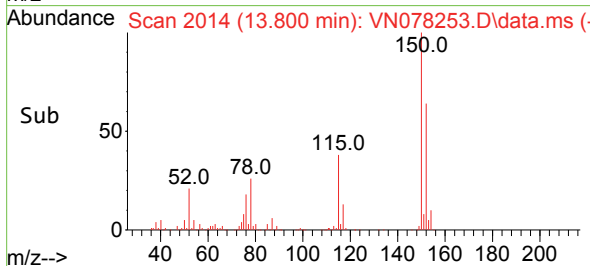


#74
N-ethyl acetate
Concen: 0.207 ug/l
RT: 12.500 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26

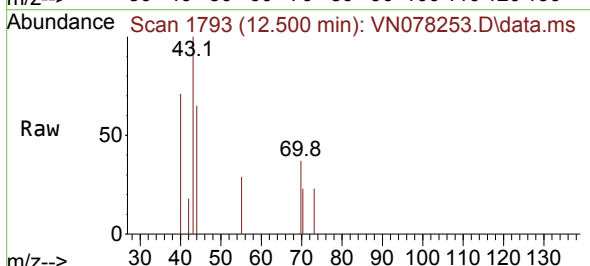

Tgt Ion: 43 Resp: 1416
Ion Ratio Lower Upper
43 100
70 24.4 43.4 65.2#
55 29.4 21.4 32.0
61 0.0 22.8 34.2#



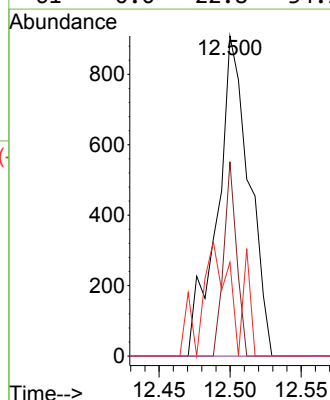
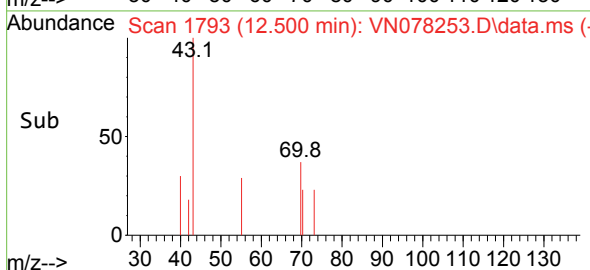


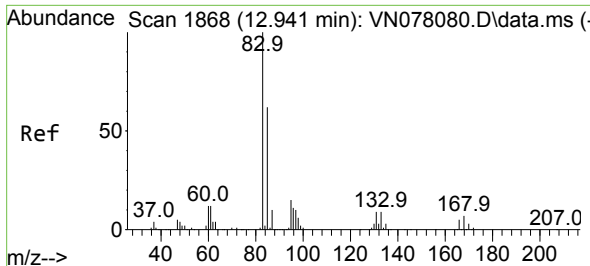

#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.947 min Scan# 1869
Delta R.T. 0.006 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 83 Resp: 495
Ion Ratio Lower Upper
83 100
131 0.0 5.0 15.0#
85 43.6 31.9 95.7

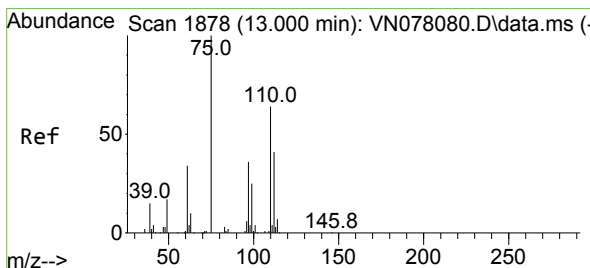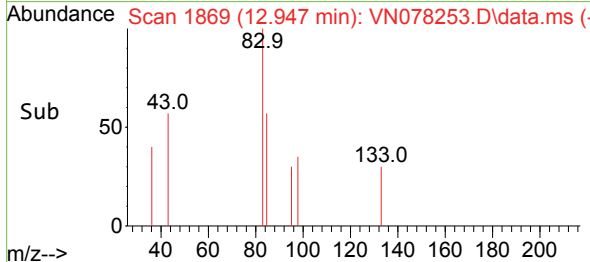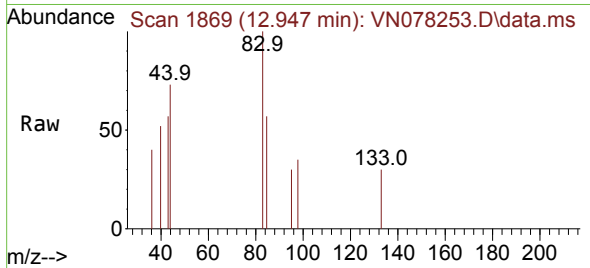

#76
1,2,3-Trichloropropane
Concen: 31.060 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.147 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26

Tgt Ion: 75 Resp: 161204
Ion Ratio Lower Upper
75 100
77 1.1 84.5 253.5#


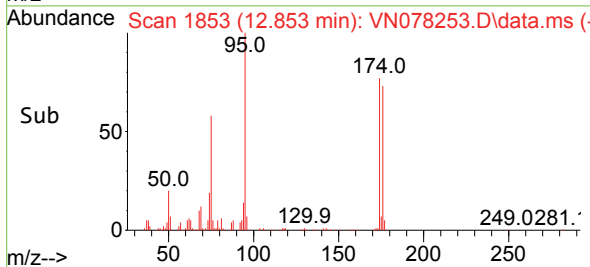

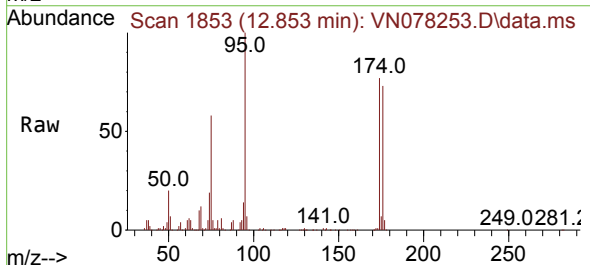


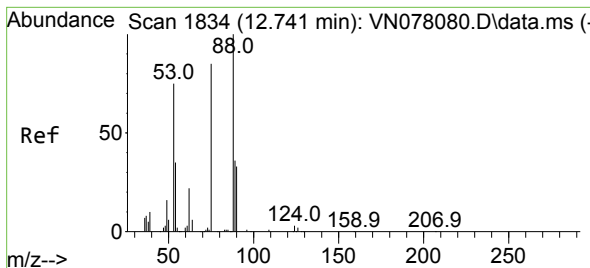

#81
trans-1,4-Dichloro-2-butene
Concen: 95.425 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.112 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 161204
Ion Ratio Lower Upper
75 100
53 0.0 67.4 101.2#
89 0.0 38.8 58.2#

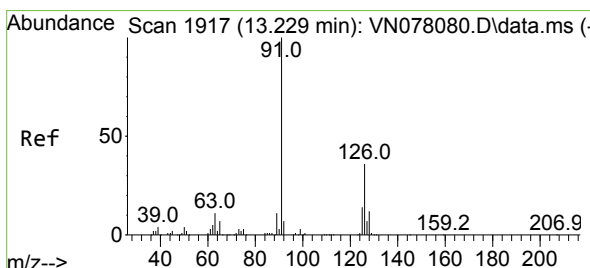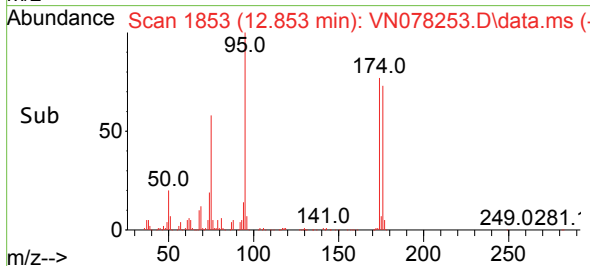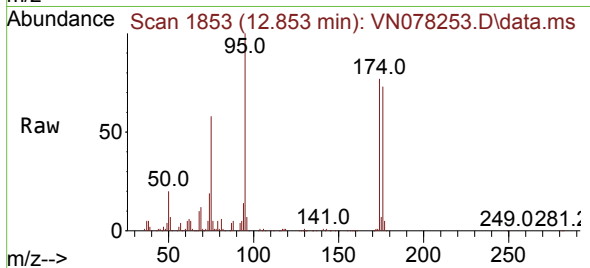

#82
4-Chlorotoluene
Concen: 0.208 ug/l
RT: 13.229 min Scan# 1917
Delta R.T. 0.000 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26

Tgt Ion: 91 Resp: 2832
Ion Ratio Lower Upper
91 100
126 28.7 16.7 50.0


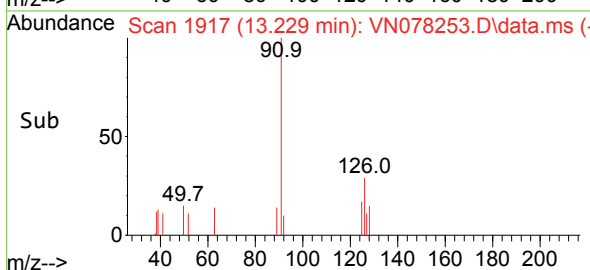

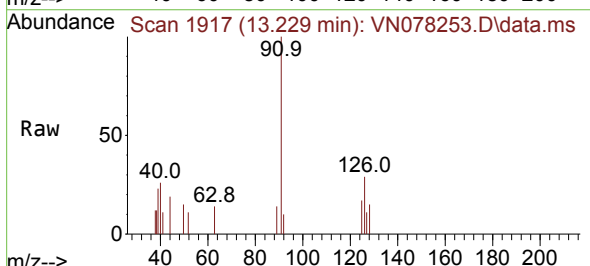


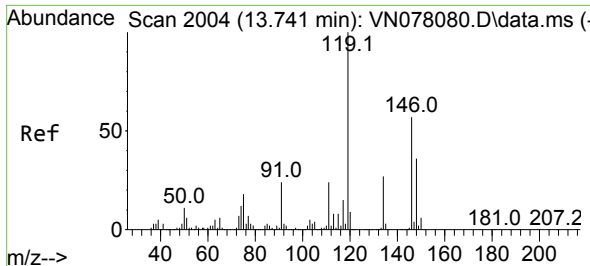

#87
1,3-Dichlorobenzene
Concen: 0.281 ug/l
RT: 13.747 min Scan# 2004
Delta R.T. 0.006 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:146 Resp: 2294
Ion Ratio Lower Upper
146 100
111 40.5 22.1 66.3
148 62.7 32.0 96.0

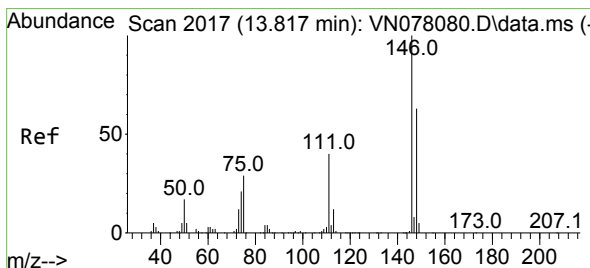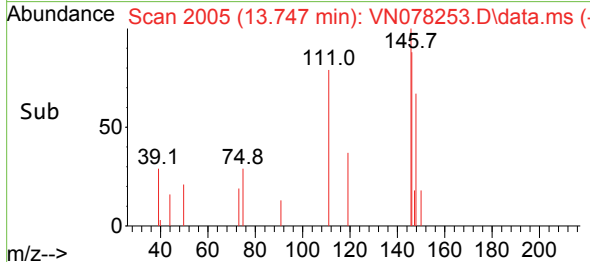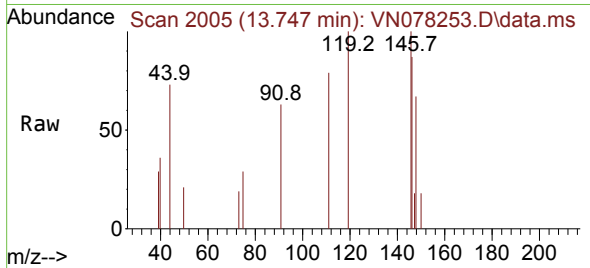

#88
1,4-Dichlorobenzene
Concen: 0.292 ug/l
RT: 13.747 min Scan# 2005
Delta R.T. -0.071 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26

Tgt Ion:146 Resp: 2294
Ion Ratio Lower Upper
146 100
111 40.5 20.6 61.8
148 62.7 31.6 94.8

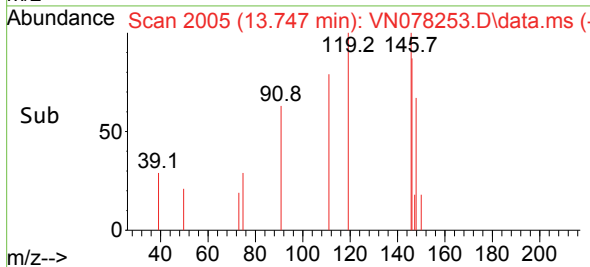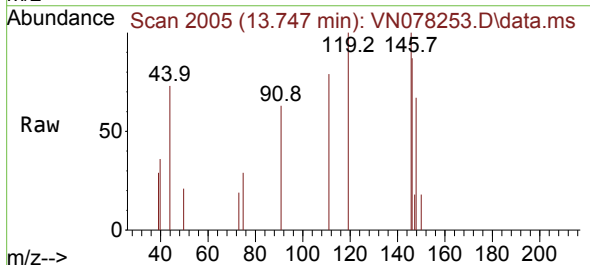



#89

n-Butylbenzene

Concen: 0.325 ug/l

RT: 14.059 min Scan# 2059

Delta R.T. -0.006 min

Lab File: VN078253.D





Acq: 16 Jun 2023 12:26

Instrument :

MSVOA_N

ClientSampleId :

Tgt Ion: 91	Resp:	3983
Ion	Ratio	Lower Upper
91	100	
92	52.2	26.4 79.0
134	20.3	12.6 37.6

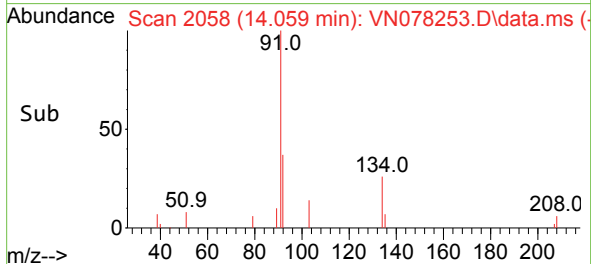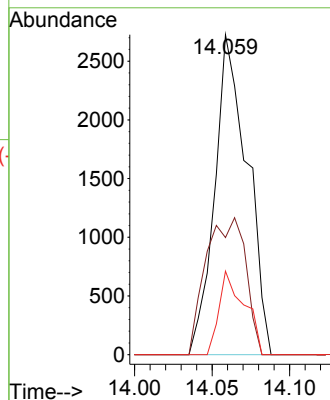

#91

1,2-Dichlorobenzene

Concen: 0.277 ug/l




RT: 14.112 min Scan# 2067


Delta R.T. 0.000 min

Lab File: VN078253.D

Acq: 16 Jun 2023 12:26

Tgt Ion: 146	Resp:	2209
Ion	Ratio	Lower Upper
146	100	
111	25.5	22.0 66.0
148	70.8	31.8 95.3



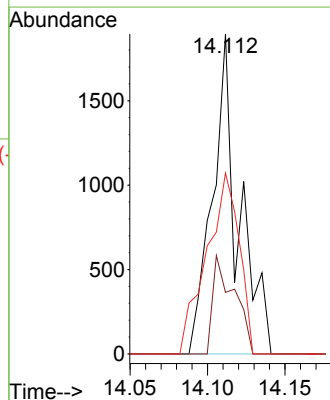





#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.481 ug/l
 RT: 14.735 min Scan# 2173
 Delta R.T. 0.012 min
 Lab File: VN078253.D
 Acq: 16 Jun 2023 12:26




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 495
 Ion Ratio Lower Upper
 75 100
 155 0.0 39.1 117.2#
 157 30.7 50.3 150.9#

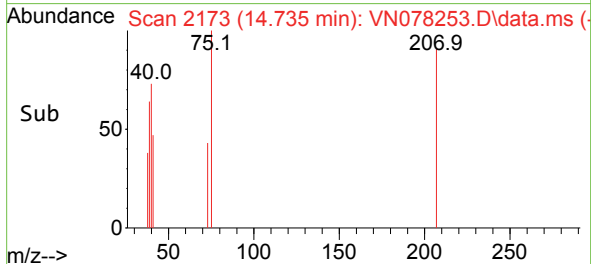

#93
 1,2,4-Trichlorobenzene
 Concen: 0.636 ug/l
 RT: 15.400 min Scan# 2286
 Delta R.T. 0.000 min
 Lab File: VN078253.D
 Acq: 16 Jun 2023 12:26


Tgt Ion: 180 Resp: 1805
 Ion Ratio Lower Upper
 180 100
 182 107.2 46.1 138.2
 145 40.8 16.6 49.8








#94
Hexachlorobutadiene
Concen: Below Cal
RT: 15.506 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26


Instrument :
MSVOA_N
ClientSampleId :

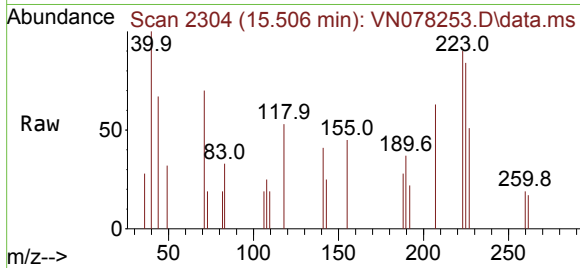



Tgt Ion	Ratio	Lower	Upper
225	100		
223	69.1	31.3	93.8
227	69.7	31.9	95.9

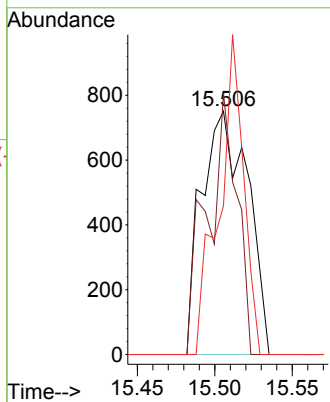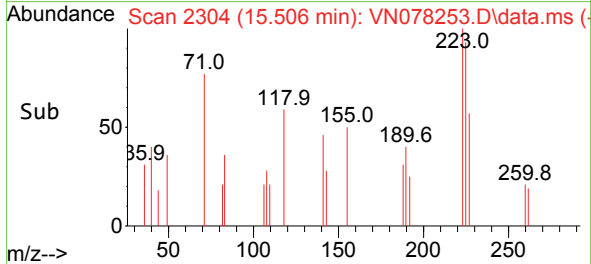


#95
Naphthalene
Concen: 0.729 ug/l
RT: 15.647 min Scan# 2328
Delta R.T. 0.000 min
Lab File: VN078253.D
Acq: 16 Jun 2023 12:26

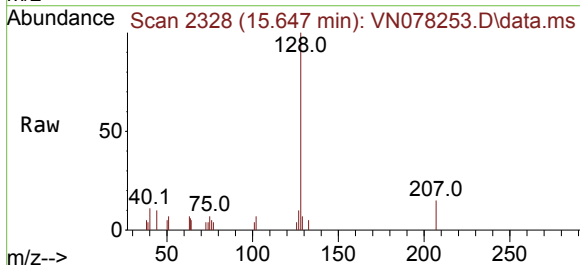


Tgt Ion	Ratio	Lower	Upper
128	100		
127	12.9	10.0	15.0
129	8.6	8.7	13.1

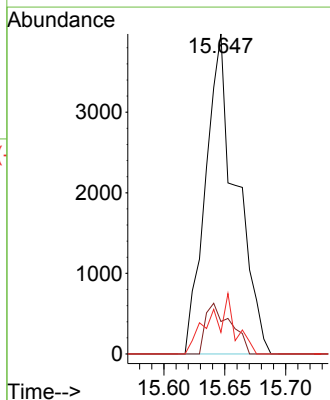

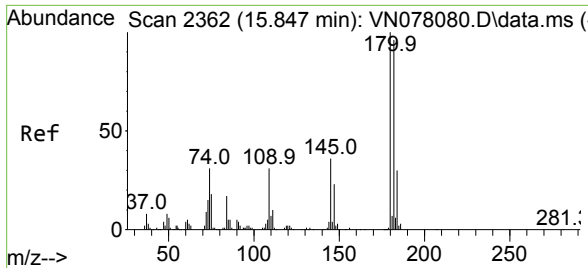

#96
 1,2,3-Trichlorobenzene
 Concen: 0.637 ug/l
 RT: 15.853 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VN078253.D
 Acq: 16 Jun 2023 12:26

Instrument :
 MSVOA_N
 ClientSampleId :

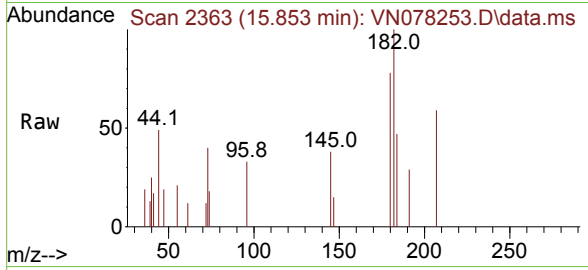

Tgt Ion:	180	Resp:	2022
Ion	Ratio	Lower	Upper
180	100		
182	135.2	46.2	138.6
145	56.0	17.5	52.6#

