
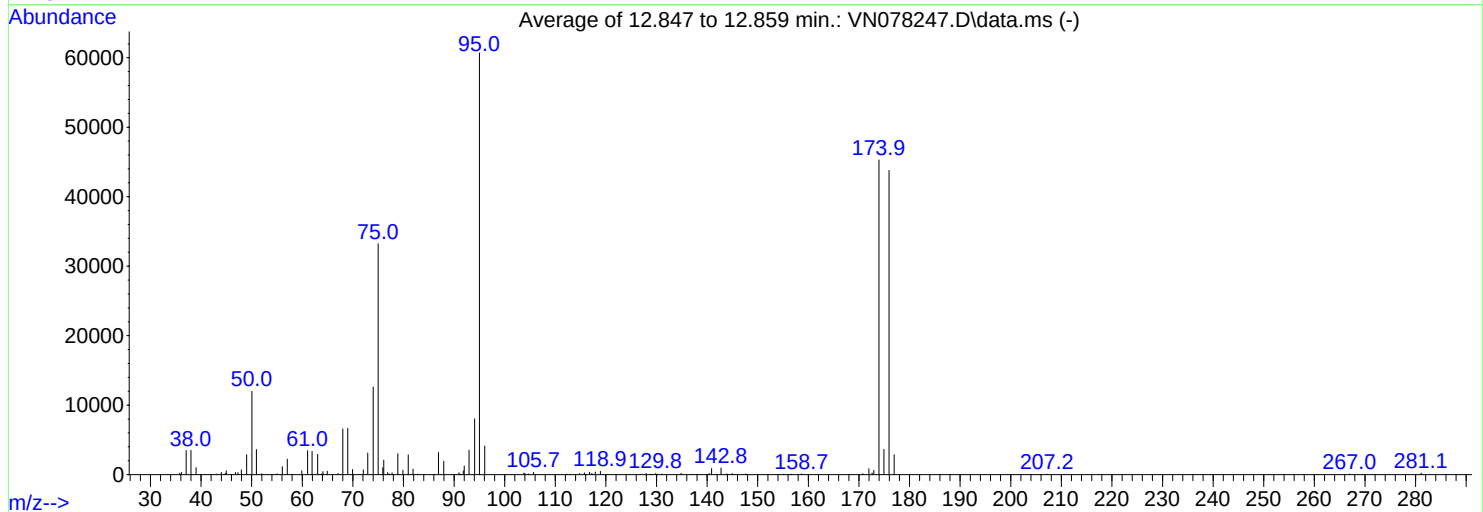


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061623\
Data File : VN078247.D
Acq On : 16 Jun 2023 08:23
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
Title : SW846 8260
Last Update : Wed Jun 07 05:05:00 2023

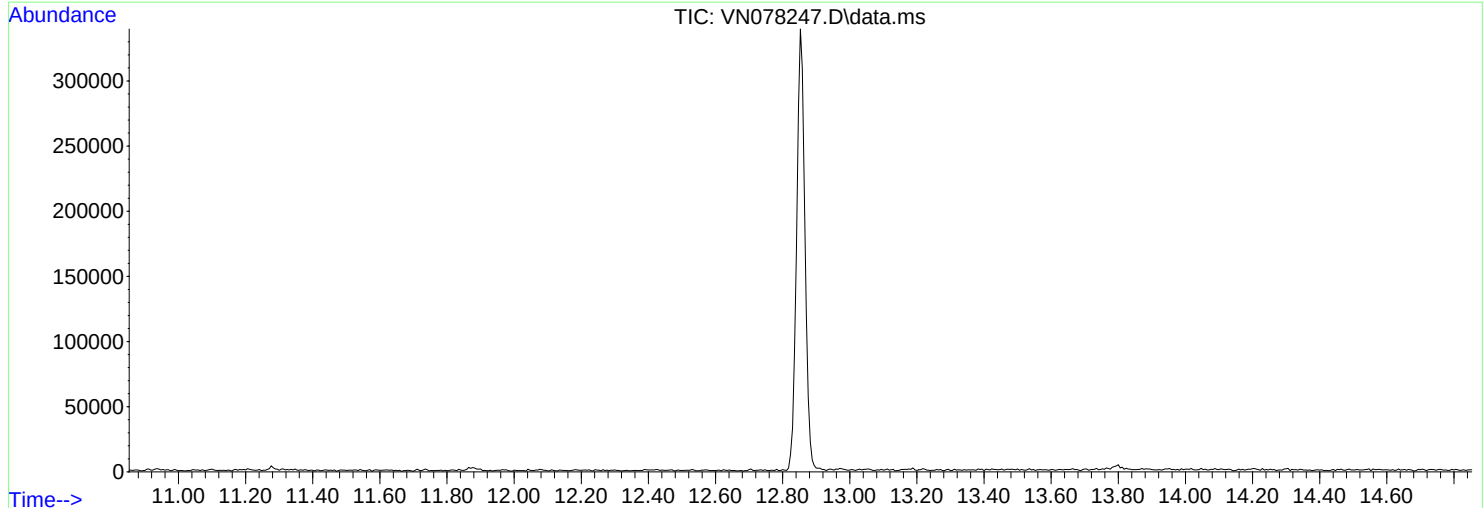

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	12007	PASS
75	95	30	60	54.7	33232	PASS
95	95	100	100	100.0	60704	PASS
96	95	5	9	6.8	4113	PASS
173	174	0.00	2	1.4	628	PASS
174	95	50	100	74.6	45285	PASS
175	174	5	9	8.1	3650	PASS
176	174	95	101	96.7	43795	PASS
177	176	5	9	6.6	2869	PASS

Average of 12.847 to 12.859 min.: VN078247.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	214	47.30	301	61.95	3371	74.00	1261
36.10	324	47.95	697	63.05	2928	75.00	3323
37.05	3468	49.00	2877	63.80	118	75.90	98
38.00	3499	50.05	12007	64.10	429	76.10	209
39.00	1006	50.95	3625	64.95	480	76.85	309
39.90	40	51.95	115	67.05	159	77.00	73
43.00	96	55.00	151	68.00	6593	77.20	95
44.00	332	56.05	1154	69.00	6668	77.75	250
44.80	210	57.05	2234	69.95	728	78.90	3017
45.00	549	59.90	561	72.05	694	79.90	651
46.80	309	61.05	3459	72.95	3107	80.95	2866

Average of 12.847 to 12.859 min.: VN078247.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.90	801	96.05	4113	117.30	99	140.90	880
82.80	74	103.80	224	117.90	368	141.90	72
86.90	3193	104.00	189	118.90	485	142.75	975
87.95	1927	104.70	101	127.95	190	143.90	120
90.95	269	105.70	330	128.90	73	144.95	165
91.20	95	112.20	77	129.85	197	147.65	120
91.80	565	113.00	50	130.20	66	147.90	56
92.00	1255	114.80	165	131.10	93	150.00	73
92.95	3518	115.75	252	134.85	191	155.10	80
94.05	8047	116.75	349	136.90	54	156.70	68
95.00	60704	117.10	131	140.40	156	158.70	113

Average of 12.847 to 12.859 min.: VN078247.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
170.75	150						
171.95	857						
172.60	259						
172.95	628						
173.95	45285						
174.95	3650						
175.95	43795						
176.95	2869						
207.20	71						
267.00	87						
281.10	240						

Instrument :

MSVOA_N

ClientSampleId :

BFB