


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061625\
Data File : VN087016.D
Acq On : 16 Jun 2025 08:39
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
Title : SW846 8260
Last Update : Sat Jun 07 02:12:50 2025

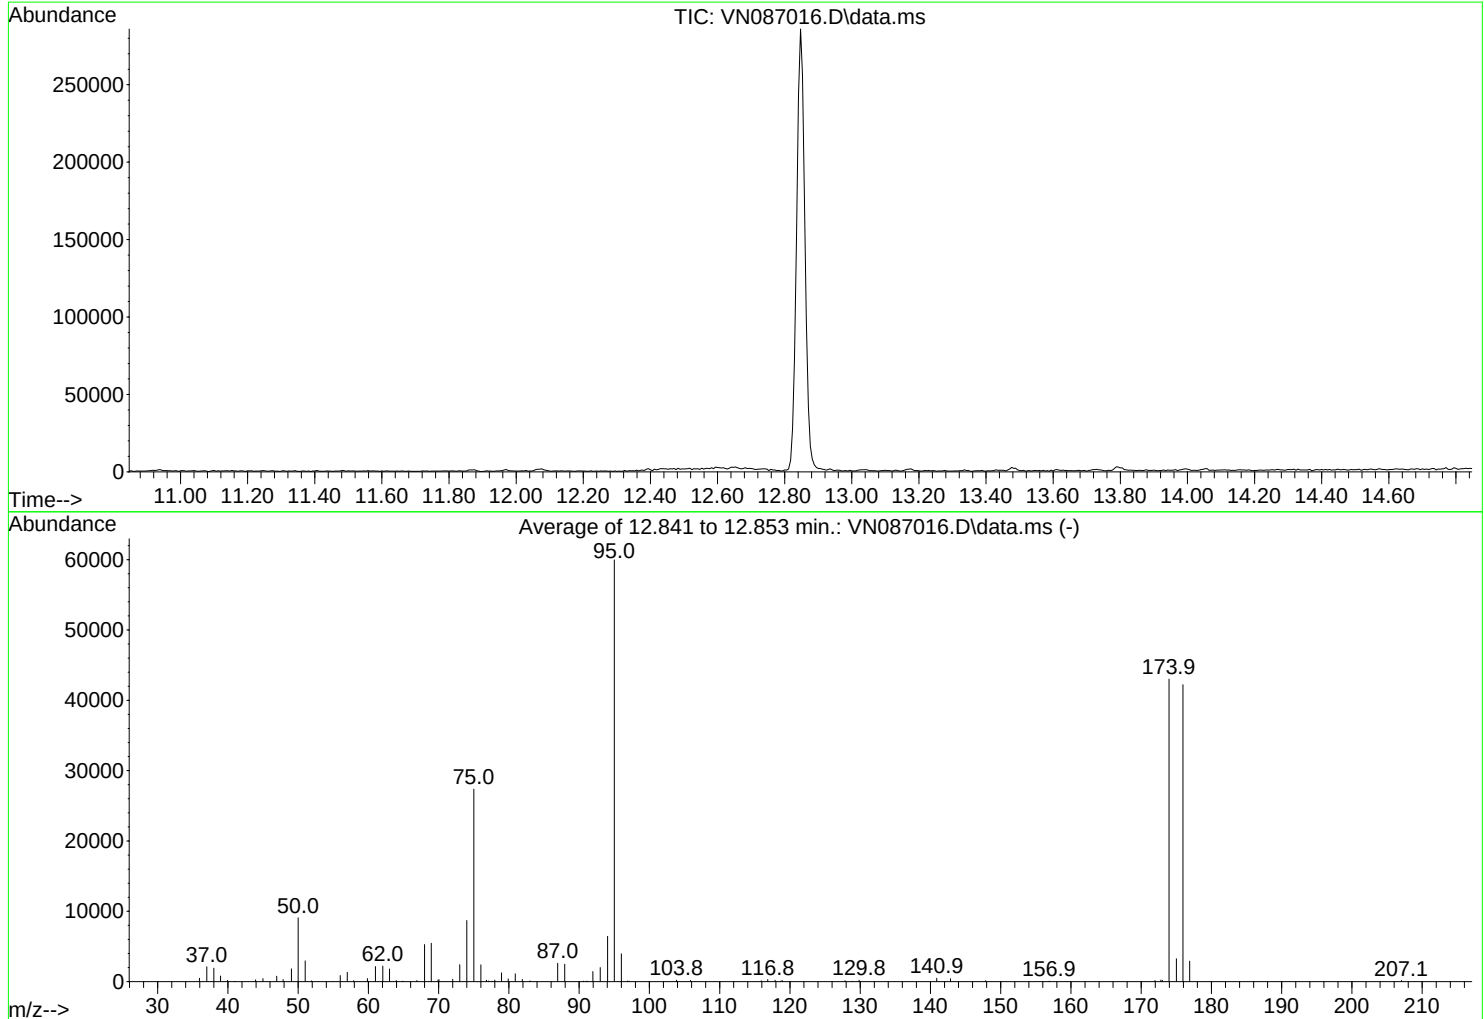

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	9076	PASS
75	95	30	60	45.6	27371	PASS
95	95	100	100	100.0	59973	PASS
96	95	5	9	6.6	3959	PASS
173	174	0.00	2	0.5	223	PASS
174	95	50	100	71.7	43013	PASS
175	174	5	9	7.6	3259	PASS
176	174	95	101	98.2	42235	PASS
177	176	5	9	6.9	2913	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	483	50.00	9076	63.95	167	76.00	239
37.00	2106	51.00	2962	64.90	66	76.80	209
38.00	1909	51.90	109	66.90	169	77.10	101
38.95	789	54.95	18	68.00	5282	77.60	5
39.95	181	56.00	861	68.95	5470	78.00	238
41.00	54	57.00	1314	69.90	223	78.95	1262
43.95	255	57.90	129	70.05	293	79.90	395
45.00	444	59.85	441	72.00	335	80.90	1115
46.95	765	61.00	2150	73.00	2411	81.90	325
47.85	303	62.05	2199	74.00	8701	83.00	116
49.05	1829	63.00	1794	75.00	27371	86.95	2623

Average of 12.841 to 12.853 min.: VN087016.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.95	2473	103.85	213	142.85	418		
90.60	60	105.85	188	147.85	126		
91.00	62	115.90	116	156.90	60		
91.20	56	116.85	307	171.95	152		
91.95	1435	117.90	217	172.80	223		
93.00	2009	118.70	58	173.00	180		
94.05	6448	118.90	195	173.95	43013		
95.00	59973	127.85	142	175.00	3259		
96.00	3959	128.90	52	175.95	42235		
96.90	91	129.85	198	176.90	2913		
97.10	71	140.90	475	207.05	159		

Instrument :

MSVOA_N

ClientSampleId :

BFB