



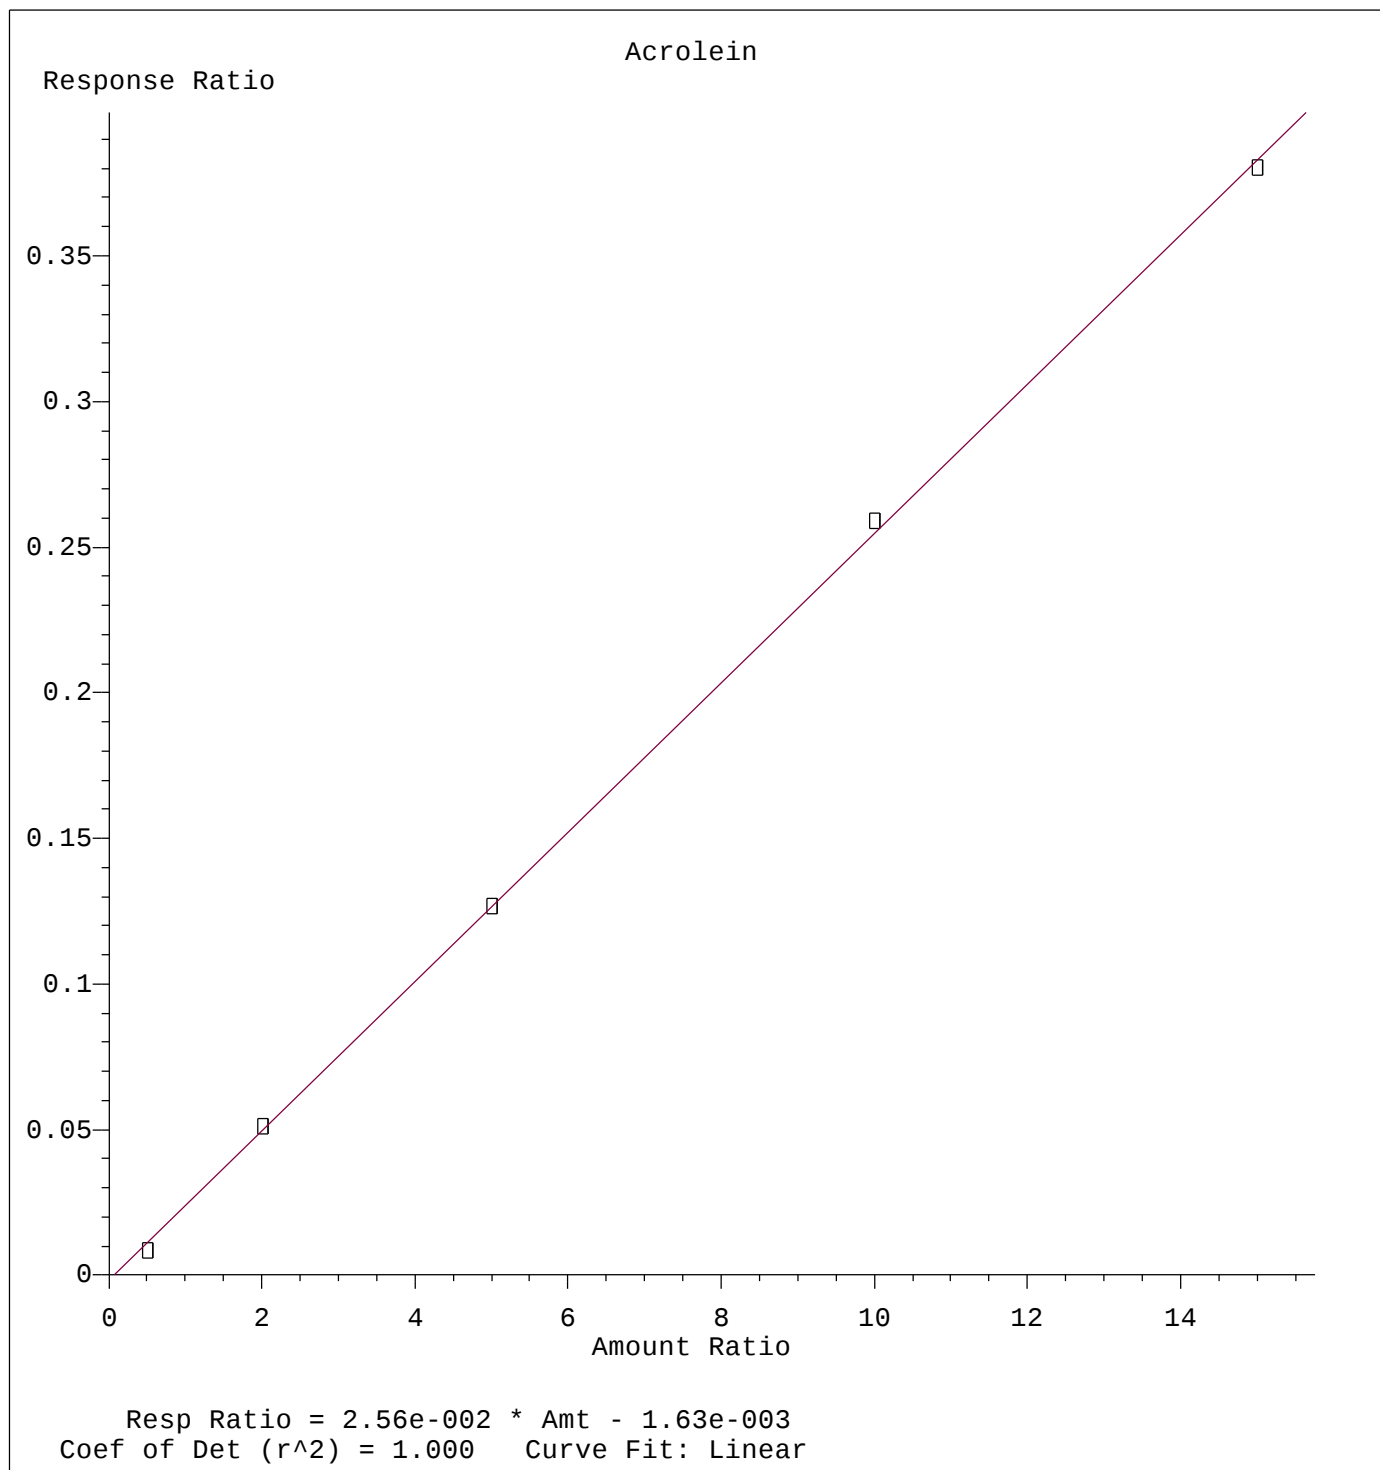


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061719W.M
Calibration Table Last Updated: Tue Jun 18 04:23:59 2019

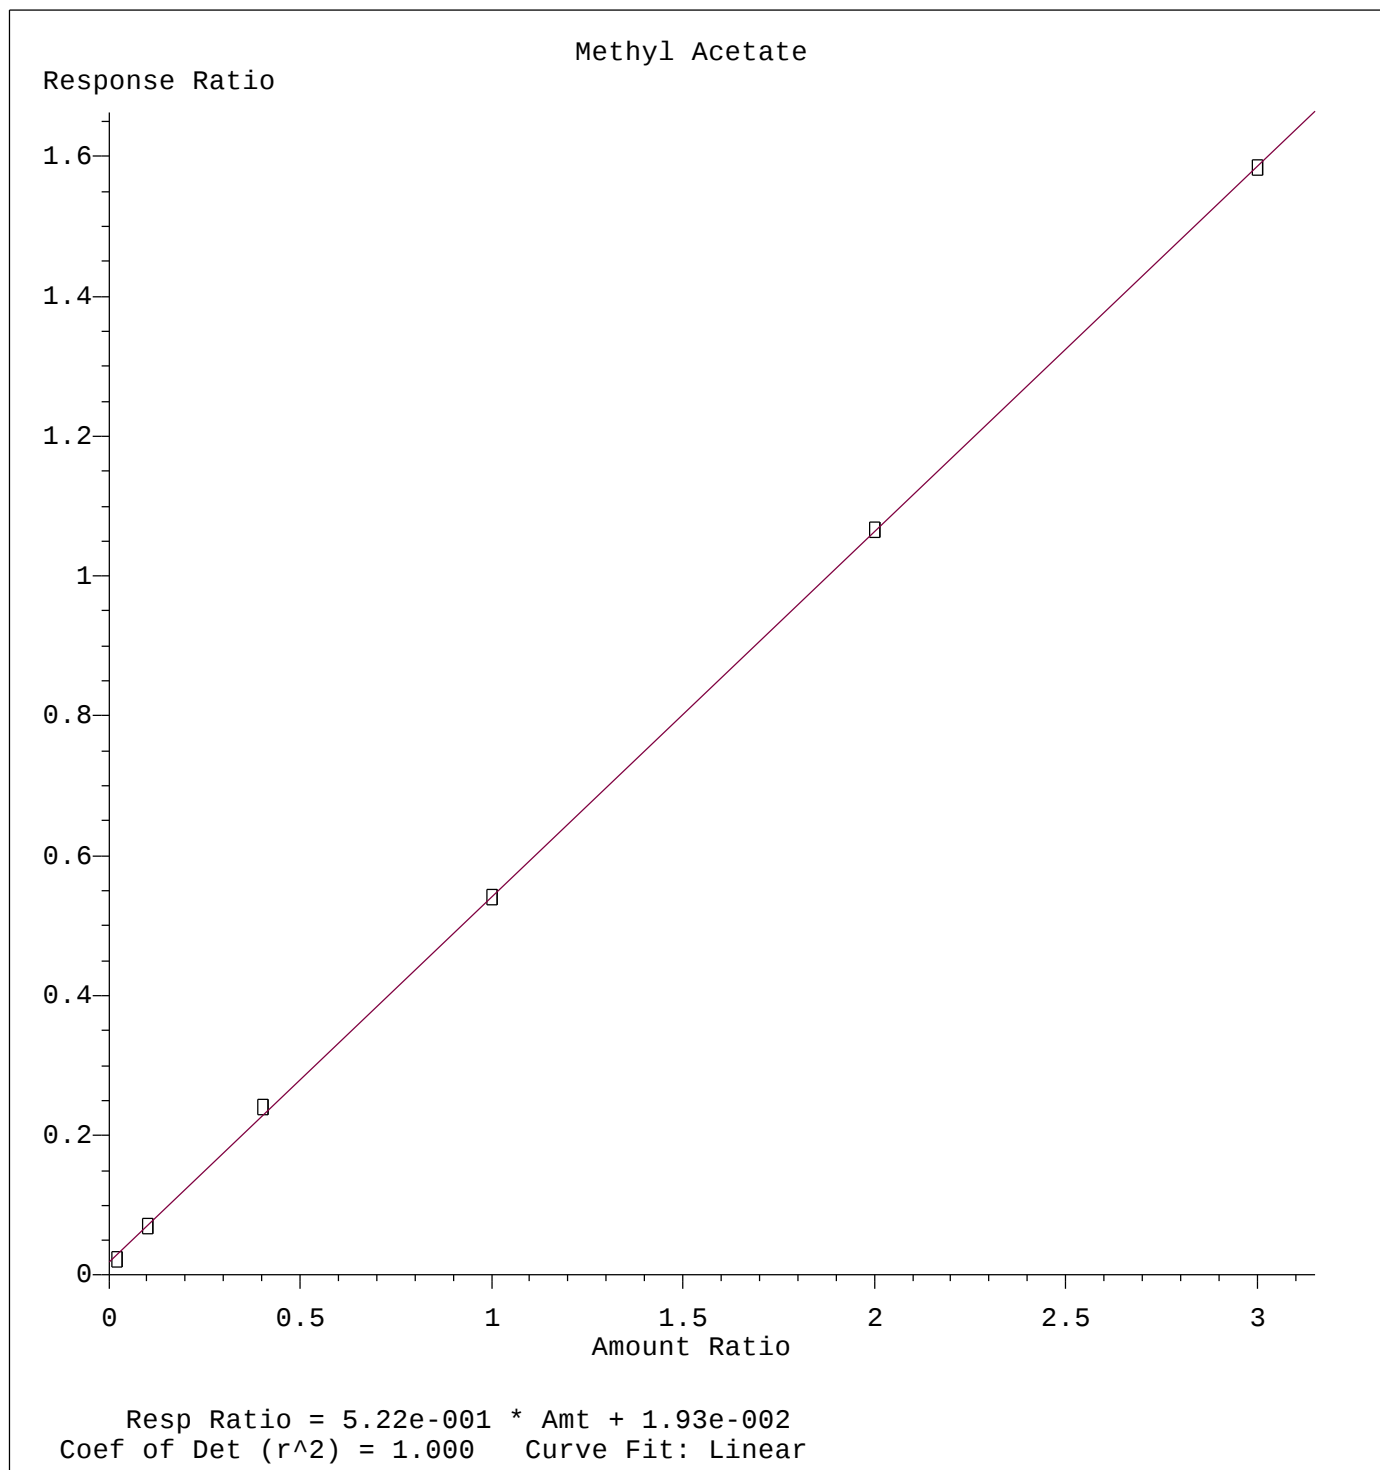

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061719W.M
Calibration Table Last Updated: Tue Jun 18 04:23:59 2019

2-Chloroethyl Vinyl ether

Response Ratio

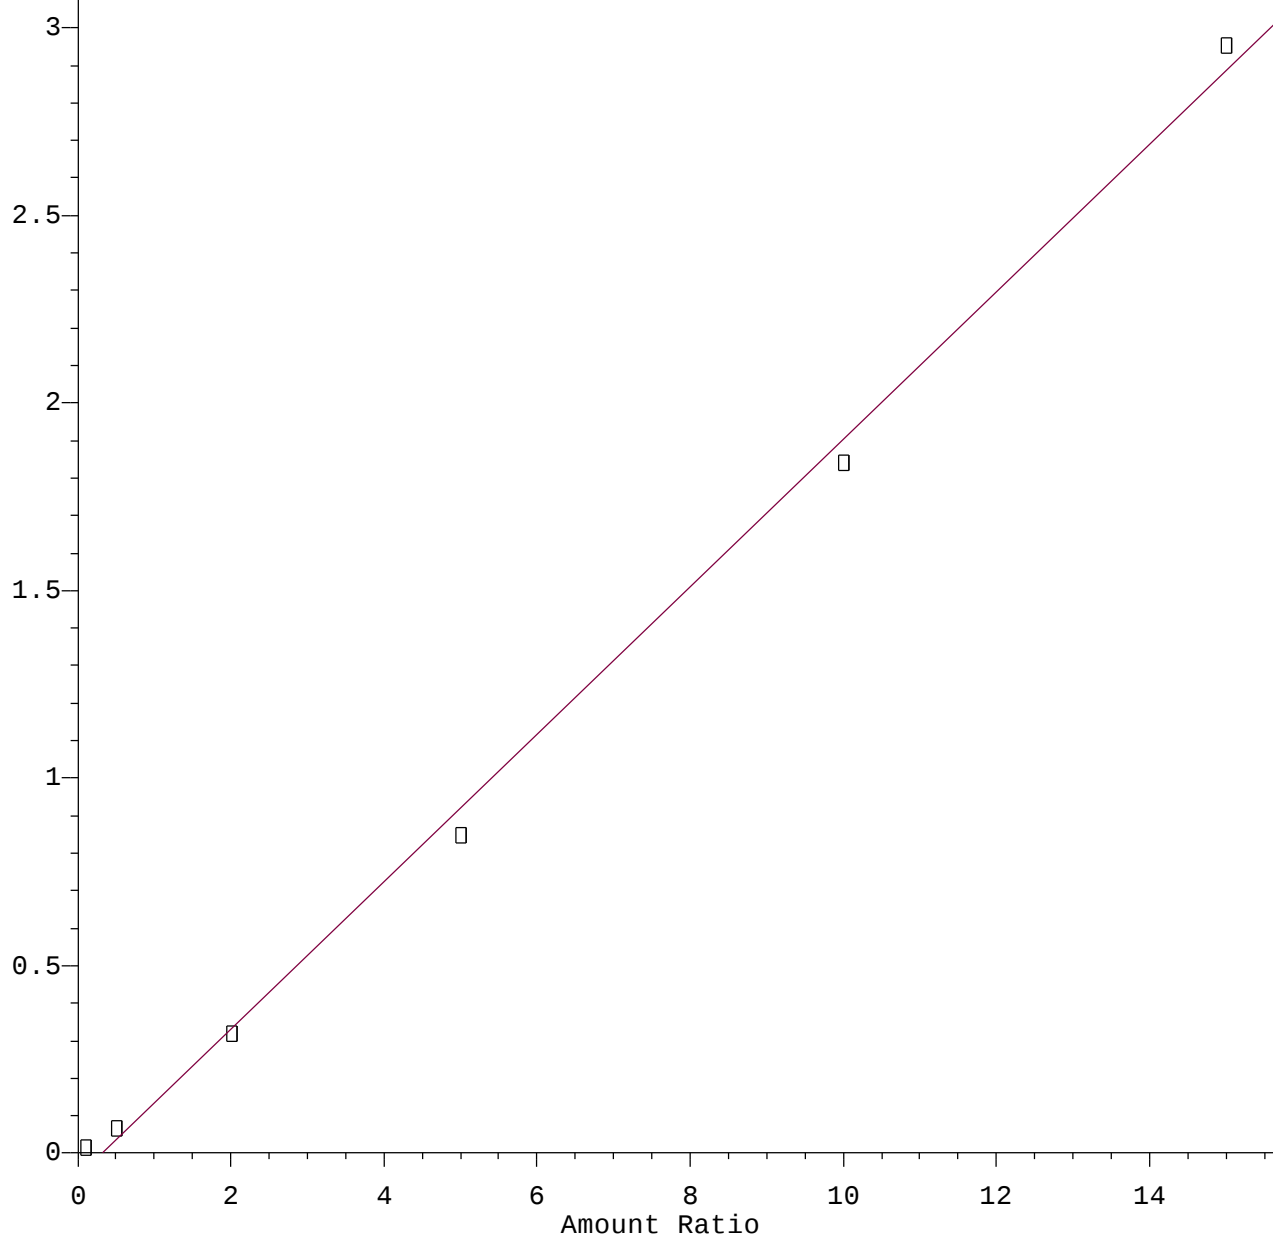


Resp Ratio = $1.96 \times 10^{-1} \times \text{Amt} - 6.20 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061719W.M
Calibration Table Last Updated: Tue Jun 18 04:23:59 2019

Isopropylbenzene

Response Ratio

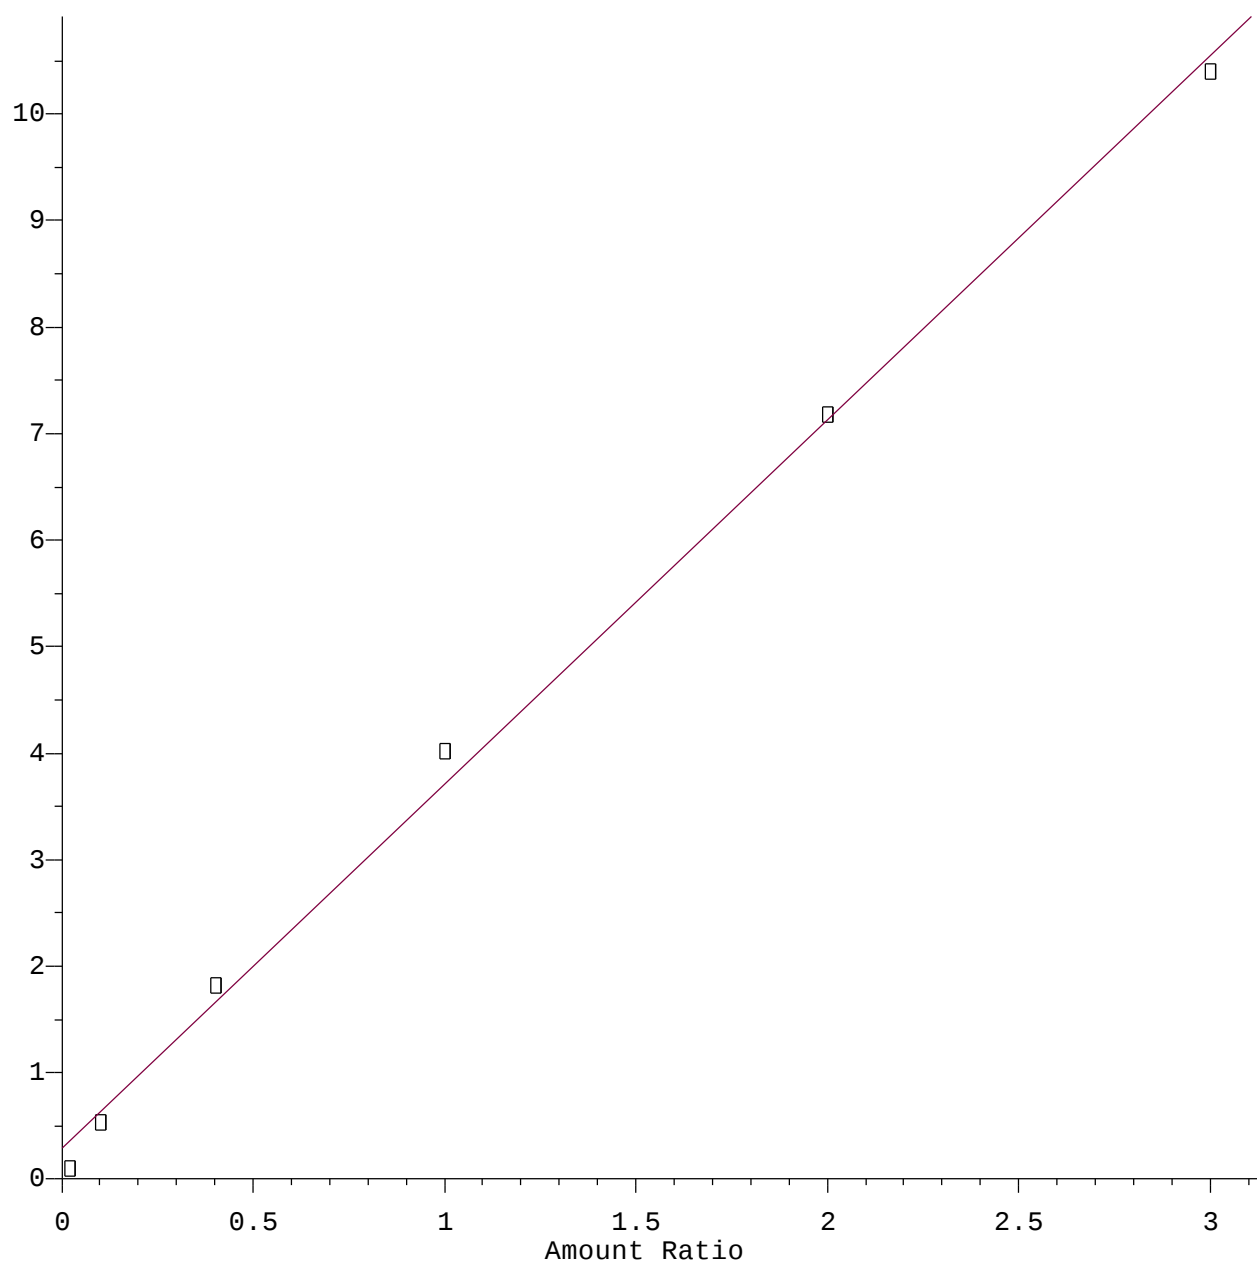


Resp Ratio = $3.42 \times 10^0 * \text{Amt} + 2.89 \times 10^{-1}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061719W.M
Calibration Table Last Updated: Tue Jun 18 04:23:59 2019


1,1,2,2-Tetrachloroethane

Response Ratio

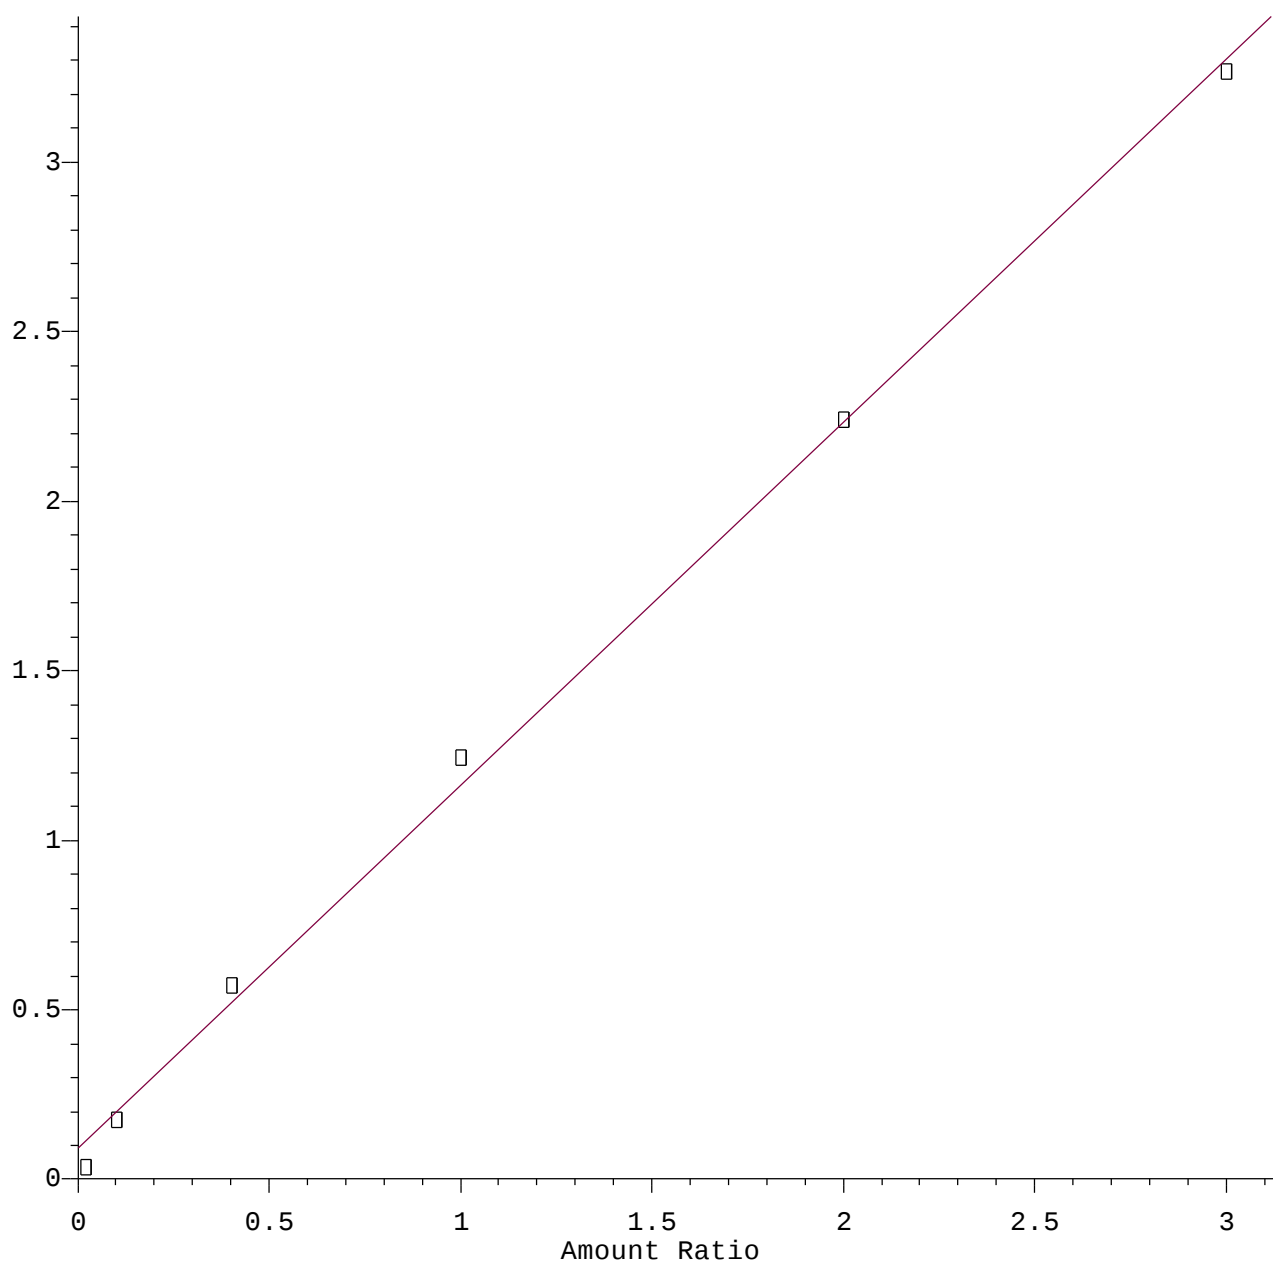

Resp Ratio = 1.07×10^0 * Amt + 9.08×10^{-2}
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061719W.M
Calibration Table Last Updated: Tue Jun 18 04:23:59 2019

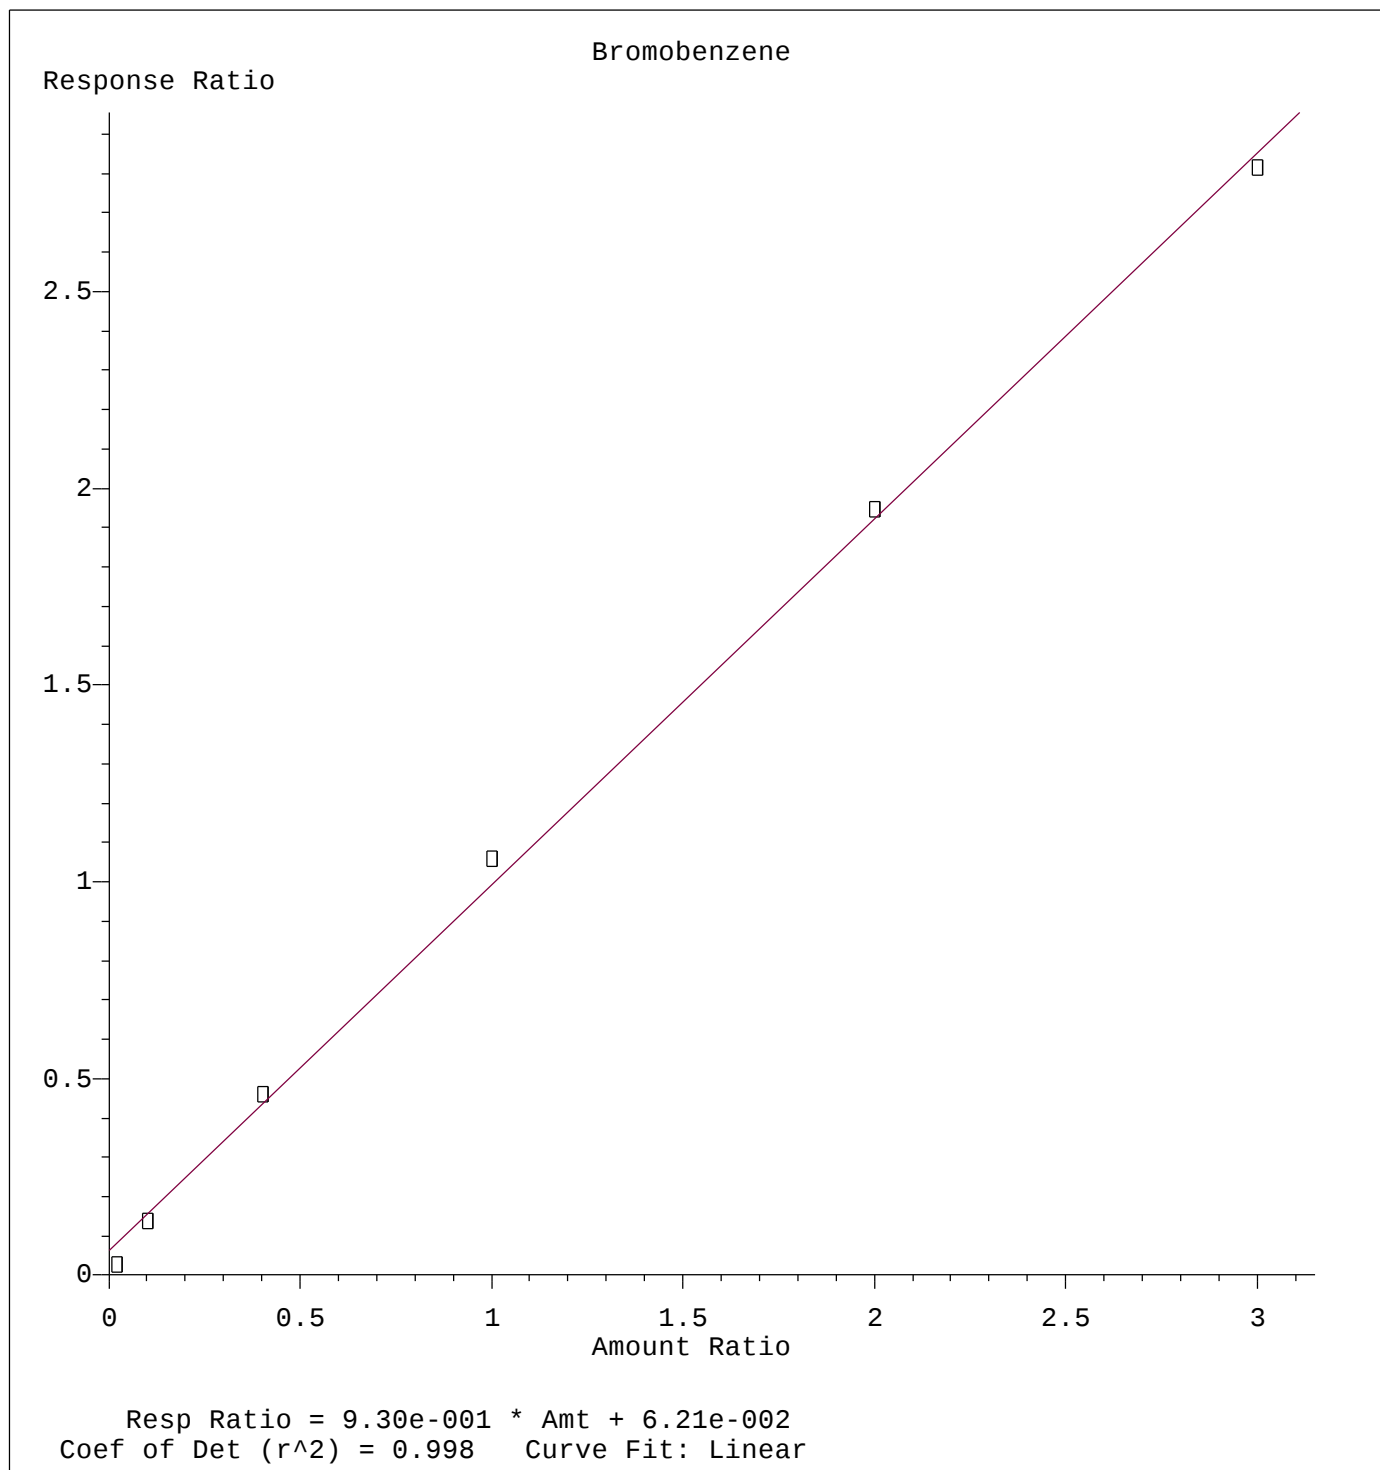

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061719W.M
Calibration Table Last Updated: Tue Jun 18 04:23:59 2019

2-Chlorotoluene

Response Ratio

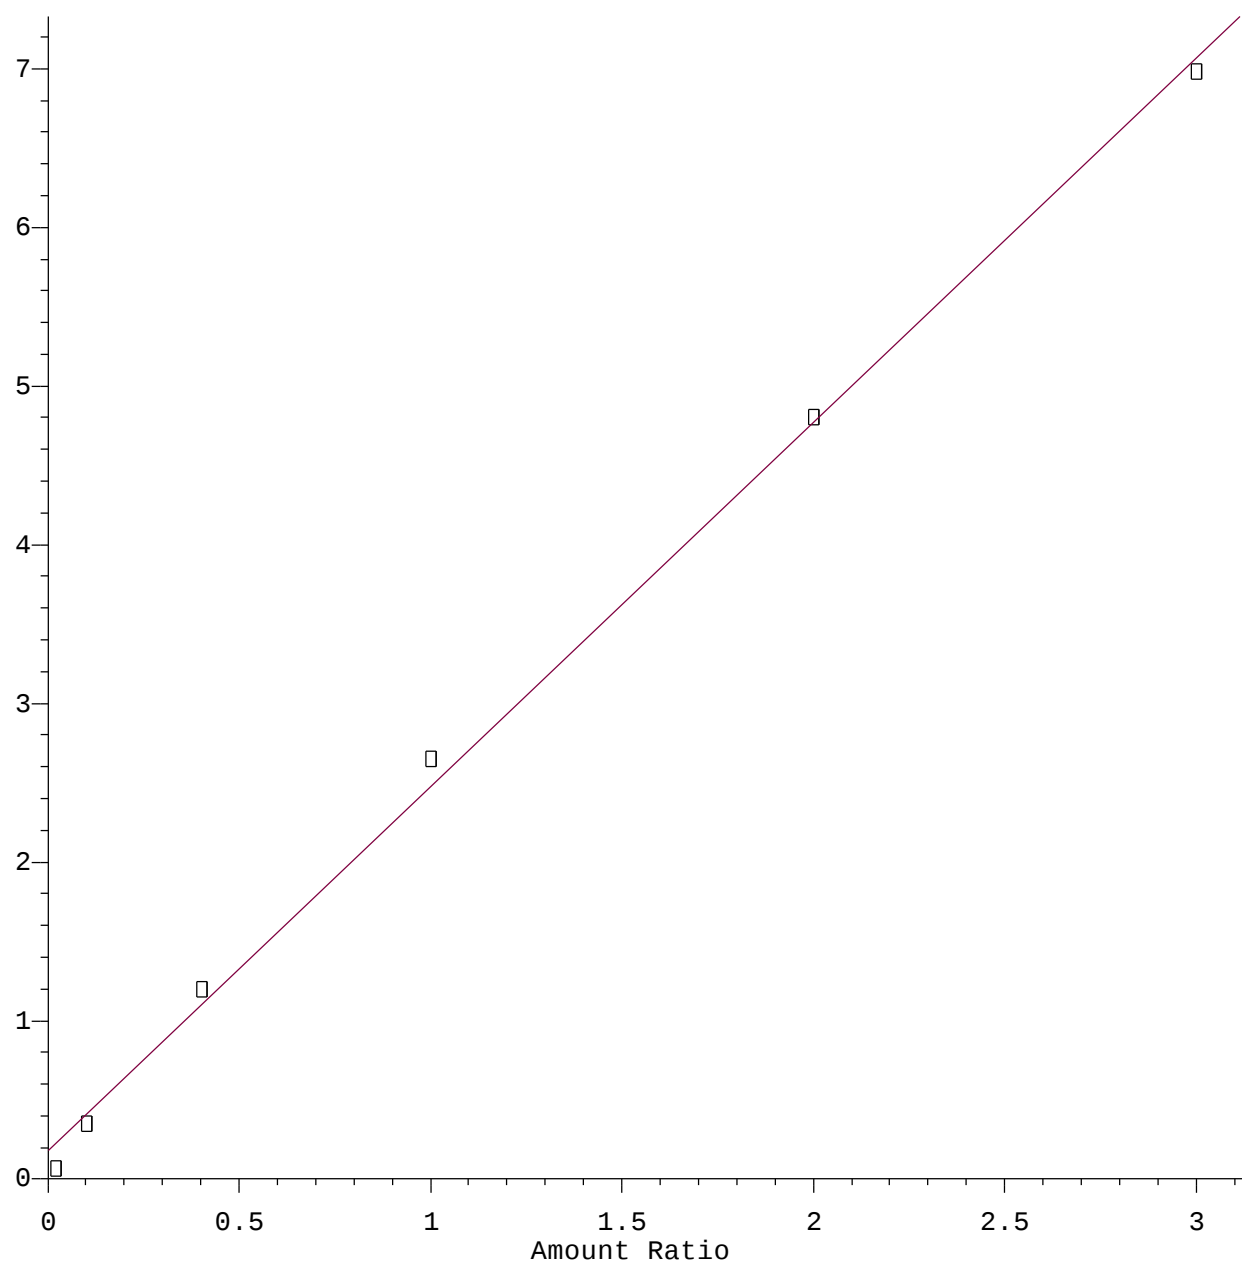


Resp Ratio = 2.30e+000 * Amt + 1.77e-001
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061719W.M
Calibration Table Last Updated: Tue Jun 18 04:23:59 2019


tert-Butylbenzene

Response Ratio

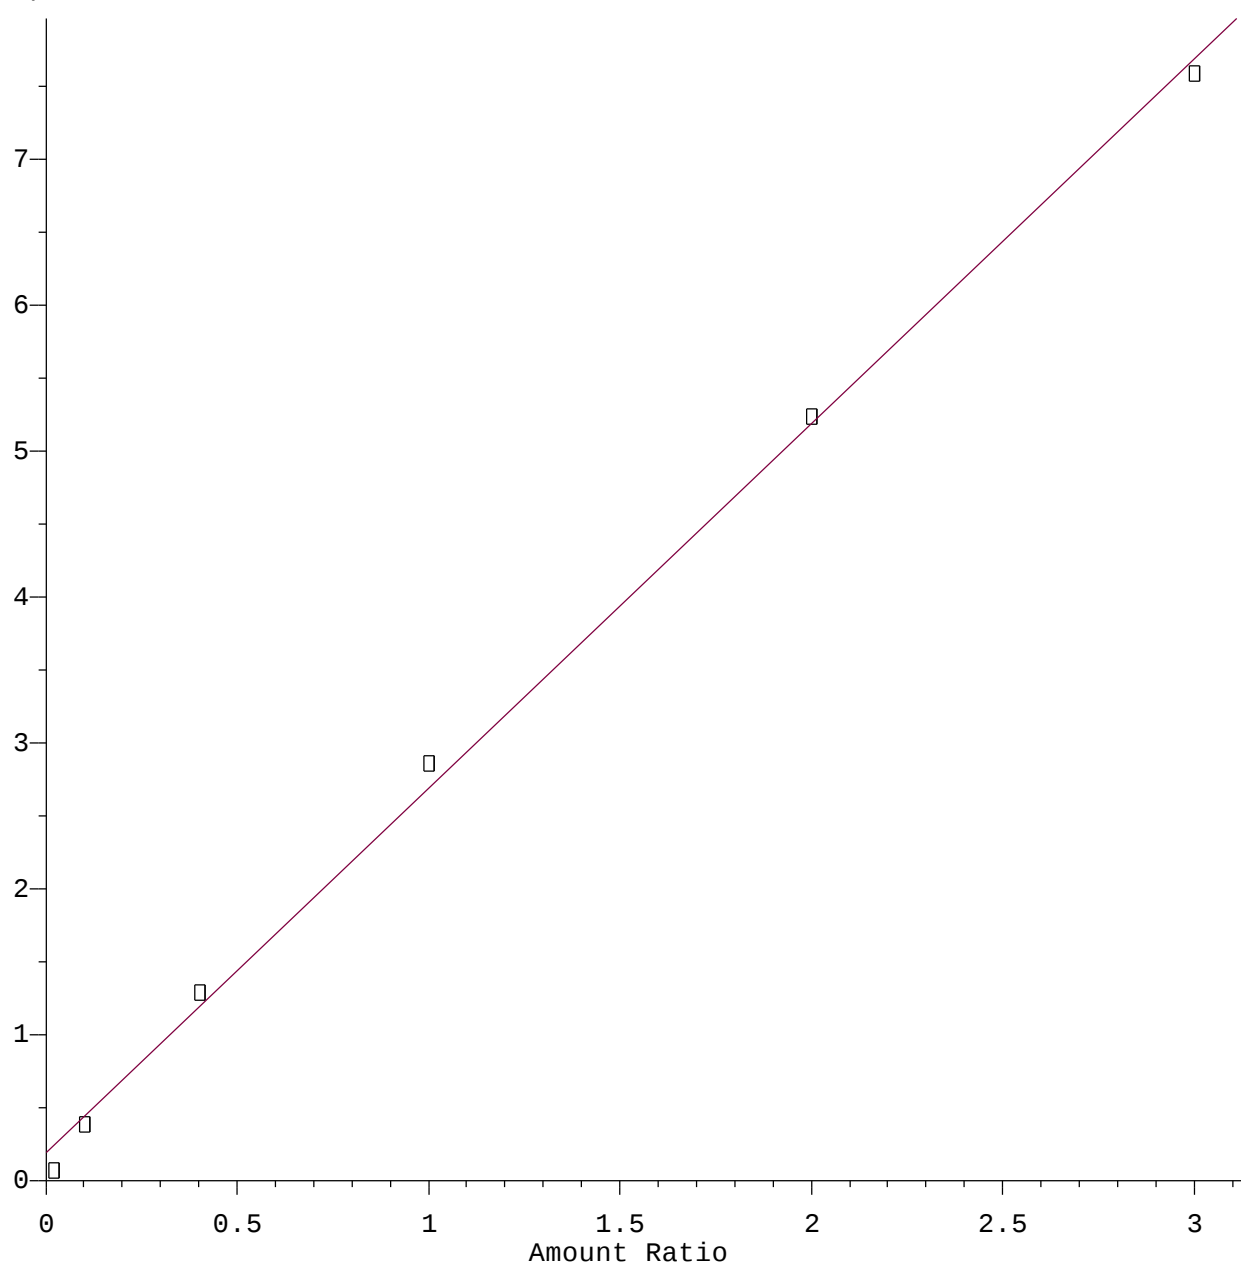

Resp Ratio = 2.50e+000 * Amt + 1.90e-001
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061719W.M
Calibration Table Last Updated: Tue Jun 18 04:23:59 2019

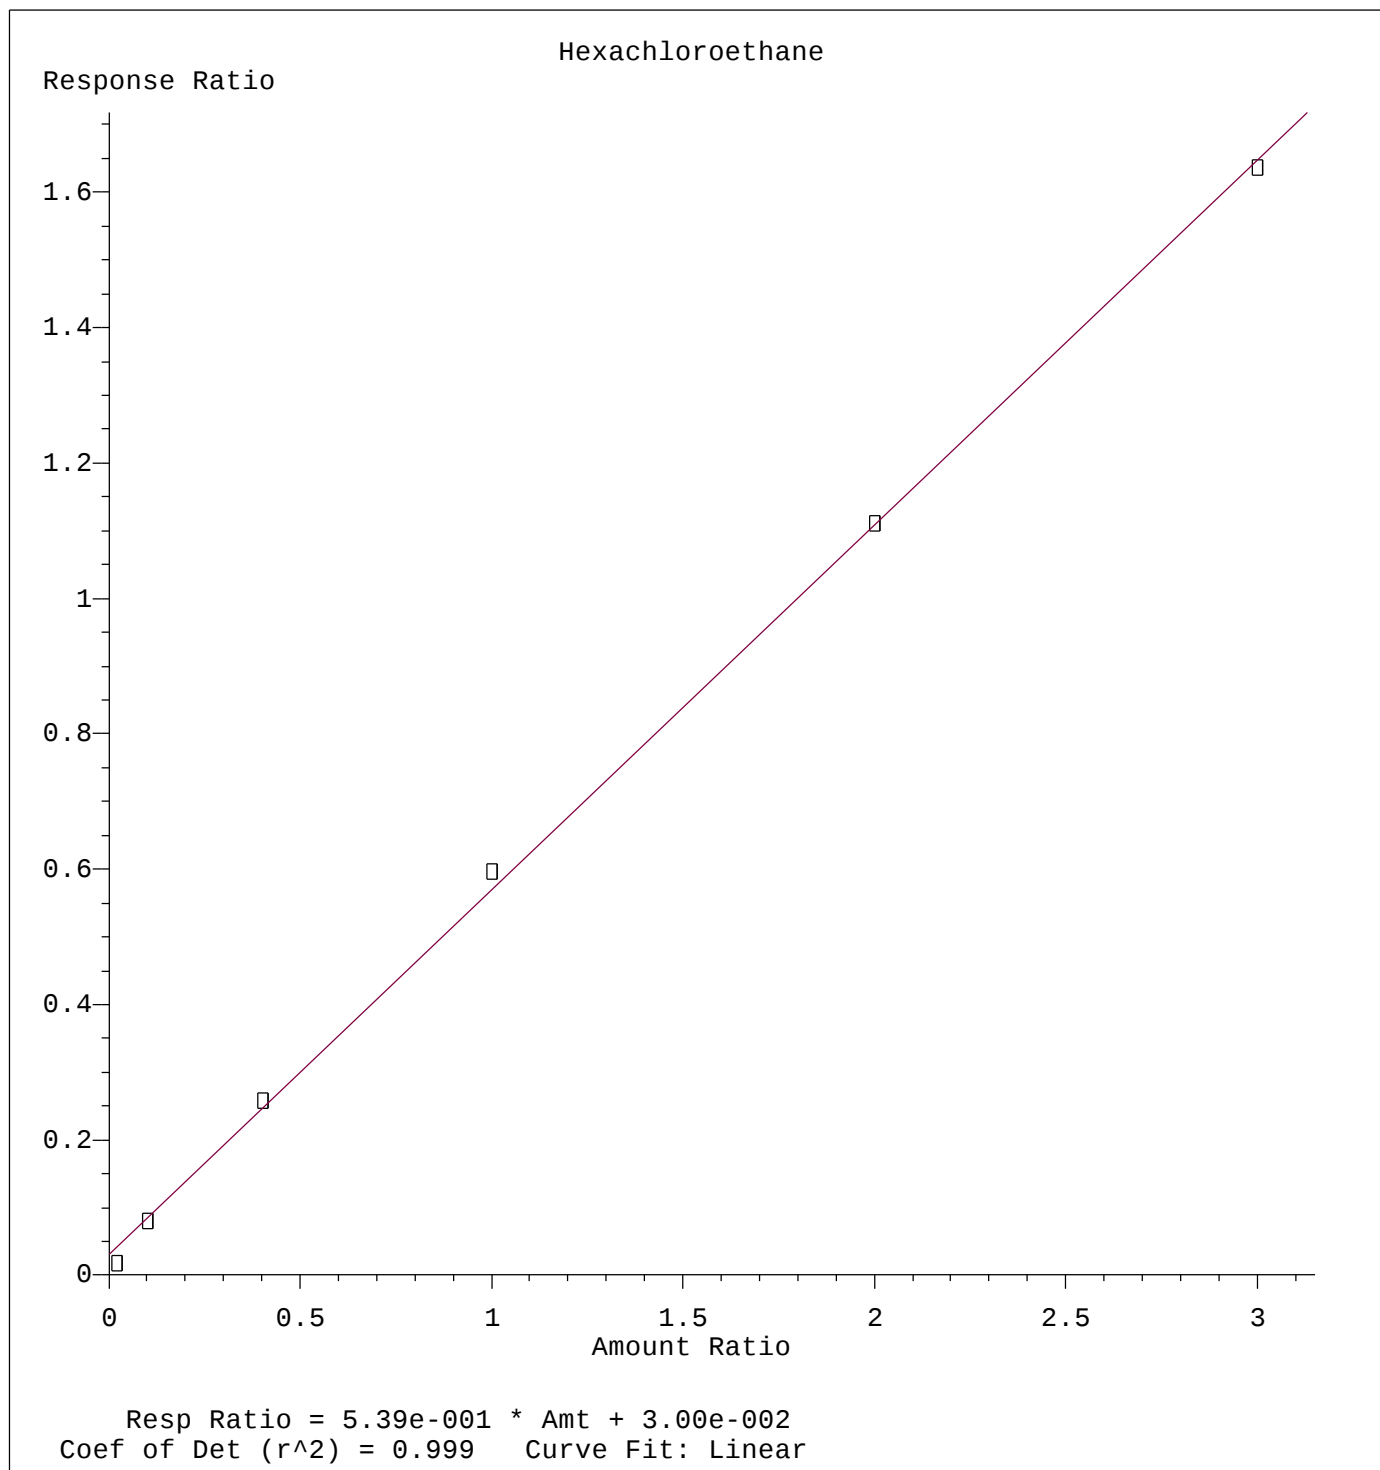

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061719W.M
Calibration Table Last Updated: Tue Jun 18 04:23:59 2019


1,2,4-Trichlorobenzene

Response Ratio

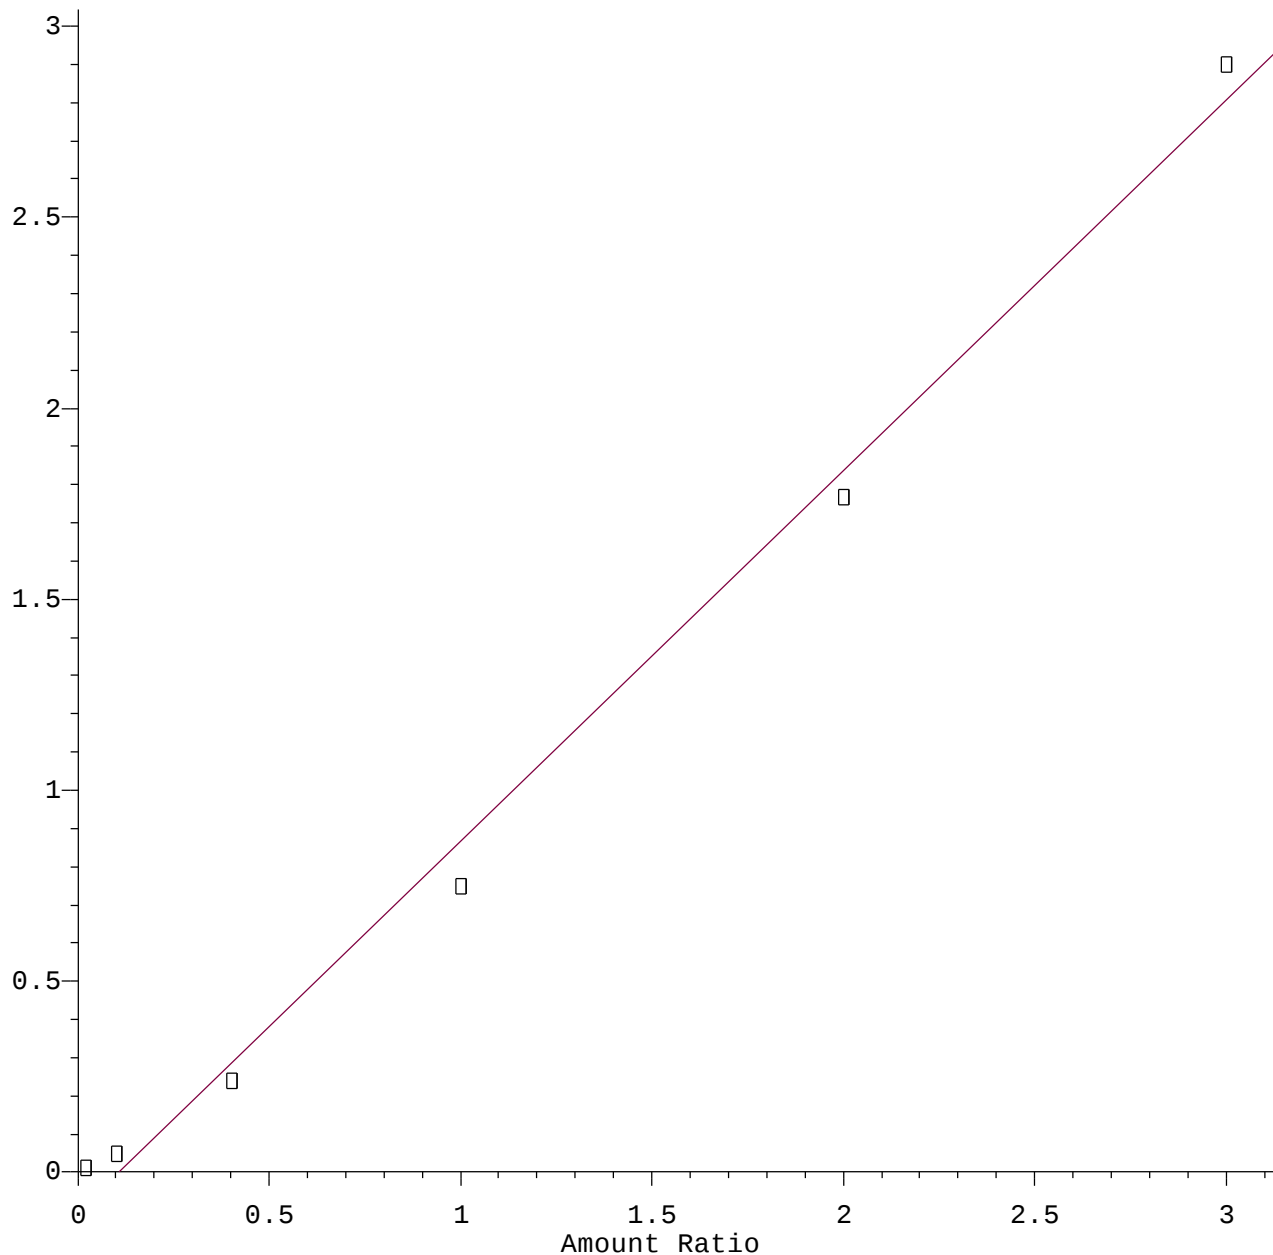

Resp Ratio = $9.70 \times 10^{-1} \times \text{Amt} - 1.03 \times 10^{-1}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061719W.M
Calibration Table Last Updated: Tue Jun 18 04:23:59 2019

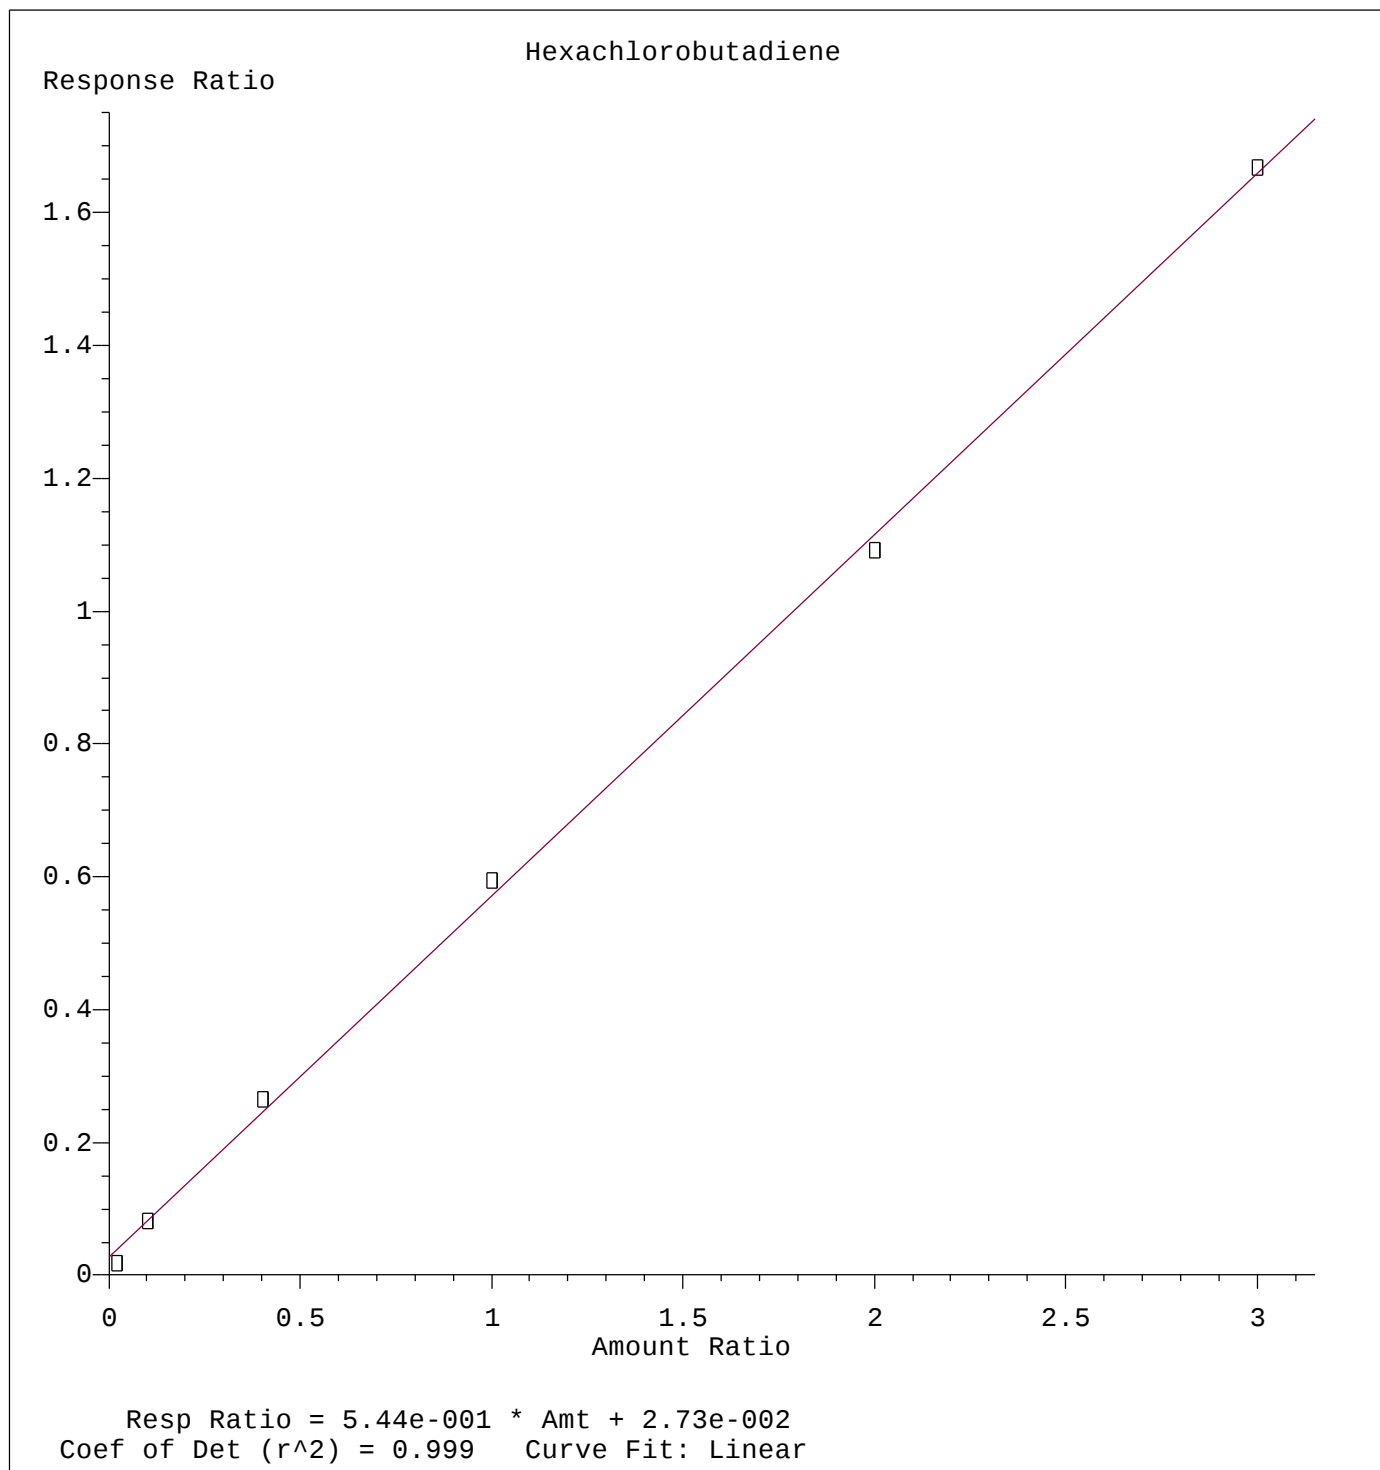

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061719W.M
Calibration Table Last Updated: Tue Jun 18 04:23:59 2019

Naphthalene

Response Ratio

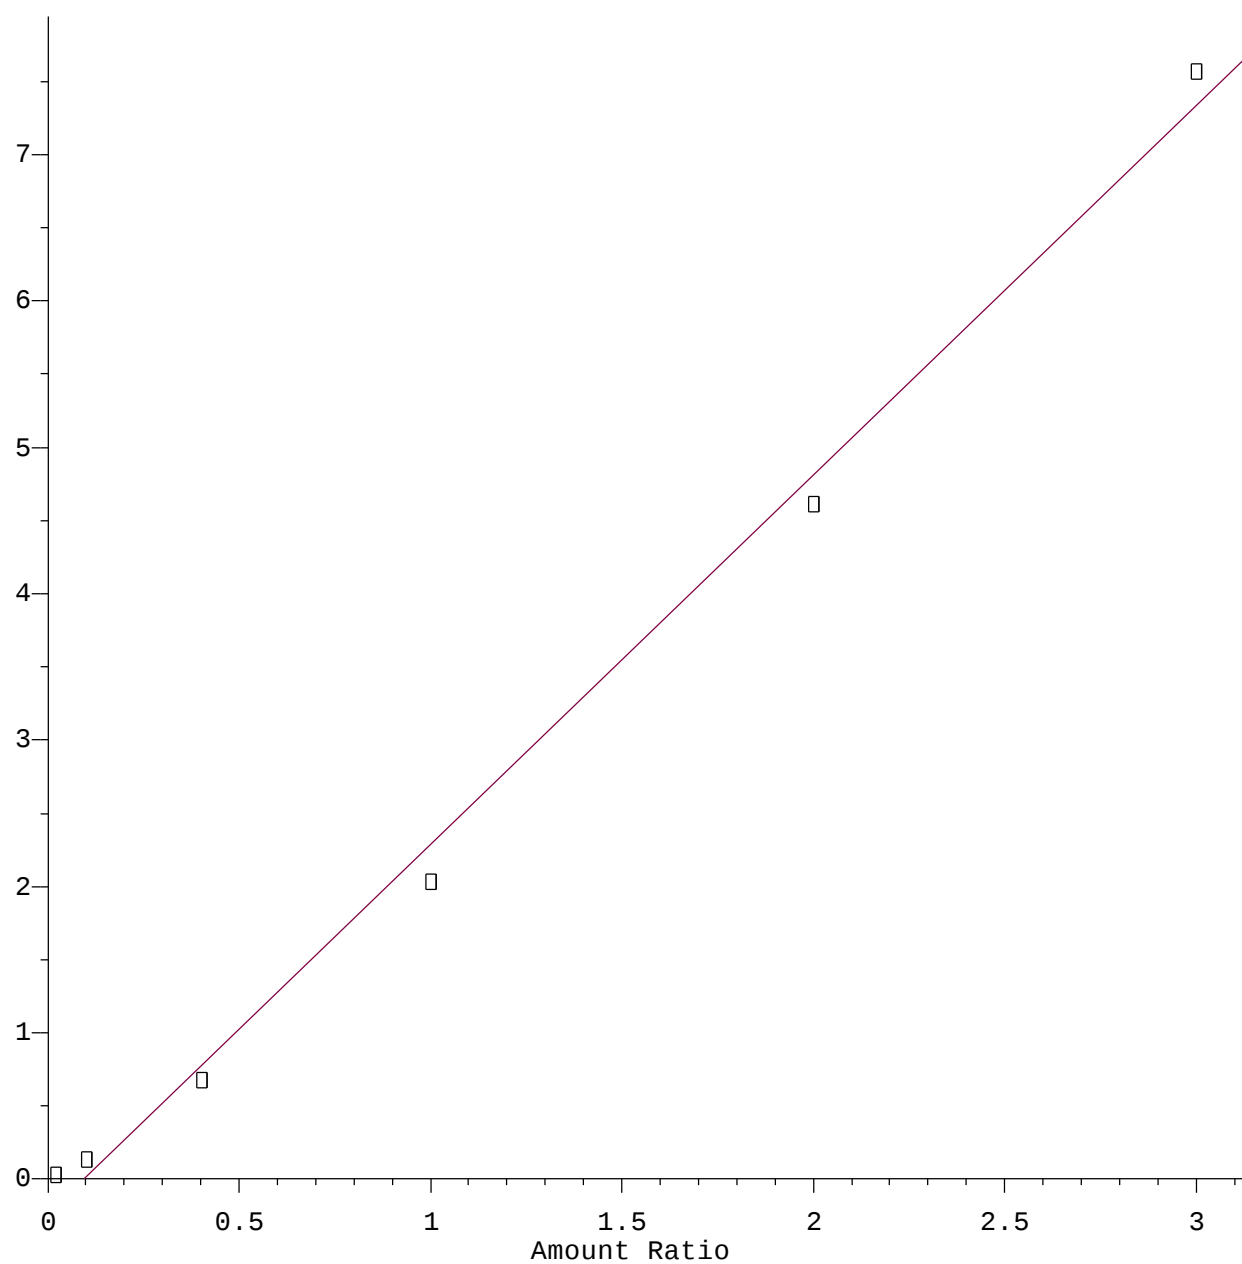


Resp Ratio = 2.52e+000 * Amt - 2.35e-001
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061719W.M
Calibration Table Last Updated: Tue Jun 18 04:23:59 2019

1,2,3-Trichlorobenzene

Response Ratio

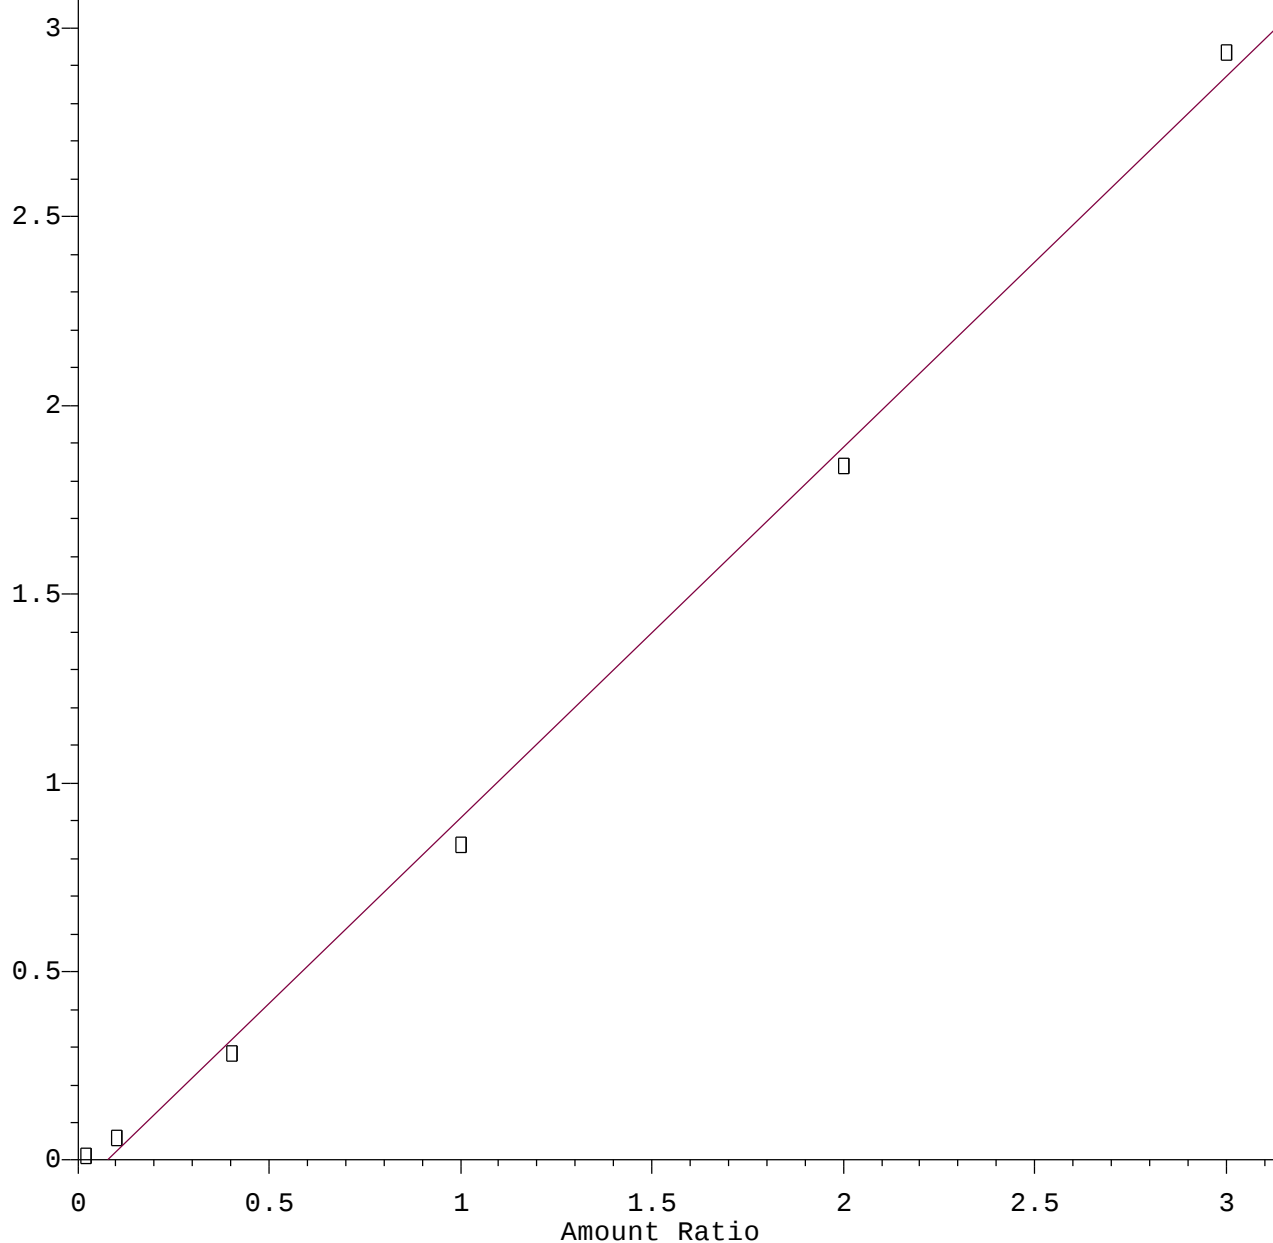

Resp Ratio = $9.82 \times 10^{-1} \times \text{Amt} - 7.47 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061719W.M
Calibration Table Last Updated: Tue Jun 18 04:23:59 2019