


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN061719\
 Data File : VN056325.D
 Acq On : 17 Jun 2019 8:21
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061719W.M
 Title : SW846 8260
 Last Update : Tue Jun 18 04:23:59 2019

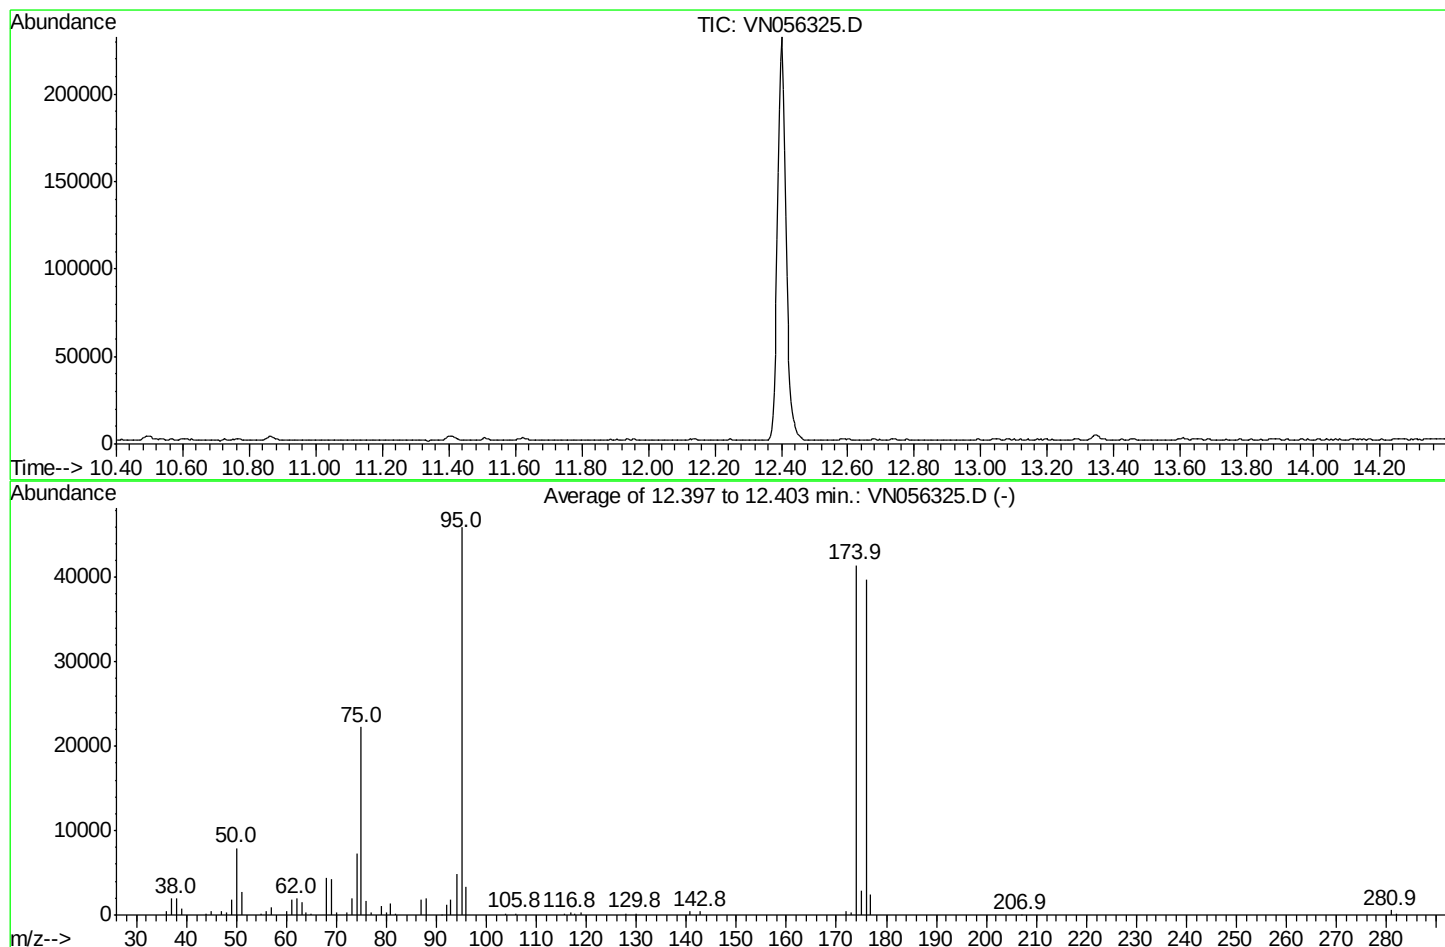

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	7965	PASS
75	95	30	60	48.5	22256	PASS
95	95	100	100	100.0	45930	PASS
96	95	5	9	7.2	3323	PASS
173	174	0.00	2	0.7	300	PASS
174	95	50	100	90.2	41418	PASS
175	174	5	9	7.1	2933	PASS
176	174	95	101	96.1	39786	PASS
177	176	5	9	6.2	2448	PASS