

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN061720\
 Data File : VN061843.D
 Acq On : 17 Jun 2020 13:04
 Operator : JC/MD
 Sample : L2989-03DL 5X
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 RE125D1-20200609DL

Quant Time: Jun 18 03:53:06 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061620W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 17 01:19:44 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.62	168	139419	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	246121	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	240229	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	106737	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	87913	47.02	ug/l	0.00
Spiked Amount						
			Recovery	=	94.04%	
35) Dibromofluoromethane	7.54	113	76456	48.56	ug/l	0.00
Spiked Amount						
			Recovery	=	97.12%	
50) Toluene-d8	10.06	98	307315	49.65	ug/l	0.00
Spiked Amount						
			Recovery	=	99.30%	
62) 4-Bromofluorobenzene	12.38	95	109937	51.78	ug/l	0.00
Spiked Amount						
			Recovery	=	103.56%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	2.03	50	388	0.200	ug/l #	42
5) Bromomethane	2.49	94	545	0.308	ug/l	87
9) 1,1,2-Trichlorotrifluoroet	3.71	101	2747	1.943	ug/l	91
10) Methyl Iodide	3.90	142	322	5.487	ug/l #	42
11) Tert butyl alcohol	4.70	59	933	3.606	ug/l #	74
12) 1,1-Dichloroethene	3.69	96	628	0.443	ug/l #	73
16) Acetone	3.76	43	303	0.549	ug/l #	40
17) Carbon Disulfide	4.00	76	1113	0.269	ug/l #	75
20) Methylene Chloride	4.50	84	367	0.204	ug/l #	75
27) cis-1,2-Dichloroethene	6.77	96	1517	0.808	ug/l	82
31) Cyclohexane	7.63	56	2879	1.168	ug/l #	47
36) 1,1-Dichloropropene	7.62	75	10856	4.836	ug/l #	47
38) Carbon Tetrachloride	7.62	117	13605	6.120	ug/l #	17
39) Methylcyclohexane	8.80	83	971	0.402	ug/l #	1
44) Trichloroethene	8.80	130	80038	44.722	ug/l	97
49) 1,4-Dioxane	9.17	88	95	3.080	ug/l #	28
59) 2-Hexanone	10.72	43	517	13.758	ug/l #	28
60) Dibromochloromethane	10.60	129	2195	1.171	ug/l #	11
64) Tetrachloroethene	10.60	164	2252	1.471	ug/l	89
76) 1,2,3-Trichloropropane	12.38	75	54773	26.138	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.38	75	54773	71.290	ug/l #	14
88) 1,4-Dichlorobenzene	13.34	146	764	0.214	ug/l #	25
93) 1,2,4-Trichlorobenzene	14.89	180	741	0.467	ug/l #	81
95) Naphthalene	15.11	128	3374	4.074	ug/l #	84
96) 1,2,3-Trichlorobenzene	15.29	180	848	0.540	ug/l #	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN061720\
Data File : VN061843.D
Acq On : 17 Jun 2020 13:04
Operator : JC/MD
Sample : L2989-03DL 5X
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
RE125D1-20200609DL

Quant Time: Jun 18 03:53:06 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N061620W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 17 01:19:44 2020
Response via : Initial Calibration

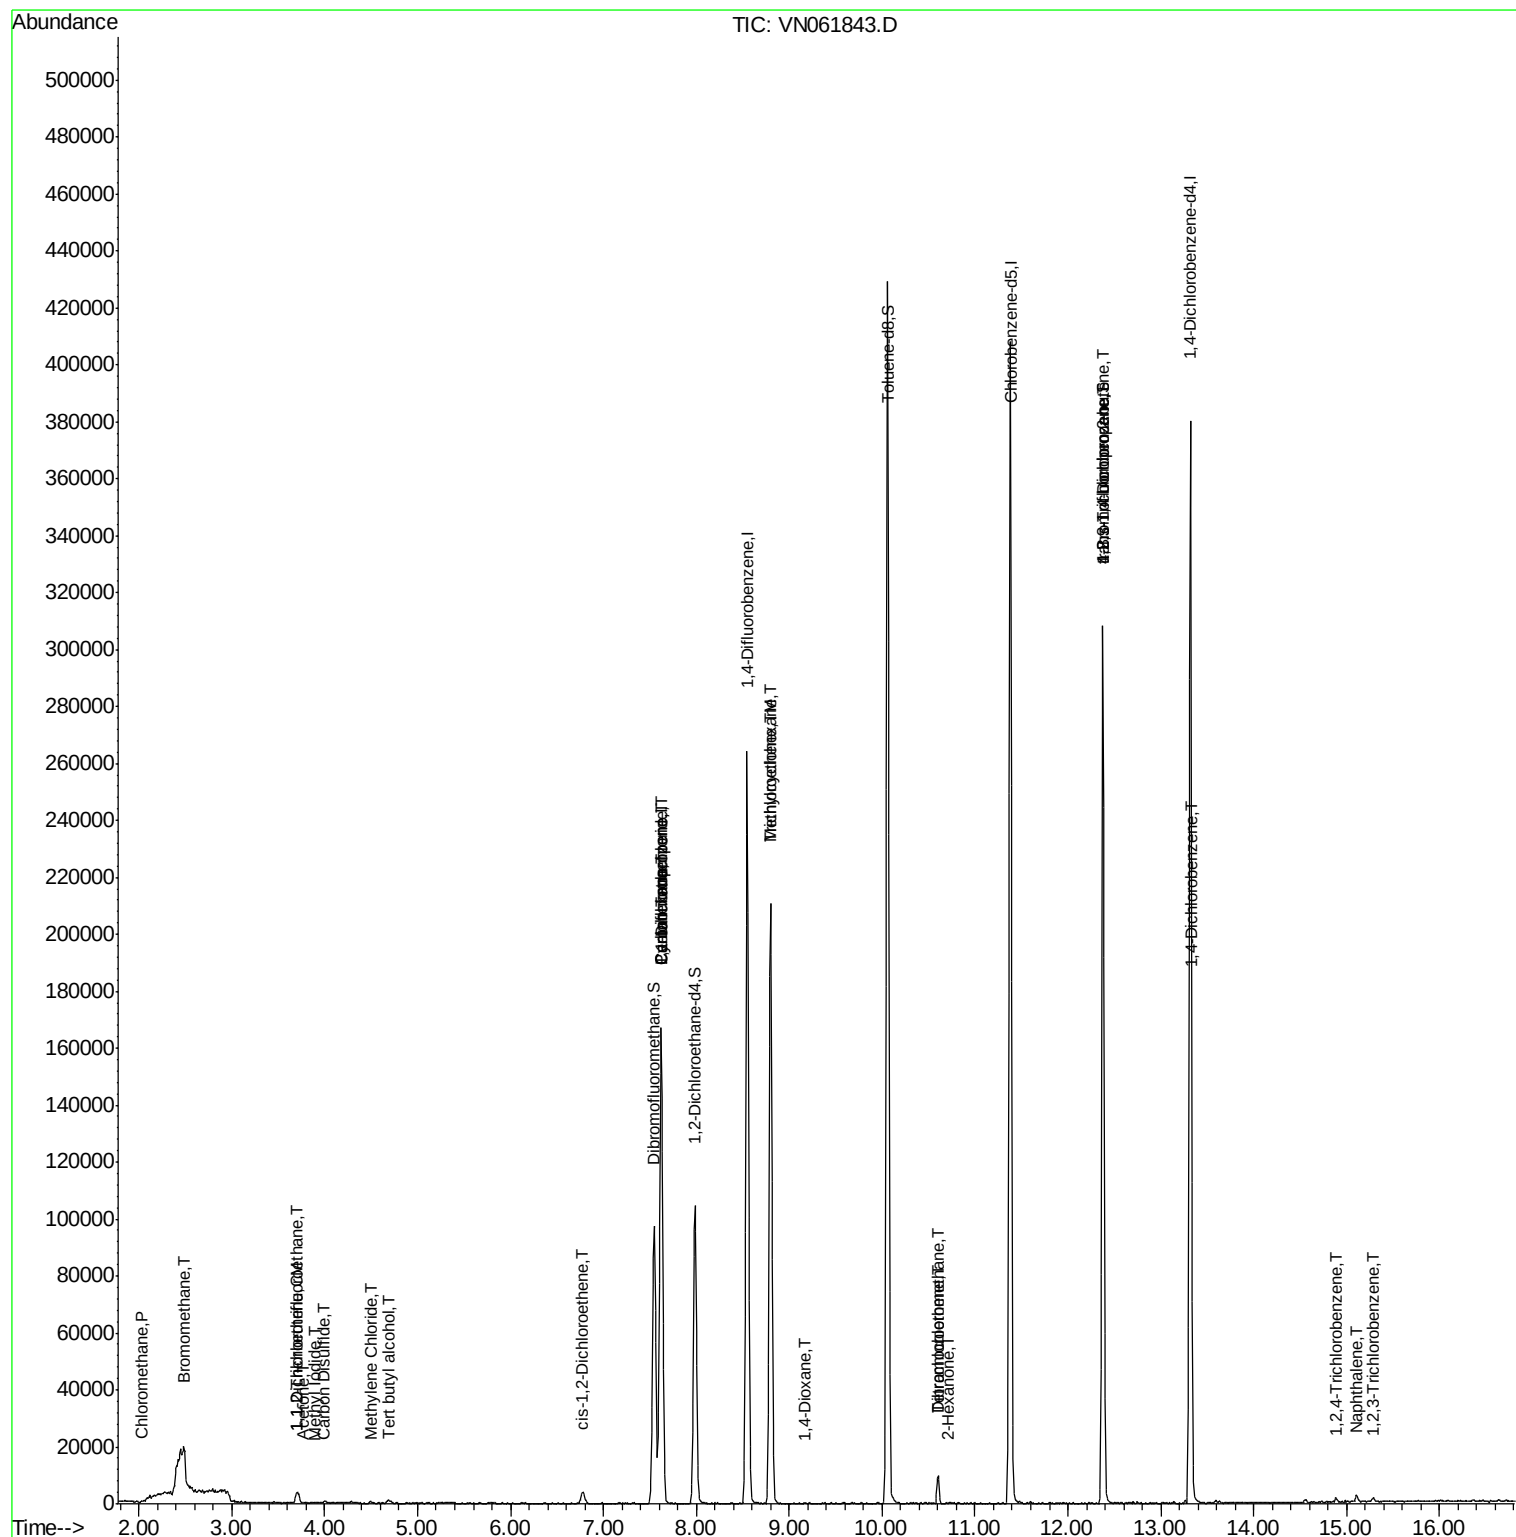

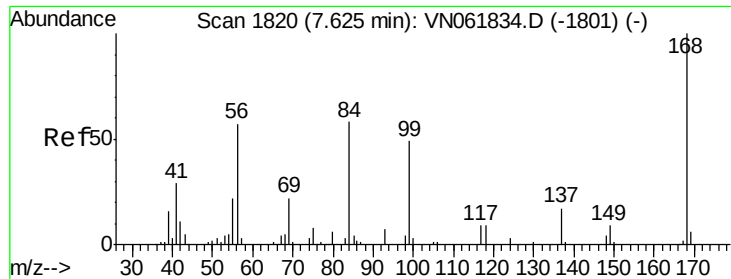

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.62 min Scan# 1819

Delta R.T. -0.00 min

Lab File: VN061843.D

Acq: 17 Jun 2020 13:04

Instrument :

MSVOA_N

ClientSampleId :


RE125D1-20200609DL

Tot Ion:168 Resp: 139419

Ion Ratio Lower Upper

168 100

99 55.1 44.6 67.0

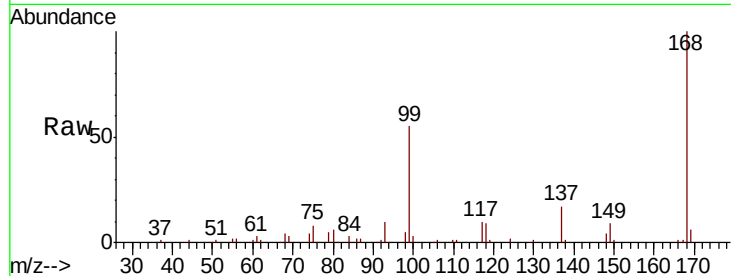

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.62



60000

40000

20000

0

Time--> 7.50 7.60 7.70



#3

Chloromethane

Concen: 0.200 ug/l

RT: 2.03 min Scan# 79

Delta R.T. -0.01 min

Lab File: VN061843.D


Acq: 17 Jun 2020 13:04

Tgt Ion: 50 Resp: 388

Ion Ratio Lower Upper

50 100

52 0.0 26.0 39.0#



Abundance Ion 49.90 (49.60 to 50.60): VN

Ion 51.90 (51.60 to 52.60): VN

2.03


300


200

100

0

Time--> 2.00 2.02 2.04 2.06





#5

Bromomethane

Concen: 0.308 ug/l

RT: 2.49 min Scan# 224

Delta R.T. -0.03 min

Lab File: VN061843.D

Acq: 17 Jun 2020 13:04

Instrument :

MSVOA_N

ClientSampleId :


RE125D1-20200609DL

Tot Ion: 94 Resp: 545

Ion Ratio Lower Upper

94 100

96 83.4 76.7 115.1

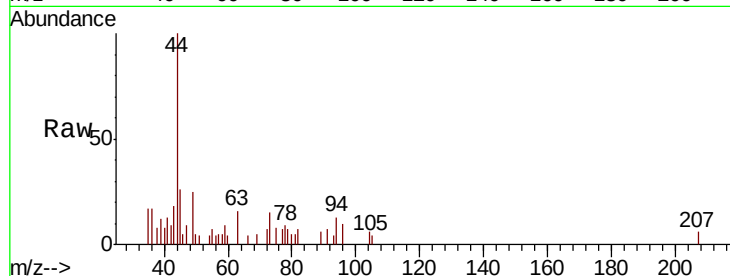

Abundance Ion 93.90 (93.60 to 94.60): VN0

Ion 95.90 (95.60 to 96.60): VN0

2.49

400



300

200

100

0

Time--> 2.46 2.48 2.50 2.52

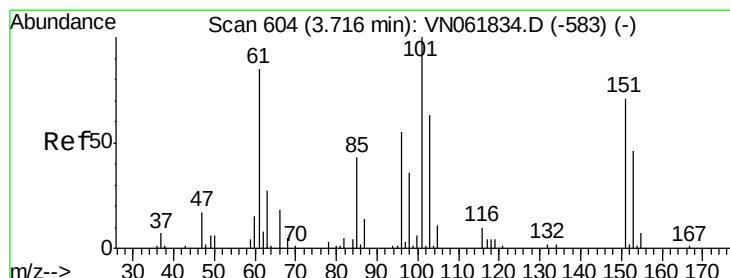

#9

1,1,2-Trichlorotrifluoroethane

Concen: 1.943 ug/l

RT: 3.71 min Scan# 603

Delta R.T. -0.00 min

Lab File: VN061843.D

Acq: 17 Jun 2020 13:04


Tgt Ion:101 Resp: 2747

Ion Ratio Lower Upper

101 100

85 36.3 35.0 52.6

151 67.7 59.2 88.8

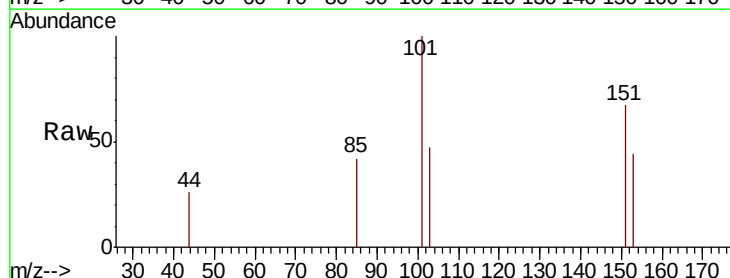

Abundance Ion 100.90 (100.60 to 101.60): V

Ion 84.90 (84.60 to 85.60): VN0

Ion 150.80 (150.50 to 151.50): V


3.71


1000

500

0

Time--> 3.65 3.70 3.75









#10
Methyl Iodide
Concen: 5.487 ug/l
RT: 3.90 min Scan# 662
Delta R.T. -0.01 min
Lab File: VN061843.D
Acq: 17 Jun 2020 13:04




Instrument :
MSVOA_N
ClientSampleId :
RE125D1-20200609DL


Tot Ion:142 Resp: 322
Ion Ratio Lower Upper
142 100
127 0.0 33.4 50.0#
141 0.0 11.3 16.9#

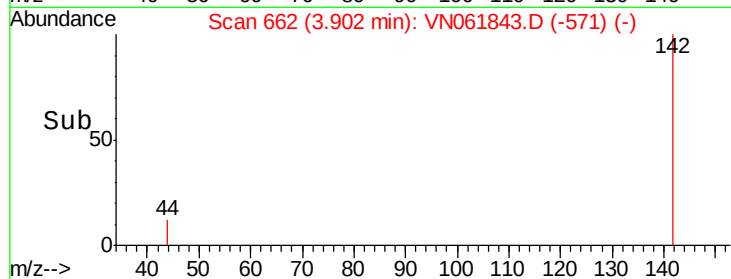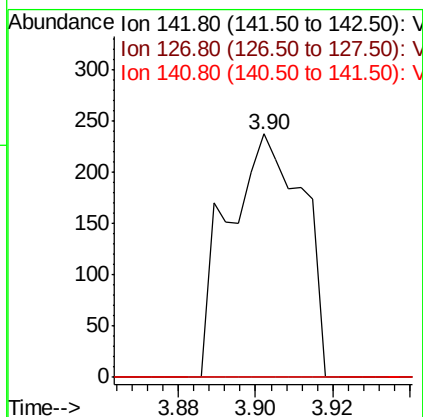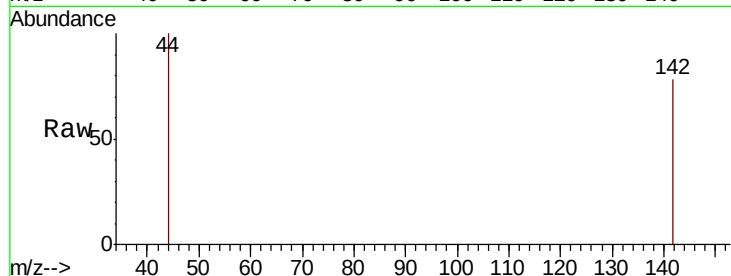

#11
Tert butyl alcohol
Concen: 3.606 ug/l
RT: 4.70 min Scan# 909
Delta R.T. -0.04 min
Lab File: VN061843.D
Acq: 17 Jun 2020 13:04

Tgt Ion: 59 Resp: 933
Ion Ratio Lower Upper
59 100
57 0.0 7.7 11.5#

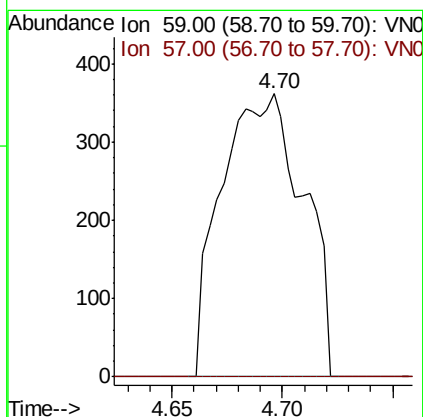

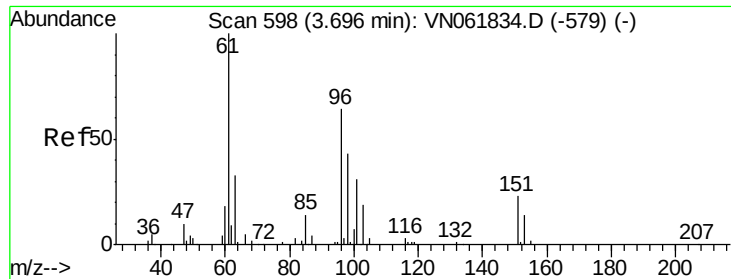

#12

1,1-Dichloroethene

Concen: 0.443 ug/l

RT: 3.69 min Scan# 597

Delta R.T. -0.00 min

Lab File: VN061843.D

Acq: 17 Jun 2020 13:04

Instrument :

MSVOA_N

ClientSampleId :

RE125D1-20200609DL





Tot Ion: 96 Resp: 628

Ion Ratio Lower Upper

96 100

61 109.5 124.3 186.5#

98 59.9 53.1 79.7

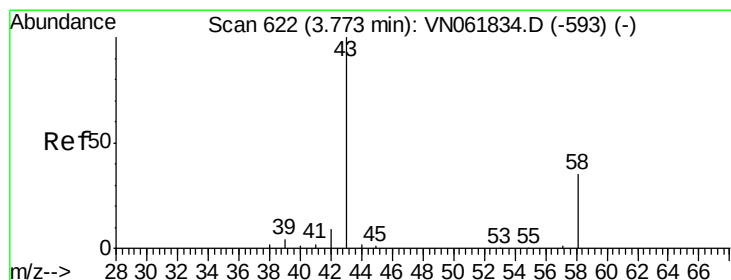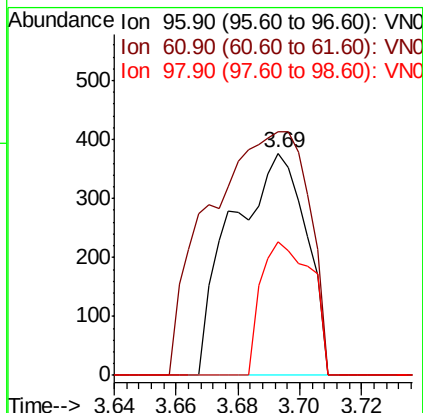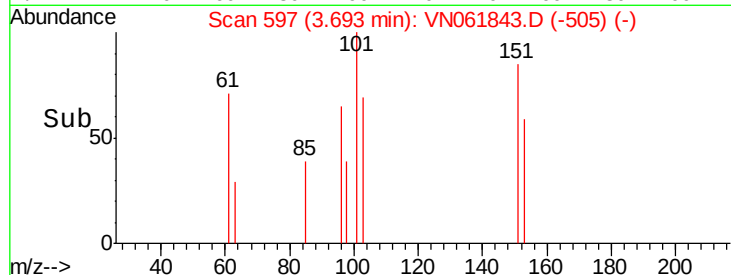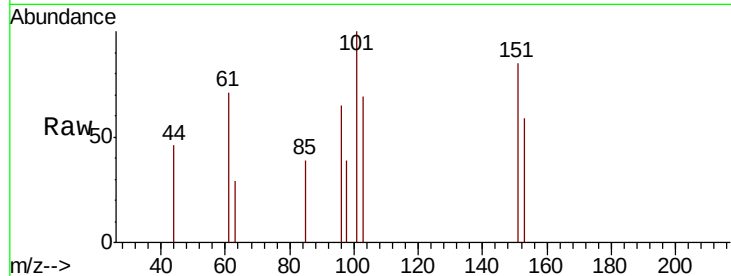

#16

Acetone

Concen: 0.549 ug/l

RT: 3.76 min Scan# 619

Delta R.T. -0.01 min

Lab File: VN061843.D




Acq: 17 Jun 2020 13:04


Tgt Ion: 43 Resp: 303

Ion Ratio Lower Upper

43 100

58 0.0 27.8 41.8#

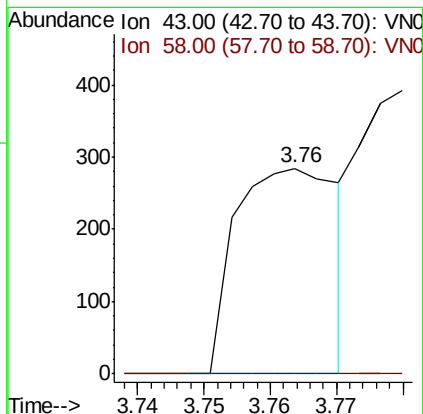



#17

Carbon Disulfide

Concen: 0.269 ug/l

RT: 4.00 min Scan# 692

Delta R.T. -0.01 min

Lab File: VN061843.D

Acq: 17 Jun 2020 13:04

Instrument :

MSVOA_N

ClientSampleId :


RE125D1-20200609DL

Tot Ion: 76 Resp: 1113

Ion Ratio Lower Upper

76 100

78 0.0 7.3 10.9#

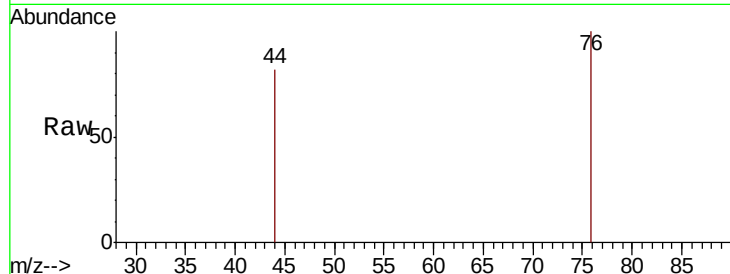

Abundance Ion 75.90 (75.60 to 76.60): VN061834.D (-675) (-)

Ion 77.90 (77.60 to 78.60): VN061834.D (-675) (-)

4.00

600

500

400



300

200

100

0

Time-->

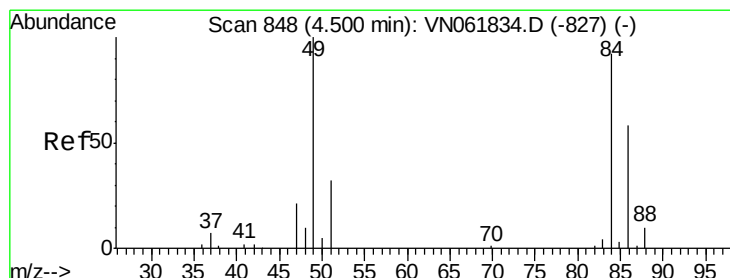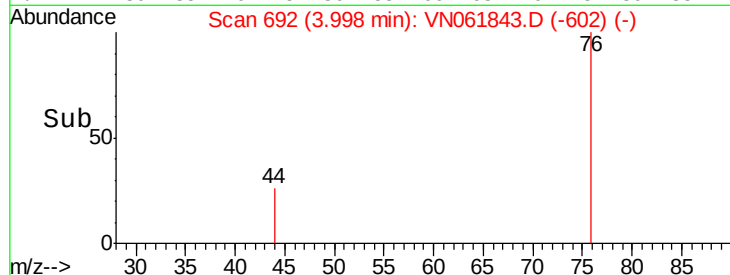

#20

Methylene Chloride

Concen: 0.204 ug/l

RT: 4.50 min Scan# 847

Delta R.T. -0.00 min

Lab File: VN061843.D

Acq: 17 Jun 2020 13:04

Tgt Ion: 84 Resp: 367


Ion Ratio Lower Upper

84 100

49 79.6 87.0 130.4#

51 0.0 27.8 41.6#

86 64.6 50.2 75.2

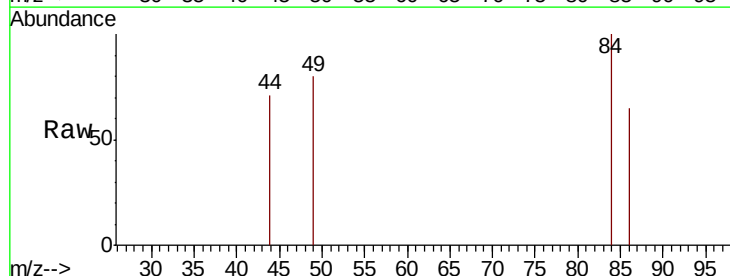

Abundance Ion 83.90 (83.60 to 84.60): VN061834.D (-827) (-)

Ion 48.90 (48.60 to 49.60): VN061834.D (-827) (-)

Ion 50.90 (50.60 to 51.60): VN061834.D (-827) (-)

Ion 85.90 (85.60 to 86.60): VN061834.D (-827) (-)

400


300


200

100

0

Time-->

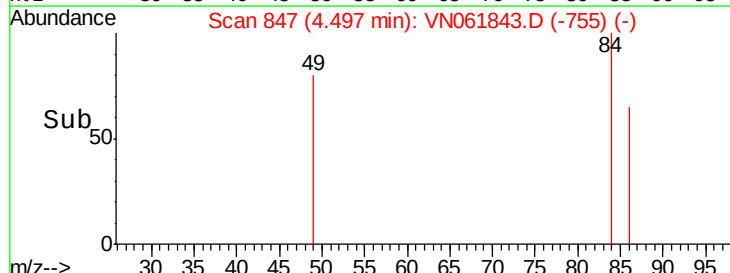

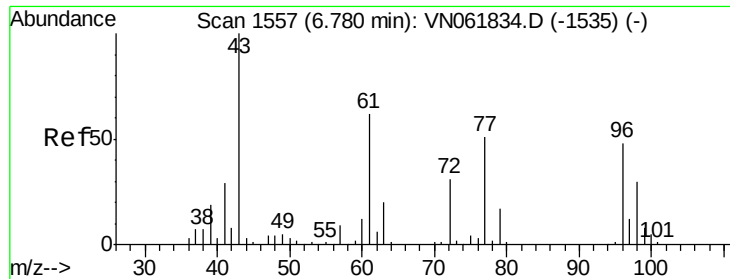

#27

cis-1,2-Dichloroethene

Concen: 0.808 ug/l

RT: 6.77 min Scan# 1554

Delta R.T. -0.01 min

Lab File: VN061843.D

Acq: 17 Jun 2020 13:04

Instrument :

MSVOA_N

ClientSampleId :

RE125D1-20200609DL



Tot Ion: 96 Resp: 1517

Ion Ratio Lower Upper

96 100

61 115.2 0.0 265.6


98 45.1 0.0 128.2

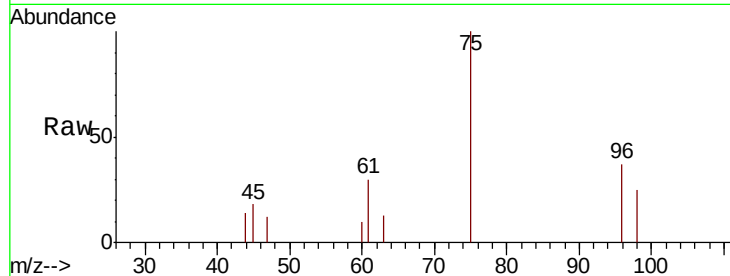


Abundance Ion 95.90 (95.60 to 96.60): VN0

Ion 60.90 (60.60 to 61.60): VN0

Ion 97.90 (97.60 to 98.60): VN0

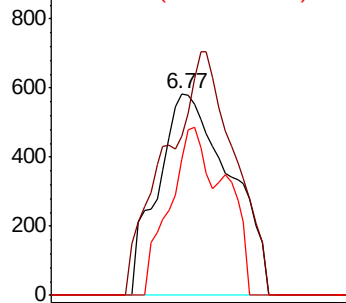

Time-->

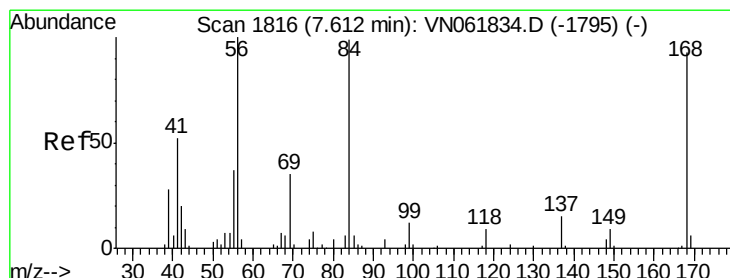

#31

Cyclohexane

Concen: 1.168 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. 0.01 min

Lab File: VN061843.D

Acq: 17 Jun 2020 13:04



Tgt Ion: 56 Resp: 2879

Ion Ratio Lower Upper

56 100

69 118.2 27.7 41.5#


84 119.1 79.1 118.7#

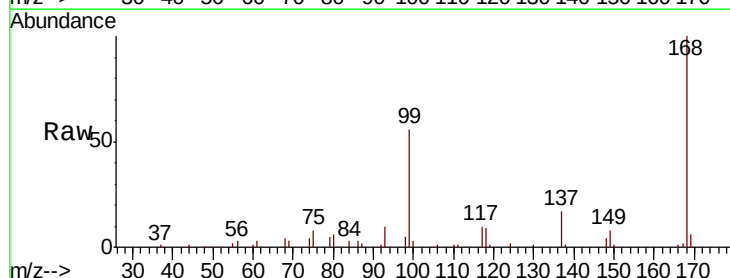


Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 84.00 (83.70 to 84.70): VN0

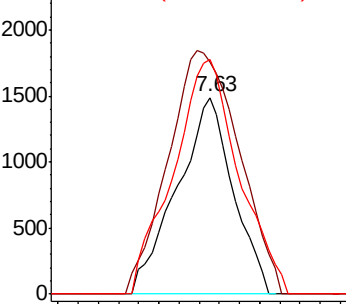





Time-->



#33
 1,2-Dichloroethane-d4
 Concen: 47.017 ug/l
 RT: 7.99 min Scan# 1932
 Delta R.T. -0.00 min
 Lab File: VN061843.D
 Acq: 17 Jun 2020 13:04




Instrument :
 MSVOA_N
 ClientSampleId :
 RE125D1-20200609DL


Tot Ion: 65 Resp: 87913
 Ion Ratio Lower Upper
 65 100
 67 51.8 0.0 106.2

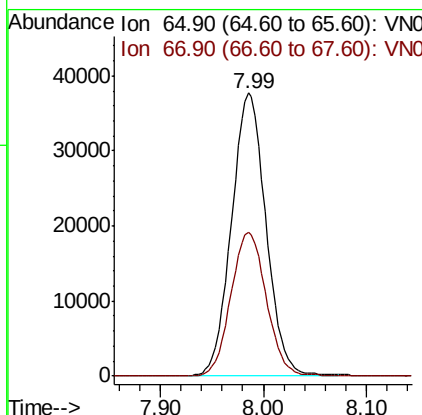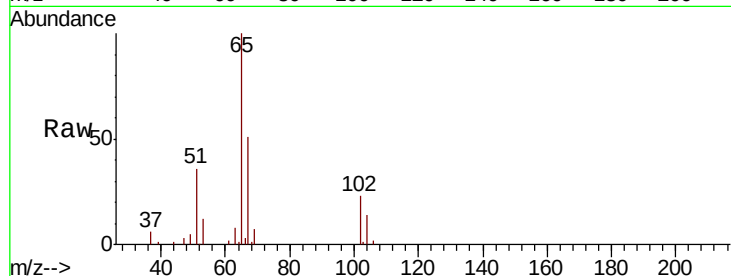

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2107
 Delta R.T. -0.00 min
 Lab File: VN061843.D
 Acq: 17 Jun 2020 13:04

Tgt Ion: 114 Resp: 246121
 Ion Ratio Lower Upper
 114 100
 63 18.9 0.0 37.6
 88 15.5 0.0 31.0



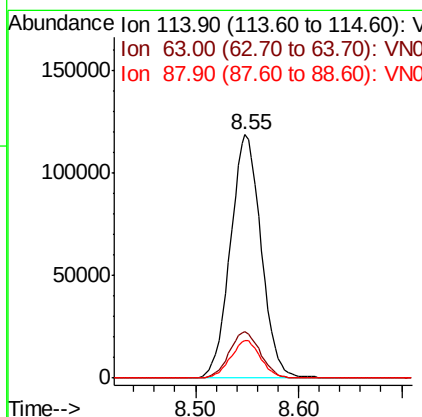





#35
 Dibromofluoromethane
 Concen: 48.557 ug/l
 RT: 7.54 min Scan# 1795
 Delta R.T. -0.00 min
 Lab File: VN061843.D
 Acq: 17 Jun 2020 13:04




Instrument :
 MSVOA_N
 ClientSampleId :
 RE125D1-20200609DL


Tot Ion	Ratio	Lower	Upper
113	100		
111	103.6	83.7	125.5
192	17.8	13.9	20.9

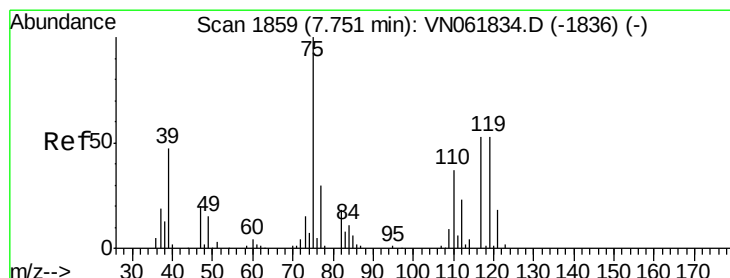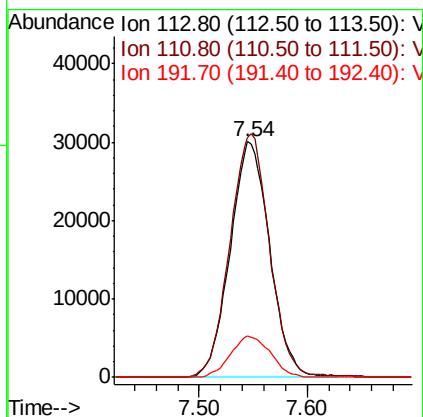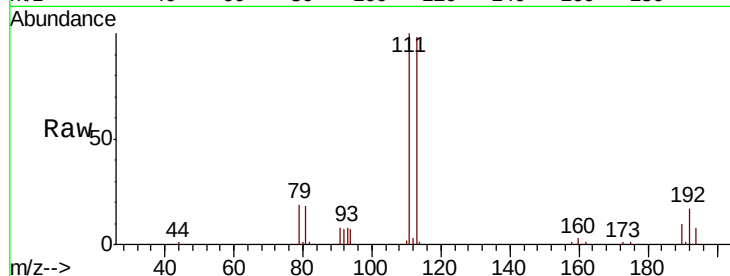

#36
 1,1-Dichloropropene
 Concen: 4.836 ug/l
 RT: 7.62 min Scan# 1818
 Delta R.T. -0.13 min
 Lab File: VN061843.D
 Acq: 17 Jun 2020 13:04

Tgt Ion	Ratio	Lower	Upper
75	100		
110	6.8	18.2	54.6#
77	0.0	24.2	36.4#

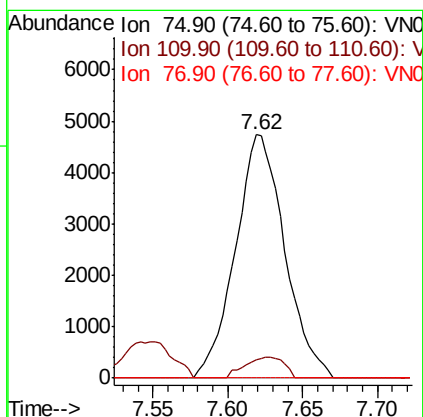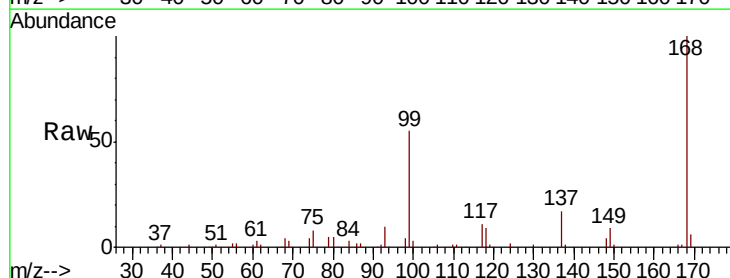

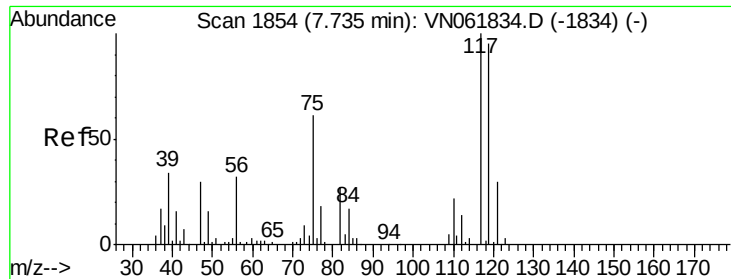

#38

Carbon Tetrachloride

Concen: 6.120 ug/l

RT: 7.62 min Scan# 1819

Delta R.T. -0.11 min

Lab File: VN061843.D

Acq: 17 Jun 2020 13:04

Instrument :

MSVOA_N

ClientSampleId :

RE125D1-20200609DL


Tot Ion:117 Resp: 13605

Ion Ratio Lower Upper

117 100

119 5.9 75.8 113.6#




121 0.0 23.8 35.6#

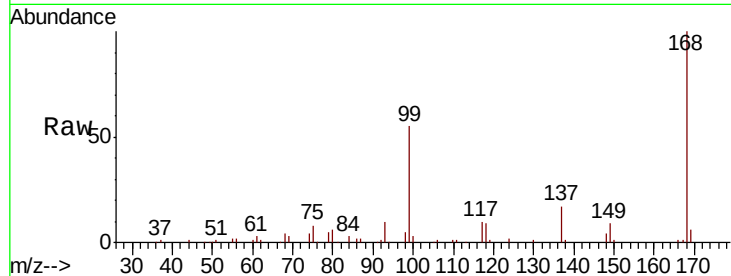

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

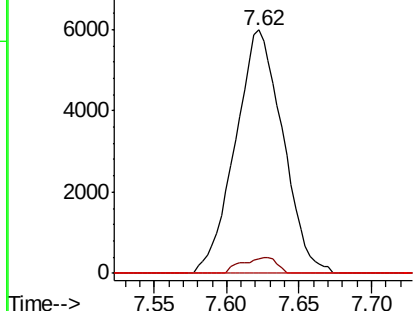

#39

Methylcyclohexane

Concen: 0.402 ug/l

RT: 8.80 min Scan# 2185

Delta R.T. -0.25 min

Lab File: VN061843.D

Acq: 17 Jun 2020 13:04


Tgt Ion: 83 Resp: 971

Ion Ratio Lower Upper

83 100

55 0.0 54.2 81.4#



98 193.5 39.8 59.6#




Abundance Ion 83.00 (82.70 to 83.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

Ion 98.00 (97.70 to 98.70): VN0

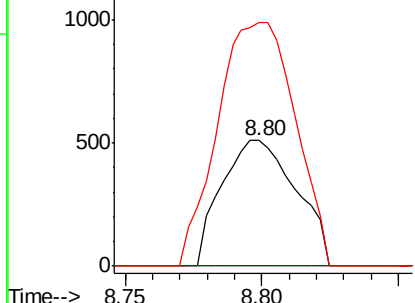



#44

Trichloroethene

Concen: 44.722 ug/l

RT: 8.80 min Scan# 2185

Delta R.T. -0.00 min

Lab File: VN061843.D

Acq: 17 Jun 2020 13:04

Instrument :

MSVOA_N

ClientSampleId :


RE125D1-20200609DL

Tot Ion:130 Resp: 80038

Ion Ratio Lower Upper




130 100

95 95.2 0.0 195.6

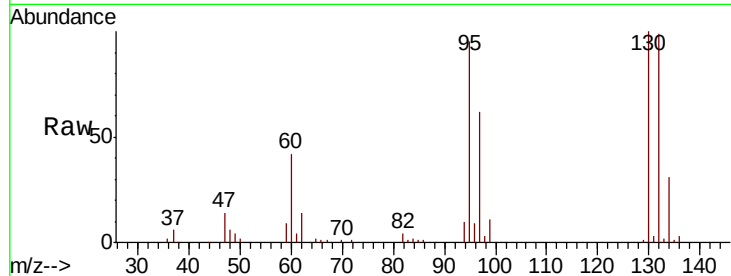

Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VN

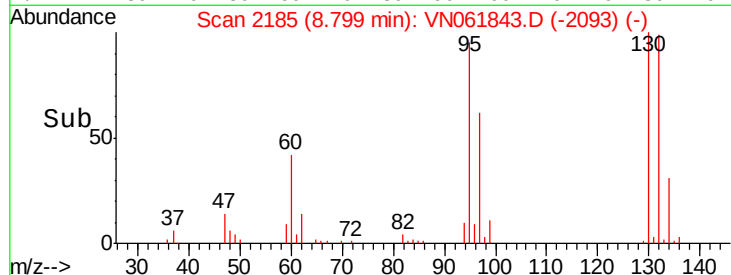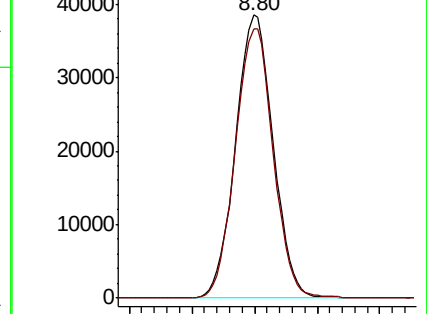

#49

1,4-Dioxane

Concen: 3.080 ug/l

RT: 9.17 min Scan# 2299

Delta R.T. 0.00 min

Lab File: VN061843.D

Acq: 17 Jun 2020 13:04


Tgt Ion: 88 Resp: 95

Ion Ratio Lower Upper

88 100

43 0.0 23.4 35.2#



58 0.0 49.8 74.6#




Abundance Ion 88.00 (87.70 to 88.70): VN

Ion 43.00 (42.70 to 43.70): VN

Ion 58.00 (57.70 to 58.70): VN




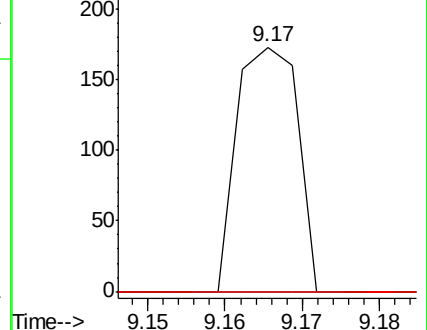


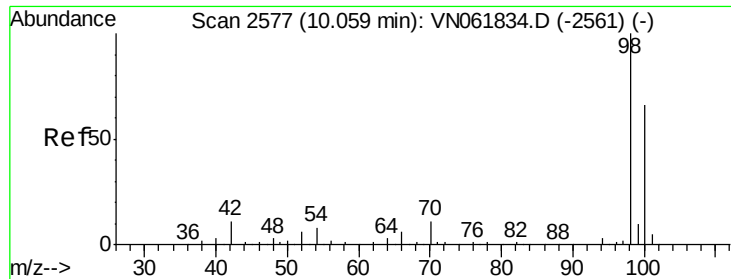

#50
Toluene-d8
Concen: 49.645 ug/l
RT: 10.06 min Scan# 2577
Delta R.T. 0.00 min
Lab File: VN061843.D
Acq: 17 Jun 2020 13:04




Instrument :
MSVOA_N
ClientSampleId :
RE125D1-20200609DL


Tot Ion: 98 Resp: 307315
Ion Ratio Lower Upper
98 100
100 64.9 52.7 79.1

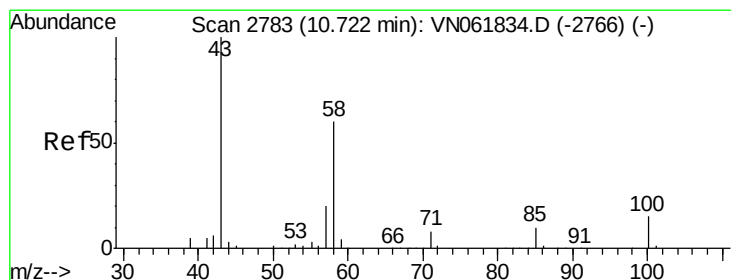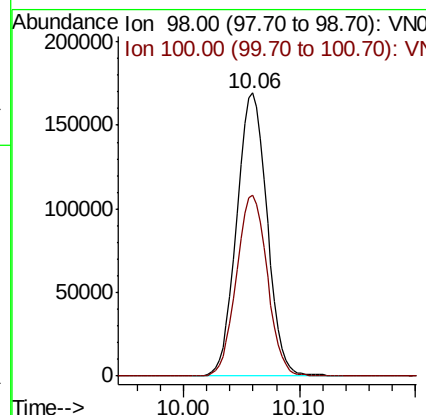

#59
2-Hexanone
Concen: 13.758 ug/l
RT: 10.72 min Scan# 2784
Delta R.T. 0.00 min
Lab File: VN061843.D
Acq: 17 Jun 2020 13:04

Tgt Ion: 43 Resp: 517
Ion Ratio Lower Upper
43 100
58 5.8 30.1 90.5#

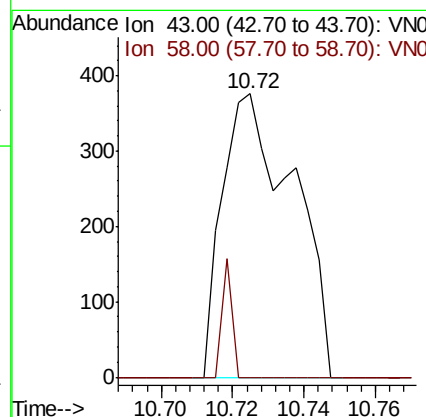



#60

Dibromochloromethane

Concen: 1.171 ug/l

RT: 10.60 min Scan# 2745

Delta R.T. -0.27 min

Lab File: VN061843.D

Acq: 17 Jun 2020 13:04

Instrument :

MSVOA_N

ClientSampleId :


RE125D1-20200609DL

Tot Ion:129 Resp: 2195

Ion Ratio Lower Upper




129 100

127 0.0 38.5 115.5#

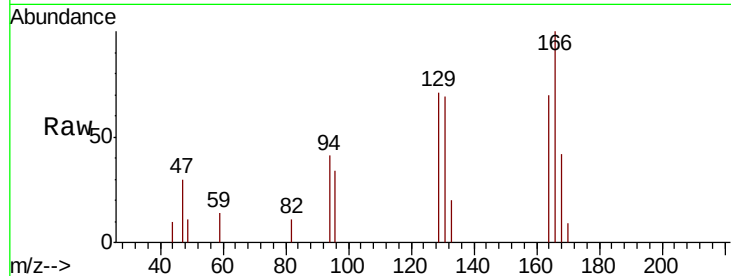

Abundance Ion 128.80 (128.50 to 129.50): V

Ion 126.80 (126.50 to 127.50): V

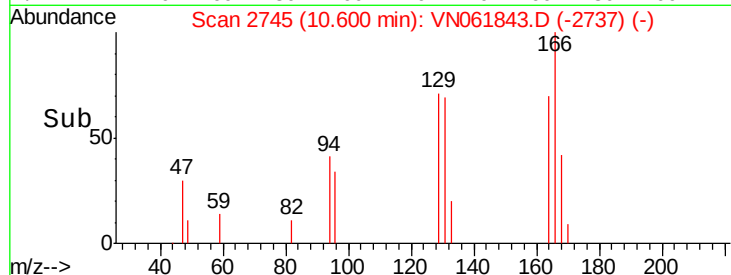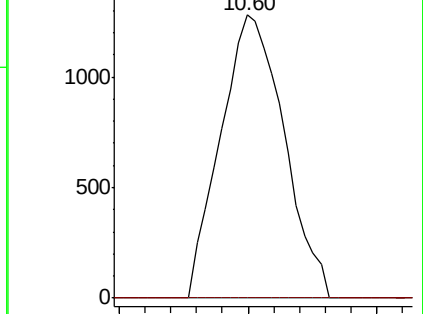

#62

4-Bromofluorobenzene

Concen: 51.776 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. 0.00 min

Lab File: VN061843.D

Acq: 17 Jun 2020 13:04


Tgt Ion: 95 Resp: 109937

Ion Ratio Lower Upper

95 100

174 80.3 0.0 158.6



176 76.1 0.0 152.0




Abundance Ion 94.90 (94.60 to 95.60): VN0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

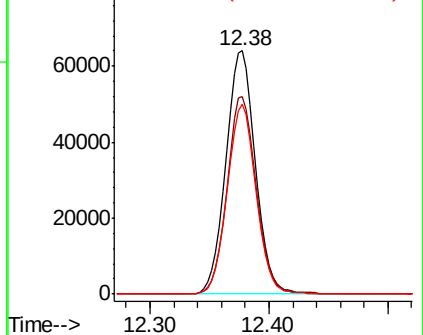







#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2988
Delta R.T. 0.00 min
Lab File: VN061843.D
Acq: 17 Jun 2020 13:04

Instrument :
MSVOA_N
ClientSampleId :
RE125D1-20200609DL

Tot Ion:117 Resp: 240229
Ion Ratio Lower Upper
117 100
82 54.6 42.6 64.0
119 31.8 24.7 37.1

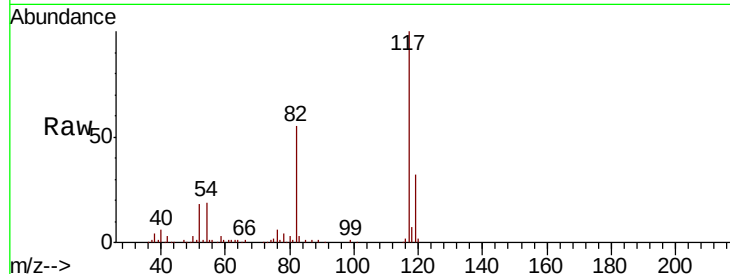


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

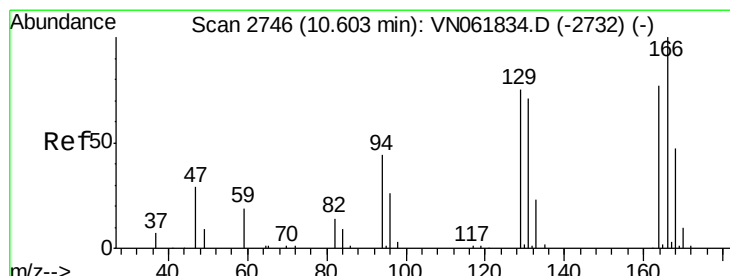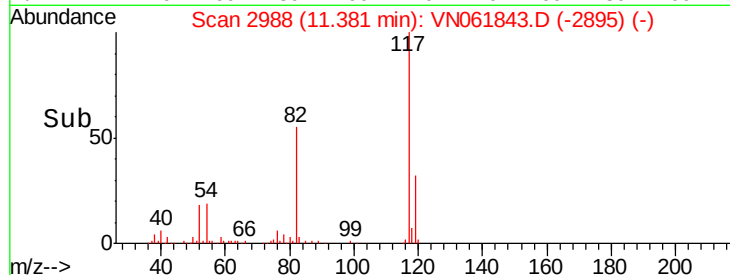
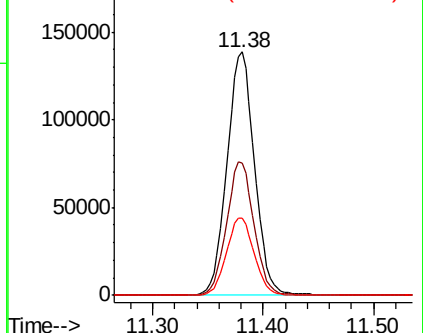



#64
Tetrachloroethene
Concen: 1.471 ug/l
RT: 10.60 min Scan# 2746
Delta R.T. 0.00 min
Lab File: VN061843.D
Acq: 17 Jun 2020 13:04

Tgt Ion:164 Resp: 2252
Ion Ratio Lower Upper
164 100
166 153.8 103.5 155.3
129 98.9 77.5 116.3
131 99.1 73.8 110.8

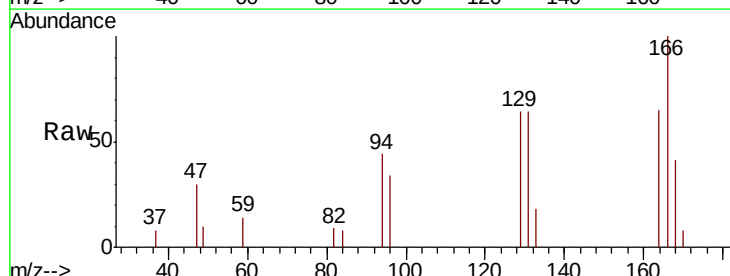

Abundance Ion 163.80 (163.50 to 164.50): V
Ion 165.80 (165.50 to 166.50): V
Ion 128.80 (128.50 to 129.50): V
Ion 130.80 (130.50 to 131.50): V

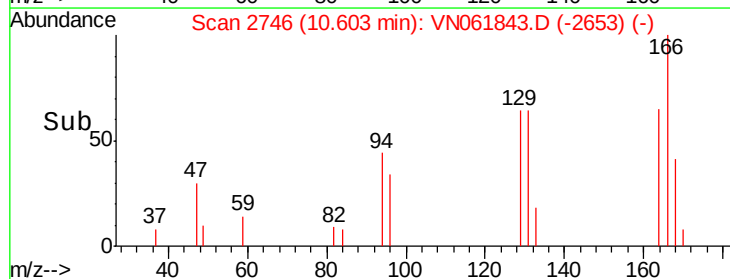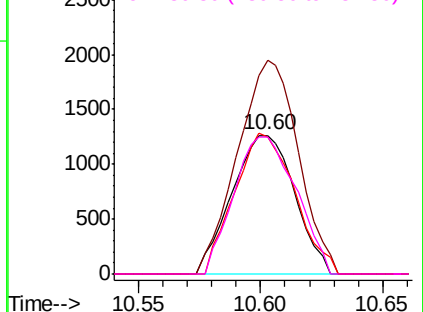



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3591

Delta R.T. 0.00 min

Lab File: VN061843.D

Acq: 17 Jun 2020 13:04

Instrument :

MSVOA_N

ClientSampleId :

RE125D1-20200609DL


Tot Ion:152 Resp: 106737

Ion Ratio Lower Upper

152 100

115 57.7 29.1 87.3




150 156.9 0.0 347.6

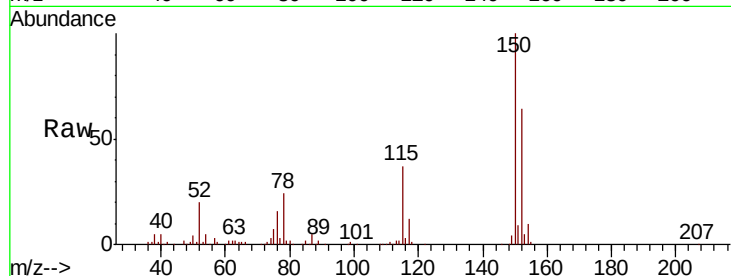

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

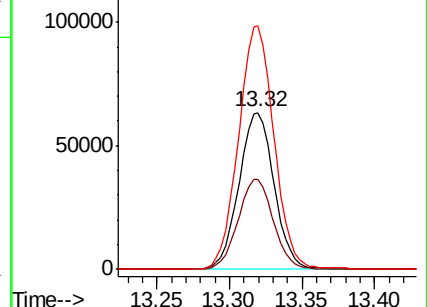

#76

1,2,3-Trichloropropane

Concen: 26.138 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. -0.15 min

Lab File: VN061843.D


Acq: 17 Jun 2020 13:04

Tgt Ion: 75 Resp: 54773

Ion Ratio Lower Upper



75 100


77 1.1 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): V

Ion 77.00 (76.70 to 77.70): V

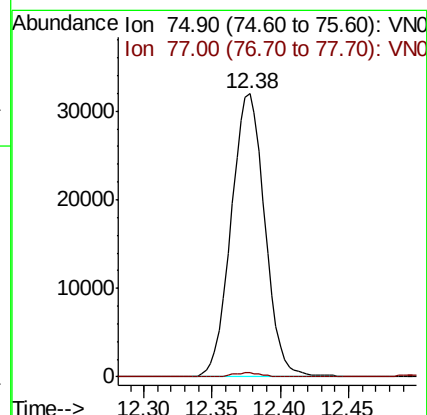


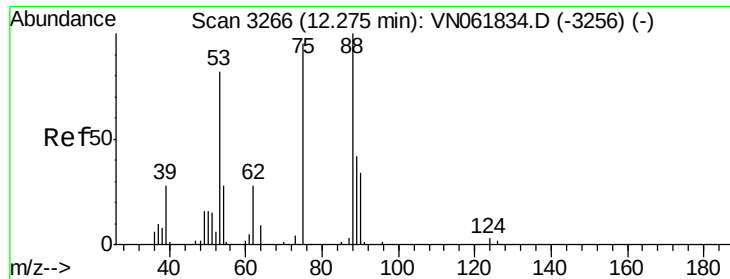




#81
trans-1,4-Dichloro-2-butene
Concen: 71.290 ug/l
RT: 12.38 min Scan# 3298
Delta R.T. 0.10 min
Lab File: VN061843.D
Acq: 17 Jun 2020 13:04

Instrument :
MSVOA_N
ClientSampleId :
RE125D1-20200609DL

Tot Ion: 75 Resp: 54773
Ion Ratio Lower Upper
75 100
53 0.0 70.4 105.6#
89 0.0 36.0 54.0#

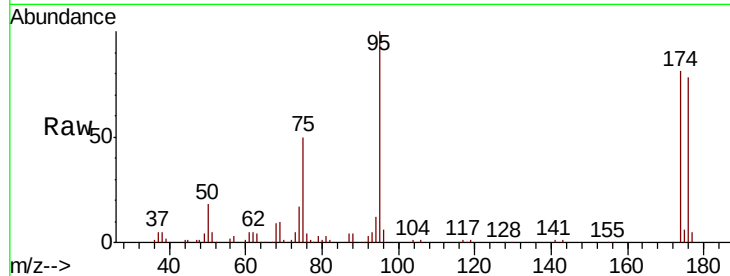


Abundance Ion 74.90 (74.60 to 75.60): VN0
Ion 53.00 (52.70 to 53.70): VN0
Ion 88.90 (88.60 to 89.60): VN0

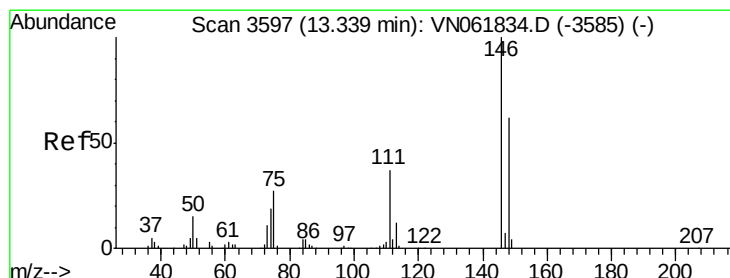
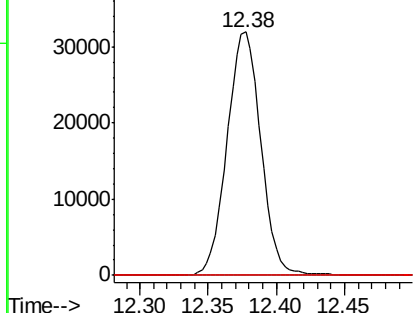



#88
1,4-Dichlorobenzene
Concen: 0.214 ug/l
RT: 13.34 min Scan# 3598
Delta R.T. 0.00 min
Lab File: VN061843.D
Acq: 17 Jun 2020 13:04

Tgt Ion: 146 Resp: 764
Ion Ratio Lower Upper
146 100
111 0.0 19.3 57.8#
148 0.0 31.6 94.7#

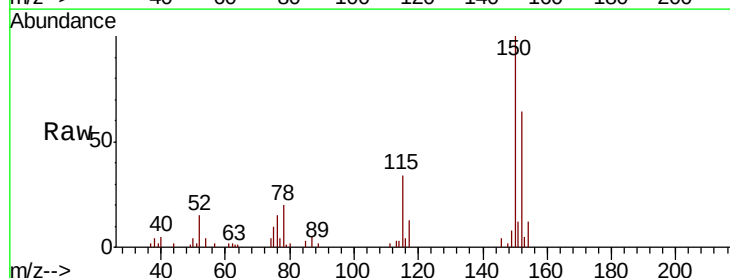

Abundance Ion 145.90 (145.60 to 146.60): V
Ion 110.90 (110.60 to 111.60): V
Ion 147.90 (147.60 to 148.60): V




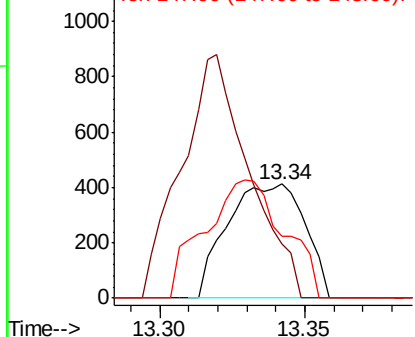




#93
 1,2,4-Trichlorobenzene
 Concen: 0.467 ug/l
 RT: 14.89 min Scan# 4079
 Delta R.T. 0.01 min
 Lab File: VN061843.D
 Acq: 17 Jun 2020 13:04




Instrument :
 MSVOA_N
 ClientSampleId :
 RE125D1-20200609DL


Tot Ion:180 Resp: 741
 Ion Ratio Lower Upper
 180 100
 182 100.0 47.0 141.2
 145 0.0 15.8 47.3#

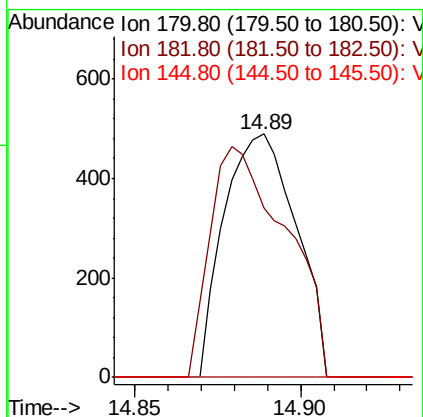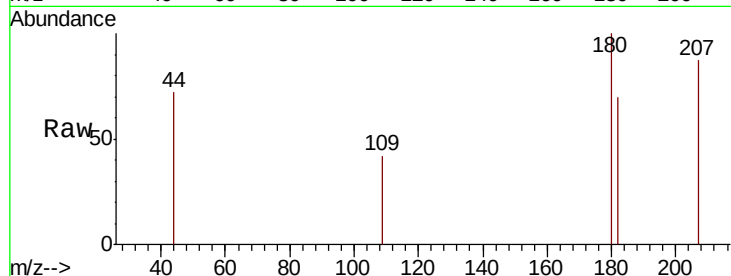

#95
 Naphthalene
 Concen: 4.074 ug/l
 RT: 15.11 min Scan# 4148
 Delta R.T. 0.01 min
 Lab File: VN061843.D
 Acq: 17 Jun 2020 13:04

Tgt Ion:128 Resp: 3374
 Ion Ratio Lower Upper
 128 100
 127 8.1 10.3 15.5#
 129 3.3 8.6 13.0#

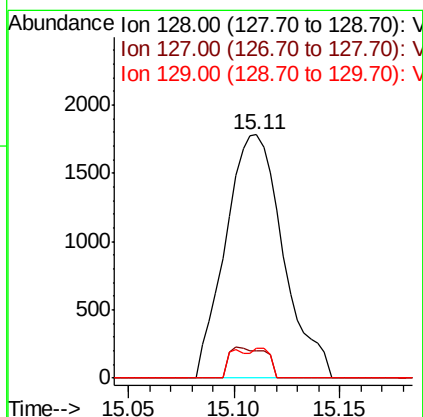



#96
 1,2,3-Trichlorobenzene
 Concen: 0.540 ug/l
 RT: 15.29 min Scan# 4204
 Delta R.T. 0.01 min
 Lab File: VN061843.D
 Acq: 17 Jun 2020 13:04

Instrument :
 MSVOA_N
 ClientSampleId :
 RE125D1-20200609DL

Tot Ion	Ratio	Lower	Upper
180	100		
182	71.0	47.9	143.6
145	7.3	16.5	49.5

