


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN061720\  
Data File : VN061838.D  
Acq On : 17 Jun 2020 9:14  
Operator : JC/MD  
Sample : BFB  
Misc : 5.00mL/MSVOA N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N061620W.M  
Title : SW846 8260  
Last Update : Wed Jun 17 01:19:44 2020

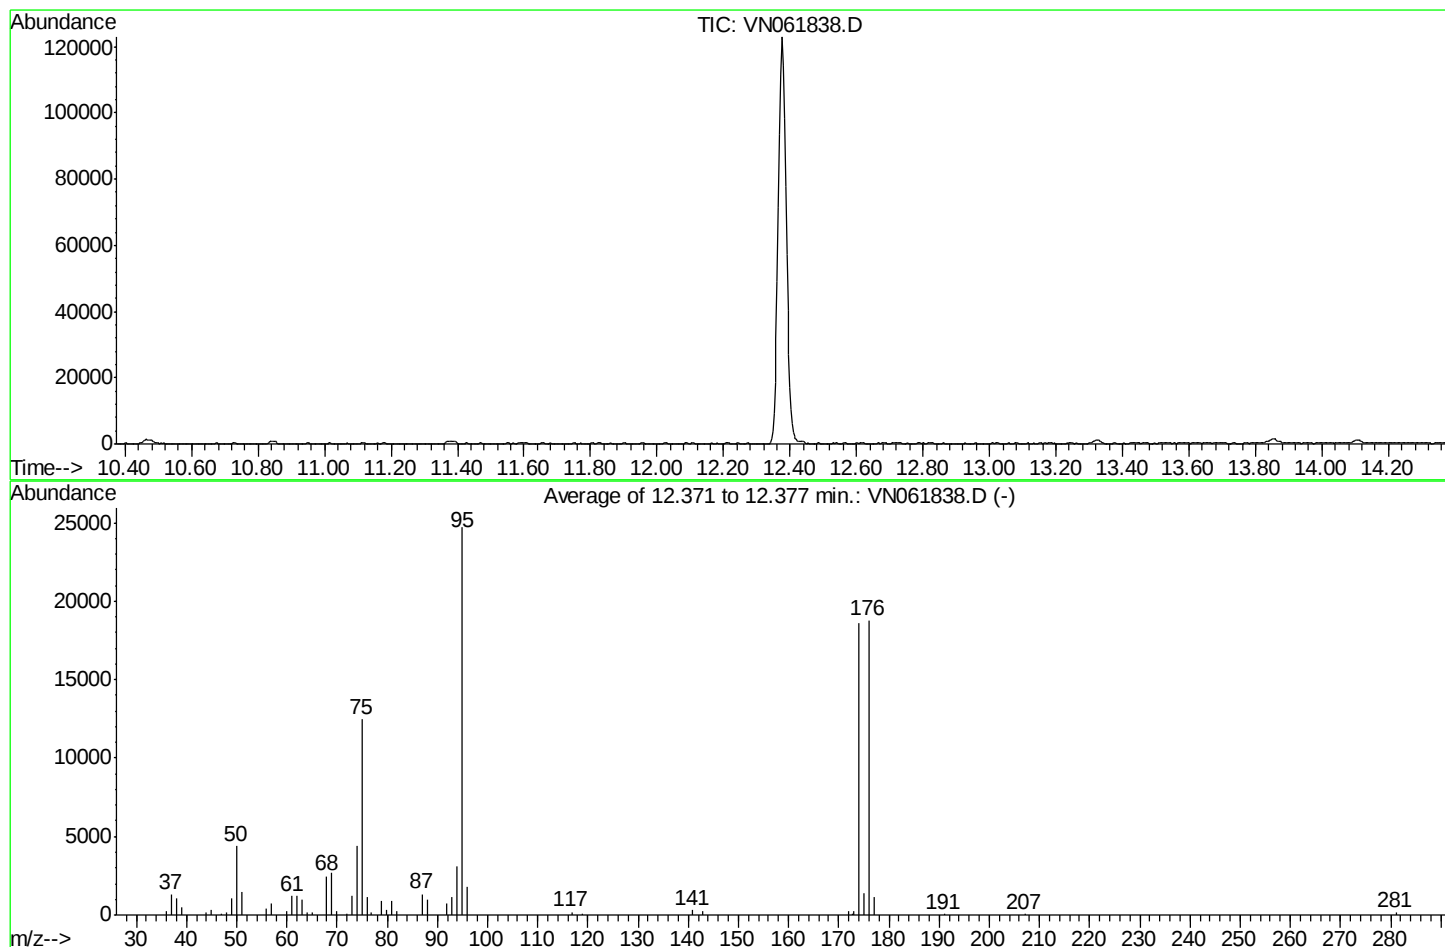

AutoFind: Scans 3296, 3297, 3298; Background Corrected with Scan 3284

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 17.8      | 4387    | PASS             |
| 75          | 95           | 30           | 60           | 50.4      | 12459   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 24709   | PASS             |
| 96          | 95           | 5            | 9            | 7.2       | 1770    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.3       | 250     | PASS             |
| 174         | 95           | 50           | 100          | 75.3      | 18600   | PASS             |
| 175         | 174          | 5            | 9            | 7.6       | 1422    | PASS             |
| 176         | 174          | 95           | 101          | 100.8     | 18754   | PASS             |
| 177         | 176          | 5            | 9            | 6.3       | 1181    | PASS             |