


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN061720\
 Data File : VN061864.D
 Acq On : 17 Jun 2020 21:52
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061620W.M
 Title : SW846 8260
 Last Update : Wed Jun 17 01:19:44 2020

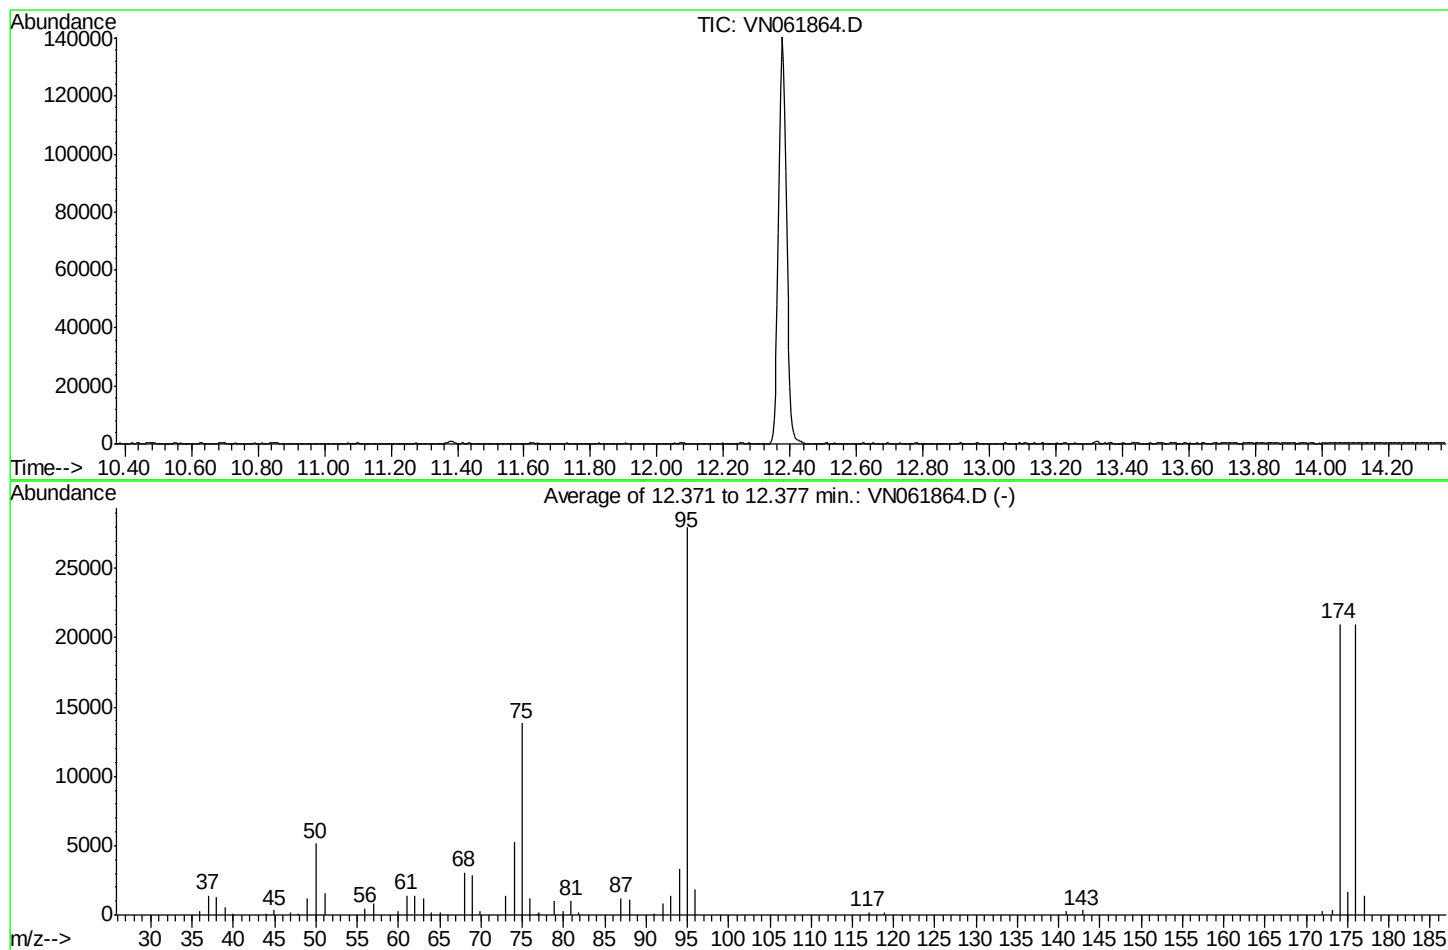

AutoFind: Scans 3296, 3297, 3298; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	5140	PASS
75	95	30	60	49.4	13815	PASS
95	95	100	100	100.0	27970	PASS
96	95	5	9	6.5	1818	PASS
173	174	0.00	2	1.6	329	PASS
174	95	50	100	75.1	21002	PASS
175	174	5	9	7.8	1647	PASS
176	174	95	101	99.8	20960	PASS
177	176	5	9	6.6	1391	PASS