


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061721\
Data File : VN067370.D
Acq On : 17 Jun 2021 8:47
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N061121W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Sat Jun 12 09:13:15 2021

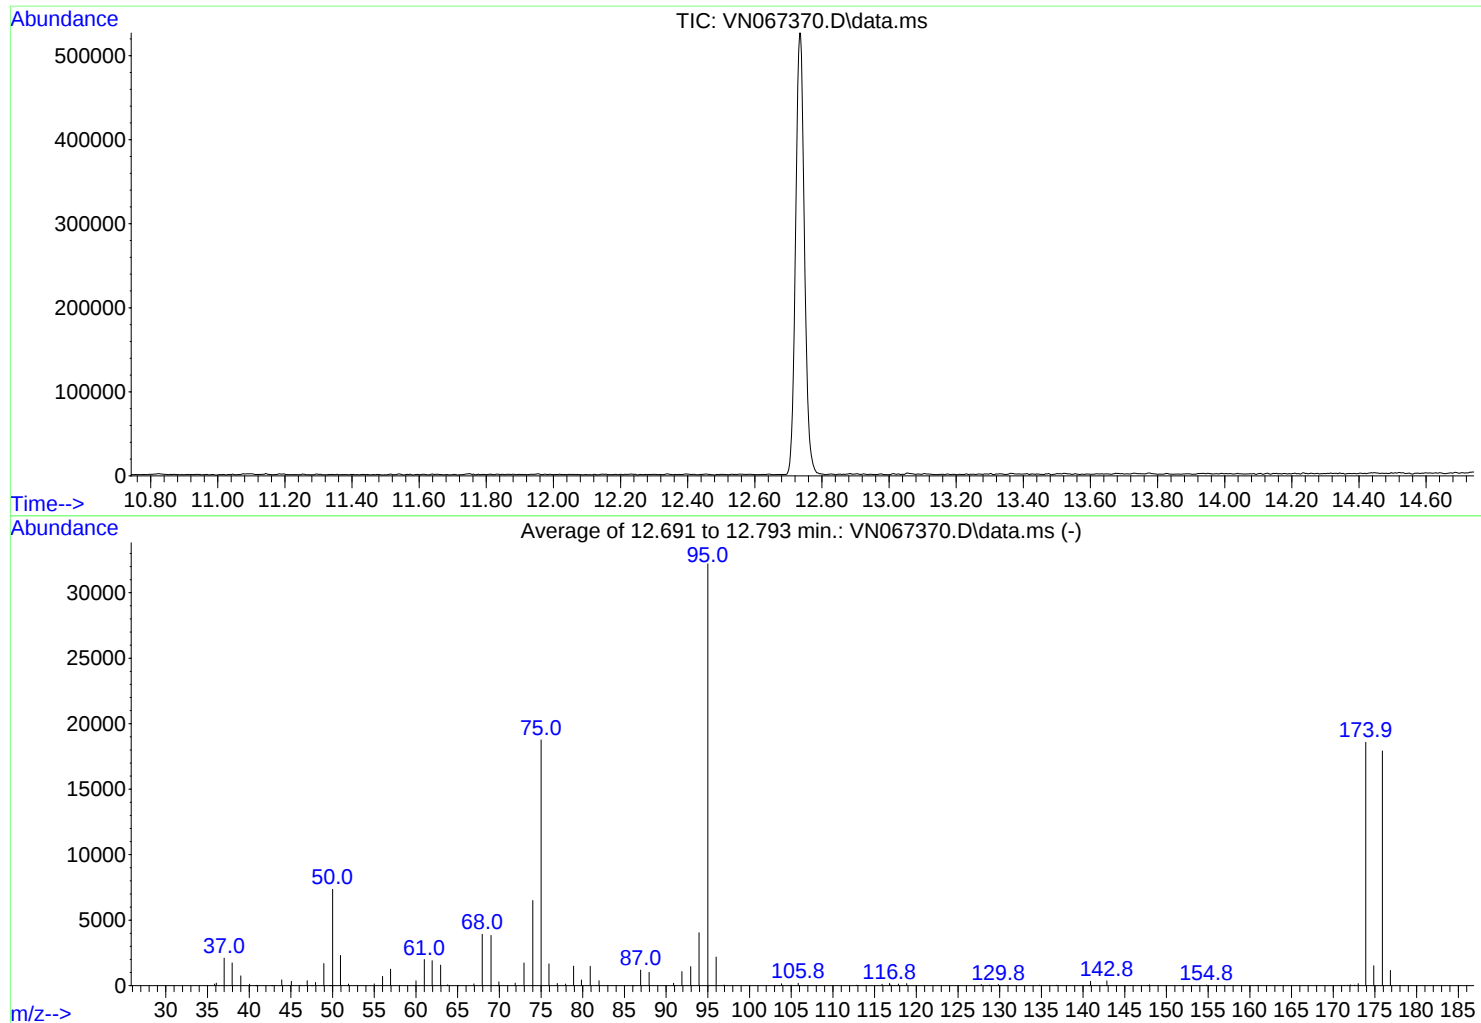

AutoFind: Averaged scan 3990 to 4028; Bkg corrected with scan 3989

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.8	7356	PASS
75	95	30	60	58.3	18761	PASS
95	95	100	100	100.0	32207	PASS
96	95	5	9	6.8	2189	PASS
173	174	0.00	2	0.8	157	PASS
174	95	50	100	57.7	18583	PASS
175	174	5	9	8.1	1511	PASS
176	174	95	101	96.5	17929	PASS
177	176	5	9	6.5	1157	PASS