


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061721\
 Data File : VN067370.D
 Acq On : 17 Jun 2021 8:47
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061421W.M
 Title : SW846 8260
 Last Update : Tue Jun 15 05:19:42 2021

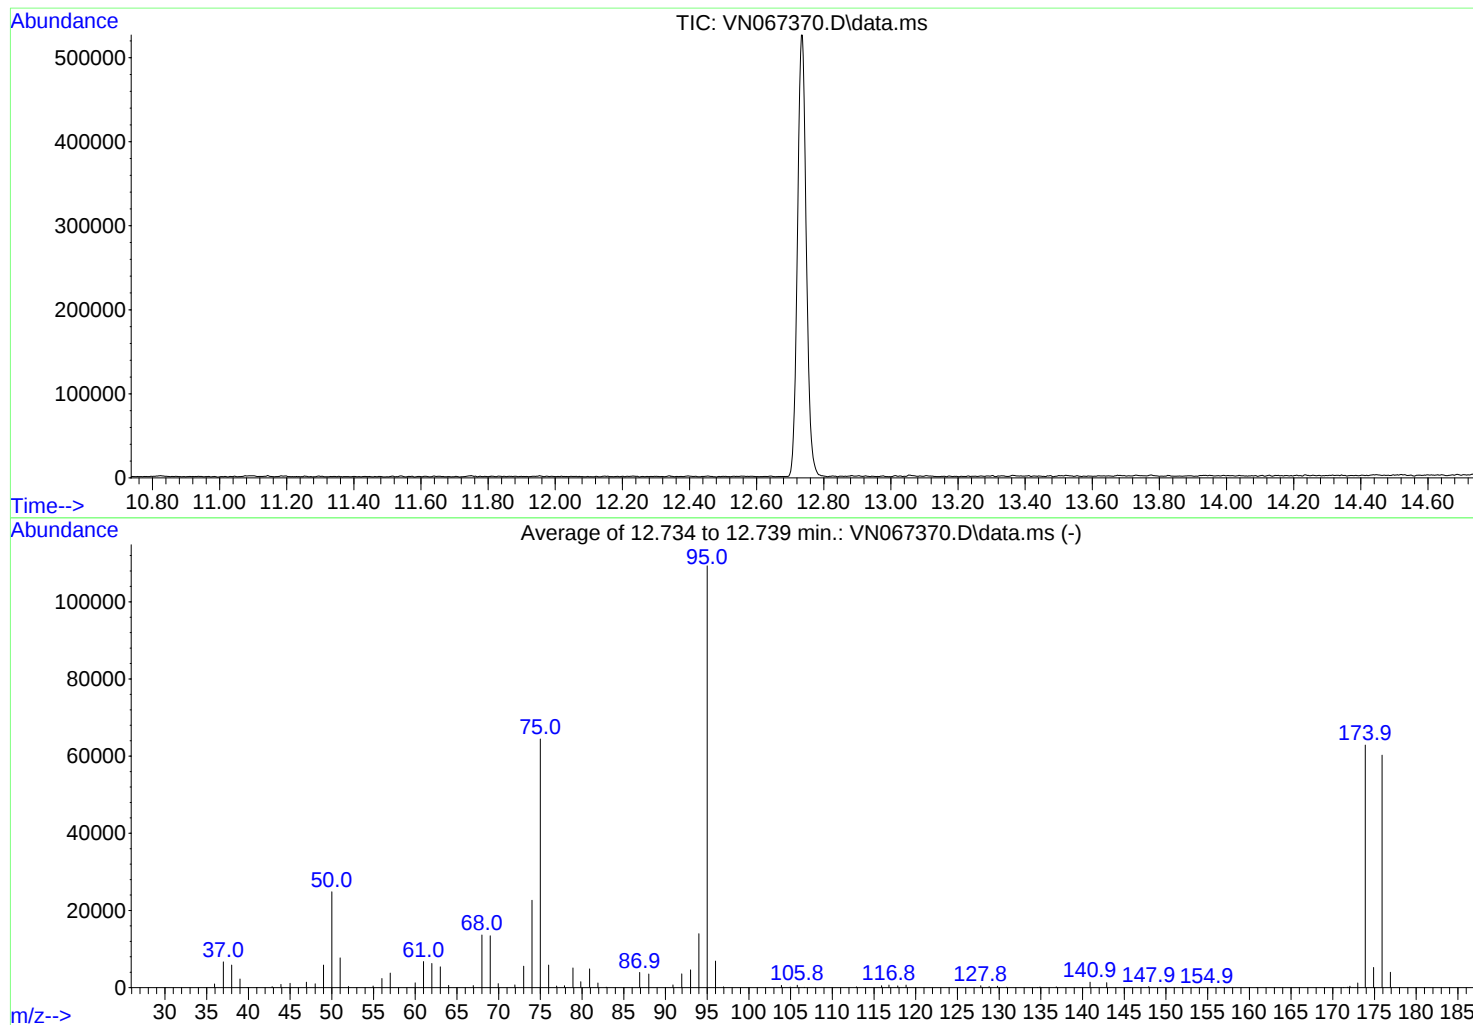

AutoFind: Scans 4006, 4007, 4008; Background Corrected with Scan 3988

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	24837	PASS
75	95	30	60	59.0	64461	PASS
95	95	100	100	100.0	109320	PASS
96	95	5	9	6.3	6887	PASS
173	174	0.00	2	1.9	1191	PASS
174	95	50	100	57.5	62880	PASS
175	174	5	9	8.3	5222	PASS
176	174	95	101	95.8	60264	PASS
177	176	5	9	6.6	3972	PASS