
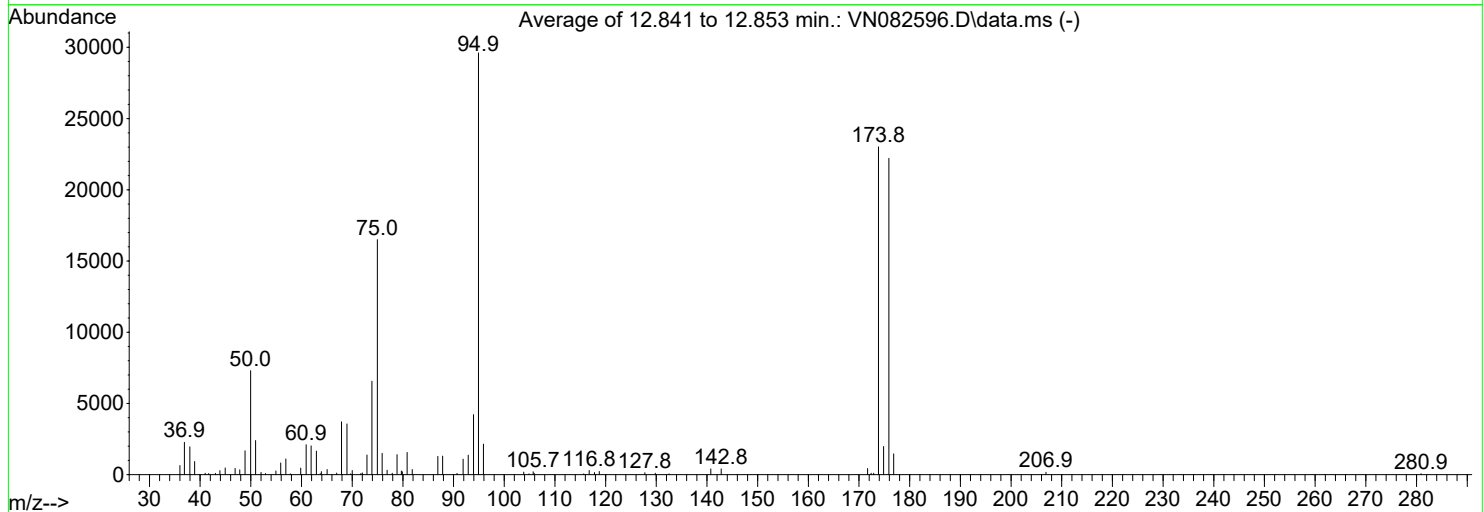


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061724\
Data File : VN082596.D
Acq On : 17 Jun 2024 08:46
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061724W.M
Title : SW846 8260
Last Update : Tue Jun 18 04:52:44 2024

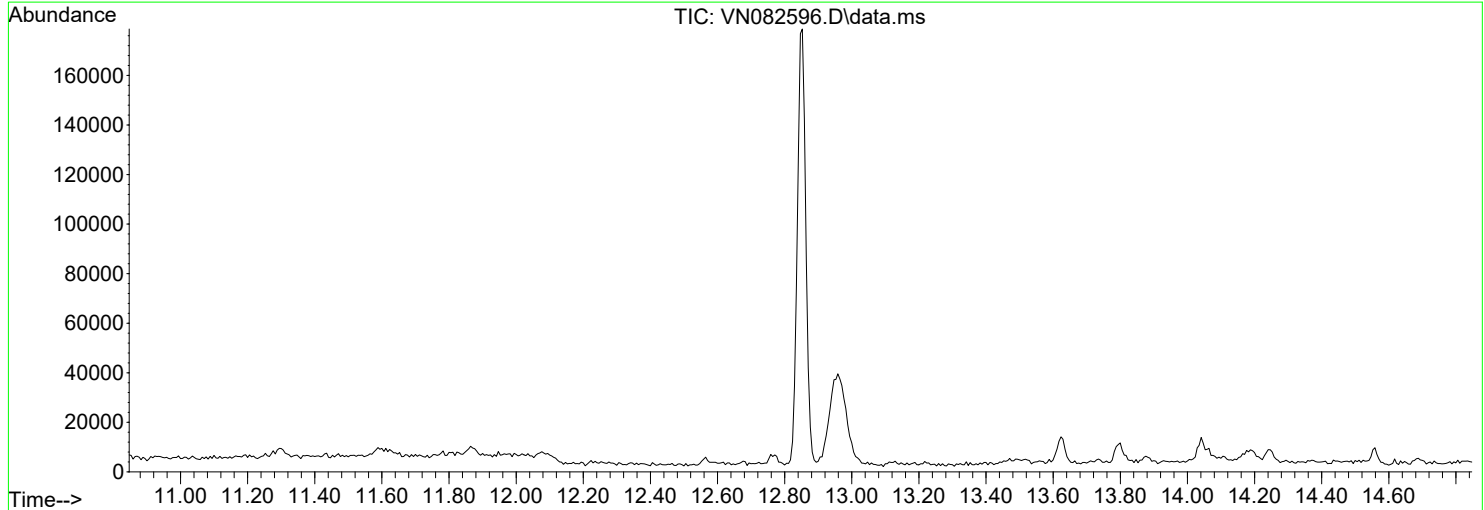

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.7	7302	PASS
75	95	30	60	55.7	16502	PASS
95	95	100	100	100.0	29613	PASS
96	95	5	9	7.2	2145	PASS
173	174	0.00	2	0.4	96	PASS
174	95	50	100	77.7	23013	PASS
175	174	5	9	8.6	1976	PASS
176	174	95	101	96.5	22211	PASS
177	176	5	9	6.6	1456	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	640	47.80	335	60.90	2100	71.70	71
36.90	2273	48.85	1677	61.90	2021	72.00	12
37.95	1951	49.95	7302	62.95	1650	72.90	138
38.90	916	50.95	2389	63.70	73	73.90	656
39.85	12	52.00	159	63.90	209	74.95	16502
41.00	103	52.90	80	65.05	365	75.90	1498
41.70	84	54.95	263	66.95	113	76.90	313
43.00	93	55.90	819	67.90	3709	77.90	97
43.90	276	56.90	1103	68.95	3564	78.85	1403
44.95	477	57.80	53	69.70	52	79.70	257
46.90	439	59.85	456	70.00	294	79.90	197

Average of 12.841 to 12.853 min.: VN082596.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.85	1560	104.90	55	142.80	410		
81.85	361	105.70	203	171.70	430		
86.90	1280	105.90	92	172.40	99		
87.85	1298	115.70	62	172.90	96		
90.70	91	116.75	297	173.85	23013		
91.90	1089	117.80	141	174.85	1976		
92.90	1366	118.75	229	175.90	22211		
93.95	4208	127.75	140	176.85	1456		
94.90	29613	129.80	107	206.90	164		
95.90	2145	132.50	51	280.90	66		
103.85	179	140.75	410				

Instrument :

MSVOA_N

ClientSampleId :

BFB