


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN061818\
Data File : VN049332.D
Acq On : 18 Jun 2018 10:00
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061618W.M
Title : SW846 8260
Last Update : Sat Jun 16 01:02:01 2018

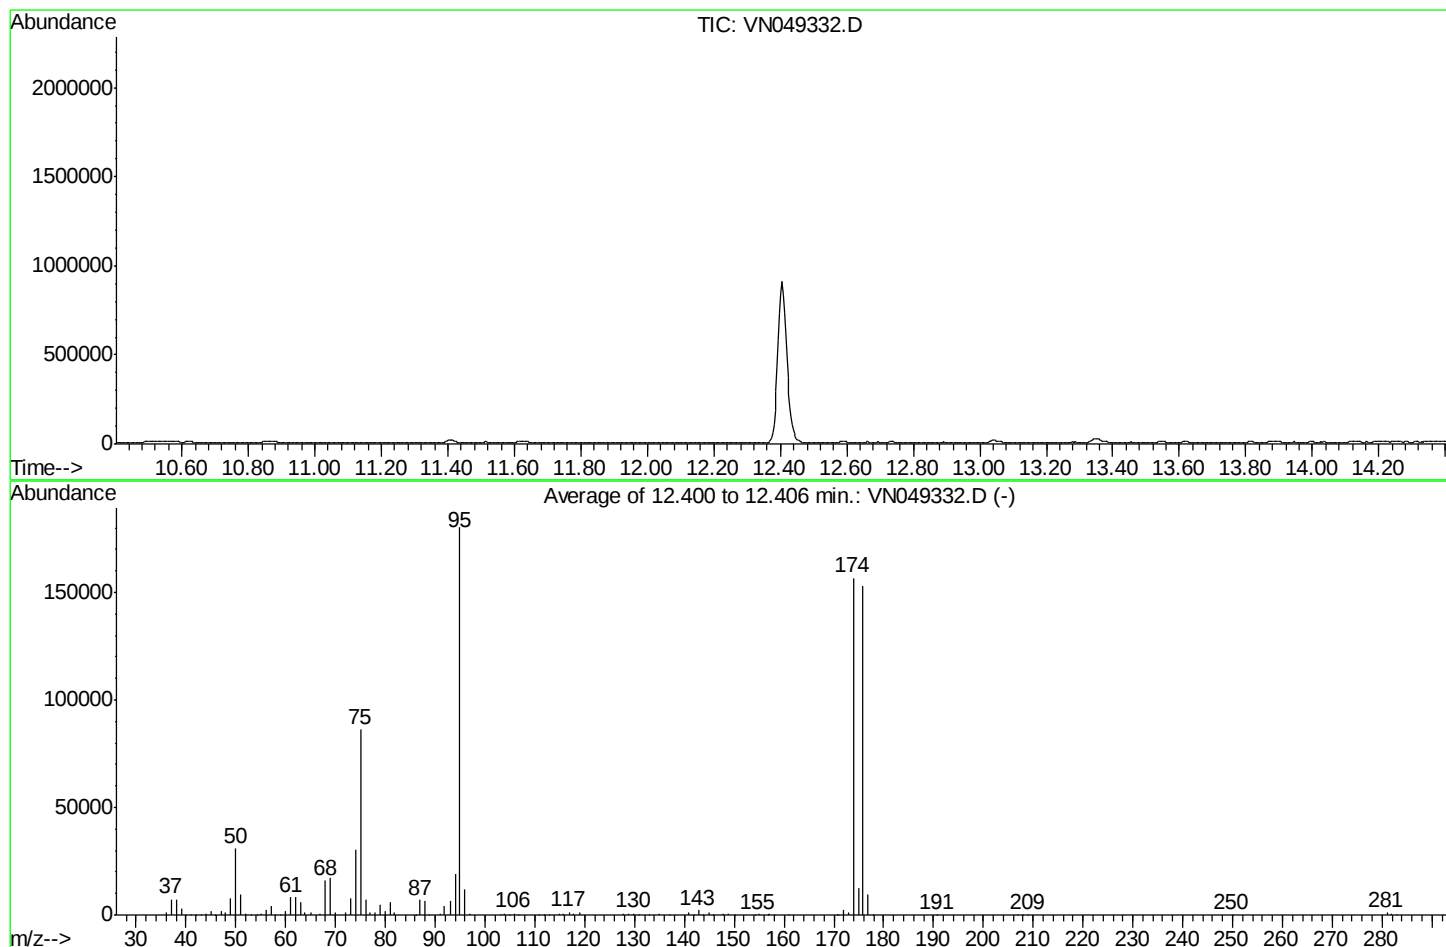

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	30709	PASS
75	95	30	60	47.9	86237	PASS
95	95	100	100	100.0	180202	PASS
96	95	5	9	6.6	11908	PASS
173	174	0.00	2	0.8	1207	PASS
174	95	50	100	87.0	156714	PASS
175	174	5	9	8.0	12599	PASS
176	174	95	101	97.4	152640	PASS
177	176	5	9	6.4	9832	PASS