

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN061820\
 Data File : VN061922.D
 Acq On : 19 Jun 2020 1:17
 Operator : JC/MD
 Sample : PB129596TB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB129596TB

Quant Time: Jun 19 05:33:04 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061620W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 17 01:19:44 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	143990	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	266644	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	270569	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	102066	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	96268	49.85	ug/l	0.00
Spiked Amount			Recovery	=	99.70%	
35) Dibromofluoromethane	7.55	113	85510	50.13	ug/l	0.00
Spiked Amount			Recovery	=	100.26%	
50) Toluene-d8	10.06	98	341438	50.91	ug/l	0.00
Spiked Amount			Recovery	=	101.82%	
62) 4-Bromofluorobenzene	12.38	95	113252	49.23	ug/l	0.00
Spiked Amount			Recovery	=	98.46%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	4.72	59	230	0.861	ug/l #	74
16) Acetone	3.78	43	5868	10.287	ug/l	96
18) Methyl Acetate	4.29	43	2018	1.229	ug/l #	63
20) Methylene Chloride	4.50	84	2236	1.203	ug/l #	80
25) 2-Butanone	6.79	43	1927	2.315	ug/l	99
29) Tetrahydrofuran	7.18	42	188	0.343	ug/l #	26
31) Cyclohexane	7.62	56	3057	1.201	ug/l #	17
36) 1,1-Dichloropropene	7.63	75	11625	4.780	ug/l #	49
37) Ethyl Acetate	6.79	43	1927	1.015	ug/l #	65
38) Carbon Tetrachloride	7.63	117	14366	5.965	ug/l #	16
43) Isopropyl Acetate	8.12	43	35347	11.044	ug/l #	89
45) 1,2-Dichloropropane	9.24	63	868	0.479	ug/l #	43
48) Methyl methacrylate	9.15	41	2171	1.492	ug/l #	5
51) 4-Methyl-2-Pentanone	9.95	43	2900	1.533	ug/l	90
52) Toluene	10.13	92	2761	0.597	ug/l	93
54) cis-1,3-Dichloropropene	9.88	75	18410	6.116	ug/l #	69
56) Ethyl methacrylate	10.51	69	723	3.147	ug/l #	1
57) 1,3-Dichloropropane	10.74	76	3568	1.157	ug/l #	42
59) 2-Hexanone	10.74	43	42995	40.335	ug/l #	50
71) Bromoform	12.38	173	1111	0.765	ug/l #	1
74) N-amyl acetate	12.01	43	1671	3.661	ug/l #	38
76) 1,2,3-Trichloropropane	12.38	75	58205	29.047	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.71	105	2427	0.404	ug/l	98
81) trans-1,4-Dichloro-2-buten	12.38	75	58205	79.224	ug/l #	14
95) Naphthalene	15.12	128	781	3.626	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN061820\
Data File : VN061922.D
Acq On : 19 Jun 2020 1:17
Operator : JC/MD
Sample : PB129596TB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB129596TB

Quant Time: Jun 19 05:33:04 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061620W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 17 01:19:44 2020
Response via : Initial Calibration

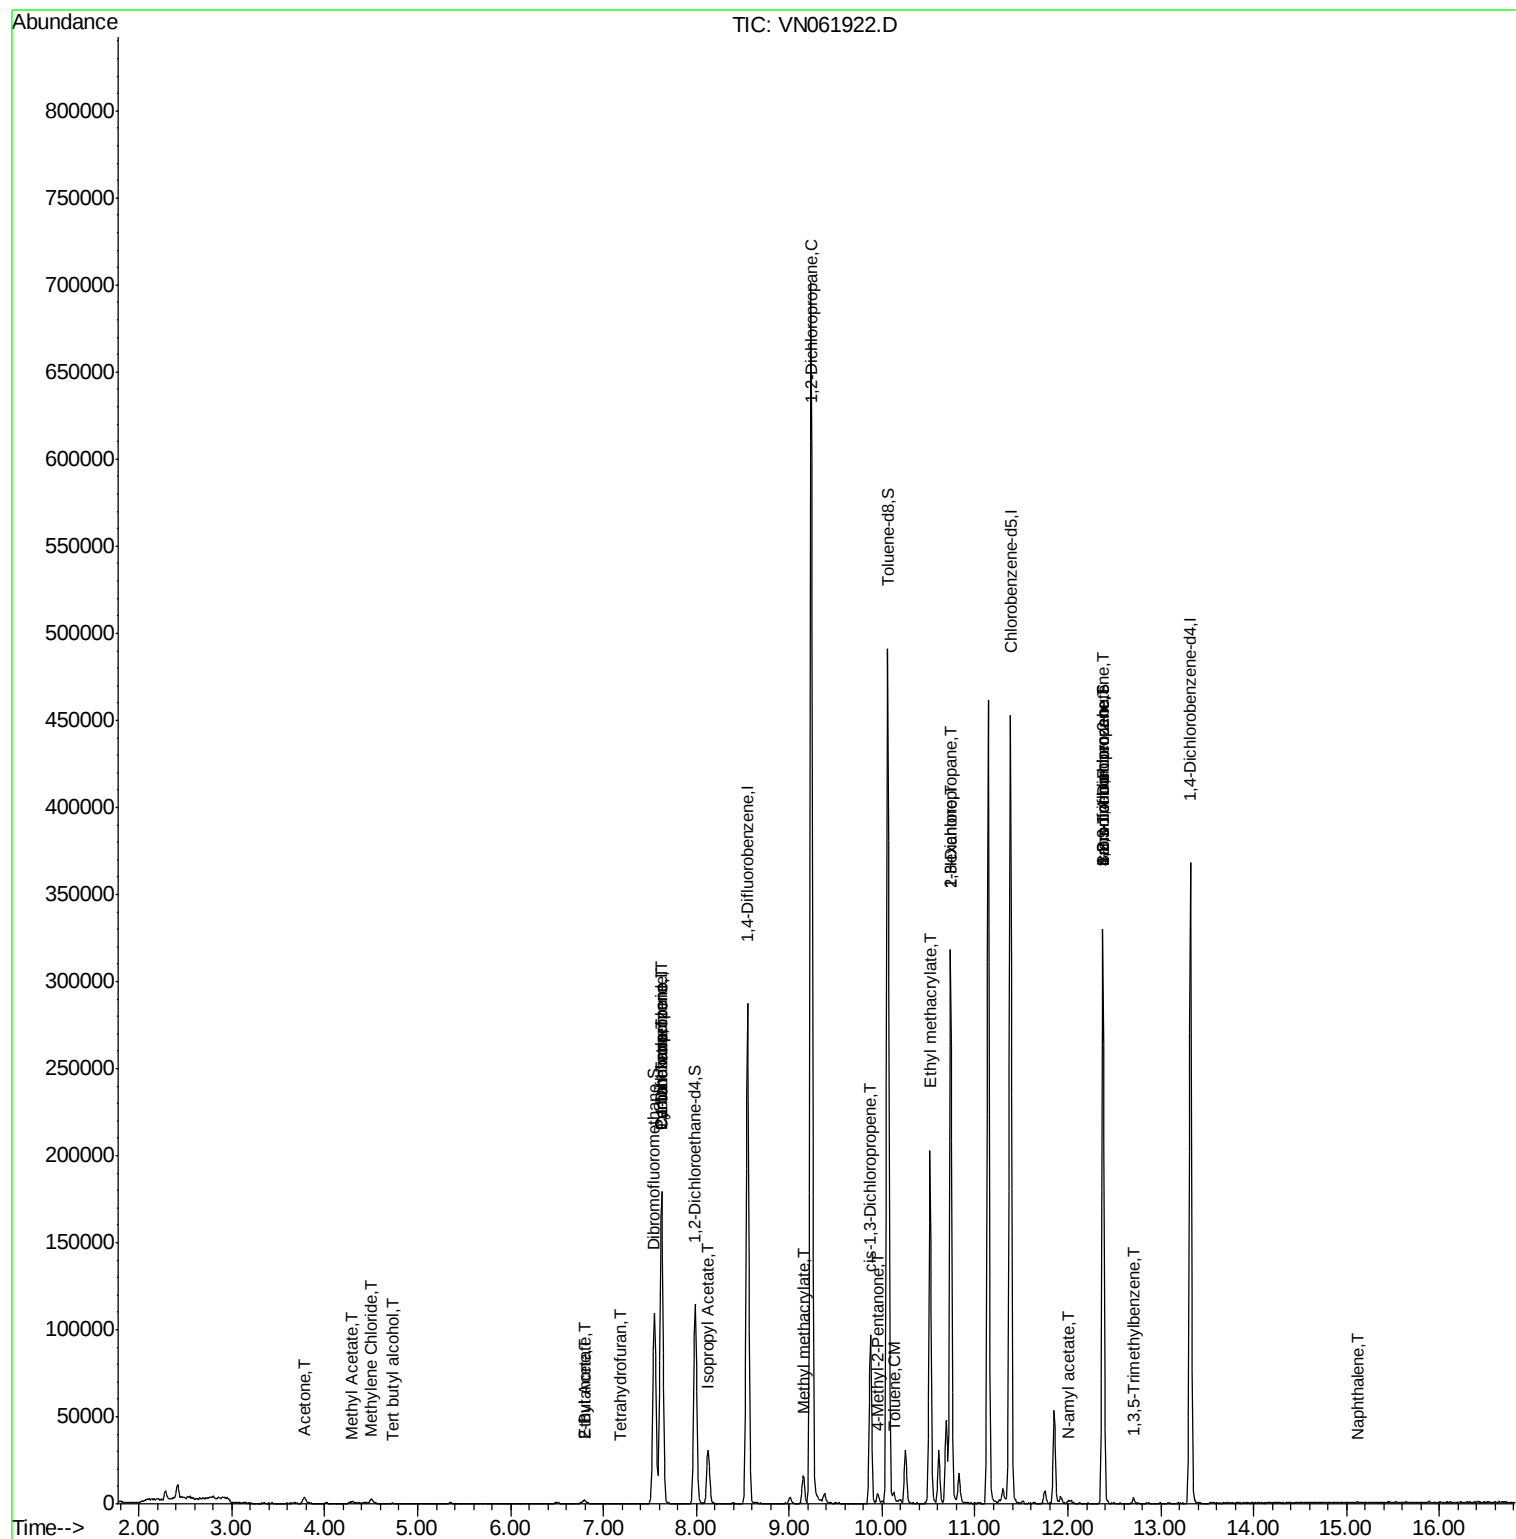



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. -0.00 min

Lab File: VN061922.D

Acq: 19 Jun 2020 1:17

Instrument :

MSVOA_N

ClientSampleId :


PB129596TB

Tot Ion:168 Resp: 143990

Ion Ratio Lower Upper




168 100

99 57.2 44.6 67.0

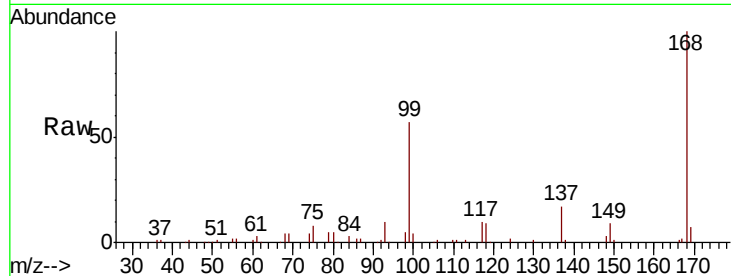

Abundance Ion 167.90 (167.60 to 168.60): VN061834.D (-1801) (-)

Ion 98.90 (98.60 to 99.60): VN061834.D (-1801) (-)

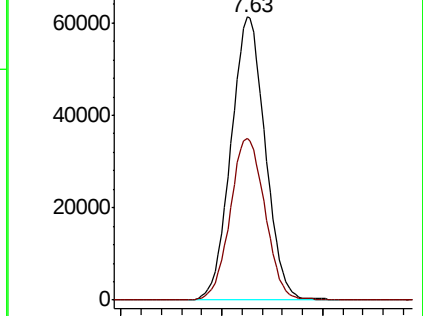

#11

Tert butyl alcohol

Concen: 0.861 ug/l

RT: 4.72 min Scan# 918

Delta R.T. -0.01 min

Lab File: VN061922.D


Acq: 19 Jun 2020 1:17

Tgt Ion: 59 Resp: 230

Ion Ratio Lower Upper



59 100


57 0.0 7.7 11.5#



Abundance Ion 59.00 (58.70 to 59.70): VN061834.D (-895) (-)

Ion 57.00 (56.70 to 57.70): VN061834.D (-895) (-)

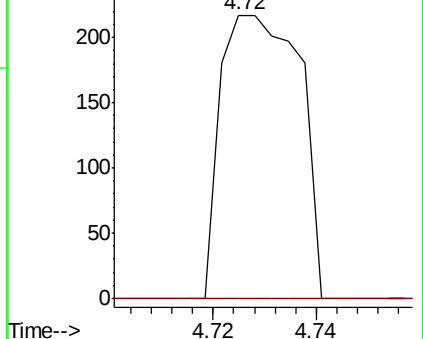



#16

Acetone

Concen: 10.287 ug/l

RT: 3.78 min Scan# 625

Delta R.T. 0.01 min

Lab File: VN061922.D

Acq: 19 Jun 2020 1:17

Instrument :

MSVOA_N

ClientSampleId :


PB129596TB

Tot Ion: 43 Resp: 5868

Ion Ratio Lower Upper




43 100

58 32.5 27.8 41.8



Abundance Ion 43.00 (42.70 to 43.70): VN061922.D (-529) (-)

Ion 58.00 (57.70 to 58.70): VN061922.D (-529) (-)

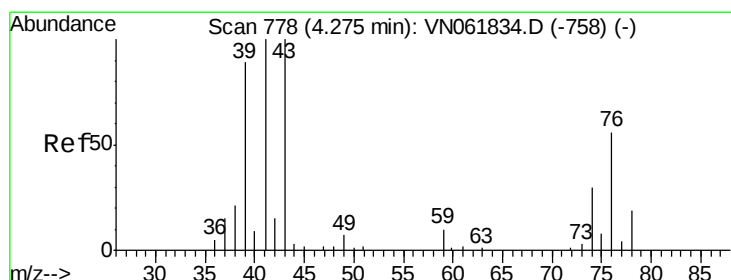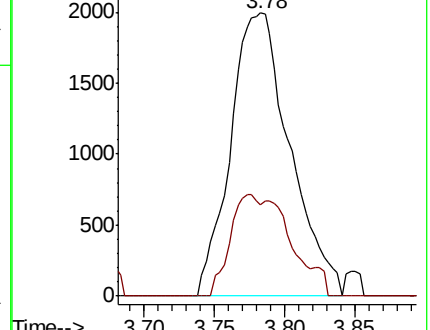

#18

Methyl Acetate

Concen: 1.229 ug/l

RT: 4.29 min Scan# 783

Delta R.T. 0.02 min

Lab File: VN061922.D


Acq: 19 Jun 2020 1:17

Tgt Ion: 43 Resp: 2018

Ion Ratio Lower Upper



43 100


74 8.8 23.0 34.4#



Abundance Ion 43.00 (42.70 to 43.70): VN061922.D (-685) (-)

Ion 74.00 (73.70 to 74.70): VN061922.D (-685) (-)




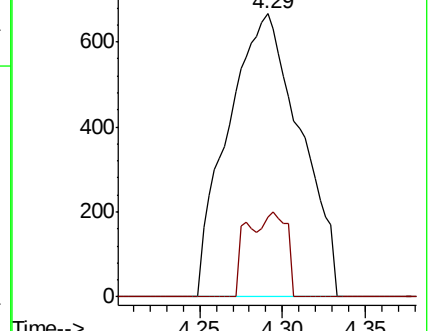




#20
Methvlene Chloride
Concen: 1.203 ug/l
RT: 4.50 min Scan# 847
Delta R.T. -0.00 min
Lab File: VN061922.D
Acq: 19 Jun 2020 1:17




Instrument :
MSVOA_N
ClientSampled :
PB129596TB


Tot Ion: 84 Resp: 2236
Ion Ratio Lower Upper
84 100
49 86.0 87.0 130.4#
51 27.0 27.8 41.6#
86 45.4 50.2 75.2#

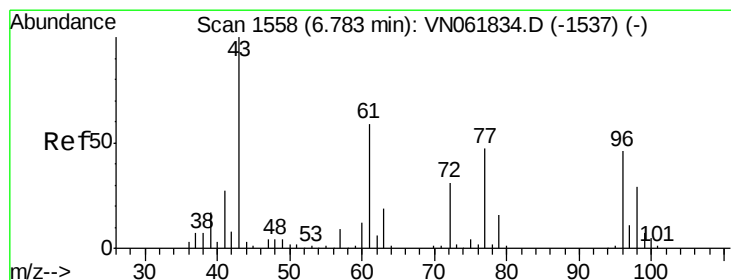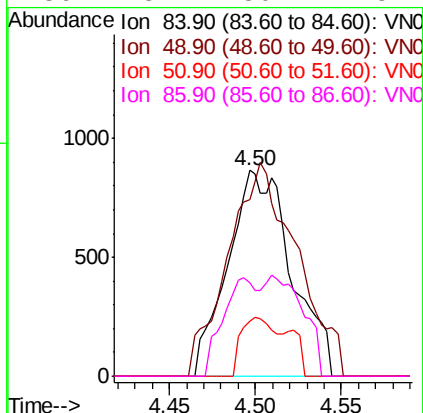

#25
2-Butanone
Concen: 2.315 ug/l
RT: 6.79 min Scan# 1561
Delta R.T. 0.01 min
Lab File: VN061922.D
Acq: 19 Jun 2020 1:17

Tgt Ion: 43 Resp: 1927
Ion Ratio Lower Upper
43 100
72 30.4 24.6 37.0


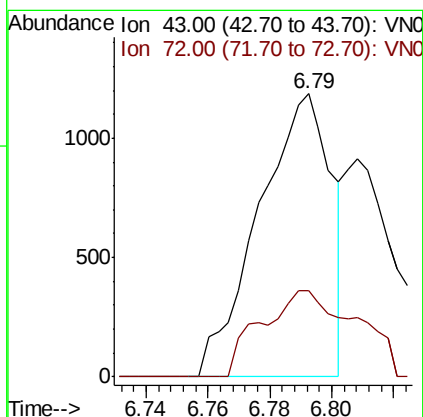






#29
Tetrahydrofuran
Concen: 0.343 ug/l
RT: 7.18 min Scan# 1681
Delta R.T. 0.01 min
Lab File: VN061922.D
Acq: 19 Jun 2020 1:17




Instrument :
MSVOA_N
ClientSampleId :
PB129596TB


Tot Ion: 42 Resp: 188
Ion Ratio Lower Upper
42 100
72 0.0 44.0 66.0#
71 0.0 40.0 60.0#

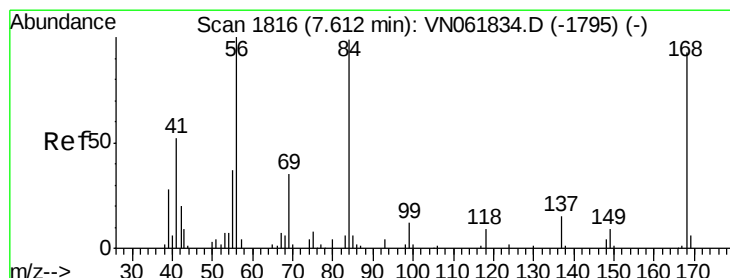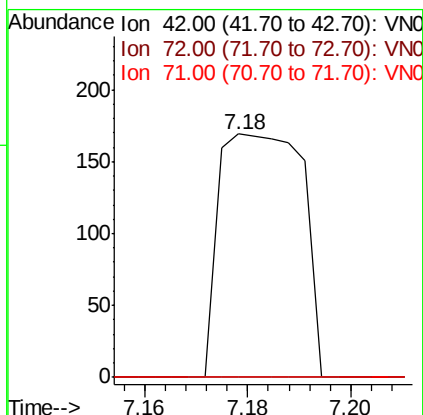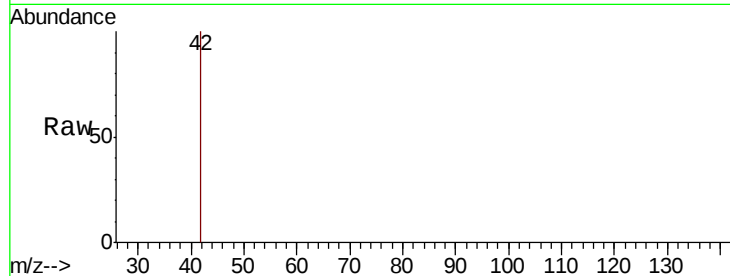

#31
Cyclohexane
Concen: 1.201 ug/l
RT: 7.62 min Scan# 1819
Delta R.T. 0.01 min
Lab File: VN061922.D
Acq: 19 Jun 2020 1:17

Tgt Ion: 56 Resp: 3057
Ion Ratio Lower Upper
56 100
69 169.9 27.7 41.5#
84 128.5 79.1 118.7#



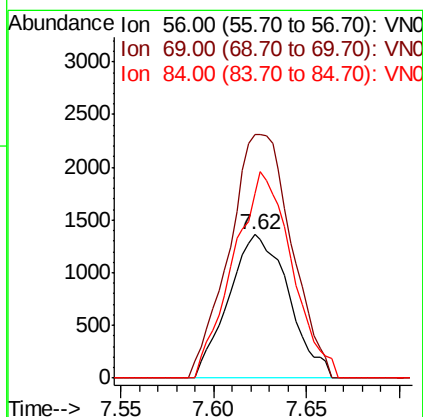
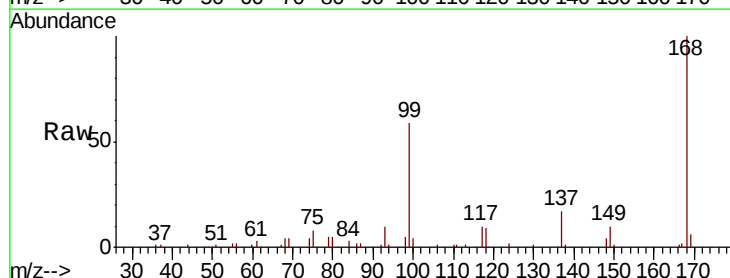




#33
 1,2-Dichloroethane-d4
 Concen: 49.851 ug/l
 RT: 7.99 min Scan# 1933
 Delta R.T. -0.00 min
 Lab File: VN061922.D
 Acq: 19 Jun 2020 1:17




Instrument :
 MSVOA_N
 ClientSampleId :
 PB129596TB


Tot Ion: 65 Resp: 96268
 Ion Ratio Lower Upper
 65 100
 67 53.4 0.0 106.2

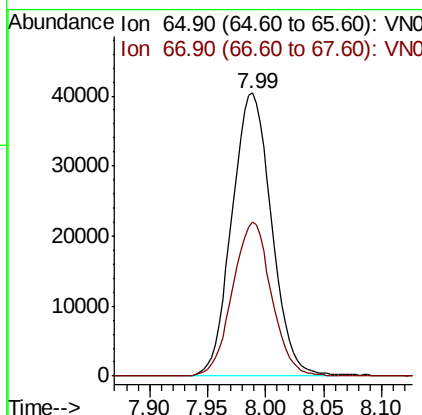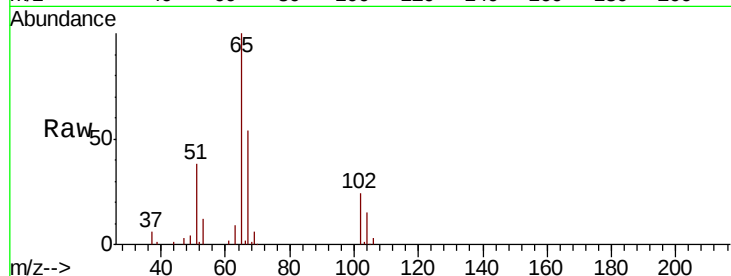

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2108
 Delta R.T. -0.00 min
 Lab File: VN061922.D
 Acq: 19 Jun 2020 1:17

Tgt Ion: 114 Resp: 266644
 Ion Ratio Lower Upper
 114 100
 63 18.0 0.0 37.6
 88 15.5 0.0 31.0



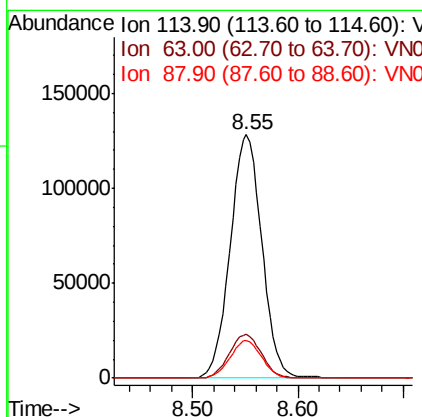





#35
 Dibromofluoromethane
 Concen: 50.128 ug/l
 RT: 7.55 min Scan# 1797
 Delta R.T. 0.00 min
 Lab File: VN061922.D
 Acq: 19 Jun 2020 1:17




Instrument :
 MSVOA_N
 ClientSampleId :
 PB129596TB


Tot Ion:113 Resp: 85510
 Ion Ratio Lower Upper
 113 100
 111 103.1 83.7 125.5
 192 17.5 13.9 20.9

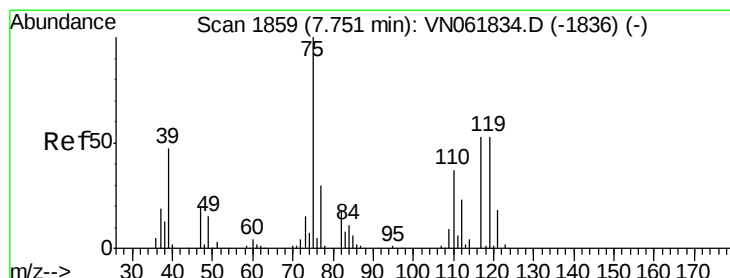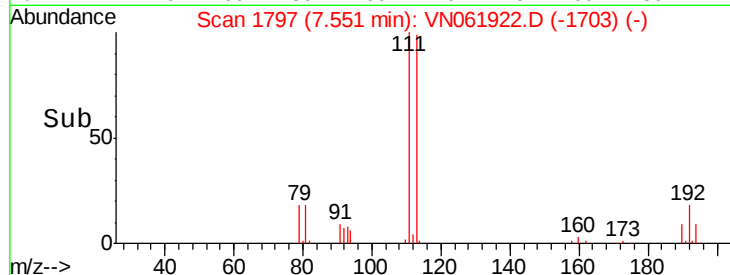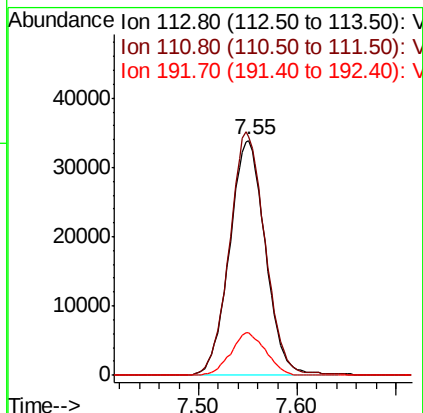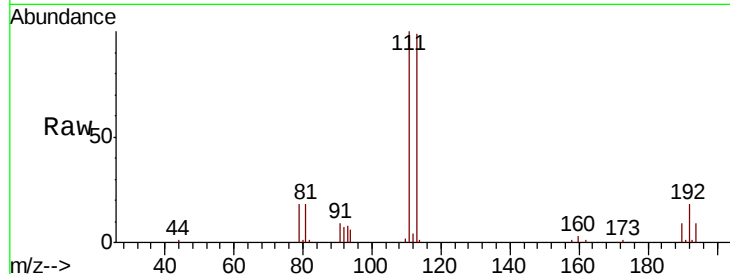

#36
 1,1-Dichloropropene
 Concen: 4.780 ug/l
 RT: 7.63 min Scan# 1821
 Delta R.T. -0.12 min
 Lab File: VN061922.D
 Acq: 19 Jun 2020 1:17

Tgt Ion: 75 Resp: 11625
 Ion Ratio Lower Upper
 75 100
 110 8.2 18.2 54.6#
 77 0.0 24.2 36.4#



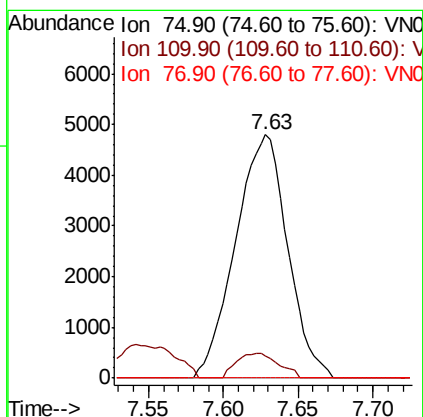
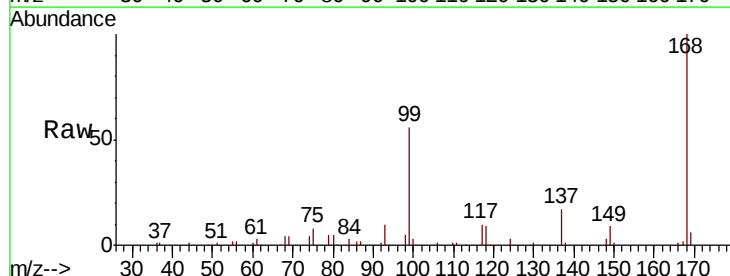




#37
Ethyl Acetate
Concen: 1.015 ug/l
RT: 6.79 min Scan# 1561
Delta R.T. -0.09 min
Lab File: VN061922.D
Acq: 19 Jun 2020 1:17




Instrument :
MSVOA_N
ClientSampleId :
PB129596TB


Tot Ion: 43 Resp: 1927
Ion Ratio Lower Upper
43 100
61 0.0 13.0 19.4#
70 0.0 9.4 14.2#

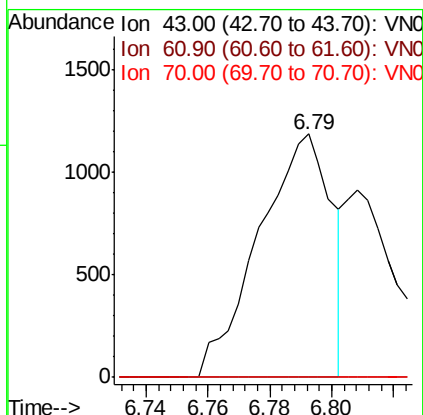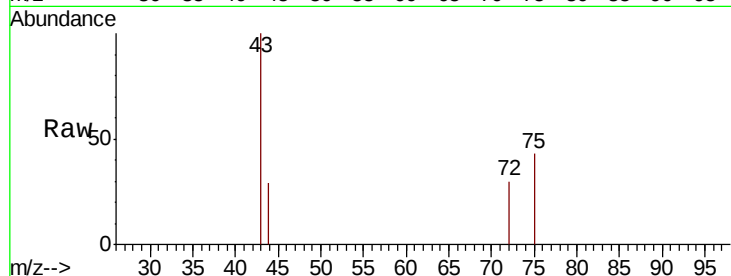

#38
Carbon Tetrachloride
Concen: 5.965 ug/l
RT: 7.63 min Scan# 1821
Delta R.T. -0.11 min
Lab File: VN061922.D
Acq: 19 Jun 2020 1:17

Tgt Ion: 117 Resp: 14366
Ion Ratio Lower Upper
117 100
119 4.2 75.8 113.6#
121 0.0 23.8 35.6#

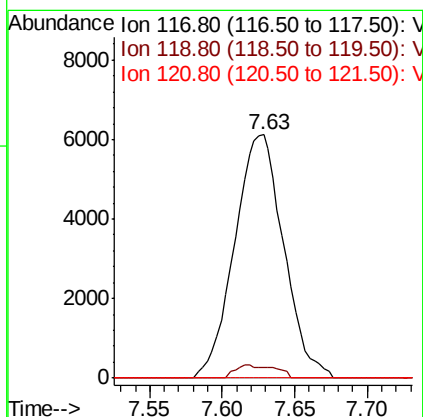



#43

Isopropyl Acetate

Concen: 11.044 ug/l

RT: 8.12 min Scan# 1975

Delta R.T. -0.00 min

Lab File: VN061922.D

Acq: 19 Jun 2020 1:17

Instrument :

MSVOA_N

ClientSampleId :

PB129596TB


Tot Ion: 43 Resp: 35347

Ion Ratio Lower Upper

43 100

61 21.0 24.0 36.0#




87 15.6 12.5 18.7

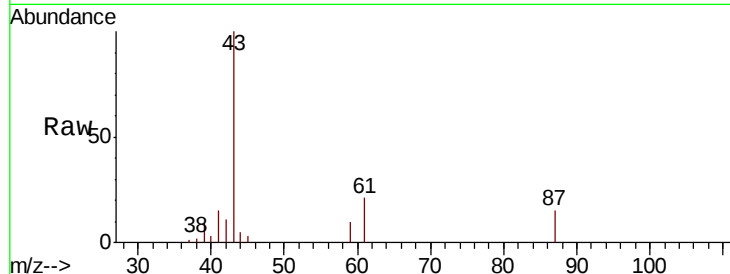

Abundance Ion 43.00 (42.70 to 43.70): VN061834.D (-1956) (-)

Ion 61.00 (60.70 to 61.70): VN061834.D (-1956) (-)

Ion 87.00 (86.70 to 87.70): VN061834.D (-1956) (-)

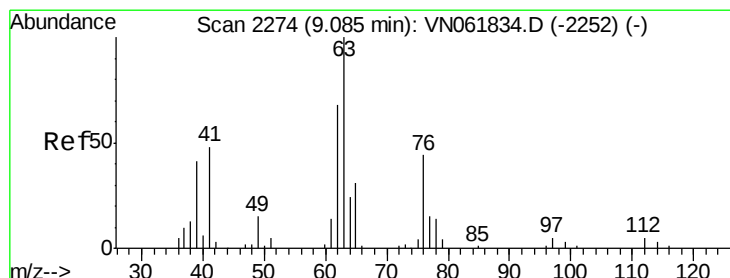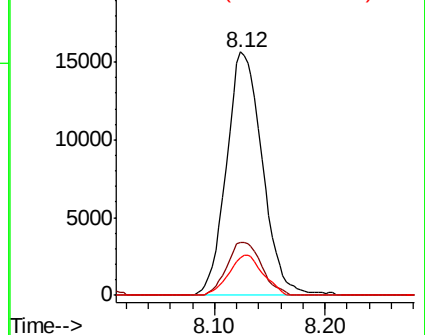

#45

1,2-Dichloropropane

Concen: 0.479 ug/l

RT: 9.24 min Scan# 2321

Delta R.T. 0.15 min

Lab File: VN061922.D


Acq: 19 Jun 2020 1:17

Tgt Ion: 63 Resp: 868

Ion Ratio Lower Upper



63 100


65 0.0 25.1 37.7#

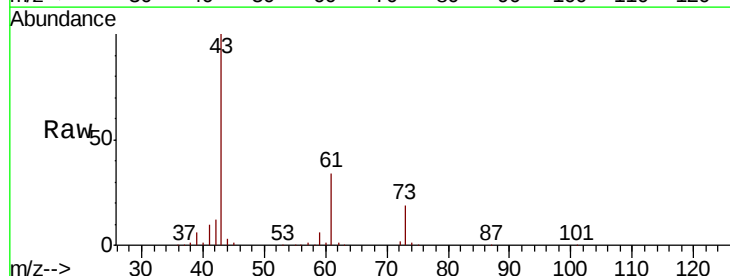

Abundance Ion 62.90 (62.60 to 63.60): VN061834.D (-2252) (-)

Ion 64.90 (64.60 to 65.60): VN061834.D (-2252) (-)




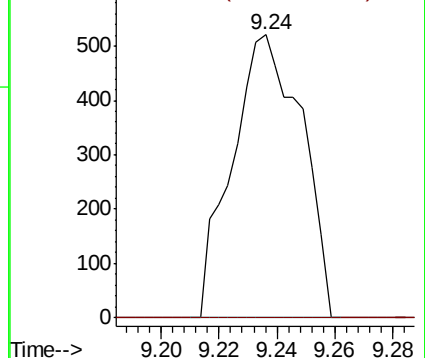




#48
Methvl methacrylate
Concen: 1.492 ug/l
RT: 9.15 min Scan# 2295
Delta R.T. -0.01 min
Lab File: VN061922.D
Acq: 19 Jun 2020 1:17




Instrument :
MSVOA_N
ClientSampleId :
PB129596TB


Tot Ion: 41 Resp: 2171
Ion Ratio Lower Upper
41 100
69 0.0 83.0 124.4#
39 0.0 55.1 82.7#

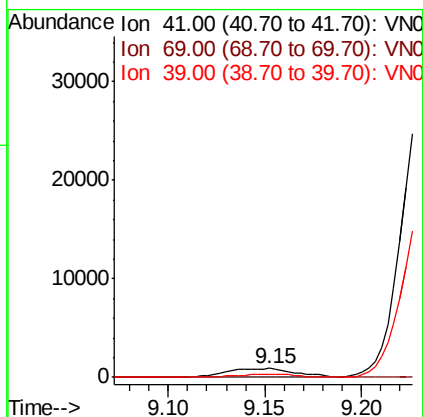

#50
Toluene-d8
Concen: 50.912 ug/l
RT: 10.06 min Scan# 2577
Delta R.T. -0.00 min
Lab File: VN061922.D
Acq: 19 Jun 2020 1:17

Tgt Ion: 98 Resp: 341438
Ion Ratio Lower Upper
98 100
100 64.7 52.7 79.1

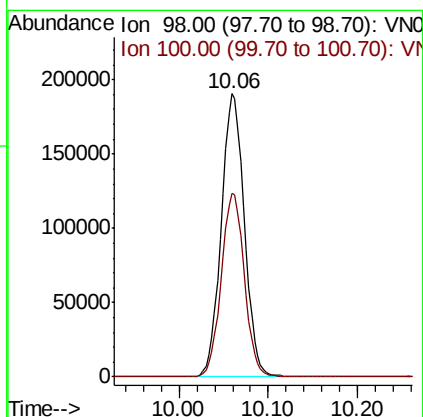



#51

4-Methyl-2-Pentanone

Concen: 1.533 ug/l

RT: 9.95 min Scan# 2543

Delta R.T. -0.00 min

Lab File: VN061922.D

Acq: 19 Jun 2020 1:17

Instrument :

MSVOA_N

ClientSampled :


PB129596TB

Tot Ion: 43 Resp: 2900

Ion Ratio Lower Upper




43 100

58 49.4 34.6 52.0

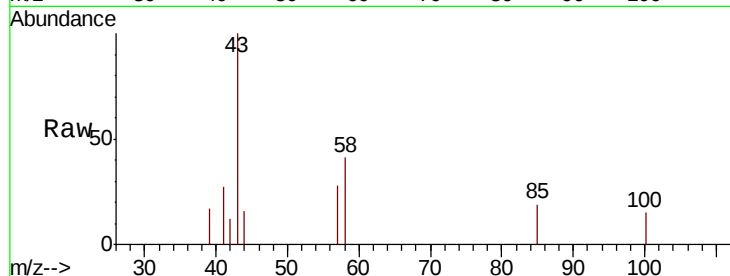

Abundance Ion 43.00 (42.70 to 43.70): VN061834.D (-2527) (-)

Ion 58.00 (57.70 to 58.70): VN061834.D (-2527) (-)

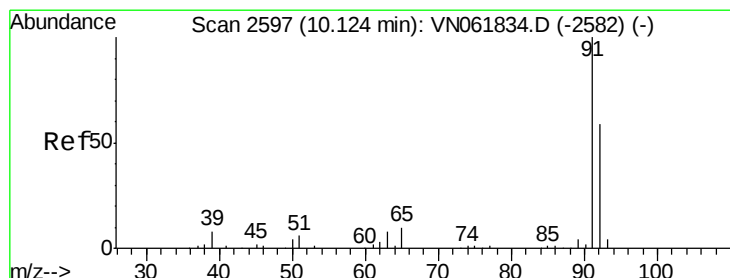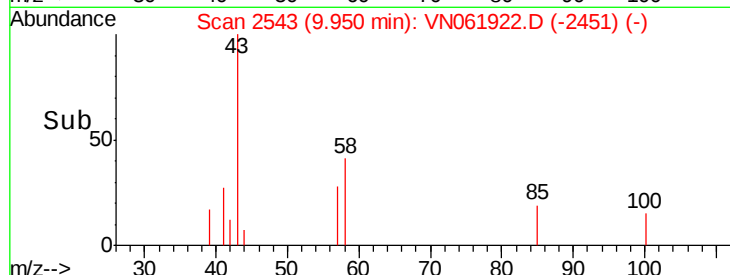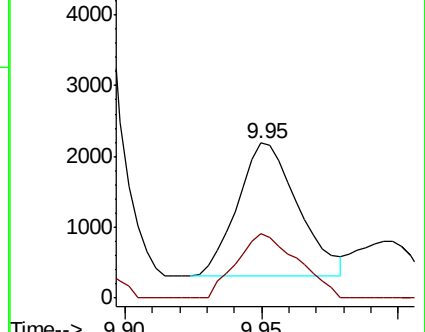

#52

Toluene

Concen: 0.597 ug/l

RT: 10.13 min Scan# 2598

Delta R.T. 0.00 min

Lab File: VN061922.D


Acq: 19 Jun 2020 1:17

Tgt Ion: 92 Resp: 2761

Ion Ratio Lower Upper



92 100


91 181.3 137.1 205.7

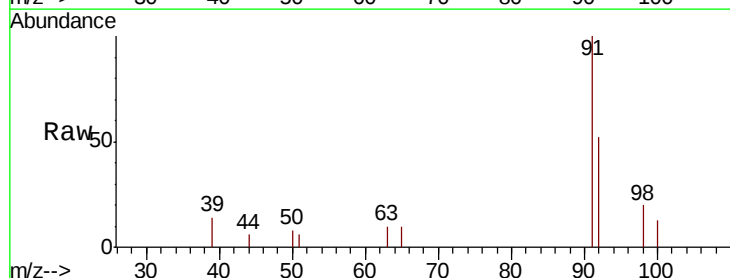

Abundance Ion 92.00 (91.70 to 92.70): VN061834.D (-2582) (-)

Ion 91.00 (90.70 to 91.70): VN061834.D (-2582) (-)

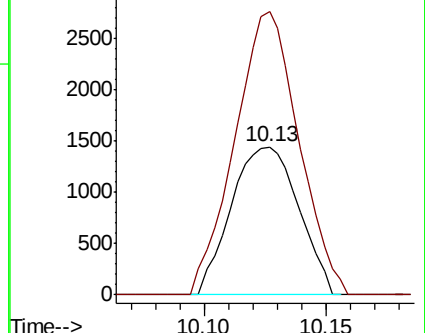







#54
 cis-1,3-Dichloropropene
 Concen: 6.116 ug/l
 RT: 9.88 min Scan# 2520
 Delta R.T. 0.07 min
 Lab File: VN061922.D
 Acq: 19 Jun 2020 1:17

Instrument :
 MSVOA_N
 ClientSampled :
 PB129596TB

Tot Ion: 75 Resp: 18410
 Ion Ratio Lower Upper
 75 100
 77 0.0 24.8 37.2#
 39 35.1 35.4 53.0#

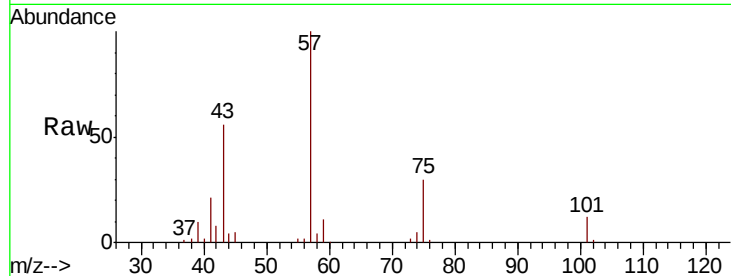


Abundance Ion 74.90 (74.60 to 75.60): VNO
 Ion 76.90 (76.60 to 77.60): VNO
 Ion 39.00 (38.70 to 39.70): VNO

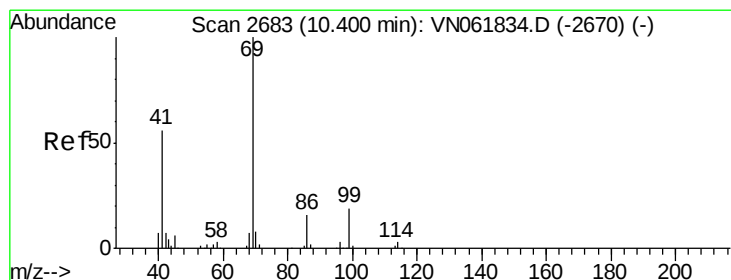
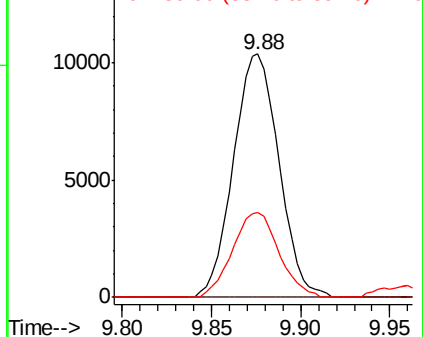



#56
 Ethyl methacrylate
 Concen: 3.147 ug/l
 RT: 10.51 min Scan# 2718
 Delta R.T. 0.11 min
 Lab File: VN061922.D
 Acq: 19 Jun 2020 1:17

Tgt Ion: 69 Resp: 723
 Ion Ratio Lower Upper
 69 100
 41 5242.5 44.9 67.3#
 39 2499.6 30.0 45.0#



Abundance Ion 69.00 (68.70 to 69.70): VNO
 Ion 41.00 (40.70 to 41.70): VNO
 Ion 39.00 (38.70 to 39.70): VNO




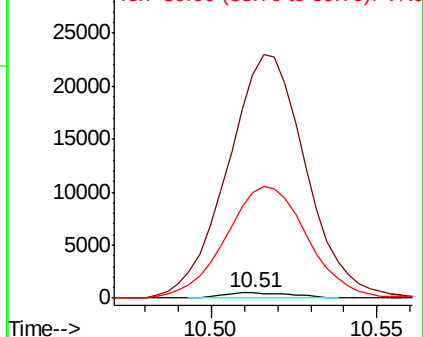




#57
 1,3-Dichloropropane
 Concen: 1.157 ug/l
 RT: 10.74 min Scan# 2788
 Delta R.T. 0.06 min
 Lab File: VN061922.D
 Acq: 19 Jun 2020 1:17




Instrument :
 MSVOA_N
 ClientSampleId :
 PB129596TB


Tot Ion: 76 Resp: 3568
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.8 38.8#

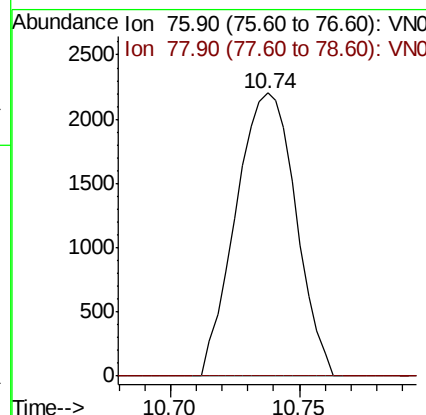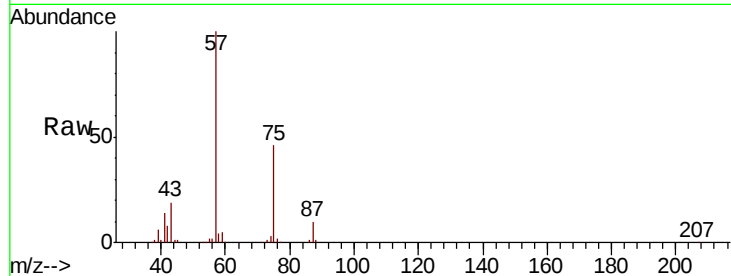

#59
 2-Hexanone
 Concen: 40.335 ug/l
 RT: 10.74 min Scan# 2788
 Delta R.T. 0.02 min
 Lab File: VN061922.D
 Acq: 19 Jun 2020 1:17

Tgt Ion: 43 Resp: 42995
 Ion Ratio Lower Upper
 43 100
 58 22.0 30.1 90.5#

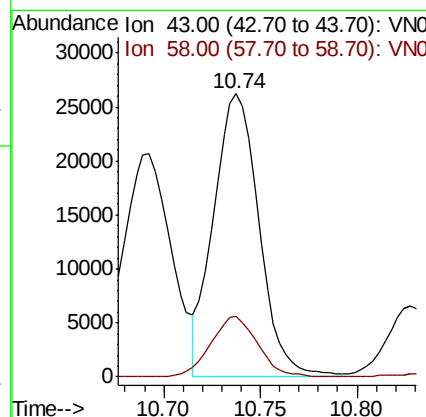



#62

4-Bromofluorobenzene

Concen: 49.232 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. -0.00 min

Lab File: VN061922.D

Acq: 19 Jun 2020 1:17

Instrument :

MSVOA_N

ClientSampleId :

PB129596TB


Tot Ion: 95 Resp: 113252

Ion Ratio Lower Upper

95 100

174 79.7 0.0 158.6




176 77.2 0.0 152.0

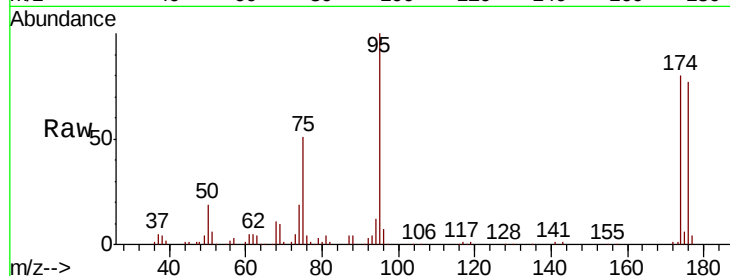

Abundance Ion 94.90 (94.60 to 95.60): VN061834.D (-3284) (-)

Ion 173.80 (173.50 to 174.50): VN061834.D (-3284) (-)

Ion 175.80 (175.50 to 176.50): VN061834.D (-3284) (-)

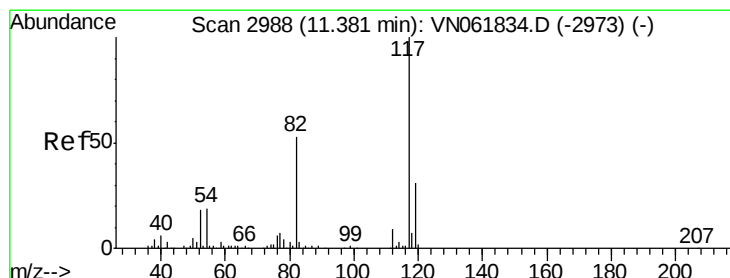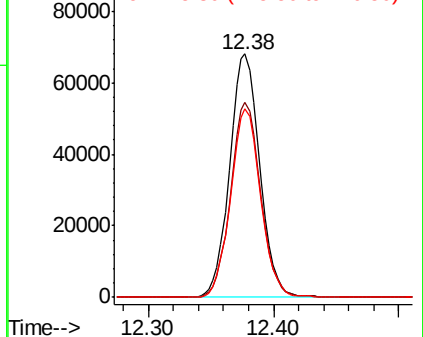

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.38 min Scan# 2988

Delta R.T. -0.00 min

Lab File: VN061922.D

Acq: 19 Jun 2020 1:17


Tgt Ion: 117 Resp: 270569

Ion Ratio Lower Upper

117 100

82 53.3 42.6 64.0



119 31.9 24.7 37.1

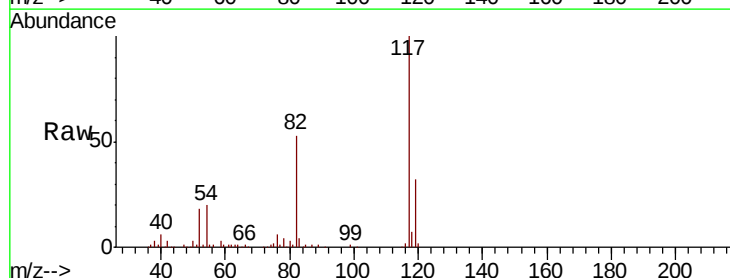


Abundance Ion 116.90 (116.60 to 117.60): VN061834.D (-2973) (-)

Ion 82.00 (81.70 to 82.70): VN061834.D (-2973) (-)

Ion 118.90 (118.60 to 119.60): VN061834.D (-2973) (-)

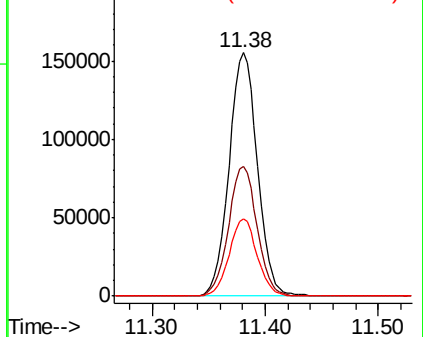



#71

Bromoform

Concen: 0.765 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. 0.28 min

Lab File: VN061922.D

Acq: 19 Jun 2020 1:17

Instrument :

MSVOA_N

ClientSampled :

PB129596TB


Tot Ion:173 Resp: 1111

Ion Ratio Lower Upper

173 100

175 519.9 23.9 71.7#




254 0.0 0.0 0.0



Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

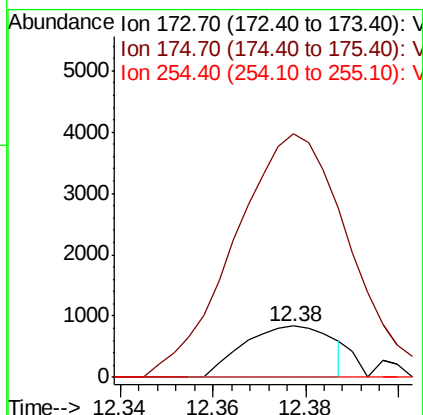

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3591

Delta R.T. 0.00 min

Lab File: VN061922.D

Acq: 19 Jun 2020 1:17


Tgt Ion:152 Resp: 102066

Ion Ratio Lower Upper

152 100

115 59.2 29.1 87.3



150 157.7 0.0 347.6




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V



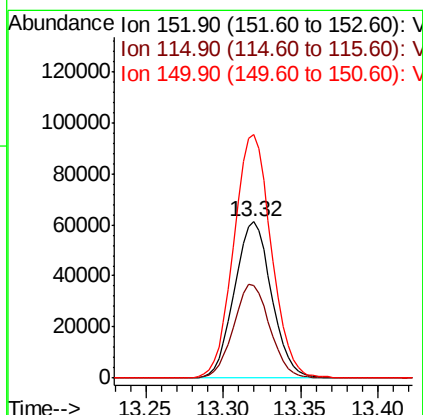





#74
N-amvl acetate
Concen: 3.661 ug/l
RT: 12.01 min Scan# 3183
Delta R.T. -0.04 min
Lab File: VN061922.D
Acq: 19 Jun 2020 1:17




Instrument :
MSVOA_N
ClientSampled :
PB129596TB


Tot Ion: 43 Resp: 1671
Ion Ratio Lower Upper
43 100
70 0.0 40.6 60.8#
55 0.0 21.5 32.3#
61 0.0 21.6 32.4#

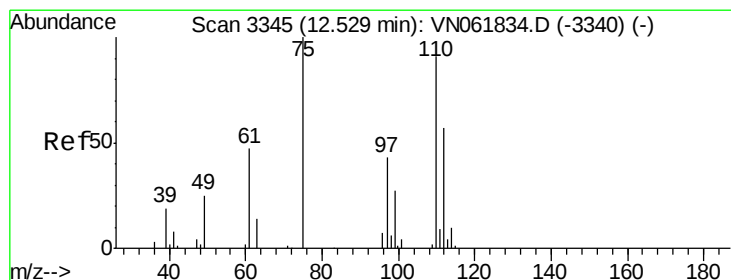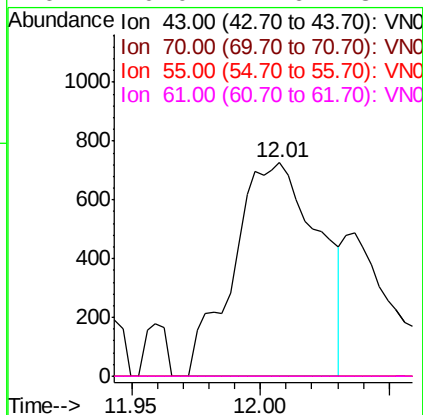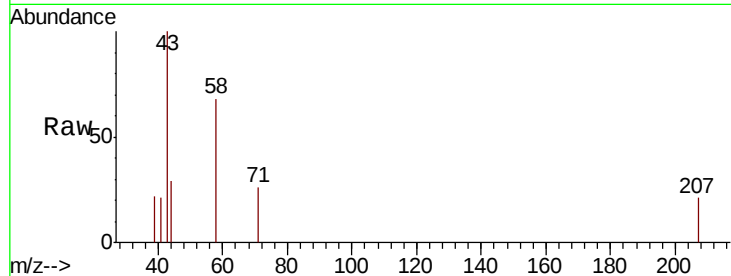

#76
1,2,3-Trichloropropane
Concen: 29.047 ug/l
RT: 12.38 min Scan# 3298
Delta R.T. -0.15 min
Lab File: VN061922.D
Acq: 19 Jun 2020 1:17

Tgt Ion: 75 Resp: 58205
Ion Ratio Lower Upper
75 100
77 1.0 0.0 0.0#


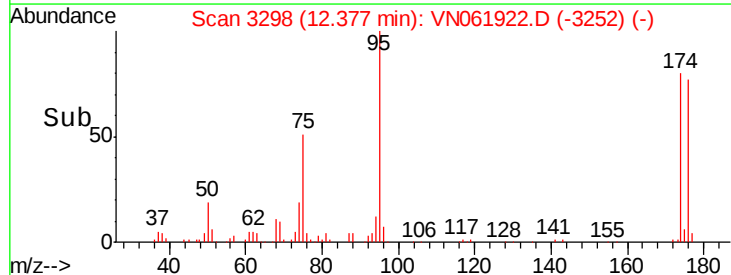
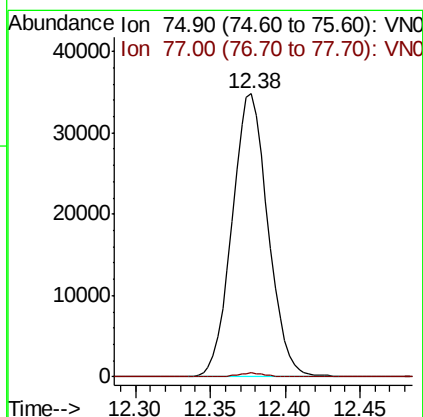





#80
 1,3,5-Trimethylbenzene
 Concen: 0.404 ug/l
 RT: 12.71 min Scan# 3401
 Delta R.T. -0.00 min
 Lab File: VN061922.D
 Acq: 19 Jun 2020 1:17




Instrument :
 MSVOA_N
 ClientSampleId :
 PB129596TB


Tot Ion:105 Resp: 2427
 Ion Ratio Lower Upper
 105 100
 120 48.3 24.9 74.7

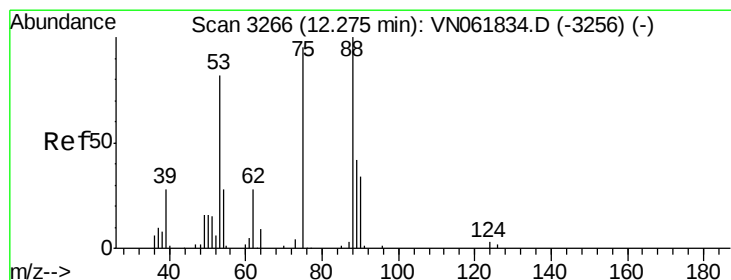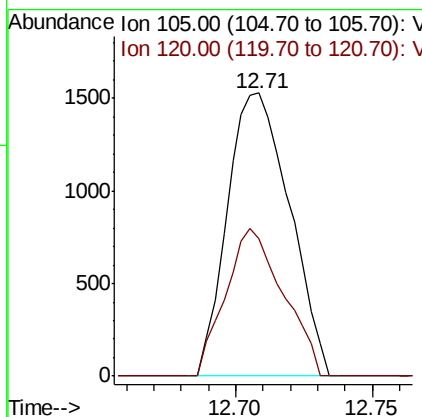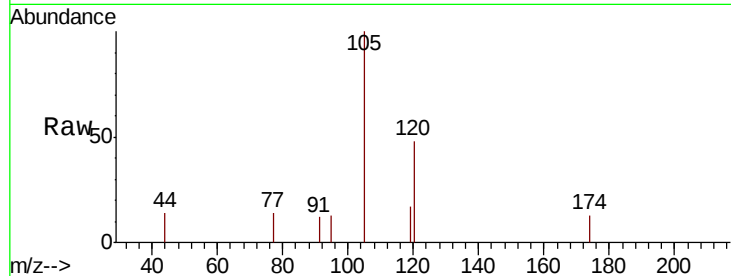

#81
 trans-1,4-Dichloro-2-butene
 Concen: 79.224 ug/l
 RT: 12.38 min Scan# 3298
 Delta R.T. 0.10 min
 Lab File: VN061922.D
 Acq: 19 Jun 2020 1:17

Tgt Ion: 75 Resp: 58205
 Ion Ratio Lower Upper
 75 100
 53 0.0 70.4 105.6#
 89 0.0 36.0 54.0#

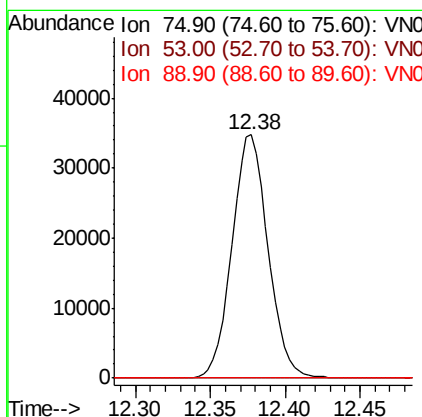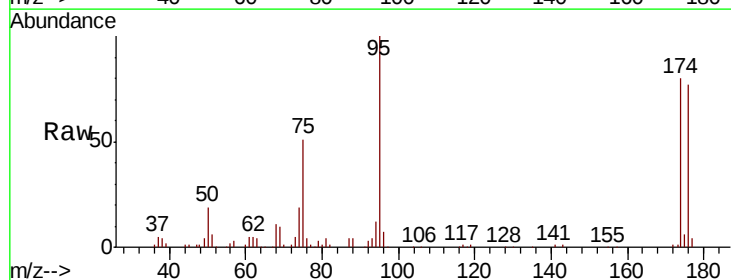

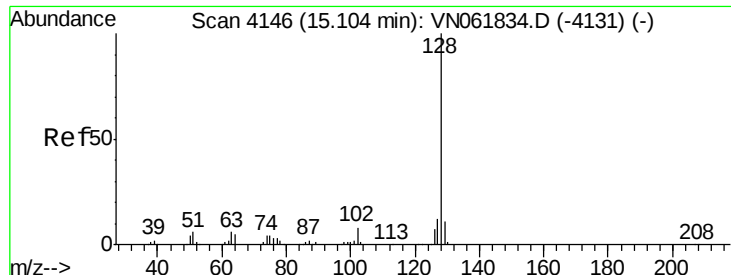

#95

Naphthalene

Concen: 3.626 ug/l

RT: 15.12 min Scan# 4150

Delta R.T. 0.01 min

Lab File: VN061922.D


Acq: 19 Jun 2020 1:17

Instrument :

MSVOA_N

ClientSampleId :

PB129596TB




Tot Ion:128 Resp: 781

Ion Ratio Lower Upper


128 100

127 0.0 10.3 15.5#

129 0.0 8.6 13.0#



Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

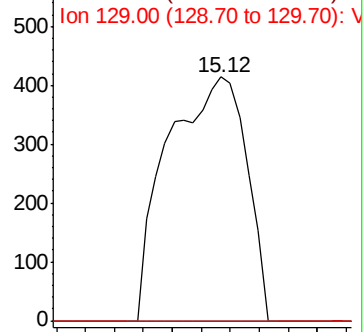

Time-->