


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN061820\
 Data File : VN061889.D
 Acq On : 18 Jun 2020 10:03
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061620W.M
 Title : SW846 8260
 Last Update : Wed Jun 17 01:19:44 2020

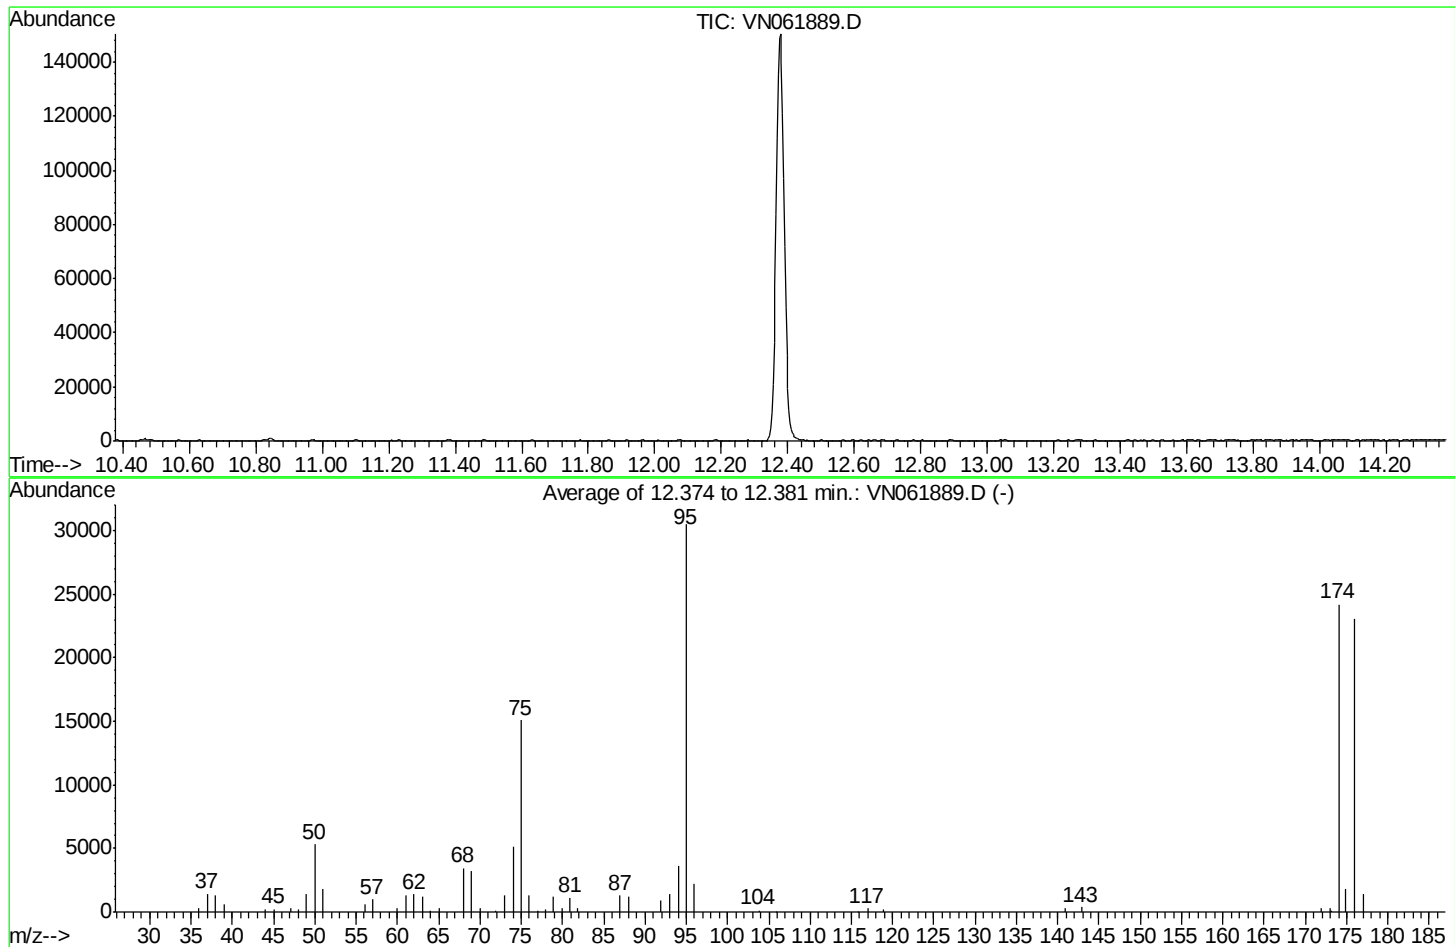

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	5303	PASS
75	95	30	60	49.5	15105	PASS
95	95	100	100	100.0	30498	PASS
96	95	5	9	7.1	2174	PASS
173	174	0.00	2	1.2	292	PASS
174	95	50	100	79.3	24186	PASS
175	174	5	9	7.7	1855	PASS
176	174	95	101	95.4	23085	PASS
177	176	5	9	6.1	1409	PASS