


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN061820\
 Data File : VN061916.D
 Acq On : 18 Jun 2020 22:04
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061620W.M
 Title : SW846 8260
 Last Update : Wed Jun 17 01:19:44 2020

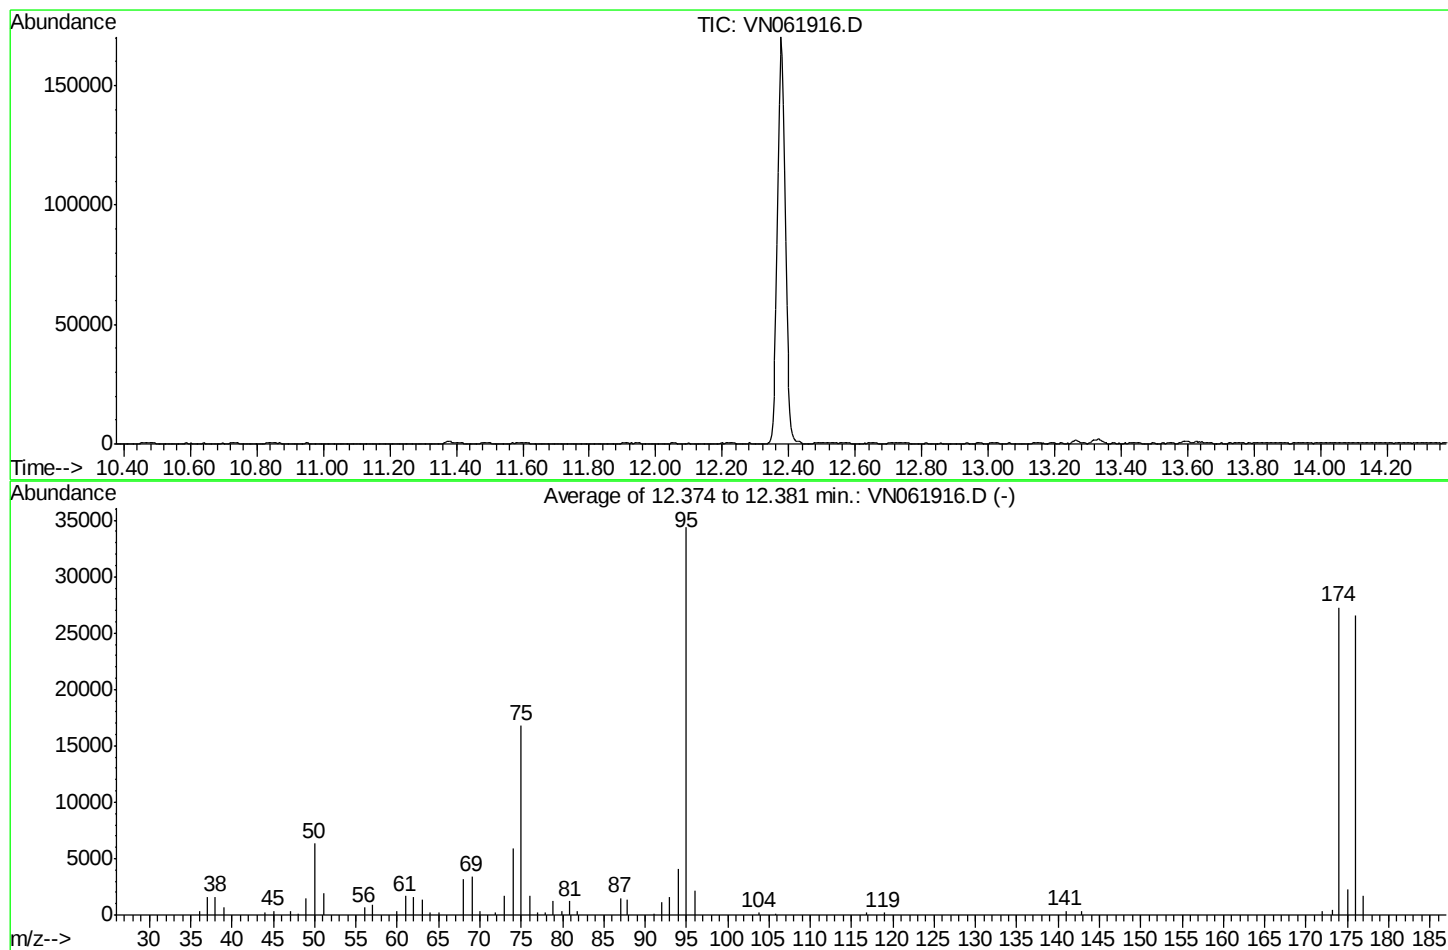

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	6327	PASS
75	95	30	60	48.8	16780	PASS
95	95	100	100	100.0	34376	PASS
96	95	5	9	6.2	2135	PASS
173	174	0.00	2	1.6	437	PASS
174	95	50	100	79.3	27258	PASS
175	174	5	9	8.2	2234	PASS
176	174	95	101	97.4	26552	PASS
177	176	5	9	6.2	1656	PASS