
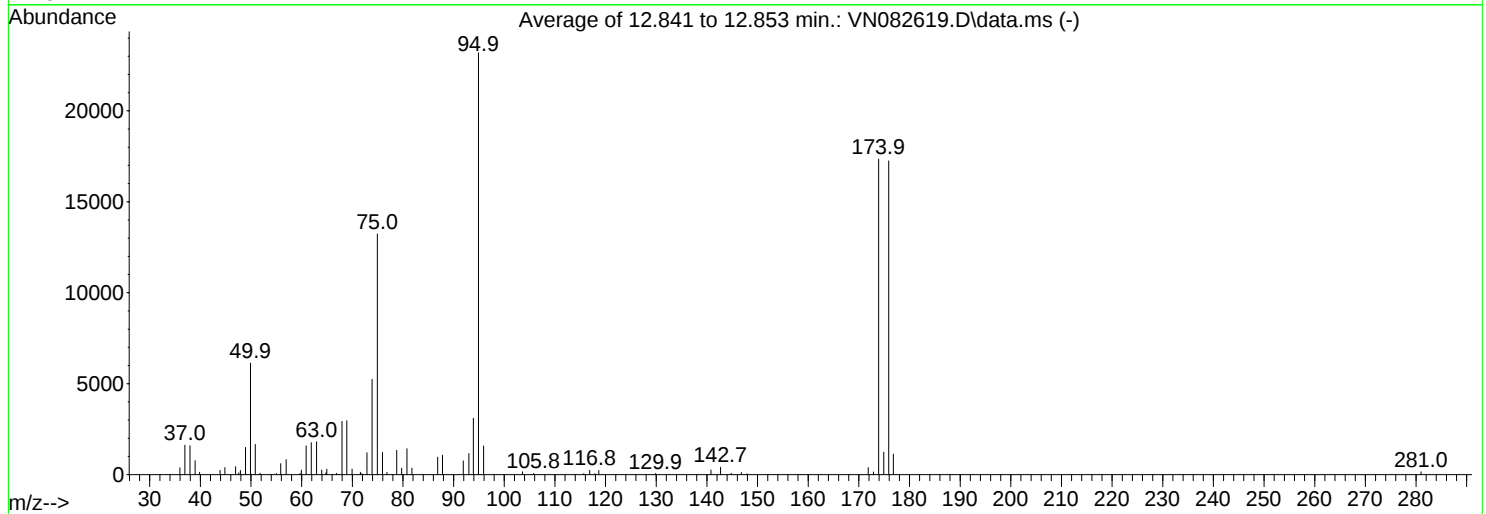


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061824\
Data File : VN082619.D
Acq On : 18 Jun 2024 09:08
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061724W.M
Title : SW846 8260
Last Update : Tue Jun 18 04:52:44 2024

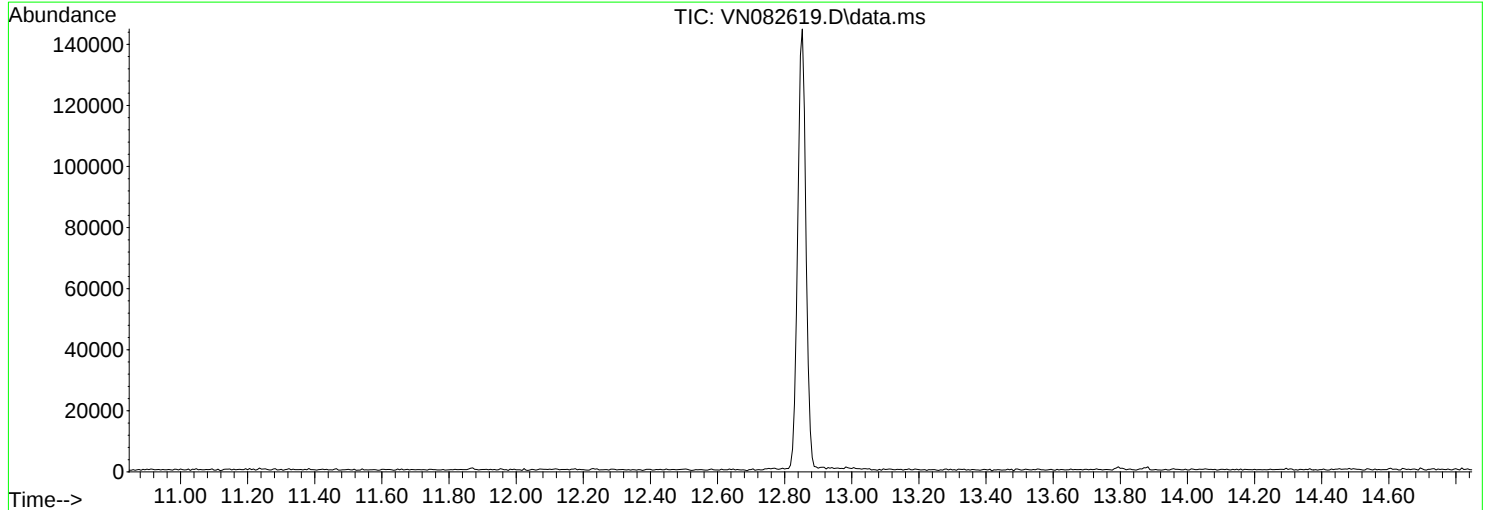

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	26.4	6127	PASS
75	95	30	60	57.1	13233	PASS
95	95	100	100	100.0	23189	PASS
96	95	5	9	6.8	1577	PASS
173	174	0.00	2	0.8	147	PASS
174	95	50	100	74.8	17347	PASS
175	174	5	9	7.1	1239	PASS
176	174	95	101	99.5	17252	PASS
177	176	5	9	6.5	1123	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	381	49.90	6127	63.95	254	74.95	1323
36.95	1615	50.85	1664	64.80	110	75.95	122
37.95	1589	51.80	79	64.95	296	76.85	12
38.95	775	55.00	61	66.90	70	78.75	133
39.85	133	55.85	609	67.95	2932	79.75	357
43.90	241	56.95	828	68.90	2963	80.80	1421
44.85	384	59.70	65	69.95	305	81.75	357
46.95	438	59.95	243	71.60	131	86.85	962
47.60	96	60.90	1580	71.90	52	87.80	1074
47.90	229	61.90	1757	72.90	1204	91.90	757
48.90	1495	62.95	1806	73.90	5246	93.00	1160

Average of 12.841 to 12.853 min.: VN082619.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.90	3103	142.70	402				
94.90	23189	144.80	70				
95.90	1577	146.80	113				
103.60	160	147.90	56				
105.80	72	171.85	390				
115.70	54	172.90	147				
116.85	238	173.90	17347				
117.90	50	174.90	1239				
118.65	231	175.90	17252				
129.90	67	176.80	1123				
140.80	257	281.00	155				

Instrument :

MSVOA_N

ClientSampleId :

BFB